

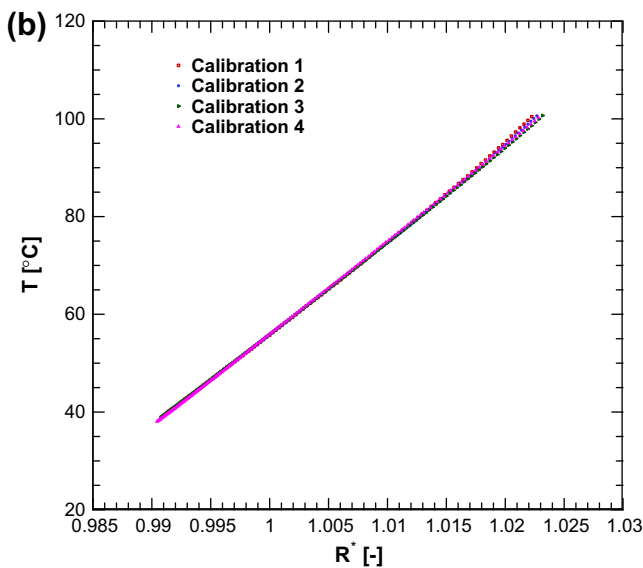
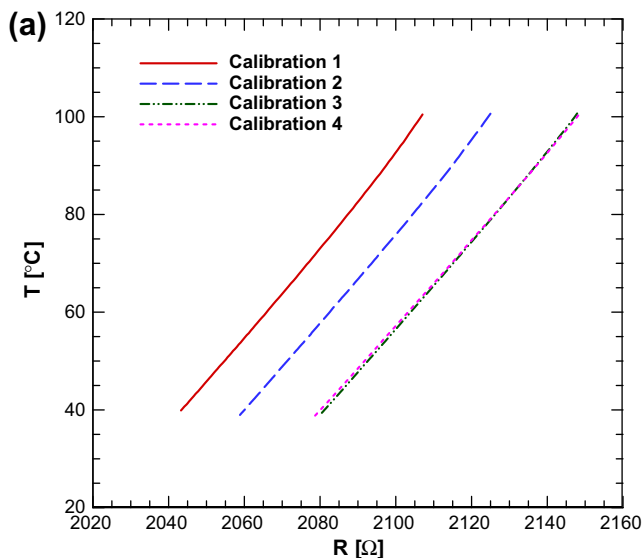


Fig. 5. Repeatability of the temperature vs resistance calibration curves for the 400- μm test strip of surface 5: (a) unrepeatable results for unmodified resistance values, and (b) repeatable results using resistance values normalized according to Eq. (1).

4.1. Temperature sensor calibration

then covered with insulation. The calibration, 10 min before damaging the stabilized, power test strips and recorded as the approximately that the thermal gap was observed system.

Sample calibration Fig. 5a for the ever, revealed distance values therefore normalized temperature T_{sat} :

$$R^*(T) \equiv \frac{R(T)}{R(T_{sat})}$$

T vs R^* curve 2nd-degree polynomial except at high all temperatures the individual $R(T_{sat})$ was measured the resistance expected amount to the right of

During boiling through the heat for the voltage (5 min). Both the determined from prior to recording eos were taken consistent over enough to capture

Between in the test strip with

