



TEKTRONIX PRODUCTION TEST REPORT

Date: 2026-02-02 12:01:36
Test Suite: AWG70002B Pulse Timing Test
Operator: N/A
DUT Serial: N/A
Oscilloscope: MSO68B (S/N: C031797)

PROBE CONFIGURATION

Channel	Probe Type	Serial Number
CH1	1X	N/A
CH2	1X	N/A
CH3	1X	N/A
CH4	1X	N/A
CH5	1X	N/A
CH6	1X	N/A
CH7	1X	N/A
CH8	1X	N/A


TEST RESULTS

#	Test Name	Nominal	Lower Limit	Upper Limit	Measured	Status
1	Delay CH1↑→CH2↑	2.000 µs	1.990 µs	2.010 µs	2.000 µs	PASS
2	Delay CH1↓→CH2↑	1.000 µs	990.000 ns	1.010 µs	1.000 µs	PASS
3	Rise Time CH1	165.000 ps	150.000 ps	180.000 ps	160.378 ps	PASS
4	Rise Time CH2	165.000 ps	150.000 ps	180.000 ps	155.054 ps	PASS
5	Fall Time CH1	165.000 ps	150.000 ps	180.000 ps	172.202 ps	PASS
6	Fall Time CH2	165.000 ps	150.000 ps	180.000 ps	168.076 ps	PASS


SUMMARY: 6 PASS, 0 FAIL - ALL TESTS PASSED

Complete SCPI command log saved to: scpi_log.txt


SCREENSHOTS

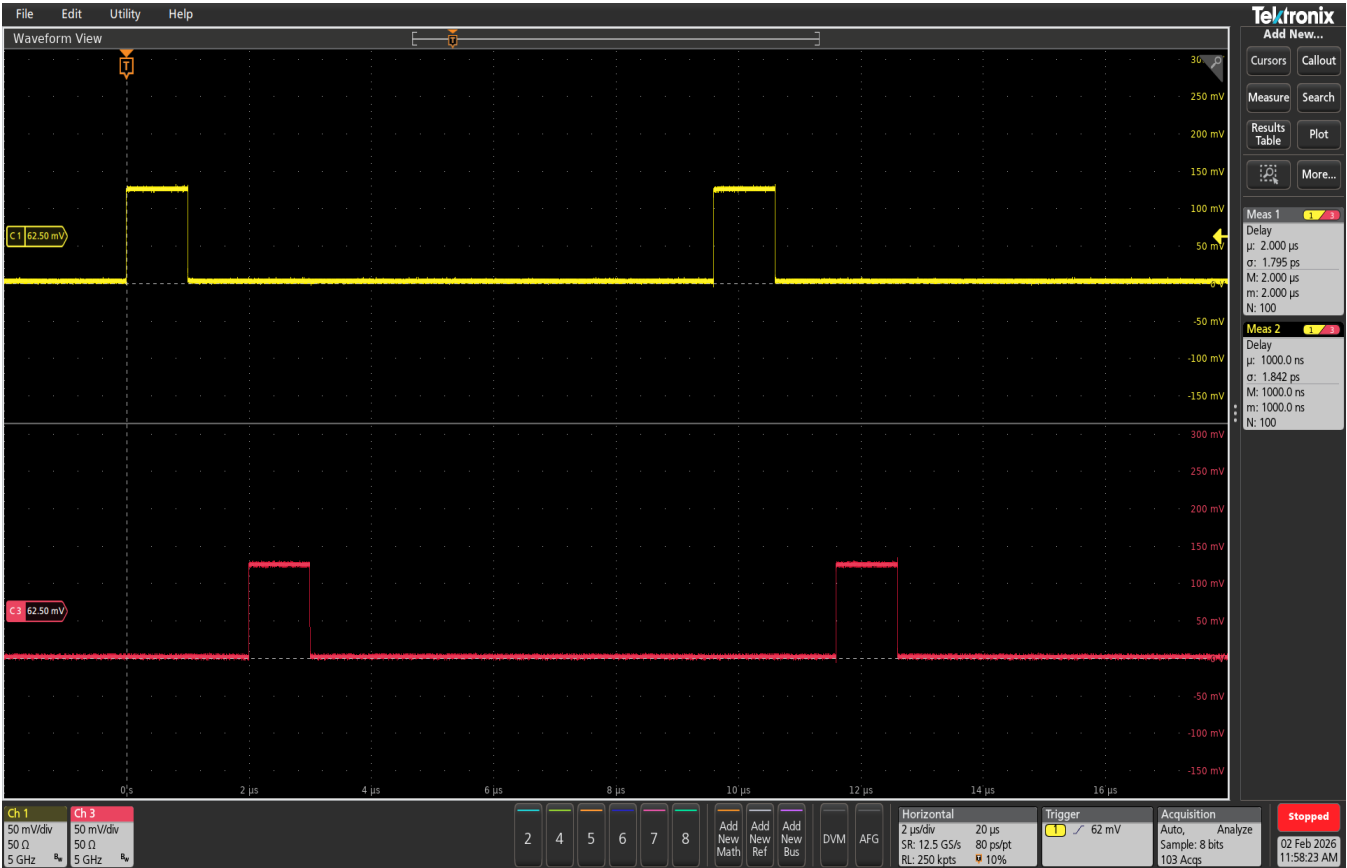


Test 1: delay_view.png

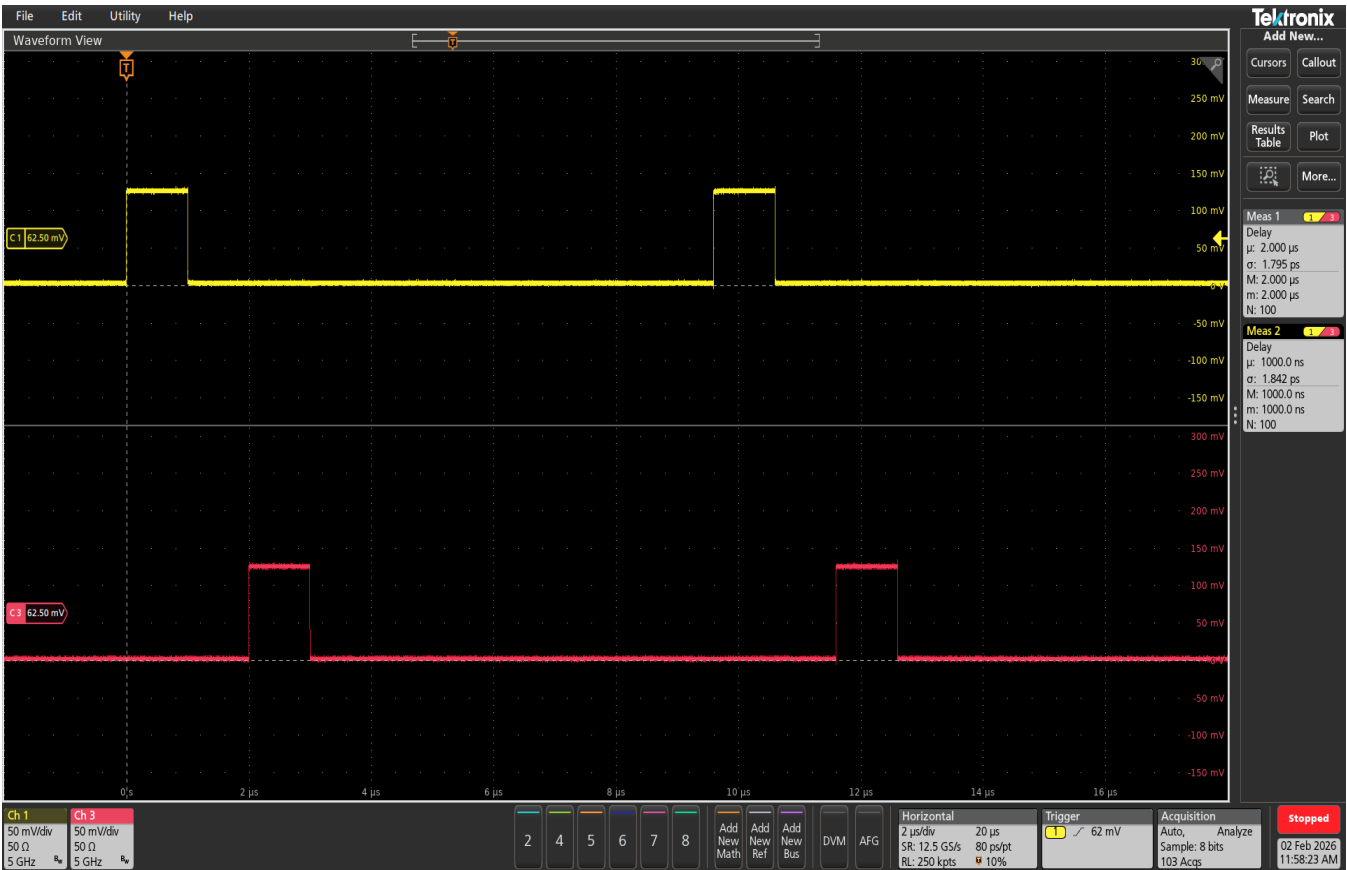


Test 2: delay_view.png

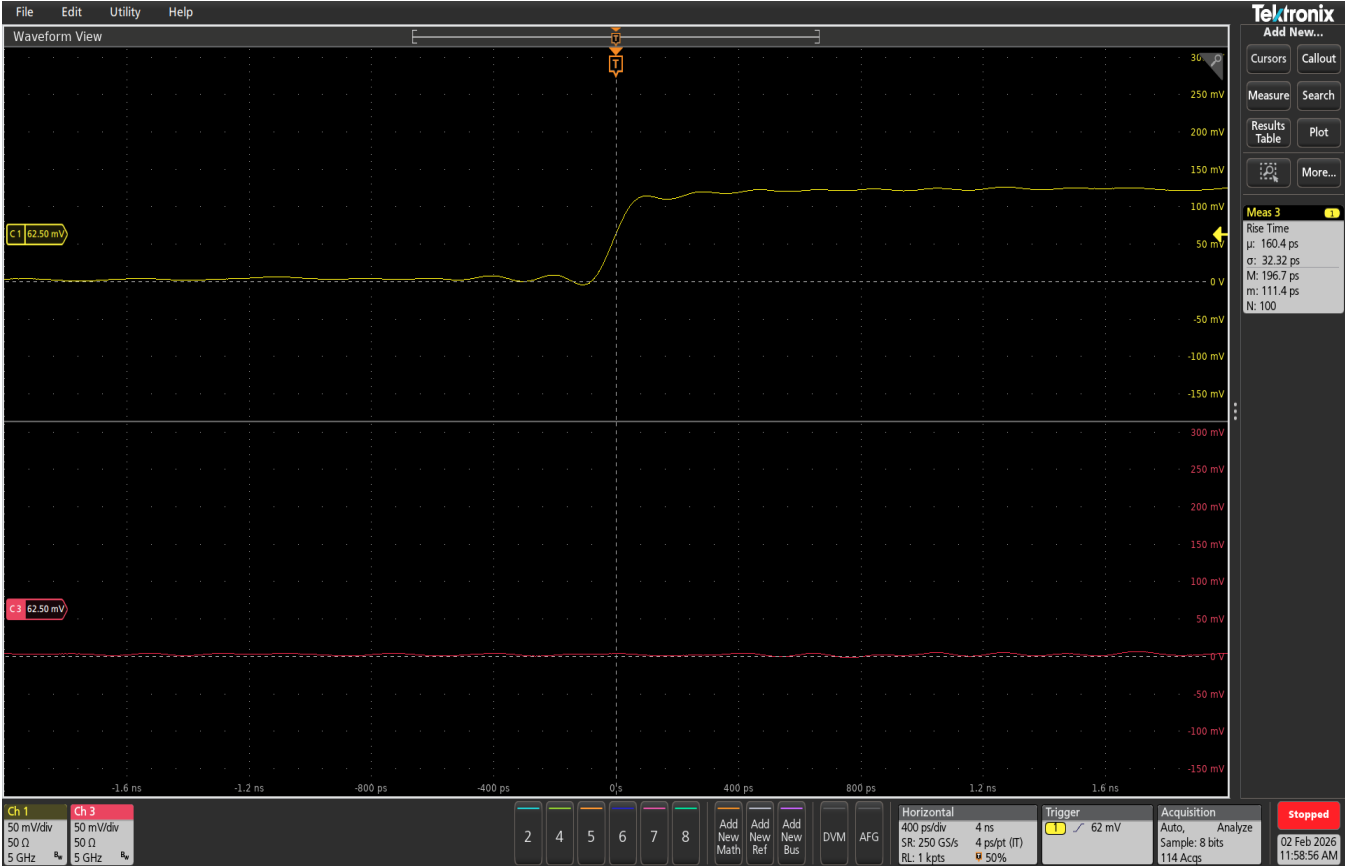


Test 3: rise_time_ch1.png



Test 4: rise_time_ch2.png

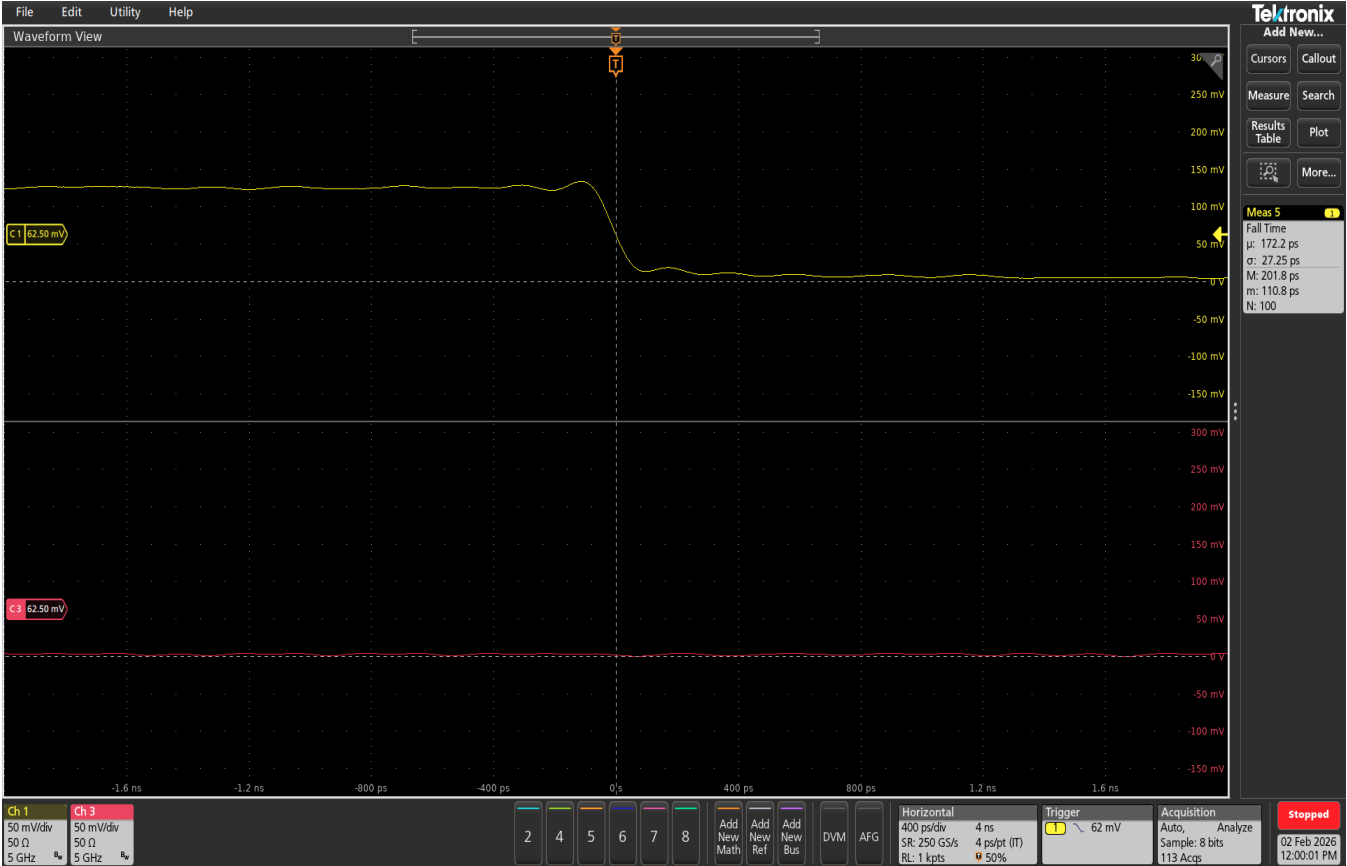

Test 5: fall_time_ch1.png



Test 6: fall_time_ch2.png