Pulse Oximeter

01. Table of Contents

02. +12V Input

03. +12V Telemetry

04. +3.3V Power Supply

05. +3.3V Telemetry

06. +1.8V Power Supply

07. +1.8V Telemetry

08. PIC32MZ Programming

09. PIC32MZ Bypass

10. PIC32MZ Clocking

11. PIC32MZ

12. USB UART Bridge

13. USB Telemetry

14. Platform ETC

15. POX Sensor

16. Display

17. Pushbuttons

Sheet: +12V Input
File: POS12_Input.sch

Sheet: +12V Telemetry
File: POS12_Telemetry.sch

Sheet: +3.3V Power Supply
File: POS3P3_Power_Supply.sch

Sheet: +3.3V Telemetry
File: POS3P3_Telemetry.sch

Sheet: +1.8V Power Supply
File: POS1P8_Power_Supply.sch

Sheet: +1.8V Telemetry
File: POS1P8_Telemetry.sch

Sheet: PIC32MZ Programming
File: PIC32MZ_Programming.sch

Sheet: PIC32MZ Bypass
File: PIC32MZ_Bypass.sch

Sheet: PIC32MZ Clocking
File: PIC32MZ_Clocking.sch

Sheet: PIC32MZ
File: PIC32MZ.sch

Sheet: USB UART Bridge
File: USB_UART_Bridge.sch

Sheet: USB Telemetry
File: USB_Telemetry.sch

Sheet: Platform ETC
File: Platform_ETC.sch

Sheet: POX Sensor
File: POX_Sensor.sch

Sheet: Display
File: Display.sch

Sheet: Pushbuttons
File: Pushbuttons.sch

18. PGOOD LEDs

19. Status LEDs

20. Misc Circuits

21. Mechanical

Sheet: PGOOD LEDs
File: PGOOD_LEDs.sch

Sheet: Status LEDs
File: Status_LEDs.sch

Sheet: Misc Circuits
File: Misc_Circuits.sch

Sheet: Mechanical
File: Mechanical.sch

Drew Maatman

Sheet: /
File: Pulse_Oximeter.sch

Title: Pulse Oximeter

Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 1/21

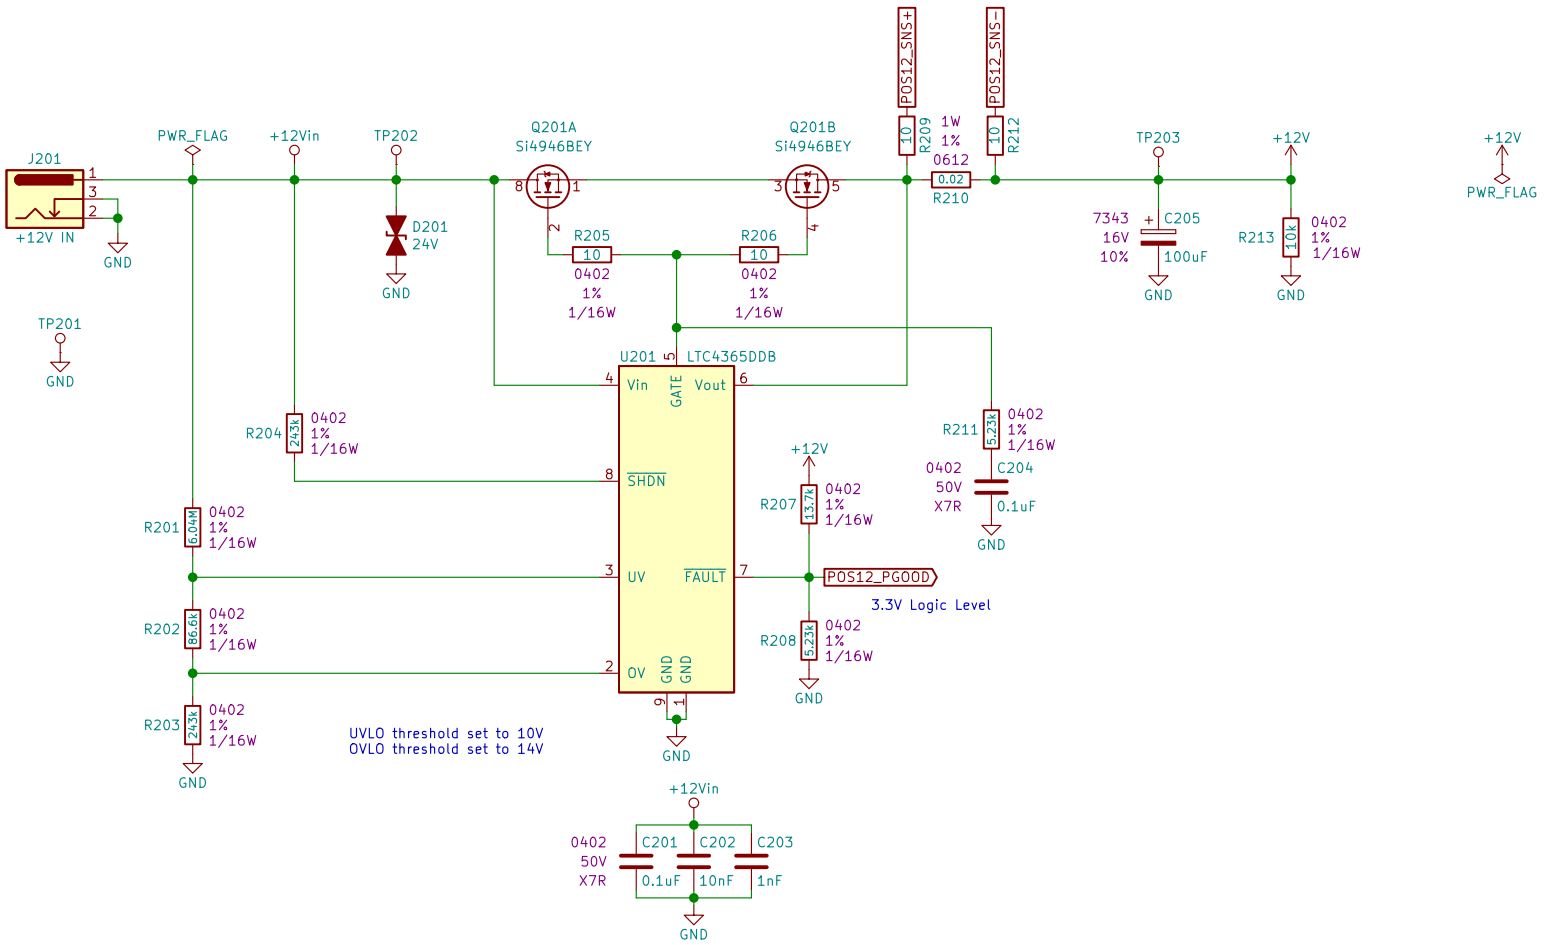

Drew Maatman	
Sheet: /+12V Input/	
File: POS12_Input.sch	
Title: Pulse Oximeter	
Size: A	Date: 2020-12-09
KiCad E.D.A. kicad (5.1.8)-1	Id: 2/21

Rev: B

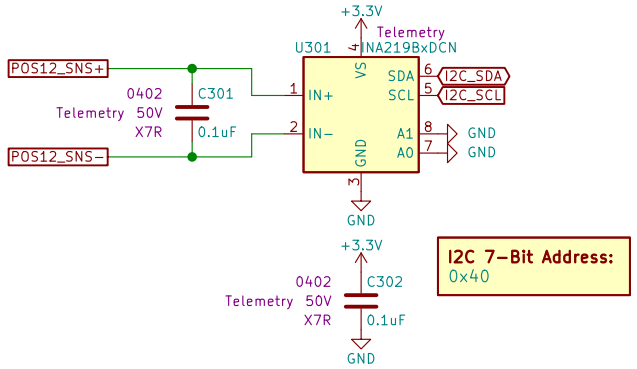

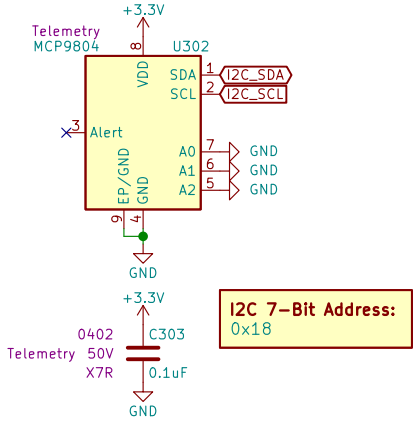

Drew Maatman		
Sheet: /+12V Telemetry/		
File: POS12_Telemetry.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020−12−09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)−1		Id: 3/21

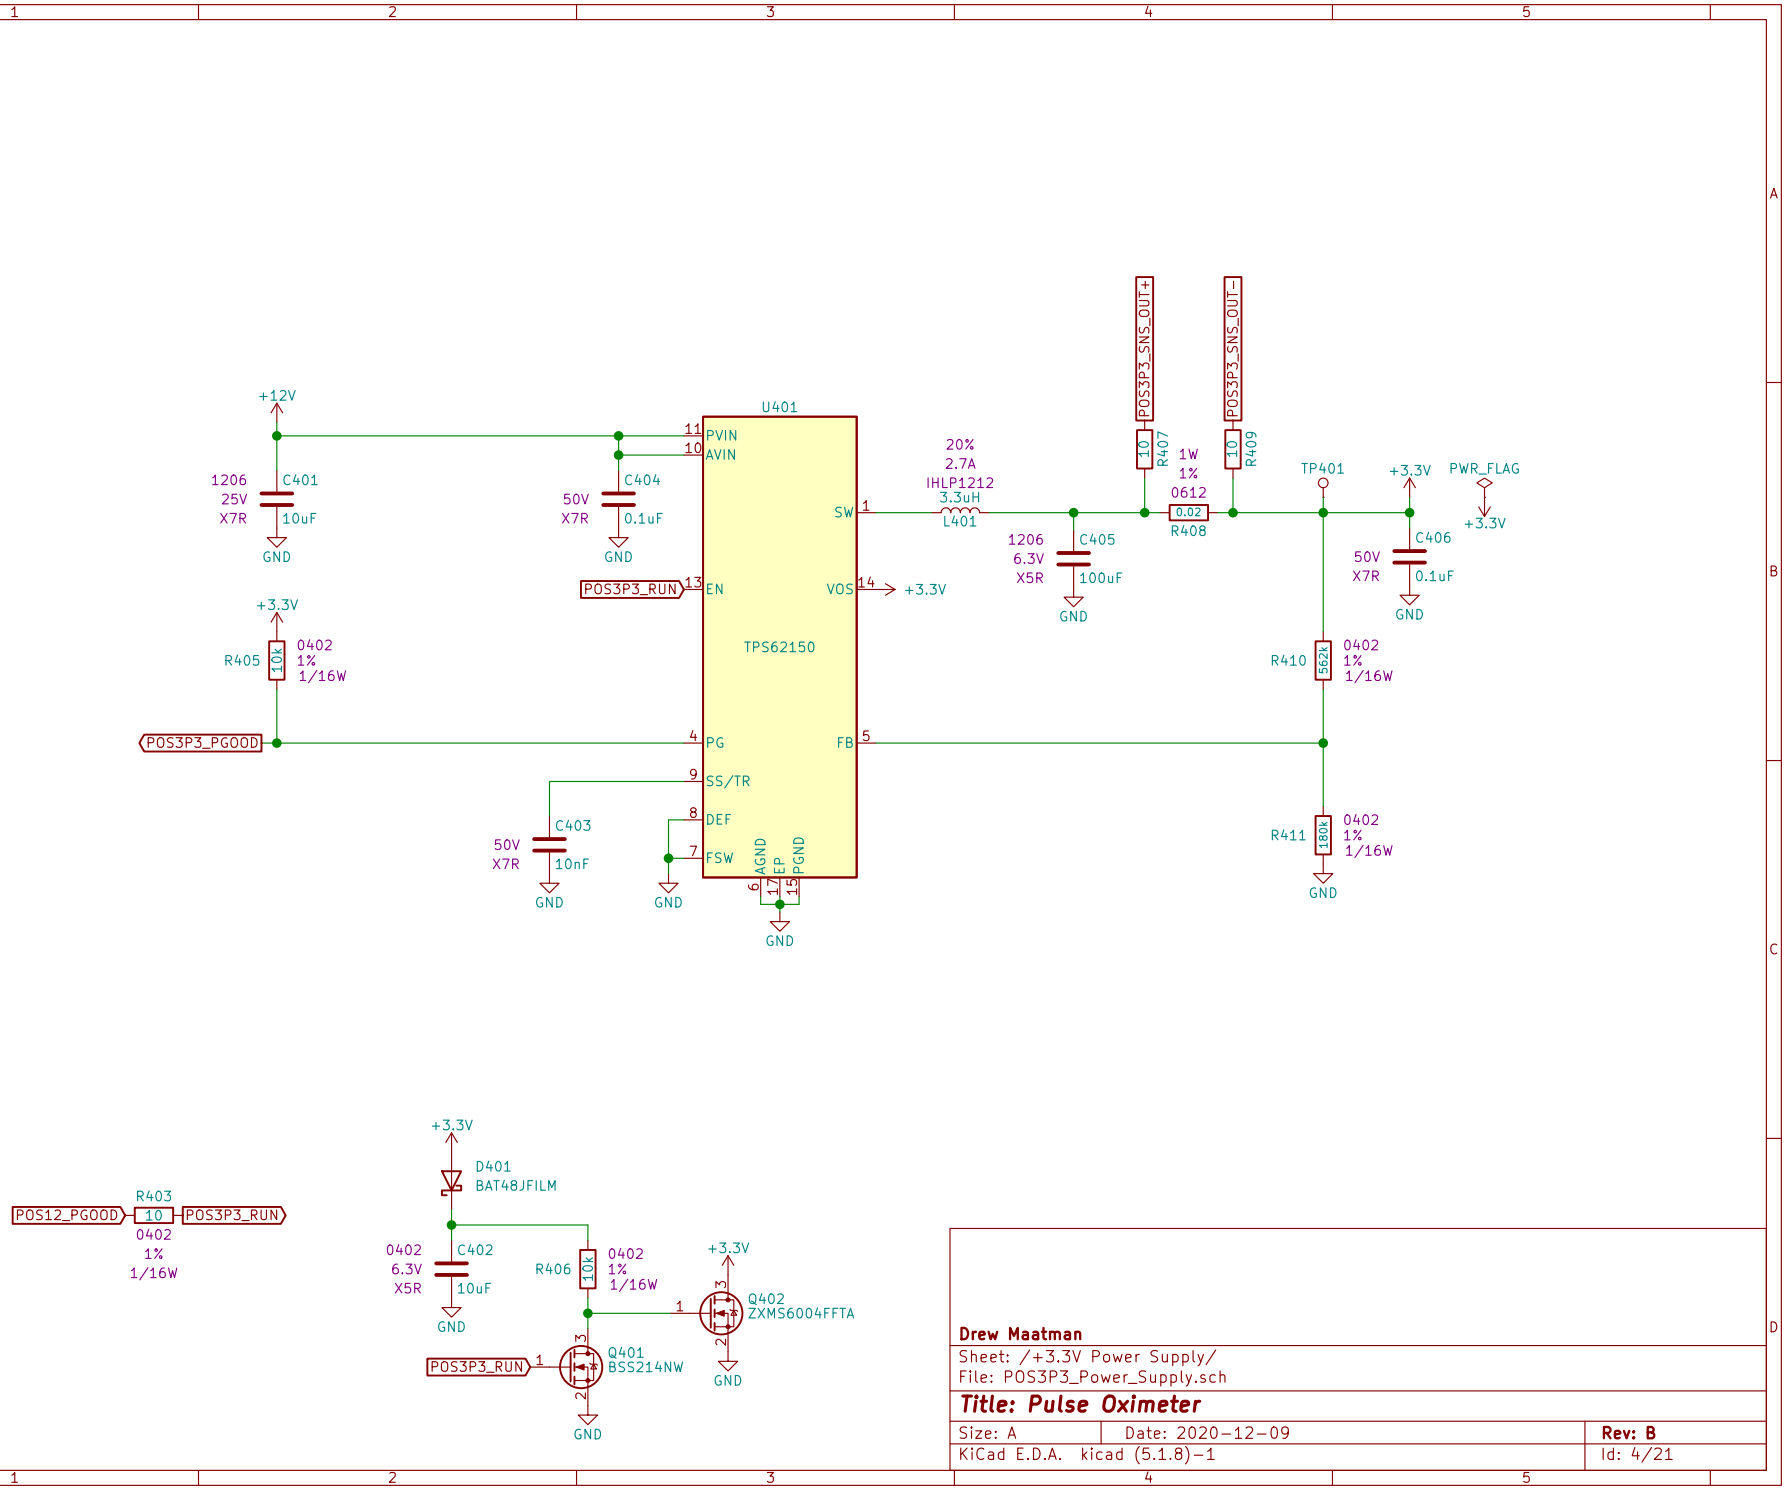

Drew Maatman	
Sheet: /+3.3V Power Supply/	
File: POS3P3_Power_Supply.sch	
Title: Pulse Oximeter	
Size: A	Date: 2020-12-09
KiCad E.D.A. kicad (5.1.8)-1	Id: 4/21

Rev: B

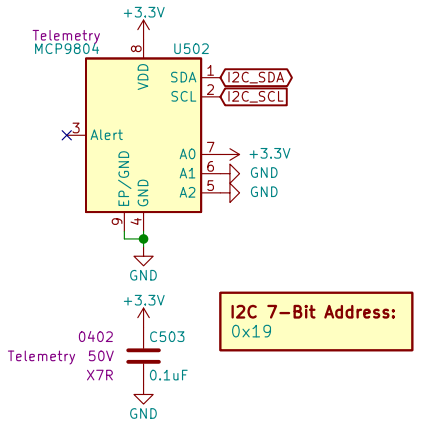

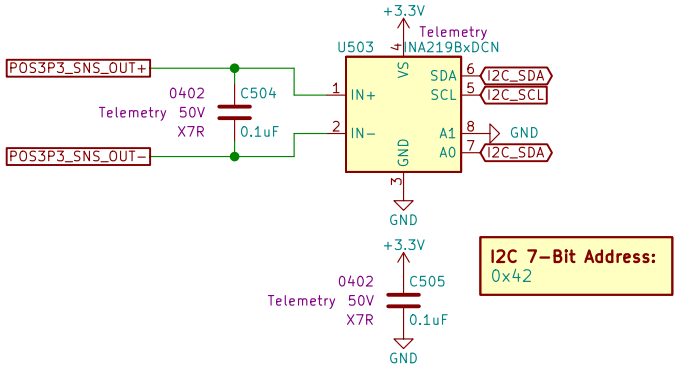

Drew Maatman		
Sheet: /+3.3V Telemetry/		
File: POS3P3_Telemetry.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 5/21

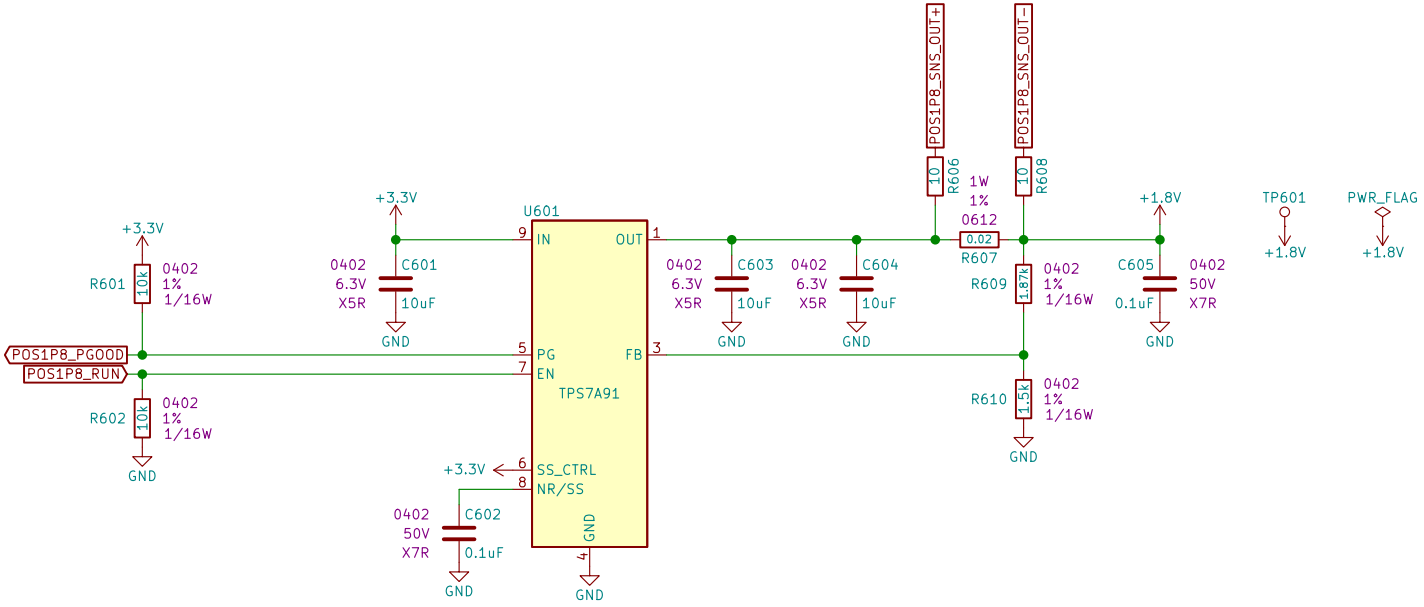

Drew Maatman		
Sheet: /+1.8V Power Supply/		
File: POS1P8_Power_Supply.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 6/21

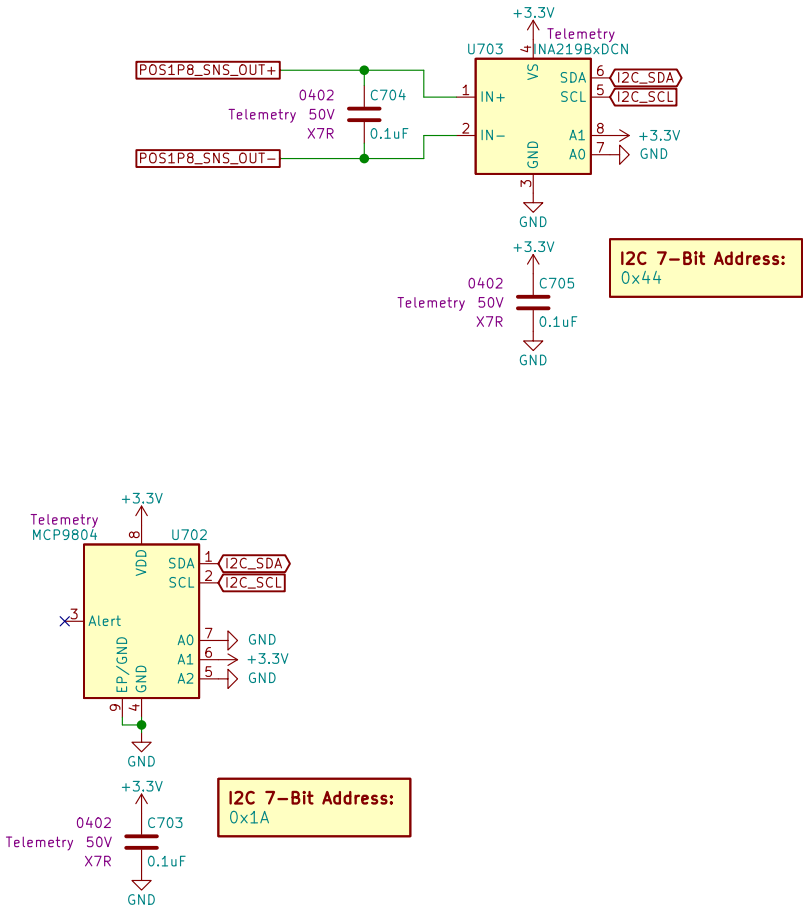

Drew Maatman		
Sheet: /+1.8V Telemetry/		
File: POS1P8_Telemetry.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020−12−09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)−1		Id: 7/21

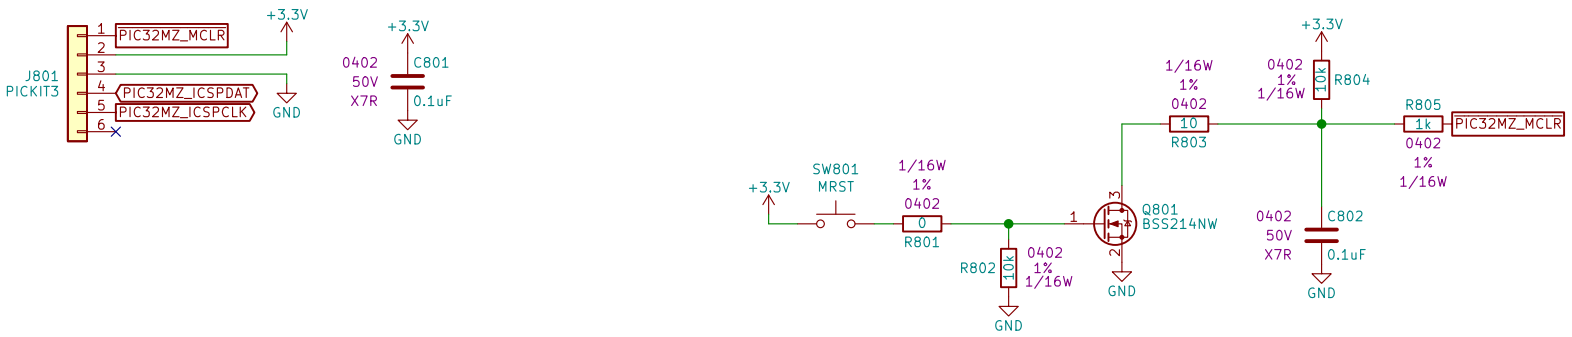

Drew Maatman		
Sheet: /PIC32MZ Programming/		
File: PIC32MZ_Programming.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 8/21

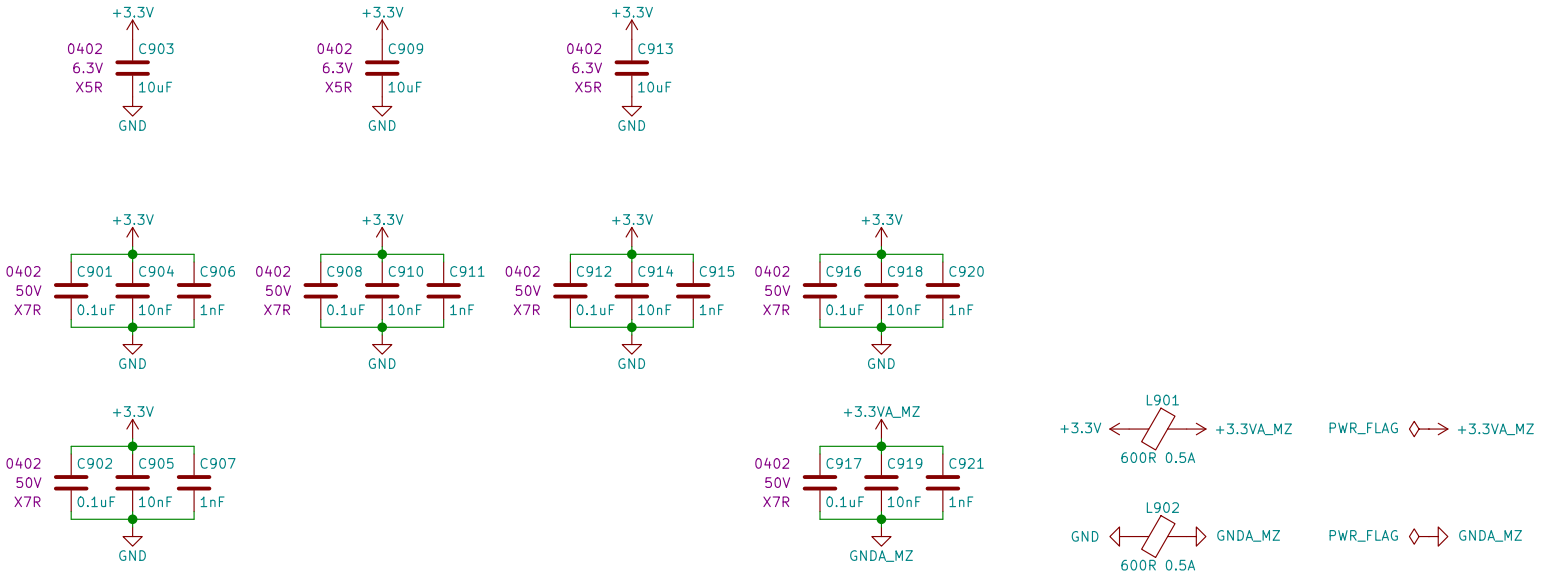

Drew Maatman		
Sheet: /PIC32MZ Bypass/		
File: PIC32MZ_Bypass.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 9/21

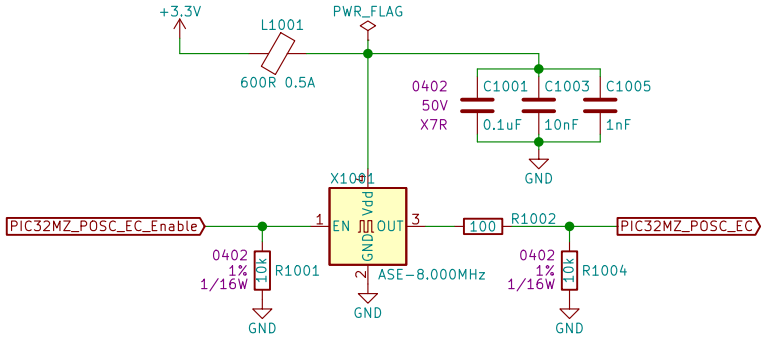



Drew Maatman		
Sheet: /PIC32MZ Clocking/		
File: PIC32MZ_Clocking.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 10/21

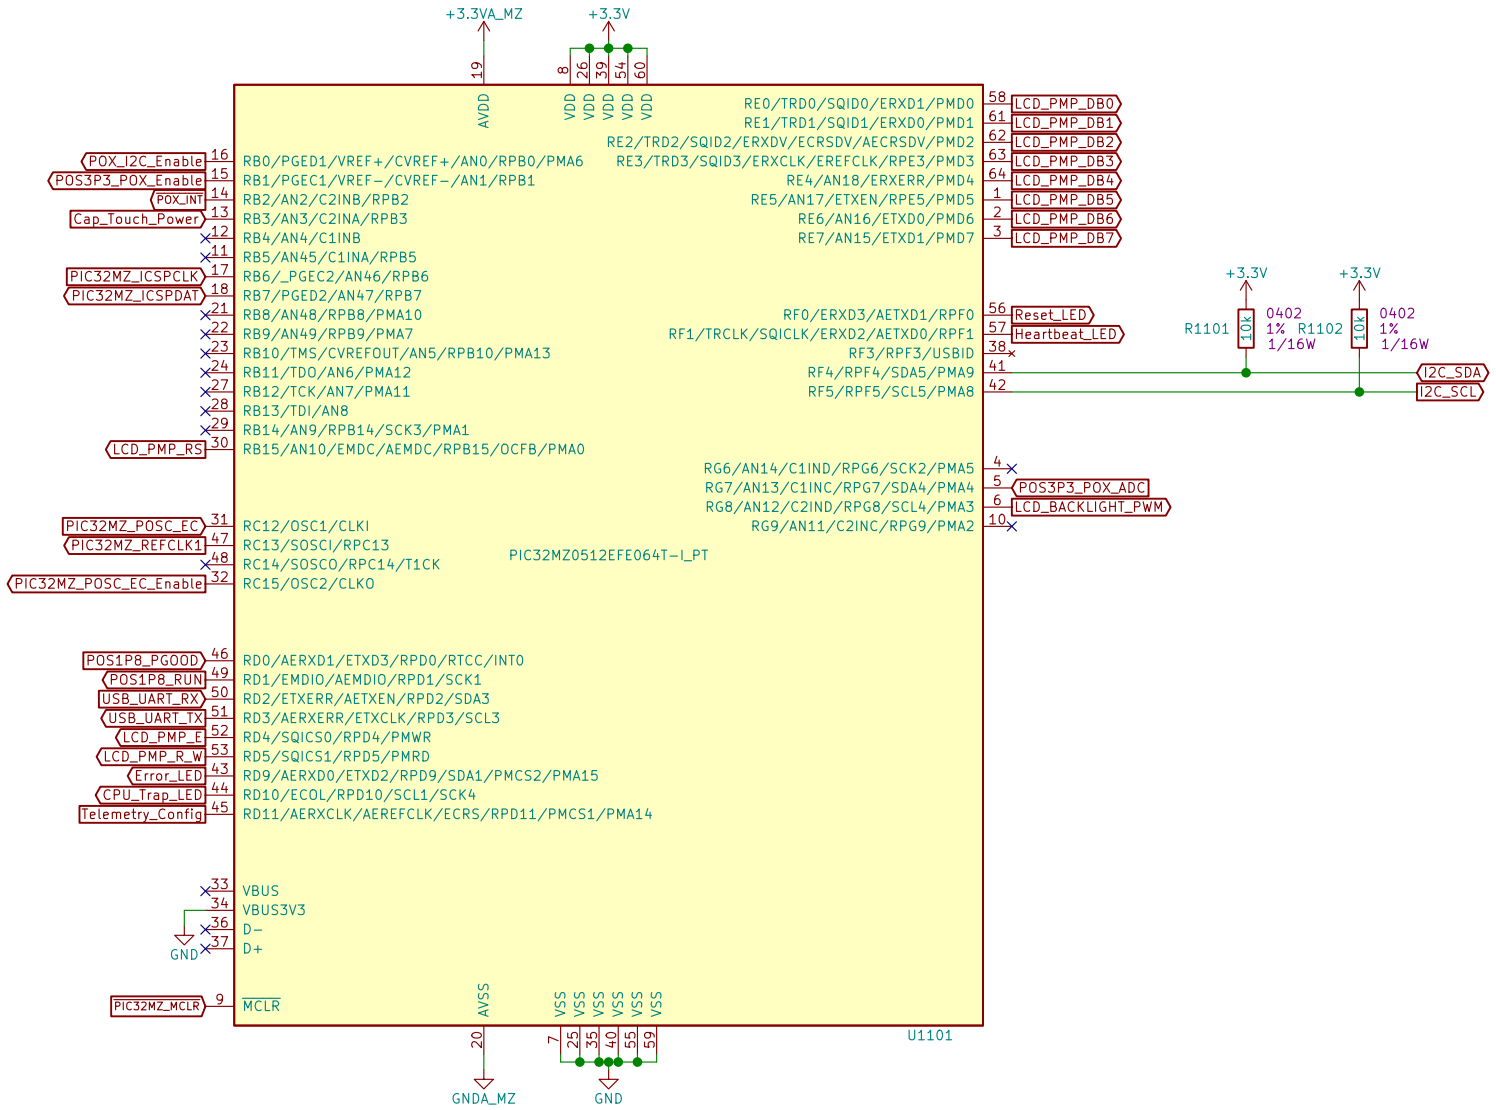

Drew Maatman		
Sheet: /PIC32MZ/		
File: PIC32MZ.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 11/21

ECO: Run a modwire from +3.3V to +5V_USB somewhere, and ensure L1201 is non-popped

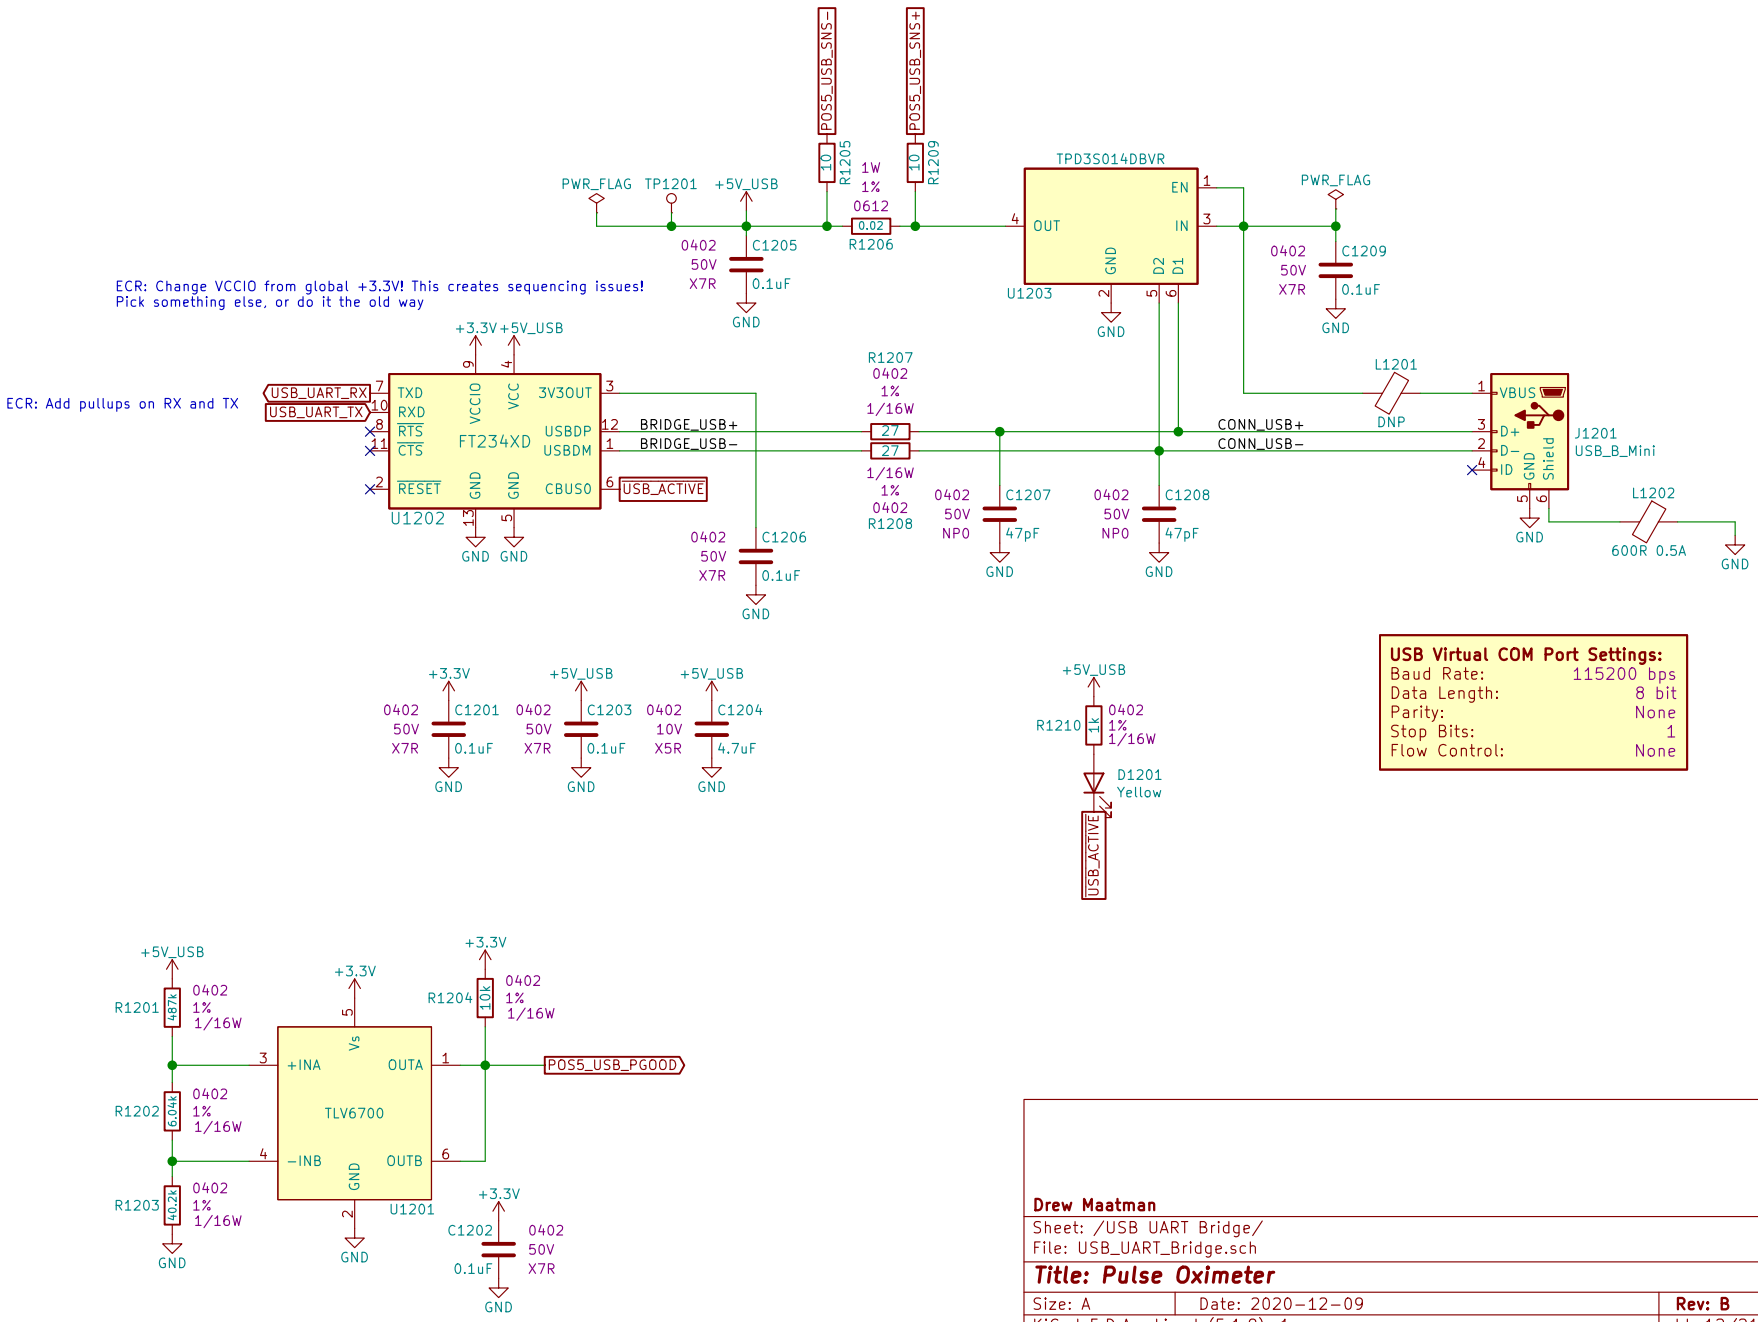

Drew Maatman	
Sheet: /USB UART Bridge/	
File: USB_UART_Bridge.sch	
Title: Pulse Oximeter	
Size: A	Date: 2020-12-09
KiCad E.D.A. kicad (5.1.8)-1	Id: 12/21

Rev: B

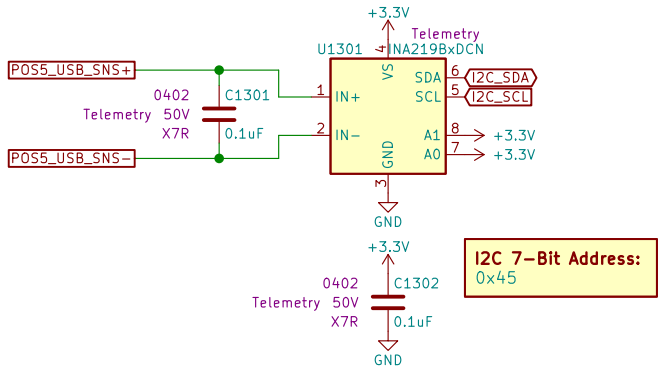

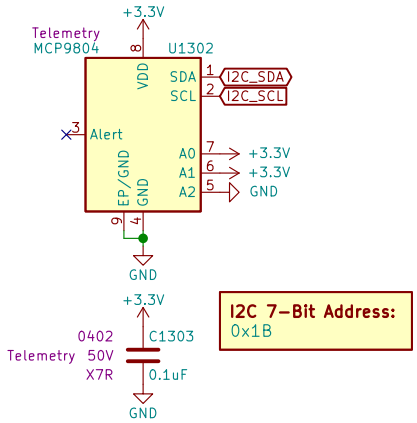

Drew Maatman		
Sheet: /USB Telemetry/		
File: USB_Telemetry.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 13/21

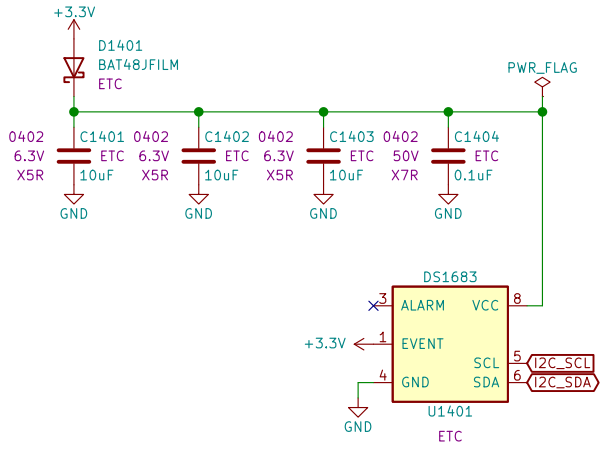

Drew Maatman		
Sheet: /Platform ETC/		
File: Platform_ETC.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 14/21

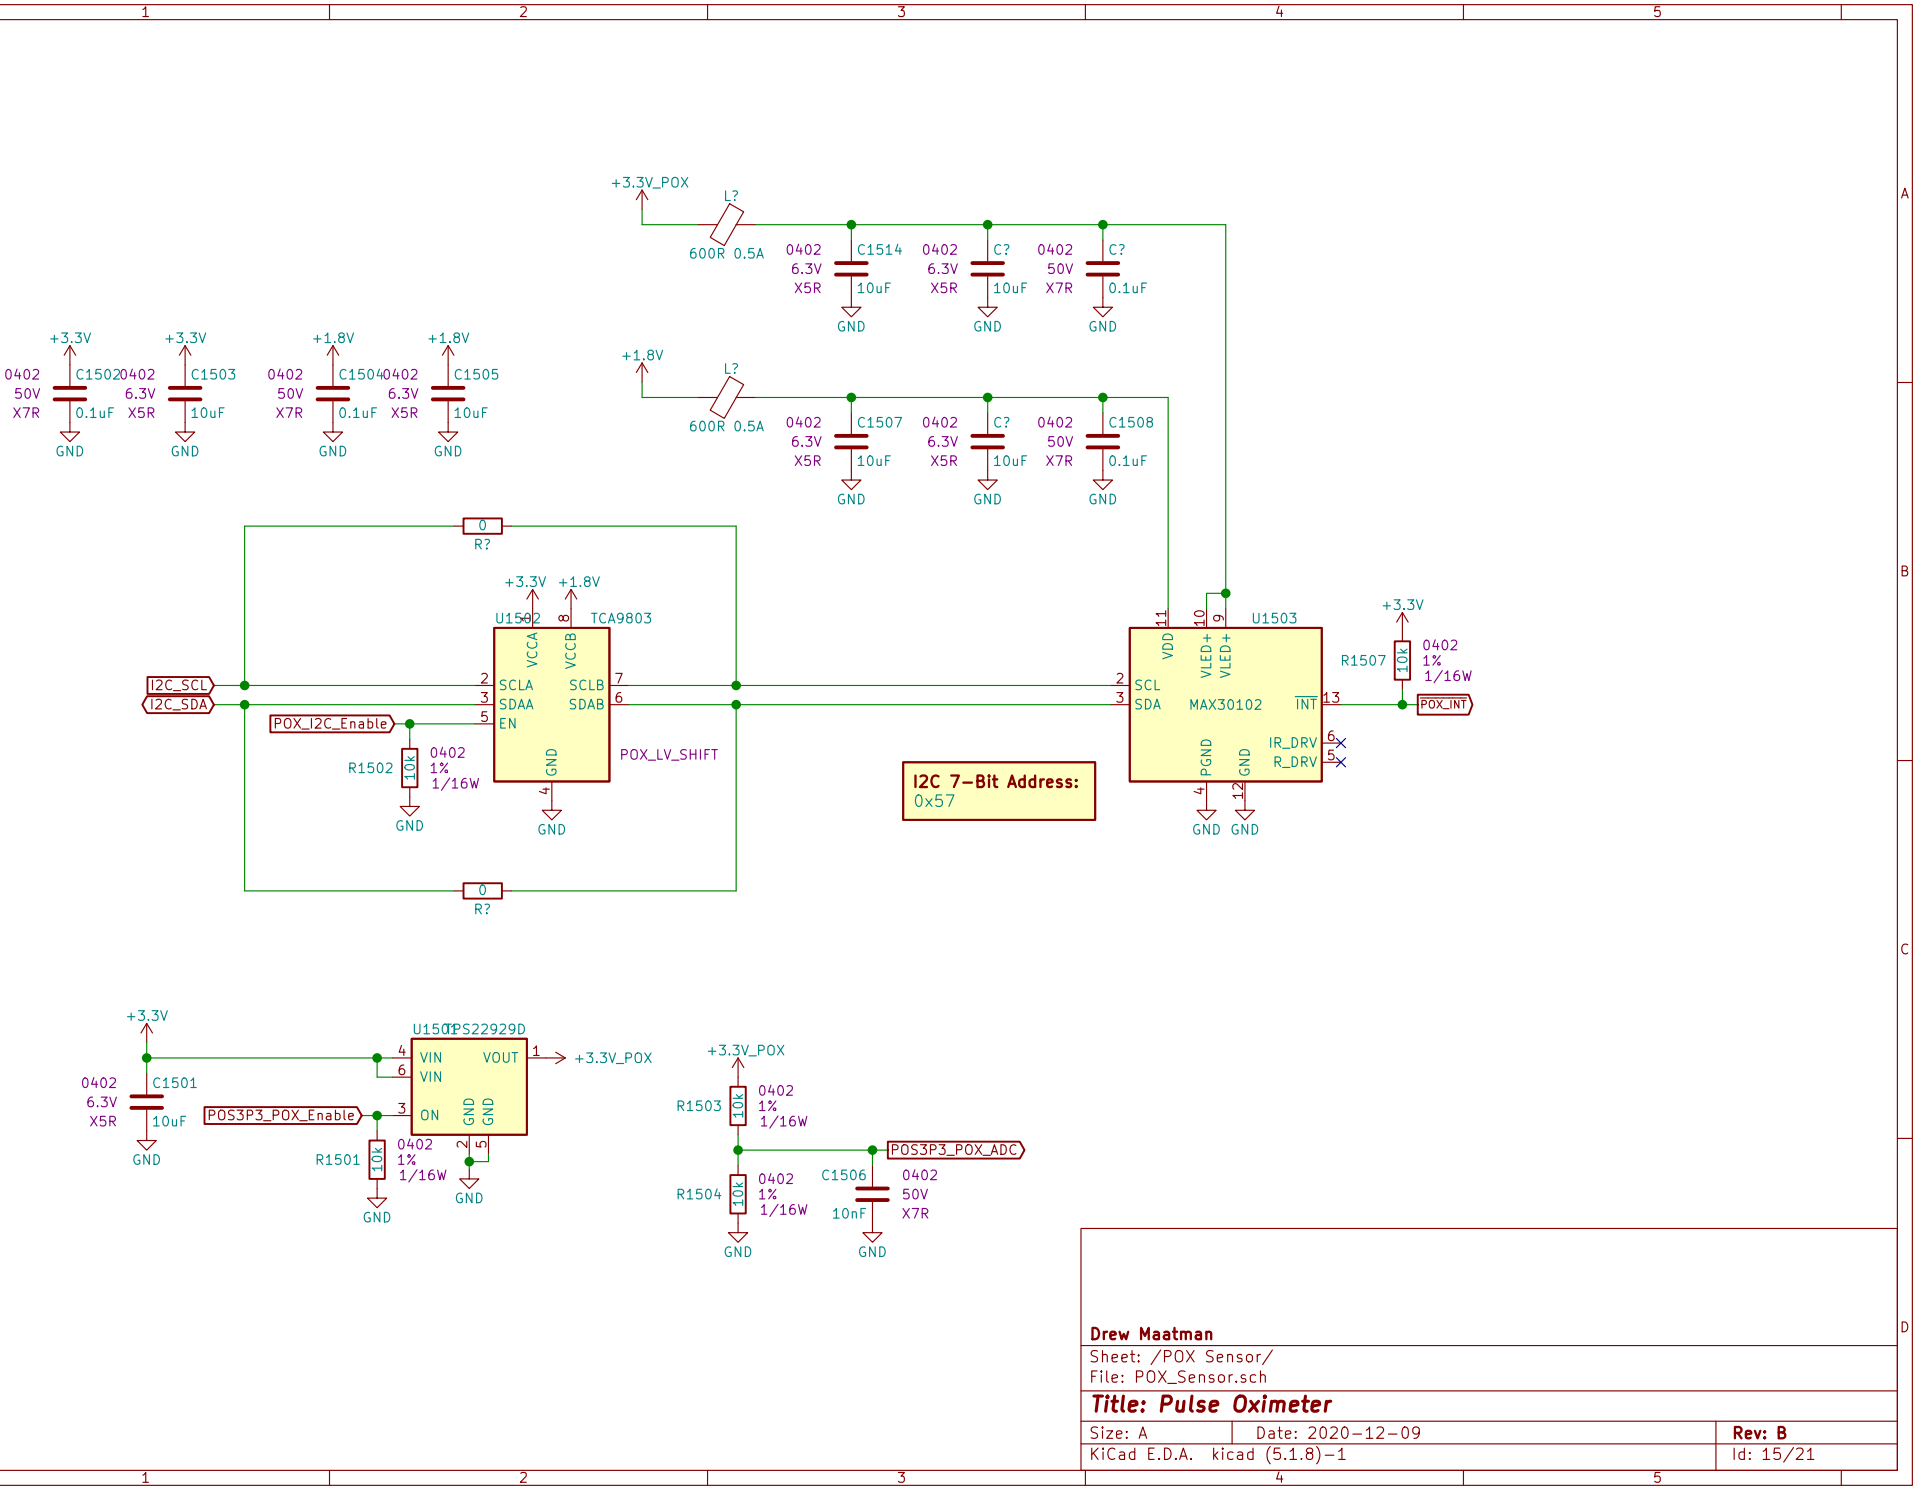

Drew Maatman	
Sheet: /POX Sensor/	
File: POX_Sensor.sch	
Title: Pulse Oximeter	
Size: A	Date: 2020-12-09
KiCad E.D.A. kicad (5.1.8)-1	Id: 15/21
	Rev: B

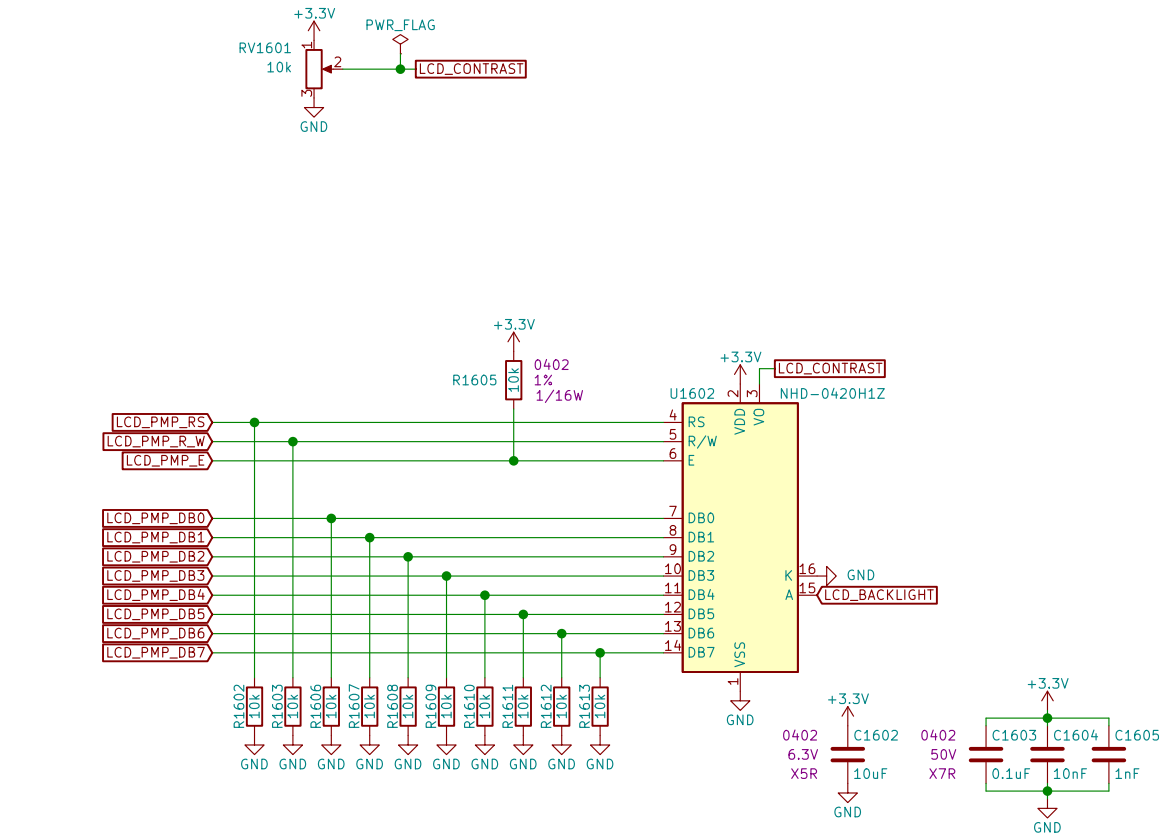

Drew Maatman		
Sheet: /Display/		
File: Display.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 16/21

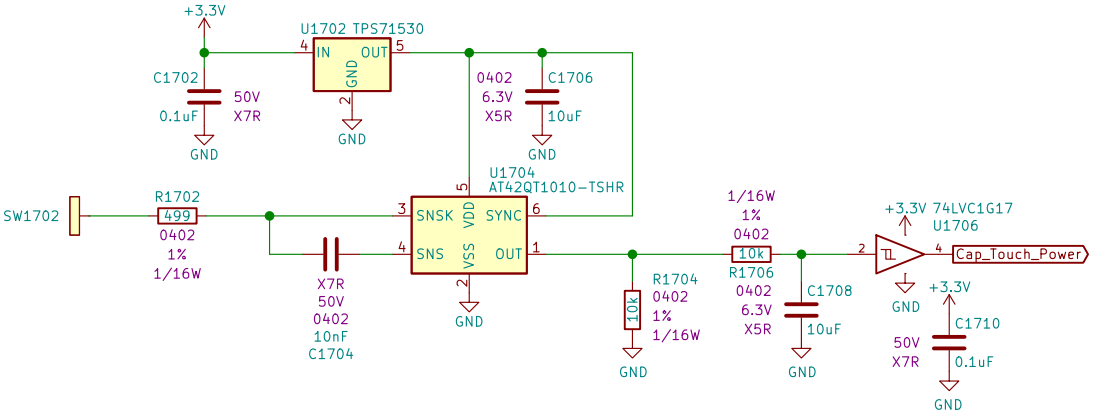

Drew Maatman		
Sheet: /Pushbuttons/		
File: Pushbuttons.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 17/21

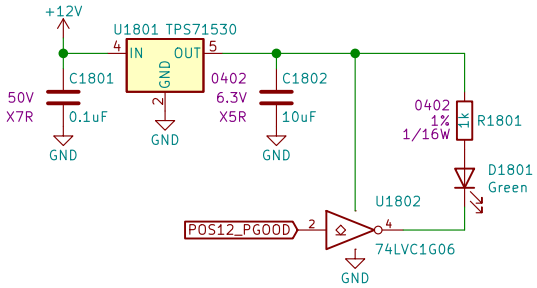

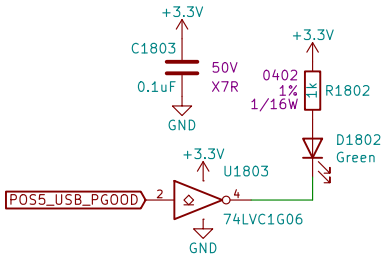

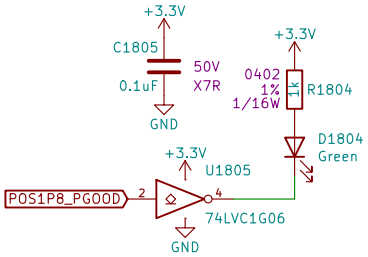

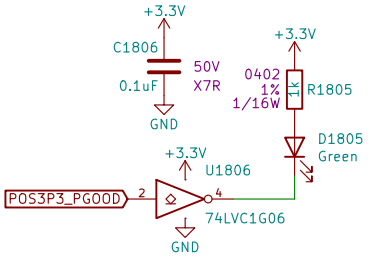

Drew Maatman		
Sheet: /PGOOD LEDs/		
File: PGOOD_LEDs.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 18/21

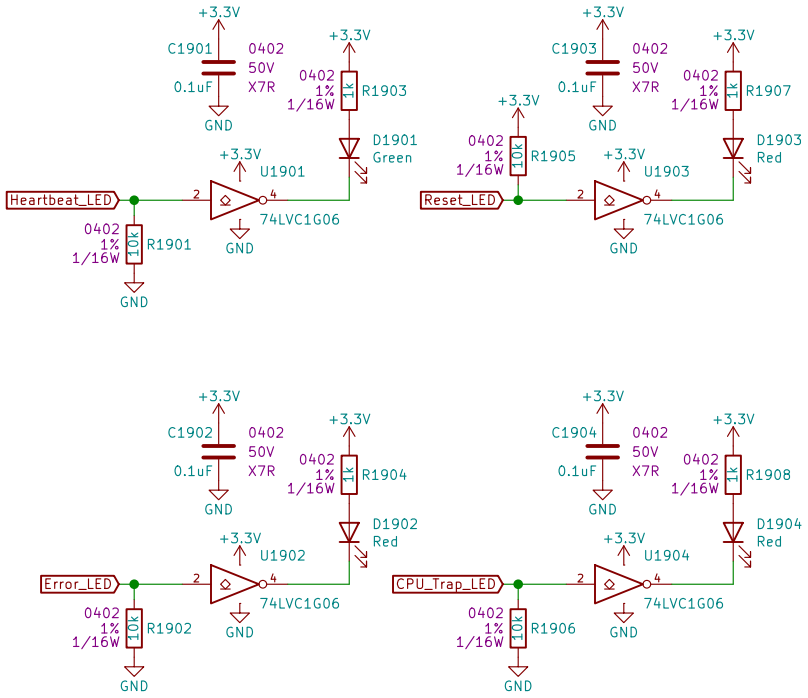

Drew Maatman

Sheet: /Status LEDs/
File: Status_LEDs.sch

Title: Pulse Oximeter

Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 19/21

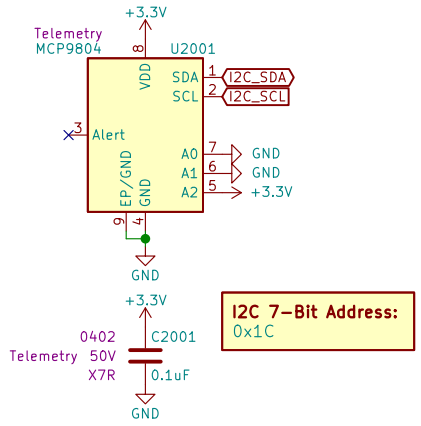

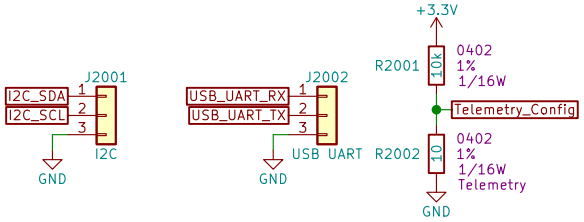

Drew Maatman		
Sheet: /Misc Circuits/		
File: Misc_Circuits.sch		
Title: Pulse Oximeter		
Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 20/21



Drew Maatman

Sheet: /Mechanical/
File: Mechanical.sch

Title: Pulse Oximeter

Size: A	Date: 2020-12-09	**Rev: B**
KiCad E.D.A. kicad (5.1.8)-1		Id: 21/21