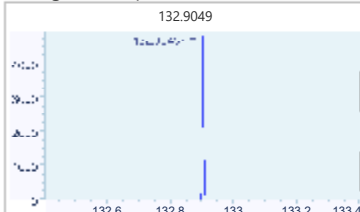
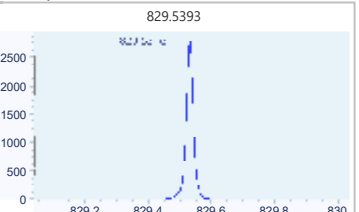
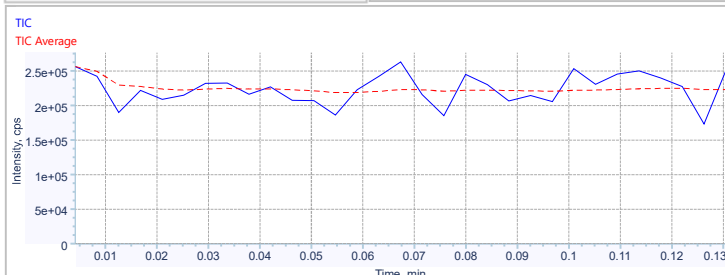


Instrument Name: ZenoTOF™ 7600 System LC200
Instrument Model: ZenoTOF 7600 System
Ion Source: OptiFlow 1-50µL Micro/MicroCal
Serial Number: FB24962403

Manufacturer: AB Sciex
Target Instrument: ZenoTOF 7600 System
Optimization Set: Positive Quick Status Check

1. Positive MS Check

Step	Result	Details																														
Achieve Stable Spray / Modify	Pass	Slope: 0.000490049587902451, previous was 0.000490049587902451 Delay: -13.5686877965015, previous was -13.5686877965015																														
Average of 30 spectra - Confirmation Mode Complete																																
																																
<table><tr><th>Item</th><th>Min</th><th>Max</th><th>Actual</th><th>Status</th></tr><tr><td>Mass (Da)</td><td>132.8049</td><td>133.0049</td><td>132.9046</td><td>Pass</td></tr><tr><td>Sum Intensity (cps)</td><td>1000</td><td>1e+11</td><td>21609</td><td>Pass</td></tr></table>	Item	Min	Max	Actual	Status	Mass (Da)	132.8049	133.0049	132.9046	Pass	Sum Intensity (cps)	1000	1e+11	21609	Pass	<table><tr><th>Item</th><th>Min</th><th>Max</th><th>Actual</th><th>Status</th></tr><tr><td>Mass (Da)</td><td>829.4393</td><td>829.6393</td><td>829.5316</td><td>Pass</td></tr><tr><td>Sum Intensity (cps)</td><td>1000</td><td>1e+11</td><td>26952</td><td>Pass</td></tr></table>	Item	Min	Max	Actual	Status	Mass (Da)	829.4393	829.6393	829.5316	Pass	Sum Intensity (cps)	1000	1e+11	26952	Pass	
Item	Min	Max	Actual	Status																												
Mass (Da)	132.8049	133.0049	132.9046	Pass																												
Sum Intensity (cps)	1000	1e+11	21609	Pass																												
Item	Min	Max	Actual	Status																												
Mass (Da)	829.4393	829.6393	829.5316	Pass																												
Sum Intensity (cps)	1000	1e+11	26952	Pass																												
																																

Channel Alignment

Sum of 10 spectra

132.9049

Intensity, cps

</

Instrument Name: ZenoTOF™ 7600 System LC200
Instrument Model: ZenoTOF 7600 System
Ion Source: OptiFlow 1-50µL Micro/MicroCal
Serial Number: FB24962403


Manufacturer: AB Sciex
Target Instrument: ZenoTOF 7600 System
Optimization Set: Positive Quick Status Check

TOF MS Mass Check

Pass

Slope: 0.000490053135470833, previous was 0.000490049587902451
Delay: -13.4301600554897, previous was -13.5686877965015

Average of 10 spectra - Confirmation Mode Complete

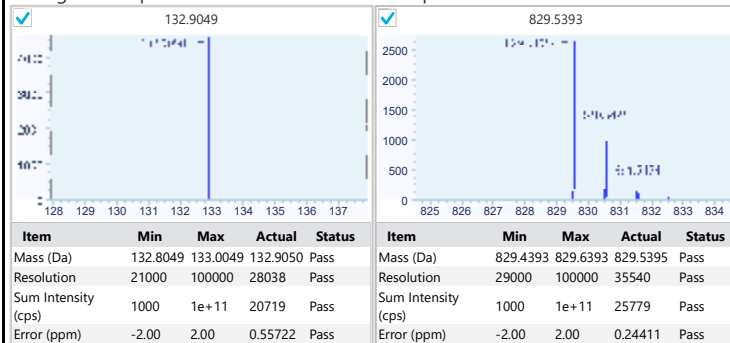


TOF MS/MS Mass Check

Pass

Slope: 0.000490052447345663, previous was 0.0004900421995101
Delay: -13.4438533137866, previous was -13.6401447945975

Average of 10 spectra - Confirmation Mode Complete

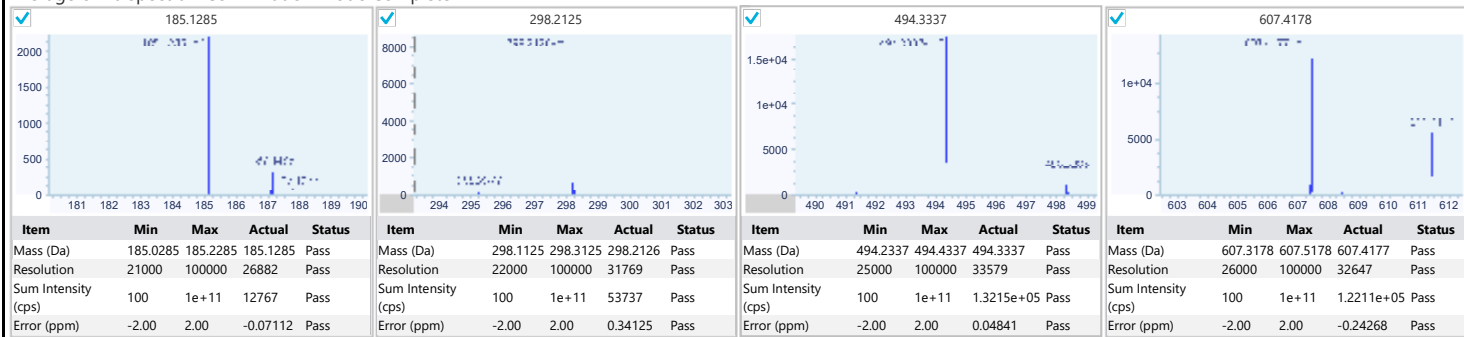

TOF MS/MS Mass Check Zeno On

Pass

Slope: 0.000490053479255802, previous was 0.000490043139071626
Delay: -13.4220185410683, previous was -13.6230843916575

Average of 10 spectra - Confirmation Mode Complete

