


# Automatic / Potentiometric Titrator

Date of Sampling: 10-Feb-25 | Time: 09:00

Specification Range	Observed Result
97.0 – 102.0 %	98.90%

## Titration Curve (mV vs mL, with equivalence point marked):

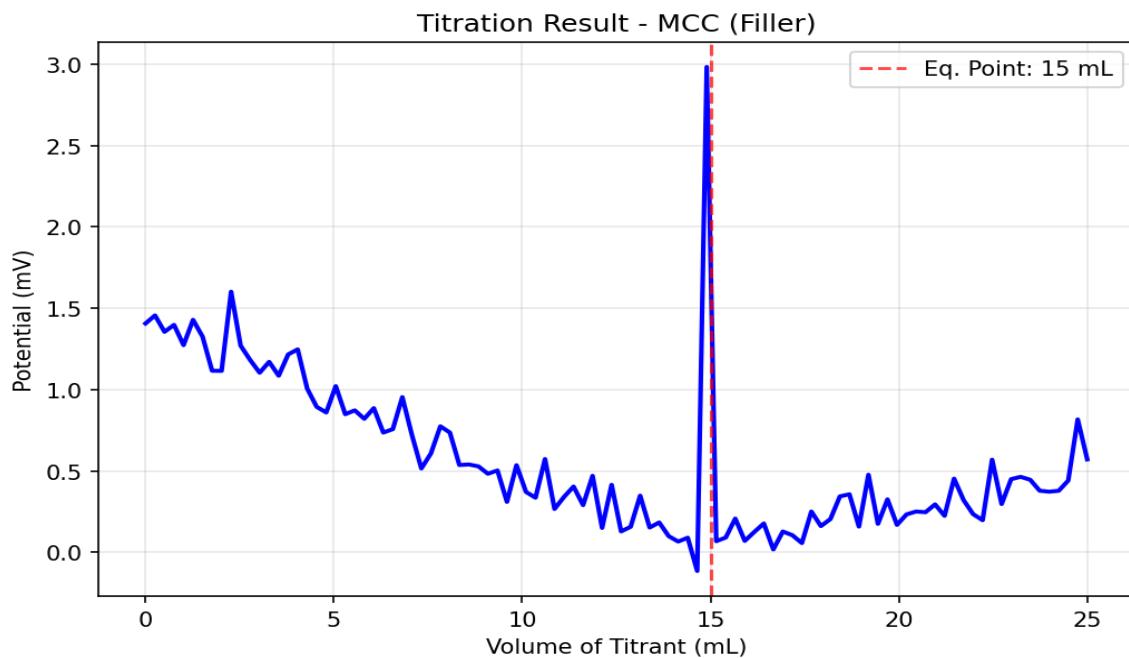

System generated | Cal Due: 2025-12-31