


Automatic / Potentiometric Titrator

Date of Sampling: 12-Feb-25 | Time: 09:00

Specification Range	Observed Result
4.0 – 5.0 % Mg	4.40%

Titration Curve (mV vs mL, with equivalence point marked):

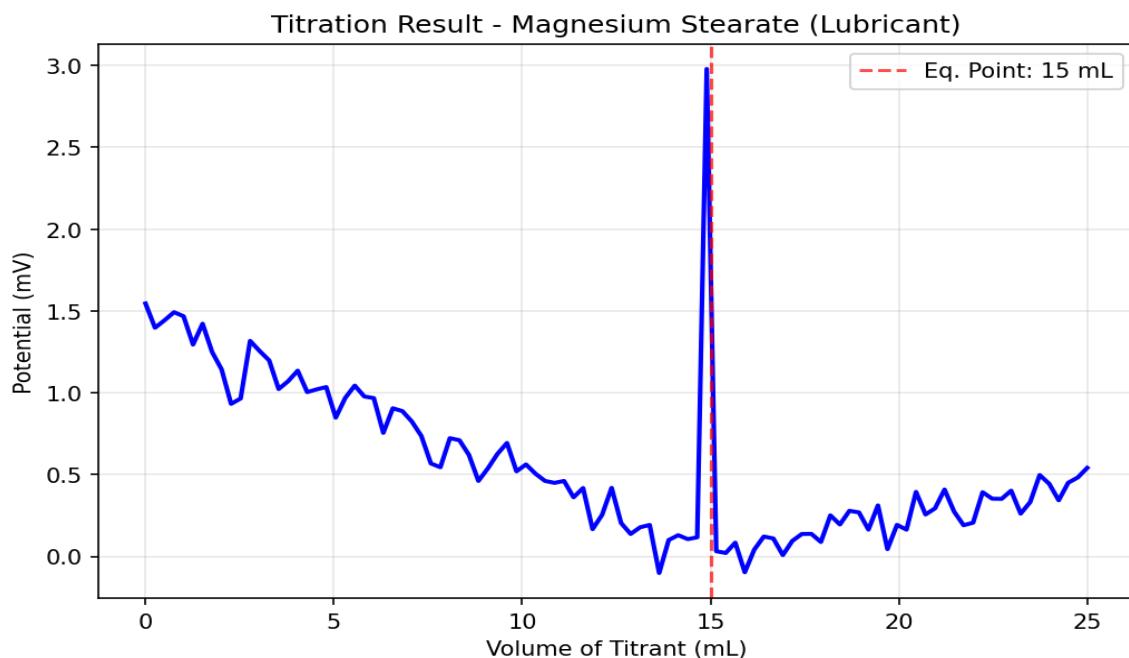

System generated | Cal Due: 2025-12-31