


FOURIER TRANSFORM INFRARED SPECTROMETER

Date of Sampling: 6-Feb-25 | Time: 09:00

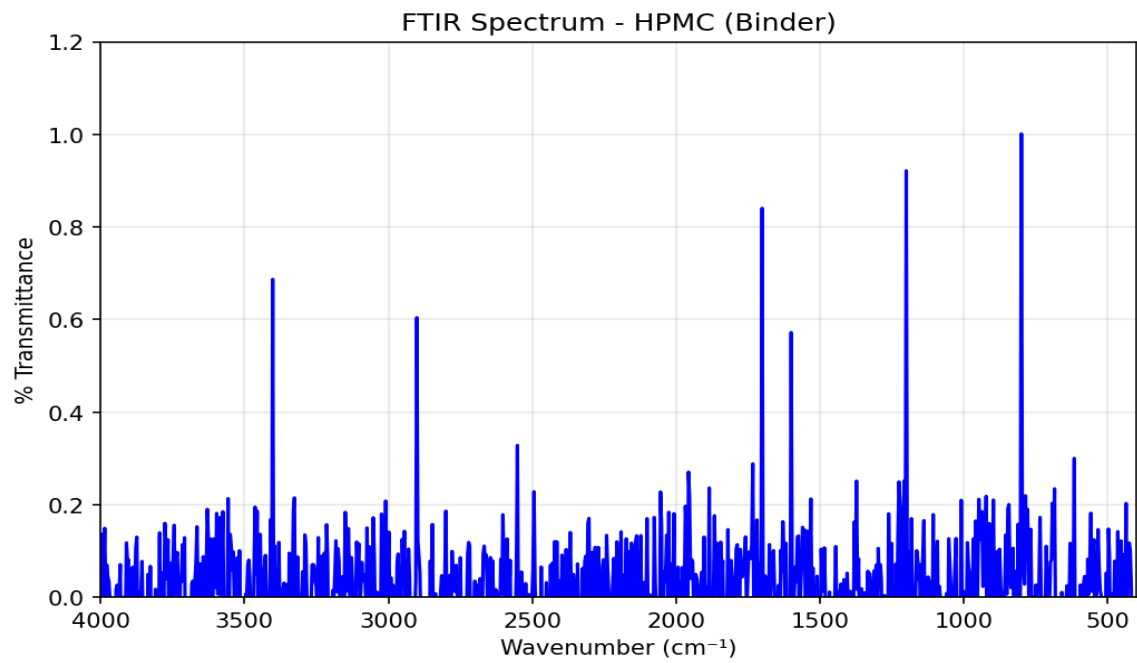

Test Parameters:

Parameter	Result	Specification
Identification	Conforms (IR Spec)	Conforms
Sample Preparation	KBr Pellet Method	Standard Method
Wavelength Range	4000 - 400 /cm	4000 - 400 /cm
Resolution	4 /cm	≤ 4 /cm
Scans	32	≥ 16

This is a system-generated printout. Calibration due: January 2026