


MELTING POINT APPARATUS

Date of Sampling: 12-Feb-25 | Time: 09:00

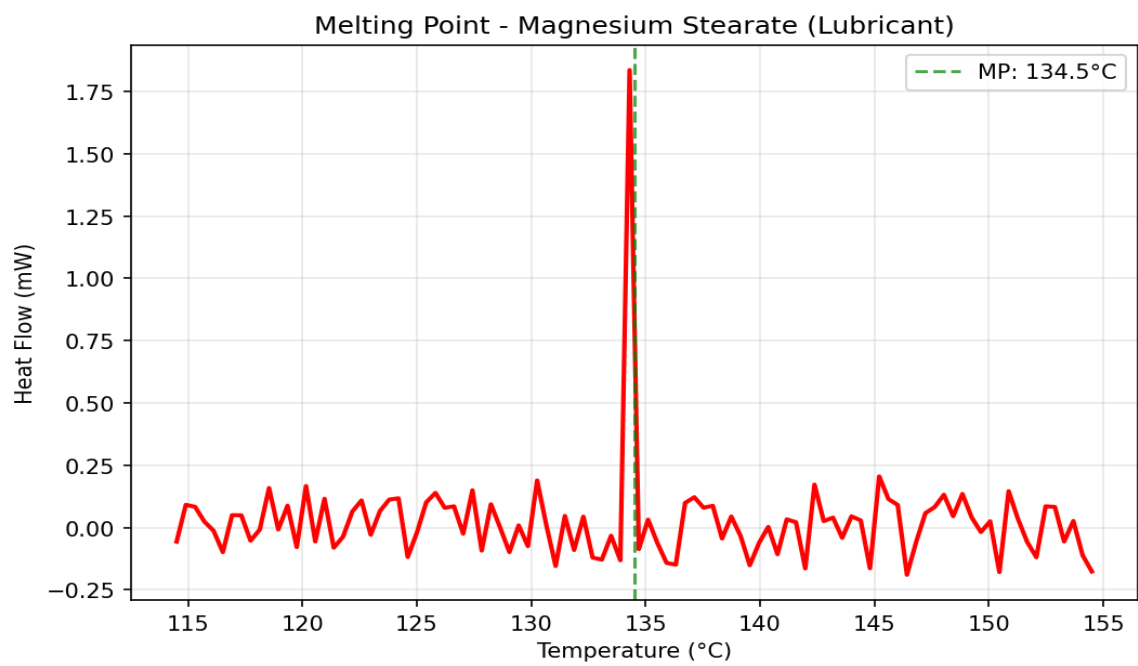

Test Parameters:

Parameter	Result	Specification
Melting Point	134.5°C – 137.2°C	As per monograph
Method	Capillary Method	USP/EP Method
Heating Rate	1°C/min	0.5 - 2°C/min
Start Temperature	100°C	Below expected MP
End Temperature	200°C	Above expected MP

This is a system-generated printout. Calibration due: January 2026