


# BULK DENSITY APPARATUS

Date of Sampling: 8-Feb-25 | Time: 09:00

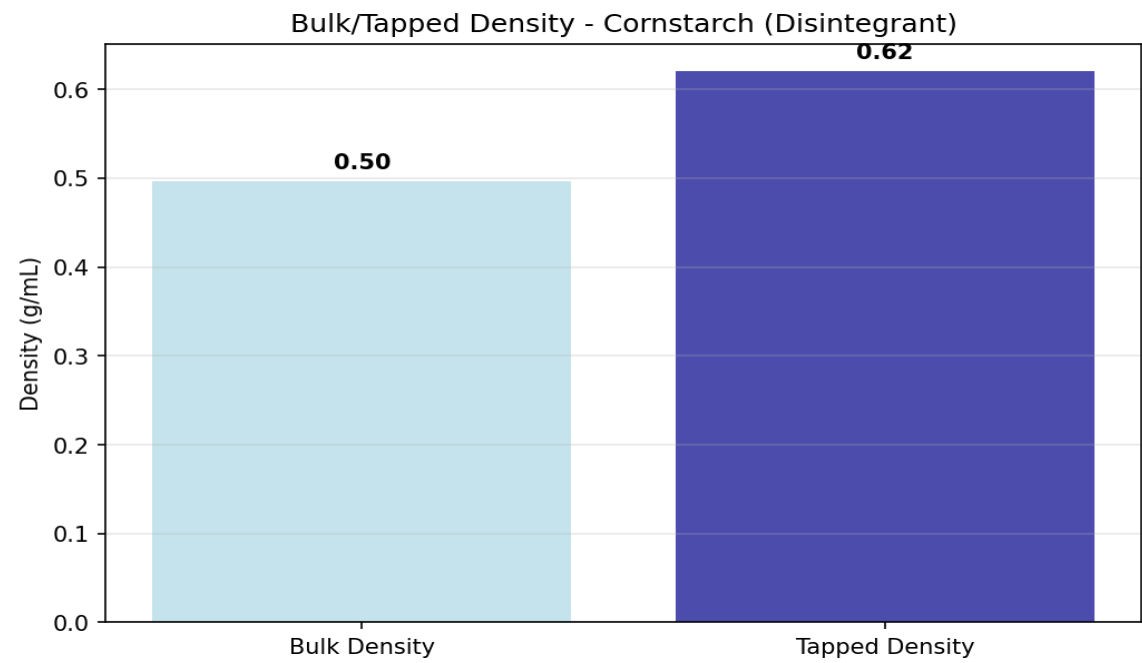

## Test Parameters:

Parameter	Result	Specification
Tapped Density	0.62 g/mL	As per monograph
Method	USP Method II	Standard Method
Tapping	1250 taps	1250 ± 50 taps

This is a system-generated printout. Calibration due: January 2026