


# Halogen Moisture Analyzer Report

Date of Sampling: 8-Feb-25

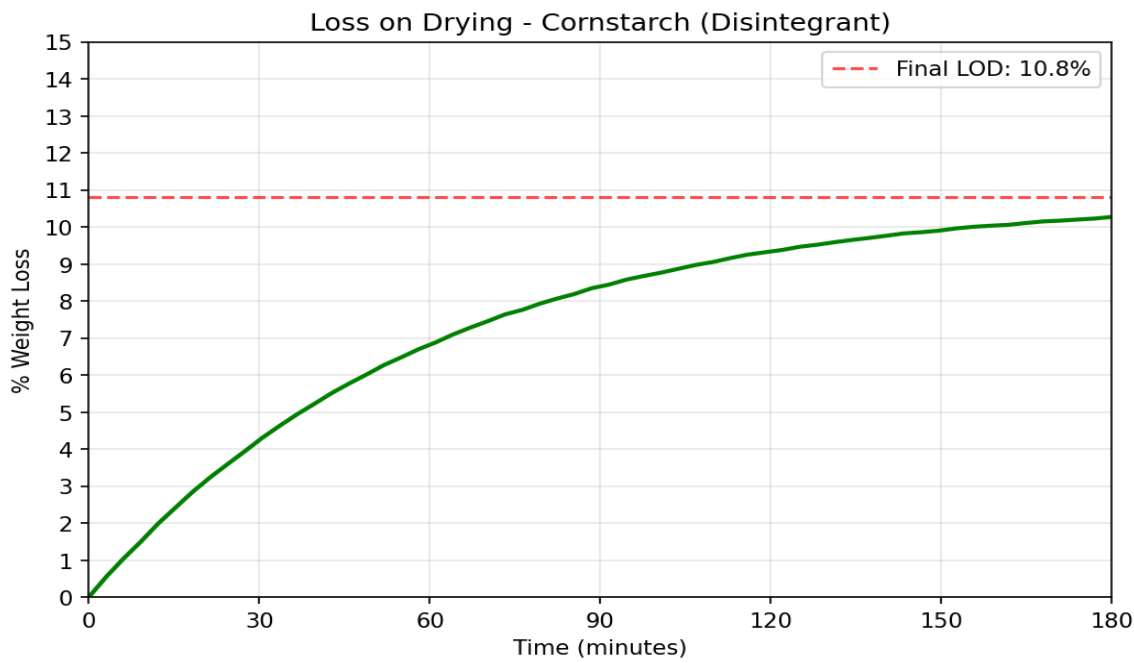

## Test Parameters:

Parameter	Result	Specification
LOD/Water Content	10.80%	As per monograph
Method	Thermogravimetric	Standard Method
Temperature	105°C ± 2°C	105°C ± 2°C

This is a system-generated printout. Calibration due: January 2026