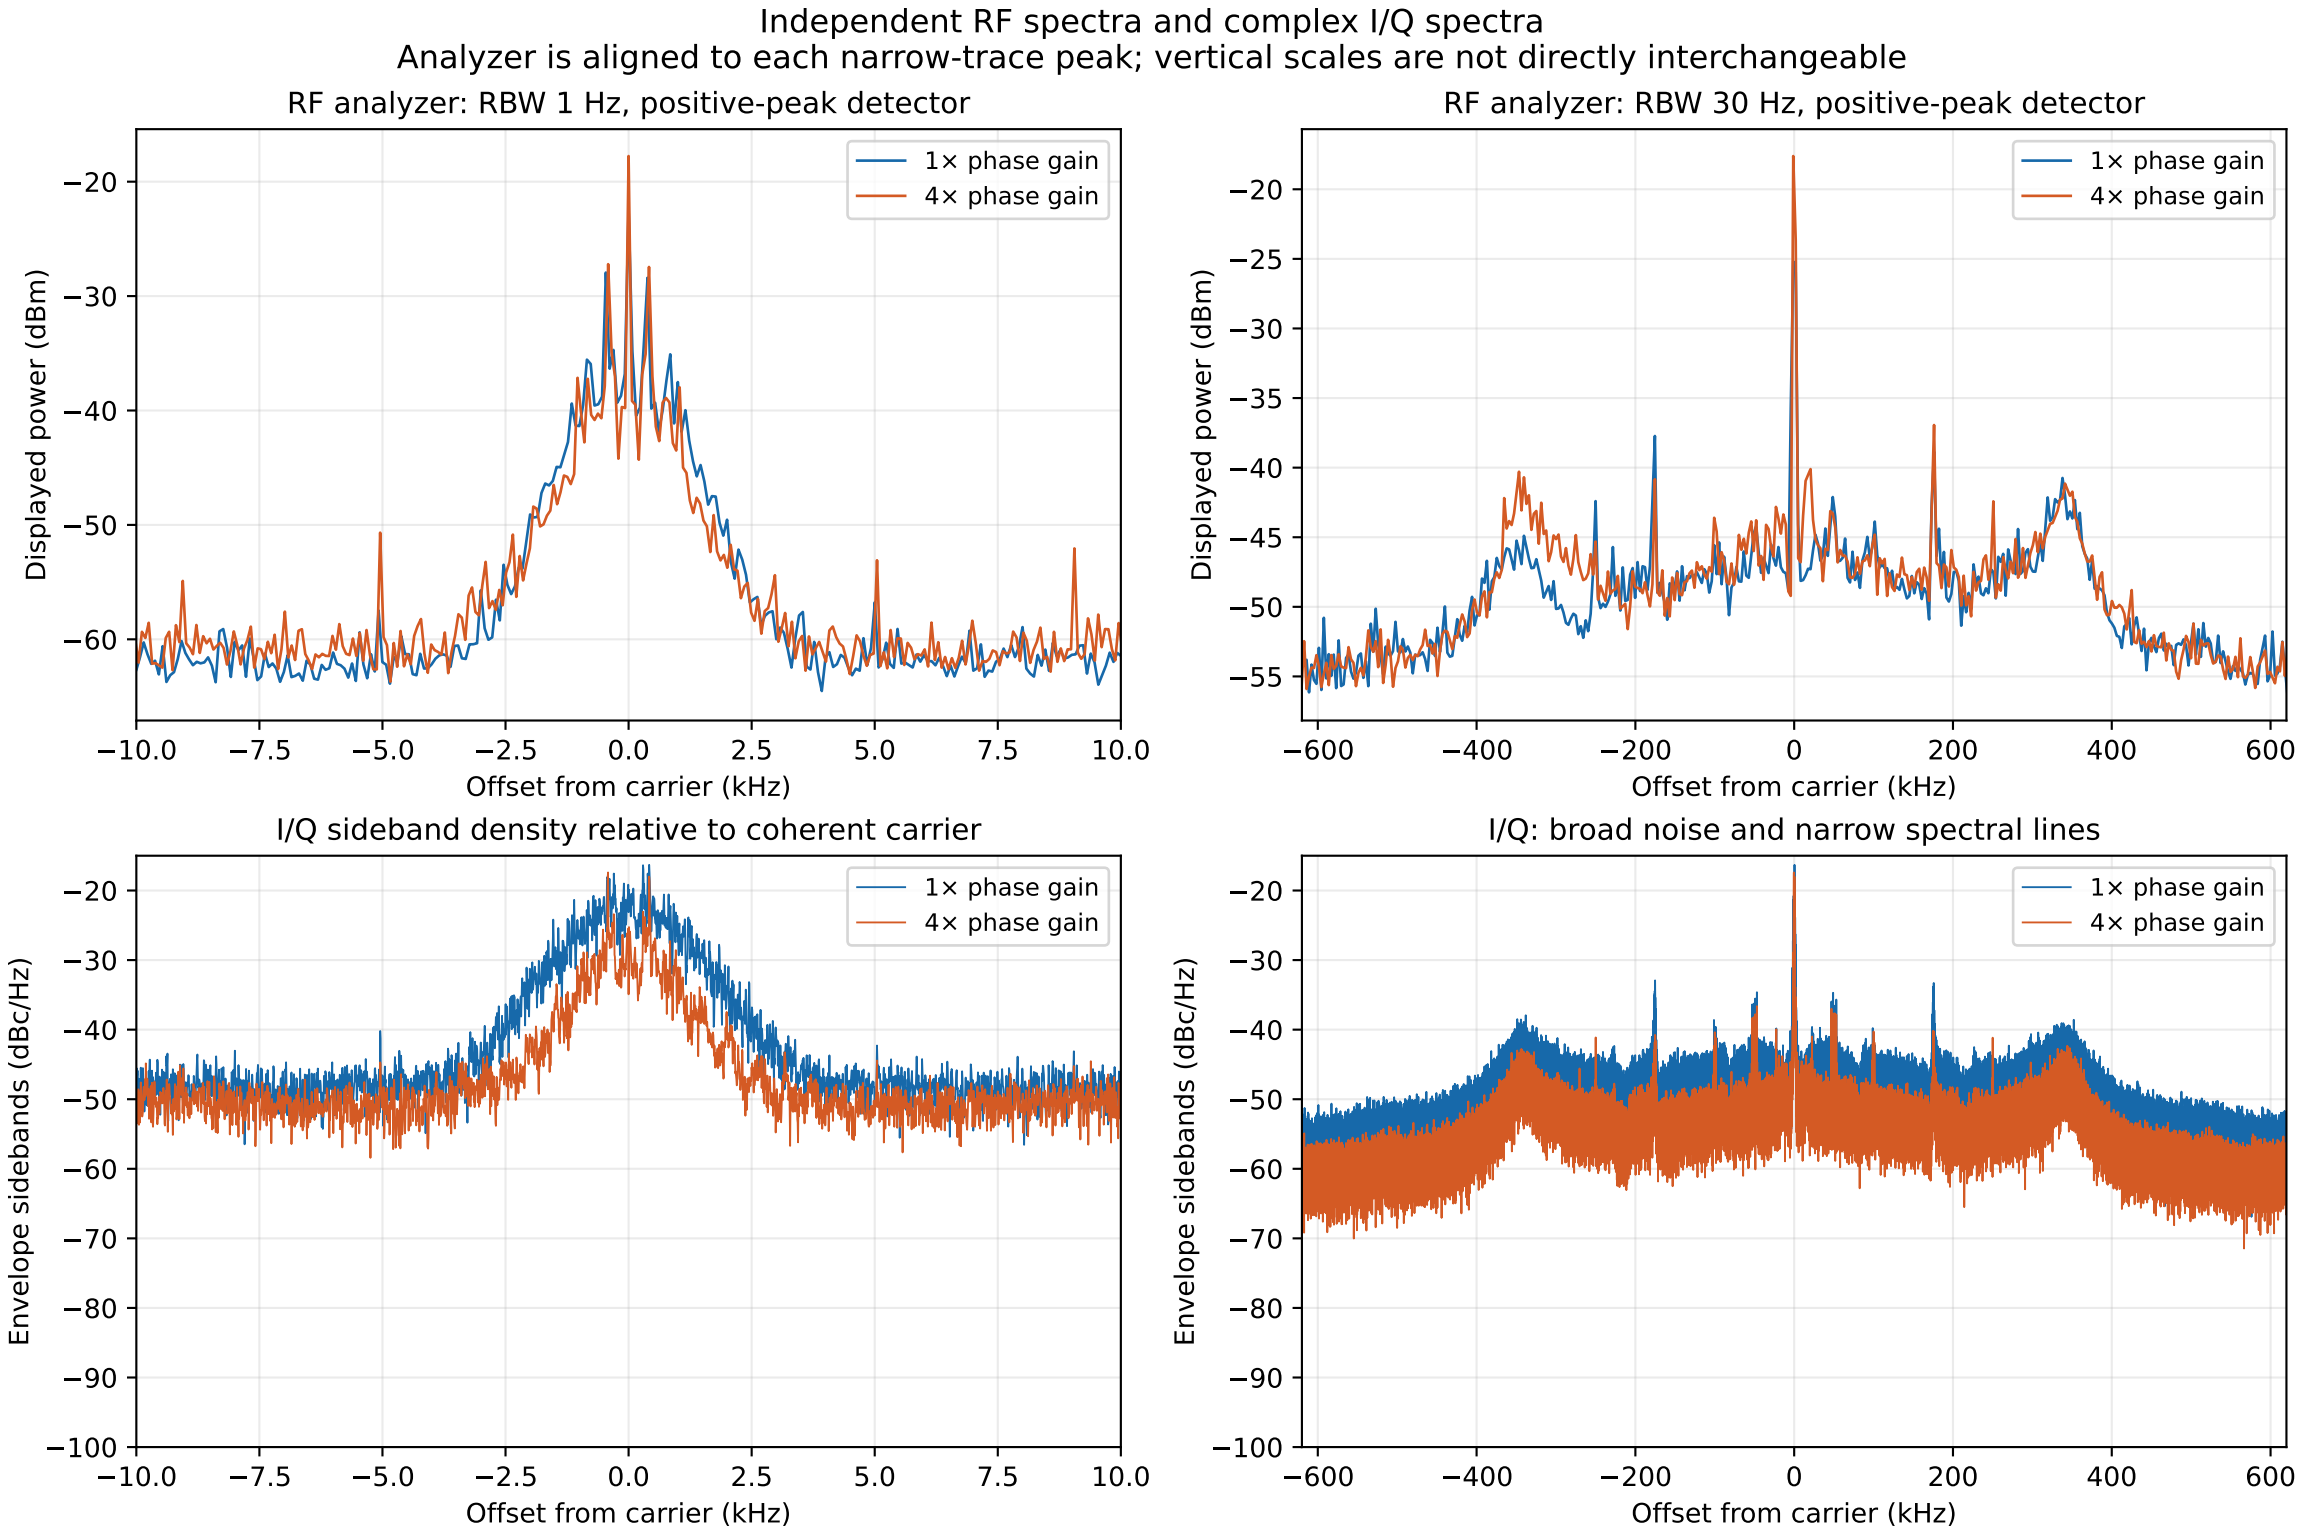

Independent RF spectra and complex I/Q spectra
Analyzer is aligned to each narrow-trace peak; vertical scales are not directly interchangeable
RF analyzer: RBW 1 Hz, positive-peak detector
RF analyzer: RBW 30 Hz, positive-peak detector
I/Q sideband density relative to coherent carrier
I/Q: broad noise and narrow spectral lines
1× phase gain
4× phase gain
Displayed power (dBm)
Envelope sidebands (dBc/Hz)
Offset from carrier (kHz)