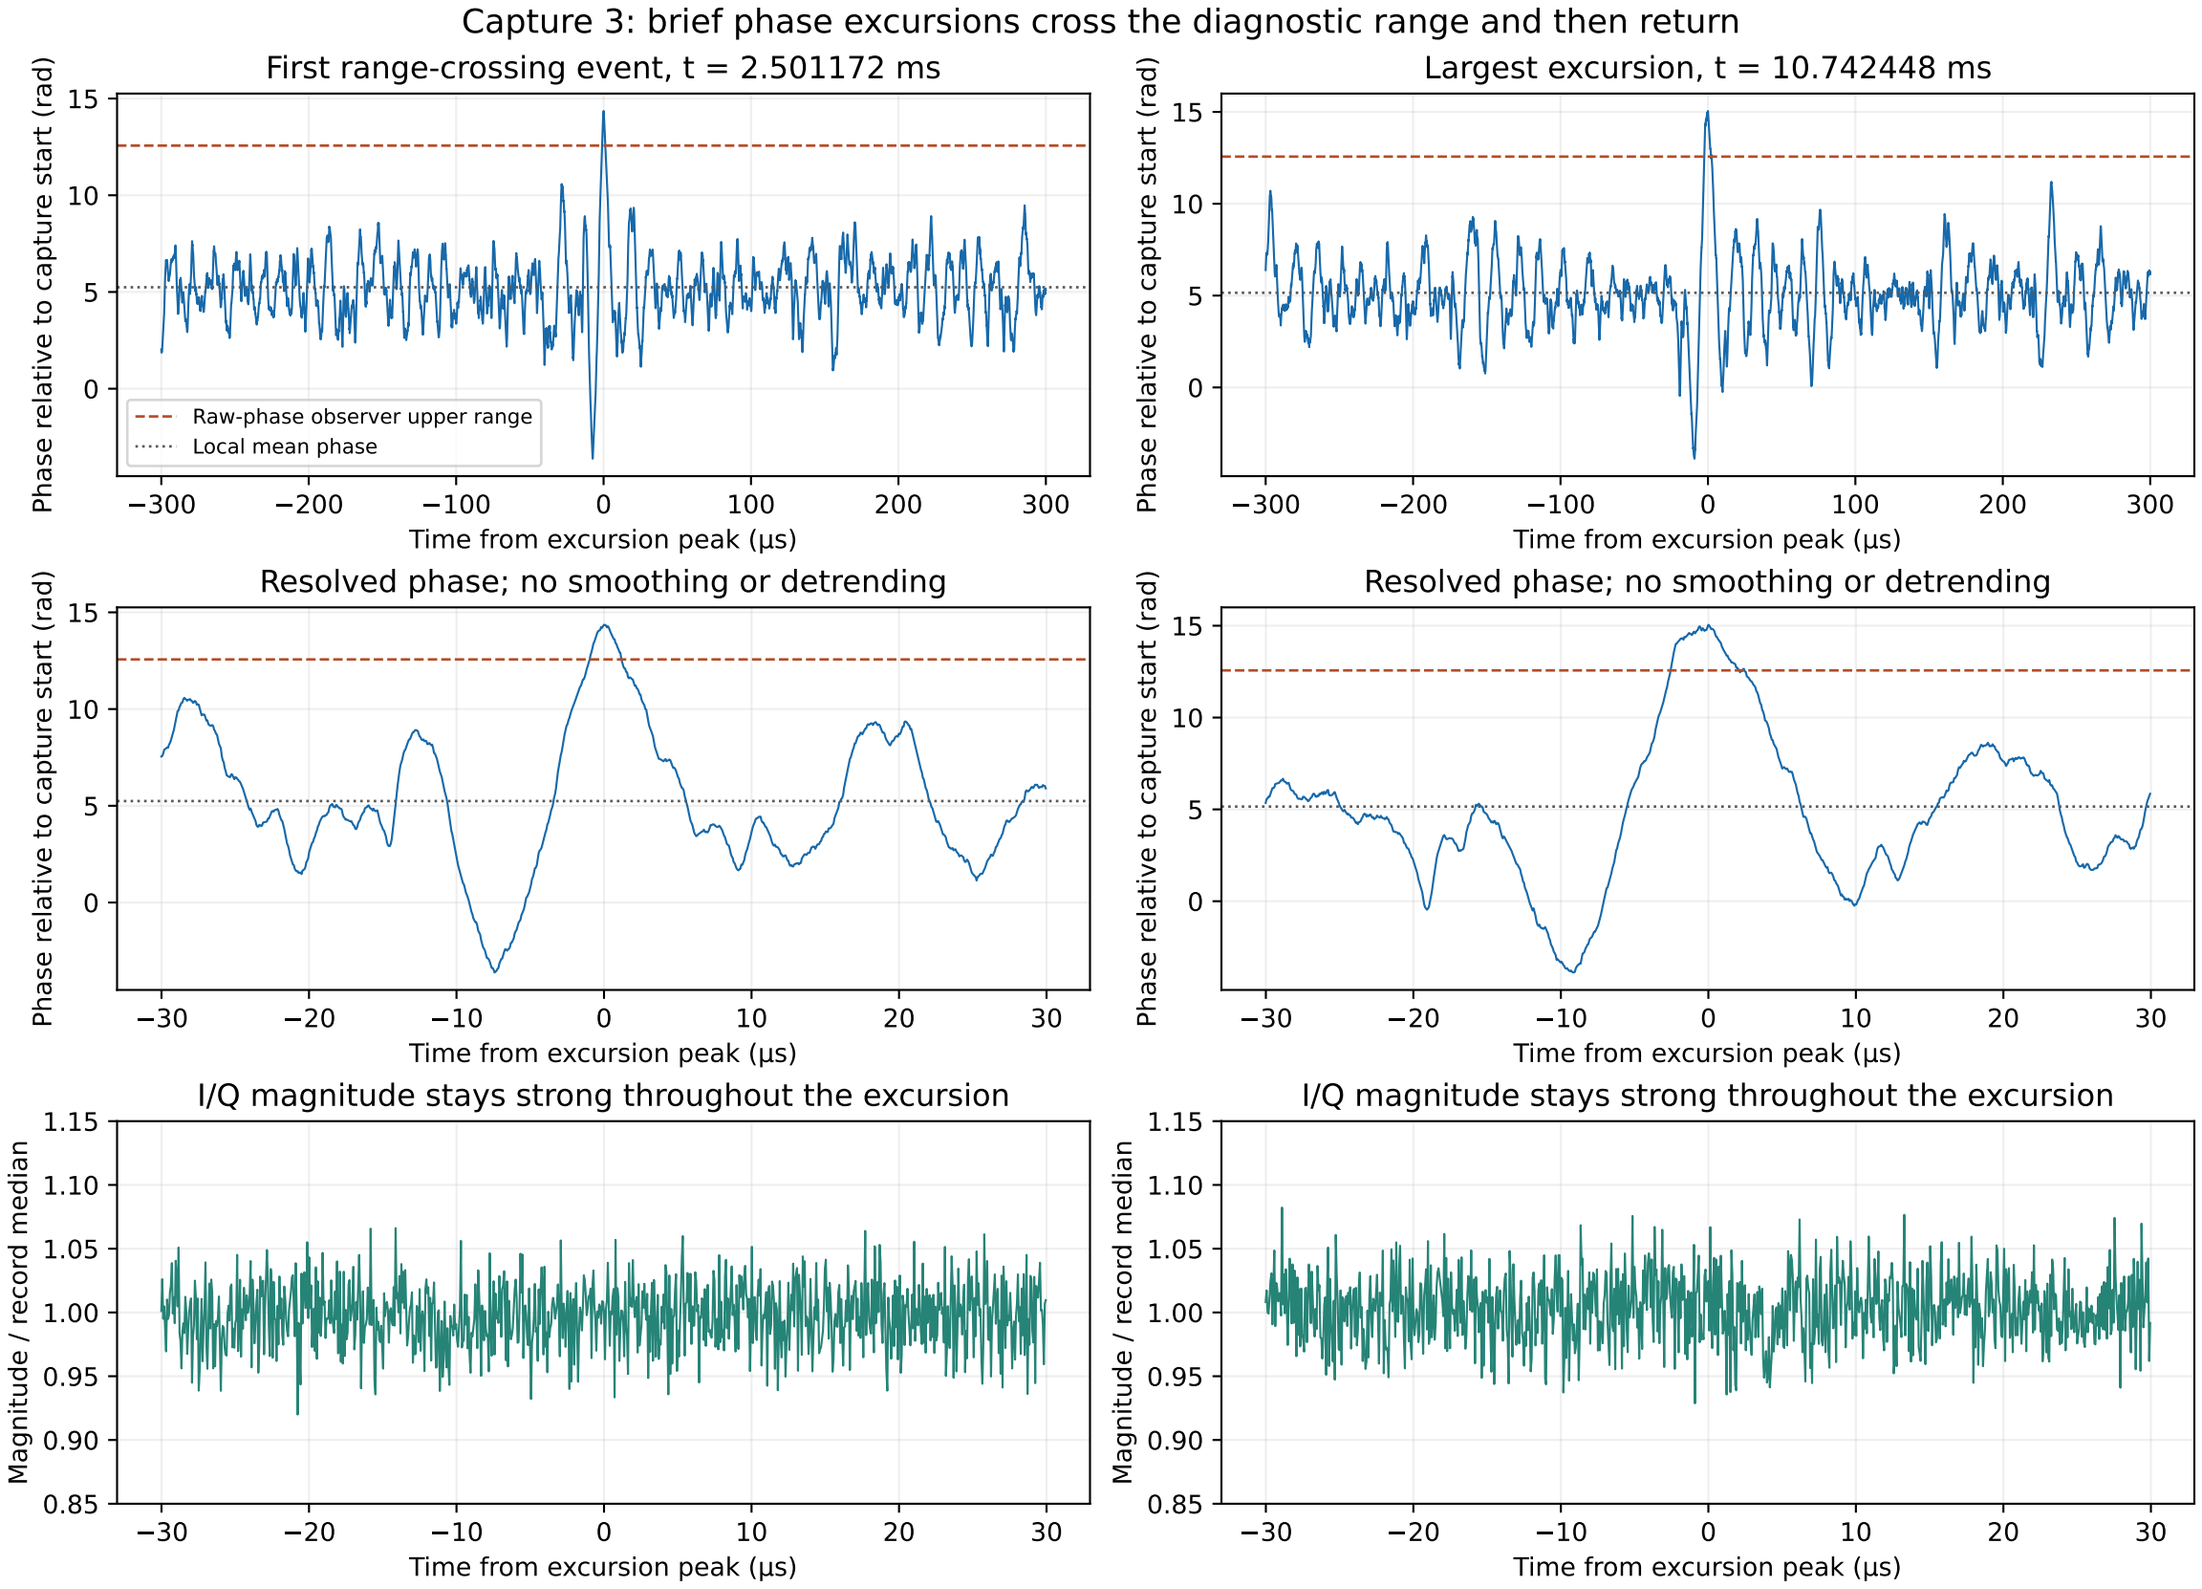

Capture 3: brief phase excursions cross the diagnostic range and then return
First range-crossing event, t = 2.501172 ms
Largest excursion, t = 10.742448 ms
Phase relative to capture start (rad)
Raw-phase observer upper range
Local mean phase
Time from excursion peak (µs)
Resolved phase; no smoothing or detrending
I/Q magnitude stays strong throughout the excursion
Magnitude / record median
Raw-phase FRA was OFF: the dashed line illustrates its ±2-turn range if armed at capture start.
These are not DAC rails. Beat phase alone cannot identify which laser caused the disturbance.