




Constant DAC code 100 · D2S output · controllers connected
No BLP; scope DC-coupled, bandwidth limit believed off. Instrument backgrounds not measured.

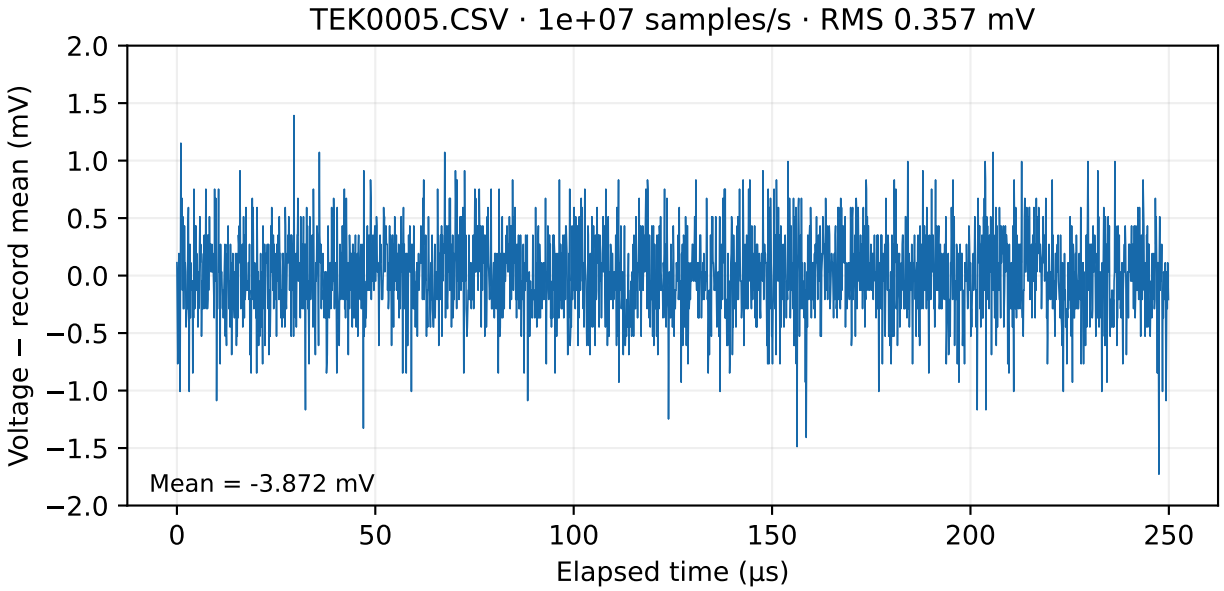


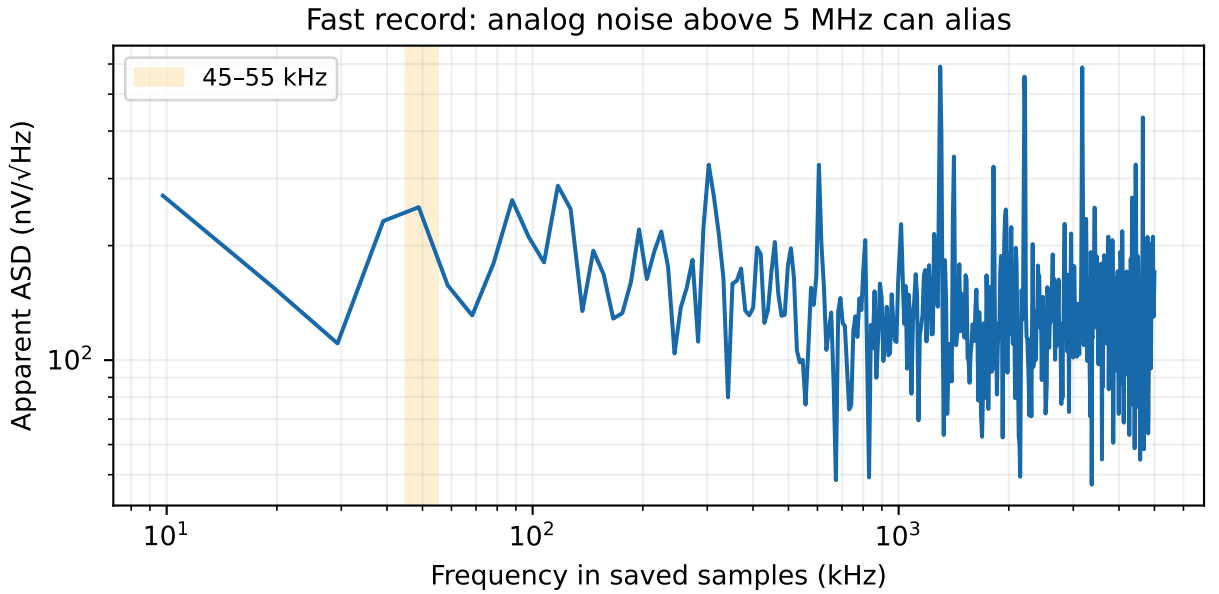

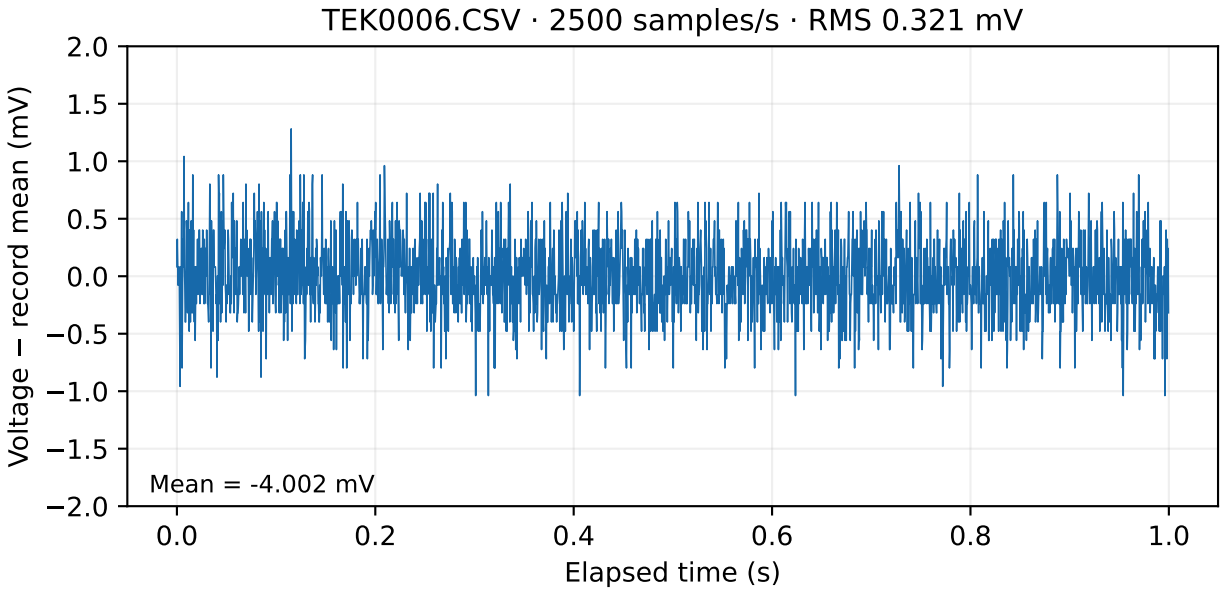

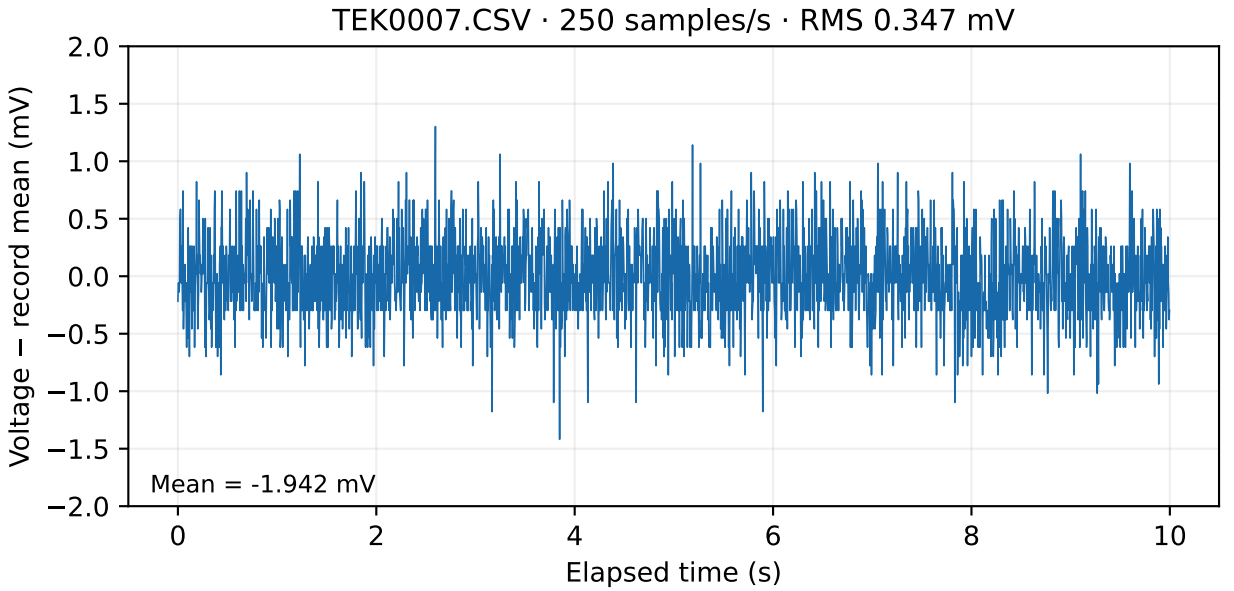

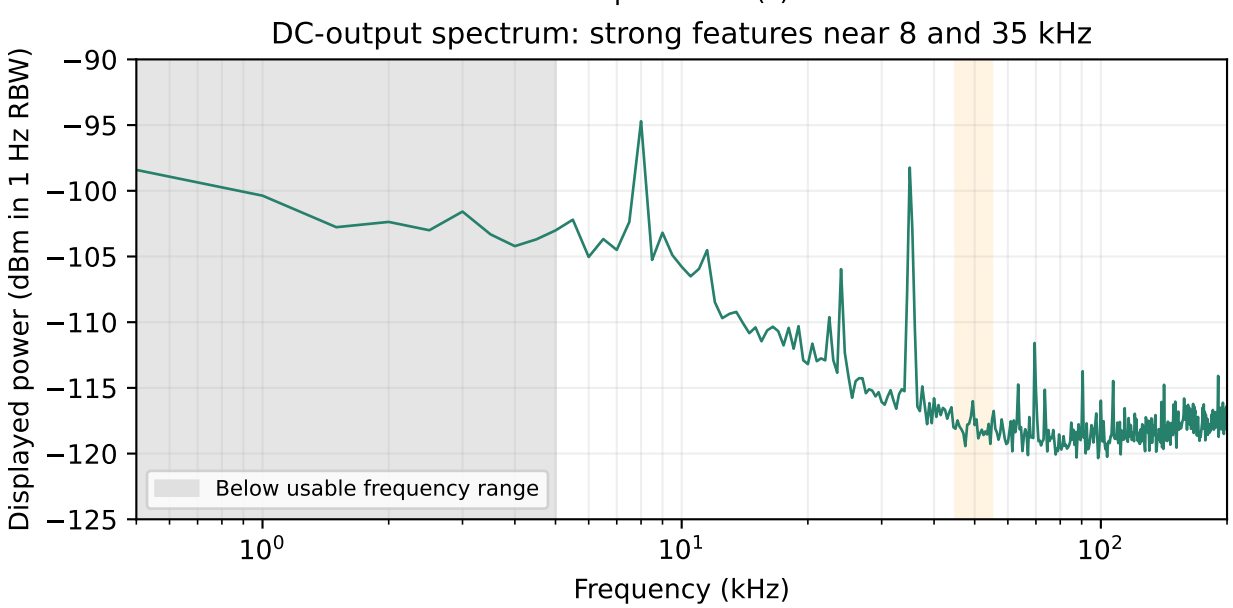

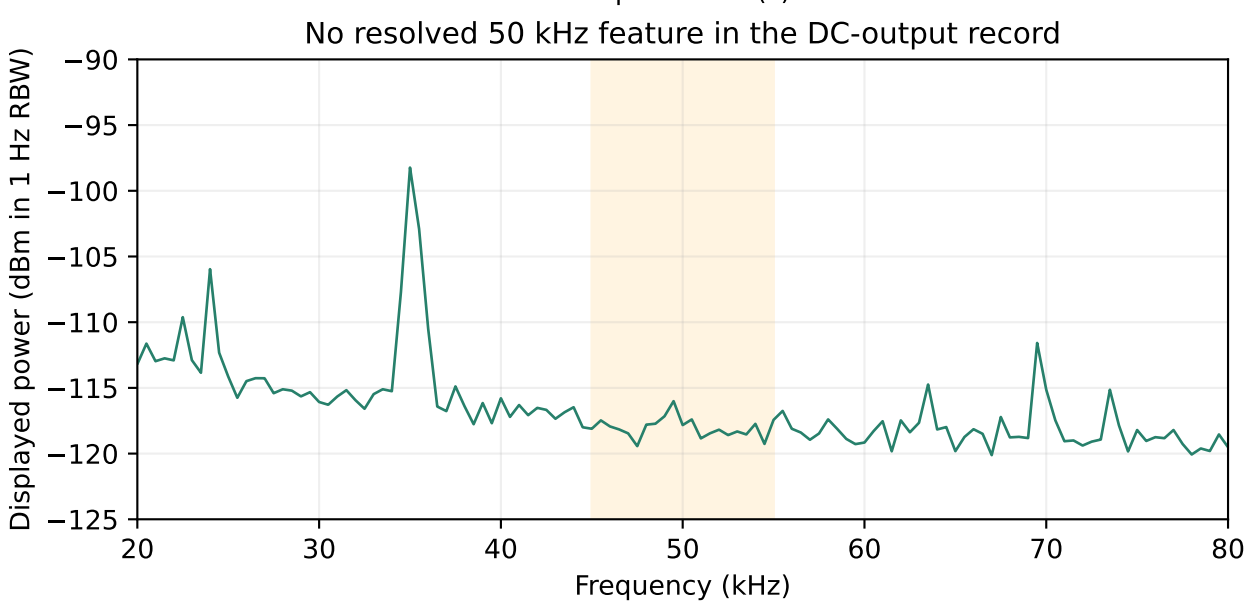

The 1 s and 10 s records are sparse scope samples; their scatter cannot be assigned to low-frequency noise.