

# Frequency Measurement System of Optical Clocks Without a Flywheel Oscillator

Miho Fujieda, Tetsuya Ido, Hidekazu Hachisu, Tadahiro Gotoh, Hiroshi Takiguchi, Kazuhiro Hayasaka, Kenji Toyoda, Kenji Yonegaki, Utako Tanaka, and Shinji Urabe

**Abstract**—We developed a system for the remote frequency comparison of optical clocks. The system does not require a flywheel oscillator at the remote end, making it possible to evaluate optical frequencies even in laboratories, where no stable microwave reference, such as an Rb clock, a Cs clock, or a hydrogen maser exists. The system is established by the integration of several systems: a portable carrier-phase two-way satellite frequency transfer station and a microwave signal generation system by an optical frequency comb from an optical clock. The measurement was as quick as a conventional method that employs a local microwave reference. We confirmed the system uncertainty and instability to be at the low  $10^{-15}$  level using an Sr lattice clock.

**Index Terms**—Clocks, frequency measurement, optical frequency conversion.

## I. INTRODUCTION

NOT only national metrological institutes but also universities and research institutes are devoting much effort to the development of highly stable optical clocks [1]–[5]. Their superb uncertainties will pave the way to the redefinition of the second. When a university decides to evaluate the absolute frequency of an optical clock, it needs to establish a frequency link to a laboratory with a primary frequency standard, or to one with a time scale traceable to international atomic time (TAI). Also, in an optical clock comparison between two sites, a frequency link is necessary. An optical fiber link and a satellite link using GNSS or a geostationary satellite are widely used for frequency transfer between two sites [6]–[10]. The former is well known as a highly accurate and stable method, and it enables frequency transfer that gives access to the stability of optical clocks without degradation [11]. However, the availability of a fiber link is sometimes limited depending on the location of the laboratories or the rental fee requested for the access to the fibers. Although satellite-based links have inferior stability to optical fiber links [12], their availability is much better, especially for intercontinental frequency transfer. Satellite-based frequency transfer needs a long measurement time to reduce the measurement noise. On the other hand, the long operation of optical clocks remains a difficult task. To bridge the difference between the measurement time and operation time, a flywheel oscillator is normally

employed [13]. When a frequency evaluation uncertainty at the low  $10^{-15}$  level is required, a measurement time of  $10^4 - 10^5$  s is necessary for satellite-based frequency transfer. Therefore, the frequency instability of the flywheel oscillator should be kept at the same level during the measurement. A hydrogen maser is typically adopted as a flywheel oscillator, though all laboratories do not have a hydrogen maser. Thus, we developed a system for the frequency measurement of remote optical clocks without a flywheel oscillator. In this system, frequency transfer by carrier-phase two-way satellite frequency transfer (TWCP) [14], [15] is performed with a portable antenna for wider availability. Since TWCP can reach an instability of the  $10^{-15}$  level within a time on the order of  $10^3$  s, effort to extend the operation time is not required for the optical clocks. Furthermore, a microwave reference signal can be directly generated from an optical clock using an optical frequency comb. No flywheel oscillator is necessary in our system. Let us assume that a frequency signal  $f_{UTC(k)}$  of UTC(k) at laboratory  $k$  is used as a reference for frequency measurement and that a TWCP frequency link is established between laboratories  $a$  and  $k$ . In this case, two measurements, a local measurement of  $f_{opt} - f_{flywheel}$  and a frequency transfer to measure  $f_{flywheel} - f_{UTC(k)}$ , have been performed independently. On the other hand, the frequency measurement demonstrated here simply measures  $f_{opt} - f_{UTC(k)}$ . In this paper, we report the details and performance of our frequency measurement system.

## II. SYSTEM SETUP

Fig. 1 shows a schematic of the frequency measurement of an optical clock at laboratory  $a$  with respect to UTC(k) at laboratory  $k$ . At laboratory  $a$ , the frequency measurement system is installed to measure the frequency of an optical clock. The system consists of a portable TWCP station and a microwave signal generation system by an optical clock. The system configuration is presented in this section. The frequency is evaluated with respect to  $f_{UTC(k)}$ , whose frequency difference from TAI will be given by circular T later. At laboratory  $k$ , a fixed TWCP station is assumed to be available. The frequency transfer between laboratories  $a$  and  $k$  is performed by the TWCP technique.

### A. Microwave Signal Generation From an Optical Clock

Fig. 2 shows a schematic of the microwave signal generation system, where an optical frequency comb converts the frequency from optical to microwave. The comb is locked to

Manuscript received August 12, 2015; accepted September 29, 2016. Date of publication October 4, 2016; date of current version December 1, 2016.

M. Fujieda, T. Ido, H. Hachisu, T. Gotoh, H. Takiguchi, and K. Hayasaka are with the National Institute of Information and Communications Technology, Tokyo 184-8795, Japan (e-mail: miho@nict.go.jp).

K. Toyoda, K. Yonegaki, U. Tanaka, and S. Urabe are with the Graduate School of Engineering Science, Osaka University, Osaka 560-8531, Japan.

Digital Object Identifier 10.1109/TUFFC.2016.2615119

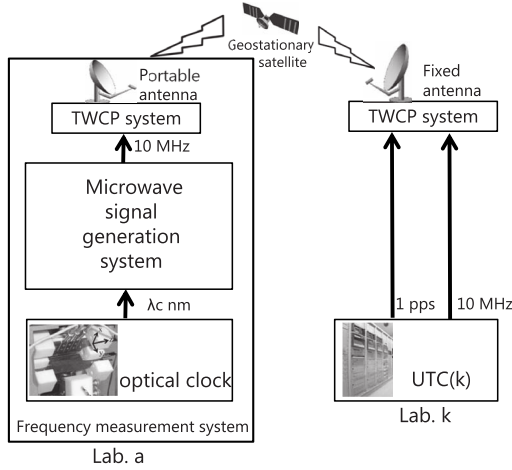


Fig. 1. Frequency measurement of an optical clock at laboratory *a* with respect to UTC(*k*) at laboratory *k*.

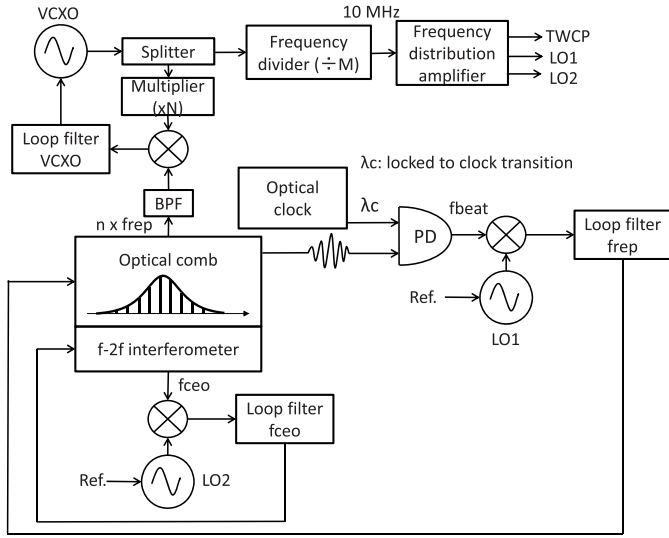


Fig. 2. Microwave signal generation system from an optical clock. PD: photodetector. VCXO: voltage-controlled crystal oscillator. LO1 and LO2: signal generators.

an optical clock by optical phase-locked loop. The beat signal between the frequency comb and the clock laser is detected by a photodetector and locked to a signal generator named LO1 through a loop filter. The carrier envelope offset frequency  $f_{ceo}$  is detected by an  $f - 2f$  self-interferometer and locked to a signal generator named LO2 through a loop filter. The signal generators LO1 and LO2 are locked to the external reference generated from the microwave signal from the comb. Therefore, both the repetition and the carrier envelope offset frequencies  $f_{rep}$  and  $f_{ceo}$ , respectively, become synchronized with the optical clock, enabling an operation free from a local microwave reference. The microwave signal to be transferred is generated from  $f_{rep}$ . The  $n$ th harmonic of  $f_{rep}$  is extracted by a photodetector and a bandpass filter. The signal from a voltage-controlled crystal oscillator is locked to the harmonic through a frequency multiplier ( $\times N$ ). Its frequency is divided by a frequency divider ( $\div M$ ). To finally achieve a 10-MHz

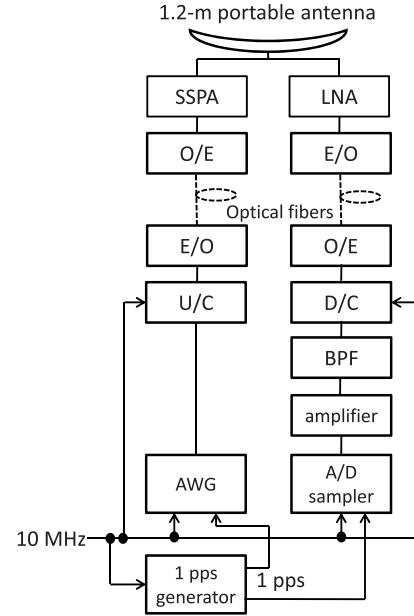


Fig. 3. Schematic of the portable TWCP station. U/C: frequency upconverter. D/C: frequency downconverter. E/O: electrical-to-optical converter. O/E: optical-to-electrical converter. SSPA: solid-state power amplifier. LNA: low-noise amplifier. AWG: arbitrary waveform generator. A/D: analog to digital. BPF: bandpass filter.

signal, appropriate values of  $n$ ,  $N$ , and  $M$  are selected. When a signal is transmitted to the air in a TWCP station, the deviation of the center frequency should be kept within a licensed frequency range. To comply with the regulation, the following are performed: a VCXO with a rather narrow tuning range is inserted for phase-locking of the harmonic of  $f_{rep}$  to avoid a frequency jump exceeding the licensed frequency deviation when an optical clock unlocks to the clock transition. The LO1 frequency is finely adjusted to keep the deviation of  $f_{rep}$  below  $10^{-5}$  Hz. A microwave signal coherent to the optical clock is generated in this way, and its frequency is divided by a frequency divider to produce a 10-MHz reference signal. In actual measurement, we confirmed using a frequency counter with the 10-MHz reference signal that the frequency deviation was less than  $3 \times 10^{-6}$  Hz.

### B. Portable TWCP Station

In this section, the details of the portable TWCP station are described. Its schematic is shown in Fig. 3. The station is equipped with a 1.2-m portable antenna and optical fibers for signal transfer between indoors and outdoors. It is easy to install in various places. An arbitrary waveform generator (AWG) is used as a signal generator [16]. The AWG generates a direct-sequence spectrum spreading signal with a bandwidth of 200 kHz at a center frequency of 70 MHz. The signal frequency is upconverted to 14 GHz by a frequency upconverter (U/C). The amplitude of a  $1.3\text{-}\mu\text{m}$  CW light is modulated by the 14-GHz signal in an electrical-to-optical converter (E/O). The light is transmitted through an optical fiber to outdoors. Since the signal loss in an optical fiber is as low as 0.2 dB/km, the length is not an issue. The light is converted to the 14-GHz signal by an optical-to-electrical converter (O/E).

It is amplified by a solid-state power amplifier and transmitted to a geostationary satellite. The signal is frequency-converted by an oscillator in the satellite and transmitted back to earth. The reception signal is amplified by a low-noise amplifier, converted to light by another E/O, and sent indoors. Another O/E extracts the microwave signal of about 10 GHz. The signal is converted to 70 MHz by a frequency downconverter (D/C). The 70-MHz signal is bandpass-filtered and amplified. Finally, the carrier-phase information is determined by software from the sampling data obtained by an analog-to-digital (A/D) sampler [17]. The configuration of the portable TWCP station is identical to that of conventional two-way satellite time and frequency transfer (TWSTFT) stations except to the AWG and A/D sampler. The AWG, A/D sampler, U/C, and D/C are connected to the 10-MHz reference signal. The 1-pulse-per-second (pps) signals are generated by a 1-pps generator from the 10-MHz signal and supplied to the AWG and A/D sampler. The time difference between the two TWCP stations is calculated from the carrier-phase information and can be converted to a frequency difference. The computation method is described in [15].

### III. SYSTEM PERFORMANCE

To evaluate the performance of the frequency measurement system, we measured a microwave signal derived from an Sr lattice clock relative to UTC(NICT). The lattice clock with an uncertainty of  $8.6 \times 10^{-17}$  was developed by the National Institutes of Information and Communications Technology (NICT) [18]. The Sr clock was operated for a few hours. An Yb optical fiber comb was used in the frequency measurement system and generated a 1-GHz signal from the fourth harmonic of  $f_{\text{rep}}$  ( $=250$  MHz). A 100-MHz VCXO was locked to the 1-GHz signal through a ten-times frequency multiplier. The 100-MHz signal was divided by a 1/10 frequency divider. The resultant 10-MHz signal was used as a reference signal of the system. On the other hand, a fixed TWCP station with a 1.8-m antenna was connected to the signal of UTC(NICT). The frequency difference between the downconverted 10-MHz signal and UTC(NICT) was measured by the TWCP technique via a geostationary satellite. Both fixed and portable TWCP antennas were installed on the same rooftop. A phase comparator also measured the frequency difference for the comparison of the results. The resultant time difference is shown in Fig. 4. The line labeled TWCP shows the result obtained by the frequency measurement system. The result measured by the phase comparator is shown in the gray dashed line. The vertical offsets were adjusted for better visibility. The measurement rates were 1 point per second for both. The gray solid line shows the double difference of them. Its slope was  $9 \times 10^{-17}$ , which indicates good agreement between the two frequency differences. The Allan deviation of the frequency difference is shown in Fig. 5. The stability at 1 s measured by TWCP is better than that measured by the phase comparator because the 1-s data of TWCP are calculated by averaging 50 points detected every 20 ms. The stability was  $1.4 \times 10^{-15}$  at 1000 s, which was comparable to that of a frequency measurement using a local hydrogen maser.

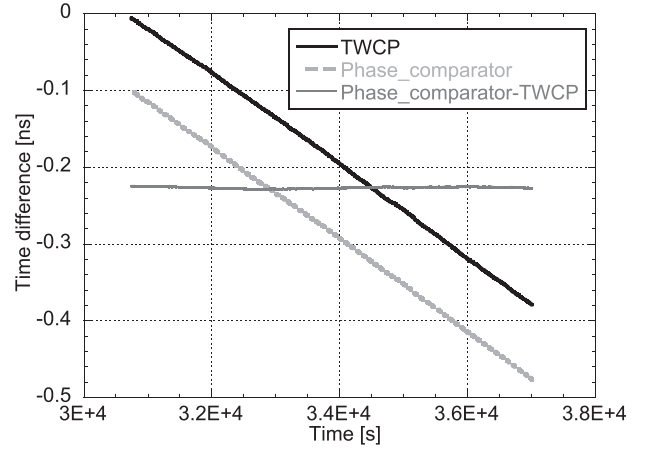


Fig. 4. Time difference between Sr-based microwave and UTC(NICT).

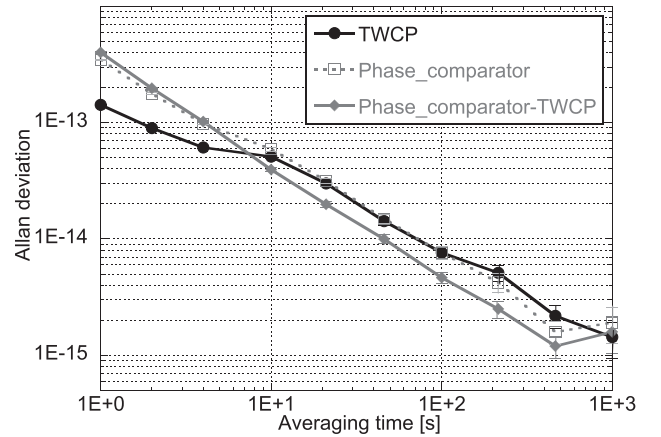


Fig. 5. Allan deviation of frequency difference between Sr-based microwave and UTC(NICT).

TABLE I  
MEAN FREQUENCY DIFFERENCE BETWEEN THE Sr-BASED MICROWAVE AND UTC(NICT)

Mean frequency difference	Sr-Microwave - UTC(NICT) (1e-15)
Calculation	$-58.8 \pm 2.0$
TWCP	$-60.0 \pm 1.6$
Phase comparator	$-59.9 \pm 1.6$

The uncertainty of the system is discussed next. The frequency of our Sr clock was already known [18] and the agreement with other Sr lattice clocks developed by the University of Tokyo and Physikalisch-Technische Bundesanstalt had been confirmed [11], [19]. Thus, we can calculate the frequency difference between TAI and the optically generated microwave signal based on the Sr clock. The frequency difference between TAI and UTC(NICT) is published with a delay in Circular T. Table I shows the frequency differences obtained by calculation and measurements using the system and phase comparator. The calculation includes the combined uncertainty of  $2 \times 10^{-15}$ , which is predominantly determined by the TAI-UTC(NICT) link uncertainty. The bias frequency of the calculation was caused by the roughly tuned frequencies of LO1 and LO2 shown in Fig. 2. The uncertainties of TWCP and

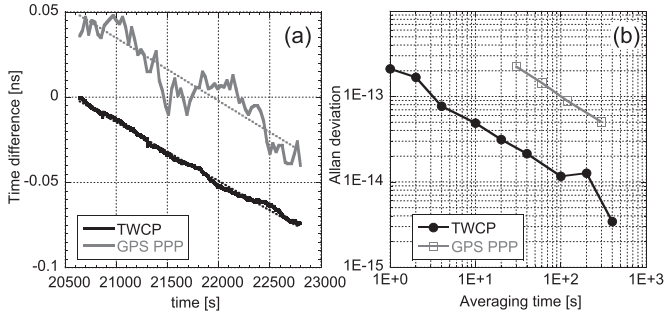


Fig. 6. Result of one of 40-min measurements "run 1". (a) Time difference and (b) Allan deviation between microwave generated from  $^{40}\text{Ca}^+$  system and UTC(NICT).

the phase comparator are mainly determined by the double-difference instabilities of the two techniques at 1000 s shown in Fig. 5. Besides that, the residual disagreement of  $9 \times 10^{-17}$  between them is also included. As shown in Table I, the uncertainty of our frequency measurement system was at the  $10^{-15}$  level.

#### IV. APPLICATION OF THE SYSTEM

A linear trap system of a single  $^{40}\text{Ca}^+$  ion has been developed at Osaka University for experiments related to quantum information processing [20]. Our portable system for optical frequency measurement was installed to establish a frequency link along a baseline of 500 km from NICT to Osaka University, where there was no atomic clock available to generate a reference signal. A microwave signal was generated from the  $^{40}\text{Ca}^+$  system that was locked to the clock transition ( $^2S_{1/2} - ^2D_{5/2}$ , 729 nm). The portable TWCP antenna was installed on a rooftop of a building with a portable GPS antenna nearby. A dual-frequency GPS receiver was also installed with the reference signal generated from the  $^{40}\text{Ca}^+$  system and used for frequency measurement. The frequency of the clock transition was evaluated with respect to UTC(NICT).

The operation of the whole system, including the  $^{40}\text{Ca}^+$  system continued from a few minutes to 1 h. The reference signal was stable, while the  $^{40}\text{Ca}^+$  system was locked to the clock transition. When it was unlocked, on the other hand, the reference signal was generated from the free-running VCXO. Such a condition of the interrupted reference signal led to a difficulty in obtaining a stable clock solution in frequency transfer by GPS PPP. This is because the carrier-phase ambiguity and the receiver clock offset cannot be fixed in a short measurement in GPS PPP. When the operation time was longer than 40 min, we could obtain an appropriate result by GPS PPP. The length of the operation time was not an issue for TWCP, in which only an instantaneous phase difference between two stations was computed. Fig. 6 shows the time difference between UTC(NICT) and the microwave signal generated from  $^{40}\text{Ca}^+$  system, from which the Allan deviation was calculated. The black and gray lines, respectively, depict the results measured by TWCP and GPS PPP. The GPS PPP computation was performed every 30 s using a static IGS orbit and 30-s clock products [21] with the software provided by Natural Resources Canada. The mean frequency differences

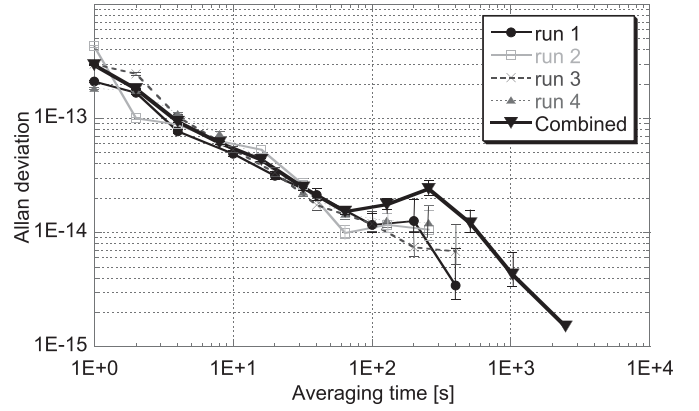


Fig. 7. Frequency stabilities of four 40-min measurements and their combination with three 5-min intervals. They are measured by TWCP.

obtained by TWCP and GPS PPP were  $-3.4 \pm 0.6 \times 10^{-14}$  and  $-3.7 \pm 5.0 \times 10^{-14}$ , respectively. The uncertainties were determined from the Allan deviation at an averaging time of 300 s. There were a total of seven measurements, where the measurement time was longer than 40 min. We confirmed from them that the results obtained by the TWCP and the GPS PPP were in agreement within the statistical uncertainty. Additionally, the TWCP result reached  $3 \times 10^{-15}$  at 400 s. The frequency measurement system worked well even in a remote location. We performed 40-min measurements four times with an interval of five minutes between them to evaluate the frequency stability at longer averaging times. During the 5-min intervals, the optical frequency comb was adjusted to keep a phase locking to the clock laser of the  $^{40}\text{Ca}^+$  system. The obtained Allan deviation is shown in Fig. 7. It was found that there was a bump due to the instability at the low  $10^{-14}$  level around an averaging time of about 300 s. The reason for this bump is unknown at present. It proved, however, that the  $^{40}\text{Ca}^+$  system has stability at the  $10^{-15}$  level at an averaging time of 1000 s. Such measurement used to be impossible, because there is no stable frequency reference at Osaka University. The measurement based on UTC(NICT) has also revealed a fluctuation of the clock laser, which has triggered effort to reduce it by half. Our frequency measurement system could effectively provide a stable reference for Osaka University. The instability was similar to that of a local hydrogen maser linked to UTC(NICT).

#### V. CONCLUSION

We developed a frequency comparison system for optical clocks without a flywheel oscillator. It enables us to evaluate the frequency of optical clocks even in a laboratory, where there is no stable microwave reference, such as an Rb clock, a Cs clock, or a hydrogen maser. The system consists of a microwave signal generation system from the optical clock and a portable TWCP station. We confirmed the system uncertainty to be at the low  $10^{-15}$  level by a frequency measurement using an Sr lattice clock. The system was actually installed at a remote university. We were able to prove that the system worked appropriately from the agreement with the GPS PPP



and the resultant stability. Our system has a superior portability. The operation of the TWCP system is designed such that nonspecialists for satellite frequency transfer can handle it. If a portable optical clock [22] is available, the system and the optical clock as an optical frequency reference can be carried to various places and provide a reference signal linking to the second. This would be the case for the laboratories in universities as well as facilities of high energy physics, where a GPS-disciplined stable microwave oscillator is normally used.

After the redefinition of the second by optical clocks, a bridge from the optical region to the microwave region will be required because many instruments require a reference signal in the microwave region. The microwave signal generation system shown in this paper is expected to be helpful in various occasions.

#### ACKNOWLEDGMENT

The authors would like to thank R. Tabuchi, R. Ichikawa, and the members of the Quantum Electronics Group, Graduate School of Engineering Science, Osaka University, for their help on the installation of the portable TWCP station. They would also like to thank F. Nakagawa and Y. Hanado for support on UTC(NICT).

#### REFERENCES

- [1] I. Ushijima, M. Takamoto, M. Das, T. Ohkubo, and H. Katori, "Cryogenic optical lattice clocks," *Nature Photon.*, vol. 9, pp. 185–189, Feb. 2015.
- [2] M. Chwalla *et al.*, "Absolute frequency measurement of the  $^{40}\text{Ca}^+ 4s^2S_{1/2} - 3d^2D_{5/2}$  clock transition," *Phys. Rev. Lett.*, vol. 102, no. 2, p. 023002, Jan. 2009.
- [3] Y. Huang *et al.*, "Hertz-level measurement of the  $^{40}\text{Ca}^+ 4s^2S_{1/2} - 3d^2D_{5/2}$  clock transition frequency with respect to the SI second through the global positioning system," *Phys. Rev. A*, vol. 85, no. 3, p. 030503, Mar. 2012.
- [4] K. Matsubara *et al.*, "Direct comparison of a  $\text{Ca}^+$  single-ion clock against a Sr lattice clock to verify the absolute frequency measurement," *Opt. Exp.*, vol. 20, no. 20, pp. 22034–22041, Sep. 2012.
- [5] Y. Huang, P. Liu, W. Bian, H. Guan, and K. Gao, "Evaluation of the systematic shifts and absolute frequency measurement of a single  $\text{Ca}^+$  ion frequency standard," *Appl. Phys. B*, vol. 114, no. 1, pp. 189–201, Jan. 2014.
- [6] S. Droste *et al.*, "Optical-frequency transfer over a single-span 1840 km fiber link," *Phys. Rev. Lett.*, vol. 111, no. 11, p. 110801, Sep. 2013.
- [7] F. Stefani *et al.*, "Tackling the limits of optical fiber links," *J. Opt. Soc. Amer. B*, vol. 32, no. 5, pp. 787–797, May 2015.
- [8] C. E. Calosso *et al.*, "Frequency transfer via a two-way optical phase comparison on a multiplexed fiber network," *Opt. Lett.*, vol. 39, no. 5, pp. 1177–1180, Mar. 2014.
- [9] F. Lahaye, G. Cerretto, and P. Tavella, "GNSS geodetic techniques for time and frequency transfer applications," *Adv. Space Res.*, vol. 47, no. 2, pp. 253–264, Jan. 2011.
- [10] S. Droste *et al.*, "Characterization of a 450-km baseline GPS carrier-phase link using an optical fiber link," *New J. Phys.*, vol. 17, no. 8, p. 083044, Aug. 2015.
- [11] A. Yamaguchi *et al.*, "Direct comparison of distant optical lattice clocks at the  $10^{-16}$  uncertainty," *Appl. Phys. Exp.*, vol. 4, no. 8, p. 082203, Aug. 2011.
- [12] A. Bauch *et al.*, "Comparison between frequency standards in Europe and the USA at the  $10^{-15}$  uncertainty level," *Metrologia*, vol. 43, no. 1, p. 109, Dec. 2005.
- [13] J. Leute *et al.*, "Frequency comparison of  $^{171}\text{Yb}^+$  ion optical clocks at PTB and NPL via GPS PPP," *IEEE Trans. Ultrason., Ferroelect., Freq. Control*, vol. 63, no. 7, pp. 981–985, Jul. 2016.
- [14] M. Fujieda, T. Gotoh, F. Nakagawa, R. Tabuchi, M. Aida, and J. Amagai, "Carrier-phase-based two-way satellite time and frequency transfer," *IEEE Trans. Ultrason., Ferroelect., Freq. Control*, vol. 59, no. 12, pp. 2625–2630, Dec. 2012.
- [15] M. Fujieda, D. Piester, T. Gotoh, J. Becker, M. Aida, and A. Bauch, "Carrier-phase two-way satellite frequency transfer over a very long baseline," *Metrologia*, vol. 51, no. 3, p. 253, May 2014.
- [16] T. Gotoh, J. Amagai, T. Hobiger, M. Fujieda, and M. Aida, "Development of a GPU-based two-way time transfer modem," *IEEE Trans. Instrum. Meas.*, vol. 60, no. 7, pp. 2495–2499, Jul. 2011.
- [17] T. Kondo, Y. Koyama, R. Ichikawa, M. Sekido, E. Kawai, and M. Kimura, "Development of the K5/VSSP system," *J. Geodetic Soc. Jpn.*, vol. 54, no. 4, pp. 233–248, 2008.
- [18] H. Hachisu and T. Ido, "Intermittent optical frequency measurements to reduce the dead time uncertainty of frequency link," *Jpn. J. Appl. Phys.*, vol. 54, no. 11, p. 112401, Oct. 2015.
- [19] H. Hachisu *et al.*, "Direct comparison of optical lattice clocks with an intercontinental baseline of 9000km," *Opt. Lett.*, vol. 39, no. 14, pp. 4072–4075, Jul. 2014.
- [20] A. Noguchi, Y. Shikano, K. Toyoda, and S. Urabe, "Aharonov-Bohm effect in the tunnelling of a quantum rotor in a linear Paul trap," *Nat. Commun.*, vol. 5, pp. 3868–1–3868–6, May 2014.
- [21] J. Kouba and P. Héroux, "Precise point positioning using IGS orbit and clock products," *GPS Solutions*, vol. 5, no. 2, pp. 12–28, Oct. 2001.
- [22] N. Poli *et al.*, "A transportable strontium optical lattice clock," *Appl. Phys. B*, vol. 117, no. 4, pp. 1107–1116, Dec. 2014.

**Miho Fujieda** received the Ph.D. degree in physics from Kyoto University, Kyoto, Japan, in 2000.

She joined the Communications Research Laboratory (currently the National Institute of Information and Communications Technology), Tokyo, Japan, in 2003. Her current research interests include the time and frequency transfer via optical fibers and satellite link.



**Tetsuya Ido** was born in Gifu, Japan, in 1970. He received the D.Tech. degree in applied physics from The University of Tokyo, Tokyo, Japan, in 1998.

During 1998–2002, he was a Postdoctoral Fellow with the Japan Science and Technology Agency, where he was involved in laser cooling and precision spectroscopy of neutral strontium atoms which led to the lattice clock. From 2002 to 2006, he was with JILA, Boulder, CO, USA, where he was involved in the precision spectroscopy of neutral strontium.

Since 2006, he has been with the National Institute of Information and Communications Technology, Tokyo. He currently develops a lattice clock using neutral strontium atoms and is seeking its application. He also studies the generation of VUV radiation as a high-harmonic generation of near infrared pulses stored in a passive enhancement cavity.

**Hidekazu Hachisu** received the Ph.D. degree in applied physics from The University of Tokyo, Tokyo, Japan, in 2006.

Since 2010, he has been with the National Institute of Information and Communications Technology, Tokyo, where he has been involved in research and development of an optical frequency standard with neutral strontium atoms.



**Tadahiro Gotoh** received the Ph.D. degree in engineering from The University of Electro-Communications, Tokyo, Japan, in 2014.

He joined the Radio Research Laboratory (currently the National Institute of Information and Communications Technology), Tokyo, in 1985. His current research interests include time and frequency transfer and precise orbit determination.



**Hiroshi Takiguchi** was born in Okayama, Japan, in 1976. He received the Ph.D. degree from Kyoto University, Kyoto, Japan, in 2006.

He is currently a Researcher with the Space-Time Standards Laboratory, National Institute of Information and Communications Technology, Tokyo, Japan. His current research interests include the research and development for the precise time and frequency transfer by using space geodetic techniques.



**Kazuhiro Hayasaka** received the B.S. and M.S. degrees from The University of Tokyo, Tokyo, Japan, in 1988 and 1990, respectively, and the Ph.D. degree from Osaka University, Suita, Japan.

From 1997 to 1998, he was a scientific guest with Max Planck Institute of Quantum Optics, Garching bei München, Germany. He joined the Communications Research Laboratory (currently the National Institute of Information and Communications Technology), Tokyo, in 1990. Since 2007, he has been a Guest Associate Professor with Osaka University.

His current research interest includes quantum optics with trapped ions.



**Kenji Toyoda** received the Ph.D. degree from the Division of Physics and Astronomy, Graduate School of Science, Kyoto University, Kyoto, Japan, in 2002.

He is currently an Assistant Professor with the Graduate School of Engineering Science, Osaka University, Suita, Japan. His current research interests include quantum information processing and frequency standards using trapped ions, the quantum simulation of coupled optical cavities (the Jaynes-Cummings-Hubbard model), analog quantum computation using phonons in trapped ions, frequency standards using calcium ions, and implementation of adiabatic quantum gates.



**Kenji Yonegaki** received the B.Sc. degree in material science from Shimane University, Matsue, Japan in 2013, and the M.Sc. degree in quantum electronics using trapped ion from Osaka University, Suita, Japan in 2015. He learned the basis of engineering, including electronics and mechatronics with the National Institute of Technology, Yonago College, Tottori, Japan.

He joined ADVANTEST Corporation in 2015. He is currently involved in the development of automated test equipment for integrated circuits. His current research interests include semiconductor electronics and measurement technologies related to medicine and basic science.



**Utako Tanaka** received the Ph.D. degree in science from the Graduate School of Science, Kyoto University, Kyoto, Japan, in 1993.

She was a JSPS Postdoctoral Fellow with Kyoto University. She was with the Communications Research Laboratory, Japan (present National Institute of Information and Communications Technology), in 1994. From 2000 to 2002, she was with the Dr. David Wineland's Group, National Institute of Standards and Technology. She joined Professor Shinji Urabe's Group, Osaka University,

Suita, Japan, in 2003, where she is currently an Associate Professor with the Graduate School of Engineering Science. Her current research interests include ion trapping, atomic clocks, quantum information processing and quantum simulation using laser-cooled ions, and development of stabilized lasers.



**Shinji Urabe** received the B.E. and M.E. degrees in applied physics from The University of Tokyo, Tokyo, Japan, in 1972 and 1975, respectively, and the Ph.D. degree from the University of Tokyo in 1985.

In 1975, he joined the Radio Research Laboratory, where he was involved in atomic frequency standards and started research in trapped ions and laser cooling. He was a Director of the Kansai Advanced Research Center, Communications Research Laboratory, from 1994 to 1998. In 1998, he became a

Professor with the Graduate School of Engineering Science, Osaka University, Suita, Japan, where he was involved in high-resolution spectroscopy and quantum information processing experiments with trapped ions. He was the team reader of the projects of quantum information processing with trapped ions in Japan, such as the JST-CREST project from 2004 to 2010, and the MEXT Quantum Cybernetics project from 2009 to 2014. He is currently a Professor Emeritus with Osaka University.