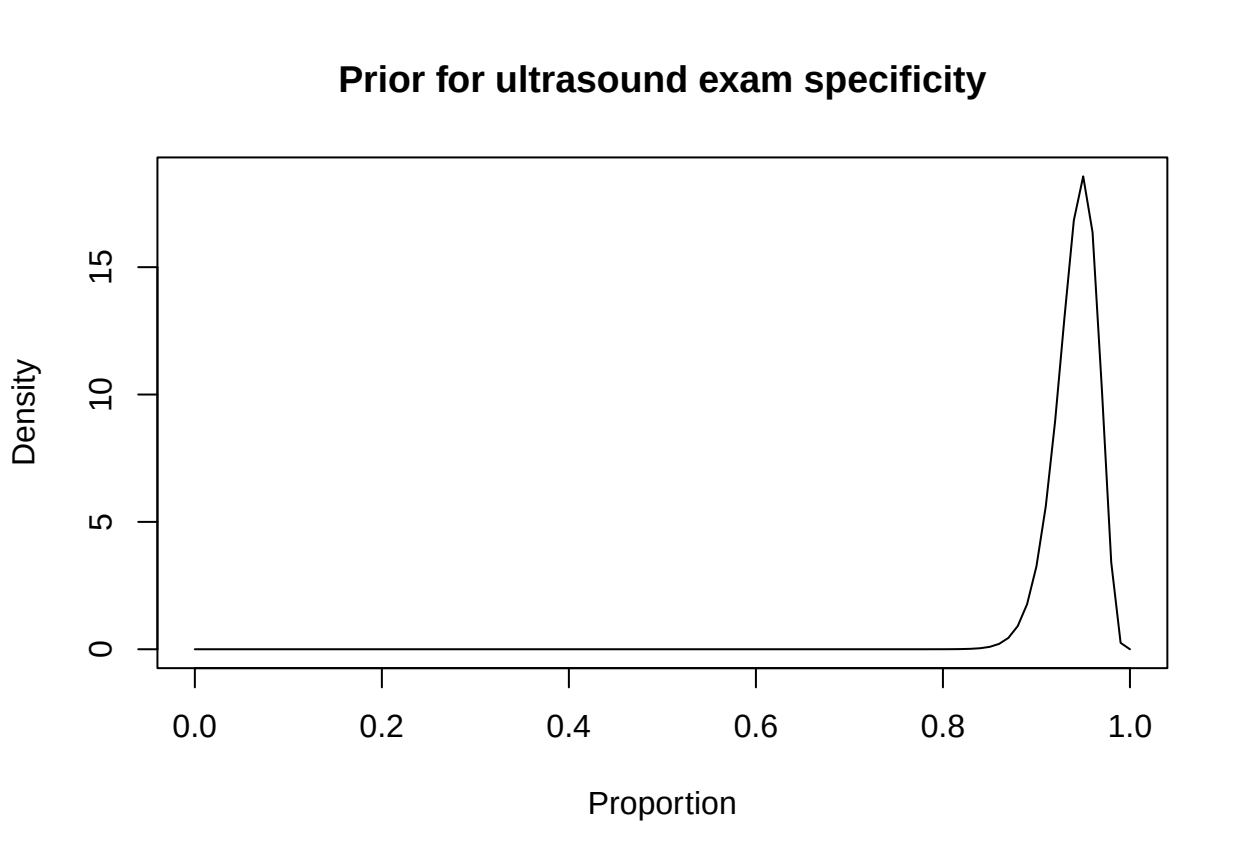
Prior for ultrasound exam specificity
Density
0
5
10
15
0.0
0.2
0.4
0.6
0.8
1.0
Proportion