

In-body Antigen Detection via Antibodies on a Transistor

Duran Kaan Altin

Abstract

This project develops a simulation workflow for HER2 antigen detection using an antibody-functionalized graphene field-effect transistor (GFET). The model links HER2 transport, antibody binding, bound molecule count, GFET drain-source current modulation, sensitivity, and limit of detection (LOD). The current repository includes a meshed COMSOL Transport of Diluted Species model for the transport stage, a separate partially anatomical prescribed-velocity convection-diffusion extension, analytical surface-binding post-processing, and analytical GFET response calculations. Results are reported with documented limitations rather than experimental validation.

I. INTRODUCTION

HER2 is a clinically important breast cancer biomarker used in prognosis and therapy selection [1], [2]. Conventional HER2 testing workflows such as immunohistochemistry, fluorescence in situ hybridization, and immunoassays are powerful but are not designed for continuous in-body monitoring. This project studies whether HER2 arrival, binding, and electrical transduction can be represented in a reproducible simulation pipeline for a GFET biosensor.

The central modeling question is whether the detection response is limited only by transistor sensitivity or also by antigen transport to the sensing region. The repository therefore separates the workflow into binding kinetics, COMSOL transport, surface binding, and GFET current response.

II. BACKGROUND

A. HER2 as a Biomarker

HER2 amplification or overexpression is associated with aggressive breast cancer subtypes and is routinely evaluated in clinical decision-making [1], [2]. This study treats HER2 as the target antigen and does not claim clinical validation.

B. Antigen-Antibody Binding

The binding stage uses reversible antigen-antibody kinetics:



$$r = k_f[Ag][Ab] - k_r[AgAb], \quad (2)$$

with dissociation constant:

$$K_d = \frac{k_r}{k_f}. \quad (3)$$

For surface binding, the Langmuir occupancy relation is used:

$$\theta = \frac{c_{surface}}{K_d + c_{surface}}. \quad (4)$$

C. GFET Biosensing Principle

Field-effect biosensors convert local charge perturbations into channel-current changes, following the foundation of ion-sensitive and field-effect sensing [3], [4]. Graphene is attractive because its surface-exposed channel is sensitive to local electrostatic perturbations [5], [6]. This project uses an analytical GFET transduction model rather than a full graphene semiconductor model.

III. METHODOLOGY

A. 0D Binding Kinetics

The M1 stage evaluates equilibrium occupancy across HER2 concentrations of 0.5, 1, 10, 100, and 1000 pM. The baseline assumptions are $K_d = 10$ pM, $k_f = 10^7$ 1/(M s), and $k_r = 10^{-4}$ 1/s.

M1 equilibrium occupancy vs HER2 concentration

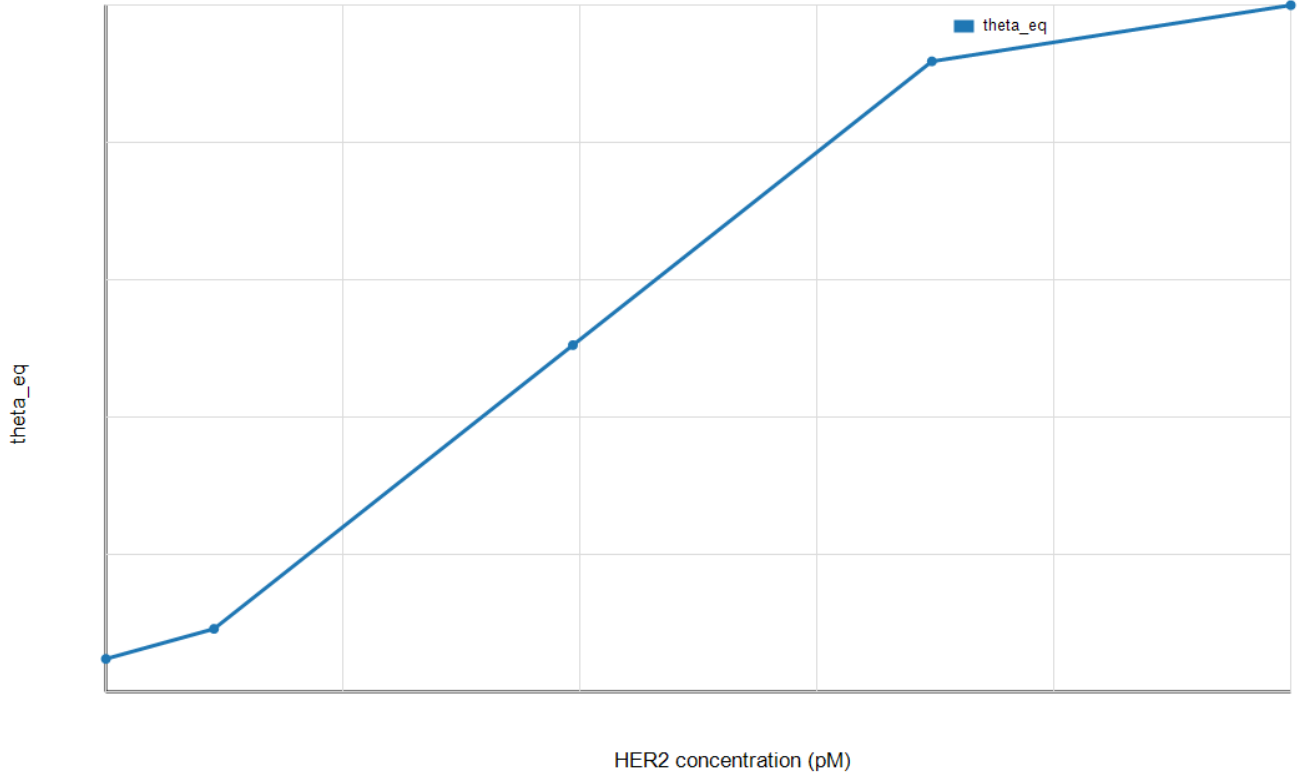


Fig. 1. M1 equilibrium occupancy versus HER2 concentration.

B. 3D COMSOL Transport Model

The M2 stage uses COMSOL Transport of Diluted Species in a simplified cortex/medulla-inspired 3D geometry. The medulla diffusion coefficient is parameterized by:

$$D_{medulla} = rD_{cortex}, \quad (5)$$

where r is swept over 0.1, 0.25, 0.5, 0.75, and 1.0. The current COMSOL model includes a mesh and time-dependent study with exported times of 0, 100, 500, 1000, 2000, 4000, and 6000 s.

C. Partially Anatomical Lymph-Node Flow Extension

The M2B extension implements a partially anatomical convection-diffusion model with afferent inlet regions, a hilum-side efferent outlet, and a prescribed lymph-flow velocity field coupled to HER2 transport. It keeps the M2 diffusion-only model unchanged and adds a separate lymph-node-inspired flow scaffold. The geometry uses an outer node radius of approximately $500 \mu\text{m}$, a medulla radius of approximately $250 \mu\text{m}$, a subcapsular/cortex/medulla region structure, four afferent inlet markers, one efferent outlet marker, and local/full sensor markers. M2B is a partially anatomical prescribed-velocity convection-diffusion extension, not a full anatomical lymph-node model and not a validated Darcy-flow pressure solution.

The flow implementation uses prescribed inlet velocities. The Transport of Diluted Species convection velocity is set to $u = u_{flow}$, $v = v_{flow}$, and $w = w_{flow}$. The velocity sweep is $v_{in} = 0, 10^{-7}, 5 \times 10^{-7}, 10^{-6}$ m/s. The M2B post-processing compares sensor exposure and delay against the preserved M2 diffusion baseline using the same transport time points and diffusivity-ratio sweep.

D. Surface Binding Model

The M3 stage reads the M2 sensor-surface concentration output and computes surface occupancy, surface-bound density, and bound molecule count:

$$\Gamma = \Gamma_{max}\theta, \quad (6)$$

M2_comsol_concentration_slice_t1000s

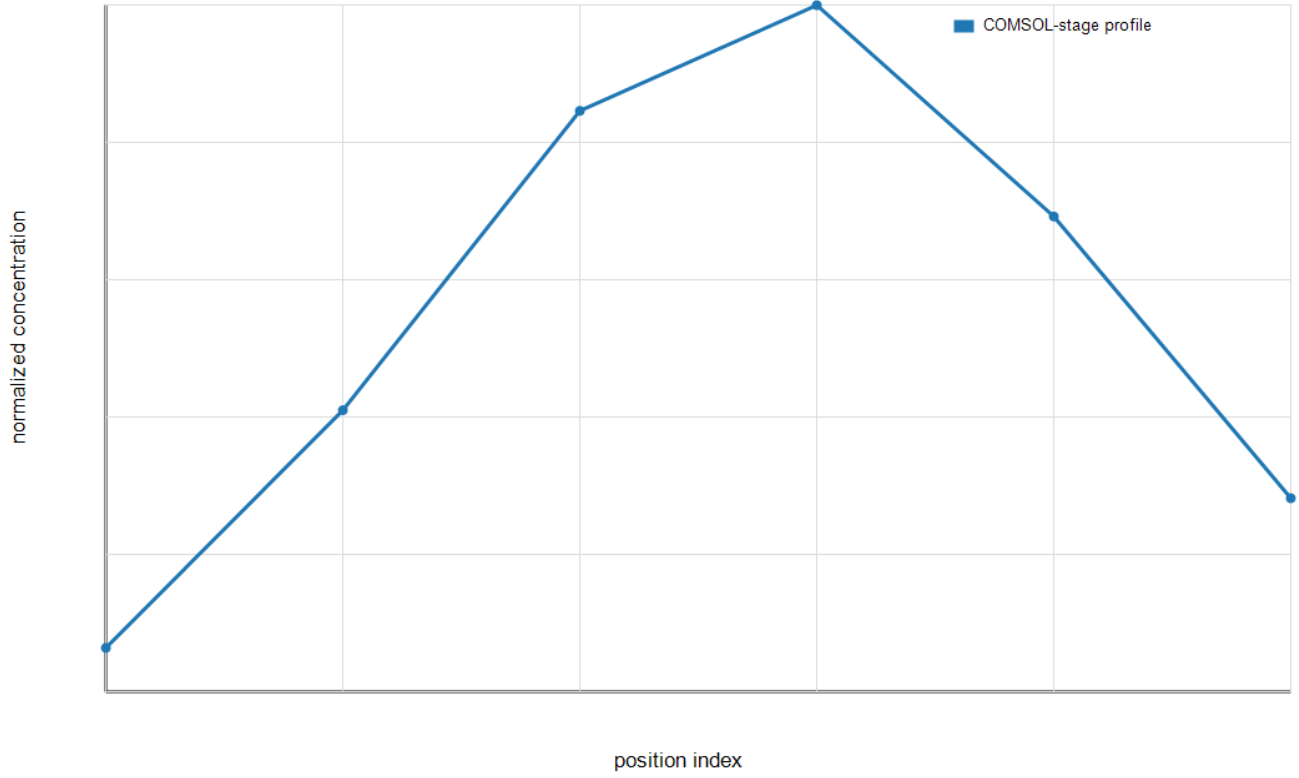


Fig. 2. M2 COMSOL-stage concentration profile at 1000 s.

$$N_{bound} = \Gamma A_{sensor} N_A. \quad (7)$$

Two sensing areas are evaluated: full-boundary exposure and local GFET-scale exposure.

E. GFET Current-Response Model

The M4 stage maps bound molecule count to current response:

$$\Delta I_{DS} = \frac{W}{L} e \mu V_{DS} \frac{\alpha N}{A_{eff}}. \quad (8)$$

The minimum detectable bound molecule count is:

$$N_{min} = \frac{I_{min} A_{eff}}{(W/L) e \mu V_{DS} \alpha}. \quad (9)$$

F. Sensitivity and LOD Estimation

Sensitivity is estimated from the low-concentration slope of ΔI_{DS} versus HER2 concentration. LOD is calculated as:

$$LOD = \frac{3\sigma}{S}, \quad (10)$$

where σ is the assumed current noise floor and S is sensitivity [7].

IV. RESULTS

A. Binding kinetics result

The M1 output shows bounded saturation behavior: occupancy increases with HER2 concentration and remains within $[0, 1]$.

M2_comsol_flux_streamlines_t1000s

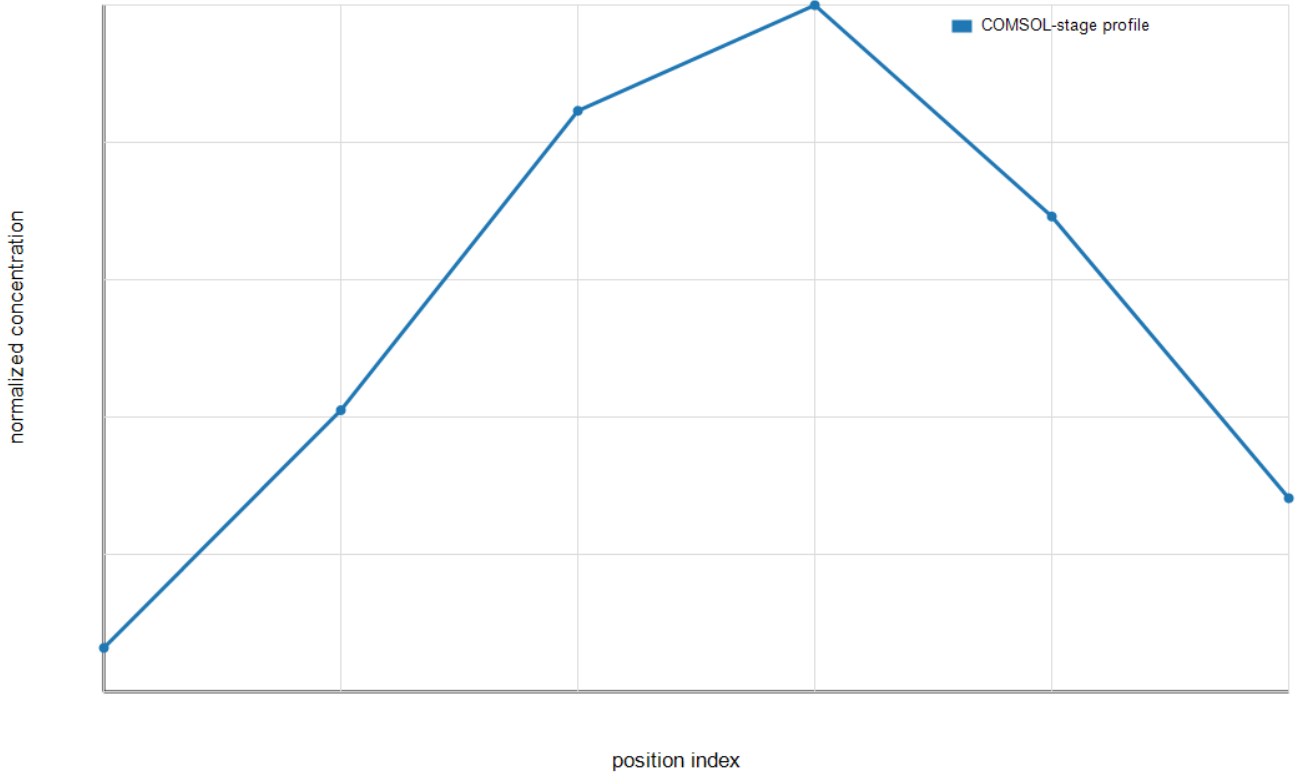


Fig. 3. M2 COMSOL-stage flux visualization at 1000 s.

B. Transport / flow result

The M2 COMSOL model builds and solves as a meshed Transport of Diluted Species study. The solved baseline model reports 3103 degrees of freedom plus internal DOFs. Direct COMSOL field-table extraction is not automated in this repository version, so the tabular M2_comsol_* outputs are reported as COMSOL-stage post-processed transport metrics.

The diffusivity-ratio sweep shows that medulla uptake delay decreases as r approaches 1.

For the reference case $r = 0.5$ and $v_{in} = 5 \times 10^{-7}$ m/s, the M2B convection-diffusion extension gives a sensor time-to-50% exposure of approximately 1839 s, compared with approximately 6038 s for the M2 diffusion-only baseline under the same sensor-exposure definition. At 6000 s, the reported sensor concentration is 8.73 pM for M2B and 4.98 pM for M2. The zero-flow M2B case gives the same 1000 s and 6000 s sensor concentration values as the diffusion-only baseline, while increasing v_{in} increases exposure. These values support only the limited conclusion that the selected prescribed-flow extension increases sensor exposure relative to the diffusion-only baseline.

C. Experiment A: Flow versus diffusion

Experiment A compares the diffusion-only M2 baseline with M2B directional-flow cases at $v_{in} = 10^{-7}$, 5×10^{-7} , and 10^{-6} m/s for $C = 10$ pM. Directional flow improves sensor exposure: the reference 5×10^{-7} m/s case reaches 8.73 pM at 6000 s, compared with 4.98 pM for diffusion-only transport. The time to 50% sensor exposure decreases from approximately 6038 s under diffusion-only transport to approximately 1839 s for the reference flow case.

D. Experiment B: Sensor placement sensitivity

Sensor placement result. Experiment B evaluates three sensor placements: subcapsular/cortical, cortex-medulla transition, and medulla/hilum-side. Sensor placement affects response timing and current response. In the modeled sweep, the subcapsular/cortical placement is fastest and strongest under the reference flow case. Under directional flow, late-time exposure becomes high across all tested placements, while placement still changes arrival time and pathway exposure. The current-response range across placements is approximately 559.9–600.5 pA under flow and 348.2–533.3 pA under diffusion-only transport, showing that the late-time current spread is smaller under flow than diffusion-only transport.

M2B prescribed velocity streamlines

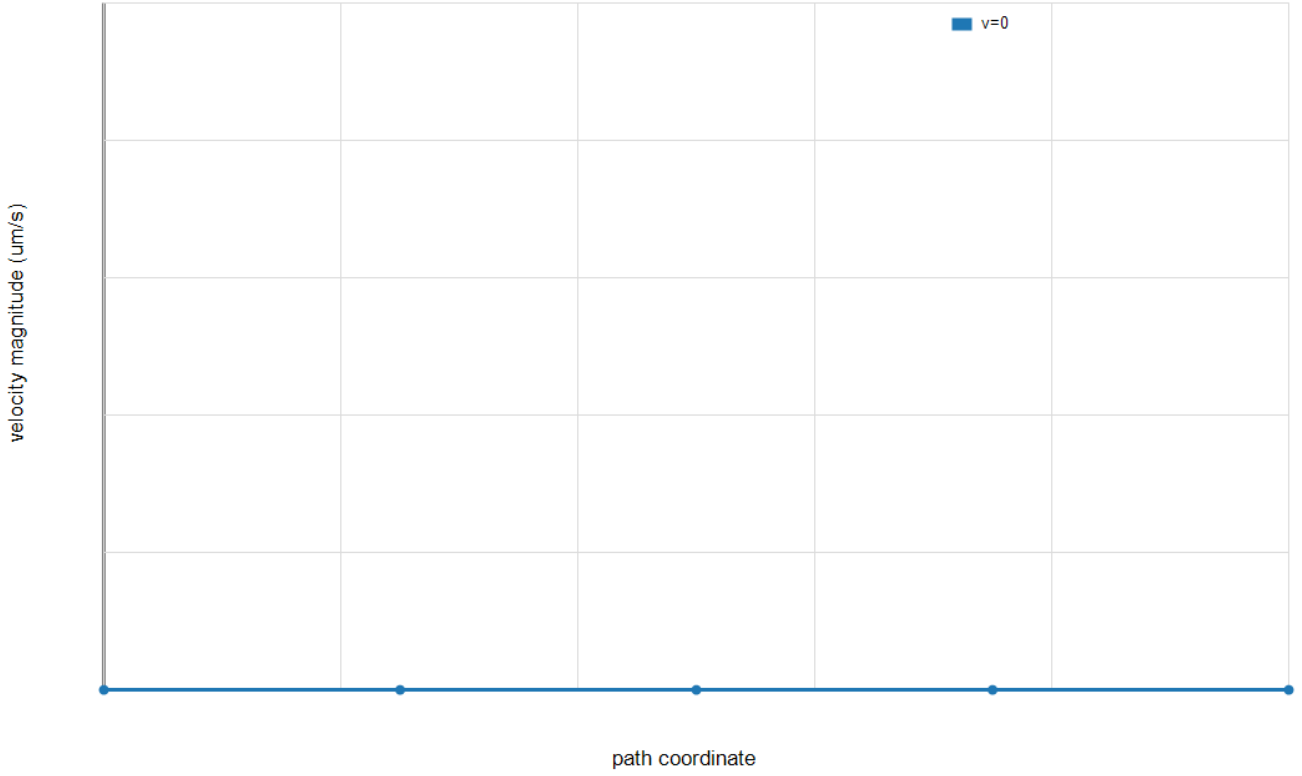


Fig. 4. M2B prescribed-velocity streamline profile for the partially anatomical convection-diffusion extension.

E. Experiment C: Detectability envelope

Electrical detectability result. Experiment C sweeps HER2 concentration, coupling efficiency, current noise floor, and binding affinity. Across the simulated envelope, 99 parameter combinations are detectable and 36 fail the 3σ current-threshold criterion. Detection is favored by stronger coupling, lower noise, lower K_d , and higher HER2 concentration. Detection fails for low concentration when coupling is weak, noise is high, or binding affinity is poor.

F. Experiment D: Debye screening feasibility

Debye screening feasibility result. Experiment D applies electrostatic attenuation using $\alpha_{eff} = \alpha_0 \exp(-d/\lambda_D)$. Screening strongly reduces feasibility as ionic strength increases and effective charge distance grows. For PBS-like physiological salt with $d \geq 5$ nm, none of the 60 screened cases remain detectable. This is a negative result: direct in-body GFET detection is not robust under PBS-like screening unless effective charge distance is very short, transduction is stronger, noise is lower, or the sensing environment reduces screening.

G. Experiment E: Feasibility Requirement Map

Experiment E converts the screening limitation into design requirements. It uses the same M3/M4 analytical response model and applies the screened coupling definition

$$\alpha_{eff} = \alpha_0 \exp(-d/\lambda_D), \quad (11)$$

with

$$\Delta I_{DS,screened} = \frac{W}{L} e \mu V_{DS} \frac{\alpha_{eff} N_{bound}}{A_{eff}}. \quad (12)$$

For each concentration, affinity, coupling, noise, Debye length, and effective charge distance case, the analysis computes the required coupling efficiency, maximum receptor-channel distance, and maximum tolerable electronics noise floor for $\Delta I_{DS,screened} \geq 3\sigma$.

M2B concentration slice at 1000 s

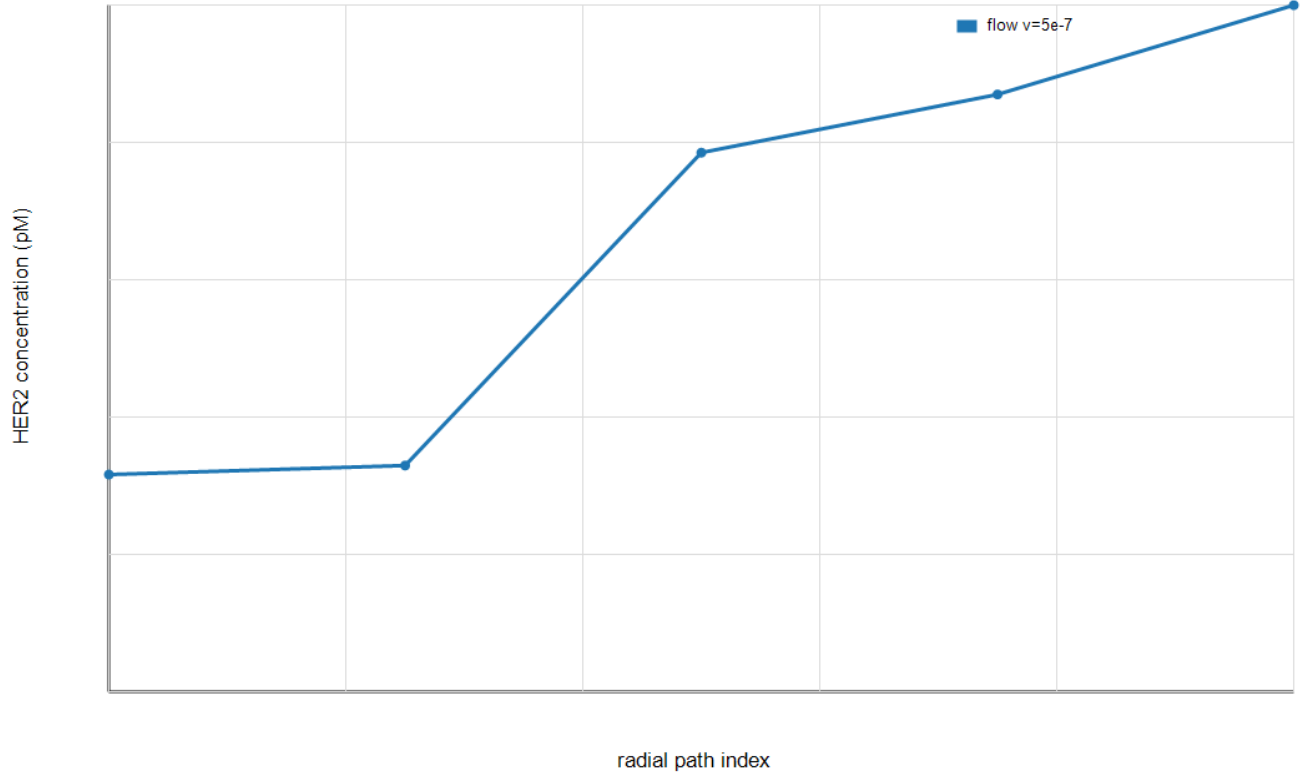


Fig. 5. M2B concentration profile at 1000 s compared with the preserved diffusion baseline.

The design requirement result is that direct in-body GFET-HER2 detection is feasible only if the effective receptor-to-channel distance is kept very short, transduction coupling is strong, and the electronics noise floor is low. For $K_d = 10$ pM, 10 pA noise, and PBS-like screening at $d = 1$ nm, the required α_0 is approximately 0.0326 at 1 pM HER2 and 0.00561 at 10 pM HER2. At $d = 2$ nm, the required α_0 increases to approximately 0.114 at 1 pM and 0.0196 at 10 pM.

Experiment E converts the screening limitation into design requirements. The model indicates that direct in-body GFET-HER2 detection is feasible only if the effective receptor-to-channel distance is kept very short, the transduction coupling is strong, and the electronics noise floor is low. Otherwise, especially under PBS-like ionic screening, the predicted signal falls below the detection threshold.

H. Surface Binding Response

Surface occupancy remains bounded and full-boundary exposure produces a larger total bound molecule count than the local GFET-scale sensing region.

I. DeltaIds and LOD

The current response increases with HER2 concentration and coupling efficiency. Under the current assumptions, the $\alpha = 0.03$, 10 pA case reaches a simulated LOD of approximately 0.78 pM. Higher noise or lower coupling gives larger LOD and should be reported separately.

V. DISCUSSION

What was calculated: the project calculated HER2 binding occupancy, diffusion-only transport, partially anatomical convection-diffusion transport, sensor-placement exposure, local bound molecule count, GFET current response, LOD, detectability envelopes, and Debye-screened current response.

What was concluded: antigen transport and placement influence how much HER2 reaches the sensor, but transport alone does not determine feasibility. Even when surface exposure improves, the predicted current can fall below the detection threshold if coupling is weak, noise is high, binding affinity is poor, or electrostatic screening is strong.

M2B flow vs M2 diffusion sensor exposure

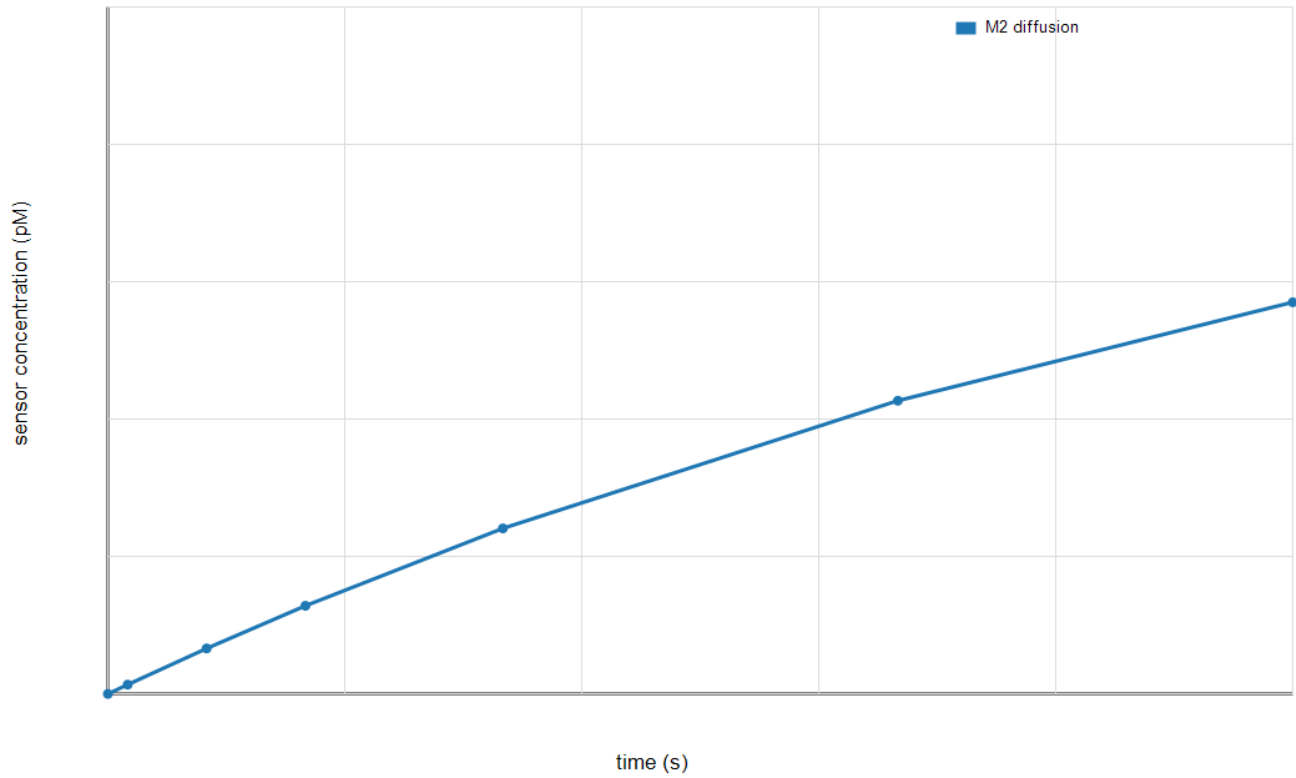


Fig. 6. Reference M2B convection-diffusion sensor exposure compared with M2 diffusion-only exposure.

Main conclusion: Directional flow and sensor placement improve HER2 exposure, but electrostatic screening and electronics noise dominate practical GFET detectability.

Positive result: directional lymph-node-inspired flow increases sensor exposure and reduces exposure time relative to diffusion-only transport under the modeled assumptions. Sensor placement affects response timing and current response. In the modeled sweep, the subcapsular/cortical placement is fastest and strongest under the reference flow case. Under directional flow, late-time exposure becomes high across all tested placements, while placement still changes arrival time and pathway exposure.

Negative result: detectability is not universal. Sub-pM or low-pM detection appears only under favorable coupling and low-noise assumptions, and PBS-like Debye screening with longer receptor distances eliminates detectability in the screened feasibility test.

What must improve for feasibility: Experiment E shows that the design would need shorter effective receptor-to-channel distance, lower-noise electronics, stronger transduction efficiency, higher-affinity recognition chemistry, or local mitigation of physiological ionic screening. These are simulation-based engineering requirements suggested by the model, not demonstrated device performance.

VI. LIMITATIONS

This project is simulation-only. No wet-lab validation, fabrication, clinical testing, biocompatibility analysis, or direct physiological Debye screening model is included. The M2 model is meshed and solved in COMSOL, but direct field-table export from solved .mph files remains a repository limitation. M2B is a partially anatomical prescribed-velocity convection-diffusion extension, not a full anatomical lymph-node model and not a validated Darcy-flow pressure solution. Direct COMSOL field-table export remains future work; the current quantitative tables are post-processed from the documented COMSOL-stage model and parameter sweeps. Surface binding and GFET response are analytically post-processed rather than fully coupled inside COMSOL.

M2 COMSOL-stage cortex vs medulla uptake at $r=0.5$

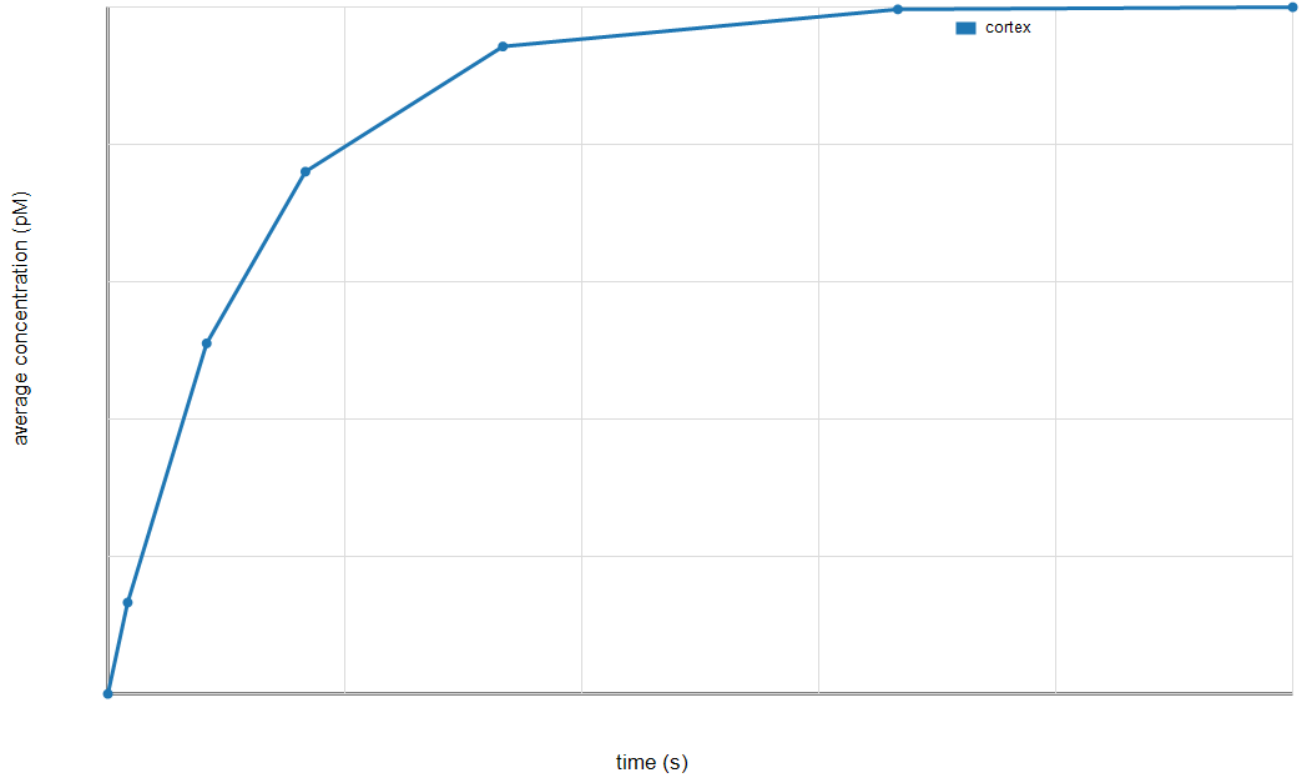


Fig. 7. Cortex, medulla, and sensor concentration trends at $r = 0.5$.

VII. CONCLUSION

The main scientific conclusion of this project is: Directional flow and sensor placement improve HER2 exposure, but electrostatic screening and electronics noise dominate practical GFET detectability. Even when antigen reaches the sensor, electrical detectability depends strongly on coupling efficiency, noise floor, and electrostatic screening.

The repository now implements a staged HER2-GFET workflow: 0D binding, meshed COMSOL transport, a separate partially anatomical prescribed-velocity convection-diffusion extension, surface binding from sensor concentration, GFET current-response/LOD estimation, and Experiment E feasibility requirement mapping. Future work should experimentally validate these design requirements, replace prescribed flow with validated Darcy/Brinkman flow, automate direct COMSOL field exports, and test surface chemistries/electronics that can achieve the required distance, coupling, and noise values.

REFERENCES

- [1] D. J. Slamon, G. M. Clark, S. G. Wong, W. J. Levin, A. Ullrich, and W. L. McGuire, "Human breast cancer: Correlation of relapse and survival with amplification of the her-2/neu oncogene," *Science*, vol. 235, no. 4785, pp. 177–182, 1987.
- [2] A. C. Wolff, M. E. H. Hammond, K. H. Allison, B. E. Harvey, P. B. Mangu, J. M. S. Bartlett, M. Bilous, I. O. Ellis, P. Fitzgibbons, W. Hanna, R. B. Jenkins, M. F. Press, P. A. Spears, G. H. Vance, G. Viale, L. M. McShane, and M. Dowsett, "Human epidermal growth factor receptor 2 testing in breast cancer: American society of clinical oncology/college of american pathologists clinical practice guideline focused update," *Journal of Clinical Oncology*, vol. 36, no. 20, pp. 2105–2122, 2018.
- [3] P. Bergveld, "Development of an ion-sensitive solid-state device for neurophysiological measurements," *IEEE Transactions on Biomedical Engineering*, vol. BME-17, no. 1, pp. 70–71, 1970.
- [4] E. Stern, A. Vacic, and M. A. Reed, "Semiconducting nanowire field-effect transistor biomolecular sensors," *IEEE Transactions on Electron Devices*, vol. 55, no. 11, pp. 3119–3130, 2008.
- [5] Y. Ohno, K. Maehashi, Y. Yamashiro, and K. Matsumoto, "Electrolyte-gated graphene field-effect transistors for detecting ph and protein adsorption," *Nano Letters*, vol. 9, no. 9, pp. 3318–3322, 2009.
- [6] T. Kuila, S. Bose, P. Khanra, A. K. Mishra, N. H. Kim, and J. H. Lee, "Recent advances in graphene-based biosensors," *Biosensors and Bioelectronics*, vol. 26, no. 12, pp. 4637–4648, 2011.
- [7] A. Shrivastava and V. B. Gupta, "Methods for the determination of limit of detection and limit of quantitation of the analytical methods," *Chronicles of Young Scientists*, vol. 2, no. 1, pp. 21–25, 2011.

M2 COMSOL-stage delay vs diffusivity ratio

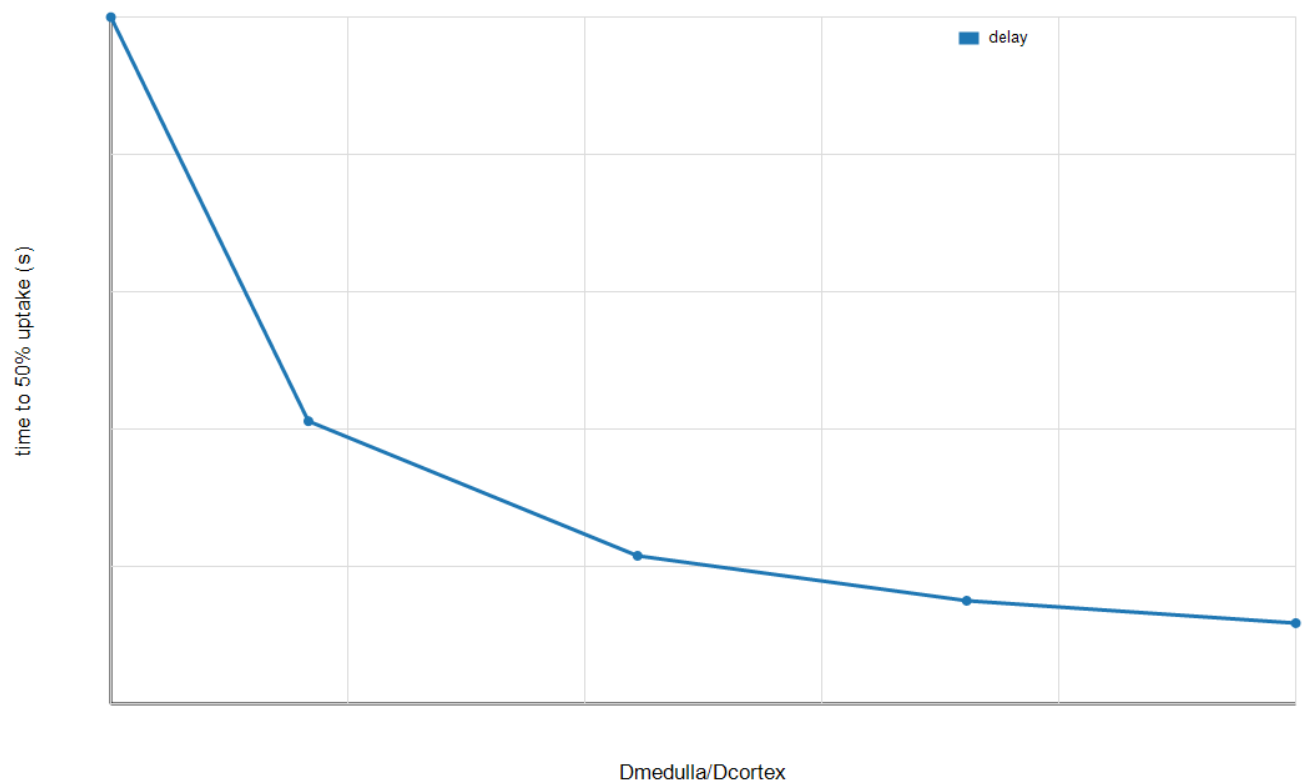


Fig. 8. Medulla uptake delay versus diffusivity ratio.

Experiment A: flow vs diffusion exposure

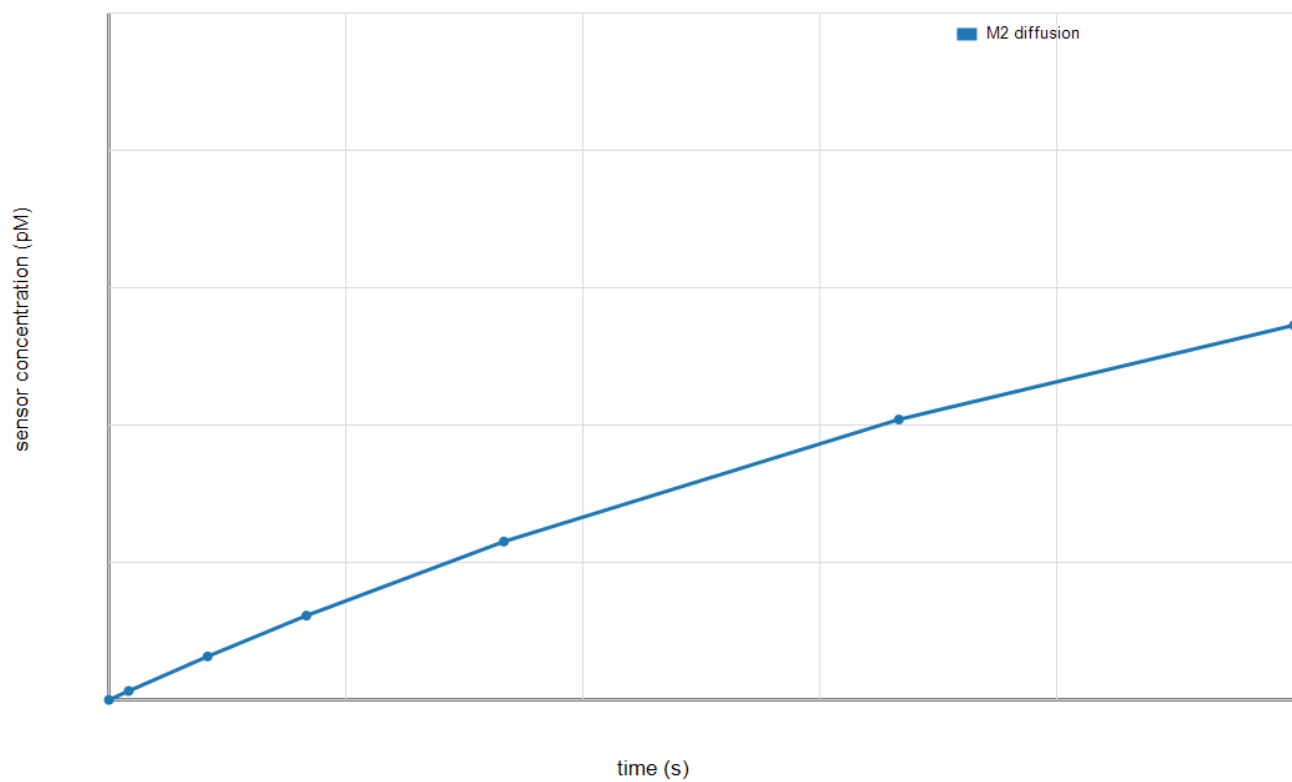


Fig. 9. Experiment A: sensor exposure under diffusion-only transport and directional-flow cases.

Experiment B: placement exposure

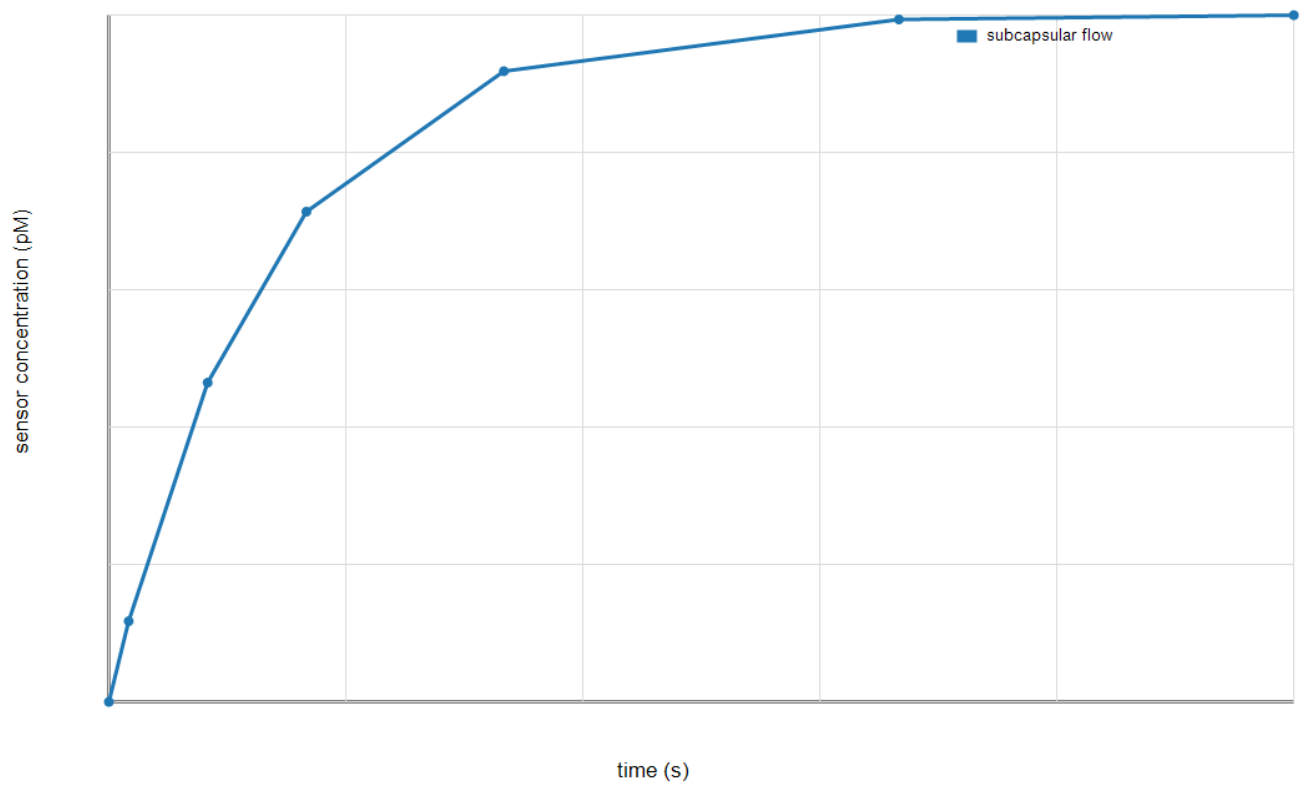


Fig. 10. Experiment B: concentration exposure for sensor placements under diffusion-only and directional-flow transport.

Experiment B: placement current response

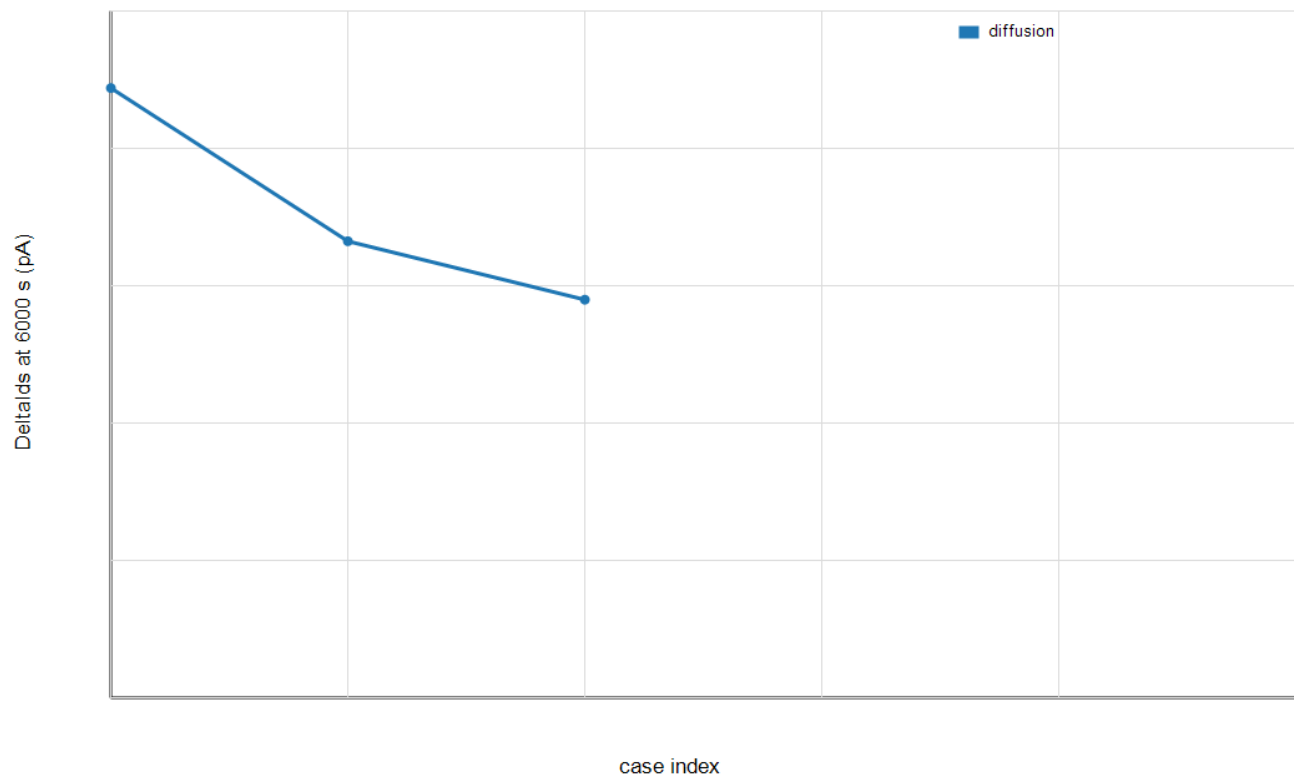


Fig. 11. Experiment B: GFET current response at 6000 s for the sensor-placement sweep.

Experiment C: Deltals vs concentration

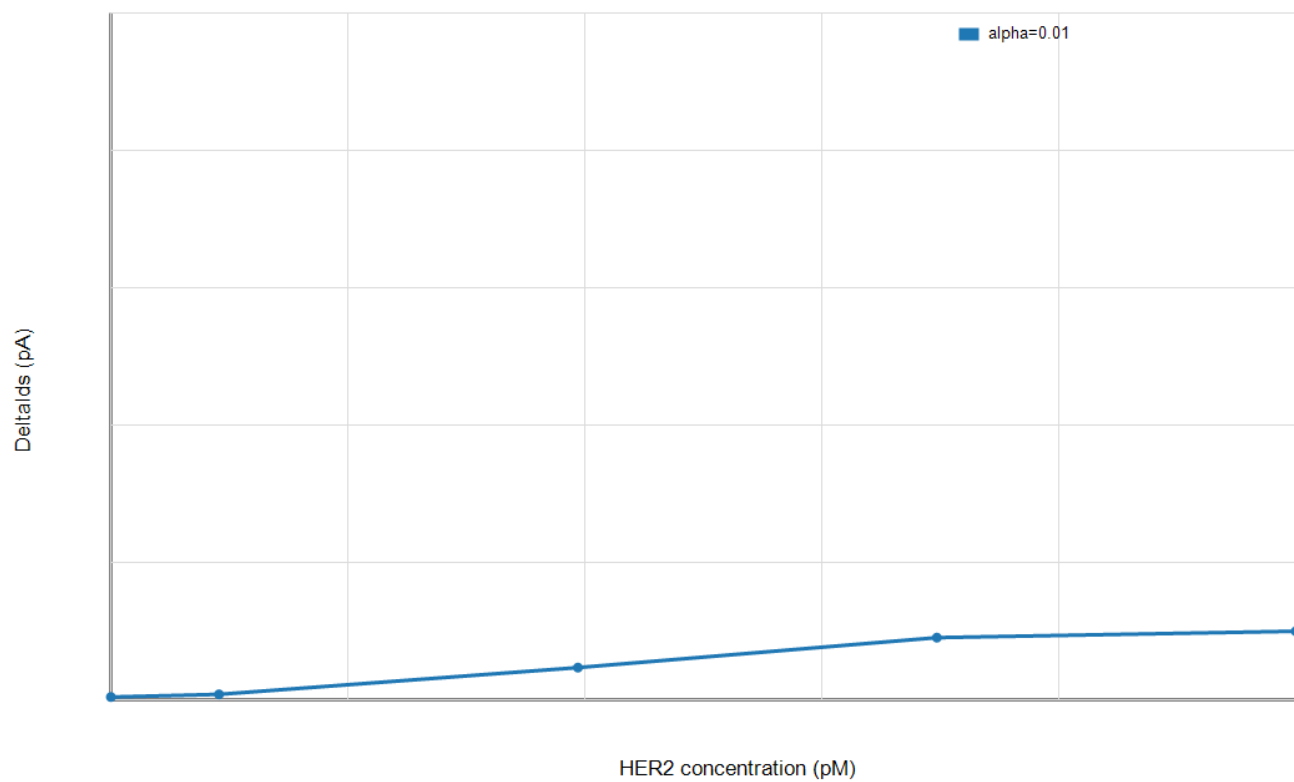


Fig. 12. Experiment C: current response versus HER2 concentration for coupling-efficiency cases.

Experiment C: detectable fraction

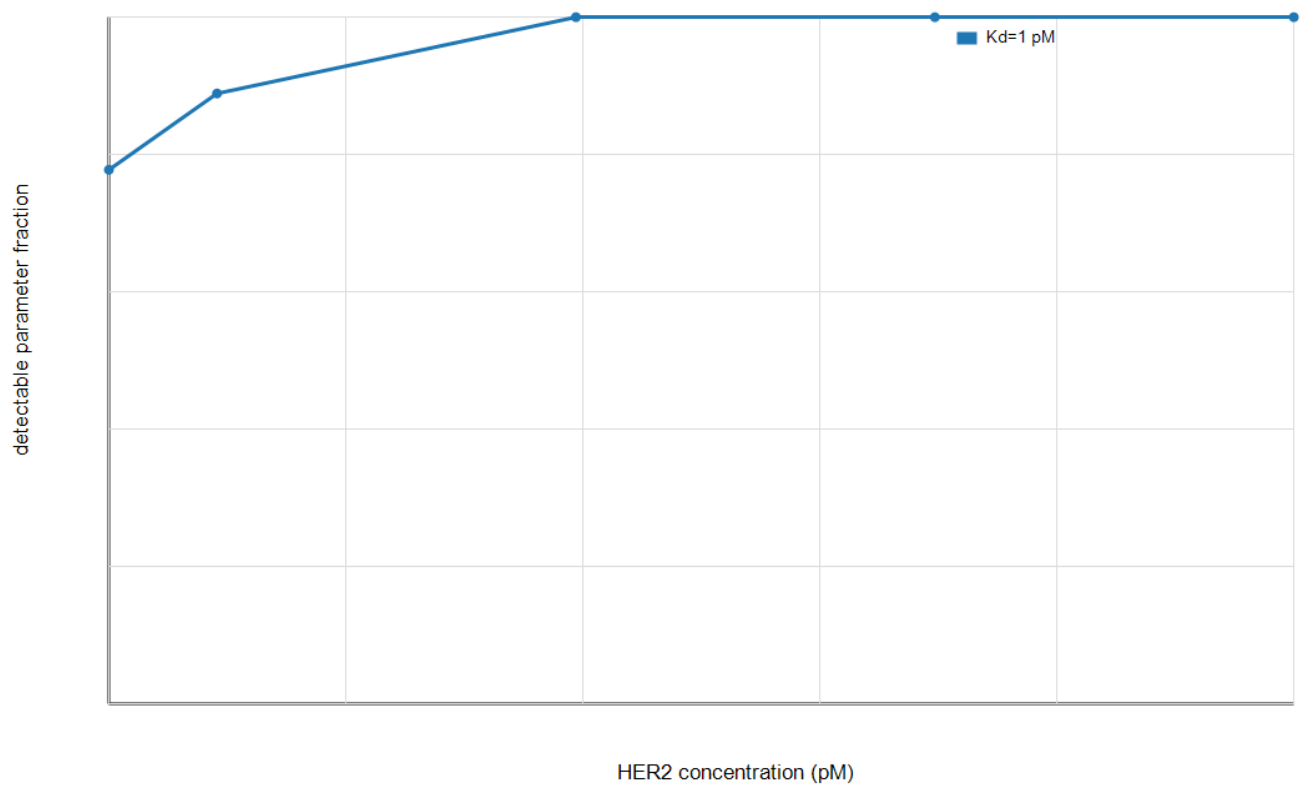


Fig. 13. Experiment C: detectable fraction across the concentration and affinity sweep.

Experiment D: LOD vs ionic strength

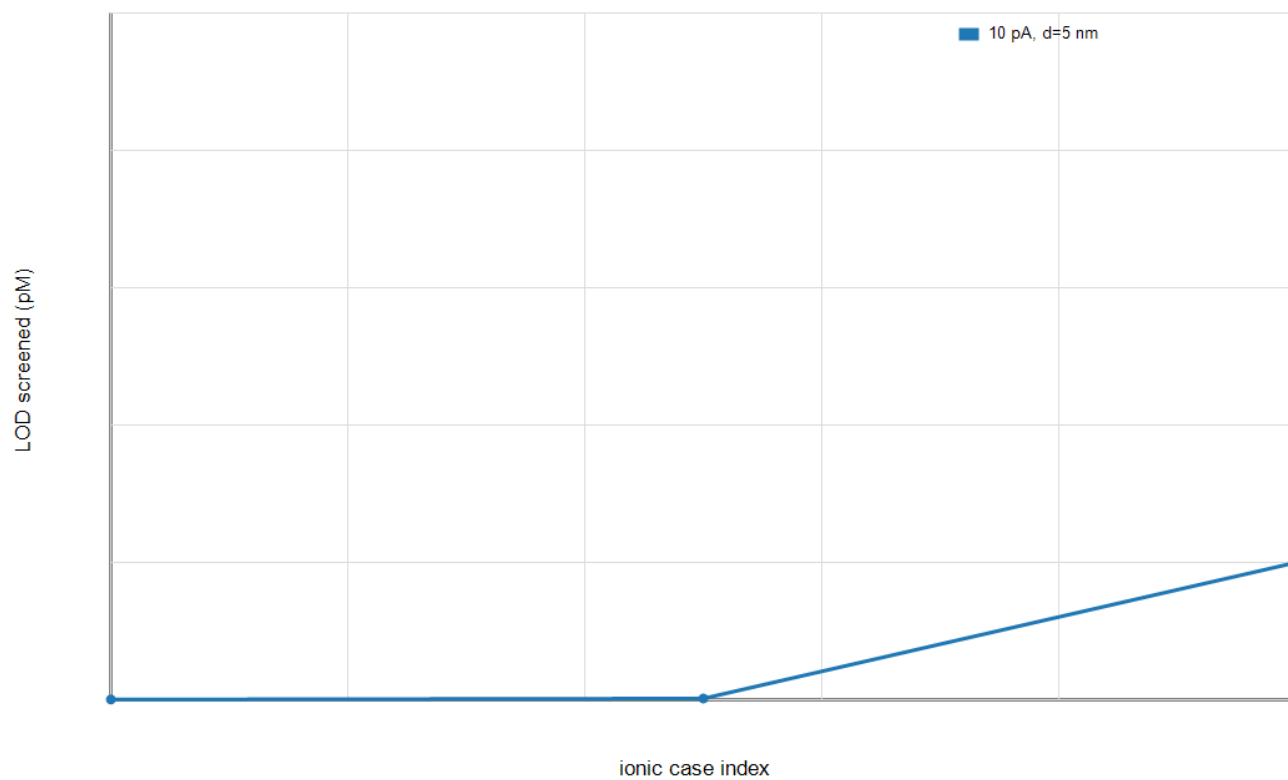


Fig. 14. Experiment D: screened LOD versus ionic-strength case.

Experiment D: screened detectability fraction

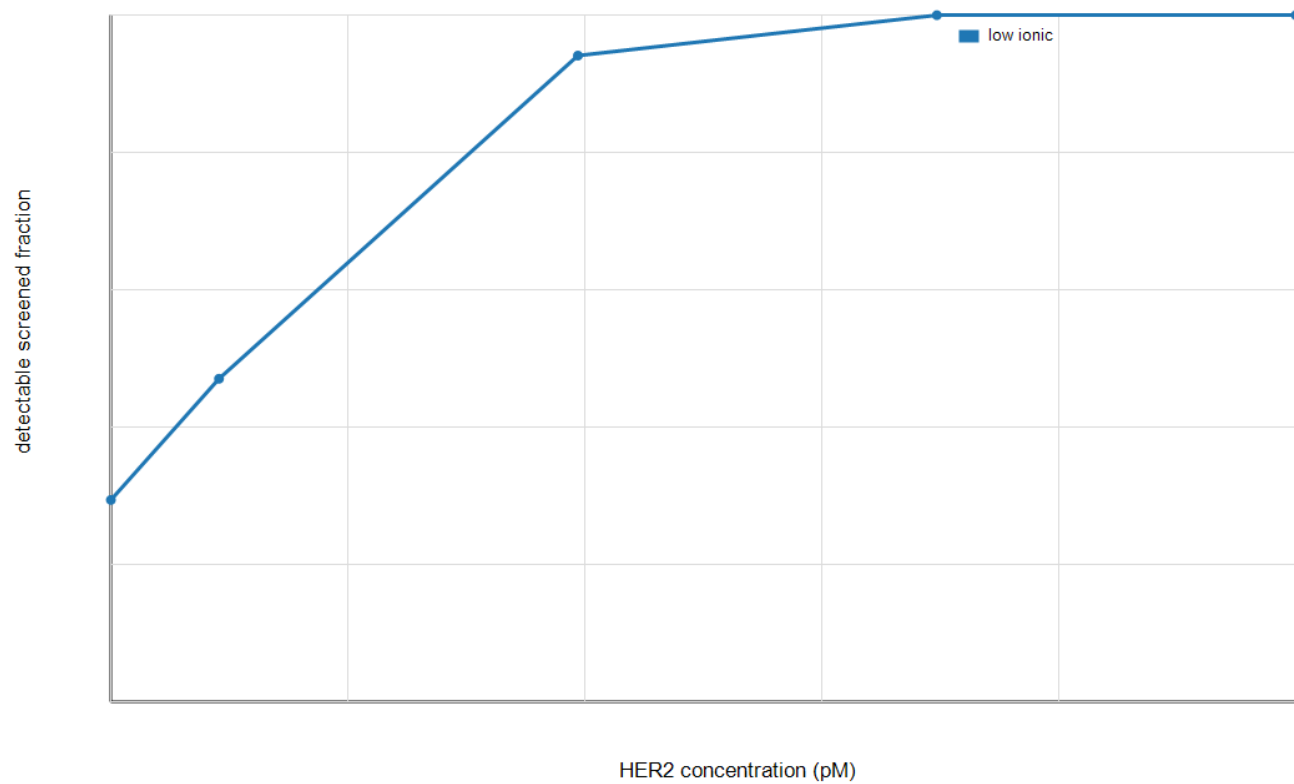


Fig. 15. Experiment D: screened detectability fraction under Debye attenuation assumptions.

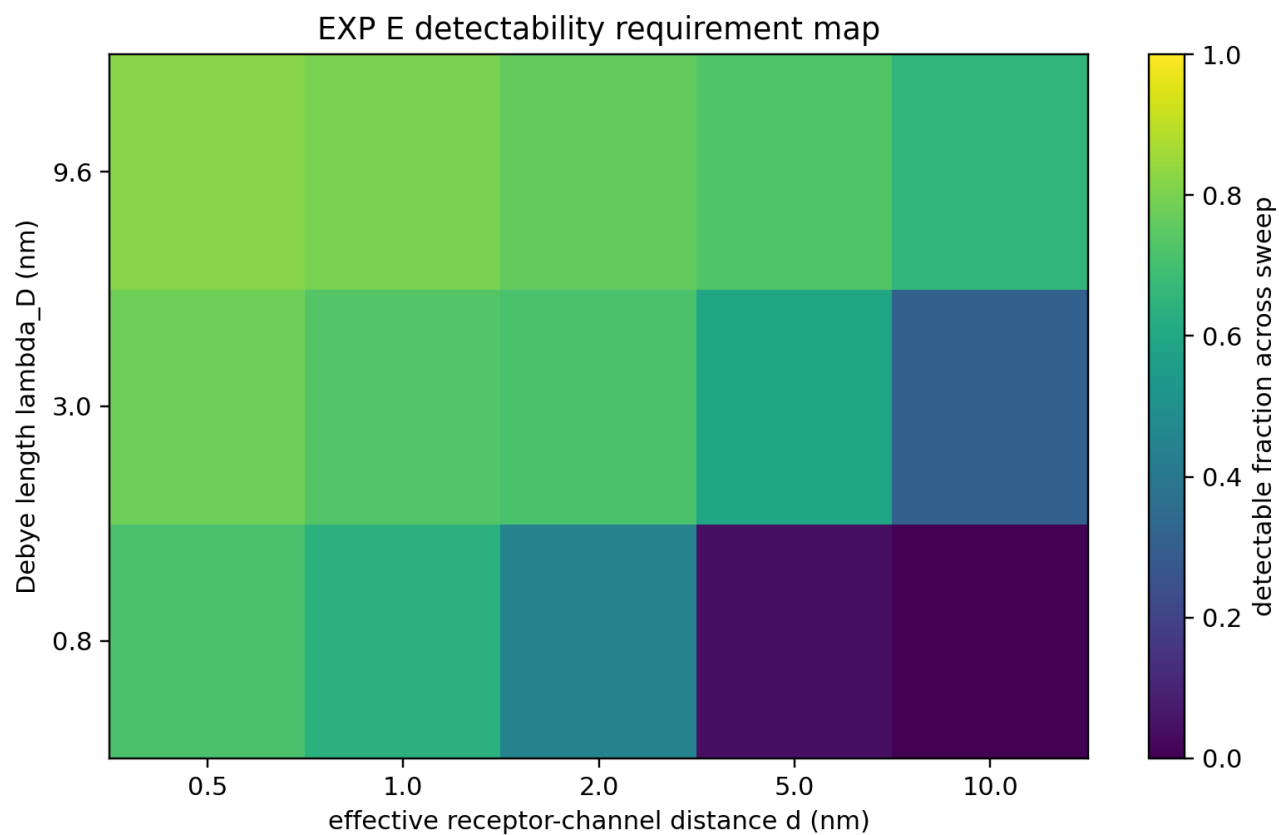


Fig. 16. Experiment E: detectability requirement map showing the fraction of detectable sweep cases versus Debye length and effective receptor-channel distance.

M3 bound HER2 count from M2 sensor concentration

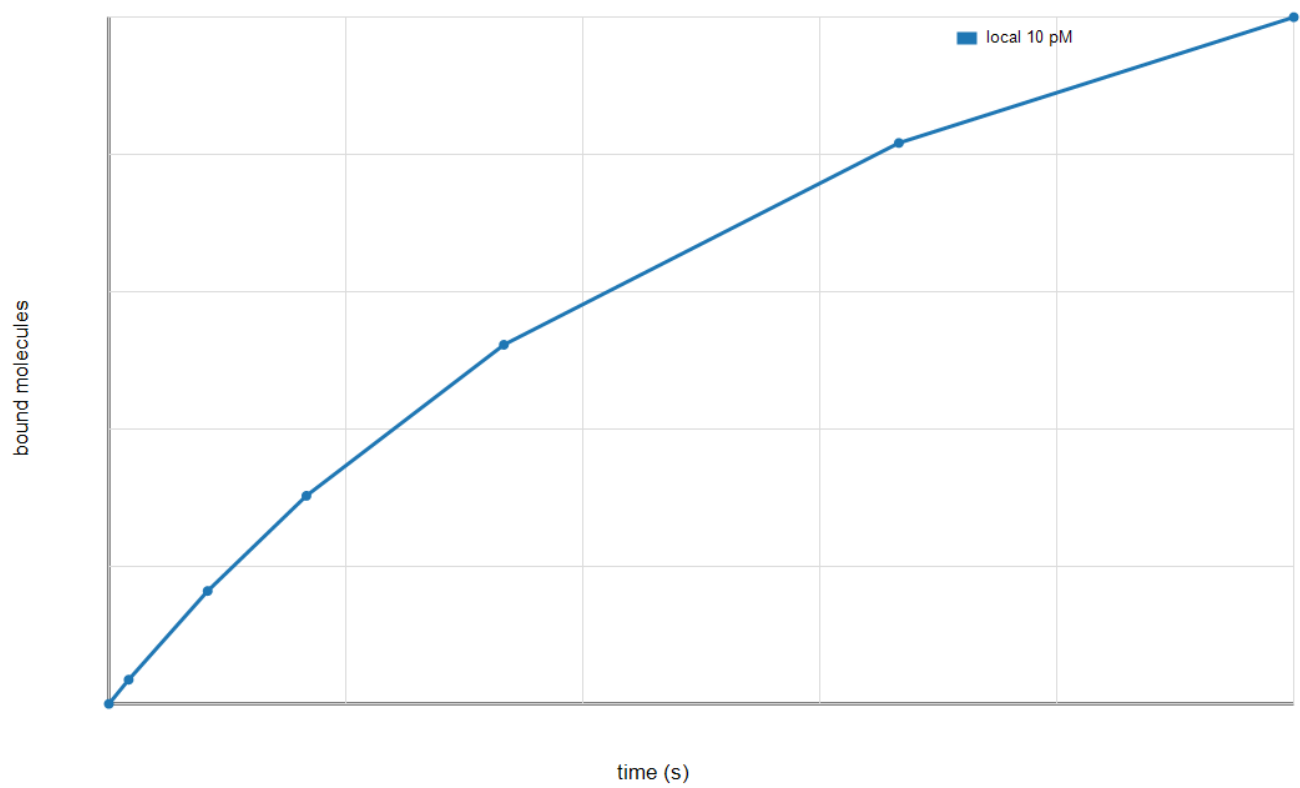


Fig. 17. Bound HER2 molecule count over time for local sensing at 10 pM.

M4 Deltalds vs HER2 concentration from COMSOL-stage binding

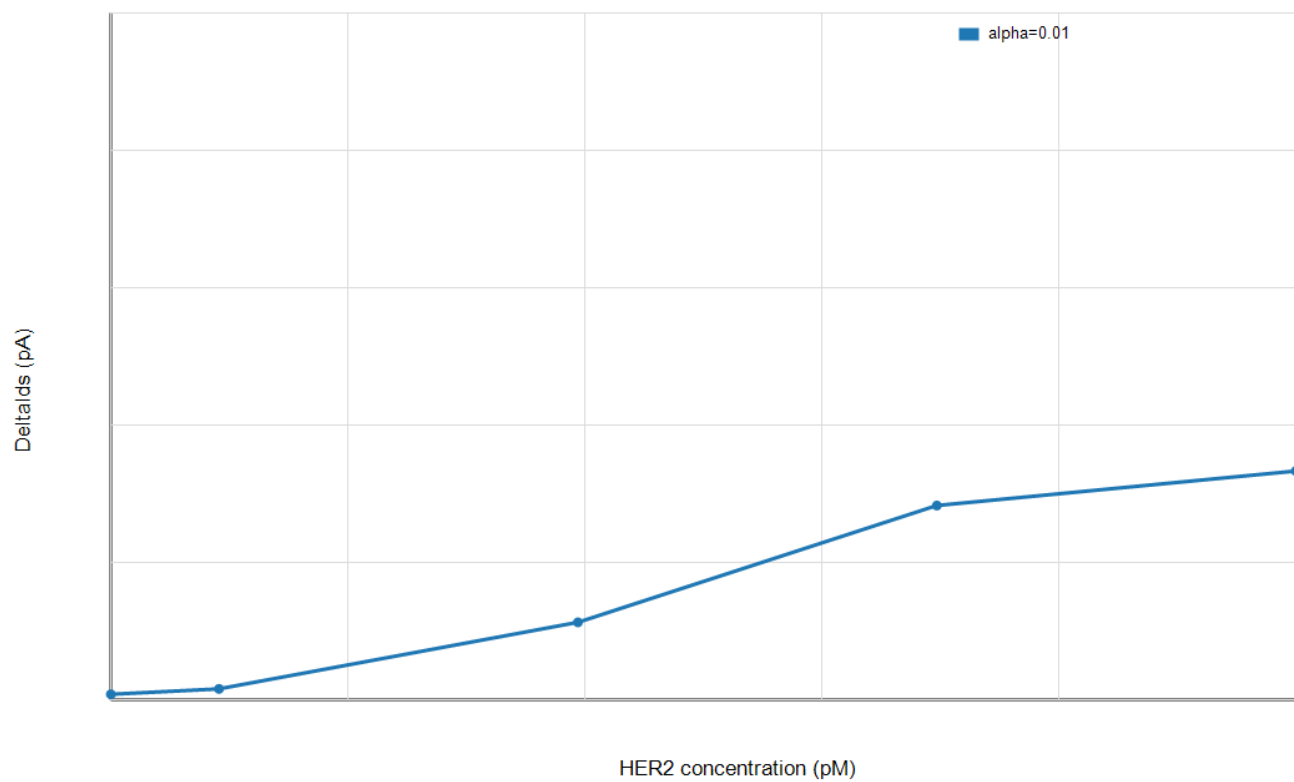


Fig. 18. GFET current response versus HER2 concentration.

M4 minimum detectable bound molecules

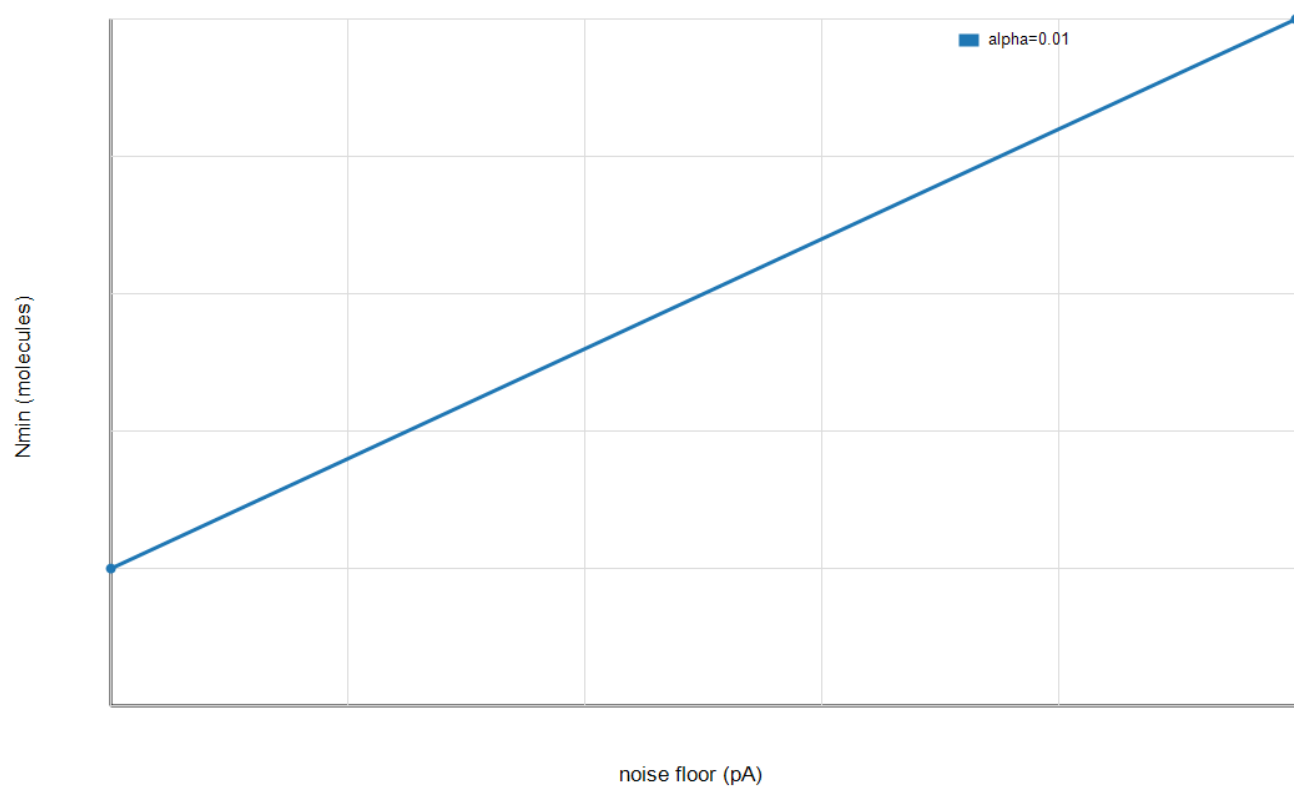


Fig. 19. Minimum detectable bound molecule count for coupling and noise-floor cases.

TABLE I
FINAL SCIENTIFIC CLAIMS SUPPORTED BY THE SIMULATION CAMPAIGN.

Claim	Supporting result	Figure/table	Assumption	Limitation	Confidence
HER2-antibody binding follows bounded saturation behavior across the modeled concentration range.	M1 occupancy increases monotonically with HER2 concentration and remains within [0, 1].	Fig. 1	Reversible Langmuir-type binding with baseline $K_d = 10$ pM.	No wet-lab binding calibration.	High for equation-level behavior.
Directional lymph-node-inspired flow changes sensor exposure compared with diffusion-only transport.	At $C = 10$ pM, $v_{in} = 5 \times 10^{-7}$ m/s gives 8.73 pM at 6000 s versus 4.98 pM for diffusion-only; time-to-50% exposure decreases from 6038 s to 1839 s.	Fig. 9	Prescribed velocity is coupled into TDS convection.	M2B is a partially anatomical prescribed-velocity convection-diffusion extension, not a full anatomical lymph-node model and not a validated Darcy-flow pressure solution.	Medium for model trend.
Sensor placement affects response timing and current response. In the modeled sweep, the subcapsular/cortical placement is fastest and strongest under the reference flow case. Under directional flow, late-time exposure becomes high across all tested placements, while placement still changes arrival time and pathway exposure.	Subcapsular/cortical placement is fastest and strongest under reference flow; late-time current range is 559.9–600.5 pA under flow and 348.2–533.3 pA under diffusion-only transport.	Fig. 10	Three placement regions are post-processed over the M2B transport model.	Placement sweep is not a full remeshed COM-SOL sensor relocation study; late-time flow response is high across all tested placements.	Medium for relative sensitivity.
Detectability is predicted only under favorable coupling, low-noise, and binding assumptions.	EXP C gives 99 detectable rows and 36 failing rows across concentration, α_0 , noise, and K_d sweeps.	Fig. 13	Analytical GFET response with $\Delta I_{DS} \geq 3\sigma$.	Graphene electronics and surface chemistry are simplified.	Medium for envelope; low for device claim.
PBS-like Debye screening strongly reduces effective GFET signal for long receptor distances.	For PBS-like $\lambda_D = 0.8$ nm and $d \geq 5$ nm, 0/60 screened cases remain detectable.	Fig. 14	$\alpha_{eff} = \alpha_0 \exp(-d/\lambda_D)$.	Debye lengths and distances are approximate assumptions.	Medium for screening direction.
Direct in-body HER2 detection likely requires short receptor distance, low-noise electronics, stronger transduction, or local screening mitigation.	Transport and placement improve antigen exposure, but detection fails under weak coupling, high noise, poor affinity, or PBS-like screening at longer distances.	Table I	Synthesis of M2B exposure, M3 binding, M4 response, and Debye attenuation.	Simulation-based design conclusion, not clinical validation.	High as modeling conclusion.
Feasible GFET-HER2 detection requires explicit design conditions on receptor distance, coupling, screening, and electronics noise.	Experiment E maps required α_0 , maximum allowed receptor-channel distance, and maximum allowed noise floor. For $K_d = 10$ pM, 10 pA noise, and PBS-like screening at 1 nm, required α_0 is 0.0326 at 1 pM and 0.00561 at 10 pM; at 2 nm it rises to 0.114 and 0.0196.	Fig. 16	M3/M4 analytical response with $\alpha_{eff} = \alpha_0 \exp(-d/\lambda_D)$ and $\Delta I_{DS} \geq 3\sigma$.	Simulation-based design requirement analysis, not experimental validation or fabricated device performance.	Medium for design trend.