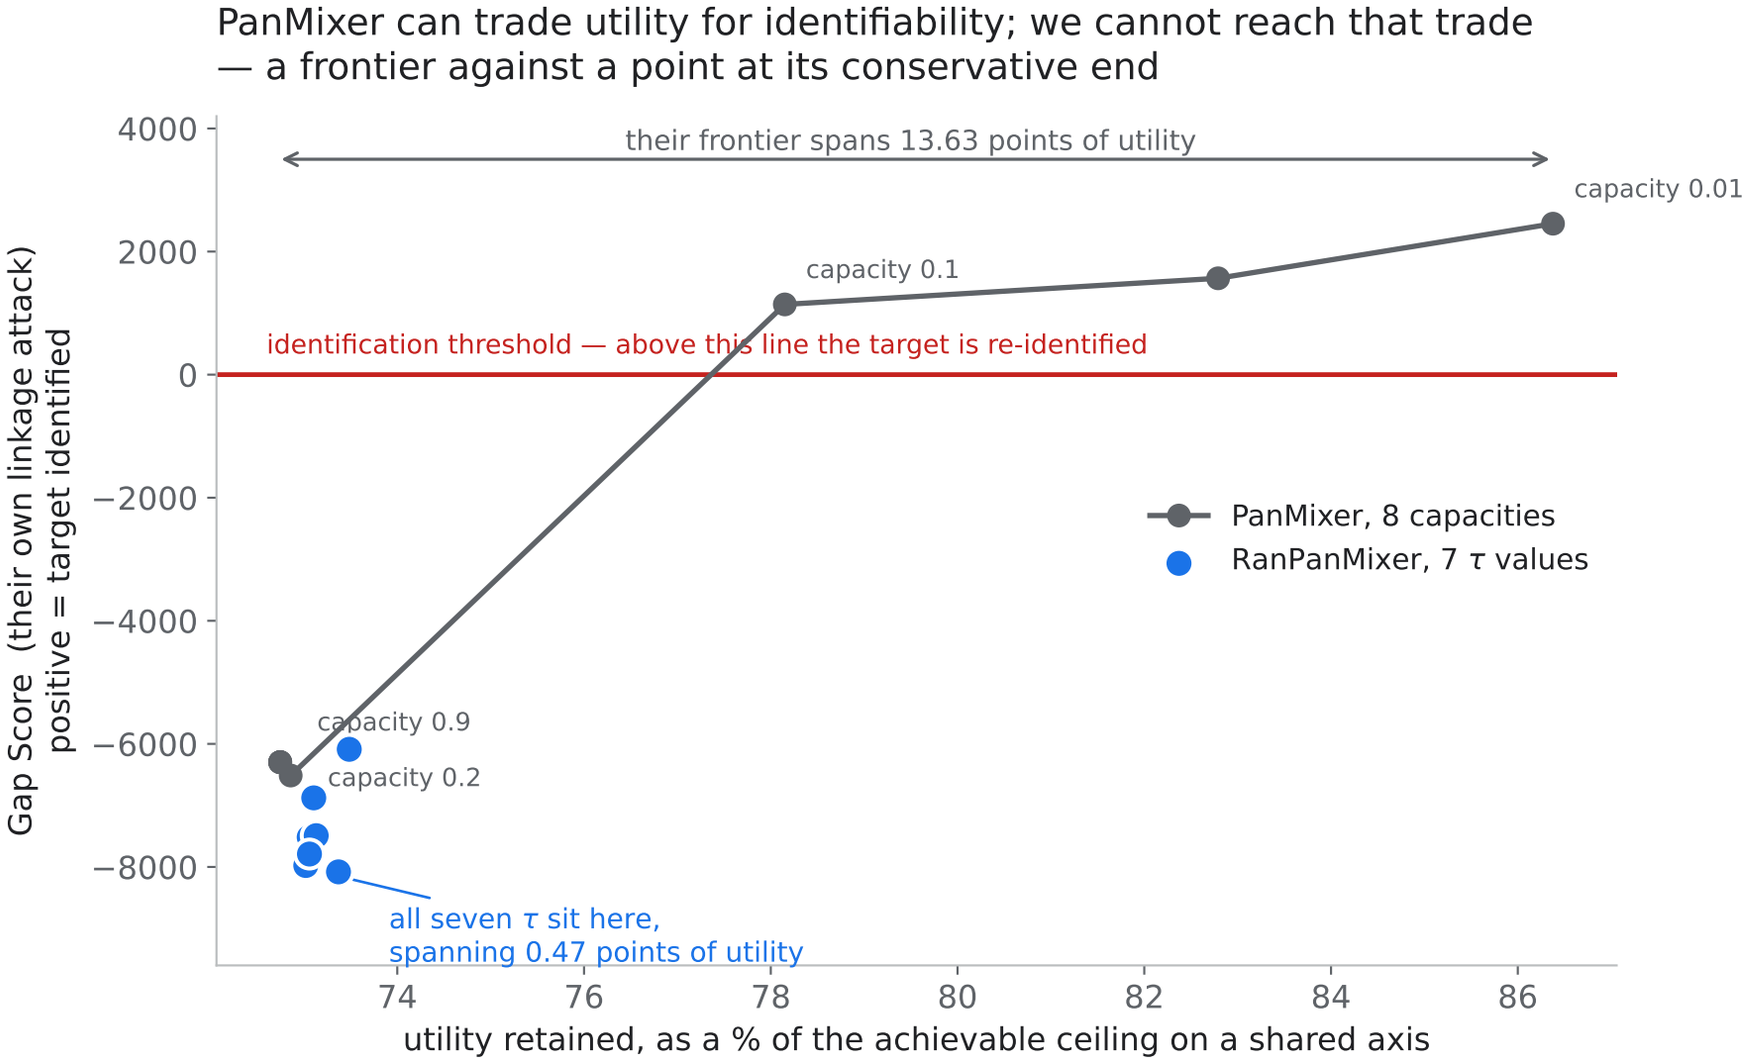

chr21, target HG00438, both tools' releases scored by ONE function on ONE shared position axis of 331,416 positions. Ceiling 0.014951984.
⚠ NOT a same-build comparison: their releases come from their own vg-1.36 pipeline and ours from our vg-1.68 rebuild, and the two builds disagree about the target's own genome at 1.34% of cells — which is LARGER than the gap between the tools. Only each side's share of its own total is quoted. ⚠ Their identification at low capacity is NOT a defect: the knob is meant to be turned up, and locating that threshold is what their published sweep is for. Provenance: logs/B_arm1_symmetric.md, logs/B_pm_eval_results.md