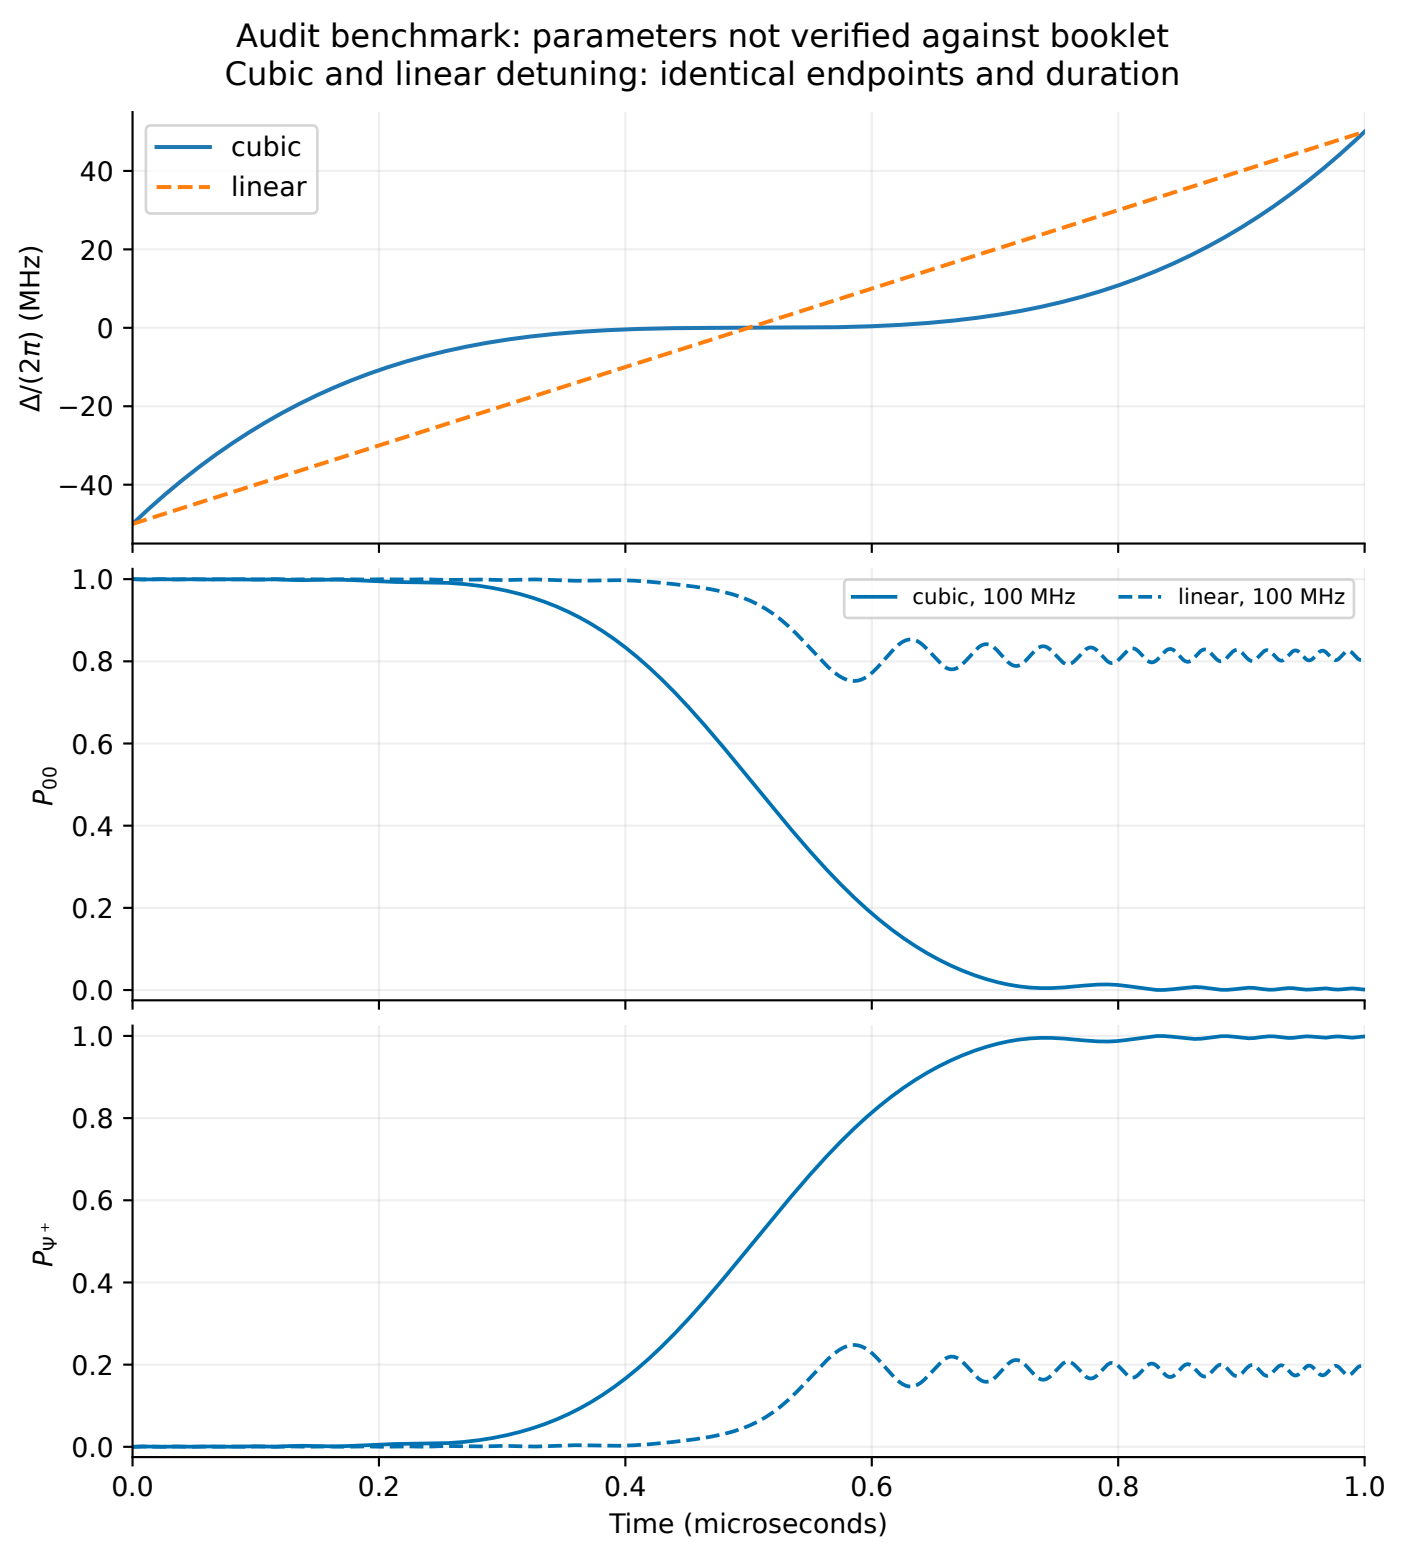
Audit benchmark: parameters not verified against booklet
Cubic and linear detuning: identical endpoints and duration
cubic
linear
Δ/(2π) (MHz)
40
20
0
−20
−40
cubic, 100 MHz
linear, 100 MHz
P_{00}
1.0
0.8
0.6
0.4
0.2
0.0
P_{Ψ^+}
1.0
0.8
0.6
0.4
0.2
0.0
0.0
0.2
0.4
0.6
0.8
1.0
Time (microseconds)