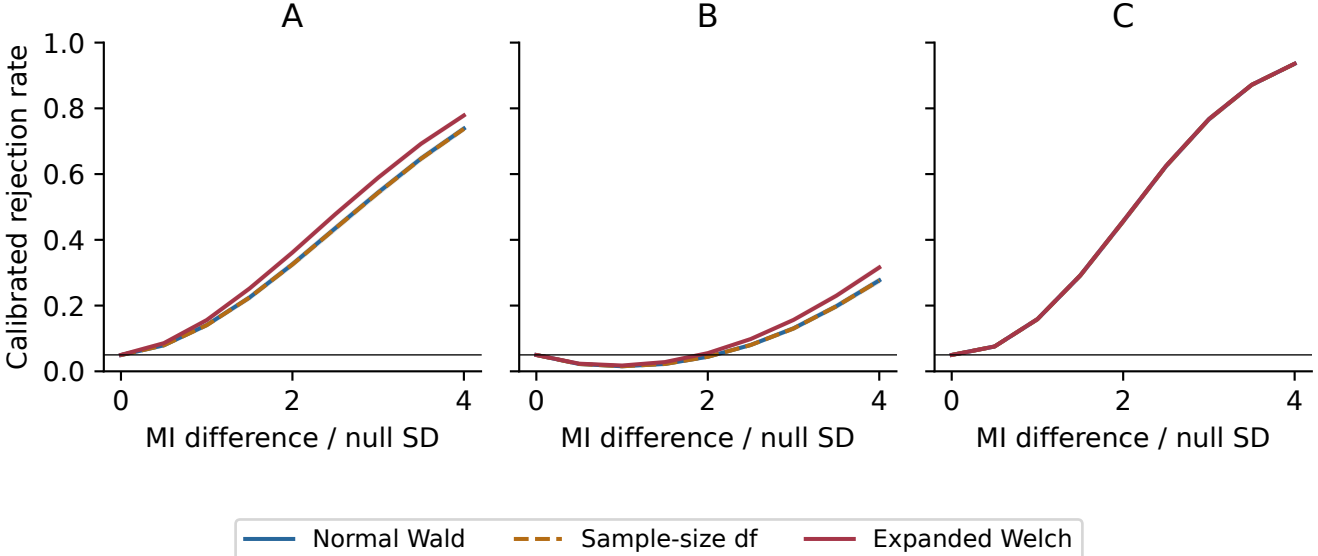
A
B
C
Calibrated rejection rate
1.0
0.8
0.6
0.4
0.2
0.0
0
2
4
MI difference / null SD
Normal Wald
Sample-size df
Expanded Welch