


AirSensEUR: Setting Automatic Calibration of sensors and displaying with InfluxDB/Grafana

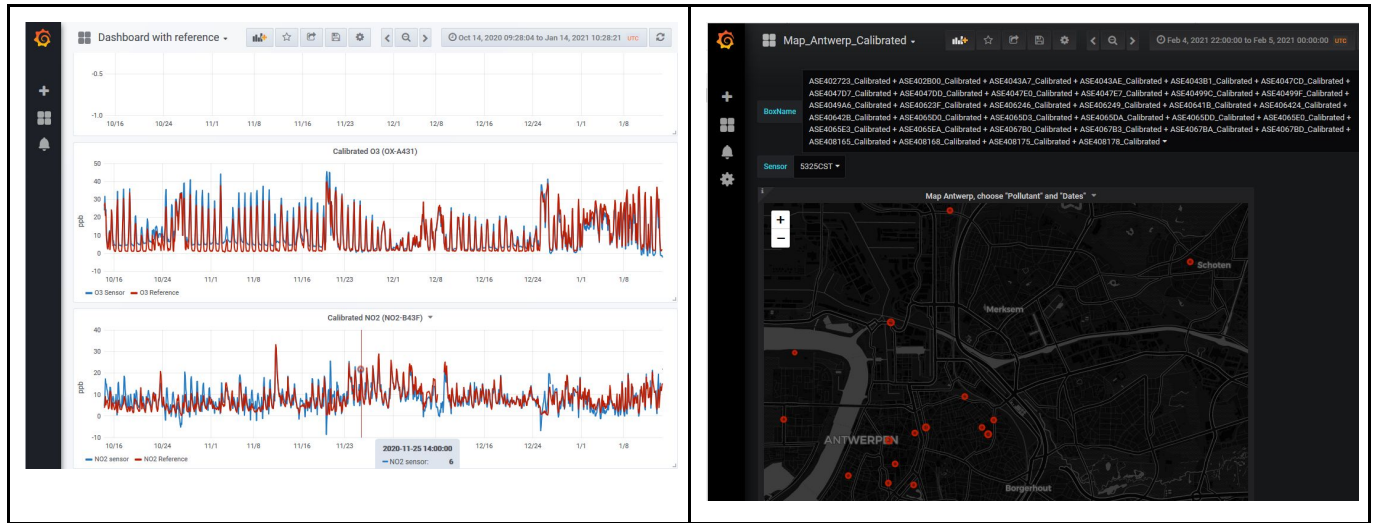

Yatkin, S., Gerboles, M., Signorini M. and Ferretti F.

The scripts needed in this document can be found at <https://github.com/ec-jrc/airsenseur-calibration>

1. Installing the necessary softwares

To install R, Rstudio and all needed scripts, follow instructions of section 3 of the ASE_App manual at <https://docs.google.com/document/d/1EYMYecUhdWfg0tKaOhZRfMb2Rbk-SQUPXWqXbw3BuII/edit?usp=sharing>


2. List of AirSenseEUR boxes for this guide

The list of AirSenseEUR boxes (ASE boxes) used for this example includes: 424A56, 42A57, 42D501, 425D0A, 425D0B and 4278FD

3. Configuration of AirSenseEUR boxes

The configuration files of at least one box among the 6 ASE boxes to set up shall be available. The simplest way to configure an ASE box is to use the ASE_App (app.R) available in the github using the configuration of a box already configured. In the following example, the ASE box 424A56 is used. However, it would be possible to manually create all the necessary config files.

1. Under the ASE_App directory (~/.Shiny) create a subdirectory where the ASE boxes configuration and data will be stored, for example “Federico”. Be sure to install a previously configured ASE boxes with similar sensor configuration with which you can duplicate the configuration files of the new ASE boxes configuration under “Federico”
2. Run RStudio
3. Open file file app.R, run the App.
4. The ASE App open in a browser or directly under RStudio.
5. If needed follows instruction in [5.1. Using the ASE_App.R](#) to clone a new ASE box from an existing one.
6. Select the project (e.g. Federico), ASE box (e.g. 424A56) and click on “Select AirSenseEUR for List”.

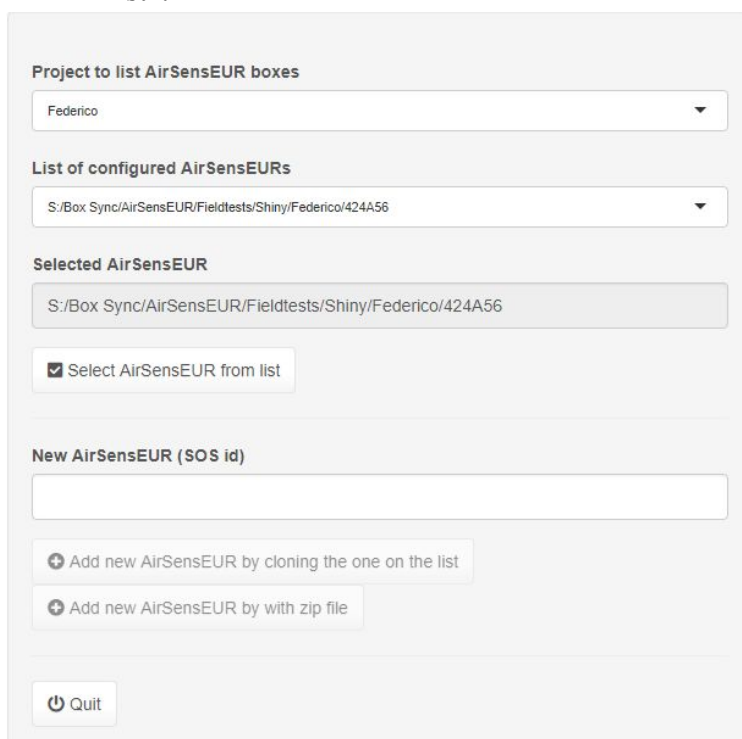

The screenshot shows the ASE_App web interface with the following elements:

- Project to list AirSenseEUR boxes:** A dropdown menu with "Federico" selected.
- List of configured AirSenseEURs:** A dropdown menu with "S:/Box Sync/AirSenseEUR/Fieldtests/Shiny/Federico/424A56" selected.
- Selected AirSenseEUR:** A text box displaying "S:/Box Sync/AirSenseEUR/Fieldtests/Shiny/Federico/424A56".
- Select AirSenseEUR from list:** A checkbox that is checked.
- New AirSenseEUR (SOS id):** An empty text input field.
- Add new AirSenseEUR by cloning the one on the list:** A button with a plus icon.
- Add new AirSenseEUR by with zip file:** A button with a plus icon.
- Quit:** A button with a power icon.

7. Under NavBarMenu “GetData”, Tab “Time.shield” set parameters as below to get minute data from InfluxDB and hourly predicted data :

Time-shield Proxy Sensor Data Reference Data

Averaging time in min for downloading

1

Averaging time in min for predicted data

60

Delay in min, add minutes to sensor time (automatic Save)

0

Sensor shield config file *.asc

200130 AS_NO2B43F_COA4_OXA431_NOB4_CO2_OPCN3_PMS5003_Final.asc

8. Defined a PROXY if needed under Tab “Proxy” set parameter for your Proxy if needed

Time-shield Proxy Sensor Data Reference Data

☒ Enable PROXY

URL of your proxy PORT

10.168.209.72 8012

LOGIN for the proxy PASSWORD of the proxy

9. Under Tab “Sensor Data”, tab “Influx”, set the parameters for InfluxDB download (url of Rest Api, port - 8086 or 3030, login, password, name of SQLite database and datasets name - ASE+AirSensEUR box ID). Click on “Enable InfluxDB”. Wait message “Server is up”. All data are downloaded when clicking on “Download Influx Data”.

Time-shield Proxy Sensor Data Reference Data

SOS Influx

☒ Enable InfluxDB Download Influx data

Influx Rest API Port

influxdb1.liberaintentio.com 8086

Login for the Host Password

shinyreader

SQLite database Available Datasets

jrcispra ASE424A56

Time Zone, Influx data are in UTC:

UTC

10. Uncheck “Enable InfluxDB”

11. Under Tab “Reference Data” set the downloading of Reference data. See ASE_App manual.

Time-shield Proxy Sensor Data **Reference Data**

☐ Enable download Reference data Download Reference data

Selected download

☐ csv ☐ ftp ☐ SOS ☒ a_i_p

csv ftp SOS **a_i_p**

URL of a_i_p Rest API

Login **Password**

ID of the Organisation **ID of the station**

Range of dates for downloading data of station:

to

Select pollutants to download

Identifier of the reference station

Longitude in decimal degrees or d'm's.s'E **Latitude in decimal degrees or d'm's.s'N**

Altitude of the reference station

Time Zone

12. Click on NavBarMenu “dataTreatment”. Wait for filtering calibration and prediction of sensor data

13. Observe your available data under Config|Downloaded

Config PlotFiltering Covariates Calibration Prediction Report M

Downloaded FilteringMain CalibMain SetTimeMain Sensors Bo

Data Sets	Exists	NeedRetrieve	INdate	ENDdate
airsenseur.db	TRUE	TRUE	2020-08-12 08:21:48	2021-01-14 20:00:46
InfluxData	TRUE	TRUE	2020-08-12 08:22	2021-01-14 20:01
SOSData	FALSE	TRUE	NULL	NULL
ReferenceData	TRUE	TRUE	2020-10-08 14:21	2021-01-14 20:00
General	TRUE	TRUE	2020-08-12 08:22	2021-01-14 20:01

14. Under Config|FilteringMain, Config|CalibMain and Config|SetTimeMain make sure that you correctly set the list of sensors you want to configure.

Edit the table. Double-click on a cell to edit data. The button "Save Config of Sensors" saves all configuration files of the ASE box The App will stop and shall be

Save Config of Sensors

	name.gas	name.sensor	gas.sensor	hoursWarming	temp.thres.min	temp.thres.max	rh.thres.min	rh.thres.max	Sens.Inval.Out
1	CO	CO_A4_P1	Carbon_monoxide	4	-20.00	40.00	15	100	<input checked="" type="checkbox"/>
2	CO2	D300	Carbon_dioxide	4	-20.00	40.00	15	100	<input checked="" type="checkbox"/>
3	NO	NO_B4_P1	Nitric_oxide	30	-20.00	40.00	15	100	<input checked="" type="checkbox"/>
4	NO2	NO2_B43F_P1	Nitrogen_dioxide	4	-20.00	40.00	15	100	<input checked="" type="checkbox"/>
5	O3	OX_A431_P1	Ozone	4	-20.00	40.00	15	100	<input checked="" type="checkbox"/>
6	PM1	5301CAT	PM1_PMSCal	4	-20.00	40.00	10	100	<input checked="" type="checkbox"/>
7	PM1	5301CST	PM1_PMSraw	4	-20.00	40.00	10	100	<input checked="" type="checkbox"/>
8	PM10	5310CAT	PM10_PMSCal	4	-20.00	40.00	10	100	<input checked="" type="checkbox"/>
9	PM10	5310CST	PM10_PMSraw	4	-20.00	40.00	10	100	<input checked="" type="checkbox"/>
10	PM2.5	5325CAT	PM25_PMSCal	4	-20.00	40.00	10	100	<input checked="" type="checkbox"/>
11	PM2.5	5325CST	PM25_PMSraw	4	-20.00	40.00	10	100	<input checked="" type="checkbox"/>
12	Patm	BMP280	Atmospheric_pressure	1	-40.00	65.00	0	100	<input checked="" type="checkbox"/>
13	RH	SHT31HE	Relative_humidity	1	-40.00	65.00	0	100	<input checked="" type="checkbox"/>
14	RH_int	SHT31HI	Relative_humidity_int	1	-40.00	65.00	0	100	<input checked="" type="checkbox"/>
15	Temp	SHT31TE	Temperature	1	-40.00	65.00	0	100	<input checked="" type="checkbox"/>
16	Temp_int	SHT31TI	Temperature_int	1	-40.00	65.00	0	100	<input checked="" type="checkbox"/>

Add a row of sensor configuration

Pollutant symbol (name.gas)

CO

Pollutant name (gas.sensor)

PM1_PMSCal

Sensor name (name.sensor)

5301CAT

Reference column (gas.reference2use)

Ref.NO2

Add

Delete a row of sensor configuration

Sensor name (name.sensor)

Del

15. Use ASE_App manual to delete sensors.
16. For example to delete sensor OPCN3PM25 select the sensor under “Delete a row of sensor configuration|Sensor name (Name.Sensor)”, click on button “Del” below and the sensor row is discarded from the table of configured sensors.
17. Use ASE_App manual to add sensors.
18. For example to add sensor OPCN3PM25 select: PM2.5 under “Add a row of sensor configuration|Pollutant symbol (name.gas), Particulate_Matter_25 under “Add a row of sensor configuration|Pollutant name (gas.sensor)”, OPCN3PM25 under “Add a row of sensor

configuration|Sensor name (name.sensor)” and Ref.PM2.5 under “Add a row of sensor configuration|Reference column (gas.reference2use)”, click on button “Add” below and the sensor row is added at the bottom of the table of configured sensors. Be sure to correctly set all columns in the 3 tables Config|FilteringMain, Config|CalibMain and Config|SetTimeMain. “Pollutant symbol (name.gas), “|Pollutant name (gas.sensor)” and “Sensor name (name.sensor)” can be found

at <https://docs.google.com/spreadsheets/d/1e1MJm8ut6s8UXP8lsMwij58CyJhWsvVuz2tdLWMpMpI/edit?usp=sharing>

19. In order to update the configuration, click on button “Save Config of Sensors” when all sensors are correctly configured. The ASE_App is automatically closed and shall be restarted to take change into account.
20. If you do not need to change any sensor in Config|FilteringMain , click on button “save” in the sidebar layout of NavBarMenu “Data Treatment” in order to save configuration files and data.

4. Calibration of AirSensEUR box (424A56)

In order to proceed with calibration it is necessary to add reference data within the ASE-App. See the ASE_App manual to insert reference data (<https://docs.google.com/document/d/1EYMYecUhdWfg0tKaOhZRFMb2Rbk-SQUPXWqXbw3BuII/edit?usp=sharing>).

The aim of the calibration is to establish calibration models, save them in files and register these calibration in the configuration files 424A56.cfg for the sensors to calibrate.

Calibration is carried out using script Compare_Model.R (see https://github.com/ec-jrc/airsenseur-calibration/tree/master/Auto_Calibration).

Please follow the following steps:

1. Update variable “Possible.Dir” corresponding to the the ASE_App directory (~/.Shiny)
2. Update variable “Project”, the sub directory where the ASE boxes are stored
3. Update variable “List .ASE”, the IDs of the ASE boxes to calibrate
4. Update variable “Place”, the name of the place where the calibration took place with colocation of sensor and reference data
5. Update variable “Cal_Interval”, the time interval for calibration
6. Update variable “Predict_Interval”, the time interval with colocation of ASE boxes and reference data for testing the calibration
7. Run the script

The calibration models are established and saved into the configuration file 424A56.cfg.

In this example only the electrochemical sensors for CO, NO, NO2 and O3 are calibrated

5. New AirSensEUR boxes configuration by cloning an existing one

When new ASE boxes have to be configured, it is necessary to clone an already configured ASE box with already existing calibration models. After cloning a box, all configuration files will be created and the ASE boxes will be using the same calibration files as the ASE box used for cloning. However, it is possible to establish dedicated calibration for the cloned ASE boxes using the file Compare_Model.R (see [4. Calibration of AirSensEUR box \(424A56 \)](#)) once the ASE boxes configurations are cloned.

There are two possibilities to configure new ASE Boxes:

- Using the ASE_App.R
- Run Script Cloning_ASE_Boxes.R if you want to create a batch of new ASE boxes

5.1. Using the ASE_App.R

Please follow the following steps:

1. Run the ASE_App in R studio

2. Select the project, the “List of Configured AirSenseEURs” will be updated listing all existing ASE boxes.
3. Select the ASE box you want to use for cloning under “List of configured AirSenseEURs”
4. Do not click on the button “Select AirSenseEUR from List” otherwise it is not possible to clone the selected ASE box to a new ASE box. The “Select AirSenseEUR” box shall remain empty.
5. In “New AirSenseEUR (SOS ID)” enter the ID of the new ASE box that you want to configure. The correct spelling of the ID is very important because the ID will be used to download sensor data from InfluxDB.
6. Click on button “Add new AirSenseEUR by cloning the one on the list”

ASE_App v0.23

SelectASE

GetData

Data Treatment

Memory

Push data

Filtering

PROXY	FA
URL	10.
PORT	80
LOGIN	
Down.Influx	FAI
Host	infl
Port	80
User	shi
Db	jrc
Dataset	AS
Influx.TZ	UT
Down.SOS	FAI
AirsensWeb	
AirSenseEur.name	42
SOS.TZ	UT
Down.Ref	FAI
FTPMode	a_i
urlref	

Project to list AirSenseEUR boxes

Federico

List of configured AirSenseEURs

S:/Box Sync/AirSenseEUR/Fieldtests/Shiny/Federico/424A56

Selected AirSenseEUR

S:/Box Sync/AirSenseEUR/Fieldtests/Shiny/Federico/424A56

☒ Select AirSenseEUR from list

New AirSenseEUR (SOS id)

+ Add new AirSenseEUR by cloning the one on the list

+ Add new AirSenseEUR by with zip file

Quit

5.2. Run Script Cloning_ASE_Boxes.R if you want to create a batch of new ASE boxes

The script for cloning ASE boxes, Cloning_ASE_Boxes.R, can be found at https://github.com/ec-jrc/airsenseur-calibration/tree/master/Auto_Calibration

Please follow the following steps:

1. Update variable “Possible.Dir” corresponding to the ASE_App directory (~ /Shiny)
2. Update variable “Project”, the sub directory where the ASE boxes are stored

3. Update variable "Cloning.path", the file path of the the ASE box used for cloning
4. Update variable "List.ASE", the list of IDs new ASE boxes to be cloned. The correct spelling of the IDs is very important because the IDs will be used to download sensor data from InfluxDB.
5. Run the script

6. Download, predict data and upload of calibrated data

6.1. Updating PROXY flag

It might be that the PROXY flag in file ./Project/Configuration/ASE_Servers.cfg is set to TRUE. If the server that will run Update_Influx.R has no configured PROXY, it is then necessary to set this flag to FALSE in order to avoid a timeout error.

All ./Project/Configuration/ASE_Servers.cfg can be edited manually to set the flag to FALSE.

Otherwise use the script Set_Proxy_FALSE.R found at https://github.com/ec-jrc/airsenseur-calibration/tree/master/Auto_Calibration

Please follow the following steps:

1. In RStudio Server, open the file Set_Proxy_FALSE.R
2. Update variable "Possible.Dir" corresponding to the the ASE_App directory (~/.Shiny)
3. Update variable "Project", the sub directory where the ASE boxes are stored, e. G. "Federico"
4. Update variable "DIR_Config", the sub directory where the config file ASE_Server.cfg are stored.
5. Update variable "List.ASE", the list of IDs of the ASE boxes to be updated, e.g. 424A56, 42A57, 42D501, 425D0A, 425D0B and 4278FD.
6. Run the script

6.2. Using script Update_Influx.R

The script for cloning ASE boxes, Update_Influx.R, can be found at https://github.com/ec-jrc/airsenseur-calibration/tree/master/Auto_Calibration

If the ASE.cfg has a calibration file registered for each sensor of the ASE box, the script Update_Influx.R can be run as it is. The aim of this script is to :

- download sensor data from InfluxDB (and reference data in requested into ASE.cfg),
- filter all data using the ASE configuration files,
- apply the calibration models,
- compute averages according to parameter UserAvgMins in ASE_sever.cfg,
- upload all calibrated data into a new InfluxDB table names ASE424A56_Calibrated.

Please follow the following steps:

1. Run RStudio
2. Open file Update_Influx.R
3. Update variable "Possible.Dir" corresponding to the the ASE_App directory (~/.Shiny)
4. Update variable "Project", the sub directory where the ASE boxes are stored
5. Update variable "DIR_Results", the sub directory where the calibrated data will be stored.
6. Update variable "List.ASE", the list of IDs of the ASE boxes to be updated, e.g. 424A56, 42A57, 42D501, 425D0A, 425D0B and 4278FD.
7. Since this script run in parallel computing, update the variables "cores" the number of cores dedicated to this script. It is necessary to set the number of cores that shall not be used and the maximum number of cores that can be used.
8. Update argument "Add.Ref", taking care whether reference data are available for each ASE box in List.ASE. i is the index of ASE box into List.ASE. Requesting to upload reference data if theory are not available will result in a crash of the script.
9. Update user and pass in Upload2Influx function call. A user with write credentials in InfluxDB.
10. Update the names of reference analysers in the argument Ref_analysers of the Upload2Influx function call if needed.
11. Run the script

This script creates a log file, named Log_Parallel.txt, in ~/Shiny with console message in order to observe info, warning and error messages.

In directory DIR_Results, a csv file with calibrated data s is created for each ASE box listed in List.ASE. The name of the file is ASE424A56_Calibrated.csv. It is a sequential file (long format) with the following headers:

- Time, datetime with UTC time zone in all rows
- ID_ASE, ID of ASE box in all rows
- Latitude, in decimal degrees if available
- Longitude, in decimal degrees if available
- Variable, name of the pollutant in all rows (see table below)
- Name.sensor, brand model of the sensor in all rows (see table below)
- Serial, part number of the sensor as stored into the ASE box in all rows
- Value, numeric pollutant concentration level in all row
- Uncertainty, not yet implemented
- Sens.unit, sensor unit for value and uncertainty in all rows, it can be ppb, ppm, µg.m-3, mg.m-3, hPa, percent or Celsius

Name.sensor	Variable (sensor)	Name.sensor	Variable (reference)
CO_A4_P1	Carbon_monoxide	As set in Ref_Analysers	Ref.CO_ppm
D300	Carbon_dioxide	As set in Ref_Analysers	Ref.CO2
NO_B4_P1	Nitric_oxide	As set in Ref_Analysers	Ref.NO
NO2_B43F_P1	Nitrogen_dioxide	As set in Ref_Analysers	Ref.No2
OX_A431_P1	Ozone	As set in Ref_Analysers	Ref.O3
5301CAT	PM1_PMSCal	As set in Ref_Analysers	Ref.PM1
5301CST	PM1_PMSraw	As set in Ref_Analysers	Ref.PM1
OPCN3PM1	Particulate_Matter_1	As set in Ref_Analysers	Ref.PM1
5310CAT	PM10_PMSCal	As set in Ref_Analysers	Ref.PM10
5310CST	PM10_PMSraw	As set in Ref_Analysers	Ref.PM10
OPCN3PM10	Particulate_Matter_10	As set in Ref_Analysers	Ref.PM10
5325CAT	PM25_PMSCal	As set in Ref_Analysers	Ref.PM2.5
5325CST	PM25_PMSraw	As set in Ref_Analysers	Ref.PM2.5
OPCN3PM25	Particulate_Matter_25	As set in Ref_Analysers	Ref.PM2.5
BMP280	Atmospheric_pressure	As set in Ref_Analysers	Ref.Patm
SHT31HE	Relative_humidity	As set in Ref_Analysers	Ref.RH
SHT31TE	Temperature	As set in Ref_Analysers	Ref.Temp

This script create a subdirectory as set by variable “Dir_results” under subdirectory “Project” with the calibrated data in csv format for each ASE box. Here below is an example file:

2020-08-17T03:00:00Z,424A56,,,Carbon_monoxide,CO_A4_P1,132770002,0.205839302283235,ppm

```

2020-08-17T04:00:00Z,424A56,,,Carbon_monoxide,CO_A4_P1,132770002,0.185832485787055,ppm
2020-08-17T05:00:00Z,424A56,,,Carbon_monoxide,CO_A4_P1,132770002,0.187809807450509,ppm
2020-08-17T06:00:00Z,424A56,,,Carbon_monoxide,CO_A4_P1,132770002,0.184110836413108,ppm
2020-08-17T07:00:00Z,424A56,45.8028491646689,8.87780811838155,Carbon_monoxide,CO_A4_P1,132770002,0.191265981781329,ppm
2020-08-17T08:00:00Z,424A56,45.8027878113959,8.87771035674331,Carbon_monoxide,CO_A4_P1,132770002,0.226326194085613,ppm
2020-08-17T09:00:00Z,424A56,45.8027952070114,8.87772618428675,Carbon_monoxide,CO_A4_P1,132770002,0.19089075050752,ppm
2020-08-17T10:00:00Z,424A56,45.8027970838767,8.87765639656857,Carbon_monoxide,CO_A4_P1,132770002,0.179253062912472,ppm
2020-08-17T11:00:00Z,424A56,45.80277316058,8.87766291271688,Carbon_monoxide,CO_A4_P1,132770002,0.210342077568943,ppm
2020-08-17T12:00:00Z,424A56,45.8027625952042,8.87766927757061,Carbon_monoxide,CO_A4_P1,132770002,0.194424178335888,ppm
2020-08-17T13:00:00Z,424A56,45.8027898293956,8.87770149511484,Carbon_monoxide,CO_A4_P1,132770002,0.155698103636009,ppm
2020-08-17T14:00:00Z,424A56,45.8028100035291,8.87770130602524,Carbon_monoxide,CO_A4_P1,132770002,0.167505013178069,ppm
2020-08-17T15:00:00Z,424A56,45.8028094830806,8.87770274949484,Carbon_monoxide,CO_A4_P1,132770002,0.0963343088766343,ppm
2020-08-17T16:00:00Z,424A56,45.8028505170434,8.87765018341248,Carbon_monoxide,CO_A4_P1,132770002,0.063821622622475,ppm
2020-08-17T17:00:00Z,424A56,45.8028260736606,8.87768216972167,Carbon_monoxide,CO_A4_P1,132770002,0.155644761935321,ppm
2020-08-17T18:00:00Z,424A56,45.8028041932017,8.8776803068755,Carbon_monoxide,CO_A4_P1,132770002,0.275444703574812,ppm
2020-08-17T19:00:00Z,424A56,45.802813142357,8.87757329618056,Carbon_monoxide,CO_A4_P1,132770002,0.247171762840897,ppm
2020-08-17T20:00:00Z,424A56,45.8027549146813,8.87762735542141,Carbon_monoxide,CO_A4_P1,132770002,0.252035054448501,ppm
2020-08-17T21:00:00Z,424A56,45.8027856085028,8.87769112066101,Carbon_monoxide,CO_A4_P1,132770002,0.251400472147206,ppm
2020-08-17T22:00:00Z,424A56,45.8027844952341,8.87761807315286,Carbon_monoxide,CO_A4_P1,132770002,0.241732748739656,ppm
2020-08-17T23:00:00Z,424A56,45.8027640579584,8.87766851260264,Carbon_monoxide,CO_A4_P1,132770002,0.242043602098841,ppm

```

7. Automatic update of calibrated data in InfluxDB

7.1. Using a Cron job under a Linux server

The automatic update of calibrated data is performed setting a CRON job file.

Create a text file (Cronjob.txt) with the following text assuming that the file path of the script is /home/shinyadmin/App and that a log of the process is saved and named Download_Predict.log:

```

30 * * * * cd /home/shinyadmin/App; Rscript Update_Influx.R
>/home/shinyadmin/App/Download_Predict.log 2>&1


```

Add it into your crontab file. You can open the file by using command `crontab -e`


7.2. Using task scheduler under windows

Open task scheduler under windows and create a job like:


General:

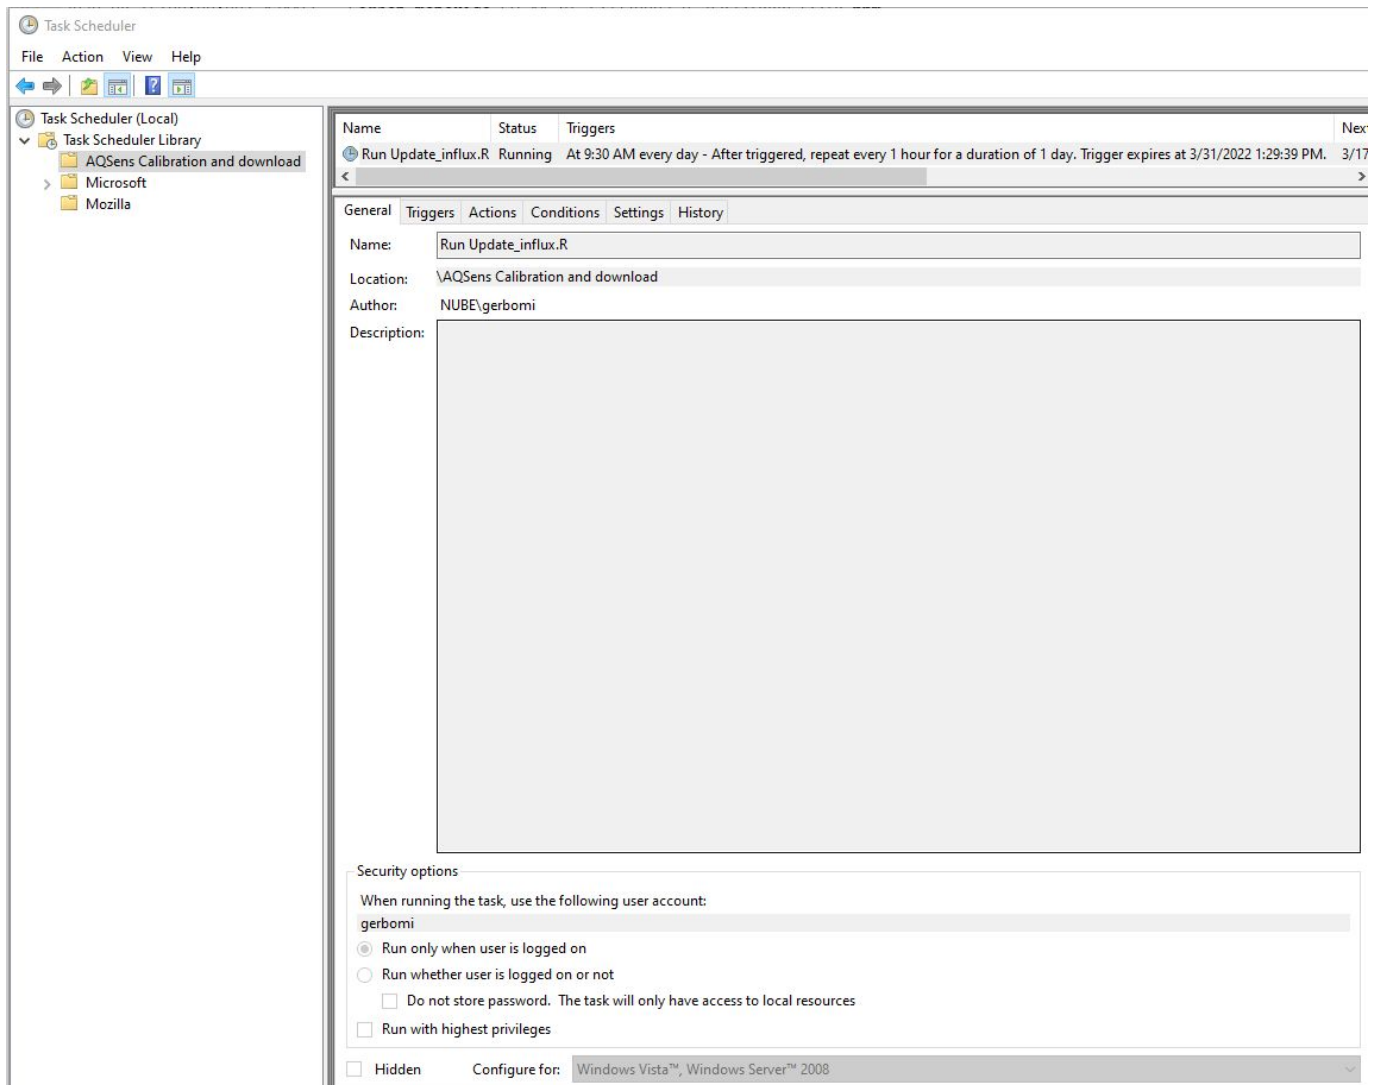

Triggers:

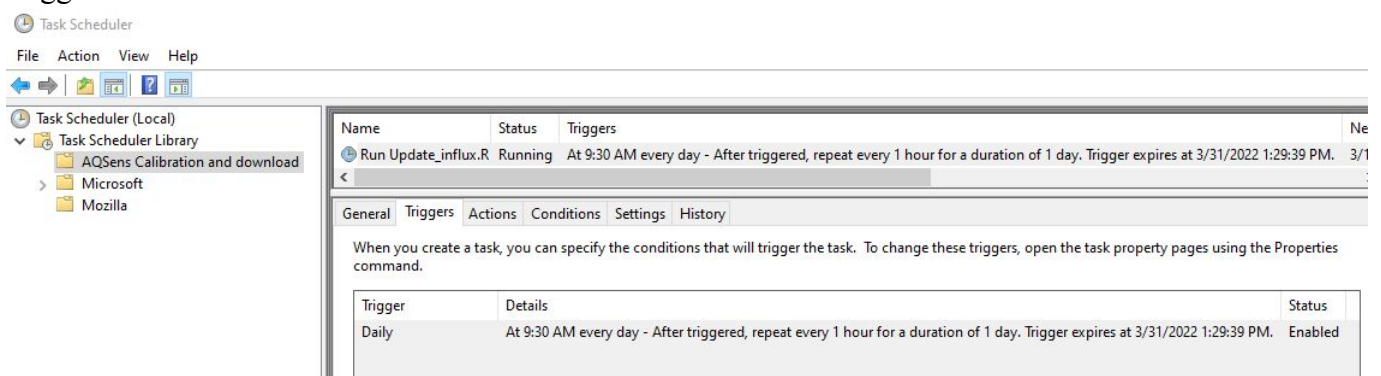

Action:

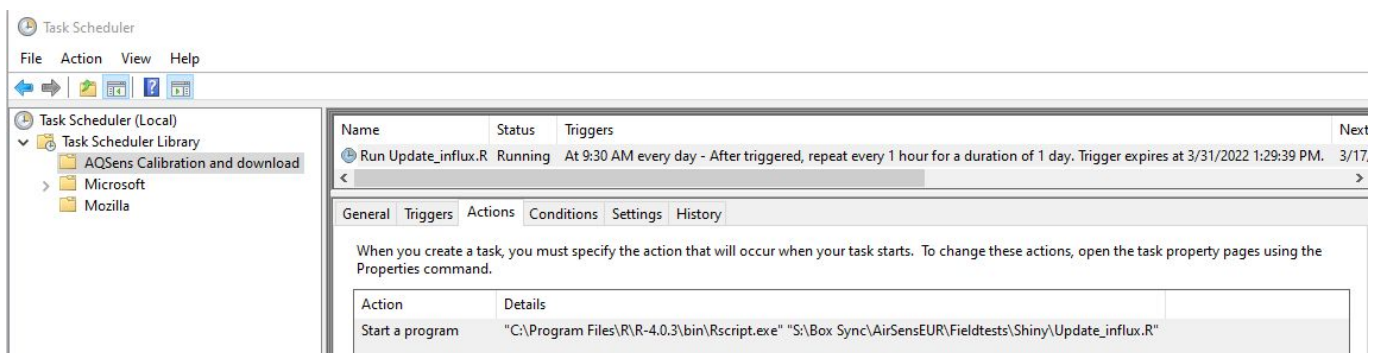


8. Display data with grafana

8.1. Dashboard with time-series data

Please follow the following steps:

1. Create a new dashboard by clicking on “Importing dashboard”

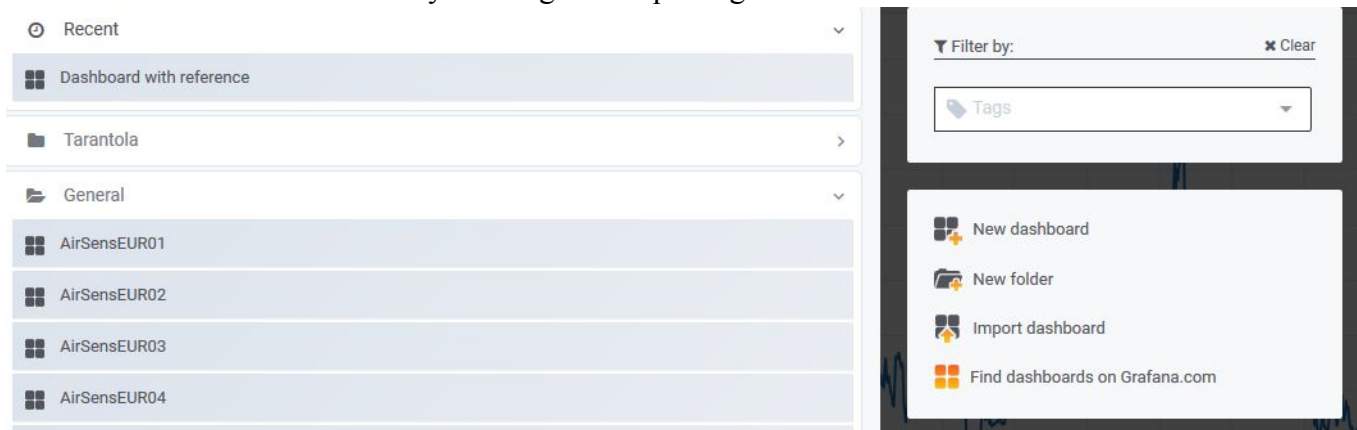

2. Paste the JSON code from JSON template “Dashboard with Reference”(https://github.com/ec-jrc/airsenseur-calibration/tree/master/Auto_Calibration/Grafana), click on load and set name

A screenshot of the 'Import dashboard' form in Grafana. At the top right is a green 'Upload .json File' button. Below it, the 'Grafana.com Dashboard' section has a text input field for 'Paste Grafana.com dashboard url or id'. The 'Or paste JSON' section features a large text area containing a JSON template. The JSON includes time ranges ('24h', '2d', '7d', '30d'), a timezone ('utc'), a title ('Dashboard with reference'), a uid ('Ugry7hEMk'), and a version ('12'). A blue 'Load' button is at the bottom left of the JSON area.

3. In settings|Variables, variable “BoxName”, update Values separated by comma with List.ASE, e.g. ASE424A56_Calibrated, ASE424A57_Calibrated, ASE42D501_Calibrated, ASE425D0A_Calibrated, ASE425D0B_Calibrated, ASE4278FD_Calibrated. Click on “Save”.

Settings

General

Annotations

Variables

Links

Versions

View JSON

Save

Save As...

Delete

Variables > Edit

General

Name	BoxName	Type	Custom
Label	optional display name	Hide	

Custom Options

Values separated by comma

ASE424A56_Calibrated, ASE424A57_Calibrated, ASE42D501_Calibrated, ASE425D0A_Calibrated, ASE425D0B_Calibrated, ASE427 ...

Selection Options

Multi-value


Include All option

Preview of values (shows max 20)

ASE424A56_Calibrated ASE424A57_Calibrated ASE42D501_Calibrated ASE425D0A_Calibrated ASE425D0B_Calibrated ASE4278FD_Calibrated

Update

4. Update source: edit all plots, under tab “Metrics” set “Data Source” to the InfluxDB database name

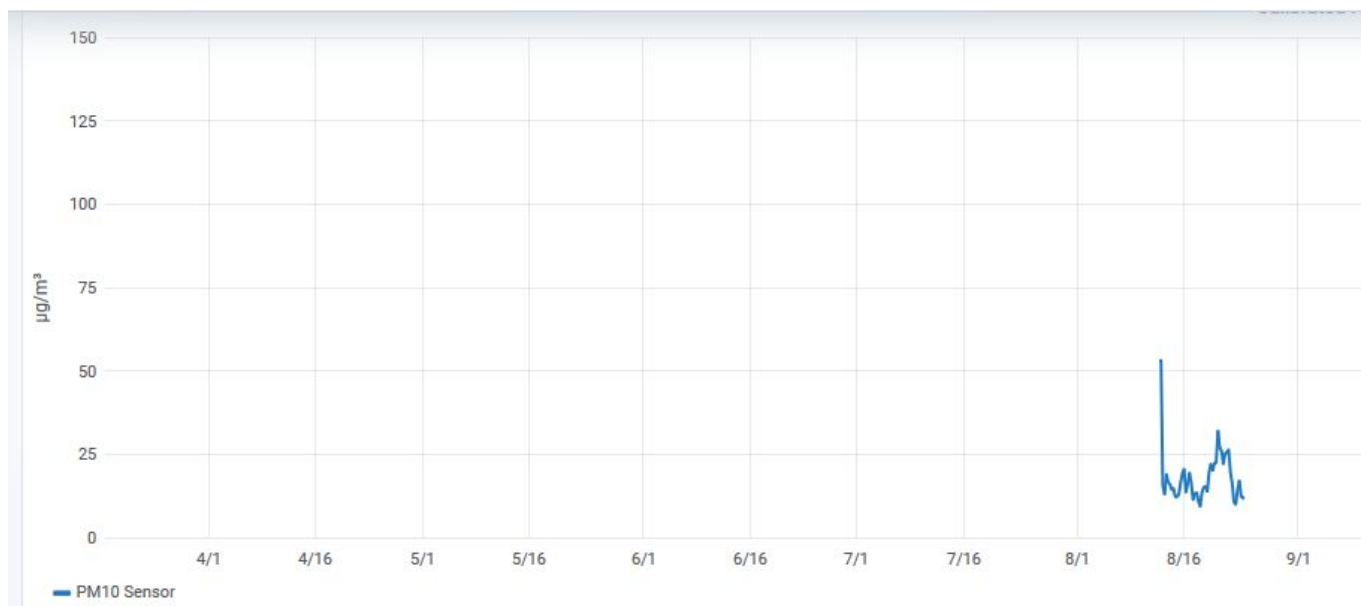


Graph General **Metrics** Axes Legend Display Alert Time range

Data Source: JRCIspra

A	FROM	default	/^\$BoxName\$/	WHERE	name_sensor	=	5310CST	+
	SELECT	field (value)	mean ()	+				
	GROUP BY	time (\$__interval)	fill (null)	+				
	FORMAT AS	Time series						
	ALIAS BY	PM10 Sensor						
B	FROM	default	/^\$BoxName\$/	WHERE	variable	=	Ref.PM10	+
	SELECT	field (value)	mean ()	+				
	GROUP BY	time (\$__interval)	fill (null)	+				
	FORMAT AS	Time series						
	ALIAS BY	PM10 Reference						

- In settings|Variables Update Values separated by comma with List.ASE, e.g. ASE424A56_Calibrated, ASE424A57_Calibrated, ASE42D501_Calibrated, ASE425D0A_Calibrated, ASE425D0B_Calibrated, ASE4278FD_Calibrated. Then click on button “Save”.

In the dashboard, it is possible to select which ASE box to display with calibrated sensor data (blue line) and reference data in red (if available) using the “BoxName” list and adapt the date interval on the upper left corner to display the desired time interval.

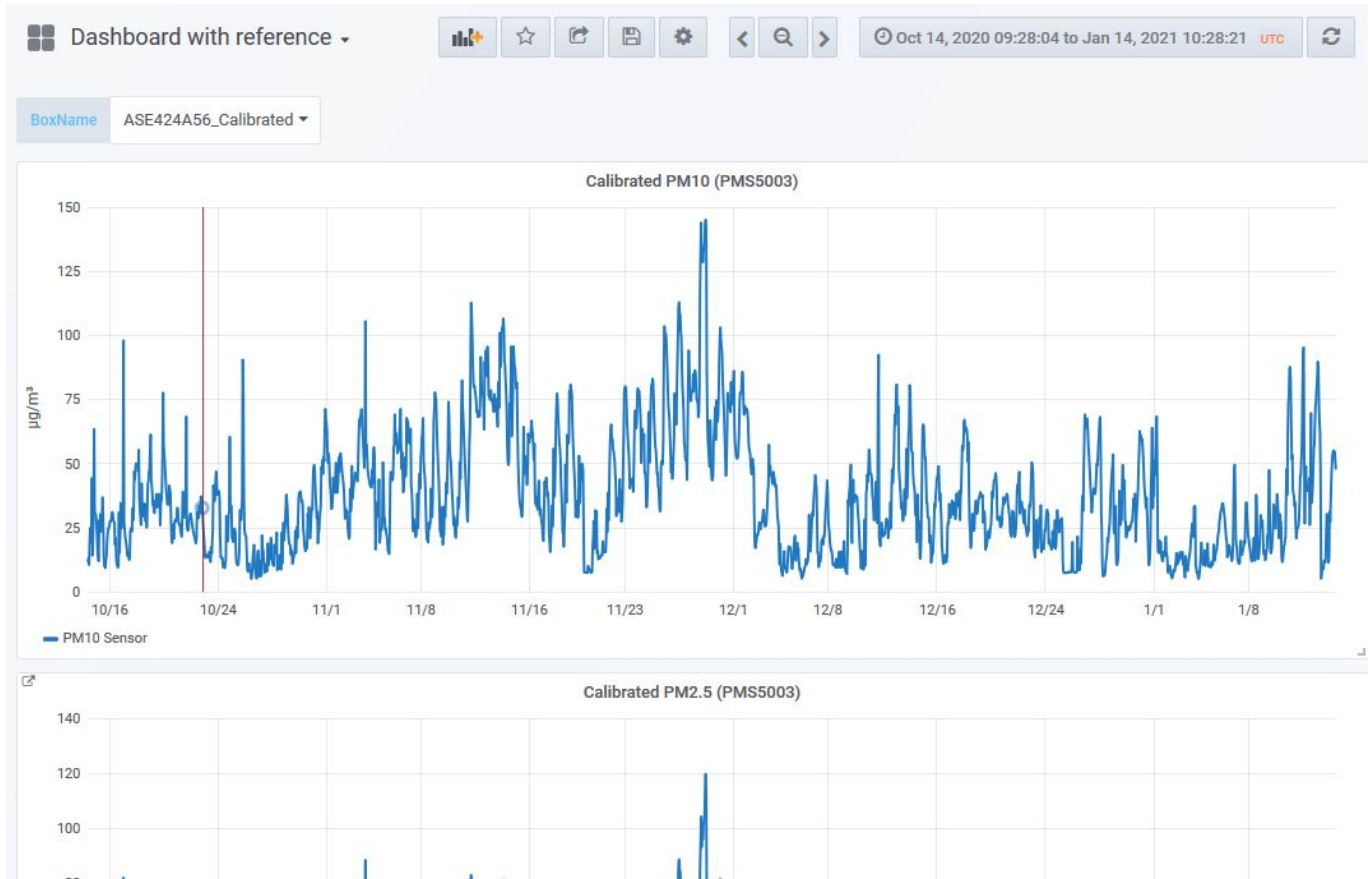

8.2. Maps

Please follow the following steps:

1. Repeat steps 1 to 3 of [8.1. Dashboard](https://github.com/ec-jrc/airsenseur-calibration/tree/master/Auto_Calibration/Grafana) using JSON template Map_Calibrated (https://github.com/ec-jrc/airsenseur-calibration/tree/master/Auto_Calibration/Grafana)
2. In settings|Variables, variable “Sensor”, update “Data Source” to the name of the InfluxDB database and update “Query” with List.ASE IDs, e.g. SHOW TAG VALUES FROM ASE424A56_Calibrated, ASE424A57_Calibrated, ASE42D501_Calibrated, ASE425D0A_Calibrated, ASE425D0B_Calibrated, ASE4278FD_Calibrated WITH KEY = "name_sensor". Click on “Save”.

Settings

General

Annotations

Variables

Links

Versions

View JSON

Save

Save As...

Delete

Variables > Edit

General

Name	Sensor	Type	Query
Label	optional display name	Hide	

Query Options

Data source		Refresh	On Time Range Change
Query	SHOW TAG VALUES FROM ASE424A56_Calibrated, ASE424A57_Calibrated, ASE42D501_Calibrated, ASE425D0A_Calibrated, ASE425D0B_Calibrat ...		
Regex	/.*(-.*)*/		
Sort	Alphabetical (asc)		

Selection Options

Multi-value	<input type="checkbox"/>
Include All option	<input type="checkbox"/>

Value groups/tags (Experimental feature)

Enabled	<input type="checkbox"/>
---------	--------------------------

Update

- Update source: edit the map, under tab “Metrics” set “Data Source” to the InfluxDB database name
- Update map coordinates: edit the map, under tab “Worldmap” set “Center” coordinates and “initial zoom”

+

-

Worldmap Panel

General

Metrics

Worldmap

Time range

Map Visual Options

Center	custom	45.810	8.63
Initial Zoom	15		
Min Circle Size	2		
Max Circle Size	8		
Sticky Labels	<input type="checkbox"/>		
Decimals	1		
Unit	singular form	plural form	
Show Legend	<input type="checkbox"/>		
Mouse Wheel Zoom	<input checked="" type="checkbox"/>		

Map Data Options

Location Data	table
Aggregation	current

Mapping Between Table Query and Worldmap

The query should be formatted as Table data and contain latitude, longitude columns and a numeric metric column.

- Location Name Field (optional):** enter the name of the Location Name column. Used to label each circle on the map. If it is empty then the value N/A is used as the label.
- Latitude/Longitude Fields:** enter the name of the latitude and longitude columns. These are used to calculate where the circle should be drawn.
- Metric Field:** enter the name of the metric column. This is used to give the circle a value - this determines how large


Threshold Options

Thresholds	0
Colors	■ ■

Hide series

With only nulls	<input checked="" type="checkbox"/>
With only zeros	<input checked="" type="checkbox"/>

- In the Dashboard under “BoxName”, select all ASE boxes.

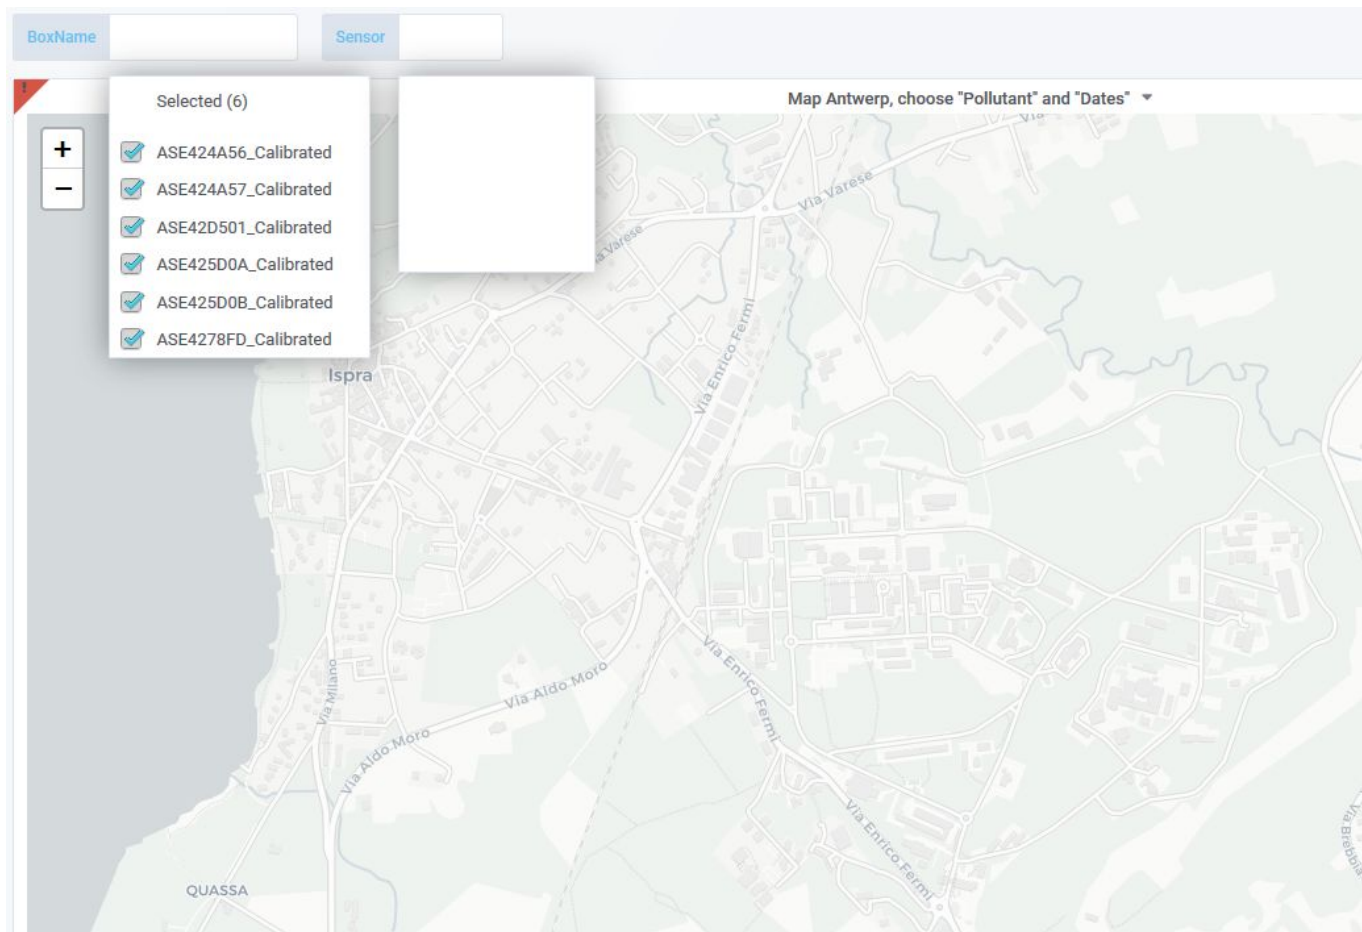

6. Update source: edit the map in the dashboard, under tab “Metrics” set “Data Source” to the InfluxDB database nameData Source” to the InfluxDB database name

BoxName

ASE424A56_Calibrated + ASE424A57_Calibrated + ASE425D01_Calibrated + ASE425D0A_Calibrated + ASE425D0B_Calibrated + ASE4278FD_Calibrated

Sensor

NO_B4_P1

Map Antwerp, choose "Pollutant" and "Dates"

Worldmap Panel

General

Metrics

Worldmap

Time range

Data Source

JRCIspra

Options

Help

FROM	default	/^{BoxName\$}/		WHERE	name_sensor	AND	/^{Sensor\$}/		+
SELECT	field (latitude)	mean ()	alias (latitude)	+					
	field (longitude)	mean ()	alias (longitude)	+					
	field (value)	mean ()	alias (calibrated_value)	+					
GROUP BY	time (\$interval)	tag (ASE)	+						
LIMIT	1								
FORMAT AS	Table								

7. Make sure all ASE boxes are selected in the “BoxName”. Choose sensor in variable list “Sensor”

In the map, it is possible to select which sensor data to display using the “BoxName” list and adapt the date interval on the upper left corner to display the desired time interval. Sensor data are displayed with red dots whose size is proportional to the value of the pollutant levels at each ASE box location. When hovering the red dots a window opens giving the ASE ID and pollutant value.

The map may not display the pollutant values if the time interval is too wide (more than a month?). In this case an error message will display.

9. Appendix 4: Description of configuration files

9.1. ASE.cfg

9.2. ASE_server.cfg

9.3. ASE_SetTime.cfg