




Passing Probes

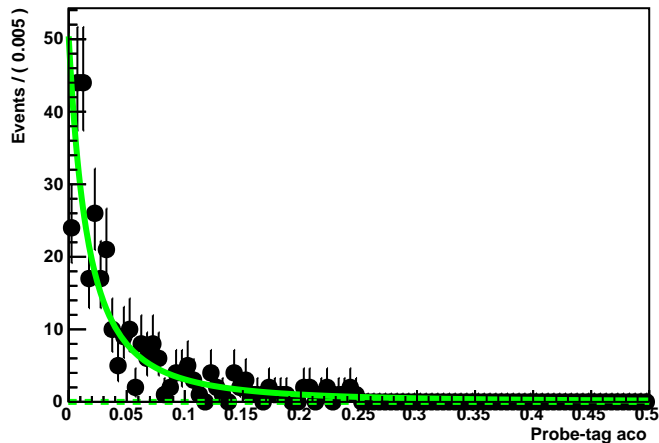

Failing Probes

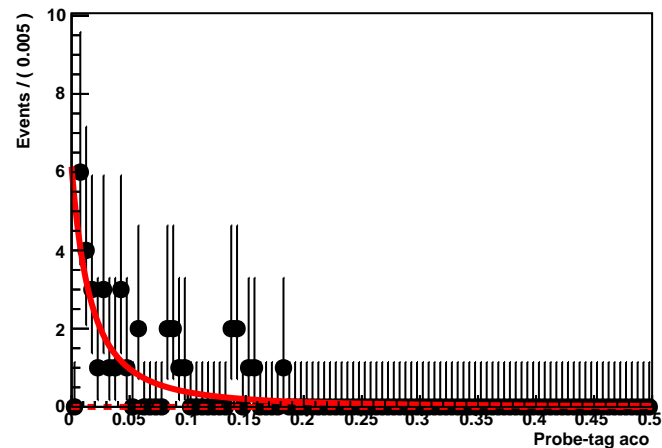

All Probes

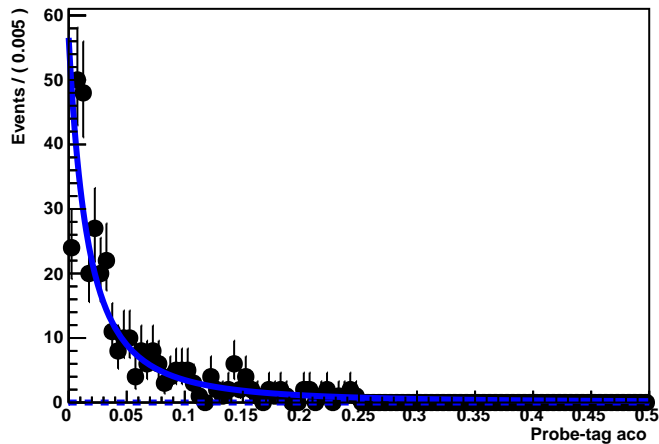

decayBkgF = -4.6
 decayBkgP = -4.6
 efficiency = 0.89 ± 0.02
 numBackgroundFail = 0 ± 2
 numBackgroundPass = 0 ± 1
 numSignalAll = 350 ± 19