




Passing Probes

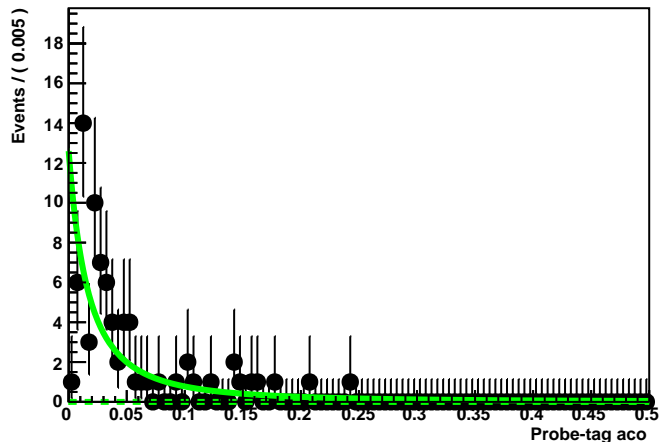

Failing Probes

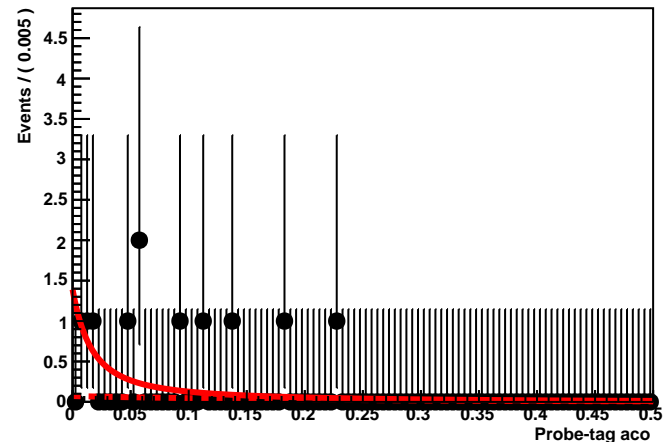

All Probes

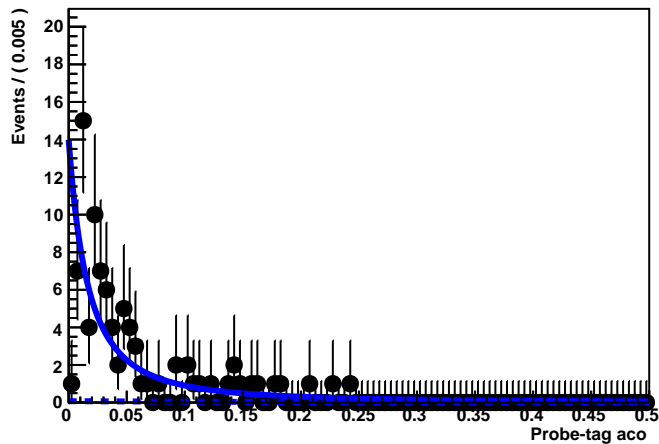

decayBkgF = -4.6
 decayBkgP = -4.6
 efficiency = 0.91 ± 0.05
 numBackgroundFail = 3 ± 4
 numBackgroundPass = 0 ± 1
 numSignalAll = 86 ± 10