




Passing Probes

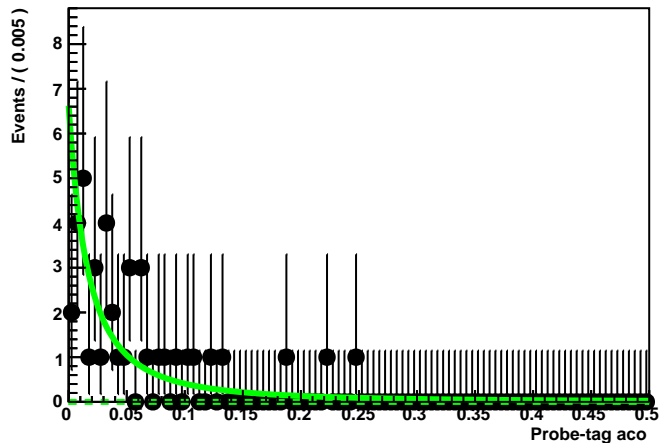

Failing Probes

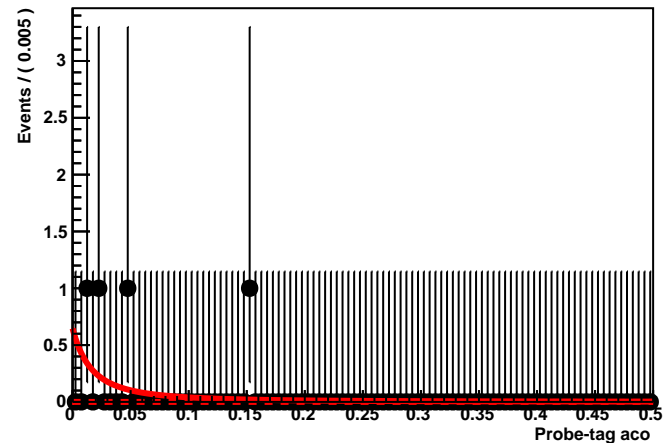

All Probes

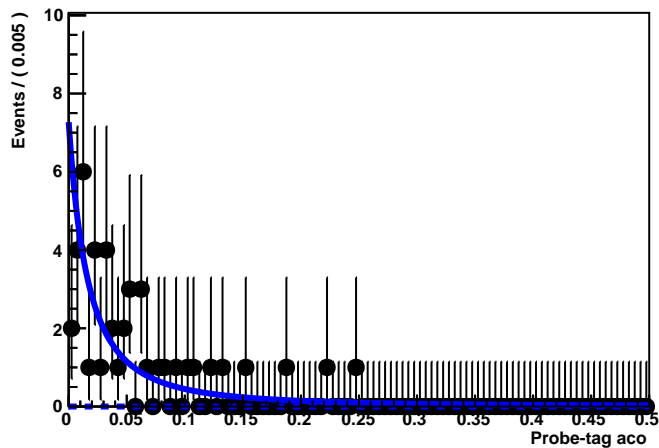

decayBkgF = -4.6
 decayBkgP = -4.6
 efficiency = 0.91 ± 0.04
 numBackgroundFail = 0 ± 3
 numBackgroundPass = 0 ± 2
 numSignalAll = 45 ± 7