

MapCHECK QA Analysis Report

Device Serial Number: 276477001

Reference Measurement Date: 06/04/25 21:49:43

Linearity Fit:

Slope:	0.9420
Intercept:	-0.2093

Dose Rate Fit:

Slope:	0.0035
Intercept:	91.8084

Field Size Dependence:

Fit Slope:	0.5788
Fit Intercept:	86.6136
Measured Values:	
5x5:	88.4305
10x10:	93.8377
25x25:	100.7246


Uniformity (Std Dev %): 0.44%

Leakage:


Central Value:	0.0000
Mean Value:	Invalid (NaN)

Report Generated: 2025-07-14 17:01:06


Linearity (Value vs. MU)

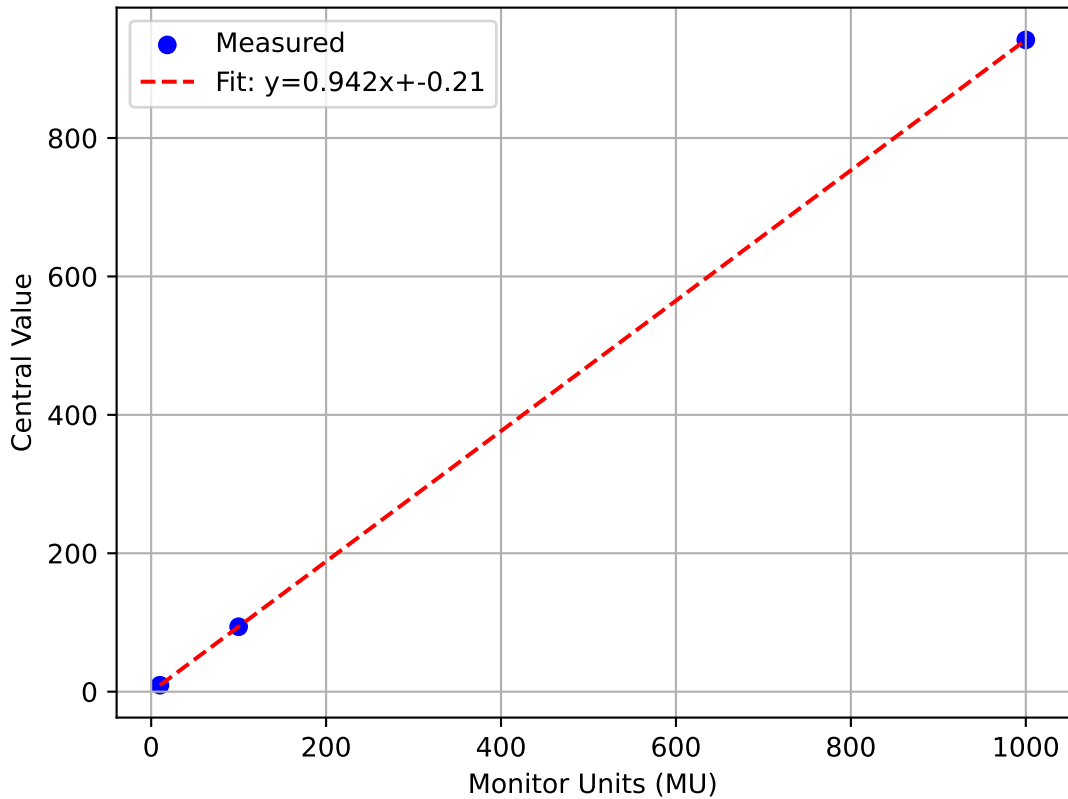

Dose Rate Dependence

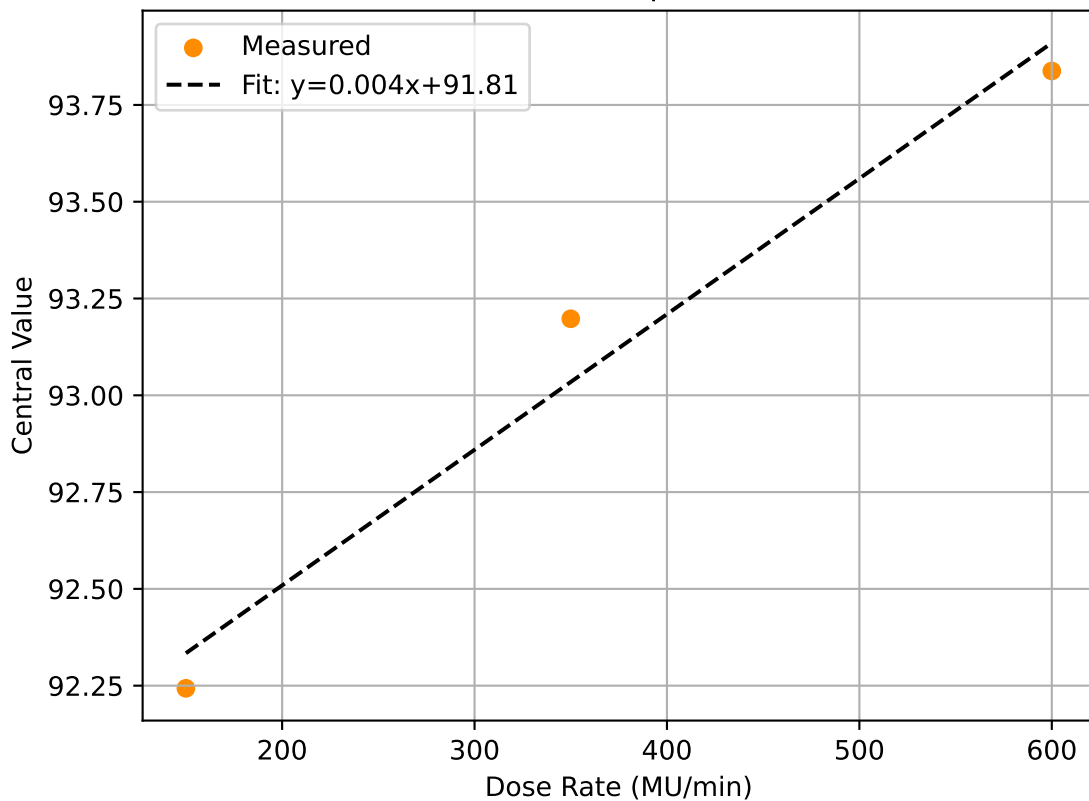

Field Size Dependence

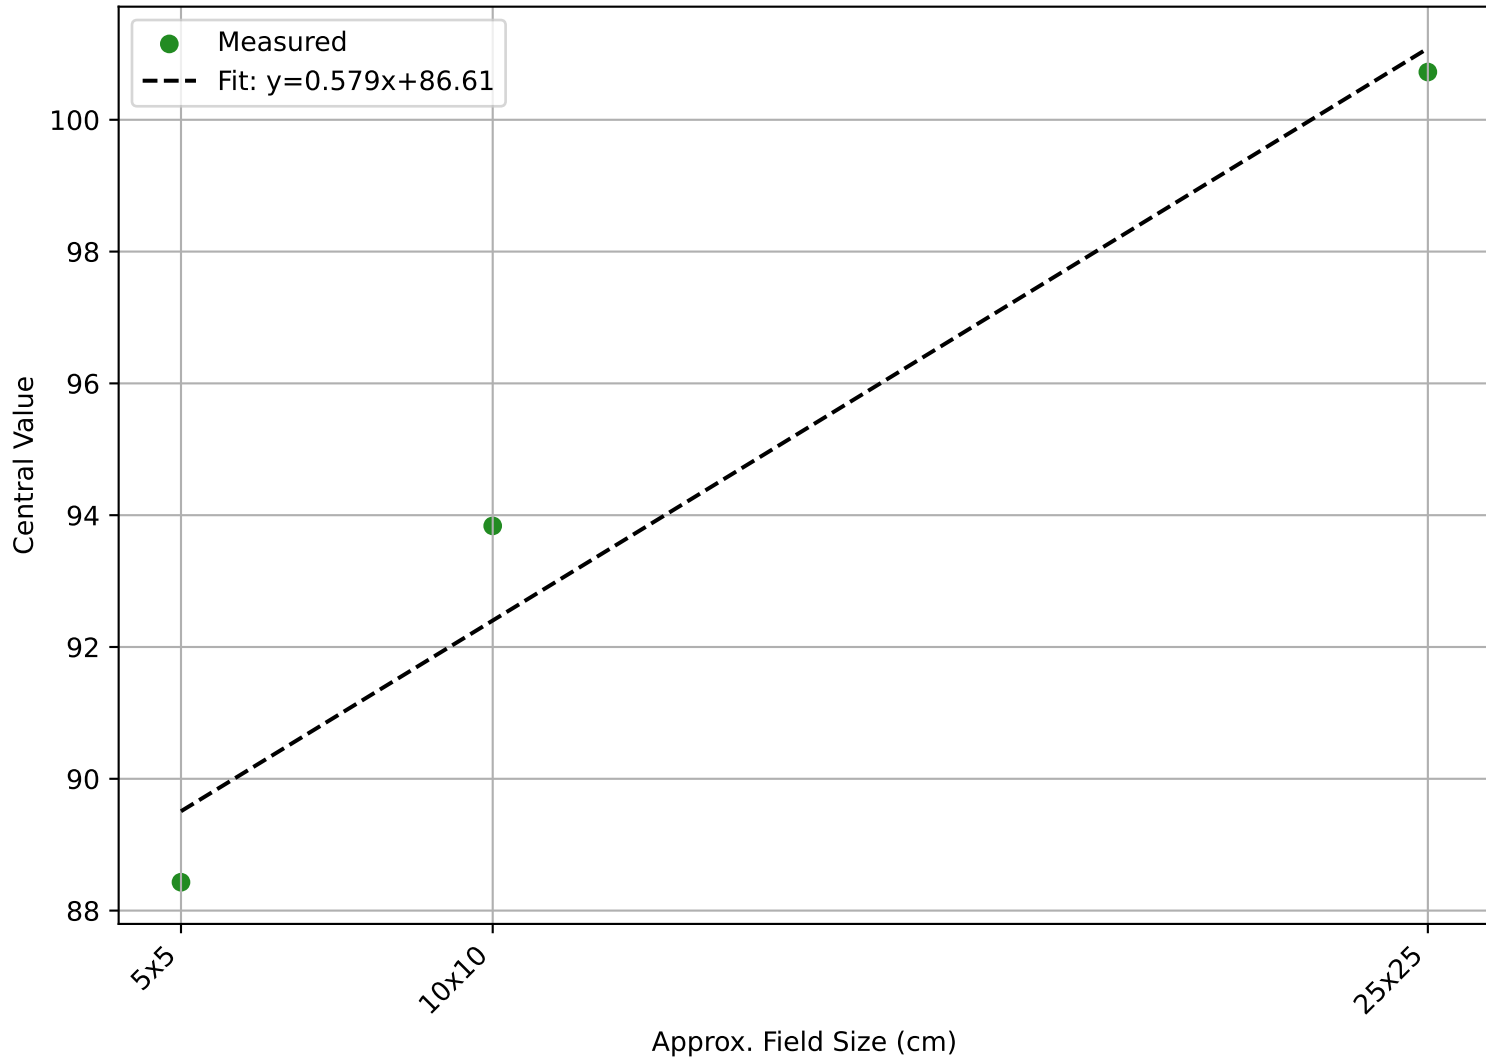

Uniformity Map (Std Dev = 0.44%)

