

# MapCHECK Analysis Report

Device Serial Number: N/A

Measurement Date: N/A N/A

## Linearity Fit:

Slope (value/MU):	0.942
Intercept (value):	-0.209

## Dose Rate Dependence Fit:

: Error: too many values to unpack (expected 2)

## Field Size Dependence:

Fit Slope (value/cm):	0.579
Fit Intercept (value):	86.614
Measured Values:	
5x5:	88.431
10x10:	93.838
25x25:	100.725


**Uniformity (Std Dev %):** 0.44%

## Leakage:


Central Value (Counts/Dose):	0.000
Mean Value (Counts/Dose):	Invalid (NaN)

Report Generated: 2025-07-14 12:33:59

Field Size Dependence

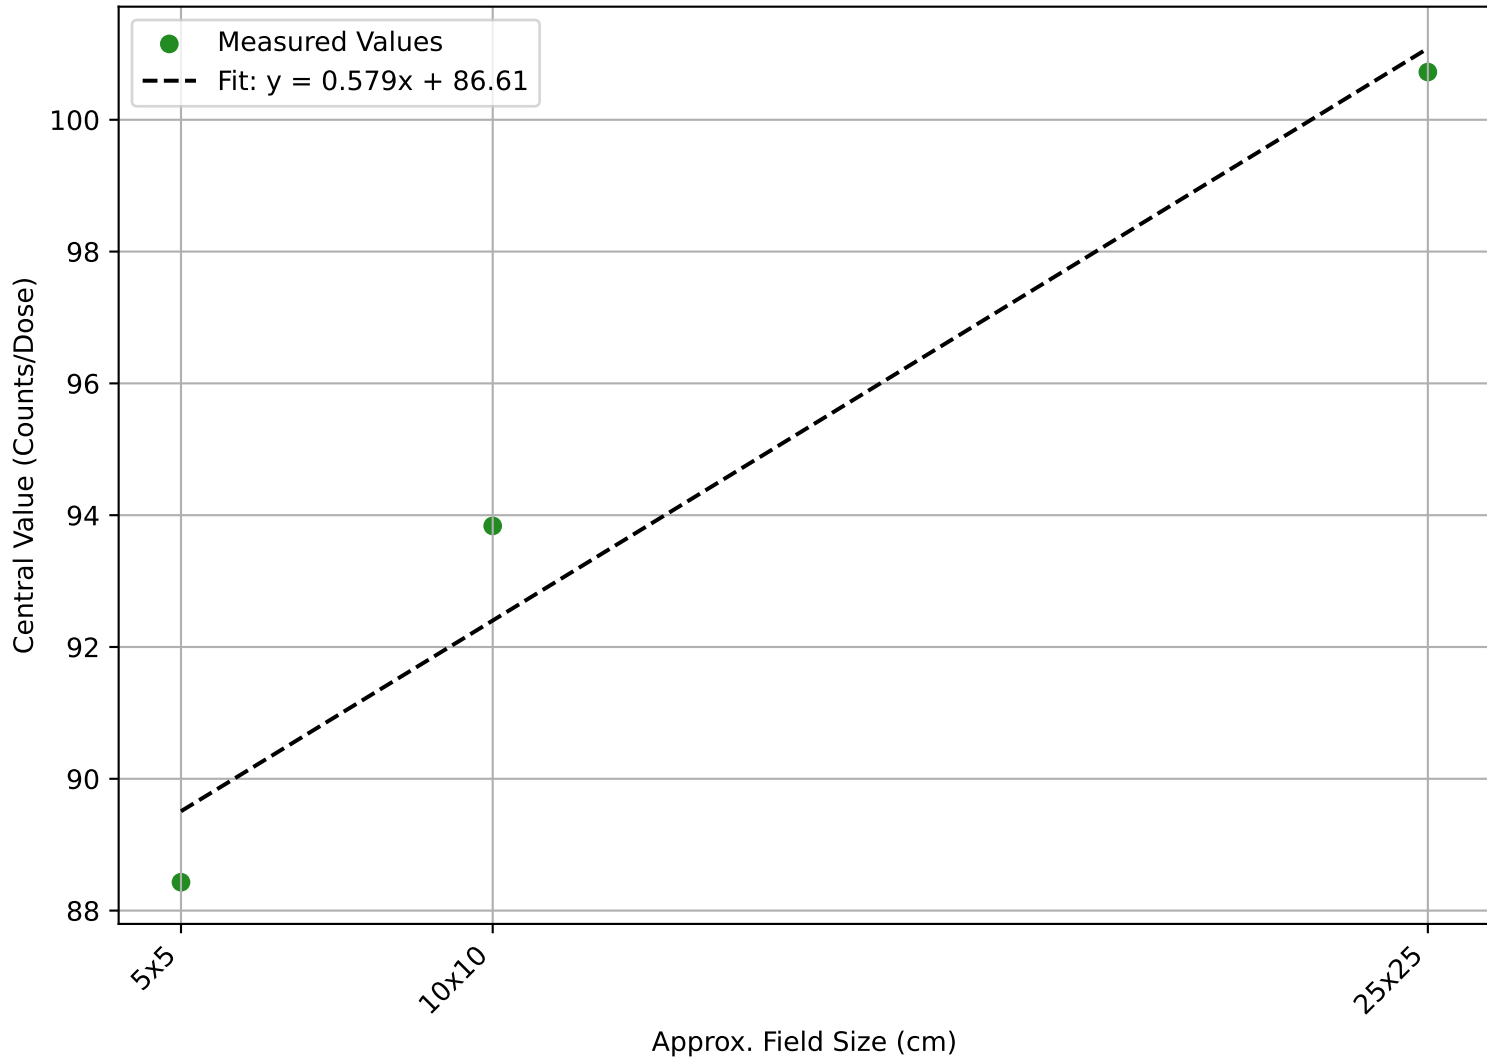

Linearity (Dose vs. MU)

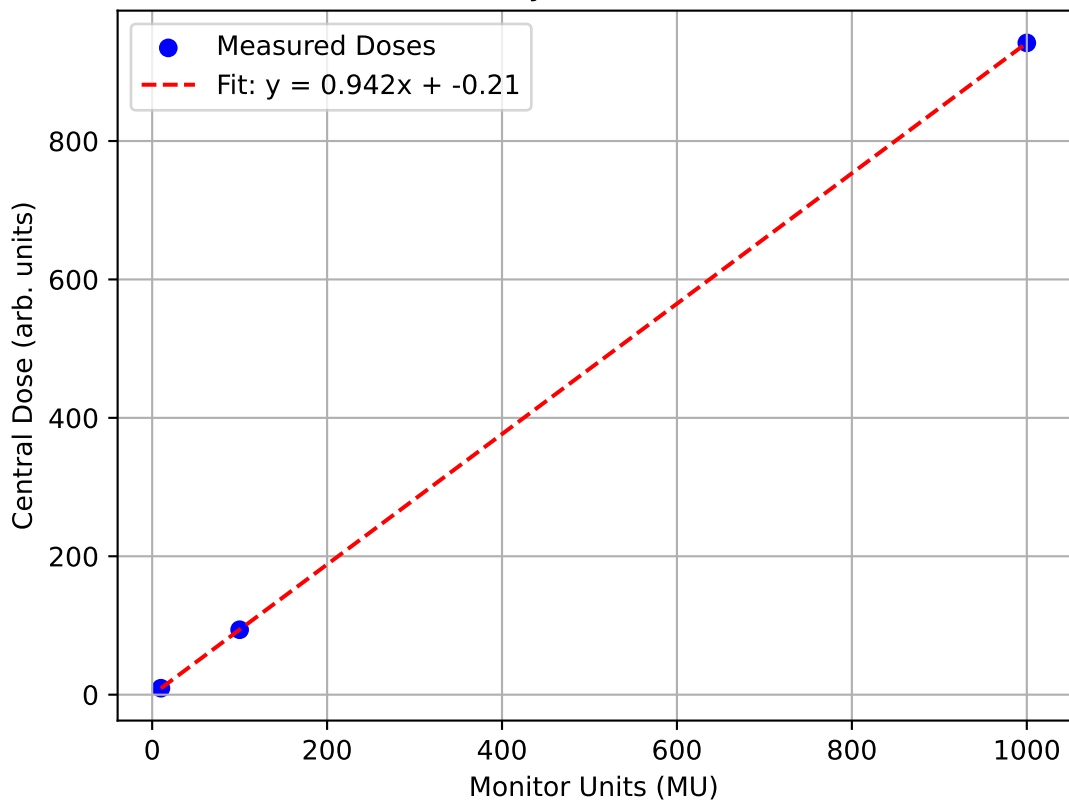

Uniformity Map (Std Dev = 0.44%)

