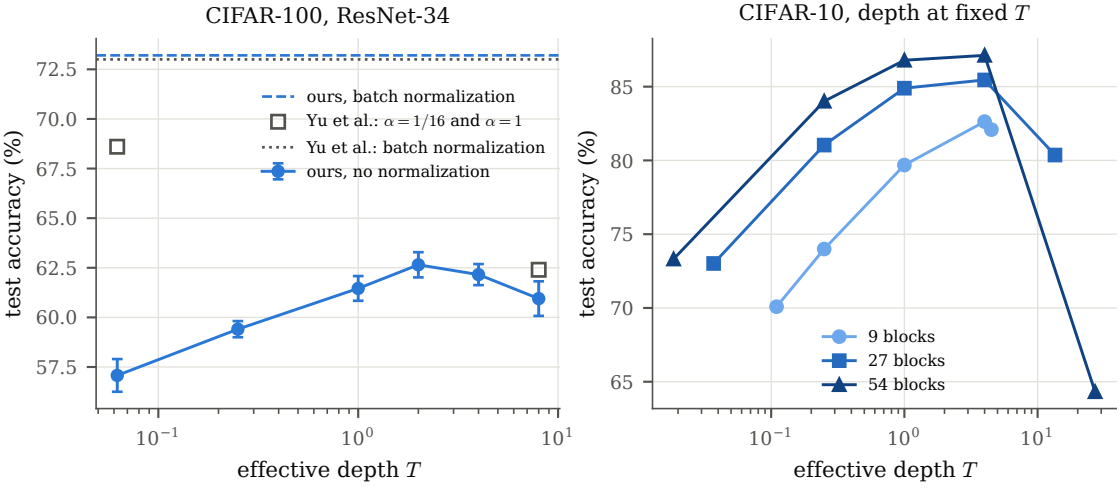
CIFAR-100, ResNet-34
test accuracy (%)
72.5
70.0
67.5
65.0
62.5
60.0
57.5
ours, batch normalization
Yu et al.: $\alpha = 1/16$ and $\alpha = 1$
Yu et al.: batch normalization
ours, no normalization
10^{-1}
10^{0}
10^{1}
effective depth T
CIFAR-10, depth at fixed T
test accuracy (%)
85
80
75
70
65
9 blocks
27 blocks
54 blocks
10^{-1}
10^{0}
10^{1}
effective depth T