

R&S®ZVH

Remote Control via LAN or USB Software Manual



1173.9005.12 – 12

ROHDE & SCHWARZ

Make ideas real



The Software Manual describes the following R&S®ZVH models and options

- R&S ZVH-K40 (1309.7013.02)

for the R&S®ZVH models:

- R&S ZVH4 (1309.6800.24)
- R&S ZVH8 (1309.6800.28)

The contents of this manual correspond to firmware version 2.00 or higher.

© 2022 Rohde & Schwarz GmbH & Co. KG

Muehldorfstr. 15, 81671 Munich. Germany

Phone: +49 89 4129-0

E-mail: info@rohde-schwarz.com

Internet: <http://www.rohde-schwarz.com>

81671 Munich, Germany

Subject to change – Data without tolerance limits is not binding.

R&S® is a registered trademark of Rohde & Schwarz GmbH & Co. KG.

Trade names are trademarks of the owners.

Throughout this manual, products from Rohde & Schwarz are indicated without the ® symbol , e.g. R&S®ZVH is indicated as R&S ZVH.

Table of Contents

Documentation Overview	6
Conventions Used in the Documentation	7
1 Introduction	8
2 Interfaces and Protocols	9
2.1 LAN Interface	11
2.2 USB Interface	11
2.3 Protocols	12
3 Setting Up the Remote Control Connection	14
3.1 Preparing for Remote Control	14
4 Instrument Model and Command Processing	15
4.1 Input Unit	15
4.2 Command Recognition	16
4.3 Data Base and Instrument Hardware	16
4.4 Status Reporting System	17
4.5 Output Unit	17
5 SCPI Command Structure and Syntax	18
5.1 Structure of a Command	19
5.1.1 Common Commands	19
5.1.2 Device-Specific Commands	20
5.1.2.1 Hierarchy	20
5.1.2.2 Multiple Keywords	20
5.1.2.3 Optional Keywords	21
5.1.2.4 Long and Short Form	21
5.1.2.5 Parameter	22
5.1.2.6 Special Characters	22
5.1.2.7 Numeric Suffix	23
5.1.3 Overview of Syntax Elements	24
5.2 Parameters	25
5.2.1 Numeric Values	25

5.2.2	Special Numeric Values.....	26
5.2.3	Boolean Parameters	26
5.2.4	Text	27
5.2.5	Strings.....	27
5.2.6	Block Data.....	27
5.3	Structure of a Program Message	28
5.4	Responses to Queries.....	29
6	Command Sequence and Command Synchronization.....	30
7	Remote Control – Commands	31
7.1	Common Commands.....	32
7.2	Remote Commands of the Cable and Antenna Analyzer	35
7.2.1	Configuring the Horizontal Axis	36
7.2.2	Configuring the Vertical Axis.....	41
7.2.3	Setting the Bandwidth	47
7.2.4	Performing and Triggering Measurements	48
7.2.4.1	Performing the Measurement	48
7.2.4.2	Triggering Measurements	48
7.2.5	Working with Traces	50
7.2.6	Using Markers.....	55
7.2.7	Using Limit Lines.....	64
7.2.8	Configuring and Using Measurement Functions	65
7.2.8.1	Selecting the Measurement Port	65
7.2.8.2	Selecting the Cable Characteristics.....	66
7.2.8.3	Selecting the Measurement Mode	66
7.2.8.4	Selecting the Measurement Format.....	67
7.2.8.5	Reading Out Measurement Results.....	68
7.2.8.6	Calibrating the Measurement.....	69
7.2.8.7	Working with a DTF List.....	73
7.3	Remote Commands of the Spectrum Analyzer	75
7.3.1	Configuring the Horizontal Axis	76
7.3.2	Configuring the Vertical Axis.....	81
7.3.3	Setting the Bandwidths	87
7.3.4	Performing and Triggering Measurements	89

7.3.4.1	Performing the Measurement	89
7.3.4.2	Capturing I/Q Data	92
7.3.4.3	Triggering Measurements	94
7.3.5	Working with Traces	97
7.3.6	Using Markers	102
7.3.6.1	Markers and Delta Markers	102
7.3.6.2	Marker Functions	102
7.3.7	Using Display Lines and Limit Lines	110
7.3.7.1	Display Lines	110
7.3.7.2	Limit Lines	111
7.3.8	Configuring and Using Measurement Functions	116
7.3.8.1	Working with Channel Tables	116
7.3.8.2	Power Measurements	119
7.3.8.3	Measuring the Channel Power	122
7.3.8.4	Measuring the Occupied Bandwidth	124
7.3.8.5	TDMA Measurements	125
7.3.8.6	Measuring the Adjacent Channel Leakage Ratio	126
7.3.8.7	Measuring the Harmonic Distortion	138
7.3.8.8	Measuring the AM Modulation Depth	140
7.3.8.9	Measuring the Spectrum Emission Mask	141
7.3.8.10	Measuring Spurious Emissions	143
7.3.8.11	Using an Isotropic Antenna	144
7.4	Remote Commands of the Network Analyzer Mode	146
7.4.1	Configuring the Horizontal Axis	146
7.4.2	Configuring the Vertical Axis	147
7.4.3	Setting the Bandwidths	152
7.4.4	Performing and Triggering the Measurement	152
7.4.5	Working with Traces	153
7.4.6	Using Markers and Deltamarkers	155
7.4.6.1	Markers and Deltamarkers	155
7.4.6.2	Marker Functions	157
7.4.7	Configuring the Measurement	159
7.4.7.1	Selecting the Measurement Port	159

7.4.7.2	Selecting the Measurement Mode	160
7.4.7.3	Calibrating the Measurement.....	160
7.4.7.4	Selecting the Result Display	162
7.4.7.5	Selecting the Measurement Format.....	162
7.4.7.6	Configuring the Vector Voltmeter (option R&S ZVH-K45).....	165
7.5	Remote Commands of the Power Meter.....	168
7.5.1	Using Power Sensors	168
7.5.1.1	Setting the Frequency.....	168
7.5.1.2	Configuring Power Level Readout.....	169
7.5.1.3	Defining the Measurement Time.....	171
7.5.1.4	Zeroing of the Power Sensor	171
7.5.1.5	Forward Power Display.....	172
7.5.1.6	Defining the Video Bandwidth.....	172
7.5.1.7	Reading Out Measurement Results.....	173
7.5.1.8	Selecting a Telecommunication Standard	174
7.6	File Management.....	175
7.7	Making and Storing Screenshots.....	183
7.8	Configuring Data Capture	185
7.9	Saving Events	187
7.10	Configuring the Instrument	190
7.10.1	Mode Selection	190
7.10.2	Controlling the GPS Receiver.....	192
7.10.3	Display Configuration.....	197
7.10.4	Audio Settings.....	199
7.10.5	Setting up a Network Connection	201
7.10.6	System Settings.....	203
7.11	Status Reporting System	214
7.11.1	Structure of an SCPI Status Register	214
7.11.1.1	CONDition part.....	214
7.11.1.2	PTRansition part	215
7.11.1.3	NTRansition part.....	215
7.11.1.4	EVENTt part	215
7.11.1.5	ENABle part	215

7.11.1.6	Sum bit.....	216
7.11.2	Overview of the Status Register	216
7.11.3	Status Byte (STB) & Service Request Enable Register (SRE)	217
7.11.4	Event Status Register (ESR) and Event Status Enable Register (ESE)	218
7.11.4.1	STATus:OPERation Register	219
7.11.4.2	STATus:QUEStionable Register.....	219
7.11.4.3	STATus:QUEStionable:FREQuency Register.....	220
7.11.4.4	STATus:QUEStionable:LIMit Register.....	220
7.11.4.5	STATus:QUEStionable:POWer Register.....	220
7.11.5	Application of the Status Reporting Systems	221
7.11.5.1	Service Request.....	221
7.11.5.2	Serial Poll.....	221
7.11.5.3	Query by Means of Commands	222
7.11.5.4	Error Queue Query	222
7.11.6	Reset Values of the Status Reporting System	223
7.11.7	Remote Commands of the Status Reporting System.....	224
	Alphabetical List of Remote Commands	229
	Index	237

Documentation Overview

The user documentation for the R&S ZVH is divided as follows:

Quick Start Guide

The Quick Start Guide provides basic information on the instrument's functions.

It covers the following topics:

- overview of all elements of the front and rear panels
- basic information on how to set up the R&S ZVH
- information on how to operate the R&S ZVH in a network
- instructions on how to perform measurements

Operating Manual

The Operating Manual provides a detailed description on the instrument's functions

It covers the following topics:

- instructions on how to set up and operate the R&S ZVH in its various operating modes
- instructions on how to perform measurements with the R&S ZVH
- instructions on how to work with the available software options and applications

Service Manual

The Service Manual provides information on maintenance.

It covers the following topics:

- instructions on how to perform a performance test
- instructions on how to repair the R&S ZVH including a spare parts list
- mechanical drawings

Release Notes

The release notes describe the installation of the firmware, new and modified functions, eliminated problems, and last minute changes to the documentation. The corresponding firmware version is indicated on the title page of the release notes. The current release notes are provided on the internet.

Internet Site

The internet site at: <https://www.rohde-schwarz.com/product/zvh.html> provides the most up to date information on the R&S ZVH. The most recent manuals are available as printable PDF files in the download area.

Also provided for download are firmware updates including the corresponding release notes, instrument drivers, current data sheets, application notes and image versions.

Conventions Used in the Documentation

The following conventions are used throughout the R&S R&S ZVH Software Manual:

Typographical conventions

Convention	Description
"Graphical user interface elements"	All names of graphical user interface elements both on the screen and on the front and rear panels, such as dialog boxes, softkeys, menus, options, buttons etc., are enclosed by quotation marks.
"KEYS"	Key names are written in capital letters and enclosed by quotation marks.
<i>Input</i>	Input to be entered by the user is displayed in italics.
File names, commands, program code	File names, commands, coding samples and screen output are distinguished by their font.
"Links"	Links that you can click are displayed in blue font.
"References"	References to other parts of the documentation are enclosed by quotation marks.

Other conventions

- **Remote commands:** Remote commands may include abbreviations to simplify input. In the description of such commands, all parts that have to be entered are written in capital letters. Additional text in lower-case characters is for information only.

1 Introduction

With the software application R&S ZVH-K40 installed on the instrument, it is possible to operate your R&S ZVH via remote control. In this manual you will find all information necessary to remotely control the R&S ZVH.

Enabling the Option

The Remote Control Option R&S ZVH-K40 is enabled by entering a key code. The key code is based on the unique serial number of the instrument. To retrofit an option, enable it with a key code.

- ▶ Press the SETUP key.
- ▶ Press the "Installed Options" softkey
- ▶ Select "Install Option..." under the "Option Administration" header.
- ▶ Confirm with ENTER.

An entry box in the lower right corner of the screen is displayed.

- ▶ Type in the the appropriate option key.
- ▶ Confirm with ENTER.

If the correct key code is entered, the R&S ZVH displays

Installation successful !

If an invalid key code is entered, the R&S ZVH displays

Invalid key code!

2 Interfaces and Protocols

The R&S ZVH supports two different interfaces for remote control.

- **LAN Interface:** The protocol is based on TCP/IP and supports the VXI-11 standard.
- **USB Interface**

The connectors are located at the side of the instrument and permit a connection to a controller for remote control via a local area network (LAN) or directly via USB.

SCPI


SCPI (Standard Commands for Programmable Instruments) commands - messages - are used for remote control. Commands that are not taken from the SCPI standard follow the SCPI syntax rules. The instrument supports the SCPI version 1999. The SCPI standard is based on standard IEEE 488.2 and aims at the standardization of device-specific commands, error handling and the status registers. The tutorial "Automatic Measurement Control - A tutorial on SCPI and IEEE 488.2" from John M. Pieper (R&S order number 0002.3536.00) offers detailed information on concepts and definitions of SCPI.

The requirements that the SCPI standard places on command syntax, error handling and configuration of the status registers are explained in detail in the following sections. Tables provide a fast overview of the bit assignment in the status registers. The tables are supplemented by a comprehensive description of the status registers.

VISA

VISA is a standardized software interface library providing input and output functions to communicate with instruments. The I/O channel (LAN or USB) is selected at initialization time by means of a channel-specific resource string. For more information about VISA refer to its user documentation.

The programming examples for remote control are all written in Microsoft® VISUAL BASIC®. Access to the VISA functions require the declaration of the functions and constants prior to their use in the project. This can be accomplished either by adding the modules VISA32.BAS and VPPTYPE.BAS or a reference to the VISA32.DLL to the project.

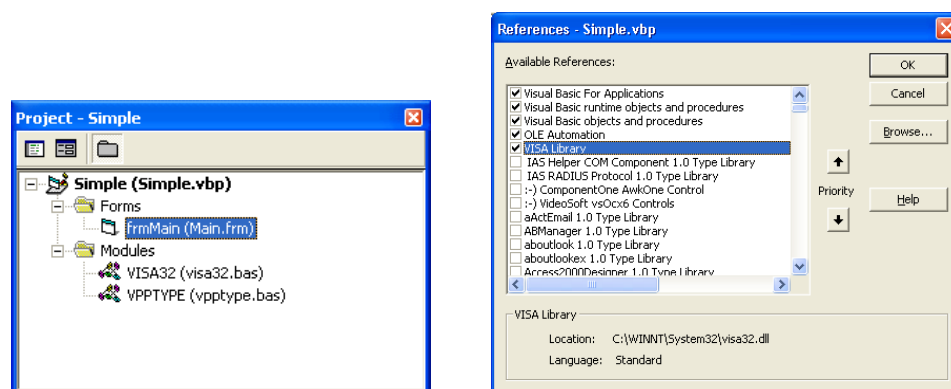

The modules visa32.bas and vpptype.bas can be found in the following location:

<VXIbnpPath>\WinNT\include (typically C:\VXIbnp\WinNT\include).

Resetting the R&S ZVH



Manual operation is designed for maximum possible operating convenience. In contrast, the priority of remote control is the "predictability" of the device status. Therefore, control programs should always define an initial device status (e.g. with the command *RST) and then implement the required settings.

2.1 LAN Interface

To be integrated in a LAN, the instrument is equipped with a standard LAN interface, consisting of a connector, a network interface and protocols (VXI-11).

Instrument access via VXI-11 is usually achieved from high level programming platforms by using VISA as an intermediate abstraction layer. VISA encapsulates the low level VXI-11 (LAN) or USB function calls and thus makes the transport interface transparent for the user. The necessary VISA library is available as a separate product. For details contact your local R&S sales representative.

2.2 USB Interface

For remote control via the USB connection, the PC and the instrument must be connected via the USB interface. The required driver comes with the R&S InstrumentView software package and is automatically installed on the PC with the software package.

The driver addresses the instrument via the USB interface with the fix IP address 172.16.10.10.

In addition, a remote control connection via the SCPI interface requires the VISA library to be installed on the PC.

2.3 Protocols

VXI-11 Basics

The VXI-11 standard is based on the ONC-RPC protocol which in turn relies on TCP/IP as the network/transport layer. The TCP/IP network protocol and the associated network services are preconfigured. TCP/IP ensures connection-oriented communication, where the order of the exchanged messages is adhered to and interrupted links are identified. With this protocol, messages cannot be lost.

Remote control of an instrument via a network is based on standardized protocols which follow the OSI reference model (see Fig. below).

Application	SCPI
Presentation	XDR (VXI-11)
Session	ONC-RPC
Transport	TCP / UDP
Network	IP
Data Link	Ethernet/802.3
Physical	802.3/10BASE-T

Figure 2-1: Example for LAN remote control based on the OSI reference model

Based on TCP/UDP, messages between the controller and the instrument are exchanged via open network computing (ONC) - remote procedure calls (RPC). With XDR (VXI-11), legal RPC messages are known as VXI-11 standard. Based on this standard, messages are exchanged between the controller and the instrument. The messages are identical with SCPI commands. They can be organized in four groups:

- program messages (control command to the instrument)
- response messages (values returned by the instrument)
- service request (spontaneous queries of the instrument)
- low-level control messages (interface messages).

A VXI-11 link between a controller and an instrument uses three channels: core, abort and interrupt channel. Instrument control is mainly performed on the core channel (program, response and low-level control messages). The abort channel is used for immediate abort of the core channel; the interrupt channel transmits spontaneous service requests of the instrument. Link setup itself is very complex. For more details refer to the VXI-11 specification.

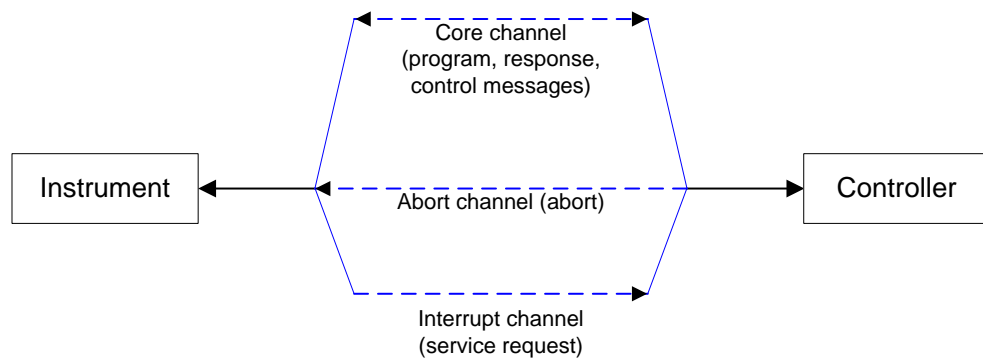


Figure 2-2: VXI-11 channels between instrument and controller

The number of controllers that can address an instrument is practically unlimited in the network. In the instrument, the individual controllers are clearly distinguished. This distinction continues up to the application level in the controller, i.e. two applications on a computer are identified by the instrument as two different controllers.

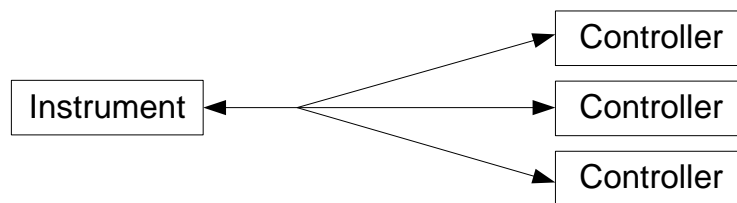


Figure 2-3: Remote control via LAN from several controllers

The controllers can lock and unlock the instrument for exclusive access. This regulates access to the instrument of several controllers.

3 Setting Up the Remote Control Connection

3.1 Preparing for Remote Control

The short and simple operating sequence below shows how to put the instrument into operation and quickly set its basic functions. The current IP address for LAN operation is shown in the SETUP – Instrument Setup Menu. In case of USB connection the IP address is fixed to 172.16.10.10.

Refer to the Quick Start Guide for instructions on how to change the IP address.

- ▶ Connect the instrument to the LAN or directly to the controller via USB.
- ▶ Switch on the instruments.
- ▶ Write and start the following program on the controller:

```
status = viOpenDefaultRM(defaultRM)
    'open default resource manager
status = viOpen(DefaultRM, "TCPIP::172.16.10.10", 0, 0, vi)
    'in case of USB connection
status = viOpen(DefaultRM, "TCPIP::xxx.xxx.xxx.xxx", 0, 0, vi)
    'in case of a LAN connection, with xxx.xxx.xxx.xxx = IP address
cmd = "*RST;*CLS"
status = viWrite(vi, Cmd, Len(Cmd), retCount)
    'reset instrument and clear status registers
cmd = "FREQ:CEN 100MHz"
status = viWrite(vi, Cmd, Len(Cmd), retCount)
    'set center frequency to 100 MHz
cmd = "FREQ:SPAN 10MHz"
status = viWrite(vi, Cmd, Len(Cmd), retCount)
    'set span to 10 MHz
cmd = "DISP:TRAC:Y:RLEV -10dBm"
status = viWrite(vi, Cmd, Len(Cmd), retCount)
    'set reference level to -10 dBm
viclose vi
viclose default RM
```

The instrument now performs a sweep in the frequency range of 95 MHz to 105 MHz.

Changing the IP Address

In order to operate the instrument via remote control, it must be accessed via LAN (IP address) or USB (fixed IP address). If the factory-set remote control address does not fit in the network environment, it can be changed. Refer to the Quick Start Guide, chapter "Setting up a LAN or USB Connection to a PC", for instructions on how to change the IP address.

4 Instrument Model and Command Processing

The block diagram in Fig. 1-2 shows how SCPI commands are serviced in the instrument. The individual components work independently and simultaneously. They communicate with each other by means of so-called "messages".

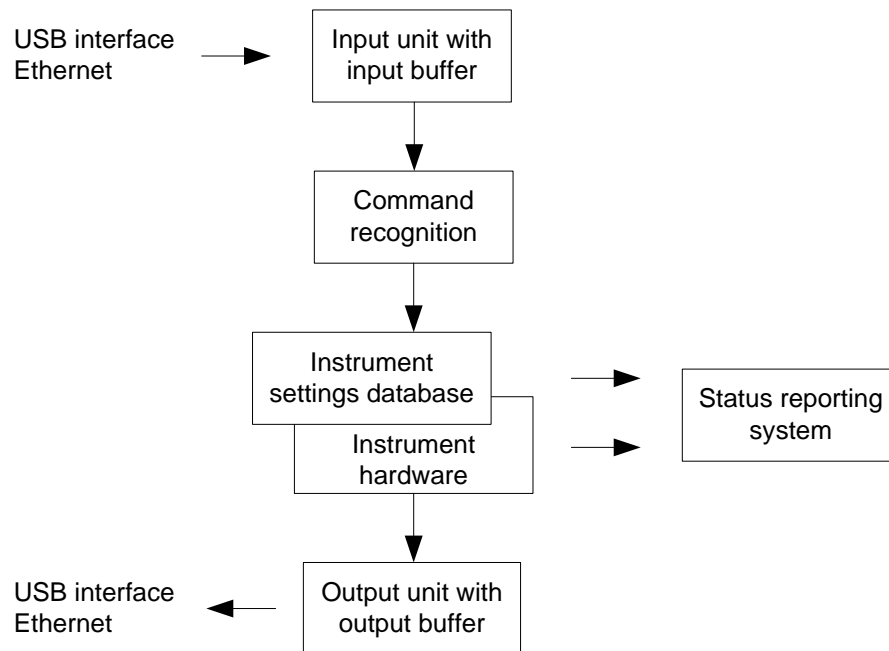


Figure 4-1: Instrument model in the case of remote control

4.1 Input Unit

The input unit receives commands character by character from the controller and collects them in the input buffer. The input unit sends a message to the command recognition as soon as the input buffer is full or as soon as it receives a delimiter, <PROGRAM MESSAGE TERMINATOR>, as defined in IEEE 488.2, or the interface message DCL.

If the input buffer is full, the traffic is stopped and the data received up to then are processed. Subsequently the traffic is continued. If, however, the buffer is not yet full when receiving the delimiter, the input unit can already receive the next command during command recognition and execution. The receipt of DCL clears the input buffer and immediately resets the command recognition.

4.2 Command Recognition

The command recognition analyses the data received from the input unit. It proceeds in the order in which it receives the data. Only DCL is serviced with priority, for example GET (Group Execute Trigger) is only executed after the commands received before. Each recognized command is immediately transferred to the internal instrument settings data base but not executed immediately.

The command recognition detects syntax errors in the commands and transfers them to the status reporting system. The rest of a program message after a syntax error is analyzed further if possible and serviced. After the syntax test, the value range of the parameter is checked, if required.

If the command recognition detects a delimiter, it passes the command to an execution unit that performs the instrument settings. In the meantime, the command recognition is ready to process new commands (overlapping execution). A DCL command is processed in the same way.

4.3 Data Base and Instrument Hardware

Here the expression "instrument hardware" denotes the part of the instrument fulfilling the actual instrument function - signal generation, measurement etc. The controller is not included. The term "data base" denotes a database that manages all the parameters and associated settings required for setting the instrument hardware.

Setting commands lead to an alteration in the data set. The data set management enters the new values (e.g. frequency) into the data set, however, only passes them on to the hardware when requested by the command recognition. This only takes place at the end of a program message.

The data are checked for compatibility with the current instrument settings before they are transmitted to the instrument hardware. If the execution is not possible, an "execution error" is signaled to the status reporting system. The corresponding settings are discarded.

Before passing on the data to the hardware, the settling bit in the STATus:OPERation register is set (refer to section "STATus:OPERation Register"). The hardware executes the settings and resets the bit again as soon as the new state has settled. This fact can be used to synchronize command servicing.

Queries induce the data set management to send the desired data to the output unit.

4.4 Status Reporting System

For detailed information refer to section "[Status Reporting System](#)".

4.5 Output Unit

The output unit collects the information requested by the controller, which it receives from the data base management. It processes it according to the SCPI rules and makes it available in the output buffer.

If the instrument is addressed as a talker without the output buffer containing data or awaiting data from the data base management, the output unit sends error message "Query UNTERMINATED" to the status reporting system. No data are sent to the controller, the controller waits until it has reached its time limit. This behavior is defined by IEEE 488.2 and SCPI.

5 SCPI Command Structure and Syntax

SCPI (Standard Commands for Programmable Instruments) describes a standard command set for programming instruments, irrespective of the type of instrument or manufacturer. The goal of the SCPI consortium is to standardize the device-specific commands to a large extent. For this purpose, a model was developed which defines the same functions inside a device or for different devices. Command systems were generated which are assigned to these functions. Thus it is possible to address the same functions with identical commands. The command systems are of a hierarchical structure.

SCPI is based on standard IEEE 488.2, i.e. it uses the same syntactic basic elements as well as the common commands defined in this standard. Part of the syntax of the device responses is defined with greater restrictions than in standard IEEE 488.2 (see section "Responses to Queries").



Remote command examples

Not all commands used in the following examples are implemented in the instrument.

5.1 Structure of a Command

The commands consist of a so-called header and, in most cases, one or more parameters. Header and parameter are separated by a "white space" (ASCII code 0 to 9, 11 to 32 decimal, e.g. blank). The headers may consist of several key words. Queries are formed by directly appending a question mark to the header.

5.1.1 Common Commands

Common commands consist of a header preceded by an asterisk "*" and one or several parameters, if any.

Examples

*RST	RESET, resets the device
*ESE 253	EVENT STATUS ENABLE, sets the bits of the event status enable register
*ESR?	EVENT STATUS QUERY, queries the contents of the event status register.

5.1.2 Device-Specific Commands

5.1.2.1 Hierarchy

Device-specific commands are of hierarchical structure. The different levels are represented by combined headers. Headers of the highest level (root level) have only one key word. This key word denotes a complete command system.

Example

`SENSe`

This key word denotes the SENSE command system.

For commands of lower levels, the complete path has to be specified, starting on the left with the highest level, the individual key words being separated by a colon ":".

Example

`SENSe:FREQuency:SPAN 10MHZ`

This command lies in the third level of the SENSE system. It sets the frequency span.

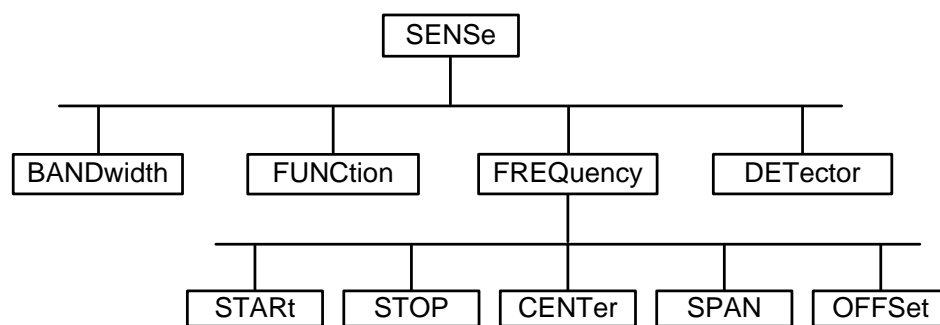


Figure 5-1: Tree structure the SCPI command systems using the SENSE system as example

5.1.2.2 Multiple Keywords

Some key words occur in several levels within one command system. Their effect depends on the structure of the command, i.e. at which position in the header of a command they are inserted.

Examples

`SOURce:FM:POLarity NORMal`

This command contains key word POLarity in the third command level. It defines the polarity between modulator and modulation signal.

`SOURce:FM:EXTernal:POLarity NORMal`

This command contains key word POLarity in the fourth command level. It defines the polarity between modulation voltage and the resulting direction of the modulation only for the external signal source indicated.

5.1.2.3 Optional Keywords

Some command systems permit certain key words to be inserted into the header or omitted. These key words are marked by square brackets in the description. The full command length must be recognized by the instrument for reasons of compatibility with the SCPI standard. Some commands are considerably shortened by these optional key words.

Example

```
[SENSe]:BANDwidth[:RESolution]:AUTO
```

This command couples the resolution bandwidth of the instrument to other parameters. The following command has the same effect:

```
BANDwidth:AUTO
```



Optional keywords with numeric suffixes

Do not omit an optional keyword if it includes a numeric suffix that is relevant for the effect of the command.

Example

```
DISPlay[:WINDow<1...4>]:MAXimize <Boolean>
```

Command `DISP:MAX ON` refers to window 1.

In order to refer to a window other than 1, you must include the optional `WINDow` parameter with the suffix for the required window.

`DISP:WIND2:MAX ON` refers to window 2.

5.1.2.4 Long and Short Form

The key words feature a long form and a short form. Either the short form or the long form can be entered, other abbreviations are not permitted.

Example

```
STATus:QUEStionable:ENABle 1
```

is equivalent to

```
STAT:QUES:ENAB 1
```



Upper and lower case notation of commands

Upper-case and lower-case notation only serves to distinguish the two forms in the manual, the instrument itself does not distinguish upper-case and lower-case letters.

5.1.2.5 Parameter

The parameter must be separated from the header by a "white space". If several parameters are specified in a command, they are separated by a comma ",". A few queries permit the parameters MINimum, MAXimum and DEFault to be entered. Refer to "[Parameters](#)" for a detailed description of the various parameters.

Example

```
SENSe:FREQuency:STOP? MAXimum
```

```
Response: 3.5E9
```

This query requests the maximal value for the stop frequency.

5.1.2.6 Special Characters

- | A vertical stroke in parameter definitions indicates alternative possibilities in the sense of "or". The effect of the command differs, depending on which parameter is used.

Example

```
DISPlay:FORMat SINGLE | SPLit
```

If parameter SINGLE is selected, full screen is displayed, in the case of SPLit, split screen is displayed.

A selection of key words with an identical effect exists for several commands. These keywords are indicated in the same line; they are separated by a vertical stroke. Only one of these keywords needs to be included in the header of the command. The effect of the command is independent of which of the keywords is used.

Example

```
SENSe:BANDwidth|BWIDth[:RESolution]
```

The two following commands with identical meaning can be created. They set the frequency of the fixed frequency signal to 1 kHz:

```
SENSe:BAND 1
```

```
SENSe:BWID 1
```

- [] Key words in square brackets can be omitted when composing the header. The full command length must be accepted by the instrument for reasons of compatibility with the SCPI standards.

Example

```
[SENSe:]BANDwidth|BWIDth[:RESolution]
```

```
SENS:BAND:RES
```

is equivalent to

```
BAND
```

Parameters in square brackets can be incorporated optionally in the command or omitted as well.

Example

```
MMEMory:NETWork:MAP
<string>,<string>[,string>,<string>,<boolean>]
```

Entries in square brackets are optional or can be omitted.

{ } Parameters in curly brackets are optional and can be inserted once or several times, or omitted.

Example

```
SENSe:LIST:FREQuency <numeric_value>{,<numeric_value>}
```

The following are valid commands:

```
SENS:LIST:FREQ 10
SENS:LIST:FREQ 10,20
SENS:LIST:FREQ 10,20,30,40
```

5.1.2.7 Numeric Suffix

If a device features several functions or features of the same kind, e.g. inputs, the desired function can be selected by a suffix added to the command. Entries without suffix are interpreted like entries with the suffix 1. Optional keywords must be specified if they select a function with the suffix.

Example

```
SYSTem:COMMunicate:SERial2:BAUD 9600
```

This command sets the baud rate of a second serial interface.

Suffix counting

In case of remote control, suffix counting may differ from the numbers of the corresponding selection used in manual operation. SCPI prescribes that suffix counting starts with 1. Suffix 1 is the default state and used when no specific suffix is specified.

Some standards define a fixed numbering, starting with 0. With GSM, for instance, slots are counted from 0 to 7. In the case of remote control, the slots are selected with the suffixes 1 to 8. If the numbering differs in manual operation and remote control, it is indicated with the respective command.

5.1.3 Overview of Syntax Elements

The following table offers an overview of the syntax elements.

- : The colon separates the key words of a command. In a program message the separating semicolon marks the uppermost command level.
- ; The semicolon separates two commands within a program message. It does not alter the path.
- , The comma separates several parameters of a command.
- ? The question mark forms a query.
- * The asterisk marks a common command.
- " Quotation marks introduce a string and terminate it.
- # The hash symbol # introduces binary, octal, hexadecimal and block data.
 - Binary: #B10110
 - Octal: #O7612
 - Hexa: #HF3A7
 - Block: #21312

A "white space" (ASCII-Code 0 to 9, 11 to 32 decimal, e.g. blank) separates header and parameter.

5.2 Parameters

For most commands a parameter needs to be supplemented. The parameter has to be separated from the header by a "white space". Possible parameters are:

- Numeric values
- Special numeric values
- Boolean parameters
- Text
- Character strings
- Block data.

The type of parameter required for each command and the allowed range of values are specified in the command description.

5.2.1 Numeric Values

Numeric values can be entered in any form, i.e. with sign, decimal point and exponent. Values exceeding the resolution of the instrument are rounded up or down. The mantissa may comprise up to 255 characters, the exponent must lie inside the value range -32000 to 32000. The exponent is introduced by an "E" or "e". Entry of the exponent alone is not permissible. In the case of physical quantities, the unit can be entered. Permissible unit prefixes are G (giga), MA (mega), MOHM and MHZ are also possible), K (kilo), M (milli), U (micro) and N (nano). If the unit is missing, the basic unit is used.

Example

```
SENSe:FREQuency:STOP 1.5GHz = SENSe:FREQuency:STOP 1.5E9
```

5.2.2 Special Numeric Values

The texts MINimum, MAXimum, DEFault, UP and DOWN are interpreted as special numeric values. In case of a query, the numeric value is returned.

- MIN/MAX

MINimum and MAXimum denote the minimum and maximum value.

- DEF

DEFault denotes a preset value which has been stored in the EPROM. This value conforms to the default setting, as it is called by the *RST command

- UP/DOWN

UP, DOWN increases or reduces the numerical value by one step. The step width can be specified via an allocated step command for each parameter which can be set via UP, DOWN.

- INF/NINF

INFinity, Negative INFinity (NINF) Negative INFinity (NINF) represent the numerical values -9.9E37 or 9.9E37, respectively. INF and NINF are only sent as device responses.

- NAN

Not A Number (NAN) represents the value 9.91E37. NAN is only sent as device response. This value is not defined. Possible causes are the division of zero by zero, the subtraction of infinite from infinite and the representation of missing values.

Example:

Setting command: `SENSe:FREQuency:STOP MAXimum`

Query: `SENSe:FREQuency:STOP?`, Response: `3.5E9`

5.2.3 Boolean Parameters

Boolean parameters represent two states. The ON state (logically true) is represented by ON or a numerical value unequal to 0. The OFF state (logically untrue) is represented by OFF or the numerical value 0. The numerical values are provided as response for query.

Example

Setting command: `CALCulate:MARKer:STATe ON`

Query: `CALCulate:MARKer:STATe?`, Response: `1`

5.2.4 Text

Text parameters observe the syntactic rules for key words, i.e. they can be entered using a short or long form. Like any parameter, they have to be separated from the header by a white space. In the case of a query, the short form of the text is provided.

Example

Setting command: `INPut:COUPling GROund`

Query: `INPut:COUPling?`, Response: `GRO`

5.2.5 Strings

Strings must always be entered in quotation marks (' or ").

Example

`SYSTem:LANGuage "SCPI"` or `SYSTem:LANGuage 'SCPI'`

5.2.6 Block Data

Block data are a transmission format which is suitable for the transmission of large amounts of data. A command using a block data parameter has the following structure:

Example

`HEADer:HEADer #45168xxxxxxxx`

ASCII character # introduces the data block. The next number indicates how many of the following digits describe the length of the data block. In the example the 4 following digits indicate the length to be 5168 bytes. The data bytes follow. During the transmission of these data bytes all end or other control signs are ignored until all bytes are transmitted.

5.3 Structure of a Program Message

A program message may consist of one or several commands. It is terminated by the program message terminator which is the NL (New Line) character for LAN and USB connections.

Several commands in a program message must be separated by a semicolon ";". If the next command belongs to a different command system, the semicolon is followed by a colon. A colon ":" at the beginning of a command marks the root node of the command tree.

Example:

```
CALL InstrWrite(analyzer, "SENSe:FREQuency:CENTer  
100MHz;:INPut:ATTenuation 10")
```

This program message contains two commands. The first one is part of the SENSE command system and is used to determine the center frequency of the instrument. The second one is part of the INPut command system and sets the input signal attenuation.

If the successive commands belong to the same system, having one or several levels in common, the program message can be abbreviated. For that purpose, the second command after the semicolon starts with the level that lies below the common levels (see also Fig. 1-1). The colon following the semicolon must be omitted in this case.

Example:

```
CALL InstrWrite(analyzer, "SENSe:FREQuency:START  
1E6;:SENSe:FREQuency:STOP 1E9")
```

This program message is represented in its full length and contains two commands separated from each other by the semicolon. Both commands are part of the SENSE command system, subsystem FREQuency, i.e. they have two common levels.

When abbreviating the program message, the second command begins with the level below SENSE:FREQuency. The colon after the semicolon is omitted. The abbreviated form of the program message reads as follows:

```
CALL InstrWrite(analyzer, "SENSe:FREQuency:START 1E6;STOP 1E9")
```

However, a new program message always begins with the complete path.

Example:

```
CALL InstrWrite(analyzer, "SENSe:FREQuency:START 1E6")  
CALL InstrWrite(analyzer, "SENSe:FREQuency:STOP 1E9")
```

5.4 Responses to Queries

A query is defined for each setting command unless explicitly specified otherwise. It is formed by adding a question mark to the associated setting command. According to SCPI, the responses to queries are partly subject to stricter rules than in standard IEEE 488.2.

- The requested parameter is transmitted without header.

Example

```
INPut:COUPling?
```

```
Response: DC
```

- Maximum values, minimum values and all further quantities, which are requested via a special text parameter are returned as numerical values.

Example

```
SENSe:FREQuency:STOP? MAX
```

```
Response: 3.5E9
```

- Numerical values are output without a unit. Physical quantities are referred to the basic units or to the units set using the Unit command.

Example

```
SENSe:FREQuency:CENTer?
```

```
Response: 1E6 (for 1 MHz)
```

- Truth values <Boolean values> are returned as 0 (for OFF) and 1 (for ON).

Example

```
SENSe:BANDwidth:AUTO?
```

```
Response: 1 (for ON)
```

- Text (character data) is returned in a short form.

Example

```
SYSTem:COMMunicate:SERial:CONTRol:RTS?
```

```
Response STAN (for standard)
```

6 Command Sequence and Command Synchronization

What has been said above makes clear that all commands can potentially be carried out overlapping. In order to prevent an overlapping execution of commands, one of the commands `*OPC`, `*OPC?` or `*WAI` must be used. All three commands cause a certain action only to be carried out after the hardware has been set. By suitable programming, the controller can be forced to wait for the respective action to occur. For more information see Table 6-1.

Table 6-1: Synchronization using `*OPC`, `*OPC?` and `*WAI`

Command	Action	Programming the controller
<code>*OPC</code>	Sets the Operation Complete bit in the ESR after all previous commands have been executed.	<ul style="list-style-type: none"> – Setting bit 0 in the ESE – Setting bit 5 in the SRE – Waiting for service request (SRQ)
<code>*OPC?</code>	Stops command processing until 1 is returned. This is only the case after the Operation Complete bit has been set in the ESR. This bit indicates that the previous setting has been completed.	Sending <code>*OPC?</code> directly after the command whose processing should be terminated before other commands can be executed.
<code>*WAI</code>	Stops further command processing until all commands sent before <code>*WAI</code> have been executed.	Sending <code>*WAI</code> directly after the command whose processing should be terminated before other commands are executed.

For a couple of commands the synchronization to the end of command execution is mandatory in order to obtain the desired result. The affected commands require either more than one measurement in order to accomplish the desired instrument setting (e.g. auto range functions), or they require a longer period of time for execution. If a new command is received during execution of the corresponding function this may either lead to either to an aborted measurement or to incorrect measurement data.

The following list includes the commands, for which a synchronization via `*OPC`, `*OPC?` or `*WAI` is mandatory:

Table 6-2: Commands with mandatory synchronization (overlapping commands)

Command	Purpose
<code>INIT</code>	start measurement (sweep)
<code>INIT:CONT OFF</code>	Set to single sweep
<code>CALC:MARK:FUNC:xx?</code>	All Marker function queries

7 Remote Control – Commands

The following chapters provide a detailed description of all remote control commands currently available for the R&S ZVH and its firmware options.

Each section describes the commands for one of the operating modes available in the R&S ZVH, beginning with the description of common commands required to operate the instrument. The structure is based on that of the operating manual.

- [Common Commands](#) on page 32
- [Remote Commands of the Cable and Antenna Analyzer](#) on page 35
- [Remote Commands of the Spectrum Analyzer](#) on page 75
- [Remote Commands of the Network Analyzer Mode](#) on page 146
- [Remote Commands of the Power Meter](#) on page 168

Each section is subdivided into various tasks required to perform measurements with the R&S ZVH, also based on the structure of the operating manual. Some commands like those for controlling markers or configuring the frequency axis are available for all operating modes. In that case you will find a list of these commands in the corresponding section. However, a detailed description is provided only in the commands section of the main application.



Availability of commands

The cable and antenna test mode is implemented in the basic unit. For the other modes, the corresponding options are required.

Following the remote control commands required to perform specific measurements, you will find a description of general commands used to set up and control basic instrument functions. These commands are independent of the operating mode. Therefore they are listed separately.

- [File Management](#) on page 175
- [Making and Storing Screenshots](#) on page 183
- [Configuring the Instrument](#) on page 190
- [Remote Commands of the Status Reporting System](#) on page 224

All chapters begin with a list of commands available in the context of that chapter. Following that list you will find a detailed description of all commands.

All individual descriptions contain:

- the complete notation and syntax of the command
- the description of the effects of the command
- a list of all parameters available for that command or the type of data the command returns in case of query commands
- an example of how a program message would look like
- the *RST value
- information on SCPI conformity

An alphabetical list of all available commands is provided at the end of this manual.

7.1 Common Commands

The common commands are taken from the IEEE 488.2 (IEC 625-2) standard. A particular command has the same effect on different devices. The headers of these commands consist of an asterisk "*" followed by three letters. Some of the common commands refer to the ["Status Reporting System"](#).

List of commands

- [*CLS](#) (p. 32)
- [*ESE](#) (p. 32)
- [*ESR?](#) (p. 32)
- [*IDN?](#) (p. 33)
- [*IST?](#) (p. 33)
- [*OPC](#) (p. 33)
- [*OPT?](#) (p. 33)
- [*RST](#) (p. 33)
- [*SRE](#) (p. 34)
- [*STB?](#) (p. 34)
- [*TRG](#) (p. 34)
- [*TST?](#) (p. 34)
- [*WAI](#) (p. 34)

*CLS

CLEAR STATUS sets the status byte (STB), the standard event register (ESR) and the EVENT part of the QUESTIONable and the OPERATION register to zero. The command does not alter the mask and transition parts of the registers. It clears the output buffer.

*ESE

EVENT STATUS ENABLE sets the event status enable register to the value indicated. The query form [*ESE?](#) returns the contents of the event status enable register in decimal form.

Parameter

0 to 255

*ESR?

STANDARD EVENT STATUS QUERY returns the contents of the event status register in decimal form (0 to 255) and subsequently sets the register to zero.

Parameter

0 to 255

***IDN?**

IDENTIFICATION QUERY queries the instrument identification.

Return values

<InstrumentName>,<SerialNumber/Model>,<FirmwareVersion>

Example for R&S ZVH:

Rohde&Schwarz,ZVH4,100005/014,1.20

***IST?**

INDIVIDUAL STATUS QUERY returns the contents of the IST flag in decimal form. The IST flag is the status bit which is sent during a parallel poll.

Parameter

0 | 1

***OPC**

OPERATION COMPLETE sets bit 0 in the event status register after all preceding commands have been executed. This bit can be used to initiate a service request.

***OPT?**

OPTION IDENTIFICATION QUERY queries the options included in the instrument and returns a list of the options installed. The options are separated from each other by means of commas.

Parameter

K<number> software options

For a list of all available options and their description refer to the CD-ROM.

Example

K40, K41, K42, K45

***RST**

RESET sets the instrument to a defined default status. The command essentially corresponds to pressing the PRESET key.

***SRE**

SERVICE REQUEST ENABLE sets the service request enable register to the indicated value. Bit 6 (MSS mask bit) remains 0. This command determines under which conditions a service request is generated. The query form *SRE? reads the contents of the service request enable register in decimal form. Bit 6 is always 0.

Parameter

0 to 255

***STB?**

READ STATUS BYTE QUERY reads out the contents of the status byte in decimal form.

***TRG**

TRIGGER initiates all actions in the currently active test screen expecting a trigger event. This command corresponds to `INITiate[:IMMediate]`.

***TST?**

SELF TEST QUERY initiates the self test of the instrument and outputs an error code in decimal form.

Parameter

0 = no error

***WAI**

WAIT TO CONTINUE permits servicing of subsequent commands only after all preceding commands have been executed and all signals have settled.

7.2 Remote Commands of the Cable and Antenna Analyzer

This section provides a detailed description of all remote control commands required to configure and perform measurements in Cable and Antenna Test (CAT) mode.

Contents

[Configuring the Horizontal Axis](#) on page 36

[Configuring the Vertical Axis](#) on page 41

[Setting the Bandwidth](#) on page 47

[Performing and Triggering Measurements](#) on page 48

[Working with Traces](#) on page 50

[Using Markers](#) on page 55

[Configuring and Using Measurement Functions](#) on page 65

7.2.1 Configuring the Horizontal Axis

The following commands configure the horizontal axis of the active display.



Commands independent of the operating mode

Note that some of the commands for configuring the horizontal axis are also valid for other operating modes. If a command is available in another mode, it is indicated by the list in the respective section.

List of commands

- [\[SENSe:\]FREQUency:CENTer <Frequency>](#) (p. 36)
- [\[SENSe:\]FREQUency:CENTer:STEP <StepSize>](#) (p. 36)
- [\[SENSe:\]FREQUency:CENTer:STEP:LINK <StepSizeCoupling>](#) (p. 37)
- [\[SENSe:\]FREQUency:SPAN](#) (p. 38)
- [\[SENSe:\]FREQUency:SPAN:AUTO <State>](#) (p. 38)
- [\[SENSe:\]FREQUency:STARt <StartFrequency>](#) (p. 39)
- [\[SENSe:\]FREQUency:STOP <StopFrequency>](#) (p. 39)
- [CALCulate:DTF:DISTance:STARt <StartDistance>](#) (p. 39)
- [CALCulate:DTF:DISTance:STOP <StopDistance>](#) (p. 40)

[SENSe:]FREQUency:CENTer <Frequency>

This command defines the center frequency of the R&S ZVH.

In spectrum analyzer mode, the command also defines the measuring frequency for time domain measurements (span = 0).

Parameter

<Frequency>

Numeric value in Hz.

The range depends on the operating mode and is specified in the data sheet.

Example

```
FREQ:CENT 100MHz
```

Defines a center frequency of 100 MHz.

Characteristics

*RST value: $f_{\max} / 2$ with f_{\max} = maximum frequency

SCPI: conform

[SENSe:]FREQUency:CENTer:STEP <StepSize>

This command defines the center frequency step size.

Parameter

<StepSize>

Numeric value in Hz.

The range is from 1 Hz to f_{\max} .

Example

```
FREQ:CENT:STEP 120MHz
```

Defines a CF step size of 120 MHz.

Characteristics

*RST value: – (AUTO 0.1*SPAN is switched on)

SCPI: conform

[SENSe:]FREQuency:CENTer:STEP:LINK <StepSizeCoupling>

This command couples and decouples the center frequency step size to the span.

For time domain measurements, the command couples the step size to the resolution bandwidth.

Parameter

<StepSizeCoupling>

DIVTen	Couples the step size to 10 % of the span.
OFF	Turns the coupling off (manual definition of the step size).

Example

```
FREQ:CENT:STEP:LINK DIVT
```

Couples the step size to 10% of the span.

Characteristics

*RST value: DIVTen

SCPI: device-specific

[SENSe:]FREQuency:SETTings:COUPling:ENABLE <State>

This command couples and decouples frequency and span settings between the DTF measurement and the other measurements available in the Antenna & Cable Test mode.

Parameter

<State>

ON	Frequency and span settings are coupled. Settings are adapted when you switch between measurements.
OFF	Frequency and span settings are decoupled. DTF measurement has its own frequency and span settings compared to the other measurements..

Example

```
FREQ:SETT:COUP:ENAB ON
```

Couples the frequency and span settings.

Characteristics

*RST value: OFF

SCPI: device-specific

**[SENSe:]FREQuency:SPAN **

This command defines the frequency span.

If you set a span of 0 Hz in spectrum mode, the R&S ZVH starts a measurement in the time domain.

Parameter

Numeric value in Hz. The value range is specified in the data sheet.

Example

```
FREQ:SPAN 10MHz
```

Defines a span of 10 MHz.

Characteristics

*RST value: f_{\max} with f_{\max} = maximum frequency

SCPI: conform

[SENSe:]FREQuency:SPAN:AUTO <State>

This command turns the automatic calculation of the ideal span on and off.

Parameter

<State>

ON | OFF

Example

```
FREQ:SPAN:AUTO ON
```

Turns automatic span determination on and off.

Characteristics

*RST value: OFF

SCPI: device-specific

[SENSe:]FREQuency:STARt <StartFrequency>

This command defines the start frequency for measurements in the frequency domain (span > 0).

Parameter

<StartFrequency>

Numeric value in Hz.

The range depends on the operating mode and is specified in the datasheet.

Example

```
FREQ:STAR 20MHz
```

Defines a start frequency of 20 MHz.

Characteristics

*RST value: 0

SCPI: conform

[SENSe:]FREQuency:STOP <StopFrequency>

This command defines the stop frequency for measurements in the frequency domain (span > 0).

Parameter

<StopFrequency>

Numeric value in Hz.

The range depends on the operating mode and is specified in the datasheet.

Example

```
FREQ:STOP 2000MHz
```

Defines a stop frequency of 2 GHz

Characteristics

*RST value: f_{\max}

SCPI: conform

CALCulate:DTF:DISTance:STARt <StartDistance>

This command defines the start distance of the cable measurement.

Parameter

<StartDistance>

Numeric value in the range from 3 m (10 ft) to 1500 m (4921 ft)

The unit is either meter or feet, depending on your selection.

Example

```
CALC:DTF:DIST:STAR 50m
```

Sets the starting point of the measurement to 50 m.

Characteristics

*RST value: 3 m (10 ft)

SCPI: device-specific

CALCulate:DTF:DISTance:STOP <StopDistance>

This command defines the end point of the cable measurement.

Parameter

<StopDistance>

numeric value in the range from 3 m (10 ft) to 1500 m (4921 ft)

The unit is either meter or feet, depending on your selection.

Example

```
CALC:DTF:DIST:STAR 500m
```

Sets the end point of the measurement to 500 m.

Characteristics

*RST value: 1500 m (4921 ft)

SCPI: device-specific

7.2.2 Configuring the Vertical Axis

The following commands configure the vertical axis of the active display.

In cable and antenna mode, the suffix <n> at CALCulate or TRACe selects the diagram in split screen mode. Its range is {1..2}.



Commands independent of the operating mode

Note that some of the commands for configuring the vertical axis are also valid for other operating modes. If a command is available in another mode, it is indicated by the list in the respective section.

List of commands

- [DISPlay\[:WINDow\]:TRACe<n>:Y\[:SCALe\]:ADJust](#) (p. 41)
- [DISPlay:LOSS:REFerence <RefValue>](#) (p. 41)
- [DISPlay:LOSS:REFerence:POSition <RefPosition>](#) (p. 42)
- [DISPlay:LOSS:Y:SCALe <DisplayRange>](#) (p. 42)
- [DISPlay<n>:MAGNitude:REFerence <RefValue>](#) (p. 43)
- [DISPlay<n>:MAGNitude:REFerence:POSition <RefPosition>](#) (p. 43)
- [DISPlay<n>:MAGNitude:Y:SCALe <DisplayRange>](#) (p. 43)
- [DISPlay<n>:MAGNitude:Y:SPACing <Scaling>](#) (p. 44)
- [DISPlay<n>:VSWR:Y:SCALe:MINimum <BottomValue>](#) (p. 44)
- [DISPlay<n>:VSWR:Y:SCALe:MAXimum <TopValue>](#) (p. 45)
- [DISPlay<n>:VSWR:Y:SCALe <DisplayRange>](#) (p. 45)
- [INPut:ATTenuation <Attenuation>](#) (p. 45)
- [SOURce:TG:ATTenuation <TGAttenuation>](#) (p. 46)

DISPlay[:WINDow]:TRACe<n>:Y[:SCALe]:ADJust

This command automatically scales the vertical axis for ideal display results.

This command is an event and therefore has no query and no *RST value.

Example

```
DISP:TRAC:Y:ADJ
```

Determines the ideal scaling for the y-axis.

Characteristics

*RST value: -

SCPI: device-specific

DISPlay:LOSS:REFerence <RefValue>

This command defines the reference value for the cable loss measurement format.

Parameter

<RefValue>

Numeric value in the range from -100 dB to 100 dB.

Example

DISP:LOSS:REF 10

Defines a reference level of 10 dB.

Characteristics

*RST value: 0 dB

SCPI: device-specific

DISPlay:LOSS:REfERENCE:POSition <RefPosition>

This command defines the position of the reference value in the diagram for the cable loss measurement format.

Each step shifts the reference position one grid line up or down.

Parameter

<RefPosition>

Numeric value in the range from 0 to 10.

Example

DISP:LOSS:REF:POS 5

Moves the reference to the fifth grid line from the bottom.

Characteristics

*RST value: 10

SCPI: device-specific

DISPlay:LOSS:Y:SCALE <DisplayRange>

This command defines the display range of the vertical axis for the cable loss measurement format.

Parameter

<DisplayRange>

Numeric value in the range from 1 dB to 100 dB.

Example

DISP:LOSS:Y:SCAL 20

Defines a display range of 20 dB

Characteristics

*RST value: 100 dB

SCPI: device-specific

DISPlay<n>:MAGNitude:REFerence <RefValue>

This command defines the reference value for the magnitude measurement format.

Parameter

<RefValue>

Numeric value in the range from -80 dB to 30 dB

Example

```
DISP:MAGN:REF -10
```

Defines a reference level of -10 dB

Characteristics

*RST value: 0 dB

SCPI: device-specific

DISPlay<n>:MAGNitude:REFerence:POSition <RefPosition>

This command defines the position of the reference value in the diagram for the magnitude measurement format.

Each step shifts the reference position one grid line up or down.

Parameter

<RefPosition>

Numeric value in the range from 0 to 10.

Example

```
DISP:MAGN:REF:POS 5
```

Moves the reference to the fifth grid line from the bottom.

Characteristics

*RST value: 10

SCPI: device-specific

DISPlay<n>:MAGNitude:Y:SCALE <DisplayRange>

This command defines the display range of the vertical axis for the magnitude measurement format.

Note that you have to set a logarithmic scaling before you can use this command with [DISPlay<n>:MAGNitude:Y:SPACing <Scaling>](#).

Parameter

<DisplayRange>

Numeric value in the range from 1 dB to 150 dB.

The number you enter is rounded up to the next possible display range. For example, if you enter 9, the R&S ZVH automatically sets the display range to 10.

Example

DISP:MAGN:Y:SCAL 50 DB
 Defines a display range of 50 dB.

Characteristics

*RST value: 100 dB
 SCPI: device-specific

DISPlay<n>:MAGNitude:Y:SPACing <Scaling>

This command selects the scaling of the vertical axis for the magnitude measurement format.

Parameter

<Scaling>

LOGarithmic	Selects a logarithmic scale (dB).
LINear	Selects a linear scale (%).

Example

DISP:MAGN:Y:SPAC LIN
 Selects linear scaling.

Characteristics

*RST value: LOGarithmic
 SCPI: device-specific

DISPlay<n>:VSWR:Y:SCALE:MINimum <BottomValue>

This command defines the bottom value of the vertical axis for the VSWR measurement format.

Parameter

<BottomValue>
 Numeric value in the range from 1.0 to 70.

Example

DISP:VSWR:Y:SCALE:MIN 3
 Defines a bottom value of 3 for the vertical axis.

Characteristics

*RST value: 1.0
 SCPI: device-specific

DISPlay<n>:VSWR:Y:SCALe:MAXimum <TopValue>

This command defines the top value of the vertical axis for the VSWR measurement format.

Parameter

<TopValue>

Numeric value in the range from 1.1 to 71.

Example

```
DISP:VSWR:Y:SCAL:MAX 25
```

Defines a top value of 25 for the vertical axis.

Characteristics

*RST value: 21

SCPI: device-specific

DISPlay<n>:VSWR:Y:SCALe <DisplayRange>

This command defines the display range of the vertical axis for the VSWR measurement format.

Parameter

<DisplayRange>

Numeric value in the range from 1.1 to 71.

The number you enter is rounded up to the next possible display range. For example, if you enter 5, the R&S ZVH automatically sets the display range to 1...6.

Example

```
DISP:VSWR:Y:SCAL 50
```

Defines a display range of 1...71.

Characteristics

*RST value: 1...21

SCPI: device-specific

INPut:ATTenuation <Attenuation>

This command defines the input attenuation.

In spectrum mode, the attenuation is coupled to the reference level. If you set the attenuation independently, the R&S ZVH turns off this coupling.

The R&S ZVH adjusts the reference level if it can not be set for the current RF attenuation.

Parameter

<Attenuation>

Numeric value in the range from 0 dB to 40 dB in 5 dB steps.

Example

```
INP:ATT 30dB
```

Defines an attenuation of 30 dB and deactivates coupling to the reference level.

Characteristics

*RST value: 0 dB (AUTO is ON)

SCPI: conform

SOURce:TG:ATTenuation <TGAttenuation>

This command defines the output level of the tracking generator.

Parameter

<TGAttenuation>

Numeric value in the range from 0 to 50 dB.

Entering an output level of, e.g., 20 dB results in an output level of -20 dBm.

Example

```
SOUR:TG:ATT 50
```

Defines the attenuation to 50 dB and therefore an output level of -50 dBm

Characteristics

*RST value: 0 dB

SCPI: device-specific

7.2.3 Setting the Bandwidth

The following commands configure the filter bandwidths of the R&S ZVH. Note that both groups of commands (BANDwidth and BWIDth) are the same.

List of commands

- [\[SENSe:\]BANDwidth|BWIDth\[:RESolution\] <MeasBW>](#) (p. 47)
- [\[SENSe:\]BANDwidth|BWIDth\[:RESolution\]:AUTO <State>](#) (p. 47)

[SENSe:]BANDwidth|BWIDth[:RESolution] <MeasBW>

This command defines the measurement bandwidth.

Analog resolution filters of 100 Hz to 100 kHz in 1 - 3 - 10 steps are available.

Parameter

<MeasBW>

Numeric value in the range from 100 Hz to 100 kHz.

Example

```
BAND 100 kHz  
Sets the bandwidth to 100 kHz
```

Characteristics

*RST value: – (AUTO is set to ON)

SCPI: conform

[SENSe:]BANDwidth|BWIDth[:RESolution]:AUTO <State>

This command couples or decouples the measurement bandwidth to the span.

Parameter

<State>

ON | OFF

Example

```
BAND:AUTO OFF  
Switches off the coupling of the resolution bandwidth to the span.
```

Characteristics

*RST value: ON

SCPI: conform

7.2.4 Performing and Triggering Measurements

7.2.4.1 Performing the Measurement

The following commands configure the sweep.

List of commands

- [INITiate:CONTinuous <SweepMode>](#) (p. 90)
- [SENSe:SWEep:POINts <Points>](#) (p. 48)

For a detailed description of commands refer to "[Performing and Triggering Measurements](#)" in spectrum analyzer mode.

SENSe:SWEep:POINts <Points>

This command selects the number of measurement points.

Parameter

<Points>

101 | 201 | 401 | 601 | 631 | 801 | 1001 | 1201

Example

```
SWE:POIN 101
```

Defines 101 measurement points.

Characteristics

*RST value: 201

SCPI: conform

7.2.4.2 Triggering Measurements

The following commands set up trigger conditions if you are using a trigger for the measurement.

List of commands

- [TRIGger\[:SEquence\]:HOLDoff\[:TIME\] <TriggerDelay>](#) (p. 48)
- [TRIGger\[:SEquence\]:SLOPe <TriggerSlope>](#) (p. 49)
- [TRIGger\[:SEquence\]:SOURce <TriggerSource>](#) (p. 49)

TRIGger[:SEquence]:HOLDoff[:TIME] <TriggerDelay>

This command defines the length of the trigger delay.

Parameter

<TriggerDelay>

Numeric value in the range from 0 s to 100 s.

Example

```
TRIG:HOLD 500us
```

Defines a trigger delay of 500 µs.

Characteristics

*RST value: 0 s

SCPI: conform

TRIGger[:SEquence]:SLOPe <TriggerSlope>

This command selects the slope of the trigger signal.

The trigger slope affects all trigger sources.

Parameter

<TriggerSlope>

POSitive | NEGative

Example

```
TRIG:SLOP NEG
```

Selects a negative trigger slope.

Characteristics

*RST value: POSitive

SCPI: conform

TRIGger[:SEquence]:SOURce <TriggerSource>

This command selects the trigger source that initiates a measurement.

Parameter

<TriggerSource>

IMMediate	Free Run measurements.
EXTernal	External triggering.

For more information see R&S ZVH operating manual chapter "Setting the Sweep"

Example

```
TRIG:SOUR EXT
```

Selects the external trigger input as source of the trigger signal

Characteristics

*RST value: IMMediate

SCPI: conform

7.2.5 Working with Traces

The following commands set up the trace and the various functions associated with it, e.g. trace mathematics or the selection of the detector.

The suffix <n> at TRACe and MATH selects the trace the command works on.

List of commands

- [CALCulate:MATH<n>:COPY:MEMory](#) (p. 50)
- [DISPlay\[:WINDow\]:TRACe<n>:MEMory\[:STATe\] <State>](#) (p. 50)
- [DISPlay\[:WINDow\]:TRACe<n>:MODE <TraceMode>](#) (p. 51)
- [FORMat\[:DATA\] <DataFormat>](#) (p. 51)
- [MEASurement:ISUP <State>](#) (p. 52)
- [MEASurement:ISUP:APER <Aperture>](#) (p. 52)
- [TRACe:DATA](#) (p. 52)
- [TRACe<n>:DATA:MEMory? <Trace>](#) (p. 53)
- [UNIT:LENGth <Unit>](#) (p. 54)

CALCulate:MATH<n>:COPY:MEMory

This command copies the current trace into the memory of the R&S ZVH.

This command is an event and therefore has no query and no *RST value.

Example

```
CALC:MATH:COPY:MEM
```

Copies the trace into the memory.

Characteristics

*RST value: -

SCPI: device-specific

DISPlay[:WINDow]:TRACe<n>:MEMory[:STATe] <State>

This command turns the memory trace on and off.

Parameter

<State>

ON | OFF

Example

```
DISP:TRAC:MEM ON
```

Turns on the memory trace.

Characteristics

*RST value: OFF

SCPI: device-specific

DISPlay[:WINDow]:TRACe<n>:MODE <TraceMode>

This command selects the trace mode.

If you are using the average, max hold or min hold trace mode, you can set the number of measurements with [SENSe:]SWEep:COUNT <SweepCount>. Note that synchronization to the end of the average count is possible only in single sweep mode.

The suffix <n> is irrelevant.

Parameter

<TraceMode>

AVERAge | MAXHold | MINHold | VIEW | WRITe

Example

```
INIT:CONT OFF
```

```
SWE:COUN 16
```

Turn on single sweep mode and defines a sweep count of 16 measurements.

```
DISP:TRAC:MODE MAXH
```

Activates MAXHold mode for the trace.

```
INIT;*WAI
```

Performs a measurement with synchronization after 16 sweeps.

Characteristics

*RST value: WRITe

SCPI: device-specific

FORMat[:DATA] <DataFormat>

This command selects the data format that is used for transmission of trace data from the R&S ZVH to the controlling computer.

Note that the command has no effect for data that you send to the R&S ZVH. The R&S ZVH automatically recognizes the data it receives, regardless of the format.

Parameter

<DataFormat>

ASCIi	ASCII format, separated by commas.
REAL,32	32-bit IEEE 754 floating point numbers in the "definite length block format".

In REAL,32 format, a string of return values would look like:

```
#42524<value 1><value 2>...<value n>
```

with

#4	Number of digits of the following number of data bytes (= 4 in this example)
2524	Number of following data bytes (2524, corresponds to the 631 sweep points of the R&S ZVH).
<value>	4-byte floating point value

Example

```
FORM ASC
```

Selects the ASCII data format.

Characteristics

*RST value: ASCii

SCPI: conform

MEASurement:ISUP <State>

This command turns interference suppression on and off.

Parameter

<State>

ON | OFF

Example

```
MEAS:ISUP ON
```

Turns interference suppression on.

Characteristics

*RST value: OFF

SCPI: device-specific

MEASurement:ISUP:APER <Aperture>

This command defines the aperture size for interference suppression.

Parameter

<Aperture>

Numeric value that defines the aperture.

Example

```
MEAS:ISUP:APER 0.8
```

Sets an aperture of 0.8.

Characteristics

*RST value: 1

SCPI: device-specific

TRACe:DATA <Destination>

This command queries the current trace data.

You can set the data format with the `FORMat[:DATA] <DataFormat>`.

Parameter

<Destination>

TRACE1	Queries the data of trace 1.
TRACE2	Queries the data of trace 2..

Return value

The R&S ZVH returns 631 values. Each value corresponds to one pixel of a trace.

The result and unit depends on the measurement format.

Example

```
TRAC:DATA? TRACE1
```

Reads out the data for trace 1.

Characteristics

*RST value: -

SCPI: conform

TRACe<n>:DATA:MEMory? <Trace>

This command queries the memory trace data.

You can set the data format with the `FORMat[:DATA] <DataFormat>`.

To query memory trace data, you have to create a memory trace first with `DISPlay[:WINDow]:TRACe<n>:MEMory[:STATe] <State>`.

Parameter

<Trace>

TRACE1	Queries the data of memory trace 1.
TRACE2	Queries the data of memory trace 2.
TRACE3	Queries the data of memory trace 3.
TRACE4	Queries the data of memory trace 4.

Only traces that are actually in the trace memory can be exported.

Return value

The R&S ZVH returns 631 values. Each value corresponds to one pixel of a trace.

The result and unit depends on the measurement format.

Example

```
DISP:TRAC2:MODE AVER
```

```
CALC:MATH2:COPY:MEM
```

```
TRAC:DATA:MEM? TRACE1
```

Reads out the data for memory trace 1.

Characteristics

*RST value: -

SCPI: conform

UNIT:LENGth <Unit>

This command selects the length unit.

Parameter

<Unit>

METer | FEET

Example

UNIT:LENGth FEET

Selects feet as the length unit.

Characteristics

*RST value: METer

SCPI: conform

7.2.6 Using Markers

The following commands position and control markers and deltamarkers.

In cable and antenna mode, the suffix <n> at CALCulate selects the trace in split screen mode. Its range is {1..2}.

The suffix <m> at MARKer selects the marker or delta marker.

List of commands

- CALCulate<n>:DELTamarker<m>[:STATe] <State> (p. 55)
- CALCulate<n>:DELTamarker<m>:AOFF (p. 56)
- CALCulate<n>:DELTamarker<m>:MAXimum[:PEAK] (p. 56)
- CALCulate<n>:DELTamarker<m>:MAXimum:NEXT (p. 56)
- CALCulate<n>:DELTamarker<m>:MINimum[:PEAK] (p. 56)
- CALCulate<n>:DELTamarker<m>:X <Coordinate> (p. 57)
- CALCulate<n>:DELTamarker<m>:X:RELative <Distance> (p. 57)
- CALCulate<n>:DELTamarker<m>:Y? (p. 58)
- CALCulate<n>:MARKer<m>[:STATe] <State> (p. 59)
- CALCulate<n>:MARKer<m>:AOFF (p. 59)
- CALCulate<n>:MARKer<m>:MAXimum[:PEAK] (p. 59)
- CALCulate<n>:MARKer<m>:MAXimum:NEXT (p. 60)
- CALCulate<n>:MARKer<m>:MINimum[:PEAK] (p. 60)
- CALCulate<n>:MARKer<m>:POSition <StepSize> (p. 60)
- CALCulate<n>:MARKer<m>:X <Coordinate> (p. 61)
- CALCulate<n>:MARKer<m>:X:SLIMits[:STATe] <State> (p. 61)
- CALCulate<n>:MARKer<m>:X:SLIMits:LEFT <SearchLimit> (p. 62)
- CALCulate<n>:MARKer<m>:X:SLIMits:RIGHT <Searchlimit> (p. 62)
- CALCulate<n>:MARKer<m>:Y? (p. 63)

CALCulate<n>:DELTamarker<m>[:STATe] <State>

This command turns delta markers on and off.

If you set the suffix at DELTmarker to 1, or use no suffix, the R&S ZVH interprets this as delta marker 2 because the first marker has to be a normal marker. If more than one normal marker (2 to 6) are already active, the command turns these marker into delta markers. If no delta marker is active yet, the command activates the delta marker and positions it on the trace maximum.

Parameter

<State>
ON | OFF

Example

CALC:DELT3 ON

Turns delta marker 3 on or turns marker 3 into a delta marker.

Characteristics

RST value: OFF
SCPI: device-specific

CALCulate<n>:DELTamarker<m>:AOFF

This command turns off all active delta markers.

This command is an event and therefore has no query and no *RST value.

Example

```
CALC:DELT:AOFF
```

Turns off all delta markers.

Characteristics

RST value: –

SCPI: device-specific

CALCulate<n>:DELTamarker<m>:MAXimum[:PEAK]

This command positions a delta marker on the current trace maximum.

If necessary, the corresponding delta marker is activated first.

This command is an event and therefore has no *RST value and no query.

Example

```
CALC:DELT3:MAX
```

Moves delta marker 3 to the maximum peak.

Characteristics

RST value: –

SCPI: device-specific

CALCulate<n>:DELTamarker<m>:MAXimum:NEXT

This command positions a delta marker on the next smaller trace maximum.

If necessary, the corresponding delta marker is activated first.

This command is an event and therefore has no *RST value and no query.

Example

```
CALC:DELT2:MAX:NEXT
```

Moves delta marker 2 to the next smaller maximum peak.

Characteristics

RST value: –

SCPI: device-specific

CALCulate<n>:DELTamarker<m>:MINimum[:PEAK]

This command positions a delta marker on the current trace minimum.

If necessary, the corresponding delta marker is activated first.

This command is an event and therefore has no *RST value and no query.

Example

```
CALC:DELT3:MIN
```

Moves delta marker 3 to the trace minimum.

Characteristics

RST value: –

SCPI: device-specific

CALCulate<n>:DELTamarker<m>:X <Coordinate>

This command positions a delta marker on a particular coordinate on the horizontal axis.

Note that it is possible to place the marker outside the visible trace. In that case, this value is invalid.

If necessary, the corresponding delta marker is activated first.

Parameter

<Coordinate>

Numeric value that indicates the coordinate on the horizontal axis.

The range corresponds to the maximum span.

The unit depends on the measurement, e.g. Hz for measurements in the frequency domain and seconds for measurements in the time domain.

Example

```
CALC:DELT:MOD REL
```

Delta marker positions are relative to marker 1.

```
CALC:DELT2:X 10.7MHz
```

Positions delta marker 2 10.7 MHz to the right of marker 1.

```
CALC:DELT2:X?
```

```
CALC:DELT2:X:REL?
```

Queries the absolute and relative position of delta marker 2.

Characteristics

RST value: –

SCPI: device-specific

CALCulate<n>:DELTamarker<m>:X:RELative <Distance>

This command positions a delta marker on a position relative to the reference marker.

If necessary, the corresponding delta marker is activated first.

Parameter

<Distance>

Numeric value that defines the distance of the marker to the reference marker

The range depends on the current scaling of the horizontal axis.

The unit depends on the measurement, e.g. Hz for measurements in the frequency domain and seconds for measurements in the time domain.

Example

```
CALC:DELT3:X:REL 5 kHz
```

Sets the delta marker at a distance of 5 kHz to the reference position.

Characteristics

RST value: –

SCPI: device-specific

CALCulate<n>:DELTaMarker<m>:Y?

This command queries the vertical position of a delta marker. The result is always a relative value in relation to marker 1.

If necessary, the corresponding delta marker is activated first.

To get a valid result, you have to perform a complete sweep with synchronization to the sweep end between activating the delta marker and reading out the result. This is only possible in single sweep mode.

Return value

<MarkerPosition>

In NA and CAT mode, the unit depends on the measurement format.

In spectrum analyzer mode, the unit depends on the unit you have set and the scaling of the vertical axis.

Parameter or measuring functions	Output unit
DBM DBPW DBUV DBMV DBUA	dB (lin/log)
WATT VOLT AMPere	dB (lin), % (log)

Example

```
INIT:CONT OFF
```

Switches to single sweep mode.

```
CALC:DELT2 ON
```

Switches on delta marker 2.

```
INIT;*WAI
```

Starts a sweep and waits for its end.

```
CALC:DELT2:Y?
```

Queries the horizontal position of delta marker 2.

Characteristics

RST value: –

SCPI: device-specific

CALCulate<n>:MARKer<m>[:STATe] <State>

This command turns markers on and off.

If you do not use a suffix at MARKer, marker 1 is selected. If one or more delta markers (2 to 6) are already active, the command turns these delta markers into normal markers.

Parameter

<State>
ON | OFF

Example

```
CALC:MARK3 ON
```

Turns on marker 3.

Characteristics

*RST value: OFF
SCPI: device-specific

CALCulate<n>:MARKer<m>:AOFF

This command turns off all active markers, delta markers and active marker measurement functions.

This command is an event and therefore has no query and no *RST value.

Example

```
CALC:MARK:AOFF
```

Turns off all markers.

Characteristics

*RST value: –
SCPI: device-specific

CALCulate<n>:MARKer<m>:MAXimum[:PEAK]

This command positions a marker on the current trace maximum.

If necessary, the corresponding marker is activated first.

This command is an event and therefore has no *RST value and no query.

Example

```
CALC:MARK2:MAX
```

Moves marker 2 to the maximum peak.

Characteristics

*RST value: –
SCPI: device-specific

CALCulate<n>:MARKer<m>:MAXimum:NEXT

This command positions a marker on the next smaller trace maximum.

If necessary, the corresponding marker is activated first.

This command is an event and therefore has no *RST value and no query.

Example

```
CALC:MARK2:MAX:NEXT
```

Moves marker 2 to the next smaller maximum peak.

Characteristics

*RST value: –

SCPI: device-specific

CALCulate<n>:MARKer<m>:MINimum[:PEAK]

This command positions a marker on the current trace minimum.

If necessary, the corresponding marker is activated first.

This command is an event and therefore has no *RST value and no query.

Example

```
CALC:MARK2:MIN
```

Moves marker 2 to the trace minimum.

Characteristics

*RST value: –

SCPI: device-specific

CALCulate<n>:MARKer<m>:POSition <StepSize>

This command selects the marker step size when you move the marker with the rotary knob.

Parameter

<StepSize>

CONTinuous	Moves the marker to the next pixel.
DISCrete	Moves the marker to the next measurement point.

Example

```
CALC:MARK:POS DISC
```

Selects discrete marker step size.

Characteristics

*RST value: CONTinuous

SCPI: device-specific

CALCulate<n>:MARKer<m>:X <Coordinate>

This command positions a marker on a particular coordinate on the horizontal axis.

If one or more delta markers (2 to 6) are already active, the command turns these delta markers into normal markers.

Note that it is possible to place the marker outside the visible trace. In that case, this value is invalid.

If necessary, the corresponding delta marker is activated first.

Parameter

<Coordinate>

Numeric value indicating the coordinate on the horizontal axis.

The range corresponds to the maximum span.

The unit in spectrum analyzer mode depends on the measurement, e.g. Hz for measurements in the frequency domain and seconds for measurements in the time domain.

Example

```
CALC:MARK2:X 10.7MHz
```

Positions marker 2 to frequency 10.7 MHz.

Characteristics

*RST value: –

SCPI: device-specific

CALCulate<n>:MARKer<m>:X:SLIMits[:STATe] <State>

This command turns marker search limits on and off.

If you perform a measurement in zero span, this command limits the evaluation range on the trace.

The numeric suffix at MARKer is irrelevant.

Parameter

<State>

ON | OFF

Example

```
CALC:MARK:X:SLIM ON
```

Turns on search limits.

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate<n>:MARKer<m>:X:SLIMits:LEFT <SearchLimit>

This command defines the left limit of the marker search range.

To use the command, you first have to turn on search limits with "[CALCulate<n>:MARKer<m>:X:SLIMits\[:STATe\] <State>](#)".

If you perform a measurement in zero span, this command, this command limits the evaluation range on the trace.

The numeric suffix at MARKer is irrelevant.

Parameter

<SearchLimit>

Numeric value that sets the left marker search limit.

The value range corresponds to the maximum span.

The unit in spectrum analyzer mode depends on the measurement, e.g. Hz for measurements in the frequency domain and seconds for measurements in the time domain.

Example

```
CALC:MARK:X:SLIM ON
CALC:MARK:X:SLIM:LEFT 10MHz
CALC:MARK:X:SLIM:RIGH 100MHz
```

Turns search limits on and defines a search range from 10 MHz to 100 MHz.

Characteristics

*RST value: – (is set to the left diagram border when switching on search limits)
SCPI: device-specific

CALCulate<n>:MARKer<m>:X:SLIMits:RIGHT <Searchlimit>

This command defines the right limit of the marker search range.

To use the command, you first have to turn on search limits with "[CALCulate<n>:MARKer<m>:X:SLIMits\[:STATe\] <State>](#)".

If you perform a measurement in zero span, this command, this command limits the evaluation range on the trace.

The numeric suffix at MARKer is irrelevant.

Parameter

<SearchLimit>

Numeric value that sets the right marker search limit.

The value range corresponds to the maximum span.

The unit depends on the measurement, e.g. Hz for measurements in the frequency domain and seconds for measurements in the time domain.

Example

```
CALC:MARK:X:SLIM ON
CALC:MARK:X:SLIM:LEFT 10MHz
CALC:MARK:X:SLIM:RIGH 100MHz
```

Turns search limits on and defines a search range from 10 MHz to 100 MHz.

Characteristics

*RST value: – (is set to the right diagram border when switching on search limits)

SCPI: device-specific

CALCulate<n>:MARKer<m>:Y?

This command queries the absolute vertical position of a marker.

If necessary, the corresponding marker is activated first.

To get a valid result, you have to perform a complete sweep with synchronization to the sweep end between activating the delta marker and reading out the result. This is only possible in single sweep mode.

Return values

<MarkerPosition>

numeric value of the marker position

In CAT mode, the unit depends on the measurement format.

In spectrum mode, the unit depends on "UNIT:POWer".

Example

```
INIT:CONT OFF
Switches to single sweep mode.
```

```
CALC:MARK2 ON
Switches marker 2.
```

```
INIT;*WAI
Starts a sweep and waits for the end.
```

```
CALC:MARK2:Y?
Outputs the measured value of marker 2.
```

Characteristics

*RST value: –

SCPI: device-specific

7.2.7 Using Limit Lines

The following commands define limit lines and perform the corresponding limit checks.

In cable and antenna mode, the suffix <n> at CALCulate selects the trace in split screen mode. Its range is {1..2}.

The suffix <k> at LIMit selects the limit line and is in the range <1...2>.

List of commands

- [CALCulate<n>:DLINe <Amplitude>](#) (p. 110)
- [CALCulate<n>:DLINe:STATe <State>](#) (p. 110)
- [CALCulate<n>:LIMit<k>:BEEP\[:STATe\] <State>](#) (p. 111)
- [CALCulate<n>:LIMit<k>:COMMENT?](#) (p. 111)
- [CALCulate<n>:LIMit<k>:DELeTe](#) (p. 113)
- [CALCulate<n>:LIMit<k>:FAIL?](#) (p. 113)
- [CALCulate<n>:LIMit<k>:LOWer:SElect <LimitLine>](#) (p. 113)
- [CALCulate<n>:LIMit<k>:STATe <State>](#) (p. 114)
- [CALCulate<n>:LIMit<k>:UNIT:X?](#) (p. 114)
- [CALCulate<n>:LIMit<k>:UNIT\[:Y\]?](#) (p. 115)
- [CALCulate<n>:LIMit<k>:UPPer:SElect <LimitLine>](#) (p. 115)

For a detailed description of all commands not included here, refer to "[Using Display Lines and Limit Lines](#)" in spectrum mode.

7.2.8 Configuring and Using Measurement Functions

This chapter provides information on how to configure two-port measurements with the tracking generator. The structure follows the order of the actual operation sequence used when performing a measurement:

- [Selecting the Cable Characteristics](#) on page 66
- [Selecting the Measurement Mode](#) on page 66
- [Calibrating the Measurement](#) on page 69

To perform the actual measurement, use the commands described in section "[Performing and Triggering Measurements](#)".

7.2.8.1 Selecting the Measurement Port

The following commands select the measurement port.

List of commands

- [MEASurement:PORT <Port>](#) (p. 65)

MEASurement:PORT <Port>

This command selects the measurement port.

Parameter

<Port>

Numeric value in the range from 1 to 2.

Example

```
MEAS:PORT 1
```

Selects port 1.

Characteristics

*RST value: 1

SCPI: device-specific

7.2.8.2 Selecting the Cable Characteristics

The following commands define the cable characteristics for the cable you are testing.

List of commands

- [CALCulate:DTF:CABLE:PRESet <CableModel>](#) (p. 66)

CALCulate:DTF:CABLE:PRESet <CableModel>

This command selects the cable model.

Parameter

<CableModel>

String containing the file name of the cable model.

Example

```
CALC:DTF:CAB:PRES '5088-HLFR.CBLMOD'
```

Selects the cable model from the file 5088-HLFR.CBLMOD

Characteristics

*RST value: -

SCPI: device-specific

7.2.8.3 Selecting the Measurement Mode

The following commands select the measurement mode.

List of commands

- [MEASurement:MODE <MeasMode>](#) (p. 66)

MEASurement:MODE <MeasMode>

This command selects the measurement mode.

Parameter

<MeasMode>

DTFault	Selects the distance-to-fault measurement.
LOSS	Selects the cable loss measurement.
REFlection	Selects the reflection measurement (S11)
TRANsmision	Selects the transmission measurement (S21) (R&S ZVH-K39).

Example

```
MEAS:MODE LOSS
```

Activates cable loss measurement.

Characteristics

*RST value: REFlection
 SCPI: device-specific

7.2.8.4 Selecting the Measurement Format

The following commands select the measurement format in CAT mode.

List of commands

- [CALCulate:TRACe:VSWR:MAX:STATe <State>](#) (p. 67)
- [MEASurement<n>:FORMat <MeasFormat>](#) (p. 67)

CALCulate:TRACe:VSWR:MAX:STATe <State>

This command turns the display of the maximum and average VSWR on and off.

Use [CALCulate<n>:TRACe:VSWR:AVG:RESult?](#) and
[CALCulate<n>:TRACe:VSWR:MAX:RESult?](#) to query the corresponding results.

Parameter

<State>
 ON | OFF

Example

CALC:TRAC:VSWR:MAX:STAT ON
 Displays the VSWR results.

Characteristics

*RST value: MAGNitude
 SCPI: device-specific

MEASurement<n>:FORMat <MeasFormat>

This command selects the measurement format.

Note:

For transmission measurements only the Magnitude, Phase, Magnitude+Phase and GDelay formats are available.

Parameter

LOSS	Selects the cable loss format.
MAGNitude	Selects the magnitude format.
REFlection	Selects the reflection coefficient format.
VSWR	Selects the VSWR format.

Example

```
MEAS:MODE VECT
```

Switches to vector measurement mode.

```
MEAS:FUNC:REFL ON
```

Activates reflection measurement.

```
MEAS:FORM SMIT
```

Displays the reflection in a Smith Chart.

Characteristics

*RST value: MAGNitude

SCPI: device-specific

7.2.8.5 Reading Out Measurement Results

The following commands query various measurement results.

In cable and antenna mode, the suffix <n> at CALCulate selects the trace in split screen mode. Its range is {1..2}.

List of commands

- [CALCulate:TRACe:CABLe:LOSS:RESult?](#) (p. 68)
- [CALCulate<n>:TRACe:VSWR:AVG:RESult?](#) (p. 68)
- [CALCulate<n>:TRACe:VSWR:MAX:RESult?](#) (p. 69)

CALCulate:TRACe:CABLe:LOSS:RESult?

This command queries the cable loss measurement result.

Return values

Cable loss in dB.

Example

```
CALC:TRAC:CABL:LOSS:RES?
```

Returns the cable loss.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate<n>:TRACe:VSWR:AVG:RESult?

This command queries the average VSWR measurement result.

The command is available when the calculation of the VSWR has been turned on with [CALCulate:TRACe:VSWR:MAX:STATe <State>](#).

Return value

Average VSWR (no unit)

Example

```
CALC:TRAC:VSWR:MAX:STAT ON  
CALC:TRAC:VSWR:AVG:RES?  
Queries the average VSWR.
```

Characteristics

*RST value: -
SCPI: device-specific

CALCulate<n>:TRACe:VSWR:MAX:RESult?

This command queries the maximum VSWR measurement result.

The command is available when the calculation of the VSWR has been turned on with [CALCulate:TRACe:VSWR:MAX:STATe <State>](#).

Return value

Maximum VSWR (no unit)

Example

```
CALC:TRAC:VSWR:MAX:STAT ON  
CALC:TRAC:VSWR:MAX:RES?  
Queries the maximum VSWR.
```

Characteristics

*RST value: -
SCPI: device-specific

7.2.8.6 Calibrating the Measurement

The following commands control calibration of cable measurements.

List of commands

- [CALibration:ABORT](#) (p. 70)
- [CALibration:ATTenuation:STATus?](#) (p. 70)
- [CALibration:CONTinue?](#) (p. 70)
- [CALibration:MODE?](#) (p. 71)
- [CALibration:START? <CalibrationMethod>](#) (p. 71)
- [SYSTem:PRESet:CALibration:DISCard <State>](#) (p. 72)

CALibration:ABORt

This command aborts calibration.

This command is an event and therefore has no query and no *RST value.

Example

CAL:ABOR

Aborts calibration.

Characteristics

*RST value: -

SCPI: device-specific

CALibration:ATTenuation:STATus?

This command queries the current calibration state.

This command is a query and therefore has no *RST value.

Return values

NORMALized full calibration

APPROximate approximate calibration (caused by a change of attenuation,
for example): measurement uncertainty must be anticipated

Example

CAL:STAT?

Queries the calibration status of the R&S ZVH.

Characteristics

*RST value: -

SCPI: device-specific

CALibration:CONTinue?

This command resumes calibration after a calibration standard has been connected.

After the command has been sent, it returns instructions on what to do to continue the calibration process and finish it successfully.

This command is a query and therefore has no *RST value.

Example

CAL:CONT?

Resumes calibration and would return, e.g.:

'Connect Load to Port 1'

Connect the load before resuming calibration.

Characteristics

*RST value: -
 SCPI: device-specific

CALibration:MODE?

This command queries the general current calibration state.

This command is a query and therefore has no *RST value.

Return values

0	Not calibrated
1	Calibrated

Example

CAL:MODE?
 would return, e.g.
 0

Characteristics

*RST value: -
 SCPI: device-specific

CALibration:START? <CalibrationMethod>

This command selects a calibration method and initiates calibration.

After the command has been sent, it returns instructions on what to do to continue the calibration process and finish it successfully.

This command is a query and therefore has no *RST value.

Parameter

<CalibrationMethod>

F2PCal	Full 2-Port calibration
F2PHighacc	Full 2-Port High Accuracy
S11Cal	Full 1-Port calibration
S11easy	Easy 1-Port calibration (Port 1) (CAT mode only)
S12Cal	Normalize transmission with isolation (CAT mode only)
S12Norm	Normalize transmission (CAT mode only)
S21Cal	Normalize transmission with isolation (CAT mode only)
S21Norm	Normalize transmission (CAT mode only)
S22Cal	Full 1-Port calibration
S22easy	Easy 1-Port calibration (Port 2) (CAT mode only)
T2PCal	Normalize transmission with isolation (network analysis only)
T2PNorm	Normalize transmission (CAT mode only)

Return values

<Instructions>

Connect Open to Port 1	Connect the open to port 1 before resuming calibration.
Connect Open to Port 2	Connect the open to port 2 before resuming calibration.
Connect Short to port 1	Connect the short to port 1 before resuming calibration.
Connect Short to port 2	Connect the short to port 2 before resuming calibration.
Connect Load to port 1	Connect the short to port 1 before resuming calibration.
Connect Load to port 2	Connect the short to port 2 before resuming calibration.
Connect Through	Connect a through to ports 1 and 2.
Disconnect DUT from port 1	
Disconnect DUT from port 2	
Calibration done	Calibration has been finished. No further actions required

Example

CAL:STAR? F2PCal

Selects and initiates a full 2-port calibration and would return, e.g.:

'Connect Open to Port 1'

Connect the open before resuming calibration.

Characteristics

*RST value: -

SCPI: device-specific

SYSTem:PRESet:CALibration:DISCard <State>

This command turns the mechanism that discards or keeps user calibration after a preset on and off.

Parameter

<State>

ON | OFF

Example

SYST:PRESet:CAL:DISC ON

Discards user calibration after a preset.

Characteristics

*RST value: OFF

SCPI: device-specific

7.2.8.7 Working with a DTF List

The following commands configure the DTF peak list. The peak list is available for DTF measurements only.

List of commands

- [CALCulate:TRANSform:DTFault:PEAK:COUNt?](#) (p. 73)
- [CALCulate:TRANSform:DTFault:PEAK:DATA<y>?](#) (p. 73)
- [CALCulate:TRANSform:DTFault:PEAK\[:STATe\] <State>](#) (p. 74)
- [CALCulate:TRANSform:DTFault:PEAK:THReshold <Threshold>](#) (p. 74)

CALCulate:TRANSform:DTFault:PEAK:COUNt?

This command queries the number of entries in the DTF list.

Return value

<DTFListEntries>

Example

```
CALC:TRAN:DTF:PEAK:COUN?
```

Queries the number of values in the DTF list.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:TRANSform:DTFault:PEAK:DATA<y>?

This command queries the DTF list.

This command is a query and therefore has no *RST value.

Suffix

<y>

Selects an entry in the DTF list.

Return value

<distance>,<return loss>

The number of values depends on the number of peaks that exceed the threshold you can set with [CALCulate:TRANSform:DTFault:PEAK:THReshold <Threshold>](#).

Example

```
CALC:TRAN:DTF:PEAK:RES2?
```

Reads out the second result in the DTF peak list.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:TRANSform:DTFault:PEAK[:STATe] <State>

This command turns the display of the DTF list on and off.

Parameter

ON | OFF

Example

```
CALC:TRAN:DTF:PEAK ON
```

Turns on the DTF peak list.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:TRANSform:DTFault:PEAK:THReshold <Threshold>

This commands defines the threshold for the DTF list.

All values that exceed the threshold are in the DTF list. You can query the list with [CALCulate:TRANSform:DTFault:PEAK:DATA<y>?](#).

Parameter

<Threshold>

Numeric value that sets the threshold level.

The unit depends on the measurement format.

Example

```
CALC:TRAN:DTF:PEAK:THR -20
```

Sets the threshold to -20 dB

Characteristics

*RST value: -

SCPI: device-specific

7.3 Remote Commands of the Spectrum Analyzer

This section provides a detailed description of all remote control commands required to configure and perform measurements with the spectrum analyzer. These commands are available in spectrum analyzer mode only.



Availability of remote commands for spectrum measurements

Note that the listed remote commands take effect only if you have installed option R&S ZVH-K1 and after you have entered the spectrum analyzer operating mode.

Contents

[Configuring the Horizontal Axis](#) on page 76

[Configuring the Vertical Axis](#) on page 81

[Setting the Bandwidths](#) on page 87

[Performing and Triggering Measurements](#) on page 89

[Working with Traces](#) on page 97

[Using Markers](#) on page 102

[Using Display Lines and Limit Lines](#) on page 110

[Configuring and Using Measurement Functions](#) on page 116

7.3.1 Configuring the Horizontal Axis

The following commands configure the horizontal (frequency) axis of the active display.

List of commands

- [\[SENSe:\]FREQUENCY:CENTer <Frequency>](#) (p. 36)
- [\[SENSe:\]FREQUENCY:CENTer:STEP <StepSize>](#) (p. 36)
- [\[SENSe:\]FREQUENCY:CENTer:STEP:LINK <StepSizeCoupling>](#) (p. 37)
- [\[SENSe:\]FREQUENCY:INPut:MODE <InputMode>](#) (p. 77)
- [\[SENSe:\]FREQUENCY:MODE <OperationMode>](#) (p. 78)
- [\[SENSe:\]FREQUENCY:OFFSet <FrequencyOffset>](#) (p. 78)
- [\[SENSe:\]FREQUENCY:SPAN](#) (p. 38)
- [\[SENSe:\]FREQUENCY:SPAN:AUTO <State>](#) (p. 38)
- [\[SENSe:\]FREQUENCY:SPAN:FULL](#) (p. 79)
- [\[SENSe:\]FREQUENCY:STARt <StartFrequency>](#) (p. 39)
- [\[SENSe:\]FREQUENCY:STOP <StopFrequency>](#) (p. 39)

For a detailed description of all commands not included here, refer to "[Configuring the Horizontal Axis](#)" in CAT mode.

[SENSe:]FREQUENCY:CENTer <Frequency>

This command defines the center frequency of the R&S ZVH.

In spectrum analyzer mode, the command also defines the measuring frequency for time domain measurements (span = 0).

Parameter

<Frequency>

Numeric value in Hz.

The range depends on the operating mode and is specified in the data sheet.

Example

```
FREQ:CENT 100MHz
```

Defines a center frequency of 100 MHz.

Characteristics

*RST value: $f_{\max} / 2$ with f_{\max} = maximum frequency

SCPI: conform

[SENSe:]FREQUENCY:CENTer:STEP <StepSize>

This command defines the center frequency step size.

Parameter

<StepSize>

Numeric value in Hz.

The range is from 1 Hz to f_{\max} .

Example

FREQ:CENT:STEP 120MHz
 Defines a CF step size of 120 MHz.

Characteristics

*RST value: – (AUTO 0.1*SPAN is switched on)
 SCPI: conform

[SENSe:]FREQuency:CENTer:STEP:LINK <StepSizeCoupling>

This command couples and decouples the center frequency step size to the span.

For time domain measurements, the command couples the step size to the resolution bandwidth.

Parameter

<StepSizeCoupling>

DIVTen	Couples the step size to the span (10 %).
OFF	Turns the coupling off (manual step size).

Example

FREQ:CENT:STEP:LINK DIVT
 Couples the step size to 10% of the span.

Characteristics

*RST value: DIVTen
 SCPI: device-specific

[SENSe:]FREQuency:INPut:MODE <InputMode>

This command selects the frequency mode. Select the Channel frequency mode only if you want to work with channel tables. In this case, the input of the center frequency is not a frequency value, but a channel number.

Parameter

<InputMode>

FREQuency	Sets the frequency input mode to frequency input (in Hz).
CHANnel	Sets the frequency input mode to selection of a channel.

Example

FREQ:INP:MODE CHAN
 Sets the frequency mode to work with channel tables.

Characteristics

*RST value: FREQ
 SCPI: device-specific

[SENSe:]FREQuency:MODE <OperationMode>

This command the measurement domain (frequency or time).

In the time domain (CW and FIXed), set the frequency with:

- [SENSe:]FREQuency:CENTer <Frequency>

In the frequency domain (SWEep), set it with

- [SENSe:]FREQuency:CENTer <Frequency>
- [SENSe:]FREQuency:SPAN
- [SENSe:]FREQuency:STARt <StartFrequency>
- [SENSe:]FREQuency:STOP <StopFrequency>

Parameter

<OperationMode>

CW	Selects the time domain (span = 0)
FIXed	Selects the time domain (span = 0)
SWEep	Selects the frequency domain (span > 0).

Example

```
FREQ:MODE SWE
```

Activates frequency domain measurements.

Characteristics

*RST value: SWEep

SCPI: conform

[SENSe:]FREQuency:OFFSet <FrequencyOffset>

This command defines a frequency offset.

Parameter

<FrequencyOffset>

Numeric value in the range from -100 GHz to 100 GHz.

Example

```
FREQ:OFFS 1GHZ
```

Defines a frequency offset of 1 GHz.

Characteristics

*RST value: 0 Hz

SCPI: conform

**[SENSe:]FREQuency:SPAN **

This command defines the frequency span.

If you set a span of 0 Hz in spectrum mode, the R&S ZVH starts a measurement in the time domain.

Parameter

Numeric value in Hz. The value range is specified in the data sheet.

Example

```
FREQ:SPAN 10MHz
```

Defines a span of 10 MHz.

Characteristics

*RST value: f_{\max} with f_{\max} = maximum frequency

SCPI: conform

[SENSe:]FREQuency:SPAN:AUTO <State>

This command turns the automatic calculation of the ideal span on and off.

Parameter

<State>

ON | OFF

Example

```
FREQ:SPAN:AUTO ON
```

Turns automatic span determination on and off.

Characteristics

*RST value: OFF

SCPI: device-specific

[SENSe:]FREQuency:SPAN:FULL

This command restores the full span.

This command is an event and therefore has no query and no *RST value.

Example

```
FREQ:SPAN:FULL
```

Restores full span.

Characteristics

*RST value: –

SCPI: conform

[SENSe:]FREQuency:STARt <StartFrequency>

This command defines the start frequency for measurements in the frequency domain (span > 0).

Parameter

<StartFrequency>

Numeric value in Hz.

The range depends on the operating mode and is specified in the datasheet.

Example

```
FREQ:STAR 20MHz
```

Defines a start frequency of 20 MHz.

Characteristics

*RST value: 0

SCPI: conform

[SENSe:]FREQuency:STOP <StopFrequency>

This command defines the stop frequency for measurements in the frequency domain (span > 0).

Parameter

<StopFrequency>

Numeric value in Hz.

The range depends on the operating mode and is specified in the datasheet.

Example

```
FREQ:STOP 2000MHz
```

Defines a stop frequency of 2 GHz

Characteristics

*RST value: f_{\max}

SCPI: conform

7.3.2 Configuring the Vertical Axis

The following commands configure the vertical (level) axis and level parameters of the active display.

The suffix <n> at TRACe is irrelevant for these commands.

The suffix <c> at TRANsducer selects the primary or secondary transducer. The range is <1...2>.

List of commands

- [DISPlay\[:WINDow\]:TRACe<n>:Y\[:SCALe\]:ADJust](#) (p. 41)
- [DISPlay\[:WINDow\]:TRACe<n>:Y:SPACing <Scaling>](#) (p. 81)
- [DISPlay\[:WINDow\]:TRACe<n>:Y\[:SCALe\] <DisplayRange>](#) (p. 82)
- [DISPlay\[:WINDow\]:TRACe<n>:Y\[:SCALe\]:RLEVel <ReferenceLevel>](#) (p. 82)
- [DISPlay\[:WINDow\]:TRACe<n>:Y\[:SCALe\]:RLEVel:OFFSet <Offset>](#) (p. 82)
- [DISPlay\[:WINDow\]:TRACe<n>:Y\[:SCALe\]:RPOSition <ReferencePosition>](#) (p. 83)
- [INPut:ATTenuation <Attenuation>](#) (p. 45)
- [INPut:ATTenuation:MODE <AttenuationMode>](#) (p. 83)
- [INPut:ATTenuation:AUTO <State>](#) (p. 84)
- [INPut:GAIN:STATe <State>](#) (p. 84)
- [INPut:IMPedance <Impedance>](#) (p. 84)
- [\[SENSe:\]CORRection:TRANsducer<c>\[:STATe\] <State>](#) (p. 85)
- [\[SENSe:\]CORRection:TRANsducer<c>:SELEct <TransducerFactor>](#) (p. 85)
- [\[SENSe:\]CORRection:TRANsducer<c>:UNIT?](#) (p. 85)
- [UNIT:POWer <Unit>](#) (p. 86)

For a detailed description of all commands not included here, refer to "[Configuring the Vertical Axis](#)" in CAT mode.

DISPlay[:WINDow]:TRACe<n>:Y:SPACing <Scaling>

This command selects the scaling of the vertical axis.

Parameter

<Scaling>

LOGarithmic	Selects a logarithmic scale.
LINear	Selects a linear scale (%).

Example

```
DISP:TRAC:Y:SPAC LIN
```

Selects linear scaling of the level axis.

Characteristics

*RST value: LOGarithmic
SCPI: conform

DISPlay[:WINDow]:TRACe<n>:Y[:SCALe] <DisplayRange>

This command defines the display range of the vertical axis.

Note that you have to set a logarithmic scaling before you can use this command with `DISPlay[:WINDow]:TRACe<n>:Y:SPACing`. For a linear scale, you can not modify the display range as it is fixed.

Parameter

<DisplayRange>

numeric value in the range from 10 dB to 200 dB

Example

```
DISP:TRAC:Y 110dB
```

Sets the display range to 110 dB.

Characteristics

*RST value: 100dB

SCPI: device-specific

DISPlay[:WINDow]:TRACe<n>:Y[:SCALe]:RLEVel <ReferenceLevel>

This command defines the reference level.

With a reference level offset $\neq 0$, the value range of the reference level is modified by the offset.

Parameter

<ReferenceLevel>

numeric value that sets the reference level; the unit depends on `UNIT:POWer`.

The available value range is specified in the data sheet.

Example

```
DISP:TRAC:Y:RLEV -60dBm
```

Sets the reference level to -60 dBm.

Characteristics

*RST value: -20dBm

SCPI: conform

DISPlay[:WINDow]:TRACe<n>:Y[:SCALe]:RLEVel:OFFSet <Offset>

This command defines a reference level offset.

Parameter

<Offset>

numeric value (dB) that sets the reference level offset

The available value range is from -200dB to 200dB.

Example

```
DISP:TRAC:Y:RLEV:OFFS -10dB
```

Characteristics

*RST value: 0dB

SCPI: conform

DISPlay[:WINDow]:TRACe<n>:Y[:SCALe]:RPOSition <ReferencePosition>

This command defines the position of the reference level on the display grid.

First, you have to set a logarithmic scale for the vertical axis with `DISPlay[:WINDow]:TRACe<n>:Y:SPACing`. For a linear scale, you can not modify the reference position.

Parameter

<ReferencePosition>

numeric value (%) that defines the reference position

The available value range is from 1 to 10.

Example

```
DISP:TRAC:Y:RPOS 5
```

Sets the reference position to the 5th grid line.

Characteristics

*RST value:10

SCPI: conform

INPut:ATTenuation:MODE <AttenuationMode>

This command selects the attenuation mode.

Parameter

<AttenuationMode>

LDISortion	Selects "Auto Low Distortion" mode.
LNOise	Selects "Auto Low Noise" mode.

Example

```
INP:ATT:MODE LNO
```

Sets the attenuation mode to Auto Low Noise.

Characteristics

*RST value: LNOise

SCPI: device-specific

INPut:ATTenuation:AUTO <State>

This command couples and decouples input attenuation to the reference level.

Parameter

<State>
ON | OFF

Example

INP:ATT:AUTO ON

Couples the attenuation set on the attenuator to the reference level.

Characteristics

*RST value: ON
SCPI: conform

INPut:GAIN:STATe <State>

This command turns the preamplifier on and off.

Parameter

<State>
ON | OFF

Example

INP:GAIN:STAT ON

Activates the preamplifier

Characteristics

*RST value: OFF
SCPI: conform

INPut:IMPedance <Impedance>

This command selects the nominal input impedance. The set impedance is taken into account in all level indications of results.

The setting $75\ \Omega$ should be selected, if the $50\ \Omega$ input impedance is transformed to a higher impedance using a $75\ \Omega$ adapter of the RAZ type (= $25\ \Omega$ in series to the input impedance of the instrument). The correction value in this case is $1.76\ \text{dB} = 10 \log (75\ \Omega / 50\ \Omega)$.

Parameter

<Impedance>
50 | 75

Example

INP:IMP 75

Sets the input impedance to 75 Ohm.

Characteristics

*RST value: 50 Ω

SCPI: conform

[SENSe:]CORRection:TRANsducer<c>[:STATe] <State>

This command turns a transducer factor on and off.

Before turning it on, you have to select a transducer factor with
[SENSe:]CORRection:TRANsducer<c>:SElect.

Parameter

<State>

ON | OFF

Example

CORR:TRAN1 ON

Activates the primary transducer

Characteristics

*RST value: OFF

SCPI: device-specific

[SENSe:]CORRection:TRANsducer<c>:SElect <TransducerFactor>

This command selects a transducer factor.

If <name> does not exist yet, a new transducer factor is created.

The suffix<1...2> specifies the primary or secondary transducer.

Parameter

<Transducerfactor>

string containing the file name of the transducer factor.

If the file does not exist, the R&S ZVH creates a new transducer factor.

Example

CORR:TRAN2:SEL 'FSH-Z38.sectrd'

Selects the FSH-Z38 secondary transducer factor.

Characteristics

*RST value: -

SCPI: device-specific

[SENSe:]CORRection:TRANsducer<c>:UNIT?

This command queries the unit of the current transducer factor.

Example

CORR:TRAN2:UNIT?

Queries the unit of the primary transducer.

Characteristics

*RST value: -
SCPI: device-specific

UNIT:POWer <Unit>

This command selects the unit of the vertical axis.

The availability of units depends on the operating mode and type of measurement.

Parameter

<Unit>

DBM | DBUV | DBMV | V | W | DUVM | DUAM | V_M | W_M2

Note that the availability of units depends on the operating mode.

Example

```
UNIT:POW DBUV
```

Sets the power unit to dB μ V.

Characteristics

*RST value: DBM
SCPI: conform

7.3.3 Setting the Bandwidths

The following commands configure the filter bandwidths of the R&S ZVH. Note that both groups of commands (BANDwidth and BWIDth) are the same.

List of commands

- [\[SENSe:\]BANDwidth|BWIDth\[:RESolution\] <ResBW>](#) (p. 87)
- [\[SENSe:\]BANDwidth|BWIDth\[:RESolution\]:AUTO <State>](#) (p. 87)
- [\[SENSe:\]BANDwidth|BWIDth:VIDeo <VideoBW>](#) (p. 88)
- [\[SENSe:\]BANDwidth|BWIDth:VIDeo:AUTO <State>](#) (p. 88)

[SENSe:]BANDwidth|BWIDth[:RESolution] <ResBW>

This command defines the resolution bandwidth.

Parameter

<ResBW>

Numeric value in Hz.

The available value range is from 1 Hz to 3 MHz in 1 - 3 - 10 steps. In addition, you can select a 200 kHz and 5 MHz bandwidth.

In zero span, the R&S ZVH also provides a 10 MHz and 20 MHz bandwidth.

Example

```
BAND 100 kHz
```

Sets the resolution bandwidth to 100 kHz

Characteristics

*RST value: - (AUTO is set to ON)

SCPI: conform

[SENSe:]BANDwidth|BWIDth[:RESolution]:AUTO <State>

This command couples and decouples the resolution bandwidth to the span.

Parameter

<State>

ON | OFF

Example

```
BAND:AUTO OFF
```

Decouples the resolution bandwidth from the span.

Characteristics

*RST value: ON

SCPI: conform

[SENSe:]BANDwidth|BWIDth:VIDeo <VideoBW>

This command defines the video bandwidth.

Parameter

<VideoBW>

Numeric value in Hz.

The available value range is from 1 Hz to 3 MHz in 1 - 3 steps.

Example

```
BAND:VID 10kHz
```

Sets the video bandwidth to 10 kHz.

Characteristics

*RST value: - (AUTO is set to ON)

SCPI: conform

[SENSe:]BANDwidth|BWIDth:VIDeo:AUTO <State>

This command couples and decouples the video bandwidth to the resolution bandwidth.

Parameter

<State>

ON | OFF

Example

```
BAND:VID:AUTO OFF
```

Turns off video bandwidth coupling.

Characteristics

*RST value: ON

SCPI: conform

7.3.4 Performing and Triggering Measurements

The following commands control the actual measurement process, including trigger functionality.

7.3.4.1 Performing the Measurement

The following commands initialize a measurement and set up the sweep.

List of commands

- [*WAI](#) (p. 34)
- [ABORt](#) (p. 89)
- [INITiate\[:IMMediate\]](#) (p. 89)
- [INITiate:CONTinuous <SweepMode>](#) (p. 90)
- [\[SENSe:\]SWEep:COUNt <SweepCount>](#) (p. 90)
- [\[SENSe:\]SWEep:POINts?](#) (p. 91)
- [\[SENSe:\]SWEep:TIME <SweepTime>](#) (p. 91)
- [\[SENSe:\]SWEep:TIME:AUTO <State>](#) (p. 91)

ABORt

This command aborts the current measurement and resets the trigger system.

This command is an event and therefore has no query and no *RST value.

Example

```
ABOR;
```

```
INIT:IMM
```

Aborts a measurement and starts a new one.

Characteristics

RST value: –

SCPI: conform

INITiate[:IMMediate]

The command initiates a new measurement sequence.

With sweep count > 0 or average count > 0, this means a restart of the indicated number of measurements. With trace functions MAXHold, MINHold and AVERage, the previous results are reset on restarting the measurement.

In single sweep mode, synchronization to the end of the indicated number of measurements can be achieved with the command *OPC, *OPC? or *WAI. In continuous-sweep mode, synchronization to the sweep end is not possible since the overall measurement never ends.

This command is an event and therefore has no query and no *RST value.

Example

```
INIT:CONT OFF
DISP:WIND:TRAC:MODE AVER
```

Turns single sweep mode and trace averaging on.

```
INIT;*WAI
```

Starts the measurement and waits for the end of the sweep.

Characteristics

*RST value: –
SCPI: conform

INITiate:CONTinuous <SweepMode>

This command selects the sweep mode.

Parameter

<SweepMode>

ON	Selects continuous sweeps.
OFF	Selects single sweep.

Example

```
INIT:CONT OFF
```

Turns on single sweep mode.

Characteristics

*RST value: ON
SCPI: conform

[SENSe:]SWEep:COUNt <SweepCount>

This command defines the number of sweeps included in a single sweep. It also defines the number of sweeps the R&S ZVH uses to average traces or calculate maximum values.

The R&S ZVH performs one sweep for sweep count 0 or 1.

Parameter

<SweepCount>
0 to 999

Example

```
SWE:COUN 64
```

Defines a sweep count of 64 sweeps.

```
INIT:CONT OFF
INIT;*WAI
```

Turns on single sweep mode, starts the sweep and waits for its end.

Characteristics

*RST value: 1

SCPI: conform

[SENSe:]SWEep:POINts?

This command queries the number of measurement points in a single sweep.

This command is a query and therefore has no *RST value.

Return value

Number of sweep points.

Example

SWE:POIN?

Returns the number of sweep points.

Characteristics

*RST value: –

SCPI: conform

[SENSe:]SWEep:TIME <SweepTime>

This command defines the sweep time.

If you set a sweep time in spectrum mode with this command, the R&S ZVH decouples the sweep time from the span and the resolution and video bandwidths.

Parameter

<SweepTime>

Numeric value in seconds.

The available value range is specified in the datasheet.

Example

SWE:TIME 10s

Sets the sweep time to 10 s

Characteristics

*RST value: - (AUTO is set to ON)

SCPI: conform

[SENSe:]SWEep:TIME:AUTO <State>

This command couples and decouples the sweep time to the span and the resolution and video bandwidths.

Parameter

<State>

ON | OFF

Example

```
SWE:TIME:AUTO ON
```

Switches on the coupling to frequency span and bandwidths.

Characteristics

*RST value: ON

SCPI: conform

7.3.4.2 Capturing I/Q Data

The following commands control I/Q data capture.

List of commands

- [TRACe:IQ:DATA:MEMory? \[<OffsetSamples>,<Samples>\]](#) (p. 92)
- [TRACe:IQ:RLENgth <Samples>](#) (p. 93)
- [TRACe:IQ:SRATe <SampleRate>](#) (p. 93)
- [TRACe:IQ\[:STATe\] <State>](#) (p. 93)

TRACe:IQ:DATA:MEMory? [<OffsetSamples>,<Samples>]

This command queries the I/Q data in the capture buffer.

By default, it returns all samples in the capture buffer. You can, however, narrow down the amount of data that the command returns using the optional parameters.

This command is a query and therefore has no *RST value.

Parameter

<OffsetSamples>

Defines the first sample to return in relation to the first sample in the capture buffer.

<Samples>

Defines the number of samples to return.

Return value

<IQData>

Measured value pair (I,Q) for each sample that has been recorded. The order is I,I,I,I,...,Q,Q,Q,Q,...

Example

```
TRAC:IQ ON
```

Turn on I/Q data capture.

```
TRAC:IQ:RLEN 10000
```

```
TRAC:IQ:SRAT 1000000
```

Capture 10000 samples with 1 MHz sample rate.

```
INIT:CONT OFF
```

```
INIT;*WAI
```

Selects single sweep and initiate measurement.

```
TRAC:IQ:DATA:MEM? 1000,5000
```

Queries 5000 samples, beginning with the 1000th sample.

Characteristics

*RST value: -

SCPI: device-specific

TRACe:IQ:RLENgth <Samples>

This command defines the number of samples to capture.

Parameter

<Samples>

Number of samples in the range from 1 to 524288.

Example

```
TRAC:IQ:RLEN 10000
```

Capture 10000 samples.

*RST value: 1000

SCPI: device-specific

TRACe:IQ:SRATe <SampleRate>

This command defines the sample rate.

The maximum sample rate depends on the instrument variant you have. It is either 38.4 MHz or 15 MHz.

Parameter

<SampleRate>

Sample rate in Hz.

Example

```
TRAC:IQ:SRAT 1000000
```

Define a 1 MHz sample rate.

```
TRAC:IQ:SRAT MAX
```

```
TRAC:IQ:SRAT?
```

Query maximum sample rate

*RST value: 10 MHz

SCPI: device-specific

TRACe:IQ[:STATe] <State>

This command turns I/Q capture mode on and off.

Parameter

<State>

ON | OFF.

Example

```
TRAC:IQ ON
```

Turn on I/Q capture mode.

*RST value: OFF

SCPI: device-specific

7.3.4.3 Triggering Measurements

The following commands set up trigger conditions if you are using a trigger for the measurement.

List of commands

- [\[SENSe:\]SWEep:EGATe <State>](#) (p. 94)
- [\[SENSe:\]SWEep:EGATe:HOLDoff <GateDelay>](#) (p. 94)
- [\[SENSe:\]SWEep:EGATe:LENGth <GateLength>](#) (p. 95)
- [\[SENSe:\]SWEep:EGATe:TIME <SweepTime>](#) (p. 95)
- [TRIGger\[:SEQuence\]:HOLDoff\[:TIME\] <TriggerDelay>](#) (p. 48)
- [TRIGger\[:SEQuence\]:LEVel:VIDeo <TriggerLevel>](#) (p. 95)
- [TRIGger\[:SEQuence\]:SLOPe <TriggerSlope>](#) (p. 49)
- [TRIGger\[:SEQuence\]:SOURce <TriggerSource>](#) (p. 96)

For a detailed description of all commands not included here, refer to "[Triggering Measurements](#)" in CAT mode.

[SENSe:]SWEep:EGATe <State>

This command turns a gated trigger on and off.

Parameter

<State>

ON | OFF

Example

```
SWE:EGAT ON
```

Activates the gated trigger.

Characteristics

*RST value: off

SCPI: device-specific

[SENSe:]SWEep:EGATe:HOLDoff <GateDelay>

This command defines the length of the gate delay.

Parameter

<GateDelay>

Numeric value in the range from 0 s to 100 s.

Example

```
SWE:EGAT:HOLD 2.5
```

Sets a gate delay of 2.5 seconds.

Characteristics

*RST value: 0 s

SCPI: device-specific

[SENSe:]SWEep:EGATe:LENGth <GateLength>

This command defines the gate length.

Parameter

<GateLength>

Numeric value in the range from 10 μ s to 100 s.

Example

```
SWE:EGAT:LENG 2.5
```

Sets a gate length of 2.5 seconds.

Characteristics

*RST value: 400 μ s

SCPI: device-specific

[SENSe:]SWEep:EGATe:TIME <SweepTime>

This command defines the sweep time for the gated trigger.

Parameter

<SweepTime>

Numeric value in seconds.

Example

```
SWE:GATE:TIME 4ms
```

Sets a sweep time of 4 ms for the gated trigger.

Characteristics

*RST value: 400 μ s

SCPI: device-specific

TRIGger[:SEQuence]:LEVel:VIDeo <TriggerLevel>

This command defines the level of the video trigger.

Video trigger is available for time domain measurements (span = 0).

Parameter

<TriggerLevel>

Numeric value in the range from 0 % to 100 %.

Example

```
TRIG:LEV:VID 50PCT
```

Sets the trigger level to 50%.

Characteristics

*RST value: 50 PCT

SCPI: device-specific

TRIGger[:SEquence]:SOURce <TriggerSource>

This command selects the trigger source.

Parameter

<TriggerSource>

IMMediate	Selects Free Run measurements.
EXTernal	Selects an external trigger.
VIDeo	Selects the video trigger.

For more information see R&S ZVH operating manual chapter "Setting the Sweep"

Example

```
TRIG:SOUR EXT
```

Selects the external trigger input as source of the trigger signal

Characteristics

*RST value: IMMediate

SCPI: conform

7.3.5 Working with Traces

The following commands set up the trace and the various functions associated with it, e.g. trace mathematics or the selection of the detector.

The suffix <n> in the following commands is irrelevant.

List of commands

- `CALCulate:MATH<n> [:EXPRession][:DEFine] <Expression>` (p. 97)
- `CALCulate:MATH<n>:COPY:MEMory` (p. 50)
- `CALCulate:MATH<n>:STATe <State>` (p. 98)
- `DISPlay[:WINDow]:TRACe<n> [:STATe] <State>` (p. 98)
- `DISPlay[:WINDow]:TRACe<n>:MEMory[:STATe] <State>` (p. 50)
- `DISPlay[:WINDow]:TRACe<n>:MODE <TraceMode>` (p. 98)
- `FORMat:BORDER <ByteOrder>` (p. 99)
- `[SENSe:]DETEctor<n> [:FUNCTion] <Detector>` (p. 99)
- `[SENSe:]DETEctor<n> [:FUNCTion]:AUTO <State>` (p. 100)
- `TRACe<n> [:DATA]? <Destination>` (p. 100)
- `TRACe<n>:DATA:MEMory? <Trace>` (p. 53)
- `FORMat[:DATA] <DataFormat>` (p. 101)

For a detailed description of all commands not included here, refer to "[Working with Traces](#)" in CAT mode.

`CALCulate:MATH<n> [:EXPRession][:DEFine] <Expression>`

This command defines the mathematical expression for relating traces to trace 1.

You have to activate trace mathematics with `CALCulate:MATH<n>:STATe <State>` first.

Parameter

<Expression>

(IMPLied - memory)	Subtracts the trace in memory from the current trace.
(memory - IMPLied)	Subtracts the current trace from the trace in memory.

Example

```
CALC:MATH (MTRACE-TRACE)
```

Selects the subtraction of the current trace from trace in the memory.

Characteristics

*RST value: –
SCPI: conform

CALCulate:MATH<n>:STATe <State>

This command turns trace mathematics on and off.

Parameter

<State>
ON | OFF

Example

CALC:MATH:STAT ON
Switches on the trace mathematics.

Characteristics

*RST value: OFF
SCPI: conform

DISPlay[:WINDow]:TRACe<n> [:STATe] <State>

This command turns a trace on and off.

Parameter

<State>
ON | OFF

Example

DISP:TRAC2 ON
Turns the trace on.

Characteristics

*RST value: ON for TRACe1, OFF for TRACe2
SCPI: conform

DISPlay[:WINDow]:TRACe<n>:MODE <TraceMode>

This command selects the trace mode.

If you are using the average, max hold or min hold trace mode, you can set the number of measurements with [SENSe:]SWEep:COUNT <SweepCount>. Note that synchronization to the end of the average count is possible only in single sweep mode.

Parameter

<TraceMode>
AVERage | MAXHold | MINHold | VIEW | WRITe

You can turn off the trace with `DISPlay[:WINDow]:TRACe<n> [:STATe] <State>`.

For more information see the operating manual, chapter "Trace Mode".

Example

```
INIT:CONT OFF
```

```
SWE:COUN 16
```

Turn on single sweep mode and sets the number of measurements to 16.

```
DISP:TRAC:MODE MAXH
```

Activates MAXHold mode for the trace.

```
INIT;*WAI
```

Starts the measurement and waits for the end of the 16 sweeps.

Characteristics

*RST value: WRITe

SCPI: device-specific

FORMat:BORDER <ByteOrder>

This command selects the format of binary data.

Parameters

<ByteOrder>

SWAPped	The least significant byte is transferred first (little endian).
NORMal	The most significant byte is transferred first big endian).

Example

```
FORM:BORD NORM
```

Changes the byte order to normal mode

Characteristics

*RST value SWAPped

SCPI: conform

[SENSe:]DETEctor<n> [:FUNCTion] <Detector>

This command selects the detector.

Parameter

<Detector>

APEak | NEGative | POSitive | SAMPlE | RMS

For more information see the operating manual, chapter "Detectors".

Example

```
DET POS
```

Sets the detector to "positive peak".

Characteristics

*RST value: POS

SCPI: conform

[SENSe:]DETEctor<n> [:FUNctioN]:AUTO <State>

This command couples and decouples the detector to the trace mode.

Parameter

<State>
ON | OFF

Example

DET:AUTO OFF
Turns off automatic detector selection.

Characteristics

*RST value: ON
SCPI: conform

TRACe<n> [:DATA]? <Destination>

This command queries the trace data of the current measurement.

It also transfers data from a file to a particular trace.

With `FORMat[:DATA] <DataFormat>` command, you can set the data format.

Parameter

<Destination>

TRACE1	Queries the data of trace 1.
TRACE2	Queries the data of trace 2.
LIST	Queries the peak list of the measurement.

Return value

The R&S ZVH returns 631 values. Each value corresponds to one pixel of a trace.

The unit depends on the measurement and the unit you have set with
`UNIT:POWer <Unit>`.

Note:

If you use the auto peak detector, the command reads out positive peak values only.

Example

TRAC:DATA? TRACE1
Reads out the data for trace 1

Characteristics

*RST value: -
SCPI: conform

FORMat[:DATA] <DataFormat>

This command selects the data format that is used for transmission of trace data from the R&S ZVH to the controlling computer.

Note that the command has no effect for data that you send to the R&S ZVH. The R&S ZVH automatically recognizes the data it receives, regardless of the format.

Parameter

<DataFormat>

ASCii	Returns the data in ASCII format, separated by commas.
REAL,32	Returns the data as 32-bit IEEE 754 floating point numbers in the "definite length block format".

In REAL,32 format, a string of return values would look like:

#42524<value 1><value 2>...<value n>

with

#4	Number of digits of the following number of data bytes (= 4 in this example)
2524	Number of following data bytes (2524, corresponds to the 631 sweep points of the R&S ZVH).
<value>	4-byte floating point value

Example

FORM ASC

Selects the ASCII data format.

Characteristics

*RST value: ASCII

SCPI: conform

7.3.6 Using Markers

- [Markers and Delta Markers](#) on page 102
- [Marker Functions](#) on page 102

7.3.6.1 Markers and Delta Markers

The following commands are for setting and controlling markers and deltamarkers.

In spectrum mode mode, the suffix <n> at CALCulate selects the trace.

The suffix <m> at MARKer is in the range {1..6} and selects the marker or deltamarker.

List of commands

- [CALCulate<n>:DELTamarker<m>\[:STATe\] <State>](#) (p. 55)
- [CALCulate<n>:DELTamarker<m>:AOFF](#) (p. 56)
- [CALCulate<n>:DELTamarker<m>:MAXimum\[:PEAK\]](#) (p. 56)
- [CALCulate<n>:DELTamarker<m>:MAXimum:NEXT](#) (p. 56)
- [CALCulate<n>:DELTamarker<m>:MINimum\[:PEAK\]](#) (p. 56)
- [CALCulate<n>:DELTamarker<m>:X <Coordinate>](#) (p. 57)
- [CALCulate<n>:DELTamarker<m>:X:RELative <Distance>](#) (p. 57)
- [CALCulate<n>:DELTamarker<m>:Y?](#) (p. 58)
- [CALCulate<n>:MARKer<m>\[:STATe\] <State>](#) (p. 59)
- [CALCulate<n>:MARKer<m>:AOFF](#) (p. 59)
- [CALCulate<n>:MARKer<m>:MAXimum\[:PEAK\]](#) (p. 59)
- [CALCulate<n>:MARKer<m>:MAXimum:NEXT](#) (p. 60)
- [CALCulate<n>:MARKer<m>:MINimum\[:PEAK\]](#) (p. 60)
- [CALCulate<n>:MARKer<m>:X <Coordinate>](#) (p. 61)
- [CALCulate<n>:MARKer<m>:X:SLIMits\[:STATe\] <State>](#) (p. 61)
- [CALCulate<n>:MARKer<m>:X:SLIMits:LEFT <SearchLimit>](#) (p. 62)
- [CALCulate<n>:MARKer<m>:X:SLIMits:RIGHT <Searchlimit>](#) (p. 62)
- [CALCulate<n>:MARKer<m>:Y?](#) (p. 63)

For a detailed description of all commands not included here, refer to "[Using Markers](#)" in CAT mode.

7.3.6.2 Marker Functions

The following commands perform various kinds of analysis at the marker position.

The suffix <m> at MARKer is irrelevant, except where noted.

List of commands

- [CALCulate:MARKer<m>:COUNT:FREQuency?](#) (p. 103)
- [CALCulate:MARKer<m>:COUNT:RESolution:MODE <Resolution>](#) (p. 103)
- [CALCulate:MARKer<m>:COUNT\[:STATe\] <State>](#) (p. 104)
- [CALCulate:MARKer<m>:FREQuency:MODE <InputMode>](#) (p. 104)
- [CALCulate:MARKer<m>:FUNCTion:CENTer](#) (p. 105)
- [CALCulate:MARKer<m>:FUNCTion:DEModulation\[:STATe\] <State>](#) (p. 105)
- [CALCulate:MARKer<m>:FUNCTion:DEModulation:HOLDoff <Time>](#) (p. 105)

- [CALCulate:MARKer<m>:FUNCTION:DEModulation:SElect <Demodulation>](#) (p.106)
- [CALCulate:MARKer<m>:FUNCTION:NDBDown <Distance>](#) (p. 106)
- [CALCulate:MARKer<m>:FUNCTION:NDBDown:FREQuency?](#) (p. 106)
- [CALCulate:MARKer<m>:FUNCTION:NDBDown:RESult?](#) (p. 107)
- [CALCulate:MARKer<m>:FUNCTION:NDBDown:STATe <State>](#) (p. 107)
- [CALCulate:MARKer<m>:FUNCTION:NOISe\[:STATe\] <State>](#) (p. 108)
- [CALCulate:MARKer<m>:FUNCTION:NOISe:RESult?](#) (p. 108)
- [CALCulate:MARKer<m>:FUNCTION:REFerence](#) (p. 109)

CALCulate:MARKer<m>:COUNT:FREQuency?

This command performs a frequency measurement at the marker position and returns the result.

To get a valid result, you have to perform a complete sweep with synchronization to the sweep end to make sure that the R&S ZVH actually reaches the frequency you want to measure. This is only possible in single sweep mode.

Before you can use the command, you have to turn on the frequency counter with [CALCulate:MARKer<m>:COUNT\[:STATe\] <State>](#).

Example

See [CALCulate:MARKer<m>:COUNT\[:STATe\] <State>](#).

Characteristics

*RST value: –
SCPI: device-specific

CALCulate:MARKer<m>:COUNT:RESolution:MODE <Resolution>

This command selects the resolution of the frequency counter.

Parameter

<State>
HIGH | LOW

Parameter

<Resolution>

HIGH	Frequency counter resolution 0.1 mHz.
LOW	Frequency counter resolution: 0.1 Hz.

Example

See [CALCulate:MARKer<m>:COUNT\[:STATe\] <State>](#).

Characteristics

*RST value: –
SCPI: device-specific

CALCulate:MARKer<m>:COUNT[:STATE] <State>

This command turns the frequency counter at the marker position on and off.

You can read out the result with `CALCulate:MARKer<m>:COUNT:FREQuency?`.

Frequency counting is possible only for one marker at a time. If it is activated for another marker, it is automatically deactivated for the previous marker.

To get a valid result, you have to perform a complete sweep with synchronization to the sweep end to make sure that the R&S ZVH actually reaches the frequency you want to measure. This is only possible in single sweep mode.

The suffix <m> selects the marker.

Parameter

<State>

ON | OFF

Example

```
INIT:CONT OFF
```

```
CALC:MARK ON
```

Turns on single sweep mode and marker 1.

```
CALC:MARK:COUN ON
```

Turns on the frequency counter for marker 1.

```
INIT;*WAI
```

```
CALC:MARK:COUN:FREQ?
```

Performs a measurement and queries the results of the frequency counter.

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate:MARKer<m>:FREQuency:MODE <InputMode>

This command selects the marker frequency display mode.

Parameter

<InputMode>

FREQuency	Sets the marker frequency mode to frequency input (in Hz).
CHANnel	Sets the marker frequency mode to channel input (as a channel number).

Example

```
CALC:MARK:FREQ:MODE FREQ
```

Selects the frequency display mode.

Characteristics

*RST value: FREQ

SCPI: device-specific

CALCulate:MARKer<m>:FUNCtion:CENTer

This command matches the center frequency to the frequency of a marker

If you use a delta marker, the R&S ZVH turns it into a normal marker.

The suffix <m> selects the marker.

This command is an event and therefore has no *RST value and no query.

Example

```
CALC:MARK1:FUNC:CENT
```

Matches the center frequency to the frequency of marker 1.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:MARKer<m>:FUNCtion:DEModulation[:STATe] <State>

This command turns the audio demodulator on and off when the measurement hits a marker position.

With a span greater than 0, you can define a hold time at the marker position with `CALCulate:MARKer<m>:FUNCtion:DEModulation:HOLDoff <Time>`.

In zero span the demodulation is on permanently.

Parameter

<State>

ON | OFF

Example

```
CALC:MARK3:FUNC:DEM ON
```

Switches on the demodulation for marker 3.

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate:MARKer<m>:FUNCtion:DEModulation:HOLDoff <Time>

This command defines the hold time at the marker position for the demodulation with span > 0.

Parameter

<Time>

Numeric value in the range from 10 ms to 500 s.

Example:

```
CALC:MARK:FUNC:DEM:HOLD 3s
```

Sets a hold time of 3 seconds.

Characteristics:

*RST value: – (DEModulation is set to OFF)

SCPI: device-specific

CALCulate:MARKer<m>:FUNCTION:DEModulation:SElect <Demodulation>

This command selects the type of demodulation type for the audio demodulator.

Parameter

<Demodulation>

AM | FM

Example

CALC:MARK:FUNC:DEM:SEL FM

Selects FM demodulation.

Characteristics

*RST value: AM

SCPI: device-specific

CALCulate:MARKer<m>:FUNCTION:NDBDown <Distance>

This command defines the distance of the n dB down markers to the reference marker.

Parameter

<Distance>

Distance of the temporary markers to the reference marker in dB.

Example

See CALCulate:MARKer<m>:FUNCTION:NDBDown:STATE <State>

Characteristics

*RST value: 3 dB

SCPI: device-specific

CALCulate:MARKer<m>:FUNCTION:NDBDown:FREQuency?

This command queries the horizontal position of the n dB down markers.

Return value

<frequency1>	Absolute frequency of the n dB marker to the left of the reference marker in Hz.
<frequency2>	Absolute frequency of the n dB marker to the right of the reference marker in Hz.

Example

See CALCulate:MARKer<m>:FUNCTION:NDBDown:STATE <State>

Characteristics

*RST value: -
 SCPI: device-specific

CALCulate:MARKer<m>:FUNCTION:NDBDown:RESult?

This command queries the frequency spacing or bandwidth of the n dB down markers.

Return value

<Bandwidth>
 Bandwidth in Hz.

Example

See `CALCulate:MARKer<m>:FUNCTION:NDBDown:STATe <State>`

Characteristics

*RST value: -
 SCPI: device-specific

CALCulate:MARKer<m>:FUNCTION:NDBDown:STATe <State>

This command turns the n dB Down marker function on and off.

Parameter

<State>
 ON | OFF

Example

`CALC:MARK:FUNC:NDBD:STAT ON`
 Turns on the n dB marker function.

`CALC:MARK:FUNC:NDBD 3`
 Positions two temporary markers 3 dB below a reference marker.

`CALC:MARK:FUNC:NDBD:FREQ?`
 Queries the frequency position of the n dB Down markers; would return e.g.
 100000000,200000000

`CALC:MARK:FUNC:NDBD:RES?`
 Queries the measurement result; would return e.g.
 100000000

Characteristics

*RST value: OFF
 SCPI: device-specific

CALCulate:MARKer<m>:FUNCtion:NOISe[:STATe] <State>

This command turns the noise measurement for all markers on and off.

You can query the results of the noise power density at the marker position with `CALCulate:MARKer<m>:FUNCtion:NOISe:RESult?`.

Parameter

<State>
ON | OFF

Example

See `CALCulate:MARKer<m>:FUNCtion:NOISe:RESult?`.

Characteristics

*RST value: OFF
SCPI: device-specific

CALCulate:MARKer<m>:FUNCtion:NOISe:RESult?

This command queries the result of the noise measurement.

To get a valid result, you have to perform a complete sweep with synchronization to the sweep end before reading out the result. This is only possible in single sweep mode.

This command is an event and therefore has no *RST value and no query.

Return value

<NoiseLevel>

The unit depends on `UNIT:POWer`.

Example

```
INIT:CONT OFF
```

Turns on single sweep mode.

```
CALC:MARK2 ON
```

```
CALC:MARK2:FUNC:NOIS ON
```

Turns on marker 2 and assigns the noise measurement to that marker.

```
INIT;*WAI
```

```
CALC:MARK2:NOIS:RES?
```

Performs the measurement and queries the noise marker results.

Characteristics

*RST value: –
SCPI: device-specific

CALCulate:MARKer<m>:FUNCtion:REFerence

This command matches the reference level to the power level of a marker

If you use a delta marker, the R&S ZVH turns it into a normal marker.

This command is an event and therefore has no *RST value and no query.

Example

```
CALC:MARK1:FUNC:REF
```

Matches the reference level to the power level of marker 1.

Characteristics

*RST value: -

SCPI: device-specific

7.3.7 Using Display Lines and Limit Lines

7.3.7.1 Display Lines

The following commands define the position of the display line.

The suffix <n> at CALCulate is irrelevant.

List of commands

- [CALCulate<n>:DLINe <Amplitude>](#) (p. 110)
- [CALCulate<n>:DLINe:STATe <State>](#) (p. 110)

CALCulate<n>:DLINe <Amplitude>

This command defines the position of a display line.

Parameter

<Amplitude>

Numeric value with a variable range and unit.

You can use any unit you want, the R&S ZVH then converts the unit to the currently selected unit. If you omit a unit, the R&S ZVH uses the currently selected unit.

Example

```
CALC:DLIN -20dBm
```

Sets the display line threshold to -20 dBm.

Characteristics

*RST value: – (STATe to OFF)

SCPI: device-specific

CALCulate<n>:DLINe:STATe <State>

This command turns display lines on and off.

Parameter

<State>

ON | OFF

Example

```
CALC:DLIN:STAT OFF
```

Turns on the display line.

Characteristics

*RST value: OFF

SCPI: device-specific

7.3.7.2 Limit Lines

The following commands define limit lines and perform the corresponding limit checks.

The suffix <n> at CALCulate is irrelevant.

The suffix <k> at LIMit selects the limit line and is in the range <1...2>.

List of commands

- CALCulate<n>:LIMit<k>:BEEP[:STATe] <State> (p. 111)
- CALCulate<n>:LIMit<k>:COMMeNt? (p. 111)
- CALCulate<n>:LIMit<k>:DEFine (p. 112)
- CALCulate<n>:LIMit<k>:DELete (p. 113)
- CALCulate<n>:LIMit<k>:FAIL? (p. 113)
- CALCulate<n>:LIMit<k>:LOWer:SELect <LimitLine> (p. 113)
- CALCulate<n>:LIMit<k>:LOWer:THReshold <Level> (p. 114)
- CALCulate<n>:LIMit<k>:STATe <State> (p. 114)
- CALCulate<n>:LIMit<k>:UNIT:X? (p. 114)
- CALCulate<n>:LIMit<k>:UNIT[:Y]? (p. 115)
- CALCulate<n>:LIMit<k>:UPPer:SELect <LimitLine> (p. 115)
- CALCulate<n>:LIMit<k>:UPPer:THReshold <Level> (p. 115)

CALCulate<n>:LIMit<k>:BEEP[:STATe] <State>

This command turns the beeper that beeps if a limit line is violated on and off.

Parameter

<State>
ON | OFF

Example

```
CALC:LIM:BEEP ON
```

Activates the audio beep.

Characteristics

*RST value: OFF
SCPI: device-specific

CALCulate<n>:LIMit<k>:COMMeNt?

This command queries the description of a limit line.

This command is a query and therefore has no RST value.

Return value

<Comment>
String containing the description of the limit line.

Example

```
CALC:LIM:COMM?
```

Queries the description of limit line 1.

Characteristics

*RST value: -
 SCPI: device-specific

CALCulate<n>:LIMit<k>:DEFine

<Name>,<Comment>,<Unit>,<Scale>,<Unit>,<x1>,<y1>[,<xn>,<yn>]

This command defines the shape of a limit line.

After you have defined the shape of the limit line you still have to activate it with [CALCulate<n>:LIMit<k>:UPPer:SElect <LimitLine>](#) before it takes effect.

Parameters

<Name>

String containing the name of the limit line.

Note: if a limit line with the same name already exists, it will be overwritten.

<Comment>

String containing a comment for the limit line.

<X-unit>

Unit of the x-axis. HZ | S | M

<Scale>

Scale of the x-axis: ABS | REL

<Y-unit>

Unit of the y-axis: DB | DBM | DBUV | DBMV | DBUVM | DBUAM | VSWR | V | W

<x1>,<xn>

Data points on the x-axis.

Note: a limit line may consist of up to 100 horizontal data points.

<y1>,<yn>

Data points on the y-axis.

Example

```
CALC:LIM:DEF 'Line', 'Example', HZ, ABS, DBM, 10000000, -10,
10000000, 0, 20000000, 0
```

Defines a limit line with three data points.

Characteristics

*RST value: -
 SCPI: device-specific

CALCulate<n>:LIMit<k>:DELeTe

This command deletes a limit line.

This command is an event and therefore has no *RST value and no query.

Example

```
CALC:LIM2:DEL
```

Deletes the second limit line

Characteristics

*RST value: -

SCPI: device-specific

CALCulate<n>:LIMit<k>:FAIL?

This command queries the result of a limit check.

To get a valid result, you have to perform a complete sweep with synchronization to the sweep end before reading out the result. This is only possible in single sweep mode.

Return value

0 for PASS and 1 for FAIL

Example

```
INIT;*WAI
```

```
CALC:LIM1:FAIL?
```

Performs a measurement and queries the result of the check for limit line 1.

Characteristics

*RST value: -

SCPI: conform

CALCulate<n>:LIMit<k>:LOWer:SElect <LimitLine>

This command selects the lower limit line.

This command is an event and therefore has no *RST value and no query.

Parameter

<LimitLine>

String containing the file name of the lower limit line.

Example

```
CALC:LIM:LOW:SEL 'GSM_Lower.rellim'
```

Selects the lower limit line.

Characteristics

*RST value:

SCPI: conform

CALCulate<n>:LIMit<k>:LOWer:THReshold <Level>

This command defines the level of a lower threshold limit line.

Parameter

<Level>

Numeric value whose unit depends on the unit you have currently selected for the vertical axis.

Example

```
CALC:LIM:LOW:THR -10DBM
```

Defines a threshold of -10 dBm

Characteristics

*RST value: -

SCPI: device-specific

CALCulate<n>:LIMit<k>:STATe <State>

This command turns a limit check on and off.

You can query the result of the limit check with

[CALCulate<n>:LIMit<k>:FAIL?](#).

Parameter

<State>

ON | OFF

Example

```
CALC:LIM:STAT ON
```

Switches on the limit check for limit line 1.

Characteristics

*RST value: OFF

SCPI: conform

CALCulate<n>:LIMit<k>:UNIT:X?

This command queries the horizontal unit of a limit line.

This command is a query and therefore has no *RST value.

Example

```
CALC:LIM:UNIT:X?
```

Queries the x-unit of the first limit line.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate<n>:LIMit<k>:UNIT[:Y]?

This command queries the vertical unit of a limit line.

This command is a query and therefore has no *RST value.

Example

```
CALC:LIM1:UNIT?
```

Queries the y-unit of the first limit line.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate<n>:LIMit<k>:UPPer:SElect <LimitLine>

This command selects the upper limit line.

This command is an event and therefore has no *RST value and no query.

Parameter

<LimitLine>

string containing the file name of the upper limit line

Example

```
CALC:LIM:UPP:SEL 'GSM_Upper.rellim'
```

Selects the upper limit line.

Characteristics

*RST value: -

SCPI: conform

CALCulate<n>:LIMit<k>:UPPer:THReshold <Level>

This command defines the level of an upper threshold limit line.

Parameter

<Level>

Numeric value whose unit depends on the unit you have currently selected for the vertical axis.

Example

```
CALC:LIM:UPP:THR -10DBM
```

Defines a threshold of -10 dBm

Characteristics

*RST value: -

SCPI: device-specific

7.3.8 Configuring and Using Measurement Functions

The R&S ZVH provides measurement functions that allow you to perform advanced measurements and can also be controlled remotely.

General measurement functions:

- [Working with Channel Tables](#) on page 116

Power measurements:

- [Power Measurements](#) on page 119
- [Measuring the Channel Power](#) on page 122
- [Measuring the Occupied Bandwidth](#) on page 124
- [TDMA Measurements](#) on page 125
- [Measuring the Adjacent Channel Leakage Ratio](#) on page 126
- [Measuring the Spectrum Emission Mask](#) on page 141
- [Measuring Spurious Emissions](#) on page 143

Other measurements

- [Measuring the Harmonic Distortion](#) on page 138
- [Measuring the AM Modulation Depth](#) on page 140

Isotropic Antenna

- [Using an Isotropic Antenna](#) on page 144

7.3.8.1 Working with Channel Tables

Use the following commands to work with channel tables.

List of commands

- [\[SENSe\]:CHANnel <ChannelNumber>](#) (p. 117)
- [\[SENSe\]:CHANnel:TABLE:SElect <ChannelTable>](#) (p. 117)
- [\[SENSe\]:CHANnel:TABLE:SElect:DOWNlink <ChannelTable>](#) (p. 118)
- [\[SENSe\]:CHANnel:TABLE:SElect:UPLink <ChannelTable>](#) (p. 118)
- [\[SENSe\]:CHANnel:TABLE:SET <Direction>](#) (p. 118)

[SENSe:]CHANnel <ChannelNumber>

This command selects the channel to be analyzed.

You have to set the frequency mode with `[SENSe:]FREQuency:INPut:MODE` to channel first.

Parameter

<ChannelNumber>

numeric value that selects the number of the channel to be analyzed

Example

See `[SENSe:]CHANnel:TABLE:SElect <ChannelTable>`.

Characteristics

*RST value: depends on the channel table

SCPI: conform

[SENSe:]CHANnel:TABLE:SElect <ChannelTable>

This command selects a channel table configured for the link direction you have selected with `[SENSe:]CHANnel:TABLE:SET <Direction>`.

Note that if you have previously selected a channel table with `[SENSe:]CHANnel:TABLE:SElect:DOWNlink <ChannelTable>` or `[SENSe:]CHANnel:TABLE:SElect:UPLink <ChannelTable>`, this command replaces that file.

Parameter

<ChannelTable>

String containing the file name of the channel table.

Example

```
CHAN:TABL:SET UP
```

Selects channel table selection for uplink signals.

```
CHAN:TABL:SEL 'TV China.CHNTAB'
```

Loads the channel table with the name 'TV China' for the uplink.

```
CHAN:TABL:SEL 'TV Italy.chntab'
```

or

```
CHAN:TABL:SEL:UPL 'TV Italy.chntab'
```

Both commands replace the uplink channel table 'TV China' with 'TV Italy'.

Downlink channel tables are not affected by the commands sent so far.

```
FREQ:INP:MODE CHAN
```

```
CHAN 10
```

Select a particular uplink channel (e.g. #10) instead of a (center) frequency.

To select an additional downlink channel table, use either:

```
CHAN:TABL:SET DOWN
```

```
CHAN:TABL:SEL 'TV Italy.chntab'
```

or

```
CHAN:TABL:SEL:DOWN 'TV Italy.chntab'
```

Characteristics

*RST value: ''

SCPI: device-specific

[SENSe]:CHANnel:TABLE:SElect:DOWNlink <ChannelTable>

This command selects a channel table configured for downlink signals.

Parameter

<ChannelTable>

string containing the name of the channel table.

Example

See [SENSe:]CHANnel:TABLE:SElect <ChannelTable>.

Characteristics

*RST value: ''

SCPI: device-specific

[SENSe]:CHANnel:TABLE:SElect:UPLink <ChannelTable>

This command selects a channel table configured for uplink signals.

Parameter

<ChannelTable>

string containing the name of the channel table.

Example

See [SENSe:]CHANnel:TABLE:SElect <ChannelTable>.

Characteristics

*RST value: ''

SCPI: device-specific

[SENSe]:CHANnel:TABLE:SET <Direction>

This command selects the link direction for measurements with channel tables.

Parameter

<Direction>

DOWN	Selects the downlink.
UP	Selects the uplink.

Example

See `[SENSe:]CHANnel:TABLE:SElect <ChannelTable>`.

Characteristics

*RST value: UP
SCPI: device-specific

7.3.8.2 Power Measurements

The following commands configure power measurements. To perform the actual measurement, use the commands described in section "[Performing and Triggering Measurements](#)".

List of commands

- `CALCulate:MARKer:FUNCTION:POWer:SElect <Measurement>` (p. 119)
- `CALCulate:MARKer:FUNCTION:POWer[:STATe] <State>` (p. 119)
- `CALCulate:MARKer:FUNCTION:POWer:PRESet <Standard>` (p. 120)
- `CALCulate:MARKer:FUNCTION:POWer:PRESet:CHECK?` (p. 120)
- `CALCulate:MARKer:FUNCTION:LEVel:ONCE` (p. 121)
- `CALCulate:MARKer:FUNCTION:POWer:RESult? <Measurement>` (p. 121)

CALCulate:MARKer:FUNCTION:POWer:SElect <Measurement>

This command selects a power measurement and turns the measurement on.

Parameter

ACPower MCACpower	Adjacent Channel Leakage Ratio measurement (ACLR or ACP)
CPOWer	Chanel power measurement
OBANdwidth OBWidth	Occupied Bandwidth measurement
TDMA	TDMA power measurement

Example

`CALC:MARK:FUNC:POW:SEL CPOW`
Selects the channel power measurement

Characteristics

*RST value: –
SCPI: device-specific

CALCulate:MARKer:FUNCTION:POWer[:STATe] <State>

This command turns a power measurement on and off.

You can select a power measurement with
`CALCulate:MARKer:FUNCTION:POWer:SElect <Measurement>`.

Parameter

ON	Turns the power measurement on.
OFF	Performs a basic spectrum measurement.

Example

```
CALC:MARK:FUNC:POW OFF
```

Switches off the power measurement.

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate:MARKer:FUNCtion:POWer:PRESet <Standard>

This command selects one of the predefined configurations for a telecommunications standard. This command only works if you have turned on power measurements with `CALCulate:MARKer:FUNCtion:POWer[:STATe]` `<State>`.

The configuration for a standard is in line with the specifications and includes parameters like weighting filter, channel bandwidth and spacing, resolution and video bandwidth, as well as detector and sweep time.

Parameter

<Standard>

string containing the file name of the standard

Example

```
CALC:MARK:FUNC:POW:PRES '3GPP WCDMA.chpstd'
```

Selects the 3GPP WCDMA standard for channel power measurements.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:MARKer:FUNCtion:POWer:PRESet:CHECK?

This command checks if the current settings are in line with the settings defined by the standard selected with `CALCulate:MARKer:FUNCtion:POWer:PRESet` `<Standard>`.

Note that the command only checks those parameters that are defined by the standard.

This command is a query and therefore has no *RST value.

Return value

0	R&S ZVH settings violate a standard configuration.
1	R&S ZVH settings comply with the standard.

Example

```
CALC:MARK:FUNC:POW:PRES:CHEC?
```

Queries compliance to the standard currently in use.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:MARKer:FUNCTION:LEVEL:ONCE

This command adjusts the reference level to the measured signal power.

This automatic routine makes sure that the that the signal power level does not overload the R&S ZVH or limit the dynamic range by too small a S/N ratio.

To determine the best reference level, the R&S ZVH aborts current measurements and performs a series of test sweeps. After it has finished the test, it continues with the actual measurement.

This command is an event and therefore has no *RST value and no query.

Example

```
CALC:MARK:FUNC:LEV:ONCE
```

Initiates an automatic level adjust routine.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:MARKer:FUNCTION:POWER:RESult? <Measurement>

This command queries the results of power measurements.

To get a valid result, you have to perform a complete sweep with synchronization to the sweep end before reading out the result. This is only possible in single sweep mode.

Before you can use this command, you have to select the power measurement with `CALCulate:MARKer:FUNCTION:POWER:SElect <Measurement>` and activate it with `CALCulate:MARKer:FUNCTION:POWER[:STATe] <State>`.

This command is a query and therefore has no *RST value.

Parameter and return value

ACPower	Returns the results for ACLR measurements
MCACpower	The number of return values depends on the number of TX and adjacent channel. The order of return values is: <ul style="list-style-type: none"> – power of the transmission channel – power of the lower adjacent channel – power of the upper adjacent channel – power of the lower alternate channel 1

	<ul style="list-style-type: none"> – power of the upper alternate channel 2 – etc. <p>The unit of the return values depends on the scaling of the vertical axis:</p> <ul style="list-style-type: none"> – logarithmic scaling returns the power in the currently selected unit (see UNIT:POWer). – linear scaling returns the power in W.
CPOWer	<p>Returns the results for channel power measurements</p> <p>The return value is the power of the channel. The unit depends on the scaling of the vertical axis:</p> <ul style="list-style-type: none"> – logarithmic scaling returns the power in the currently selected unit (see UNIT:POWer). – linear scaling returns the power in W.
OBANdwidth OBWidth	<p>Returns the results for measurements of the occupied bandwidth.</p> <p>The return value is the occupied bandwidth in Hz.</p>
TDMA	<p>Returns the results for TDMA power measurements.</p> <p>The return value is the power of the signal. The unit depends on the scaling of the vertical axis:</p> <ul style="list-style-type: none"> – logarithmic scaling returns the power in the currently selected unit (see UNIT:POWer). – linear scaling returns the power in W.

Example of occupied bandwidth measurement

POW:BAND 90PCT

Defines the occupied bandwidth (90%).

INIT:CONT OFF

INIT;*WAI

CALC:MARK:FUNC:POW:RES? OBW

Turns on single sweep mode, performs a measurement and queries the results.

Characteristics

*RST value: -

SCPI: device-specific

7.3.8.3 Measuring the Channel Power

The following commands configure channel power measurements. To perform the actual measurement, use the commands described in section "[Performing and Triggering Measurements](#)".

The suffix <m> at MARKer is irrelevant.

List of commands

- [CALCulate:MARKer<m>:FUNCTION:CPOWer:BANDwidth <Bandwidth>](#) (p. 123)
- [CALCulate:MARKer<m>:FUNCTION:CPOWer:MODE <DisplayMode>](#) (p. 123)
- [CALCulate:MARKer<m>:FUNCTION:CPOWer:UNIT <Unit>](#) (p. 123)
- [CALCulate:MARKer<m>:FUNCTION:POWer:RESult:PHZ <State>](#) (p. 124)

CALCulate:MARKer<m>:FUNCTION:CPOWer:BANDwidth <Bandwidth>

This command defines the channel bandwidth for channel power measurements.

Parameter

<Bandwidth>

Numeric value in Hz.

Example

```
CALC:MARK:FUNC:CPOW:BAND 4 MHZ
```

Sets the channel bandwidth to 4 MHz.

Characteristics

*RST value: 3.84 MHz

SCPI: device-specific

CALCulate:MARKer<m>:FUNCTION:CPOWer:MODE <DisplayMode>

This command selects the display mode for channel power measurements.

Parameter

<DisplayMode>

CLR	Displays the currently measured value (Clear / Write).
MAX	Displays the highest measured value (Max Hold).

Example

```
CALC:MARK:FUNC:CPOW:MODE CLR
```

Selects clear/write trace mode

Characteristics

*RST value: CLR

SCPI: device-specific

CALCulate:MARKer<m>:FUNCTION:CPOWer:UNIT <Unit>

This command selects the unit of the vertical axis for channel power measurements.

Parameter

<Unit>

DBM | DBMV | DBUV | VOLT | WATT | V | W

Example

```
CALC:MARK:FUNC:CPOW:UNIT DBM
```

Sets the unit to dBm.

Characteristics

*RST value: dBm

SCPI: device-specific

CALCulate:MARKer<m>:FUNCTION:POWER:RESult:PHZ <State>

This command turns the display of the channel power per Hertz on and off.

Parameter

ON | OFF

Example

CALC:MARK:FUNC:POW:RES:PHZ ON

Displays the measured Channel Power / Hz.

Characteristics

*RST value: dBm

SCPI: device-specific

7.3.8.4 Measuring the Occupied Bandwidth

The following commands configure the measurement of the Occupied Bandwidth. To perform the actual measurement, use the commands described in section "[Performing and Triggering Measurements](#)".

The suffix <m> at MARKer is irrelevant.

List of commands

- [CALCulate:MARKer<m>:FUNCTION:OBAN:BANDwidth <Bandwidth>](#) (p. 124)
- [CALCulate:MARKer<m>:FUNCTION:OBAN:BANDwidth:PCT <OBW>](#) (p. 125)

CALCulate:MARKer<m>:FUNCTION:OBAN:BANDwidth <Bandwidth>

This command defines the channel bandwidth for occupied bandwidth measurements.

Instead of OBANwidth, you can also use the alias OBWidth

Parameter

<Bandwidth

Numeric value in Hz.

Example

CALC:MARK:FUNC:OBW:BAND 1 MHZ

Sets the channel bandwidth to 1 MHz

Characteristics

*RST value: 3.84 MHz

SCPI: device-specific

CALCulate:MARKer<m>:FUNCTION:OBAN:BANDwidth:PCT <OBW>

This command defines the percentage of the total power that defines the occupied bandwidth.

Instead of OBANwidth, you can also use the alias OBWidth

Parameter

<Percentage>

Numeric value in the range from 10% to 99.9%.

Example

```
CALC:MARK:FUNC:OBW:BAND:PCT 95
```

Sets the power percentage to 95%

Characteristics

*RST value: 99%

SCPI: device-specific

7.3.8.5 TDMA Measurements

The following commands configure TDMA measurements. To perform the actual measurement, use the commands described in section "[Performing and Triggering Measurements](#)".

The suffix <m> at MARKer is irrelevant.

List of commands

- [CALCulate:MARKer<m>:FUNCTION:TDMA:BURSt <BurstLength>](#) (p. 125)

CALCulate:MARKer<m>:FUNCTION:TDMA:BURSt <BurstLength>

This command defines the burst length of the TDMA signal.

Parameter

<BurstLength>

Numeric value in seconds.

The value range depends on the current sweep time.

Example

```
CALC:MARK:FUNC:TDMA:BURS 80 US
```

Sets the burst length to 80 us.

Characteristics

*RST value: 470 us

SCPI: device-specific

7.3.8.6 Measuring the Adjacent Channel Leakage Ratio

The following commands configure Adjacent Channel Leakage Ratio (ACLR) measurements. To perform the actual measurement, use the commands described in section "[Performing and Triggering Measurements](#)".

The suffix <y> selects one of the 11 alternate channels. The range is <1...11>.

The suffix <k> at LIMit is irrelevant.

- [Configuring and Performing the ACLR Measurement](#) on page 126
- [ACLR Limit Check](#) on page 132

Configuring and Performing the ACLR Measurement

The following commands configure and perform the ACLR measurements.

List of commands

- [CALCulate:MARKer:FUNCTION:ACPower:UNIT <Unit>](#) (p. 126)
- [\[SENSe:\]POWer:ACHannel:ACPairs <ChannelPairs>](#) (p. 127)
- [\[SENSe:\]POWer:ACHannel:BANDwidth\[:CHANnel\] <Bandwidth>](#) (p. 127)
- [\[SENSe:\]POWer:ACHannel:BANDwidth:ACHannel <Bandwidth>](#) (p. 127)
- [\[SENSe:\]POWer:ACHannel:BANDwidth:ALternate<y> <Bandwidth>](#) (p. 128)
- [\[SENSe:\]POWer:ACHannel:MODE <PowerMode>](#) (p. 128)
- [\[SENSe:\]POWer:ACHannel:PRESet:RLEVel](#) (p. 129)
- [\[SENSe:\]POWer:ACHannel:REFeRence:TXCHannel:AUTO <RefChannel>](#) (p. 129)
- [\[SENSe:\]POWer:ACHannel:REFeRence:TXCHannel:MANual <RefChannel>](#) (p. 129)
- [\[SENSe:\]POWer:ACHannel:SPACing\[:ACHannel\]](#) (p. 130)
- [\[SENSe:\]POWer:ACHannel:SPACing:ALternate<y> <Spacing>](#) (p. 130)
- [\[SENSe:\]POWer:ACHannel:SPACing:CHANnel<Tx> <Spacing>](#) (p. 131)
- [\[SENSe:\]POWer:ACHannel:TXCHannel:COUNt <TxChannels>](#) (p. 131)

CALCulate:MARKer:FUNCTION:ACPower:UNIT <Unit>

This command selects the unit of the ACLR results.

Parameter

<Unit>

DBM | DBMV | DBUV | VOLT | WATT

Example

```
CALC:MARK:FUNC:ACP:UNIT DBM
```

ACLR results are converted into the unit dBm.

Characteristics

*RST value: 1

SCPI: device-specific

[SENSe:]POWer:ACHannel:ACPairs <ChannelPairs>

This command defines the number of pairs of adjacent channels.

Parameter

<ChannelPairs>

Numeric value in the range from 1 to 12.

The number corresponds to a pair of adjacent channels, one channel on the left and one on the right of the transmission channel.

Example

See `[SENSe:]POWer:ACHannel:TXChannel:COUNt <TxChannels>`

Characteristics

*RST value: 1

SCPI: device-specific

[SENSe:]POWer:ACHannel:BANDwidth[:CHANnel] <Bandwidth>

This command defines the channel bandwidth of the transmission channels.

Instead of BANDwidth, you can also use the alias BWIDth

Parameter

<Bandwidth>

Numeric value in Hz.

Example

See `[SENSe:]POWer:ACHannel:TXChannel:COUNt <TxChannels>`

Characteristics

*RST value: 14 kHz

SCPI: device-specific

[SENSe:]POWer:ACHannel:BANDwidth:ACHannel <Bandwidth>

This command defines the channel bandwidth of the adjacent channel.

The adjacent channel is the first pair of channels next to the transmission channels. If you set the channel bandwidth for these channels, the R&S ZVH sets the bandwidth of the alternate channels to the same value.

Instead of BANDwidth, you can also use the alias BWIDth

Parameter

<Bandwidth>

Numeric value in Hz.

Example

See `[SENSe:]POWer:ACHannel:TXChannel:COUNt <TxChannels>`

Characteristics

*RST value: 14 kHz
 SCPI: device-specific

[SENSe:]POWer:ACHannel:BANDwidth:ALTerNate<y> <Bandwidth>

This command defines the bandwidth of the alternate channels.

If you set the channel bandwidth for the first alternate channel, the R&S ZVH sets the bandwidth of the other alternate channels to the same value. The command works hierarchically: to set a bandwidth of the 10th and 8th channel, you have to set the bandwidth of the 8th channel first.

Instead of BANDwidth, you can also use the alias BWIDth

Parameter

<Bandwidth>
 Numeric value in Hz.

Example

See [SENSe:]POWer:ACHannel:TXCHannel:COUnT <TxChannels>

Characteristics

*RST value: 14 kHz
 SCPI: device-specific

[SENSe:]POWer:ACHannel:MODE <PowerMode>

This command selects the way the R&S ZVH displays the power of adjacent channels.

The number of adjacent and alternate channels has to be greater than 0 for the command to work.

Parameter

<PowerMode>

ABSolute	Shows the absolute power of all channels..
RELative	Shows the power of adjacent and alternate channels in relation to the transmission channel.

Example

POW:ACH:MODE ABS
 Shows absolute powers for all channels.

Characteristics

*RST value
 SCPI: device-specific

[SENSe:]POWer:ACHannel:PRESet:RLEVel

This command adjusts the reference level to the measured signal power.

This automatic routine makes sure that the that the signal power level does not overload the R&S ZVH or limit the dynamic range by too small a S/N ratio.

To determine the best reference level, the R&S ZVH aborts current measurements and performs a series of test sweeps. After it has finished the test, it continues with the actual measurement.

This command is an event and therefore has no *RST value and no query.

Example

```
POW:ACH:PRESet:RLEV
```

Initiates an ACP measurement and adjusts the reference level.

Characteristics

*RST value: -

SCPI: device-specific

[SENSe:]POWer:ACHannel:REFeRence:TXCHannel:AUTO <RefChannel>

This command automatically selects a reference channel for relative ACLR measurements.

The number of transmission channels and adjacent / alternate channels has to be greater than 0 for the command to work.

Parameter

<RefChannel>

MINimum	Reference is the transmission channel with the lowest power.
MAXimum	Reference is the transmission channel with the highest power.
LHIGest	Reference is the lowest transmission channel for lower adjacent channels and highest transmission channel for upper adjacent channels.

Example

```
POW:ACH:REF:TXCH:AUTO MIN
```

Sets the TX channel with the lowest power as reference channel

Characteristics

*RST value

SCPI: device-specific

[SENSe:]POWer:ACHannel:REFeRence:TXCHannel:MANual <RefChannel>

This command defines a reference channel for relative ACLR measurements.

The number of transmission channels and adjacent / alternate channels has to be greater than 0 for the command to work.

Parameter

<RefChannel>

Numeric value from 1 to 12.

The actual value range depends on the number of active transmission channels.

ExampleSee `[SENSe:]POWer:ACHannel:TXChannel:COUNT <TxChannels>`**Characteristics**

*RST value: 1

SCPI: device-specific

[SENSe:]POWer:ACHannel:SPACing[:ACHannel]] <Spacing>

This command defines the spacing between the transmission channel and its adjacent channel.

A change of the adjacent channel spacing causes a change in the spacing of all alternate channels above the adjacent channel.

Parameter

<Spacing>

Numeric value in Hz.

ExampleSee `[SENSe:]POWer:ACHannel:TXChannel:COUNT <TxChannels>`**Characteristics**

*RST value: 14 kHz

SCPI: device-specific

[SENSe:]POWer:ACHannel:SPACing:ALTErnate<y> <Spacing>

This command defines the spacing between alternate channels.

If you set the channel spacing for the first alternate channel, the R&S ZVH sets the bandwidth of the other alternate channels to the same value. The command works hierarchically: to set a spacing of the 10th and 8th channel, you have to set the spacing of the 8th channel first.

Parameter

<Spacing>

Numeric value in Hz.

ExampleSee `[SENSe:]POWer:ACHannel:TXChannel:COUNT <TxChannels>`**Characteristics**

*RST value: ALT1: 40 kHz; ALT2: 60 kHz; ALT3: 80 kHz etc.

SCPI: device-specific

[SENSe:]POWer:ACHannel:SPACing:CHANnel<Tx> <Spacing>

This command defines the spacing between transmission channels.

If you set the channel spacing for the first transmission channel, the R&S ZVH sets the bandwidth of the other transmission channels to the same value. The command works hierarchically: to set a spacing between the 9th and 10th and 8th and 9th channel, you have to set the spacing between the 8th and 9th channel first.

The suffix at CHANnel selects the transmission channel.

Parameter

<Spacing>

Numeric value in Hz.

Example

See [SENSe:]POWer:ACHannel:TXChannel:COUNT <TxChannels>

Characteristics

*RST value: 20 kHz

SCPI: device-specific

[SENSe:]POWer:ACHannel:TXChannel:COUNT <TxChannels>

This command defines the number of transmission channels.

The command is available for measurements with span > 0.

Parameter

<TxChannels>

Numeric value from 1 to 12.

Example

CALC:MARK:FUNC:POW:SEL CPOW

Selects the channel power measurement

POW:ACH:TXCH:COUN 2

Defines 2 transmission channels.

POW:ACH:ACP 2

Defines 2 pairs of neighboring channels to the left and right of the TX channel(s).

POW:ACH:SPAC:CHAN2 20KHZ

Defines a distance of 20 kHz between the first and the second Tx channel.

POW:ACH:BAND:CHAN2 120KHZ

Defines a bandwidth of 120 kHz for the second TX channel.

POW:ACH:REF:TXCH:MAN 2

Selects the second Tx channel as reference channel.

POW:ACH:SPAC 10KHZ

Defines a distance of 10 kHz from the TX channel to the adjacent channel.

POW:ACH:BAND:ACH 120KHZ

Defines a bandwidth of 120 kHz for the adjacent channel.

POW:ACH:SPAC:ALT 20KHZ

Defines a distance of 20 kHz from the adjacent to the first alternate channel.

POW:ACH:BAND:ALT 120KHZ

Defines a bandwidth of 120 kHz for the first alternate channel

Characteristics

*RST value: 1

SCPI: device-specific

ACLR Limit Check

The following commands configure and perform limit checks when measuring the adjacent channel power.

The suffix <k> at LIMit is irrelevant.

List of commands

- [CALCulate:LIMit<k>:ACPower\[:STATe\] <State>](#) (p. 132)
- [CALCulate:LIMit<k>:ACPower:ACHannel\[:RELative\] <Limit>](#) (p. 133)
- [CALCulate:LIMit<k>:ACPower:ACHannel\[:RELative\]:STATe <State>](#) (p. 133)
- [CALCulate:LIMit<k>:ACPower:ACHannel:ABSolute <Limit>](#) (p. 134)
- [CALCulate:LIMit<k>:ACPower:ACHannel:ABSolute:STATe <State>](#) (p. 134)
- [CALCulate:LIMit<k>:ACPower:ACHannel:RESult?](#) (p. 134)
- [CALCulate:LIMit<k>:ACPower:ALternate<y>\[:RELative\] <Limit>](#) (p. 135)
- [CALCulate:LIMit<k>:ACPower:ALternate<y>\[:RELative\]:STATe <State>](#) (p. 135)
- [CALCulate:LIMit<k>:ACPower:ALternate<y>:ABSolute <Limit>](#) (p. 136)
- [CALCulate:LIMit<k>:ACPower:ALternate<y>:ABSolute:STATe <State>](#) (p. 136)
- [CALCulate:LIMit<k>:ACPower:ALternate<y>:RESult?](#) (p. 137)

CALCulate:LIMit<k>:ACPower[:STATe] <State>

This command turns the limit check for ACLR measurements on and off.

You have to use

[CALCulate:LIMit<k>:ACPower:ACHannel\[:RELative\]:STATe <State>](#)

or [CALCulate:LIMit<k>:ACPower:ALternate<y>\[:RELative\]:STATe <State>](#) in combination with this command to select the channels the limit check should be performed on.

Parameter

<State>

ON | OFF

Example

CALC:LIM:ACP ON

Activates the limit check

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate:LIMit<k>:ACPower:ACHannel[:RELative] <Limit>

This command defines the relative limit of the adjacent channels. The reference value for the relative limit value is the measured channel power.

Note that the relative limit has no effect on the limit check if it is below the absolute limit value (see [CALCulate:LIMit<k>:ACPower:ACHannel:ABSolute <Limit>](#)). This mechanism allows automatic checking of the absolute basic values of adjacent-channel power as defined in mobile radio standards.

Parameter

<Limit>

Numeric value in the range from 0 dB to 100 dB.

Example

```
CALC:LIM:ACP:ACH 30
```

Defines a limit of 30 dB.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:LIMit<k>:ACPower:ACHannel[:RELative]:STATe <State>

This command turns the relative limit check for the adjacent channels on and off.

You have to activate the general ACLR limit check before using this command with [CALCulate:LIMit<k>:ACPower\[:STATe\] <State>](#) first.

Parameter

<State>

ON | OFF

Example

```
CALC:LIM:ACP:ACH:STAT ON
```

Activates the relative limit check.

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate:LIMit<k>:ACPower:ACHannel:ABSolute <Limit>

This command defines the absolute limit for the adjacent channels.

Note that the absolute limit has no effect on the limit check if it is below the relative limit (see `CALCulate:LIMit<k>:ACPower:ACHannel[:RELative] <Limit>`). This mechanism allows automatic checking of the absolute basic values of adjacent-channel power as defined in mobile radio standards.

Parameter

<Limit>

Numeric value in the range from -200 dBm to 200 dBm.

Example

```
CALC:LIM:ACP:ACH:ABS -30
```

Sets the absolute limit to -30 dBm

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:LIMit<k>:ACPower:ACHannel:ABSolute:STATe <State>

This command turns the absolute limit check for the adjacent channel on and off.

You have to activate the general ACLR limit check before using this command with `CALCulate:LIMit<k>:ACPower[:STATe] <State>` first.

Parameter

<State>

ON | OFF

Example

```
CALC:LIM:ACP:ACH:ABS:STAT ON
```

Activates the absolute limit check.

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate:LIMit<k>:ACPower:ACHannel:RESult?

This command queries the result of the limit check of the adjacent channels.

To get a valid result, you have to perform a complete sweep with synchronization to the sweep end before reading out the result. This is only possible in single sweep mode.

This command is a query and therefore has no *RST value.

Return value

The return value consists of two values, one for the lower and one for the upper adjacent channel.

FAILed	Limit check failed.
PASSed	Limit check passed.

Example

`CALC:LIM:ACP:ACH:RES?`

Queries the limit check results. The command would return, e.g.

`FAILED, FAILED`

Upper and lower adjacent channels violate a limit.

Characteristics

*RST value: -

SCPI: device-specific

`CALCulate:LIMit<k>:ACPower:ALternate<y>[:RELative] <Limit>`

This command defines the relative limit of the alternate channels. The reference value for the relative limit value is the measured channel power.

Note that the relative limit has no effect on the limit check if it is below the absolute limit value (see `CALCulate:LIMit<k>:ACPower:ALternate<y>:ABSolute <Limit>`). This mechanism allows automatic checking of the absolute basic values of adjacent-channel power as defined in mobile radio standards.

Parameter

`<Limit>`

Numeric value in the range from 0 dB to 100 dB.

Example

`CALC:LIM:ACP:ALT3 30`

Defines a limit of 30 dB for the third alternate channel.

Characteristics

*RST value: -

SCPI: device-specific

`CALCulate:LIMit<k>:ACPower:ALternate<y>[:RELative]:STATe <State>`

This command turns the relative limit check for an alternate channels on and off.

You have to activate the general ACLR limit check before using this command with `CALCulate:LIMit<k>:ACPower[:STATe] <State>` first.

Parameter

`<State>`

ON | OFF

Example

```
CALC:LIM:ACP:ALT3:STAT ON
```

Activates the relative limit check for the third alternate channel.

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate:LIMit<k>:ACPower:ALTernate<y>:ABSolute <Limit>

This command defines the absolute limit for the alternate channels.

Note that the absolute limit has no effect on the limit check if it is below the relative limit (see [CALCulate:LIMit<k>:ACPower:ALTernate<y>\[:RELative\] <Limit>](#)). This mechanism allows automatic checking of the absolute basic values of adjacent-channel power as defined in mobile radio standards.

Parameters

<Limit>

Numeric value in the range from -200 dBm to 200 dBm.

Example

```
CALC:LIM:ACP:ALT3:ABS -30
```

Sets the absolute limit to -30 dBm for the third alternate channel.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:LIMit<k>:ACPower:ALTernate<y>:ABSolute:STATe <State>

This command turns the absolute limit check for an alternate channel on and off.

You have to activate the general ACLR limit check before using this command with [CALCulate:LIMit<k>:ACPower\[:STATe\] <State>](#) first.

Parameter

<State>

ON | OFF

Example

```
CALC:LIM:ACP:ALT3:ABS:STAT ON
```

Activates the absolute limit check for the third alternate channel.

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate:LIMit<k>:ACPower:ALTErnate<y>:RESult?

This command queries the result of the limit check of the alternate channels.

To get a valid result, you have to perform a complete sweep with synchronization to the sweep end before reading out the result. This is only possible in single sweep mode.

This command is a query and therefore has no *RST value.

Return value

The return value consists of two values, one for the lower and one for the upper alternate channel.

FAILED	Limit check failed.
PASSED	Limit check passed.

Example

```
CALC:LIM:ACP:ALT2:RES?
```

Queries the limit check results for the second alternate channels. The command would return, e.g.

```
FAILED, FAILED
```

Upper and lower alternate channels violate a limit.

Characteristics

*RST value: -

SCPI: device-specific

ACLR Result Query

The following commands query results specific to the adjacent channel power measurement.

The suffixes<n> and <m> at CALCulate and MARKer are irrelevant.

List of commands

- [CALCulate<n>:MARKer<m>:FUNCTION:TXPower:RESult?](#) (p. 137)

CALCulate<n>:MARKer<m>:FUNCTION:TXPower:RESult?

This command queries the total TX channel power.

(Use [CALCulate:MARKer:FUNCTION:POWER:RESult? <Measurement>](#) to query the power of each TX channel.)

Return value

<Power>

Example

```
CALC:MARK:FUNC:TXP:RES?
```

Queries the total channel power over all TX channels.

Characteristics

*RST value: -

SCPI: device-specific

7.3.8.7 Measuring the Harmonic Distortion

The following commands configure Harmonic Distortion measurements. To perform the actual measurement, use the commands described in section "[Performing and Triggering Measurements](#)".

The numeric suffixes <n> and <m> at CALCulate and MARKer are irrelevant.

List of commands

- [CALCulate<n>:MARKer<m>:FUNCTION:HARMonics\[:STATe\] <State>](#) (p. 138)
- [CALCulate<n>:MARKer<m>:FUNCTION:HARMonics:DISToRTion?](#) (p. 138)
- [CALCulate<n>:MARKer<m>:FUNCTION:HARMonics:LIST?](#) (p. 139)
- [CALCulate<n>:MARKer<m>:FUNCTION:HARMonics:NHARMonics <Harmonics>](#) (p. 139)
- [CALCulate<n>:MARKer<m>:FUNCTION:HARMonics:PRESet](#) (p. 140)

CALCulate<n>:MARKer<m>:FUNCTION:HARMonics[:STATe] <State>

This command turns the harmonic distortion measurement on and off.

Parameter

<State>

ON | OFF

Example

See [CALCulate<n>:MARKer<m>:FUNCTION:HARMonics:PRESet](#).

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate<n>:MARKer<m>:FUNCTION:HARMonics:DISToRTion? TOTal

This command queries the total harmonic distortion of the signal.

To get a valid result, you have to perform a complete sweep with synchronization to the sweep end before reading out the result. This is only possible in single sweep mode.

This command is a query and therefore has no *RST value.

Parameter

TOTal

Return value

<Distortion%>,<DistortiondB>

Pair of values, one showing the THD in %, one in dB.

ExampleSee `CALCulate<n>:MARKer<m>:FUNCTION:HARMonics:PRESet`.**Characteristics**

*RST value: -

SCPI: device-specific

CALCulate<n>:MARKer<m>:FUNCTION:HARMonics:LIST?

 This command queries the position of the harmonics.

To get a valid result, you should perform a complete sweep in single sweep mode before querying the results.

This command is a query and therefore has no *RST value.

Return value

Returns one value for every harmonic.

The first value is the absolute power of the first harmonic. The level unit depends on the unit you have set with the `UNIT:POWER` command. The other values are power levels relative to the first harmonic. The unit for these is dB.

The total number of return values depends on the number of harmonics you have set with `CALCulate<n>:MARKer<m>:FUNCTION:HARMonics:NHARmonics<Harmonics>`.

ExampleSee `CALCulate<n>:MARKer<m>:FUNCTION:HARMonics:PRESet`.**Characteristics**

*RST value: -

SCPI: device-specific

CALCulate<n>:MARKer<m>:FUNCTION:HARMonics:NHARmonics <Harmonics>

 This command sets the number of harmonics. The valid range is from 1 to 6 harmonics.
Parameter

<Harmonics>

Numeric value in the range from 1 to 6.

Example

See `CALCulate<n>:MARKer<m>:FUNCtion:HARMonics:PRESet`.

Characteristics

*RST value: 2

SCPI: device-specific

CALCulate<n>:MARKer<m>:FUNCtion:HARMonics:PRESet

This command optimizes the settings for the harmonic distortion measurement.

This command is an event and therefore has no query and no *RST value.

Example

`CALC:MARK:FUNC:HARM ON`

Activates the harmonic distortion measurement.

`CALC:MARK:FUNC:HARM:NHAR 4`

Sets the number of harmonics to 4.

`CALC:MARK:FUNC:HARM:PRES`

Adjusts the settings of the measurement.

`CALC:MARK:FUNC:HARM:LIST?`

`CALC:MARK:FUNC:HARM:DIST? TOT`

Queries the position of the harmonics and the total harmonic distortion.

Characteristics

*RST value: -

SCPI: device-specific

7.3.8.8 Measuring the AM Modulation Depth

The following commands configure AM Modulation Depth measurements. To perform the actual measurement, use the commands described in section "[Performing and Triggering Measurements](#)".

The numeric suffixes <n> and <m> at CALCulate and MARKer are irrelevant.

List of commands

- `CALCulate<n>:MARKer<m>:FUNCtion:MDEPth[:STATe] <State>` (p. 141)
- `CALCulate<n>:MARKer<m>:FUNCtion:MDEPth:RESult?` (p. 141)

CALCulate<n>:MARKer<m>:FUNCtion:MDEPth[:STATe] <State>

This command turns the AM Modulation Depth measurement on and off.

The numeric suffixes at CALCulate and MARKer are irrelevant.

Parameter

<State>

ON | OFF

Example

CALC:MARK:FUNC:MDEP ON

Activates the harmonic distortion measurement.

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate<n>:MARKer<m>:FUNCtion:MDEPth:RESult?

This command queries the results of the AM modulation depth measurement.

This command is a query and therefore has no *RST value.

Return value

<ModulationDepth>

Modulation depth in %.

Example

CALC:MARK:FUNC:MDEP:RES?

Queries the AM modulation depth.

Characteristics

*RST value: -

SCPI: device-specific

7.3.8.9 Measuring the Spectrum Emission Mask

The following commands configure Spectrum Emission Mask (SEM) measurements. To perform the actual measurement, use the commands described in section "[Performing and Triggering Measurements](#)".

List of commands

- [\[SENSe:\]ESpectrum:PRESet\[:STANdard\] <Standard>](#) (p. 142)
- [\[SENSe:\]ESpectrum:PRESet:SETTings](#) (p. 142)
- [\[SENSe:\]SWEep:MODE <State>](#) (p. 143)
- [CALCulate<n>:MARKer<m>:FUNCtion:TXPower:RESult?](#) (p. 142)

CALCulate<n>:MARKer<m>:FUNCtion:TXPower:RESult?

This command queries the TX channel power.

Return value

<Power>

The power is either the peak power or the channel power, depending on the selected standard.

Example

```
CALC:MARK:FUNC:TXP:RES?
```

Queries the total channel power over all TX channels.

Characteristics

*RST value: -

SCPI: device-specific

[SENSe:]ESpectrum:PRESet[:STANdard] <Standard>

This command loads one of the predefined spectrum emission masks for a telecommunications standard.

Parameter

<Standard>

String containing the file name of the spectrum emission mask.

Example

```
ESP:PREs 'W-CDMA 3GPP.semstd'
```

Loads the SEM for 3GPP WCDMA.

Characteristics

*RST value: -

SCPI: device-specific

[SENSe:]ESpectrum:PRESet:SETTings ONCE

This command optimizes the settings for the SEM measurement.

This command is an event and therefore has no query and no *RST value.

Parameter

ONCE

Example

```
ESP:PREs:SET ONCE
```

Initializes an adjustment of the settings.

Characteristics

*RST value: -

SCPI: device-specific

[SENSe:]SWEep:MODE <State>

This command turns the spectrum emission mask measurement on and off.

Parameter

AUTO	Turns on the Spectrum mode.
ESpectrum	Turns on the SEM measurement.
LIST	Turns on the Spurious Emission measurement.

Example

```
SWE:MODE ESP
```

Starts the SEM measurement.

Characteristics

*RST value: AUTO

SCPI: device-specific

7.3.8.10 Measuring Spurious Emissions

The following commands configure Spurious Emission measurements. To perform the actual measurement, use the commands described in section "[Performing and Triggering Measurements](#)".

List of commands

- [\[SENSe:\]FREQuency:CARRier:STARt <Frequency>](#) (p. 143)
- [\[SENSe:\]FREQuency:CARRier:STOP <Frequency>](#) (p. 144)
- [\[SENSe:\]SWEep:MODE <State>](#) (p. 143)

[SENSe:]FREQuency:CARRier:STARt <Frequency>

This command defines the start frequency of the 3GPP carrier.

Parameter

<Frequency>

Numeric value in Hz.

Example

```
FREQ:CARR:STAR 1910MHZ
```

Defines a carrier start frequency of 1910 MHz.

Characteristics

*RST value: -

SCPI: device-specific

[SENSe:]FREQuency:CARRier:STOP <Frequency>

This command defines the start frequency of the 3GPP carrier.

Parameter

<Frequency>
Numeric value in Hz.

Example

FREQ:CARR:STOP 1990MHZ
Defines a carrier stop frequency of 1990 MHz.

Characteristics

*RST value: -
SCPI: device-specific

7.3.8.11 Using an Isotropic Antenna

This chapter describes all commands available to set up measurements with an isotropic antenna.

You can use an isotropic antenna with all measurement modes that are described above.

List of commands

- [INPut:ANTenna:MEASure <Direction>](#) (p. 144)
- [INPut:ANTenna:STATe <State>](#) (p. 145)
- [\[SENSe:\]CORRection:TRANsducer<c>:ISOTropic\[:STATe\]?](#) (p. 145)

INPut:ANTenna:MEASure <Direction>

This command selects the direction that the isotropic antenna measures.

Parameter

<Direction>

AUTO	Automatically selects the direction.
X Y Z	Measures the corresponding direction only.

Example

INP:ANT:MEAS X
Measures in x-direction.

Characteristics

*RST value: AUTO
SCPI: device-specific

INPut:ANTenna:STATe <State>

This command turns the use of an isotropic antenna on and off.

Parameter

<State>
ON | OFF

Example

```
INP:ANT:STAT ON
```

Activates the isotropic antenna

Characteristics

*RST value: OFF
SCPI: device-specific

[SENSe:]CORRection:TRANsducer<c>:ISOTropic[:STATe]?

This command queries if the currently selected transducer is an isotropic antenna.

When you use the command for 3GPP WCDMA measurements in the Digital Modulation operating mode, the command also turns the use of an isotropic antenna on and off.

The numeric suffix <t> at TRANsducer selects the primary or secondary transducer and is in the range <1...2>.

Return values

0	Transducer is not an isotropic antenna.
1	Transducer is an isotropic antenna.

Example

```
CORR:TRAN:ISOT?
```

Characteristics

*RST value: -
SCPI: device-specific

7.4 Remote Commands of the Network Analyzer Mode

The chapter provides information on remote commands that configure and perform two-port measurements with the tracking generator. These commands are available in network analyzer mode only.



Availability of remote commands for the Network Analyzer

Note that some of the listed remote commands take effect only if options R&S ZVH-K42 Vector Reflection and Transmission Measurements and / or R&S ZVH-K45 Vector Voltmeter are installed.

Contents

[Configuring the Horizontal Axis](#) on page 146
[Configuring the Vertical Axis](#) on page 147
[Setting the Bandwidths](#) on page 152
[Performing and Triggering the Measurement](#) on page 152
[Working with Traces](#) on page 153
[Using Markers and Deltamarkers](#) on page 155
[Configuring the Measurement](#) on page 159

7.4.1 Configuring the Horizontal Axis

The following commands configure the horizontal axis of the active display.

List of commands

- [\[SENSe:\]FREQuency:CENTer <Frequency>](#) (p. 36)
- [\[SENSe:\]FREQuency:CENTer:STEP <StepSize>](#) (p. 36)
- [\[SENSe:\]FREQuency:CENTer:STEP:LINK <StepSizeCoupling>](#) (p. 37)
- [\[SENSe:\]FREQuency:SPAN](#) (p. 38)
- [\[SENSe:\]FREQuency:SPAN:FULL](#) (p. 79)
- [\[SENSe:\]FREQuency:STARt <StartFrequency>](#) (p. 39)
- [\[SENSe:\]FREQuency:STOP <StopFrequency>](#) (p. 39)

For a detailed description of the commands refer to "[Configuring the Horizontal Axis](#)" in CAT mode.

7.4.2 Configuring the Vertical Axis

The following commands configure the level axis (y-axis) and level parameters of the active display.

The suffix <n> at DISPlay selects the measurement screen in dual trace mode. The range is {1...2}.

List of commands

- [DISPlay<n>:GDElay:REference <RefValue>](#) (p. 147)
- [DISPlay<n>:GDElay:REference:POStion <RefPosition>](#) (p. 148)
- [DISPlay<n>:GDElay:Y:SCALE <DisplayRange>](#) (p. 148)
- [DISPlay<n>:IMPedance:REference:POStion <Impedance>](#) (p. 157)
- [DISPlay:LOSS:REference <RefValue>](#) (p. 41)
- [DISPlay:LOSS:REference:POStion <RefPosition>](#) (p. 42)
- [DISPlay:LOSS:Y:SCALE <DisplayRange>](#) (p. 42)
- [DISPlay<n>:MAGNitude:REference <RefValue>](#) (p. 43)
- [DISPlay<n>:MAGNitude:REference:POStion <RefPosition>](#) (p. 43)
- [DISPlay<n>:MAGNitude:Y:SCALE <DisplayRange>](#) (p. 43)
- [DISPlay<n>:MAGNitude:Y:SPACing <Scaling>](#) (p. 44)
- [DISPlay<n>:PHASe:REference <RefValue>](#) (p. 149)
- [DISPlay<n>:PHASe:REference:POStion <RefPosition>](#) (p. 149)
- [DISPlay<n>:PHASe:Y:SCALE <DisplayRange>](#) (p. 149)
- [DISPlay<n>:PHASe:UNWRap <State>](#) (p. 150)
- [DISPlay<n>:REFLection:Y:SCALE <DisplayRange>](#) (p. 150)
- [DISPlay<n>:REFLection:UNIT <Unit>](#) (p. 151)
- [DISPlay<n>:VSWR:Y:SCALE:MINimum <BottomValue>](#) (p. 44)
- [DISPlay<n>:VSWR:Y:SCALE:MAXimum <TopValue>](#) (p. 45)
- [DISPlay<n>:VSWR:Y:SCALE <DisplayRange>](#) (p. 45)
- [INPut:ATTenuation <Attenuation>](#) (p. 45)
- [SOURce:TG:ATTenuation <TGAttenuation>](#) (p. 46)
- [UNIT:POWer <Unit>](#) (p. 86)

For a detailed description of commands not described below refer to "[Configuring the Vertical Axis](#)" in CAT mode and "[Configuring the Vertical Axis](#)" in spectrum mode.

DISPlay<n>:GDElay:REference <RefValue>

This command sets the reference value for the group delay measurement format.

Parameter

<RefValue>

Numeric value in the range from 1 ns to 1000 ns.

Example

```
DISP:GDEL:REF 20
```

Sets the reference level to 20 nanoseconds

Characteristics

*RST value: 0 ns

SCPI: device-specific

DISPlay<n>:GDElay:REfereNce:POSition <RefPosition>

This command defines the position of the reference value on the display for the group delay measurement format.

Each step shifts the reference position one grid line up or down.

Parameter

<RefPosition>

Numeric value in the range from 0 to 10.

Example

```
DISP:GDEL:REF:POS 1
```

Sets the reference to the first grid line from the bottom.

Characteristics

*RST value: 5

SCPI: device-specific

DISPlay<n>:GDElay:Y:SCALe <DisplayRange>

This command defines the display range of the vertical axis for the group delay measurement format.

Parameter

<DisplayRange>

Numeric value in the range from 10 ns to 100000 ns.

The number you enter is rounded up to the next possible display range. For example, if you enter 9, the R&S ZVH automatically sets the display range to 10.

Example

```
DISP:GDEL:Y:SCAL 20E-9
```

Sets the display range to 20 nanoseconds

Characteristics

*RST value: 100 ns

SCPI: device-specific

DISPlay<n>:PHASe:REFerence <RefValue>

This command sets the reference value for the phase measurement format.

Parameter

<RefValue>

Numeric value in the range from -100000° to 100000°.

Example

```
DISP:MAGN:REF -10
```

Sets the reference level to -10 dB

Characteristics

*RST value: 0 dB

SCPI: device-specific

DISPlay<n>:PHASe:REFerence:POSition <RefPosition>

This command defines the position of the reference value on the display for the phase measurement format.

Each step shifts the reference position one grid line up or down.

Parameter

<RefPosition>

Numeric value in the range from 0 to 10.

Example

```
DISP:LOSS:REF:POS 5
```

Sets the reference to the center of the display (i.e. the fifth grid line from the bottom).

Characteristics

*RST value: 10

SCPI: device-specific

DISPlay<n>:PHASe:Y:SCALE <DisplayRange>

This command defines the display range of the vertical axis for the phase measurement format.

Parameter

<DisplayRange>

Numeric value in the range from 90° to 100000°.

The number you enter is rounded up to the next possible display range. For example, if you enter 80°, the R&S ZVH automatically sets the display range to 90°.

Example

```
DISP:PHAS:Y:SCAL 180
```

Sets the display range of the phase measurement to 180°

Characteristics

*RST value: 360°

SCPI: device-specific

DISPlay<n>:PHASe:UNWRap <State>

This command removes the restriction limiting the value range to +/- 180°.

Parameter

<State>

ON | OFF

Example

```
DISP:PHAS:UNWR ON
```

Activates the phase unwrap

Characteristics

*RST value: OFF

SCPI: device-specific

DISPlay<n>:REFLection:Y:SCALe <DisplayRange>

This command defines the display range of the vertical axis for the reflection coefficient measurement format.

Parameter

<DisplayRange>

Numeric value in the range from 1 dB to 1000 mrho.

The number you enter is rounded up to the next possible display range. For example, if you enter 18, the R&S ZVH automatically sets the display range to 20 mrho.

Example

```
DISP:REFL:Y:SCAL 100
```

Sets a display range of 100 mrho.

Characteristics

*RST value: 1000 mp

SCPI: device-specific

DISPlay<n>:REFLection:UNIT <Unit>

This command defines the unit of the reflection coefficient.

Parameter

<Unit>

RHO | MRHO

Example

DISP:REFL:UNIT RHO

Sets the unit to RHO.

Characteristics

*RST value: MRHO

SCPI: device-specific

7.4.3 Setting the Bandwidths

The following commands configure the filter bandwidths of the R&S ZVH. Note that both groups of commands (BANDwidth and BWIDth) are the same.

List of commands

- [\[SENSe:\]BANDwidth|BWIDth\[:RESolution\] <MeasBW>](#) (p. 47)
- [\[SENSe:\]BANDwidth|BWIDth\[:RESolution\]:AUTO <State>](#) (p. 47)

For a detailed description of commands refer to "[Setting the Bandwidth](#)" in CAT mode.

7.4.4 Performing and Triggering the Measurement

The following commands configure the sweep.

List of commands

- [*WAI](#) (p. 34)
- [ABORt](#) (p. 89)
- [INITiate\[:IMMediate\]](#) (p. 89)
- [INITiate:CONTinuous <SweepMode>](#) (p. 90)
- [\[SENSe:\]SWEep:COUNT <SweepCount>](#) (p. 90)
- [SENSe:SWEep:POINTs <Points>](#) (p. 48)
- [\[SENSe:\]SWEep:TIME <SweepTime>](#) (p. 91)
- [\[SENSe:\]SWEep:TIME:AUTO <State>](#) (p. 91)
- [TRIGger\[:SEQuence\]:HOLDoff\[:TIME\] <TriggerDelay>](#) (p. 48)
- [TRIGger\[:SEQuence\]:SLOPe <TriggerSlope>](#) (p. 49)
- [TRIGger\[:SEQuence\]:SOURce <TriggerSource>](#) (p. 49)

For a detailed description of commands refer to "[Performing and Triggering Measurements](#)" in CAT mode and "[Performing and Triggering Measurements](#)" in spectrum analyzer mode.

7.4.5 Working with Traces

The following commands set up the trace and the various functions associated with it, e.g. the selection of the detector.

The suffix <n> in the following commands selects the measurement screen in dual trace mode and is in the range {1...2}.

List of commands

- [DISPlay\[:WINDow\]:TRACe<n>:MEMory\[:STATe\] <State>](#) (p. 50)
- [DISPlay\[:WINDow\]:TRACe<n>:MODE <TraceMode>](#) (p. 51)
- [FORMat\[:DATA\] <DataFormat>](#) (p. 51)
- [FORMat:BORDER <ByteOrder>](#) (p. 99)
- [\[SENSe:\]DETEctor<n> \[:FUNctIon\] <Detector>](#) (p. 99)
- [\[SENSe:\]DETEctor<n> \[:FUNctIon\]:AUTO <State>](#) (p. 100)
- [TRACe\[:DATA\]?](#) (p. 153)
- [TRACe<n>:DATA:MEMory? <Trace>](#) (p. 53)

For a detailed description of commands not described here refer to "[Working with Traces](#)" in CAT mode and "[Working with Traces](#)" in spectrum analyzer mode.

TRACe[:DATA]?

This command reads out the trace data of the current measurement.

With the [FORMat\[:DATA\] <DataFormat>](#) command, you can set the data format.

Parameter

The available parameters depend on the format of the result display.

Display of one S-parameter

TRACE1	Queries the data of the currently displayed trace.
--------	--

Display of two S-parameters (split screen mode)

TRACE1	Queries the data displayed in the upper screen.
TRACE2	Queries the data displayed in the lower screen.

Display of four S-parameters (split screen mode)

TRACE1	Queries the data of S11.
TRACE2	Queries the data of S21.
TRACE3	Queries the data of S22.
TRACE4	Queries the data of S12.

Return value

The R&S ZVH returns 631 values. Each value corresponds to one pixel of a trace.

The result and unit depends on the measurement format.

Note that for the MPHase format (simultaneous measurement of magnitude and phase), you can read out the magnitude data with the parameter `TRACE1` and the phase data with the parameter `TRACE2`.

Example

```
TRAC:DATA? TRACE1
```

Reads out the data for trace 1.

Characteristics

*RST value: -

SCPI: conform

7.4.6 Using Markers and Deltamarkers

7.4.6.1 Markers and Deltamarkers

The following commands are for setting and controlling markers and deltamarkers. If not otherwise noted, the numeric suffix <1...6> at MARKer or DELTamarkeR select the marker to be controlled.

The suffix <n> at CALCulate selects the measurement screen in dual trace mode and is in the range {1...2}.

The suffix <m> at MARKer selects the marker and is in the range {1...6}.

List of commands

- CALCulate<n>:DELTamarkeR<m>[:STATe] <State> (p. 55)
- CALCulate<n>:DELTamarkeR<m>:AOFF (p. 56)
- CALCulate<n>:DELTamarkeR<m>:MAXimum[:PEAK] (p. 56)
- CALCulate<n>:DELTamarkeR<m>:MAXimum:NEXT (p. 56)
- CALCulate<n>:DELTamarkeR<m>:MINimum[:PEAK] (p. 56)
- CALCulate<n>:DELTamarkeR<m>:X <Coordinate> (p. 57)
- CALCulate<n>:DELTamarkeR<m>:X:RELative <Distance> (p. 57)
- CALCulate<n>:DELTamarkeR<m>:Y? (p. 58)
- CALCulate<n>:MARKer<m>[:STATe] <State> (p. 59)
- CALCulate<n>:MARKer<m>:AOFF (p. 59)
- CALCulate<n>:MARKer<m>:MAXimum[:PEAK] (p. 59)
- CALCulate<n>:MARKer<m>:MAXimum:NEXT (p. 60)
- CALCulate<n>:MARKer<m>:MINimum[:PEAK] (p. 60)
- CALCulate<n>:MARKer<m>:MODE <MarkerMode> (p. 155)
- CALCulate<n>:MARKer<m>:POSition <StepSize> (p. 60)
- CALCulate<n>:MARKer<m>:X <Coordinate> (p. 61)
- CALCulate<n>:MARKer<m>:X:SLIMits[:STATe] <State> (p. 61)
- CALCulate<n>:MARKer<m>:X:SLIMits:LEFT <SearchLimit> (p. 62)
- CALCulate<n>:MARKer<m>:X:SLIMits:RIGHT <SearchLimit> (p. 62)
- CALCulate<n>:MARKer<m>:Y? (p. 156)

For a detailed description of commands not described below refer to "[Using Markers](#)" in CAT mode.

CALCulate<n>:MARKer<m>:MODE <MarkerMode>

This command selects the type of information a marker shows.

Parameter

ADMittance	admittance in complex format (real + imaginary)
IMPedance	impedance in complex format (real + imaginary)
NADMittance	standardized admittance in complex format (real + imaginary)
NIMPedance	standardized impedance in complex format (real + imaginary)
NORMal	normal marker

RPDB	reflection coefficient in complex format (magnitude (dB) + phase)
RPL	reflection coefficient in complex format (magnitude (lin) + phase)
RSCalar	reflection coefficient in complex format (real + imaginary)

Example

```
CALC:MARK:MODE ADM
```

Selects admittance in complex format with real and imaginary components

Characteristics

*RST value: NORMAl

SCPI: device-specific

CALCulate<n>:MARKer<m>:Y?

This command queries the measurement results at the marker position.

If necessary, the corresponding marker is activated first.

To get a valid result, you have to perform a complete sweep with synchronization to the sweep end between activating the delta marker and reading out the result. This is only possible in single sweep mode.

Return value

The return value depends on the marker format you have selected with

[CALCulate<n>:MARKer<m>:MODE](#).

ADMittance	<real part>, <imaginary part>
IMPedance	<real part>, <imaginary part>
NADMittance	<real part>, <imaginary part>
NIMPedance	<real part>, <imaginary part>
NORMAl	<value> = trace value
RPDB	<magnitude in dB>, <phase>
RPL	<magnitude linear>, <phase>
RSCalar	<real part>, <imaginary part>

Example

```
INIT:CONT OFF
```

```
CALC:MARK2 ON
```

Turns on single sweep mode and marker 2.

```
INIT;*WAI
```

```
CALC:MARK2:Y?
```

Performs a measurement and queries the marker position.

Characteristics

*RST value: –

SCPI: device-specific

7.4.6.2 Marker Functions

The following commands perform various kinds of analysis at the marker position.

The suffix <n> at DISPlay selects the measurement screen in dual trace mode and is in the range <1...2>.

List of commands

- [DISPlay<n>:IMPedance:REFErence:POSition <Impedance>](#) (p. 157)
- [DISPlay<n>:ZOOM:AREA\[:STAT\] <State>](#) (p. 157)
- [DISPlay<n>:ZOOM:FACTor <ZoomFactor>](#) (p. 158)
- [DISPlay<n>:ZOOM:X <HorizShift>](#) (p. 158)
- [DISPlay<n>:ZOOM:Y <VerticalShift>](#) (p. 158)

DISPlay<n>:IMPedance:REFErence:POSition <Impedance>

This command sets the reference impedance for the smith chart measurement format. The impedance can be between 1 mΩ and 10 kΩ.

Parameter

<Impedance>

Numeric value in the range from 1 mΩ to 10 kΩ.

Example

```
DISP:IMP:REF:POS 75 OHM
```

Sets the reference impedance to 75 Ohm.

Characteristics

*RST value: 50

SCPI: device-specific

DISPlay<n>:ZOOM:AREA[:STAT] <State>

This command turns the marker zoom function in a Smith chart on and off.

Parameter

<State>

ON | OFF

Example

```
DISP:ZOOM:AREA ON
```

Activates the marker zoom function.

Characteristics

*RST value: OFF

SCPI: device-specific

DISPlay<n>:ZOOM:FACTOR <ZoomFactor>

This command sets the zoom factor of the marker zoom function in a Smith chart.

Parameter

<ZoomFactor>

2 | 4 | 8

Example

DISP:ZOOM:FACT 4

Sets the zoom factor to 4

Characteristics

*RST value: -

SCPI: device-specific

DISPlay<n>:ZOOM:X <HorizShift>

This command shifts the zoom window horizontally in the Smith chart.

'0%' marks the center on the horizontal axis.

Parameter

<HorizShift>

Numeric value in the range from -50 % to 50 %.

Example

DISP:ZOOM:X 10

Shift the zoom window 10% to the right.

Characteristics

*RST value: 0

SCPI: device-specific

DISPlay<n>:ZOOM:Y <VerticalShift>

This command shifts the zoom window vertically in the Smith chart.

'0%' marks the center on the vertical axis.

Parameter

<VerticalShift>

Numeric value in the range from -50 % to 50 %.

Example

DISP:ZOOM:Y -25

Shifts the zoom window 25% down.

Characteristics

*RST value: 0

SCPI: device-specific

7.4.7 Configuring the Measurement

This chapter provides information on how to configure two-port measurements with the tracking generator. The structure follows the order of the actual operation sequence used when performing a measurement:

The suffix <n> at MEASurement selects the measurement screen in dual trace mode and is in the range from {1...2}.

- [Selecting the Measurement Port](#) on page 159
- [Calibrating the Measurement](#) on page 160
- [Selecting the Result Display](#) on page 162
- [Selecting the Measurement Format](#) on page 162

It also deals with configuring the Vector Voltmeter (Option R&S ZVH-K45).

- [Configuring the Vector Voltmeter \(option R&S ZVH-K45\)](#) on page 165

To perform the actual measurement, use the commands described in section "[Performing and Triggering the Measurement](#)".



Commands independent of the operating mode

Note that some of the commands for configuring two-port measurements are also valid for other operating modes. If a command is available in another mode, it is indicated by the list in the respective section.

7.4.7.1 Selecting the Measurement Port

The following commands select the measurement port.

List of commands

- [MEASurement:PORT <Port>](#) (p. 65)

7.4.7.2 Selecting the Measurement Mode

The following commands select the measurement mode for two-port measurements.

List of commands

- [MEASurement<n>:MODE <MeasMode>](#) (p. 160)

MEASurement<n>:MODE <MeasMode>

This command sets the measurement mode for network analysis measurements.

Parameter

<MeasMode>

SCALar	Scalar measurements.
VECTor	Vector measurements.

Example

```
MEAS:MODE SCAL
Starts a scalar measurement.
```

Characteristics

*RST value: VECTor
SCPI: device-specific

7.4.7.3 Calibrating the Measurement

The following commands query and control calibration for two-port measurements.

List of commands

- [CALCulate:CALKit:USER:OFFSet<p>:LENGth <ElecLengthOffs>](#) (p. 160)
- [CALibration:MODE?](#) (p. 161)
- [CALibration:STATus?](#) (p. 161)

The suffix <p> selects the measurement port. It is in the range <1...2>.

CALCulate:CALKit:USER:OFFSet<p>:LENGth <ElecLengthOffs>

This command sets the offset of the electrical length. It is taken into account for phase measurements and in the Smith Chart when phase correction for additional cables and adapters has to be performed.

The offset is taken into account for phase measurements and the Smith chart if you perform phase correction for additional cables and adapters.

Parameter

<ElecLengthOffset>

Numeric value in the range from 0 mm to 100 m.

Example

CALK:USER:OFFS2:LENG 500 MM

Sets the offset length of port 2 to 500 millimeter.

Characteristics

*RST value: 0 mm

SCPI: device-specific

CALibration:MODE?

This command queries if the current measurement is calibrated.

This command is a query and therefore has no *RST value.

Return value

0	R&S ZVH is not calibrated.
1	R&S ZVH is calibrated.

Example

CAL:MODE?

Queries the calibration state.

Characteristics

*RST value: -

SCPI: device-specific

CALibration:STATus?

This command queries if the R&S ZVH is fully calibrated for the current measurement.

This command is a query and therefore has no *RST value.

Return value

NORMALized	Full factory calibration or user calibration.
APPROximated	Approximate calibration: measurement uncertainty must be anticipated.

Example

CAL:STAT?

Queries the calibration status of the R&S ZVH.

Characteristics

*RST value: -

SCPI: device-specific

7.4.7.4 Selecting the Result Display

The following commands select the result display for two-port measurements.

List of commands

- [MEASurement<n>:FUNCTION:SElect <ResultDisplay>](#) (p. 162)

MEASurement<n>:FUNCTION:SElect <ResultDisplay>

This command selects the result display.

Parameter

<ResultDisplay>

S11 | S12 | S21 | S22

Example

```
MEAS:FUNC:SEL S11
```

Characteristics

*RST value: S11

SCPI: device-specific

7.4.7.5 Selecting the Measurement Format

The following commands are for selecting and configuring the measurement formats available for two-port measurements.

List of commands

- [CALCulate:TRACe:CABLe:LENGth\[:STATe\] <State>](#) (p. 162)
- [CALCulate:TRACe:CABLe:LENGth:RESult?](#) (p. 163)
- [CALCulate:TRACe:CABLe:TIME\[:STATe\] <State>](#) (p. 163)
- [CALCulate:TRACe:CABLe:TIME:RESult?](#) (p. 163)
- [DISPlay:GDElay:APERture:STEP <Aperture>](#) (p. 164)
- [MEASurement<n>:FORMat <MeasFormat>](#) (p. 164)

CALCulate:TRACe:CABLe:LENGth[:STATe] <State>

This command turns the electrical length format on and off.

Parameter

<State>

ON | OFF

Example

```
CALC:TRAC:CABL:LENG ON
```

Activates the electrical cable length.

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate:TRACe:CABLe:LENGth:RESult?

This command queries the results of the electrical cable length.

This command is a query and therefore has no *RST value.

Return value

<ElLength>

Numerical value in mm

Example

```
CALC:TRAC:CABL:LENG:RES?
```

Queries the measurement result of the electrical cable length.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:TRACe:CABLe:TIME[:STATe] <State>

This command turns the delay time format on and off.

Parameter

<State>

ON | OFF

Example

```
CALC:TRAC:CABL:TIME ON
```

Activates the cable delay time.

Characteristics

*RST value: OFF

SCPI: device-specific

CALCulate:TRACe:CABLe:TIME:RESult?

This command queries the results of the cable delay time.

This command is a query and therefore has no *RST value.

Return value

<DelayTime>

Numerical value in s.

Example

```
CALC:TRAC:CABL:TIME:RES?
```

Queries the measurement result of the delay time.

Characteristics

*RST value: -

SCPI: device-specific

DISPlay:GDElay:APERture:STEP <Aperture>

This command sets the aperture steps for the group delay measurement format.

Parameter

<Aperture>

Numeric value in the range from 1 to 630.

Example

DISP:GDEL:APER:STEP 100

Defines an aperture size of 100w.

Characteristics

*RST value: 10

SCPI: device-specific

MEASurement<n>:FORMat <MeasFormat>

This command selects the measurement format.

Note:

For transmission measurements only the Magnitude, Phase, Magnitude+Phase and GDelay formats are available.

Parameter

GDElay	Group delay format.
LOSS	Cable loss format.
MAGNitude	Magnitude format.
PHASe	Phase format.
REFlection	Refelction coefficient format.
SMITH	Smith chart format.
VSWR	VSWR format.

Example

MEAS:MODE VECT

Switches to vector measurement mode.

MEAS:FUNC:REFL ON

Activates reflection measurement.

MEAS:FORM SMITH

Displays the reflection in a Smith Chart.

Characteristics

*RST value: MAGNitude

SCPI: device-specific

7.4.7.6 Configuring the Vector Voltmeter (option R&S ZVH-K45)

The following commands configure the vector voltmeter.



Availability of remote commands for the Vector Voltmeter

Note that the listed remote commands take effect only if option R&S ZVH-K45 Vector Voltmeter is installed.

List of commands

- [CALCulate:VVMeter:MAGNitude:REference?](#) (p. 165)
- [CALCulate:VVMeter:MAGNitude:RESult?](#) (p. 165)
- [CALCulate:VVMeter:PHASe:REference?](#) (p. 166)
- [CALCulate:VVMeter:PHASe:RESult?](#) (p. 166)
- [CALCulate:VVMeter:REference\[:STATe\] <State>](#) (p. 166)

CALCulate:VVMeter:MAGNitude:REference?

This command queries the reference value for the magnitude.

To get a result, you first have to turn on the reference value with [CALCulate:VVMeter:REference\[:STATe\] <State>](#).

This command is a query and therefore has no *RST value.

Return value

<ReferenceValue>

Reference value for the magnitude in dB.

Example

```
CALC:VVM:PHAS:REF?
```

Queries the reference values for the phase.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:VVMeter:MAGNitude:RESult?

This command queries the magnitude of the measurement results.

This command is a query and therefore has no *RST value.

Return values:

<Magnitude>

Magnitude of the return loss in dB.

Example

```
CALC:VVM:MAGN:RES?
```

Queries the current return loss of the DUT

Characteristics

*RST value: -
SCPI: device-specific

CALCulate:VVMeter:PHASe:REFeRence?

This command queries the reference value for the phase of the DUT.

To get a result, you first have to turn on the reference value with
[CALCulate:VVMeter:REFeRence\[:STATe\] <State>](#).

This command is a query and therefore has no *RST value.

Return values

<ReferenceValue>
Reference value for the phase in degrees.

Example

```
CALC:VVM:PHAS:REF?
```

Characteristics

*RST value: -
SCPI: device-specific

CALCulate:VVMeter:PHASe:RESult?

This command queries the phase of the measurement results.

This command is a query and therefore has no *RST value.

Return values

<Phase>
Phase of the return loss in degrees.

Example

```
CALC:VVM:PHAS:RES?
```

Queries the current phase of the DUT

Characteristics

*RST value: -
SCPI: device-specific

CALCulate:VVMeter:REFeRence[:STATe] <State>

This command saves the current measurement values as reference values. The reference values can be used for comparison measurements.

Parameter

<State>
ON | OFF

Example

CALC:VVM:REF ON

Activates the reference values.

Characteristics

*RST value: OFF

SCPI: device-specific

7.5 Remote Commands of the Power Meter

The chapter provides information on remote commands that configure and perform power measurements with the power sensor. These commands are available in power meter mode only.



Availability of remote commands for Power Sensor measurements

Note that the listed remote commands take effect only if a power sensor is connected.

7.5.1 Using Power Sensors

Contents

[Setting the Frequency](#) on page 168

[Configuring Power Level Readout](#) on page 169

[Defining the Measurement Time](#) on page 171

[Zeroing of the Power Sensor](#) on page 171

7.5.1.1 Setting the Frequency

The following chapter describes commands necessary to define frequency settings.

List of commands

- [\[SENSe:\]PMETer:FREQuency <Frequency>](#) (p. 168)
- [CALCulate:PMETer:CPOWer:BANDwidth <Bandwidth>](#) (p. 169)

[SENSe:]PMETer:FREQuency <Frequency>

This command sets the frequency of the power sensor.

Parameter

<Frequency>

Numeric value in Hz.

The available value range is specified in the data sheet.

Example

```
PMET:FREQ 500 MHZ
```

Sets the power sensor's frequency to 500 MHz

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:PMETer:CPOWer:BANDwidth <Bandwidth>

This command defines the channel bandwidth.

Available for the channel power meter.

Parameter

<Bandwidth>

Numeric value in Hz.

Example

```
CALC:PMET:CPOW:BAND 5 MHZ
```

Sets the channel bandwidth to 5 MHz

Characteristics

*RST value: -

SCPI: device-specific

7.5.1.2 Configuring Power Level Readout

The following chapter describes commands that configure the power level readout.

List of commands

- [CALCulate:PMETer:RELative\[:MAGNitude\] <RefValue>](#) (p. 169)
- [CALCulate:PMETer:RELative\[:MAGNitude\]:AUTO](#) (p. 169)
- [CALCulate:PMETer:RELative\[:MAGNitude\]:OFFSet <Offset>](#) (p. 170)
- [UNIT<z>:PMETer:POWer <Unit>](#) (p. 170)

CALCulate:PMETer:RELative[:MAGNitude] <RefValue>

This command sets the reference value for relative measurements.

Parameter

<RefValue>

Numeric value in dBm.

Example

```
CALC:PMET:REL 30
```

The the reference value to 30 dBm.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:PMETer:RELative[:MAGNitude]:AUTO ONCE

This command sets the current measurement result as the reference level for relative measurements.

This command is an event and therefore has no *RST value and no query.

Parameter

ONCE

Example

CALC:PMET:REL ONCE

Adjusts the reference level to the measurement result.

Characteristics

*RST value: -

SCPI: device-specific

CALCulate:PMETer:RELative[:MAGNitude]:OFFSet <Offset>

This command sets an offset for the reference value.

Parameter

<Offset>

Numeric value in dB.

Example

CALC:PMET:REL:OFFS -10

Defines an offset of -10 dB.

Characteristics

*RST value: -

SCPI: device-specific

UNIT<z>:PMETer:POWER <Unit>

This command selects the unit of the power sensor.

The suffix <z>at UNIT has the following effects:

Power Measurement with R&S ZVH-Z1, R&S ZVH-Z18 and USB power sensors:

Unit 1	Power unit.
Unit 2	Not available.

Power Measurement with R&S ZVH-Z14 and R&S ZVH-Z44:

Unit 1	Forward power.
Unit 2	Reflected power.

Parameter

<Unit>

DBM | WATT | W | DB | VSWR

Note on the parameter DB: when applied to UNIT1, the power is relative to the reference level, when applied to UNIT2, the return loss is displayed.

Note on the parameter VSWR: the parameter is only available if applied to UNIT2.

Example

```
UNIT1:PMET:POW DBM
```

When measuring with the R&S ZVH-Z1, R&S ZVH-Z18 or USB power sensors: sets unit to dBm.

When measuring with the R&S ZVH-Z14 or R&S ZVH-Z44: sets unit of forward power to dBm.

Characteristics

*RST value: -
SCPI: device-specific

7.5.1.3 Defining the Measurement Time

The following chapter describes commands to define the measurement time of the power sensor.

- [\[SENSe:\]PMETer:MTIME <MeasTime>](#) (p. 171)

[SENSe:]PMETer:MTIME <MeasTime>

This command sets the duration of measurements.

Available for measurements with a power sensor.

Parameter

<MeasTime>
SHORT | NORMal | LONG

Example

```
PMET:MTIME SHOR
```

Sets a short measurement time for power measurements.

Characteristics

*RST value: -
SCPI: device-specific

7.5.1.4 Zeroing of the Power Sensor

List of commands

- [CALibration:PMETer:ZERO:AUTO](#) (p. 171)

CALibration:PMETer:ZERO:AUTO ONCE

This commands starts to zero the power sensor.

This command is an event and therefore has no *RST value and no query.

Parameter

ONCE

Example

CAL:PMET:ZERO:AUTO ONCE
Starts to zero the power meter.

Characteristics

*RST value: -
SCPI: device-specific

7.5.1.5 Forward Power Display

Note that the forward power is only available in conjunction with the R&S ZVH-Z14 or R&S ZVH-Z44.

List of commands

- [\[SENSe:\]PMETer:DETector\[:FUNction\] <PowerDisplay>](#) (p. 172)

[SENSe:]PMETer:DETector[:FUNction] <PowerDisplay>

This command selects the forward power display of the power sensor.

Parameter

<PowerDisplay>

AVERage	Displays the average power.
PENvelope	Displays the peak envelope power.

Example

PMET:DET AVER
Selects the Average weighting mode.

Characteristics

*RST value: -
SCPI: device-specific

7.5.1.6 Defining the Video Bandwidth

Selecting a video bandwidth is only possible when you are measuring the peak envelope power with the R&S ZVH-Z44 power sensor based on a customized (= user) standard.

See the following commands for more information about these conditions:

- [\[SENSe:\]PMETer:DETector\[:FUNction\] <PowerDisplay>](#)
- [CALCulate:PMETer:PRESet\[:STATe\] <State>](#)
- [CALCulate:PMETer:PRESet:SElect <Standard>](#)

List of commands

- [CALCulate:PMETer:PRESet:BANDwidth:VIDeo <Bandwidth>](#) (p. 173)

CALCulate:PMETer:PRESet:BANDwidth:VIDeo <Bandwidth>

This command defines the video bandwidth of the R&S ZVH-Z44 power sensor.

Parameter

<Bandwidth>

Video bandwidth of the power sensor in Hz.

Example

`CALC:PMET:PRESet:BAND:VID 10MHZ`

Defines a video bandwidth of 10 MHz.

Characteristics

*RST value: -

SCPI: device-specific

7.5.1.7 Reading Out Measurement Results**List of commands**

- [FETCh<z>:PMETer?](#) (p. 173)

FETCh<z>:PMETer?

This command queries the results of measurements with the power sensor.

Return value

The return values depend on the power sensor in use and the selected suffix at FETCh.

Measurements with R&S ZVH-Z1 or R&S ZVH-Z18:

FETC1:PMET? power in dBm

FETC2:PMET? n/a

Measurements with R&S ZVH-Z14 or R&S ZVH-Z44

FETC1:PMET? forward power in dBm

FETC2:PMET? reflected power in dBm

Example

`FETC2:PMET?`

Returns nothing for R&S ZVH-Z1 / R&S ZVH-Z18 and the reflected power for R&S ZVH-Z14 / Z44.

Characteristics

*RST value: -
 SCPI: device-specific

7.5.1.8 Selecting a Telecommunication Standard

These commands apply radio communication standards to measurements with the power sensor.

Note that the selection of a standard is available only for the power sensors R&S FSH-Z1, -Z14, -Z18 and -Z44.

List of commands

- [CALCulate:PMETer:PRESet\[:STATe\] <State>](#) (p. 174)
- [CALCulate:PMETer:PRESet:SElect <Standard>](#) (p. 174)

CALCulate:PMETer:PRESet[:STATe] <State>

This command turns the use of a standard on and off.

Parameters

<State>
 ON | OFF

Example

```
CALC:PMET:PRESet ON
```

Activates usage of a standard

Characteristics

*RST value: -
 SCPI: device-specific

CALCulate:PMETer:PRESet:SElect <Standard>

This command selects the standard for power sensor measurements.

Parameter

<Standard>
 GSM | EDGE | WCDMA | CDMAOne | CDMA2000 | DVBT | DAB | TETRA | USER

Example

```
CALC:PMET:PRESet:SElect GSM
```

Selects the GSM standard for power sensor measurements

Characteristics

*RST value: -
 SCPI: device-specific

7.6 File Management

The following commands perform various tasks in the context of file management.

These commands are independent from the operating mode.

List of commands

- [MMEMory:CATalog?](#) (p. 175)
- [MMEMory:CATalog:DIRectories?](#) (p. 176)
- [MMEMory:CDIRectory <Directory>](#) (p. 176)
- [MMEMory:COpy <SourceFile>,<DestinationFile>](#) (p. 176)
- [MMEMory:DATA <FileName>\[,<BlockData>\]](#) (p. 177)
- [MMEMory:DELeTe <File>](#) (p. 178)
- [MMEMory:FILE <File>](#) (p. 178)
- [MMEMory:FILE:DATE <FileName>,<Date>](#) (p. 178)
- [MMEMory:FILE:TIME <FileName>,<Time>](#) (p. 179)
- [MMEMory:INIT](#) (p. 179)
- [MMEMory:LOAD:STATe 1,<FileName>](#) (p. 180)
- [MMEMory:MDIRectory <Directory>](#) (p. 180)
- [MMEMory:MOVE <SourceFile>,<NewFileName>](#) (p. 180)
- [MMEMory:RDIRectory <Directory>](#) (p. 181)
- [MMEMory:STORe:STATe 1,<FileName>](#) (p. 181)
- [SYSTem:SET:LOCK <FileName>](#) (p. 182)
- [SYSTem:SET:UNLock <FileName>](#) (p. 182)

MMEMory:CATalog?

This command queries the files of the current directory.

You can select directories with [MMEMory:CDIRectory <Directory>](#).

This command is a query and therefore has no *RST value.

Return value

<UsedDiskSpace>,<FreeDiskSpace>,<FileName_1>,<SizeFile_1><Modification
DateFile_1>,<ModificationTimeFile_1>,...,<FileName_n>,<SizeFile_n>
<ModificationDateFile_n>,<ModificationTimeFile_n>

Example

```
MMEM:CDIR '\Public\Limit Lines'
Opens directory 'Limit Lines'
```

```
MMEM:CAT?
Returns all files in \Public\Limit Lines
```

Characteristics

*RST value: -
SCPI: conform

MMEMory:CATalog:DIRectories?

This command queries the directories of the current directory.

This command is a query and therefore has no *RST value.

Return value

<UsedMemory>,<FreeMemory>,<DirName_1>,<ModificationDateDir_1>,
<ModificationTimeDir_1>,...,<DirName_n>,<ModificationDateDir_n>,
<ModificationTimeDir_n>

Example

```
MMEM:CDIR '\Public'
```

Opens directory \Public.

```
MMEM:CAT:DIR?
```

Returns all directories in the \Public directory

Characteristics

*RST value: -

SCPI: device-specific

MMEMory:CDIRectory <Directory>

This command changes the current directory.

Parameter

<Directory>

String containing the path to another directory.

Example

```
MMEM:CDIR '\Public'
```

Opens directory \Public.

Characteristics

*RST value: -

SCPI: conform

MMEMory:COPY <SourceFile>,<DestinationFile>

This command copies one or more files to another directory.

This command is an event and therefore has no *RST value and no query.

Parameter

<SourceFile>

String containing the path and file name of the source file.

<DestinationFile>

String containing the path and name of the destination file.

Example

```
MMEM: COPY
'\Public\Standards\cdmaOne.obwstd', '\\USB\cdmaOne.std'
```

Copies the cdmaOne standard file file to a memory stick.

Characteristics

*RST value: -
SCPI: conform

MMEMory:DATA <FileName>[,<BlockData>]

This command writes block data into a file. The delimiter must be set to EOI to obtain error-free data transfer.

When you query the contents of a file, you can save them in a file on the remote control computer.

The command is useful for reading stored settings files or trace data from the instrument or for transferring them to the instrument.

Parameter

<FileName>

String containing the path and file name.

<BlockData>

Data block with the structure

#	hash sign
<number>	length of the length information
<number>	length information of the binary data (number of bytes)
<data>	binary data with the indicated number of bytes

Example

```
MMEM:NAME '\Public\User\Testfile.txt'
```

Creates a new file called 'Testfile.txt'.

```
MMEM:DATA '\Public\User\Testfile.txt',#220
```

Contents of the file

The parameter mean:

- '\Public\...' selects the target file
- #2: hash sign and length of the length information (20 bytes = 2 digits)
- 20: indicates the number of subsequent binary data bytes
- Contents of the file: store 20 binary bytes (characters) to the file

```
MMEM:DATA? '\Public\User\Testfile.txt'
```

Transfers the contents of the file 'Testfile.txt' to the control computer.

Characteristics

*RST value: -
SCPI: conform

MMEMory:DELeTe <File>

This command deletes a file.

Parameter

<File>

String containing the path and file name of the file to delete.

Example

```
MMEM:DEL '\Public\Screen Shots\Screen0001.png'
```

Deletes the file Screen0001.png.

Characteristics

*RST value: -
SCPI: conform

MMEMory:FILE <File>

This command creates a file.

Parameter

<File>

String containing the file name.

Example

```
MMEM:FILE 'TEST.TXT'
```

Creates the file TEST.TXT

Characteristics

*RST value: -
SCPI: conform

MMEMory:FILE:DATE <FileName>,<Date>

This command sets the date of a file.

Parameter

<FileName>

String containing the path and file name.

<Date>

Numeric values indicating the date

You have to enter the date as comma separated values after the string with the file name. The sequence is year,month,day.

The available value range is 1980...2099, 1...12, 1...31

Example

```
MMEM:FILE:DATE '\Public\Screen  
Shots\Screen0001.png', 2006, 04, 01
```

Sets the date to April, 1st, 2006.

MMEM:FILE:DATE? '\Public\Screen Shots\Screen0001.png'
Returns the modification date of the file Screen0001.png.

Characteristics

*RST value: -
SCPI: conform

MMEMory:FILE:TIME <FileName>,<Time>

This command sets the time of a file. The sequence of entry is hour, minute, second.

Parameter

<FileName>

String containing the path and file name.

<Time>

Numeric values indicating the time.

You have to enter the time as comma separated values after the string with the file name. The sequence is hour,minute,second.

The available value range is 0...23, 0...59, 0...59.

Example

MMEM:FILE:TIME '\Public\Screen Shots\Screen0006.png',11,04,00
Sets the time to 11:04:00

Characteristics

*RST value: -
SCPI: conform

MMEMory:INIT

This command formats the indicated drive.

Note

Formatting deletes all data stored on the memory drive.

This command is an event and therefore has no *RST value and no query.

Example:

MMEM:INIT

Formats and deletes all data from the drive.

Characteristics:

*RST value: -
SCPI: conform

MMEMory:LOAD:STATe 1,<FileName>

This command loads the settings from a *.set file.

Parameter

<FileName>

String containing the path and file name.

Example

```
MMEM:LOAD:STAT 1, '\Public\Datasets\Dataset001.set'
```

Loads the settings from the file Dataset001.

Characteristics

*RST value: -
SCPI: conform

MMEMory:MDIRectory <Directory>

This command creates a new directory.

This command is an event and therefore has no *RST value and no query.

Parameter

<Directory>

String containing the path and new directory name.

Example

```
MMEM:MDIR '\Public\USER'
```

Creates the a directory called 'User'

Characteristics

*RST value: -
SCPI: device-specific

MMEMory:MOVE <SourceFile>,<NewFileName>

This command renames files, if <file_destination> contains no path. Otherwise the file is moved to the indicated path and stored under the file name specified there.

This command is an event and therefore has no *RST value and no query.

Parameter

<SourceFile>

String containing the path and file name of the source file.

<DestinationFile>

String containing the path and name of the destination file.

Example

```
MMEM:MOVE '\Public\Screen  
Shots\Screen0002.png', '\Public\Screen Shots\Screen0001.png'
```

Renames Screen0002.png to Screen0001.png

```
MMEM:MOVE '\Public\Screen  
Shots\Screen0001.png', '\Public\Test\Pic1.png'  
Moves file Screen0006.png to the 'Test' folder and renames the file Pic1.png
```

Characteristics

*RST value: -
SCPI: conform

MMEMory:RDIRECTory <Directory>

This command deletes the indicated directory. The directory name includes the path and may also include the drive name. The path name complies with DOS conventions.

This command is an event and therefore has no *RST value and no query.

Parameter

<Directory>
String containing the path of the directory to delete.

Example

```
MMEM:RDIR '\Public\Screen Shots\  
Deletes the directory 'Screen Shots'.
```

Characteristics

*RST value: -
SCPI: device-specific

MMEMory:STORe:STATe 1,<FileName>

This command stores the current device settings in a *set file.

This command is an event and therefore has no *RST value and no query.

Parameter

1,<FileName>
String containing the path and name of the destination file.

Example

```
MMEM:STOR:STAT 1, 'DATASET001.SET'  
Saves the current device settings in the file DATASET001.SET.
```

Characteristics

*RST value: -
SCPI: conform

SYSTem:SET:LOCK <FileName>

This command adds write-protection to a dataset.

Parameter

<FileName>

String containing the path and name of the dataset.

Example

```
SYST:SET:LOCK 'Dataset001.set'
```

Protects the file Dataset001.set from overwriting.

Characteristics

*RST value: -

SCPI: device-specific

SYSTem:SET:UNLock <FileName>

This command removes write-protection from a dataset.

Parameter

<FileName>

String containing the path and name of the dataset.

Example

```
SYST:SET:UNL 'Dataset001.set'
```

Removes write-protection from the file Dataset001.set.

Characteristics

*RST value: -

SCPI: device-specific

7.7 Making and Storing Screenshots

The following commands manage screenshots.

These commands are independent from the operating mode.

List of commands

- [DISPlay:WINDow:STORe](#) (p. 183)
- [HCOPy:DEVice:LANGuage](#) (p. 183)
- [HCOPy\[:IMMediate\]](#) (p. 184)
- [MMEMory:NAME <FileName>](#) (p. 184)

DISPlay:WINDow:STORe

This command makes a screenshot of the current display contents in png or jpg format and stores it on the R&S ZVH internal memory.

You can select a file name for the screenshot in png format with [MMEMory:NAME <FileName>](#) and select the file format of the screenshot with [HCOPy:DEVice:LANGuage](#).

This command is an event and therefore has no *RST value and no query.

Example

```
HCOP:DEV:LANG PNG
MMEM:NAME '\Public\Screen Shots\Test.png'
DISP:WIND:STOR
```

Makes and stores a screenshot of the current screen in a file 'Test.png'.

Characteristics

*RST value: -
SCPI: device-specific

HCOPy:DEVice:LANGuage

This command selects the file format for screenshots.

Parameter

PNG | JPG

Example

```
HCOP:DEV:LANG PNG
Selects the png format for screenshots.
```

Characteristics

*RST value: -
SCPI: device-specific

HCOPy[:IMMEDIATE]

This command makes a screenshot of the current display contents in png format and stores it on the R&S ZVH internal memory.

You can select a file name for the screenshot in png format with `MMEMory:NAME <FileName>` and select the file format of the screenshot with `HCOPy:DEvice:LANGuage`.

To make a screenshot in jpg format, use `DISPlay:WINDow:STORe`.

This command is an event and therefore has no *RST value and no query.

Example

```
HCOP:DEV:LANG PNG
MMEM:NAME '\Public\Screen Shots\Test.png'
HCOP
```

Makes and stores a screenshot of the current screen in a file 'Test.png'.

Characteristics

*RST value: -
SCPI: device-specific

MMEMory:NAME <FileName>

This command defines the path and file name that the R&S FSH uses for storing screenshots (see `HCOPy[:IMMEDIATE]`). The path and file name comply with DOS conventions.

This command is an event and therefore has no *RST value and no query.

Parameter

<FileName>
String containing the file name.

Example

```
MMEM:NAME 'Public\Screenshots\Test.png'
```

Stores the screenshot on the in the corresponding directory on the R&S ZVH.

Characteristics

*RST value: -
SCPI: device-specific

7.8 Configuring Data Capture

The following commands configure the data capture.

These commands are independent from the operating mode.

List of commands

- [SYSTem:CAPTure:COUNter <Counter>](#) (p. 185)
- [SYSTem:CAPTure:DATaset\[:STATe\] <State>](#) (p. 185)
- [SYSTem:CAPTure:GPX\[:STATe\] <State>](#) (p. 186)
- [SYSTem:CAPTure:SCReen\[:STATe\] <State>](#) (p. 186)

SYSTem:CAPTure:COUNter <Counter>

This command defines the start of the file name counter.

The counter numbers the files stored when you capture data (screenshots, datasets etc.).

Parameter

<Counter>

String containing the number with which to start numbering files.

Example

```
SYST:CAPT:COUN '0100'
```

Starts numbering files with 0100, e.g. Measurement0100.png.

Characteristics

*RST value: '0000'

SCPI: device-specific

SYSTem:CAPTure:DATaset[:STATe] <State>

This command includes or excludes datasets from the data capture.

Parameter

<State>

ON | OFF

Example

```
SYST:CAPT:DAT ON
```

Includes datasets into the data capture

Characteristics

*RST value: OFF

SCPI: device-specific

SYSTem:CAPTure:GPX[:STATe] <State>

This command includes or excludes GPX information from the data capture.

Parameter

<State>
ON | OFF

Example

SYST:CAPT:GPX ON
Includes GPX information into the data capture

Characteristics

*RST value: OFF
SCPI: device-specific

SYSTem:CAPTure:SCReen[:STATe] <State>

This command includes or excludes screenahots from the data capture.

Parameter

<State>
ON | OFF

Example

SYST:CAPT:SCR ON
Includes screenshots into the data capture

Characteristics

*RST value: ON
SCPI: device-specific

7.9 Saving Events

The following commands configure the circumstances under which the R&S ZVH saves events.

These commands are independent from the operating mode.

Using the commands requires an GPS receiver and a storage device (SD card or memory stick).

List of commands

- [SYSTem:SOEVent:DIStance:INterval <Distance>](#) (p. 187)
- [SYSTem:SOEVent:LIMits:MODE <Mode>](#) (p. 187)
- [SYSTem:SOEVent:RECORDing:STORage <Device>](#) (p. 188)
- [SYSTem:SOEVent:SOURce <EventType>](#) (p. 188)
- [SYSTem:SOEVent:TIME:INterval <Time>](#) (p. 189)
- [SYSTem:SOEVent\[:STATe\] <State>](#) (p. 189)

SYSTem:SOEVent:DIStance:INterval <Distance>

This command defines a distance that you must cover before the R&S ZVH saves another coordinate.

Parameter

<Distance>

Distance between one coordinate and the next.

Example

```
SYST:SOEV ON
```

Turns on saving coordinates on an event.

```
SYST:SOEV:REC:STOR USB
```

Selects an USB device as the storage device.

```
SYST:SOEV:SOUR DIST
```

```
SYST:SOEV:DISt:INT 5
```

Saves the coordinates every 5 m.

Characteristics

*RST value: 1 m

SCPI: device-specific

SYSTem:SOEVent:LIMits:MODE <Mode>

This command selects the limit check condition that must occur in order to save a coordinate.

Parameter

<Mode>

FAILonly	Saves only sweeps that contain a limit check violation.
STARtonfail	Starts to save all sweeps from the moment a limit check fails.
STOPonfail	Saves all sweeps until a limit check fails.

Example

```
SYST:SOEV:SOUR LIM
```

```
SYST:SOEV:LIM:MODE FAIL
```

Saves all sweeps that contain a violation of a limit check.

Characteristics

*RST value: STAR

SCPI: device-specific

SYSTem:SOEVent:RECORDing:STORage <Device>

This command selects the storage device to save the coordinates to.

Parameter

<Device>

SDCard	Saves coordinates to an SD card.
USB	Saves coordinates to an USB device.

Example

See [SYSTem:SOEVent:DISTance:INTerval <Distance>](#).

Characteristics

*RST value: SDCard

SCPI: device-specific

SYSTem:SOEVent:SOURce <EventType>

This command selects the type of event that triggers saving the coordinates of your current location.

Parameter

<EventType>

ALLSweeps	Saves coordinates after each sweep.
DISTanceint	Saves coordinates after a certain distance has been covered.
LIMitsfail	Saves coordinates when a limit check has failed.
TIMEinterval	Saves coordinates after a certain length of time has passed.

Example

See [SYSTem:SOEVent:DISTance:INTerval <Distance>](#).

Characteristics

*RST value: TIMEinterval

SCPI: device-specific

SYSTem:SOEVent:TIME:INTerval <Time>

This command defines a time interval that must pass before the R&S ZVH saves another coordinate.

Parameter

<Time>

Time that must pass between one coordinate and the next.

Example

```
SYST:SOEV ON
```

Turns on saving coordinates on an event.

```
SYST:SOEV:REC:STOR USB
```

Selects an USB device as the storage device.

```
SYST:SOEV:SOUR TIM
```

```
SYST:SOEV:TIME:INT 5
```

Saves the coordinates every 5 seconds.

Characteristics

*RST value: 1 s

SCPI: device-specific

SYSTem:SOEVent[:STATE] <State>

This command turns saving of your current coordinates in case of certain events on and off.

Parameter

<State>

ON | OFF

Example

See [SYSTem:SOEVent:DISTance:INTerval <Distance>](#).

Characteristics

*RST value: OFF

SCPI: device-specific

7.10 Configuring the Instrument

The following commands configure general instrument settings.

These commands are independent from the operating mode.

Contents

[Mode Selection](#) on page 190

[Controlling the GPS Receiver](#) on page 192

[Display Configuration](#) on page 197

[Audio Settings](#) on page 199

[Setting up a Network Connection](#) on page 201

[System Settings](#) on page 203

7.10.1 Mode Selection

This chapter describes all commands that select the operating mode of the R&S ZVH.

List of commands

- [INSTrument\[:SElect\] <OperatingMode>](#) (p. 190)
- [INSTrument:NSElect <OperatingMode>](#) (p. 191)

INSTrument[:SElect] <OperatingMode>

This command selects the operating mode.

Parameter

<OperatingMode>

ACT	cable and antenna analyzer
NAN	network analyzer
PM	power meter
SANalyzer	spectrum analyzer
VVMeter	vector voltmeter

Example

```
INST SAN
```

Selects spectrum analyzer mode.

Characteristics

*RST value: ACT

SCPI: conform

INSTrument:NSElect <OperatingMode>

This command selects the operating mode.

Parameter

1	spectrum analyzer
2	network analyzer
5	power meter
11	Cable and antenna analyzer
12	vector voltmeter

Example

```
INST:NSEL 1
```

Selects spectrum analyzer mode.

Characteristics

*RST value: 11

SCPI: conform

7.10.2 Controlling the GPS Receiver

This chapter describes all commands that control the GPS receiver.

List of commands

- [SYSTem:POSition:ALTitude?](#) (p. 192)
- [SYSTem:POSition:COMPass:ANGLE?](#) (p. 192)
- [SYSTem:POSition:COMPass\[:STATe\] <State>](#) (p. 193)
- [SYSTem:POSition:COMPass:VALid?](#) (p. 193)
- [SYSTem:POSition:GPS\[:STATe\] <State>](#) (p. 193)
- [SYSTem:POSition:GPS:CONNected?](#) (p. 194)
- [SYSTem:POSition:GPS:CORRection:FREQUency?](#) (p. 194)
- [SYSTem:POSition:GPS:QUALity](#) (p. 194)
- [SYSTem:POSition:GPS:SATellites?](#) (p. 195)
- [SYSTem:POSition:LATitude?](#) (p. 195)
- [SYSTem:POSition:LONGitude?](#) (p. 196)
- [SYSTem:POSition:VALid?](#) (p. 196)

SYSTem:POSition:ALTitude?

This command queries the altitude of the current position of the R&S ZVH.

Return value

<Altitude>

Altitude in meters above sea level.

If the GPS receiver is inactive, this query returns 0.

Example

```
SYST:POS:ALT?
```

Return value would be, for example, 554.1

Characteristics:

*RST value: -

SCPI: device-specific

SYSTem:POSition:COMPass:ANGLE?

This command queries the compass information of your position.

Return value

<Angle>

Angle to magnetic north in degrees.

If the GPS receiver is inactive, this query returns 0.

Example

```
SYST:POS:COMP:ANGL?
```

Return value would be, for example, 90

Characteristics:

*RST value: -
SCPI: device-specific

SYSTem:POStion:COMPass[:STATe] <State>

This command turns the compass on and off.

Parameter

<State>
ON | OFF

Example

```
SYST:POS:COMP ON
```

Turns on the compass.

Characteristics:

*RST value: OFF
SCPI: device-specific

SYSTem:POStion:COMPass:VALid?

This command queries the validity of the compass information.

Example

```
SYST:POS:COMP:VAL?
```

Returns if the compass information is valid.

Characteristics:

*RST value: -
SCPI: device-specific

SYSTem:POStion:GPS[:STATe] <State>

This command turns the GPS receiver (R&S HA-Z240) on and off.

Note that the GPS receiver only works if a connection between the R&S ZVH and a GPS signal transmitter is established.

Parameter

<State>
ON | OFF

Example

```
SYST:POS:GPS ON
```

Activates the GPS receiver.

Characteristics:

*RST value: OFF
SCPI: device-specific

SYSTem:POSition:GPS:CONNected?

This command queries if the R&S ZVH is currently connected to the GPS receiver.

Return values

0	No connection to a satellite.
1	Connection to a satellite established.

Example

```
SYST:POS:GPS:CONN?
```

Characteristics:

*RST value: -
SCPI: device-specific

SYSTem:POSition:GPS:CORRection:FREQuency?

This command queries the frequency correction factor.

The R&S ZVH calculates this factor from a reference signal provided by the GPS receiver R&S HA-Z240. The reference signal is used to determine the deviation of the internal clock of the instrument. The deviation can be turned into a correction factor for the measured frequency.

Return values

<floating point value>

If the GPS receiver is inactive, this query returns 0.

Example

```
SYST:POS:GPS:CORR:FREQ?
```

Queries the frequency correction factor.

Characteristics:

*RST value: -
SCPI: device-specific

SYSTem:POSition:GPS:QUALity?

This command queries the quality of the GPS signal.

Return values

INSufficient | LOW | MEDium | HIGH | EXCellent

Example

```
SYST:POS:GPS:QUAL?
```

Characteristics:

*RST value: -
SCPI: device-specific

SYSTem:POSition:GPS:SATellites?

This command queries the number of tracked satellites.

Return values

<number of satellites>

Example

```
SYST:POS:GPS:SAT?
```

Characteristics:

*RST value: -

SCPI: device-specific

SYSTem:POSition:LATitude?

This command queries the latitude of the current position of the R&S ZVH.

Return values

<sign><degrees>,<minutes>,<seconds>

<sign>	No sign = northern hemisphere Negative sign (-) = southern hemisphere
<degrees>	Degrees of latitude (integer value)
<minutes>	Minutes of latitude (integer value)
<seconds>	Seconds of latitude (floating point value)

Example

```
SYST:POS:LAT?
```

Return value would be, for example, 48,7,40.0 for 48°, 7', 40.0" in the northern hemisphere.

Characteristics:

*RST value: -

SCPI: device-specific

SYSTem:POSition:LONGitude?

This command queries the longitude of the current position of the R&S ZVH.

Return values

<sign><degrees>,<minutes>,<seconds>

<sign>	No sign = east Negative sign (-) = west
<degrees>	Degrees of longitude (integer value)
<minutes>	Minutes of longitude (integer value)
<seconds>	Seconds of longitude (floating point number)

Example

SYST:POS:LONG?

Return value would be, for example, 11,36,46.2 for 11°, 36', 46.2" East

Characteristics:

*RST value: -

SCPI: device-specific

SYSTem:POSition:VALid?

This command queries if the current position is valid.

Return values

0	GPS position is not valid.
1	GPS position is valid.

Example

SYST:POS:VAL?

Characteristics:

*RST value: -

SCPI: device-specific

7.10.3 Display Configuration

This chapter describes commands to set up the display of the R&S ZVH via remote control.

List of Commands

- [DISPlay:BRIGhtness <Brightness>](#) (p. 197)
- [DISPlay:CMAP <ColorScheme>](#) (p. 197)
- [DISPlay:CMAP:DEFault](#) (p. 198)
- [DISPlay:DATE:FORMat <DateFormat>](#) (p. 198)

DISPlay:BRIGhtness <Brightness>

This command sets the brightness of the display backlight.

Parameter

<Brightness>

Numeric value in the range from 0 to 1

Example

```
DISP:BRIG 0.80
```

Sets the brightness of the display to 80%

Characteristics

*RST value: 0.5 (50%)

SCPI: device-specific

DISPlay:CMAP <ColorScheme>

This command sets the color scheme of the display.

Parameter

<ColorScheme>

COLor	Color.
BW	Black & white.
PF	Printer friendly.

Example

```
DISP:CMAP BW
```

Sets the screen colors to black and white

Characteristics

*RST value: COLor

SCPI: conform

DISPlay:CMAP:DEFault

This command sets the display to the default state.

This command is an event and therefore has no query and no *RST value.

Example

```
DISP:CMAP:DEF
```

Restores the original color scheme

Characteristics

*RST value: -

SCPI: conform

DISPlay:DATE:FORMat <DateFormat>

This command sets the display date format.

Parameter

<DateFormat>

DDMMyyyy | MMDDyyyy

Example

```
DISP:DATE:FORM DDMMyyyy
```

Characteristics

*RST value: DDMMyyyy

SCPI: device-specific

7.10.4 Audio Settings

This chapter describes all commands to control the audio functions of the R&S ZVH.

List of commands

- [SYSTem:AUDio:VOLume <Volume>](#) (p. 199)
- [SYSTem:BEEPer:VOLume <Volume>](#) (p. 199)
- [SYSTem:BEEPer:KEY:VOLume <Volume>](#) (p. 199)

SYSTem:AUDio:VOLume <Volume>

This command sets the volume of the internal speaker.

Parameter

<Volume>

Numeric value in the range from 0 to 1

Example

```
SYST:AUD:VOL 0.40  
Sets the volume to 40%
```

Characteristics

*RST value: 0.3 (30%)
SCPI: device-specific

SYSTem:BEEPer:VOLume <Volume>

This command sets the volume of the system beeper.

Parameter

<Volume>

Numeric value in the range from 0 to 1

Example

```
SYST:BEEP:VOL 0.50  
Sets the volume of the beeper to 50%
```

Characteristics

*RST value: 0.6 (60%)
SCPI: conform

SYSTem:BEEPer:KEY:VOLume <Volume>

This command sets the volume of the keyboard click noise.

Parameter

<Volume>

Numeric value in the range from 0 to 1

Example

```
SYST:BEEP:KEY:VOL 0.10
```

Sets of keyboard clicking volume to 10%

Characteristics

*RST value: 0.3 (30%)

SCPI: conform

7.10.5 Setting up a Network Connection

This chapter describes all commands that are used if the R&S ZVH is part of a network.

List of commands

- [SYSTem:COMMunicate:LAN:ETHernet?](#) (p. 201)
- [SYSTem:COMMunicate:LAN:GATeway <Gateway>](#) (p. 201)
- [SYSTem:COMMunicate:LAN:SUBMask <SubnetMask>](#) (p. 201)
- [SYSTem:COMMunicate:SOCKet:ADDRess <IPAddress>](#) (p. 202)
- [SYSTem:COMMunicate:SOCKet:DHCP\[:STATe\] <State>](#) (p. 202)
- [SYSTem:COMMunicate:SOCKet:PORT <Port>](#) (p. 202)

SYSTem:COMMunicate:LAN:ETHernet?

This command queries the MAC address of the R&S ZVH.

This command is a query and therefore has no *RST value.

Example

```
SYST:COMM:LAN:ETH?  
Returns the MAC address
```

Characteristics

*RST value: -
SCPI: device-specific

SYSTem:COMMunicate:LAN:GATeway <Gateway>

This command sets the gateway in the LAN.

Parameter

<Gateway>
String containing the identifier of the gateway.

Characteristics

*RST value: -
SCPI: device-specific

SYSTem:COMMunicate:LAN:SUBMask <SubnetMask>

This command sets the subnet mask of the R&S ZVH.

Parameter

<SubnetMask>
String containing the subnet mask ('x.x.x.x').

Example

```
SYST:COMM:LAN:SUBM '255.255.255.0'  
Sets the subnet mask address to 255.255.255.0
```

Characteristics

*RST value: 255.255.255.0

SCPI: device-specific

SYSTem:COMMunicate:SOCKet:ADDRess <IPAddress>

This command sets the IP address of the R&S ZVH.

Parameter

<IPAddress>

String containing the IP address ('x.x.x.x').

Example

```
SYST:COMM:SOCK:ADDR '172.76.68.30'
```

Sets the IP address of the R&S ZVH to 172.76.68.30

Characteristics

*RST value: 172.76.68.24

SCPI: device-specific

SYSTem:COMMunicate:SOCKet:DHCP[:STATe] <State>

This command turns the Dynamic Host Configuration Protocol (DHCP) on and off.

Parameter

<State>

ON | OFF

Example

```
SYST:COMM:SOCK:DHCP ON
```

Activates DHCP.

Characteristics

*RST value: ON

SCPI: device-specific

SYSTem:COMMunicate:SOCKet:PORT <Port>

This command sets the port number for the connection.

Parameter

<Port>

Port number

Example

```
SYST:COMM:SOCK:PORT 1000
```

Sets the port number to 1000

Characteristics

*RST value: 5555

SCPI: device-specific

7.10.6 System Settings

This chapter describes all commands that define or query general system settings.

List of commands

- [INPut:IMPedance:PAD <MatchingPad>](#) (p. 203)
- [\[SENSe:\]ROSCillator:SOURce <RefSource>](#) (p. 204)
- [SYSTem:ACCessory?](#) (p. 204)
- [SYSTem:ACCessory:AUTO <State>](#) (p. 204)
- [SYSTem:BNC<1...2>:MODE <BNCFunction>](#) (p. 205)
- [SYSTem:DATE <Date>](#) (p. 205)
- [SYSTem:ERRor\[:NEXT\]?](#) (p. 206)
- [SYSTem:ERRor:ALL?](#) (p. 206)
- [SYSTem:ERRor:COUNT?](#) (p. 208)
- [SYSTem:ERRor:CODE\[:NEXT\]?](#) (p. 207)
- [SYSTem:ERRor:CODE:ALL?](#) (p. 207)
- [SYSTem:HELP:HEADers?](#) (p. 208)
- [SYSTem:HELP:SYNTax?](#) (p. 208)
- [SYSTem:LANGuage:CATalog?](#) (p. 209)
- [SYSTem:POWer:SOURce?](#) (p. 209)
- [SYSTem:POWer:STATus?](#) (p. 210)
- [SYSTem:PRESet](#) (p. 210)
- [SYSTem:PRESet:FACTory](#) (p. 210)
- [SYSTem:PRESet:MODE <Mode>](#) (p. 211)
- [SYSTem:PRESet:USER <Preset>](#) (p. 211)
- [SYSTem:REBoot](#) (p. 211)
- [SYSTem:SHUTdown](#) (p. 212)
- [SYSTem:TIME <Time>](#) (p. 212)
- [SYSTem:TZONee <TimeShift>](#) (p. 212)
- [SYSTem:VERSion?](#) (p. 213)

INPut:IMPedance:PAD <MatchingPad>

This command selects the matching pad connected to the R&S ZVH.

Parameter

<MatchingPad>
RAM | RAZ | HZTE

Example

```
INPut:IMP 75;PAD RAZ
```

Selects 75 Ω input impedance and the R&S RAZ as the matching pad.

Characteristics

*RST value: -
SCPI: device-specific

[SENSe:]ROSCillator:SOURce <RefSource>

This command selects the source of the frequency reference oscillator.

If you use an external reference signal, make sure to connect the signal to the Ext Ref BNC connector of the R&S ZVH.

Parameter

<RefSource>

INTernal	Internal reference.
EXTernal	External reference.

Example

ROSC:SOUR EXT

Activates external source as reference signal.

Characteristics

*RST value: -
SCPI: device-specific

SYSTem:ACCEssory?

This command queries the type of measurement accessory, if one is connected to the R&S ZVH (for example an isotropic antenna or power sensor).

Return value

Name of the accessory.

Example

SYST:ACC?

Queries connected measurement accessories.

Characteristics

*RST value: -
SCPI: device-specific

SYSTem:ACCEssory:AUTO <State>

This command turns automatic detection of connected measurement accessories on and off.

Parameter

<State>
ON | OFF

Example

SYST:ACC:AUTO ON

Turns on automatic accessory detection.

Characteristics

*RST value: -
 SCPI: device-specific

SYSTem:BNC<1...2>:MODE <BNCFunction>

This command configures the BNC sockets.

The numeric suffix at BNC selects the BNC socket you want to configure.

Parameter

<BNCFunction>

REFerence	Input for external reference signal (BNC 1)
TRIGger	Input for external trigger (BNC 1)
BIAS	BIAS port (BNC1 and BNC 2)
IF3	IF output (BNC 2)
INTernalbias	Internal DC BIAS (BNC 2)

Example

```
SYST:BNC2:MODE TRIG
```

Sets the seconds BNC socket to trigger input.

Characteristics

*RST value: BNC 1: TRIGger, BNC 2: IF3
 SCPI: device-specific

SYSTem:DATE <Date>

This command sets the date for the internal calendar.

Parameter

<Date>

Numeric value indicating the date

You have to enter the date as comma separated values after the string with the file name. The sequence is year,month,day.

The available value range is 1980...2099, 1...12, 1...31

Example

```
SYST:DATE 2000,6,1
```

Sets the date to 1/6/2000

Characteristics

*RST value: -
 SCPI: conform

SYSTem:ERRor[:NEXT]?

This command queries the oldest entry in the error queue and deletes it.

This command is a query and therefore has no *RST value.

Return value

<error number>,<error description>

<error number>	Number that contains information about the error. Negative number: error as defined in the SCPI standard. Positive number: error that is specific to the R&S ZVH.
<error description>	String containing a short error description.

If the error queue is empty, the command returns 0,'no error'.

Example

STAT:ERR?

Characteristics

*RST value: -
SCPI: conform

SYSTem:ERRor:ALL?

This command queries the complete error queue.

This command is a query and therefore no *RST value.

Return value

<error number>,<error description>

<error number>	Number that contains information about the error. Negative number: error as defined in the SCPI standard. Positive number: error that is specific to the R&S ZVH.
<error description>	String containing a short error description.

The number of values depends on the length of the queue.

If the error queue is empty, the command returns 0,'no error'.

Example

SYST:ERR:ALL?

Characteristics

*RST value: -
SCPI: device-specific

SYSTem:ERRor:CODE[:NEXT]?

This command queries the code of the next error in the error queue.

This command is a query and therefore has no *RST value.

Return value

<error number>

number that contains information about the error

Negative number: error as defined in the SCPI standard

Positive number: error that is specific to the R&S ZVH

If the error queue is empty, the command returns 0.

Example

```
STAT:ERR:CODE?
```

Characteristics

*RST value: -

SCPI: conform

SYSTem:ERRor:CODE:ALL?

This command queries the complete error queue.

This command is a query and therefore no *RST value.

Return value

<error number>

number that contains information about the error

Negative number: error as defined in the SCPI standard

Positive number: error that is specific to the R&S ZVH

The number of values depends on the length of the queue.

If the error queue is empty, the command returns 0,'no error'.

Example

```
SYST:ERR:CODE:ALL?
```

Characteristics

*RST value: -

SCPI: device-specific

SYSTem:ERRor:COUNt?

This command queries the number of errors currently in the error queue.

This command is a query and therefore no *RST value.

Return value

<numeric_value>

number of the errors in the queue

Example

```
SYST:ERR:COUN?
```

Characteristics

*RST value: -

SCPI: device-specific

SYSTem:HELP:HEADers?

This command returns a list of all available remote control commands.

This command is a query and therefore no *RST value.

Example

```
SYST:HELP:HEAD?
```

Returns the syntax of all available commands.

Characteristics

*RST value: -

SCPI: conform

SYSTem:HELP:SYNTax?

This command returns the full syntax of the specified command.

This command is a query and therefore no *RST value.

Parameter

<Command>

String containing the command you want to query

Example

```
SYST:HELP:SYNT? 'SYST:ERR?'
```

Returns the full syntax. In this case: 'SYSTem:ERRor[:NEXT]'.

Characteristics

*RST value: -

SCPI: device-specific

SYSTem:LANGuage <Language>

This command sets the language of the R&S ZVH user interface. You can query a list of available languages with `SYSTem:LANGuage:CATalog?`.

Parameter

<Language>
string containing the language

Example

```
SYST:LANG 'english'
```

Sets the system language to English

Characteristics

*RST value: -
SCPI: conform

SYSTem:LANGuage:CATalog?

This command lists all languages available for the user interface.

This command is a query and therefore no *RST value.

Example

```
SYST:LANG:CAT?
```

Queries available languages.

Characteristics

*RST value: -
SCPI: device-specific

SYSTem:POWer:SOURce?

This command queries the current R&S ZVH power source.

This command is a query and therefore has no *RST value.

Return values

ADAP	R&S ZVH is powered by the AC power supply.
BATT	R&S ZVH is powered by the battery.

Example

```
SYST:POW:SOUR?
```

Queries current power source.

Characteristics

*RST value: -
SCPI: conform

SYSTem:POWer:STATus?

This command queries the remaining power of the battery.

This command is a query and therefore has no *RST value.

Return values

Numeric value in the range from 0 to 100 %.

Example

```
SYST:POW:STAT?
```

Checks remaining battery power.

Characteristics

*RST value: -
SCPI: conform

SYSTem:PRESet

Resets the R&S ZVH to its default state or a state defined by the user, depending on SYSTem:PRESet:MODE.

This command is an event and therefore has no *RST value and no query.

Example

```
SYST:PRESet
```

Presets the instrument.

Characteristics

*RST value: -
SCPI: conform

SYSTem:PRESet:FACTory

This command initiates an instrument reset back to factory settings.

This command is an event and therefore has no query and no *RST value.

Example

```
SYST:PRESet:FACT
```

Resets the R&S ZVH to its factory settings.

Characteristics

*RST value: -
SCPI: device-specific

SYSTem:PRESet:MODE <Mode>

This command selects the preset mode.

Parameter

<Mode>

DEFault	Default preset state.
USER	User defined preset state.

Example

```
SYST:PRESet:MODE USER
```

Selects a user defined preset.

Characteristics

*RST value: -

SCPI: conform

SYSTem:PRESet:USER <Preset>

This command selects a file containing a user defined preset state.

Parameter

<Preset>

filename of the user defined preset state

Characteristics

*RST value: -

SCPI: conform

SYSTem:REBoot

This command initiates a reboot of the R&S ZVH.

This command is an event and therefore has no *RST value and no query.

Example

```
SYST:REB
```

Restarts the R&S ZVH.

Characteristics

*RST value: -

SCPI: conform

SYSTem:SHUTdown

This command turns the R&S ZVH off.

This command is an event and therefore has no *RST value and no query.

Example

```
SYST:SHUT
```

Turns the R&S ZVH off.

Characteristics

*RST value: -
SCPI: conform

SYSTem:TIME <Time>

This command sets the internal clock.

Parameter

<Time>

Numeric value indicating the time

You have to enter the time as comma separated values after the string with the file name. The sequence is hour,minute,second.

The available value range is 0...23, 0...59, 0...59.

Example

```
SYST:TIME 12,30,30
```

Characteristics

*RST value: -
SCPI: conform

SYSTem:TZONee <TimeShift>

This command defines a shift of the system time to select another time zone.

Parameter

<TimeShift>

Numeric value indicating the time shift.

You have to enter the time shift as comma separated value. The sequence is hour,minute.

The available value range is 0...23, 0...59.

Example

```
SYST:TZON 01,00
```

Shifts the time an hour ahead

Characteristics

*RST value: 0,0

SCPI: device-specific

SYSTem:VERSion?

This command queries the SCPI version the remote control is based on.

This command is a query and therefore has no *RST value.

Return value

1999.0

Example

```
SYST:VERS?
```

Characteristics

*RST value: -

SCPI: conform

7.11 Status Reporting System

The status reporting system stores all information on the present operating state of the instrument, and on errors which have occurred. This information is stored in the status registers and in the error queue. The status registers and the error queue can be queried via Ethernet.

The information is of a hierarchical structure. The register status byte (STB) defined in IEEE 488.2 and its associated mask register service request enable (SRE) form the uppermost level. The STB receives its information from the standard event status register (ESR) which is also defined in IEEE 488.2 with the associated mask register standard event status enable (ESE) and registers STATus:OPERation and STATus:QUEStionable which are defined by SCPI and contain detailed information on the instrument.

The output buffer contains the messages the instrument returns to the controller. It is not part of the status reporting system but determines the value of the MAV bit in the STB.

7.11.1 Structure of an SCPI Status Register

Each standard SCPI register consists of 5 parts which each have a width of 16 bits and have different functions. The individual bits are independent of each other, i.e. each hardware status is assigned a bit number that applies to all five parts. For example, bit 0 of the STATus:OPERation register is assigned to the calibration status of the R&S ZVH. Bit 15 (the most significant bit) is set to zero for all parts. Thus the contents of the register parts can be processed by the controller as positive integer.

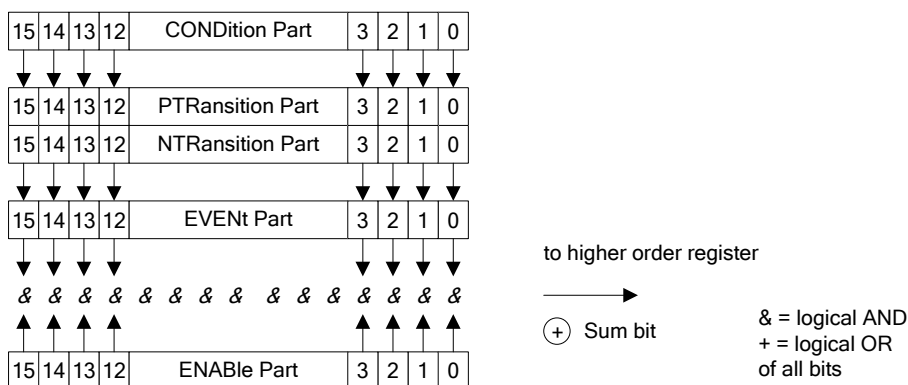


Figure 7-1: The status-register model

7.11.1.1 CONDition part

The CONDition part is directly written into by the hardware or the sum bit of the next lower register. Its contents reflects the current instrument status. This register part can only be read, but not written into or cleared. Its contents is not affected by reading.

7.11.1.2 PTRansition part

The Positive-TRansition part acts as an edge detector. When a bit of the CONDition part is changed from 0 to 1, the associated PTR bit decides whether the EVENT bit is set to 1.

PTR bit =1: the EVENT bit is set.

PTR bit =0: the EVENT bit is not set.

This part can be written into and read at will. Its contents is not affected by reading.

7.11.1.3 NTRansition part

The Negative-TRansition part also acts as an edge detector. When a bit of the CONDition part is changed from 1 to 0, the associated NTR bit decides whether the EVENT bit is set to 1.

NTR-Bit = 1: the EVENT bit is set.

NTR-Bit = 0: the EVENT bit is not set.

This part can be written into and read at will. Its contents is not affected by reading.

With these two edge register parts the user can define which state transition of the condition part (none, 0 to 1, 1 to 0 or both) is stored in the EVENT part.

7.11.1.4 EVENT part

The EVENT part indicates whether an event has occurred since the last reading, it is the "memory" of the condition part. It only indicates events passed on by the edge filters. It is permanently updated by the instrument. This part can only be read by the user. Reading the register clears it. This part is often equated with the entire register.

7.11.1.5 ENABLE part

The ENABLE part determines whether the associated EVENT bit contributes to the sum bit (see below). Each bit of the EVENT part is ANDed with the associated ENABLE bit (symbol '&'). The results of all logical operations of this part are passed on to the sum bit via an OR function (symbol '+').

ENABLE-Bit = 0: the associated EVENT bit does not contribute to the sum bit

ENABLE-Bit = 1: if the associated EVENT bit is "1", the sum bit is set to "1" as well.

This part can be written into and read by the user at will. Its contents is not affected by reading.

7.11.1.6 Sum bit

As indicated above, the sum bit is obtained from the EVENT and ENABLE part for each register. The result is then entered into a bit of the CONDition part of the higher-order register.

The instrument automatically generates the sum bit for each register. Thus an event, e.g. a PLL that has not locked, can lead to a service request throughout all levels of the hierarchy.



The service request enable register SRE defined in IEEE 488.2 can be taken as ENABLE part of the STB if the STB is structured according to SCPI. By analogy, the ESE can be taken as the ENABLE part of the ESR.

7.11.2 Overview of the Status Register

The following figure shows the status registers used by the R&S ZVH.

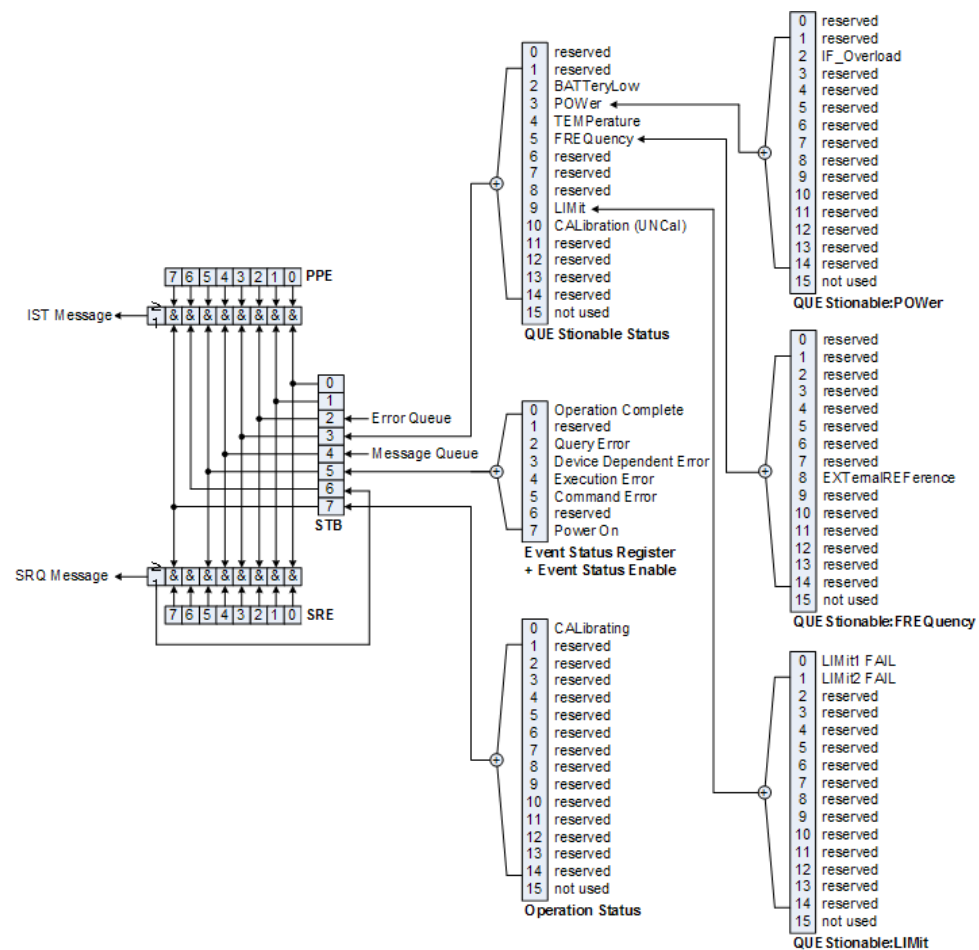


Figure 7-2: Overview of the status registers

7.11.3 Status Byte (STB) & Service Request Enable Register (SRE)

The STB is already defined in IEEE 488.2. It provides a rough overview of the instrument status by collecting the pieces of information of the lower registers. It can thus be compared with the CONDition part of an SCPI register and assumes the highest level within the SCPI hierarchy. A special feature is that bit 6 acts as the sum bit of the remaining bits of the status byte.

The STATUS BYTE is read using the command "***STB?**" or a serial poll.

The STB is linked to the SRE. The latter corresponds to the ENABLE part of the SCPI registers in its function. Each bit of the STB is assigned a bit in the SRE. Bit 6 of the SRE is ignored. If a bit is set in the SRE and the associated bit in the STB changes from 0 to 1, a service request (SRQ) is generated, which triggers an interrupt in the controller if this is appropriately configured and can be further processed there. The SRE can be set using the command "***SRE**" and read using the command "***SRE?**"

Table 7-1: Meaning of the bits used in the Status Byte

Bit No.	Meaning
0 to 1	Not used
2	Error Queue not empty The bit is set when an entry is made in the error queue. If this bit is enabled by the SRE, each entry of the error queue generates a service request. Thus an error can be recognized and specified in greater detail by polling the error queue. The poll provides an informative error message. This procedure is to be recommended since it considerably reduces the problems involved with remote control.
3	QUESTionable status sum bit The bit is set if an EVENT bit is set in the QUESTionable: status register and the associated ENABLE bit is set to 1. A set bit indicates a questionable instrument status, which can be specified in greater detail by polling the QUESTionable status register.
4	MAV bit (message available) The bit is set if a message is available in the output buffer which can be read. This bit can be used to enable data to be automatically read from the instrument to the controller.
5	ESB bit Sum bit of the event status register. It is set if one of the bits in the event status register is set and enabled in the event status enable register. Setting of this bit indicates a serious error which can be specified in greater detail by polling the event status register.
6	MSS bit (master status summary bit) The bit is set if the instrument triggers a service request. This is the case if one of the other bits of this registers is set together with its mask bit in the service request enable register SRE.
7	OPERation status register sum bit The bit is set if an EVENT bit is set in the OPERation status register and the associated ENABLE bit is set to 1. A set bit indicates that the instrument is just performing an action. The type of action can be determined by polling the OPERation status register.

7.11.4 Event Status Register (ESR) and Event Status Enable Register (ESE)

The ESR is defined in IEEE 488.2. It can be compared with the EVENT part of a SCPI register. The event status register can be read out using command *ESR?.

The ESE is the associated ENABLE part. It can be set using the command *ESE and read using the command *ESE?.

Table 7-2: Meaning of the bits in the event status register

Bit No.	Meaning
0	Operation Complete This bit is set on receipt of the command *OPC exactly when all previous commands have been executed.
1	Not used
2	Query Error This bit is set if either the controller wants to read data from the instrument without having sent a query, or if it does not fetch requested data and sends new instructions to the instrument instead. The cause is often a query which is faulty and hence cannot be executed.
3	Device-dependent Error This bit is set if a device-dependent error occurs. An error message with a number between -300 and -399 or a positive error number, which denotes the error in greater detail, is entered into the error queue.
4	Execution Error This bit is set if a received command is syntactically correct but cannot be performed for other reasons. An error message with a number between -200 and -300, which denotes the error in greater detail, is entered into the error queue.
5	Command Error This bit is set if a command is received, which is undefined or syntactically incorrect. An error message with a number between -100 and -200, which denotes the error in greater detail, is entered into the error queue.
6	Not used
7	Power On (supply voltage on) This bit is set on switching on the instrument.

7.11.4.1 STATus:OPERation Register

In the CONDition part, this register contains information on which actions the instrument is being executing or, in the EVENT part, information on which actions the instrument has executed since the last reading. It can be read using the commands STATus:OPERation:CONDition? or STATus:OPERation[:EVENT]?

Table 7-3: Meaning of the bits in the STATus:OPERation register

Bit No.	Meaning
0	CALibrating This bit is set as long as the instrument is performing a calibration.
1 to 14	Not used
15	This bit is always 0

7.11.4.2 STATus:QUEStionable Register

This register contains information about indefinite states which may occur if the unit is operated without meeting the specifications. It can be read using the commands STATus:QUEStionable: CONDition? and STATus:QUEStionable[:EVENT]?

Table 7-4: Meaning of bits in STATus:QUEStionable register

Bit No.	Meaning
0 to 1	These bits are not used
2	BATTERY LOW If the instrument is running without any external power supply and the charging level of the internal battery is approximately lower than 5% this bit is set to indicate that the system will be shut down automatically in approx. 5 minutes.
3	Not used
4	TEMPerature This bit is set if a questionable temperature occurs.
5 to 8	Not used
9	LIMit (device-specific) This bit is set if a limit value is violated
10	CALibration The bit is set if a measurement is performed unaligned (label UNCAL)
11 to 14	Not used
15	This bit is always 0.

7.11.4.3 STATus:QUEStionable:FREQuency Register

This register contains information about the reference frequency. It can be read using the commands STATus:QUEStionable:LIMit:FREQuency? and STATus:QUEStionable:FREQuency[:EVENT]?

Table 7-5: Meaning of bits in STATus:QUEStionable:FREQuency register

Bit No.	Meaning
0 to 7	Not used
8	EXtErnal REference This bit is set if an external reference is used.
9 to 14	Not used
15	This bit is always 0.

7.11.4.4 STATus:QUEStionable:LIMit Register

This register contains information about the observance of limit lines. It can be read using the commands STATus:QUEStionable:LIMit:CONDition? and STATus:QUEStionable:LIMit[:EVENT]?

Table 7-6: Meaning of bits in STATus:QUEStionable:LIMit register

Bit No.	Meaning
0	LIMit 1 FAIL This bit is set if limit line 1 is violated.
1	LIMit 2 FAIL This bit is set if limit line 2 is violated.
2 to 14	Not used
15	This bit is always 0.

7.11.4.5 STATus:QUEStionable:POWer Register

This register contains information about possible overload states. It can be read using the commands STATus:QUEStionable:POWer:CONDition? and STATus:QUEStionable:POWer[:EVENT]?

Table 7-7: Meaning of bits in STATus:QUEStionable:POWer register

Bit No.	Meaning
0 to 1	Not used
2	IF_Overload This bit is set if the IF path is overloaded. 'IFOVL' is displayed.
3 to 14	Not used
15	This bit is always 0.

7.11.5 Application of the Status Reporting Systems

In order to be able to effectively use the status reporting system, the information contained there must be transmitted to the controller and further processed there. There are several methods which are represented in the following.

7.11.5.1 Service Request

Under certain circumstances, the instrument can send a service request (SRQ) to the controller. Usually this service request initiates an interrupt at the controller, to which the control program can react appropriately. As evident from Fig. 1-4, an SRQ is always initiated if one or several of bits 2, 3, 4, 5 or 7 of the status byte are set and enabled in the SRE. Each of these bits combines the information of a further register, the error queue or the output buffer. The ENABLE parts of the status registers can be set so that arbitrary bits in an arbitrary status register initiate an SRQ. In order to make use of the possibilities of the service request effectively, all bits should be set to "1" in enable registers SRE and ESE.

Example

Use of the command *OPC to generate an SRQ at the end of a sweep

```
CALL InstrWrite(analyzer, "*ESE 1")  
'Set bit 0 in the ESE (Operation Complete)  
  
CALL InstrWrite(analyzer, "*SRE 32")  
'Set bit 5 in the SRE (ESB)?
```

After its settings have been completed, the instrument generates an SRQ.

The SRQ is the only possibility for the instrument to become active on its own. Each controller program should set the instrument in a way that a service request is initiated in the case of malfunction. The program should react appropriately to the service request.

7.11.5.2 Serial Poll

In a serial poll, just as with command *STB, the status byte of an instrument is queried. However, the query is realized via interface messages and is thus clearly faster. The serial-poll method has already been defined in IEEE 488.1 and used to be the only standard possibility for different instruments to poll the status byte. The method also works with instruments which do not adhere to SCPI or IEEE 488.2.

The VISUAL BASIC command for executing a serial poll is IBRSP(). Serial poll is mainly used to obtain a fast overview of the state of several instruments connected to the controller.

7.11.5.3 Query by Means of Commands

Each part of any status register can be read by means of queries. The individual commands are listed in the description of the STATUS Subsystem. The returned value is always a number that represents the bit pattern of the queried register. This number is evaluated by the controller program.

Queries are usually used after an SRQ in order to obtain more detailed information on the cause of the SRQ.

7.11.5.4 Error Queue Query

Each error state in the instrument leads to an entry in the error queue. The entries of the error queue are detailed plain-text error messages that can be displayed via manual operation using the setup menu or queried via remote control using the command `SYSTEM:ERRor?`. Each call of `SYSTEM:ERRor?` provides one entry from the error queue. If no error messages are stored there any more, the instrument responds with 0, "No error".

The error queue should be queried after every SRQ in the controller program as the entries describe the cause of an error more precisely than the status registers. Especially in the test phase of a controller program the error queue should be queried regularly since faulty commands from the controller to the instrument are recorded there as well.

7.11.6 Reset Values of the Status Reporting System

Table 7-8 contains the different commands and events causing the status reporting system to be reset. None of the commands, except *RST and SYSTem:PRESet, influences the functional instrument settings. In particular, DCL does not change the instrument settings.

Table 7-8: Resetting the status reporting system

Event	Switching on supply voltage		DCL,SDC			
	Power-On-Status-Clear		(Device Clear, Selected Device Clear)	*RST or SYSTem:PRESet	STATus:PRESet	*CLS
Effect	0	1				
Clear STB,ESR	—	yes	—	—	—	yes
Clear SRE,ESE	—	yes	—	—	—	—
Clear PPE	—	yes	—	—	—	—
Clear EVENT parts of the registers	—	yes	—	—	—	yes
Clear ENABLE parts of all OPERATION and QUESTIONable registers; Fill ENABLE parts of all other registers with "1".	—	yes	—	—	yes	—
Fill PTRansition parts with "1"; Clear NTRansition parts	—	yes	—	—	yes	—
Clear error queue	yes	yes	—	—	—	yes
Clear output buffer	yes	yes	yes	1)	1)	1)
Clear command processing and input buffer	yes	yes	yes	—	—	—

1) Every command being the first in a program message, i.e., immediately following a <PROGRAM MESSAGE TERMINATOR> clears the output buffer.

7.11.7 Remote Commands of the Status Reporting System

The following commands control the status-reporting system. *RST does not influence the status registers.

The OPERation status register contains information about the calibration status of the instrument.

The QUEStionable status register contains information about the status of the reference and local oscillator, possible overloads of the instrument and the status of limit checks and limit margins.

The commands are independent from the operating mode.

List of commands

- [STATus:PRESet](#) (p. 224)
- [STATus:QUEue\[:NEXT\]](#) (p. 225)
- [STATus:OPERation\[:EVENT\]?](#) (p. 225)
- [STATus:OPERation:CONDition?](#) (p. 225)
- [STATus:OPERation:ENABLE <SumBit>](#) (p. 225)
- [STATus:OPERation:NTRansition <SumBit>](#) (p. 226)
- [STATus:OPERation:PTRansition <SumBit>](#) (p. 226)
- [STATus:QUEStionable\[:EVENT\]?](#) (p. 226)
- [STATus:QUEStionable:CONDition?](#) (p. 227)
- [STATus:QUEStionable:ENABLE <SumBit>](#) (p. 227)
- [STATus:QUEStionable:NTRansition <SumBit>](#) (p. 227)
- [STATus:QUEStionable:PTRansition <SumBit>](#) (p. 228)

STATus:PRESet

This command resets the edge detectors and ENABLE parts of all registers to a defined value. All PTRansition parts are set to FFFFh, i.e. all transitions from 0 to 1 are detected. All NTRansition parts are set to 0, i.e. a transition from 1 to 0 in a CONDition bit is not detected. The ENABLE part of the STATus:OPERation and STATus:QUEStionable registers are set to 0, i.e. all events in these registers are not passed on.

Example

```
STAT:PRESet
```

Characteristics

*RST value: -
SCPI: conform

STATus:QUEue[:NEXT]

This command returns the earliest entry to the error queue and deletes it.

Positive error numbers indicate device-specific errors, negative error numbers are error messages defined by SCPI. If the error queue is empty, the error number 0, "no error", is returned. This command is identical with the command SYSTem:ERRor.

Example

STAT:QUE?

Characteristics

*RST value: –
SCPI: conform

STATus:OPERation[:EVENT]?

This command reads out the EVENT section of the OPERation register.

The command at the same time deletes the contents of the EVENT section.

Characteristics

*RST value: -
SCPI: conform

STATus:OPERation:CONDition?

This command reads out the CONDition section of the OPERation register.

The command does not delete the contents of the EVENT section.

Characteristics

*RST value: -
SCPI: conform

STATus:OPERation:ENABLE <SumBit>

This command controls the ENABLE part of the OPERation register.

The ENABLE part allows true conditions in the EVENT part of the status register to be reported in the summary bit. If a bit is 1 in the enable register and its associated event bit transitions to true, a positive transition will occur in the summary bit reported to the next higher level.

Parameter

<SumBit>
0 to 65535

Characteristics

*RST value: -
SCPI: conform

STATus:OPERation:NTRansition <SumBit>

This command controls the Negative TRansition part of the OPERation register.

Setting a bit causes a 1 to 0 transition in the corresponding bit of the associated register. The transition also writes a 1 into the associated bit of the corresponding EVENT register.

Parameter

<SumBit>
0 to 65535

Characteristics

*RST value: -
SCPI: conform

STATus:OPERation:PTRansition <SumBit>

This command controls the Positive TRansition part of the OPERation register.

Setting a bit causes a 0 to 1 transition in the corresponding bit of the associated register. The transition also writes a 1 into the associated bit of the corresponding EVENT register.

Parameter

<SumBit>
0 to 65535

Characteristics

*RST value: -
SCPI: conform

STATus:QUEStionable[:EVENT]?**STATus:QUEStionable:FREQuency[:EVENT]?****STATus:QUEStionable:LIMit[:EVENT]?****STATus:QUEStionable:POWEr[EVENT]?**

This command reads out the EVENT section of the QUEStionable register.

The command at the same time deletes the contents of the EVENT section.

Characteristics

*RST value: -
SCPI: conform

STATus:QUEStionable:CONDition?
STATus:QUEStionable:FREQuency:CONDition?
STATus:QUEStionable:LIMit:CONDition?
STATus:QUEStionable:POWer:CONDition?

This command reads out the CONDition section of the QUEStionable register.

The command does not delete the contents of the EVENt section.

Characteristics

*RST value: -
 SCPI: conform

STATus:QUEStionable:ENABle <SumBit>
STATus:QUEStionable:FREQuency:ENABle <SumBit>
STATus:QUEStionable:LIMit:ENABle <SumBit>
STATus:QUEStionable:POWer:ENABle <SumBit>

This command controls the ENABle part of the QUEStionable register.

The ENABle part allows true conditions in the EVENt part of the status register to be reported in the summary bit. If a bit is 1 in the enable register and its associated event bit transitions to true, a positive transition will occur in the summary bit reported to the next higher level.

Parameter

<SumBit>
 0 to 65535

Characteristics

*RST value: -
 SCPI: conform

STATus:QUEStionable:NTRansition <SumBit>
STATus:QUEStionable:FREQuency:NTRansition <SumBit>
STATus:QUEStionable:LIMit:NTRansition <SumBit>
STATus:QUEStionable:POWer:NTRansition <SumBit>

This command controls the Negative TRansition part of the QUEStionable register.

Setting a bit causes a 1 to 0 transition in the corresponding bit of the associated register. The transition also writes a 1 into the associated bit of the corresponding EVENt register.

Parameter

<SumBit>
 0 to 65535

Example

```
STAT:QUES:NTR 65535
```

Characteristics

*RST value: -

SCPI: conform

STATus:QUEStionable:PTRansition <SumBit>

STATus:QUEStionable:FREQuency:PTRansition <SumBit>

STATus:QUEStionable:LIMit:PTRansition <SumBit>

STATus:QUEStionable:POWer:PTRansition <SumBit>

This command control the Positive TRansition part of the QUEStionable register.

Setting a bit causes a 0 to 1 transition in the corresponding bit of the associated register. The transition also writes a 1 into the associated bit of the corresponding EVENT register.

Parameter

<SumBit>

0 to 65535

Characteristics

*RST value: -

SCPI: conform

Alphabetical List of Remote Commands

*CLS.....	32
*ESE	32
*ESR?	32
*IDN?	33
*IST?	33
*OPC.....	33
*OPT?	33
*RST	33
*SRE	34
*STB?.....	34
*TRG	34
*TST?.....	34
*WAI.....	34
 ABORt.....	 89
 CALCulate:CALKit:USER:OFFSet<p>:LENGth <ElecLengthOffs>	 160
CALCulate:DTF:CABLe:PRESet <CableModel>	66
CALCulate:DTF:DISTance:STARt <StartDistance>	39
CALCulate:DTF:DISTance:STOP <StopDistance>	40
CALCulate:LIMit<k>:ACPower:ACHannel:ABSolute <Limit>	134
CALCulate:LIMit<k>:ACPower:ACHannel:ABSolute:STATe <State>	134
CALCulate:LIMit<k>:ACPower:ACHannel:RESult?	134
CALCulate:LIMit<k>:ACPower:ACHannel[:RELative] <Limit>	133
CALCulate:LIMit<k>:ACPower:ACHannel[:RELative]:STATe <State>	133
CALCulate:LIMit<k>:ACPower:ALTErnate<y>:ABSolute <Limit>	136
CALCulate:LIMit<k>:ACPower:ALTErnate<y>:ABSolute:STATe <State>	136
CALCulate:LIMit<k>:ACPower:ALTErnate<y>:RESult?	137
CALCulate:LIMit<k>:ACPower:ALTErnate<y>[:RELative] <Limit>	135
CALCulate:LIMit<k>:ACPower:ALTErnate<y>[:RELative]:STATe <State>	135
CALCulate:LIMit<k>:ACPower[:STATe] <State>	132
CALCulate:MARKer:FUNCTion:ACPower:UNIT <Unit>	126
CALCulate:MARKer:FUNCTion:LEVel:ONCE	121
CALCulate:MARKer:FUNCTion:POWer:PRESet <Standard>	120
CALCulate:MARKer:FUNCTion:POWer:PRESet:CHECK?	120
CALCulate:MARKer:FUNCTion:POWer:RESult? <Measurement>	121
CALCulate:MARKer:FUNCTion:POWer:SElect <Measurement>	119
CALCulate:MARKer:FUNCTion:POWer[:STATe] <State>	119
CALCulate:MARKer<m>:COUNT:FREQuency?	103
CALCulate:MARKer<m>:COUNT:RESolution:MODE <Resolution>	103
CALCulate:MARKer<m>:COUNT[:STATe] <State>	104
CALCulate:MARKer<m>:FREQuency:MODE <InputMode>	104
CALCulate:MARKer<m>:FUNCTion:CENTEr	105
CALCulate:MARKer<m>:FUNCTion:CPOWer:BANDwidth <Bandwidth>	123
CALCulate:MARKer<m>:FUNCTion:CPOWer:MODE <DisplayMode>	123
CALCulate:MARKer<m>:FUNCTion:CPOWer:UNIT <Unit>	123
CALCulate:MARKer<m>:FUNCTion:DEModulation:HOLDoff <Time>	105
CALCulate:MARKer<m>:FUNCTion:DEModulation:SElect <Demodulation>	106
CALCulate:MARKer<m>:FUNCTion:DEModulation[:STATe] <State>	105
CALCulate:MARKer<m>:FUNCTion:NDBDown <Distance>	106
CALCulate:MARKer<m>:FUNCTion:NDBDown:FREQuency?	106

CALCulate:MARKer<m>:FUNCTION:NDBDown:RESult?	107
CALCulate:MARKer<m>:FUNCTION:NDBDown:STATe <State>	107
CALCulate:MARKer<m>:FUNCTION:NOISe:RESult?	108
CALCulate:MARKer<m>:FUNCTION:NOISe[:STATe] <State>	108
CALCulate:MARKer<m>:FUNCTION:OBAN:BANDwidth <Bandwidth>	124
CALCulate:MARKer<m>:FUNCTION:OBAN:BANDwidth:PCT <OBW>	125
CALCulate:MARKer<m>:FUNCTION:POWer:RESult:PHZ <State>	124
CALCulate:MARKer<m>:FUNCTION:REFeRence	109
CALCulate:MARKer<m>:FUNCTION:TDMA:BURSt <BurstLength>	125
CALCulate:MATH<n>[:EXPRession][:DEFine] <Expression>	97
CALCulate:MATH<n>:COPY:MEMory	50
CALCulate:MATH<n>:STATe <State>	98
CALCulate:PMETer:CPOWer:BANDwidth <Bandwidth>	169
CALCulate:PMETer:PRESet:BANDwidth:VIDeo <Bandwidth>	173
CALCulate:PMETer:PRESet:SELEct <Standard>	174
CALCulate:PMETer:PRESet[:STATe] <State>	174
CALCulate:PMETer:RELative[:MAGNitude] <RefValue>	169
CALCulate:PMETer:RELative[:MAGNitude]:AUTO ONCE	169
CALCulate:PMETer:RELative[:MAGNitude]:OFFSet <Offset>	170
CALCulate:TRACe:CABLe:LENGth:RESult?	163
CALCulate:TRACe:CABLe:LENGth:STATe <State>	162
CALCulate:TRACe:CABLe:LOSS:RESult?	68
CALCulate:TRACe:CABLe:TIME:RESult?	163
CALCulate:TRACe:CABLe:TIME[:STATe] <State>	163
CALCulate:TRACe:VSWR:MAX:STATe <State>	67
CALCulate:TRANSform:DTFault:PEAK:COUNT?	73
CALCulate:TRANSform:DTFault:PEAK:DATA<y>?	73
CALCulate:TRANSform:DTFault:PEAK:THREShold <Threshold>	74
CALCulate:TRANSform:DTFault:PEAK[:STATe] <State>	74
CALCulate:VVMeter:MAGNitude:REFeRence?	165
CALCulate:VVMeter:MAGNitude:RESult?	165
CALCulate:VVMeter:PHASe:REFeRence?	166
CALCulate:VVMeter:PHASe:RESult?	166
CALCulate:VVMeter:REFeRence[:STATe] <State>	166
CALCulate<n>:DELTamarker<m>:AOFF	56
CALCulate<n>:DELTamarker<m>:MAXimum:NEXT	56
CALCulate<n>:DELTamarker<m>:MAXimum[:PEAK]	56
CALCulate<n>:DELTamarker<m>:MINimum[:PEAK]	56
CALCulate<n>:DELTamarker<m>:X <Coordinate>	57
CALCulate<n>:DELTamarker<m>:X:RELative <Distance>	57
CALCulate<n>:DELTamarker<m>:Y?	58
CALCulate<n>:DELTamarker<m>[:STATe] <State>	55
CALCulate<n>:DLINe <Amplitude>	110
CALCulate<n>:DLINe:STATe <State>	110
CALCulate<n>:LIMit<k>:BEEP[:STATe] <State>	111
CALCulate<n>:LIMit<k>:COMMENT?	111
CALCulate<n>:LIMit<k>:DEFine	112
CALCulate<n>:LIMit<k>:DELeTe	113
CALCulate<n>:LIMit<k>:FAIL?	113
CALCulate<n>:LIMit<k>:LOWer:SELEct <LimitLine>	113
CALCulate<n>:LIMit<k>:LOWer:THREShold <Level>	114
CALCulate<n>:LIMit<k>:STATe <State>	114
CALCulate<n>:LIMit<k>:UNIT:X?	114
CALCulate<n>:LIMit<k>:UNIT[:Y]?	115
CALCulate<n>:LIMit<k>:UPPer:SELEct <LimitLine>	115

CALCulate<n>:LIMit<k>:UPPer:THReshold <Level>	115
CALCulate<n>:MARKer<m>:AOFF	59
CALCulate<n>:MARKer<m>:FUNCTion:HARMonics:DISToRtion? TOTal	138
CALCulate<n>:MARKer<m>:FUNCTion:HARMonics:LIST?	139
CALCulate<n>:MARKer<m>:FUNCTion:HARMonics:NHARmonics <Harmonics>	139
CALCulate<n>:MARKer<m>:FUNCTion:HARMonics:PRESet	140
CALCulate<n>:MARKer<m>:FUNCTion:HARMonics[:STATe] <State>	138
CALCulate<n>:MARKer<m>:FUNCTion:MDEPth:RESult?	141
CALCulate<n>:MARKer<m>:FUNCTion:MDEPth[:STATe] <State>	141
CALCulate<n>:MARKer<m>:FUNCTion:TXPower:RESult?	137
CALCulate<n>:MARKer<m>:FUNCTion:TXPower:RESult?	142
CALCulate<n>:MARKer<m>:MAXimum:NEXT	60
CALCulate<n>:MARKer<m>:MAXimum[:PEAK]	59
CALCulate<n>:MARKer<m>:MINimum[:PEAK]	60
CALCulate<n>:MARKer<m>:MODE <MarkerMode>	155
CALCulate<n>:MARKer<m>:POSition <StepSize>	60
CALCulate<n>:MARKer<m>:X <Coordinate>	61
CALCulate<n>:MARKer<m>:X:SLIMits:LEfT <SearchLimit>	62
CALCulate<n>:MARKer<m>:X:SLIMits:RIGHt <Searchlimit>	62
CALCulate<n>:MARKer<m>:X:SLIMits[:STATe] <State>	61
CALCulate<n>:MARKer<m>:Y?	156
CALCulate<n>:MARKer<m>:Y?	63
CALCulate<n>:MARKer<m>[:STATe] <State>	59
CALCulate<n>:TRACe:VSWR:AVG:RESult?	68
CALCulate<n>:TRACe:VSWR:MAX:RESult?	69
CALibration:ABORt	70
CALibration:ATTenuation:STATus?	70
CALibration:CONTInue?	70
CALibration:MODE?	161
CALibration:MODE?	71
CALibration:PMETer:ZERO:AUTO ONCE	171
CALibration:STARt? <CalibrationMethod>	71
CALibration:STATus?	161
DISPlay:BRIGHtness <Brightness>	197
DISPlay:CMAp <ColorScheme>	197
DISPlay:CMAp:DEFault	198
DISPlay:DATE:FORMat <DateFormat>	198
DISPlay:GDELay:APERture:STEP <Aperture>	164
DISPlay:LOSS:REFerence <RefValue>	41
DISPlay:LOSS:REFerence:POSition <RefPosition>	42
DISPlay:LOSS:Y:SCALE <DisplayRange>	42
DISPlay:WINDow:STORE	183
DISPlay[:WINDow]:TRACe<n> [:STATe] <State>	98
DISPlay[:WINDow]:TRACe<n>:MEMory[:STATe] <State>	50
DISPlay[:WINDow]:TRACe<n>:MODE <TraceMode>	51
DISPlay[:WINDow]:TRACe<n>:MODE <TraceMode>	98
DISPlay[:WINDow]:TRACe<n>:Y:SPACing <Scaling>	81
DISPlay[:WINDow]:TRACe<n>:Y[:SCALE] <DisplayRange>	82
DISPlay[:WINDow]:TRACe<n>:Y[:SCALE]:ADJJust	41
DISPlay[:WINDow]:TRACe<n>:Y[:SCALE]:RLEVel <ReferenceLevel>	82
DISPlay[:WINDow]:TRACe<n>:Y[:SCALE]:RLEVel:OFFSet <Offset>	82
DISPlay[:WINDow]:TRACe<n>:Y[:SCALE]:RPOSition <ReferencePosition>	83

DISPlay<n>:GDElay:REFerence <RefValue>.....	147
DISPlay<n>:GDElay:REFerence:POSition <RefPosition>.....	148
DISPlay<n>:GDElay:Y:SCALE <DisplayRange>	148
DISPlay<n>:IMPedance:REFerence:POSition <Impedance>.....	157
DISPlay<n>:MAGNitude:REFerence <RefValue>.....	43
DISPlay<n>:MAGNitude:REFerence:POSition <RefPosition>.....	43
DISPlay<n>:MAGNitude:Y:SCALE <DisplayRange>	43
DISPlay<n>:MAGNitude:Y:SPACing <Scaling>	44
DISPlay<n>:PHASe:REFerence <RefValue>	149
DISPlay<n>:PHASe:REFerence:POSition <RefPosition>	149
DISPlay<n>:PHASe:UNWRap <State>	150
DISPlay<n>:PHASe:Y:SCALE <DisplayRange>	149
DISPlay<n>:REFlection:UNIT <Unit>.....	151
DISPlay<n>:REFlection:Y:SCALE <DisplayRange>	150
DISPlay<n>:VSWR:Y:SCALE <DisplayRange>	45
DISPlay<n>:VSWR:Y:SCALE:MAXimum <TopValue>.....	45
DISPlay<n>:VSWR:Y:SCALE:MINimum <BottomValue>	44
DISPlay<n>:ZOOM:AREA[:STAT] <State>	157
DISPlay<n>:ZOOM:FACTor <ZoomFactor>	158
DISPlay<n>:ZOOM:X <HorizShift>.....	158
DISPlay<n>:ZOOM:Y <VerticalShift>	158
 FETCh<z>:PMETer?	 173
 FORMat:BORDER <ByteOrder>	 99
FORMat[:DATA] <DataFormat>	101
FORMat[:DATA] <DataFormat>	51
 HCOPy:DEVice:LANGuage.....	 183
HCOPy[:IMMEDIATE]	184
 INITiate:CONTinuous <SweepMode>	 90
INITiate[:IMMEDIATE]	89
 INPut:ANTenna:MEASure <Direction>.....	 144
INPut:ANTenna:STATe <State>.....	145
INPut:ATTenuation <Attenuation>.....	45
INPut:ATTenuation:AUTO <State>.....	84
INPut:ATTenuation:MODE <AttenuationMode>.....	83
INPut:GAIN:STATe <State>	84
INPut:IMPedance <Impedance>.....	84
INPut:IMPedance:PAD <MatchingPad>	203
 INSTrument:NSElect <OperatingMode>	 191
INSTrument[:SElect] <OperatingMode>.....	190
 MEASurement:ISUP <State>	 52
MEASurement:ISUP:APER <Aperture>	52
MEASurement:MODE <MeasMode>	66
MEASurement:PORT <Port>.....	65
MEASurement<n>:FORMat <MeasFormat>	164
MEASurement<n>:FORMat <MeasFormat>	67

MEASurement<n>:FUNCTION:SElect <ResultDisplay>	162
MEASurement<n>:MODE <MeasMode>	160
MMEMory:CATalog:DIRectories?	176
MMEMory:CATalog?	175
MMEMory:CDIRectory <Directory>	176
MMEMory:COPY <SourceFile>,<DestinationFile>	176
MMEMory:DATA <FileName>[,<BlockData>]	177
MMEMory:DELeTe <File>	178
MMEMory:FILE <File>	178
MMEMory:FILE:DATE <FileName>,<Date>	178
MMEMory:FILE:TIME <FileName>,<Time>	179
MMEMory:INIT	179
MMEMory:LOAD:STATe 1,<FileName>	180
MMEMory:MDIRectory <Directory>	180
MMEMory:MOVE <SourceFile>,<NewFileName>	180
MMEMory:NAME <FileName>	184
MMEMory:RDIRectory <Directory>	181
MMEMory:STORe:STATe 1,<FileName>	181
[SENSe:]BANDwidth BWIDth:VIDeo <VideoBW>	88
[SENSe:]BANDwidth BWIDth:VIDeo:AUTO <State>	88
[SENSe:]BANDwidth BWIDth[:RESolution] <MeasBW>	47
[SENSe:]BANDwidth BWIDth[:RESolution] <ResBW>	87
[SENSe:]BANDwidth BWIDth[:RESolution]:AUTO <State>	47
[SENSe:]BANDwidth BWIDth[:RESolution]:AUTO <State>	87
[SENSe:]CHANnel <ChannelNumber>	117
[SENSe:]CHANnel:TABLE:SElect <ChannelTable>	117
[SENSe:]CORRection:TRANSDucer<c>:ISOTropic[:STATe]?	145
[SENSe:]CORRection:TRANSDucer<c>:SElect <TransducerFactor>	85
[SENSe:]CORRection:TRANSDucer<c>:UNIT?	85
[SENSe:]CORRection:TRANSDucer<c>[:STATe] <State>	85
[SENSe:]DETEctor<n> [:FUNCTION] <Detector>	99
[SENSe:]DETEctor<n> [:FUNCTION]:AUTO <State>	100
[SENSe:]ESpectrum:PRESet:SETTings ONCE	142
[SENSe:]ESpectrum:PRESet[:STANdard] <Standard>	142
[SENSe:]FREQuency:CARRier:STARt <Frequency>	143
[SENSe:]FREQuency:CARRier:STOP <Frequency>	144
[SENSe:]FREQuency:CENTer <Frequency>	36
[SENSe:]FREQuency:CENTer <Frequency>	76
[SENSe:]FREQuency:CENTer:STEP <StepSize>	36
[SENSe:]FREQuency:CENTer:STEP <StepSize>	76
[SENSe:]FREQuency:CENTer:STEP:LINK <StepSizeCoupling>	37
[SENSe:]FREQuency:CENTer:STEP:LINK <StepSizeCoupling>	77
[SENSe:]FREQuency:INPut:MODE <InputMode>	77
[SENSe:]FREQuency:MODE <OperationMode>	78
[SENSe:]FREQuency:OFFSet <FrequencyOffset>	78
[SENSe:]FREQuency:SETTings:COUPling:ENABle <State>	37
[SENSe:]FREQuency:SPAN 	38
[SENSe:]FREQuency:SPAN 	79
[SENSe:]FREQuency:SPAN:AUTO <State>	38
[SENSe:]FREQuency:SPAN:AUTO <State>	79
[SENSe:]FREQuency:SPAN:FULL	79
[SENSe:]FREQuency:STARt <StartFrequency>	39

[SENSe:]FREQuency:STARt <StartFrequency>	80
[SENSe:]FREQuency:STOP <StopFrequency>	39
[SENSe:]FREQuency:STOP <StopFrequency>	80
[SENSe:]PMETer:DETEctor[:FUNCTion] <PowerDisplay>	172
[SENSe:]PMETer:FREQuency <Frequency>	168
[SENSe:]PMETer:MTIME <MeasTime>	171
[SENSe:]POWer:ACHannel:ACPairs <ChannelPairs>	127
[SENSe:]POWer:ACHannel:BANDwidth:ACHannel <Bandwidth>	127
[SENSe:]POWer:ACHannel:BANDwidth:ALTErnate<y> <Bandwidth>	128
[SENSe:]POWer:ACHannel:BANDwidth[:CHANnel] <Bandwidth>	127
[SENSe:]POWer:ACHannel:MODE <PowerMode>	128
[SENSe:]POWer:ACHannel:PRESet:RLEVel	129
[SENSe:]POWer:ACHannel:REFeRence:TXCHannel:AUTO <RefChannel>	129
[SENSe:]POWer:ACHannel:REFeRence:TXCHannel:MANual <RefChannel>	129
[SENSe:]POWer:ACHannel:SPACing:ALTErnate<y> <Spacing>	130
[SENSe:]POWer:ACHannel:SPACing:CHANnel<Tx> <Spacing>	131
[SENSe:]POWer:ACHannel:SPACing[:ACHannel]] <Spacing>	130
[SENSe:]POWer:ACHannel:TXCHannel:COUNt <TxChannels>	131
[SENSe:]ROSCilator:SOURce <RefSource>	204
[SENSe:]SWEep:COUNt <SweepCount>	90
[SENSe:]SWEep:EGATE <State>	94
[SENSe:]SWEep:EGATE:HOLDoff <GateDelay>	94
[SENSe:]SWEep:EGATE:LENGth <GateLength>	95
[SENSe:]SWEep:EGATE:TIME <SweepTime>	95
[SENSe:]SWEep:MODE <State>	143
[SENSe:]SWEep:POINts?	91
[SENSe:]SWEep:TIME <SweepTime>	91
[SENSe:]SWEep:TIME:AUTO <State>	91
[SENSe:]CHANnel:TABLE:SElect:DOWNlink <ChannelTable>	118
[SENSe:]CHANnel:TABLE:SElect:UPLink <ChannelTable>	118
[SENSe:]CHANnel:TABLE:SET <Direction>	118
 SENSe:SWEep:POINts <Points>	 48
 SOURce:TG:ATTenuation <TGAttenuation>	 46
 STATus:OPERation:CONDition?	 225
STATus:OPERation:ENABLE <SumBit>	225
STATus:OPERation:NTRansition <SumBit>	226
STATus:OPERation:PTRansition <SumBit>	226
STATus:OPERation[:EVENT]?	225
STATus:PRESet	224
STATus:QUEStionable:CONDition?	227
STATus:QUEStionable:ENABLE <SumBit>	227
STATus:QUEStionable:FREQuency:CONDition?	227
STATus:QUEStionable:FREQuency:ENABLE <SumBit>	227
STATus:QUEStionable:FREQuency:NTRansition <SumBit>	227
STATus:QUEStionable:FREQuency:PTRansition <SumBit>	228
STATus:QUEStionable:FREQuency[:EVENT]?	226
STATus:QUEStionable:LIMit:CONDition?	227
STATus:QUEStionable:LIMit:ENABLE <SumBit>	227
STATus:QUEStionable:LIMit:NTRansition <SumBit>	227
STATus:QUEStionable:LIMit:PTRansition <SumBit>	228
STATus:QUEStionable:LIMit[:EVENT]?	226

STATus:QUEStionable:NTRansition <SumBit>	227
STATus:QUEStionable:POWer:CONDition?	227
STATus:QUEStionable:POWer:ENABLE <SumBit>	227
STATus:QUEStionable:POWer:NTRansition <SumBit>	227
STATus:QUEStionable:POWer:PTRansition <SumBit>	228
STATus:QUEStionable:POWer[EVENT]?	226
STATus:QUEStionable:PTRansition <SumBit>	228
STATus:QUEStionable[:EVENT]?	226
STATus:QUEue[:NEXT]	225
SYSTem:ACCessory:AUTO <State>	204
SYSTem:ACCessory?	204
SYSTem:AUDio:VOLume <Volume>	199
SYSTem:BEEPer:KEY:VOLume <Volume>	199
SYSTem:BEEPer:VOLume <Volume>	199
SYSTem:BNC<1...2>:MODE <BNCFunction>	205
SYSTem:CAPTure:COUNter <Counter>	185
SYSTem:CAPTure:DATaset[:STATe] <State>	185
SYSTem:CAPTure:GPX[:STATe] <State>	186
SYSTem:CAPTure:SCReen[:STATe] <State>	186
SYSTem:COMMunicate:LAN:ETHernet?	201
SYSTem:COMMunicate:LAN:GATeway <Gateway>	201
SYSTem:COMMunicate:LAN:SUBMask <SubnetMask>	201
SYSTem:COMMunicate:SOCKet:ADDRess <IPAddress>	202
SYSTem:COMMunicate:SOCKet:DHCP[:STATe] <State>	202
SYSTem:COMMunicate:SOCKet:PORT <Port>	202
SYSTem:DATE <Date>	205
SYSTem:ERRor:ALL?	206
SYSTem:ERRor:CODE:ALL?	207
SYSTem:ERRor:CODE[:NEXT]?	207
SYSTem:ERRor:COUNt?	208
SYSTem:ERRor[:NEXT]?	206
SYSTem:HELP:HEADers?	208
SYSTem:HELP:SYNTax?	208
SYSTem:LANGuage <Language>	209
SYSTem:LANGuage:CATalog?	209
SYSTem:POSition:ALTitude?	192
SYSTem:POSition:COMPass:ANGLE?	192
SYSTem:POSition:COMPass:VALid?	193
SYSTem:POSition:COMPass[:STATe] <State>	193
SYSTem:POSition:GPS:CONNected?	194
SYSTem:POSition:GPS:CORRection:FREQuency?	194
SYSTem:POSition:GPS:QUALity?	194
SYSTem:POSition:GPS:SATellites?	195
SYSTem:POSition:GPS[:STATe] <State>	193
SYSTem:POSition:LATitude?	195
SYSTem:POSition:LONGitude?	196
SYSTem:POSition:VALid?	196
SYSTem:POWer:SOURce?	209
SYSTem:POWer:STATus?	210
SYSTem:PRESet	210
SYSTem:PRESet:CALibration:DISCard <State>	72
SYSTem:PRESet:FACTory	210
SYSTem:PRESet:MODE <Mode>	211
SYSTem:PRESet:USER <Preset>	211

SYSTem:REBoot	211
SYSTem:SET:LOCK <FileName>	182
SYSTem:SET:UNLock <FileName>	182
SYSTem:SHUTdown	212
SYSTem:SOEVent[:STATe] <State>	189
SYSTem:SOEVent:DISTance:INTerval <Distance>	187
SYSTem:SOEVent:LIMits:MODE <Mode>	187
SYSTem:SOEVent:RECORDing:STORage <Device>	188
SYSTem:SOEVent:SOURce <EventType>	188
SYSTem:SOEVent:TIME:INTerval <Time>	189
SYSTem:TIME <Time>	212
SYSTem:TZONee <TimeShift>	212
SYSTem:VERSion?	213
TRACe:DATA <Destination>	52
TRACe:IQ:DATA:MEMory? [<OffsetSamples>,<Samples>]	92
TRACe:IQ:RLENgth <Samples>	93
TRACe:IQ:SRATe <SampleRate>	93
TRACe:IQ[:STATe] <State>	93
TRACe[:DATA]?	153
TRACe<n> [:DATA]? <Destination>	100
TRACe<n>:DATA:MEMory? <Trace>	53
TRIGger[:SEQUence]:HOLDoff[:TIME] <TriggerDelay>	48
TRIGger[:SEQUence]:LEVel:VIDeo <TriggerLevel>	95
TRIGger[:SEQUence]:SLOPe <TriggerSlope>	49
TRIGger[:SEQUence]:SOURce <TriggerSource>	49
TRIGger[:SEQUence]:SOURce <TriggerSource>	96
UNIT:LENgth <Unit>	54
UNIT:POWer <Unit>	86
UNIT<z>:PMETer:POWer <Unit>	170

Index

Abort measurement	89	cable loss	42
ACLR	126	group delay	82, 148
limit check	132, 137	magnitude	43
Adjacent channel spacing	130	phase	149
Adjacent channels	127	reflection coefficient	150
Adjust scale	41	VSWR	45
Alternate channel spacing	130	Distance	36
Alternate channels	128	DTF list	73
AM modulation depth	140	DTF threshold	74
Aperture	52	Electrical length	162
Aperture step	164	Error queue	206
Attenuation	45	File	175
Attenuation coupling	84	Frequency	
Attenuation mode	83	cable tests	36
Audio demodulation	105	power meter	168
Bandwidth		span	38
ACLR	127	span auto	79
adjacent channels	127	step size	36
alternate channels	128	Frequency counter	104
channel power	123	Frequency domain	78
occupied bandwidth	124	Frequency mode	77
resolution	87	Frequency mode (marker)	104
video	88	Frequency offset	78
Battery	210	Frequency span	79
Beeper	199	Frequency step size	76
BNC	205	Frequency step size coupling	77
Brightness	197	Full span	79
Burst length	125	Gate delay	94
Cable distance	36	Gate length	95
Cable selection	66	Gated trigger	94
Calibration	160	Gateway	201
Center frequency	36, 76	GPS	192
Channel power		Hardcopy	183
trace mode	123	Harmonic distortion	138
unit	123	I/Q capture	92
Channel power measurement	122	Impedance	84, 157, 203
Channel selection	117	Input attenuation	45
Channel spacing	130	Interference suppression	52
Channel table selection	117	Isotropic antenna	144
Color scheme	197	LAN	201
Common commands	32	Language	209
Continuous sweep	90	Length unit	54
Conventions	7	Level axis	41
Data capture	185, 187	Limit check	
Data format	51, 101	ACLR	132, 137
Data management	175	Limit lines	64, 111
Date	205	Marker	59
Delay time	48, 163	deactivation	59
Delta marker	55	horizontal position	61
deactivation	56	search limits	61
horizontal position	57	vertical position	63
vertical position	58	zoom	157
Detector	99	Marker mode	155
Display	197	Measurement	
Display line	110	abort	89
Display range	44, 81	ACLR	126

AM modulation depth	140	Restoring	175
channel power	122	Result display	162
harmonic distortion	138	Results	52, 100, 121, 153
network analysis	160	delay time	163
noise	108	electrical length	163
occupied bandwidth	124	power meter	173
selection	119	Saving	175
spectrum emission mask	141	Scale adjust	41
spurious emission	143	Screenshot	183
start	89	Single sweep	90
TDMA	125	Slope (trigger)	49
Measurement control	48	Smith chart	
Measurement format	162	zoom	157
Measurement results	121	Span	38, 79
Measurement time		Spectrum emission mask	141
power sensor	171	Spurious emissions	143
Memory trace	50	Standard compliance check	120
Mode	190	Standard selection	120, 142
n dB down	107	Start frequency	39, 80
Network	201	Start measurement	89
Noise measurement	108	Stop frequency	39, 80
Occupied bandwidth	124	Sweep count	90
Operating mode	190	Sweep mode	90
Option		Sweep points	48, 91
K42	146	Sweep time	91, 95
K45	146	TDMA burst length	125
Phase unwrap	150	TDMA measurement	125
Port	65	Time	212
Position	192	Time domain	78
Power (system)	209	Trace math	97
Power percentage	125	Trace memory	50
Preamplifier	84	Trace mode	51
Preset	33, 210	Trace read out	52, 100, 153
Reference impedance	157	Trace selection	98
Reference level	82	Tracking generator	46
adjustment	121, 129	Transducer	85
power meter	170	Transducer (isotropic antenna)	145
Reference level offset	82	Transducer factor unit	85
Reference position	83	Transducer selection	85
cable loss	42	Transmission channels	131
group delay	148	Trigger	48, 96
magnitude	43	gate	94
phase	149	Trigger source	96
Reference value		Unit	86
cable loss	41	power sensor	170
group delay	147	vector voltmeter	165
magnitude	43	Video bandwidth	88
phase	149	Video trigger level	95
power meter	169	Volume	199
Resolution bandwidth	87	Zeroing	171