


=====

Acq. Operator	: SYSTEM	Seq. Line	: 1
Acq. Instrument	: MRK0111734	Location	: 1
Injection Date	: 9/30/2021 5:21:19 PM	Inj	: 1
		Inj Volume	: Manually
Sequence File	: C:\Chem32\2\Data\Photobromination\E-Z 2021-09-30 17-18-47\E-Z.S		
Method	: C:\Chem32\2\Data\Photobromination\E-Z 2021-09-30 17-18-47\Photobromination-09-30-2021.M (Sequence Method)		
Last changed	: 9/30/2021 5:18:47 PM by SYSTEM		

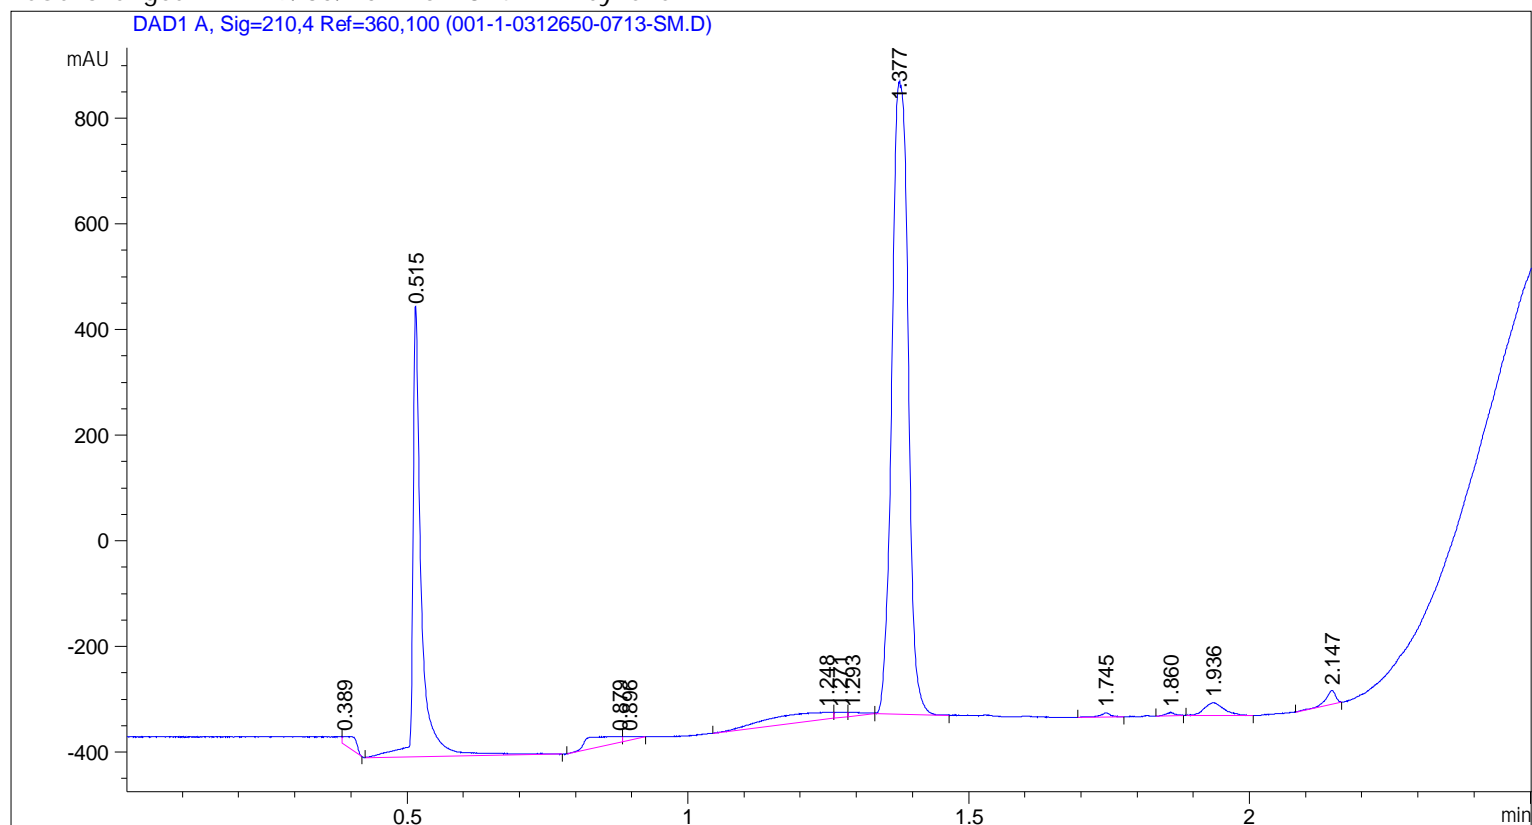

=====  
Area Percent Report  
=====

Sorted By : Signal  
Multiplier : 1.0000  
Dilution : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=210,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	0.389	VB	0.0281	34.52074	14.83516	0.9311
2	0.515	BV R	0.0154	898.96716	845.81909	24.2468
3	0.879	BV	0.0821	73.20538	10.79736	1.9745
4	0.896	VB	0.0211	12.55488	7.30049	0.3386
5	1.248	BV	0.1282	141.52744	13.35166	3.8173
6	1.271	VV	0.0193	14.99162	10.41850	0.4044
7	1.293	VB	0.0276	11.87349	7.16116	0.3202
8	1.377	BB	0.0320	2409.49829	1196.56750	64.9886
9	1.745	VB R	0.0188	11.64653	8.57712	0.3141

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
10	1.860	BB	0.0174	7.76987	6.30026	0.2096
11	1.936	BB	0.0345	59.63470	24.02159	1.6085
12	2.147	BB	0.0179	31.38164	26.25699	0.8464

Totals : 3707.57174 2171.40689

=====  
\*\*\* End of Report \*\*\*