


=====

Acq. Operator	: SYSTEM	Seq. Line	: 2
Acq. Instrument	: MRK0111734	Location	: 2
Injection Date	: 9/30/2021 5:26:25 PM	Inj	: 1
		Inj Volume	: Manually
Sequence File	: C:\Chem32\2\Data\Photobromination\E-Z 2021-09-30 17-18-47\E-Z.S		
Method	: C:\Chem32\2\Data\Photobromination\E-Z 2021-09-30 17-18-47\Photobromination-09-30-2021.M (Sequence Method)		
Last changed	: 9/30/2021 5:18:47 PM by SYSTEM		

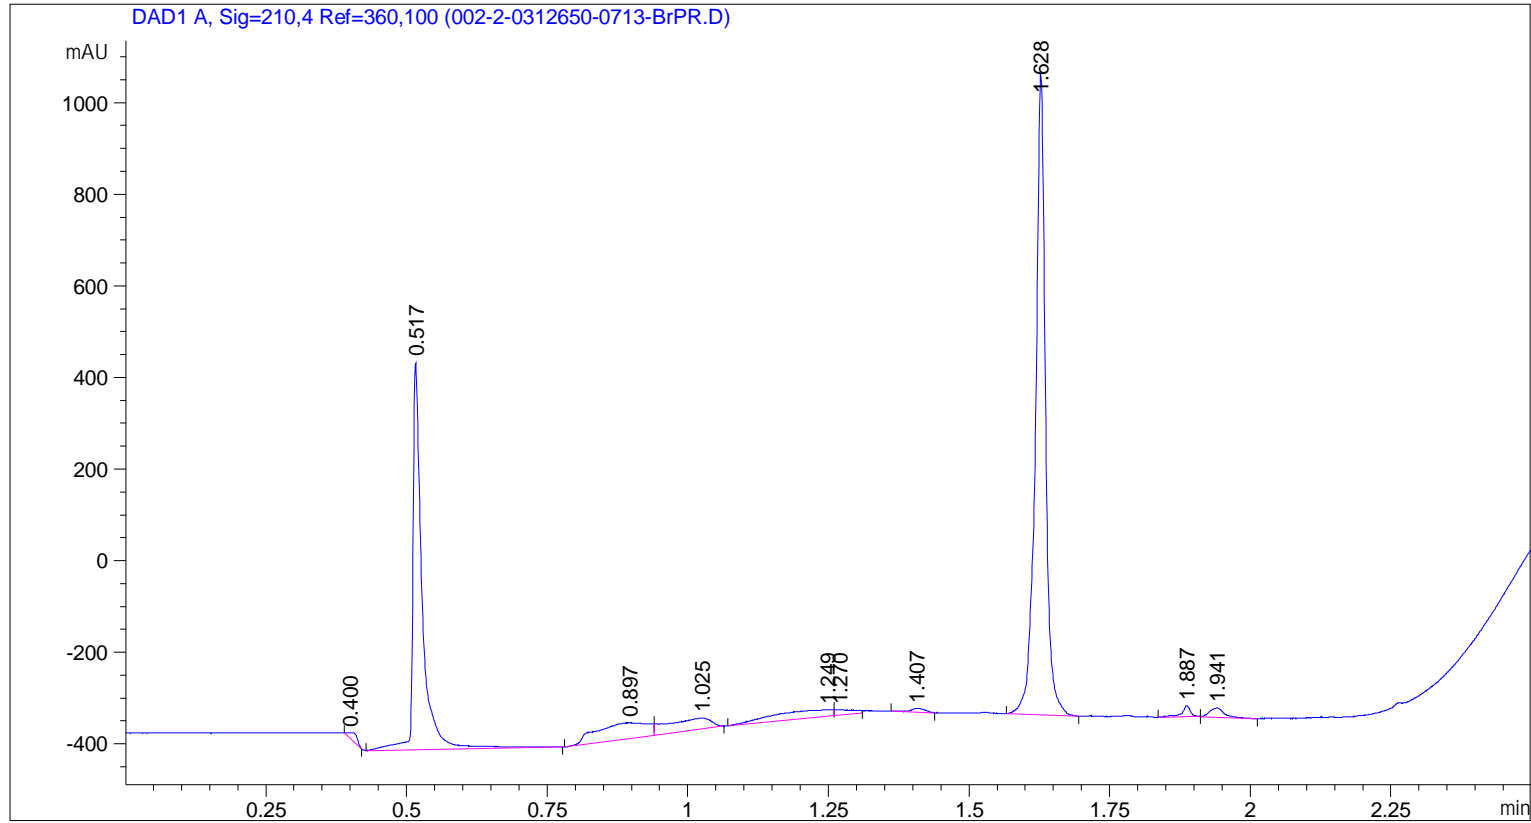

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=210,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	0.400	BB	0.0243	18.95500	11.78653	0.5664
2	0.517	BV R	0.0166	985.67773	846.32306	29.4553
3	0.897	BV	0.0843	230.61633	34.37188	6.8916
4	1.025	VB	0.0721	142.90073	23.78867	4.2703
5	1.249	BV	0.1118	129.43759	13.94251	3.8680
6	1.270	VV	0.0274	26.11085	11.53128	0.7803
7	1.407	VB R	0.0246	14.52770	8.04364	0.4341
8	1.628	BB	0.0180	1734.63611	1395.96057	51.8366
9	1.887	VB R	0.0159	26.88609	24.33208	0.8034

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
10	1.941	BB	0.0284	36.60779	19.92050	1.0940

Totals : 3346.35593 2390.00071

=====
*** End of Report ***