


```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    3
Acq. Instrument : MRK0111734                 Location  :    3
Injection Date  : 9/30/2021 5:31:33 PM        Inj       :    1
                                           Inj Volume: Manually
Sequence File   : C:\Chem32\2\Data\Photobromination\E-Z 2021-09-30 17-18-47\E-Z.S
Method          : C:\Chem32\2\Data\Photobromination\E-Z 2021-09-30 17-18-47\Photobromination-
                  09-30-2021.M (Sequence Method)
Last changed    : 9/30/2021 5:18:47 PM by SYSTEM
=====
```

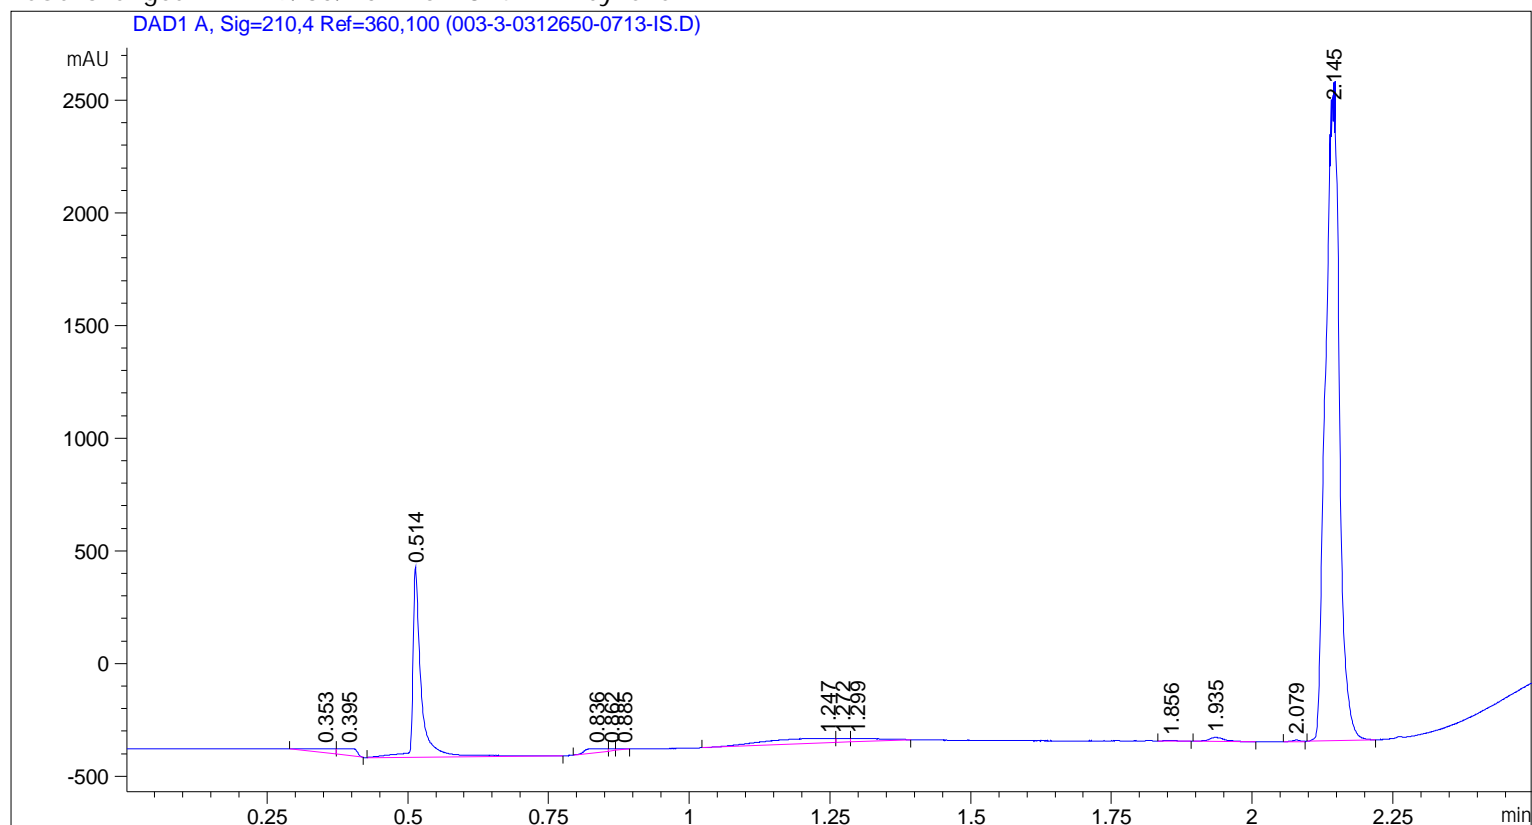

Area Percent Report

```
Sorted By      : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=210,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	0.353	VV R	0.0443	61.99318	19.15078	0.9736
2	0.395	VB	0.0270	70.77362	31.77917	1.1115
3	0.514	BV R	0.0148	880.76385	836.17328	13.8321
4	0.836	BV	0.0380	43.84267	16.50947	0.6885
5	0.862	VV	9.57e-3	6.76123	9.20469	0.1062
6	0.885	VB	0.0255	5.57192	2.82657	0.0875
7	1.247	BV	0.1180	203.84419	20.50791	3.2013
8	1.272	VV	0.0196	27.85519	17.93297	0.4375
9	1.299	VB	0.0466	54.63644	14.94552	0.8580

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
10	1.856	BB	0.0200	5.38268	3.79929	0.0845
11	1.935	BB	0.0303	36.78321	18.03216	0.5777
12	2.079	BB	0.0138	6.48007	6.97272	0.1018
13	2.145	BB	0.0261	4962.83008	2816.32788	77.9398

Totals : 6367.51834 3814.16241

=====  
\*\*\* End of Report \*\*\*