

Material Damage to Multielectrode Arrays after Electrolytic Lesioning is in the Noise

Reviewed Preprint

v1 • June 9, 2025

Not revised

Alice Tor, Stephen E Clarke, Iliana E Bray, Paul Nuyujukian , the Brain Interfacing Laboratory

Electrical Engineering Department, Stanford University, Stanford, United States • Bioengineering Department, Stanford University, Stanford, United States • Neurosurgery Department, Stanford University, Stanford, United States • Wu Tsai Neurosciences Institute, Stanford University, Stanford, United States • Stanford Bio-X, Stanford University, Stanford, United States

 https://en.wikipedia.org/wiki/Open_access Copyright information

eLife Assessment

This **useful** manuscript addresses a stability issue for long-term chronically implanted array recordings and electrolytic lesioning, which is relevant to both basic science and translational research. The authors provide a systematic scanning electron microscopy (SEM) of explanted arrays, evaluating electrode damage and sharing extensive datasets accessible through interactive plots. The strength of the evidence is **solid**, but it can be improved by performing additional analyses on complementary neurophysiology, functional, or histological data.

<https://doi.org/10.7554/eLife.106452.1.sa2>

Abstract

The quality of stable long-term recordings from chronically implanted electrode arrays is essential for experimental neuroscience and brain-computer interfaces. This work uses scanning electron microscopy (SEM) to image and analyze eight 96-channel Utah arrays previously implanted in motor cortical regions of four subjects (subject H = 2242 days implanted, F = 1875, U = 2680, C = 594), providing important contributions to a growing body of long-term implant research leveraging this imaging technology. Four of these arrays have been used in electrolytic lesioning experiments (H = 10 lesions, F = 1, U = 4, C = 1), a novel electrolytic perturbation technique using small direct currents. In addition to surveying physical damage, such as biological debris and material deterioration, this work also analyzes whether electrolytic lesioning created damage beyond what is typical for these arrays. Each electrode was scored in six damage categories, identified from the literature: abnormal debris, metal coating cracks, silicon tip breakage, parylene C delamination, parylene C cracks, and shank fracture. This analysis confirms previous results that observed damage on explanted arrays is more severe on the outer-edge electrodes versus inner electrodes. These findings also indicate that there are no statistically significant differences between the damage observed on normal electrodes versus electrodes used for electrolytic lesioning. This work provides evidence that electrolytic lesioning does not significantly affect the quality of chronically implanted electrode arrays and can be a useful tool in understanding

perturbations to neural systems. Finally, this work also includes the largest collection of single-electrode SEM images for previously implanted multielectrode Utah arrays, spanning eleven different intact arrays and one broken array. As the clinical relevance of chronically implanted electrodes with single-neuron resolution continues to grow, these images may be used to provide the foundation for a larger public database and inform further electrode design and analyses.

Introduction

In the past two decades, the advancement of implanted electrode arrays has drastically shifted the field of neuroscience from theories based on individually recorded neurons to those based on the systems-level activity of neuron populations [1–3]. Specifically, the 96-channel Utah array (Blackrock Neurotech, Salt Lake City, UT) has been used to make pivotal discoveries in motor systems neuroscience and develop clinically impactful brain-computer interfaces [2, 4–8]. These electrode arrays are widely used in neuroprosthetics research for patients with motor disorders and have been used for a variety of purposes, such as movement and speech decoding [9, 10]. Much of this work in humans relies on the translation of results discovered in non-human primates (NHPs), a crucial animal model in neuroscience research [11, 12]. One useful application of these arrays in animal studies is microstimulation and electrolytic lesion experiments [13]. Electrolytic lesioning results in small, controllable, and precise amounts of neuron loss. This makes it a helpful technique to study damage to targeted areas of the brain, serving as a model for clinical injury-based neuron loss events at a small scale.

Electrolytic lesion has been experimented with since the 19th century [14], and methods have been researched in many species, including cats, dogs, monkeys, and humans [15, 16]. In electrolytic lesion experiments, researchers pass current through nearby electrodes on arrays in order to mark the position of electrodes or create lesions in brain tissue [17, 18]. In particular, recent work has established a novel lesioning technique to create consistent, controllable electrolytic lesions in NHPs using already-implanted Utah arrays, without damaging the ability to record from the array [19]. However, while recording capabilities seem to remain stable, the physical effect of electrolytic lesioning on the recording array needs further characterization.

Previous studies have shown temporally decreasing performance of collected signals from long-term implanted arrays, thought to be a consequence of the immune response, mechanical movement of the array relative to surrounding tissue, and physical degradation of the array [20–22]. This is also reflected in studies that specifically examine the damages that occur to electrode arrays while they are implanted in NHPs [23, 24]. In particular, the use of scanning electrode microscopy (SEM) has been used to visually examine and analyze the effect of neural implantation on arrays with extremely high definition [24–28]. These studies, which span both NHPs and humans, provide direct evidence that the observable physical damage incurred by implanted arrays has direct impact on the array's performance.

The Utah array is a silicon-based array manufactured with several layers of different materials [29]. Silicon electrodes are first etched out of a glass and silicon base. Each individual electrode is then metallized at the tip. Finally, a layer of parylene C coats all but these metallized tips to help isolate and insulate each electrode [30, 31]. Both *in vitro* and *in vivo* testing of electrode arrays revealed environmental damage to these materials, such as cracking, textural defects, and degradation in response to the brain's temperature and salinity [32]. The immune response of the brain also damages the electrodes due to effects like glial scarring (gliosis) and inflammation [33, 34]. This damage may be exacerbated by the surgical techniques used during implantation, which include pushing the electrode array into cortex and tethering the implant to the skull [33, 35, 36].

Additionally, the Utah array is available with both platinum and iridium oxide-based coatings. Aggressive electrical stimulation is known to dissolve platinum-based electrodes [37, 38]. Other studies have shown iridium oxide to be more resistant to stimulation-related damage, but not completely insusceptible [39, 40]. However, the physical electrode damage associated with electrolytic lesioning remains to be studied.

This work comprises images of eleven different multielectrode Utah arrays (ten 96-channel, one 64-channel). Of these imaged arrays, eight arrays chronically implanted in regions of the motor cortex for varying amounts of time were analyzed further (monkey H = 2242 days, F = 1875, U = 2680, C = 594). Four out of eight of these arrays were used to perform electrolytic lesioning experiments (n = 4 monkeys; H = 10 lesions, F = 1, U = 4, C = 1). Additionally, the image set includes images of a broken 96-channel Utah array, which was shattered during explant but remained intact while implanted. This set of images represents the largest publicly available collection of high-quality, single-electrode SEM images of explanted multielectrode Utah arrays. A total of 938 individual electrodes are available to view, along with 11 additional images from the broken array. Specific details for each imaged array are available in Table 1 (*arrays.csv*).

Methods

Array Preparation

Monkey H, F, and C were each implanted with two 96-channel Utah arrays in M1 and PMd. H's M1 array was used for electrolytic lesioning experiments. F's and C's PMd arrays were used for electrolytic lesioning experiments. Monkey U was implanted with three 96-channel arrays; two in M1 and one in PMd. U's lateral M1 array was used for electrolytic lesioning experiments. U's medial M1 array was not used for recording and was severely damaged during extraction. Monkey H's arrays were implanted for 2242 days (electrolytic lesions on days 2088, 2129, 2136, 2164, 2172, 2180, 2187, 2192, 2221, 2228). Monkey F's arrays were implanted for 1875 days (electrolytic lesion on day 1875). Monkey U's arrays were implanted for 2680 days (electrolytic lesions on days 1215, 1250, 1264, 1286). Monkey C's arrays were implanted for 594 days (electrolytic lesion on day 304). Further details on each monkey's arrays, as well as any additional imaged arrays, are available in **Supplemental Table 1**.

All arrays used in this work were multielectrode Utah arrays (Blackrock Neurotech, Salt Lake City, UT). Monkey C was implanted with an array with electrode shank lengths of 1.5 mm, while Monkeys H, F, and U were implanted with arrays with electrode shank lengths of 1 mm. Monkey U and C's arrays were manufactured with an iridium oxide metal coating, while H and F's arrays were manufactured with platinum coatings.

Arrays were first soaked in either a 0.9% saline or 10% formalin solution immediately following explant surgery, then stored separately in either water, formalin, ethanol, or dry in a closed container. Prior to imaging, all arrays were allowed to dry without any further cleaning or preparation.

Scanning Electron Microscopy

Scanning Electron Microscopy (SEM) images were collected using a Hitachi TM4000+ Tabletop SEM (Hitachi Ltd., Tokyo, Japan). Arrays were mounted on PELCO SEMClip™ Pin Mounts (Ted Pella, Redding, CA) using conductive copper tape, carbon tape, and included clip mounts. Arrays were not sputter-coated for imaging. Due to the amount of organic material left on the arrays, images were collected in low-vacuum mode to avoid distortion from accumulated electrical charge of the non-conductive material. Full array images were collected with the arrays flat on the mount surface, while single-electrode images were collected with the arrays positioned at an approximate 45° angle. Most images were collected using a mixed backscatter/secondary electron (BSE/SE)

mode with a low accelerating voltage of 5kV, although modes and voltage values were adjusted for certain electrodes to optimize image clarity. Specific settings for each collected image are included in **Figure 1** [↗](#).

Figure 1:

Interactive Display [↗](#): Interactive display of all captured SEM array images. Once an array has been selected, a diagram of each array's anatomical position (derived from surgical drawings and notes) appears, along with an SEM image of the array. All array images are displayed with the wire bundle to the right side. Specific electrodes may be selected from the array image; SEM images of each electrode and their scores in each of the five damage categories will appear along with any additional notes. Furthermore, examples of specific scores for each damage type are selectable through an additional drop-down menu for each array. Similarly, electrodes used for electrolytic lesioning are also selectable through an additional drop-down menu for each array.

Damage Scoring

A prior study categorized damage observable with SEM into six distinct types: abnormal debris, tip breakage, coating cracks (cracking of the metal coating around the silicon core of an electrode), parylene C cracks, parylene C delamination, and shank fracture [26 [↗](#)]. Similarly, damage to the arrays in this study were scored in five categories: abnormal debris (AB), silicon tip breakage (TB), platinum coating cracks (CC), parylene C coating cracks (PC), and parylene C coating delamination (PD). Each recording electrode was scored from 0 to 3 in five different categories, as described above. Electrodes with shank fractures (SF) were not scored, as these fractures may have reasonably occurred during explantation and handling of the arrays separate from the damage incurred while in the brain. Each electrode was scored between 0-3, where 0 indicated no visible effects, 1 indicated visible effects but likely no impact on recording ability, 2 indicated possible impact on recording ability, and 3 indicated likely impact on recording ability. Scores were given without prior knowledge of which electrodes had been used for electrolytic lesioning. Although this scoring system is subjective and based on visual observation, all images used to compute these scores are publicly available in **Figure 1** [↗](#) for independent evaluation.

Statistical Tests

First, the Pearson's correlation coefficient was calculated between each subcategory of damage to determine whether any types of damage were related. To explore potential spatial relationships, this analysis was repeated for each radial ring of electrodes, as shown in **Supplemental Figure 4** [↗](#).

Statistical significance was also assessed between electrodes used in the electrolytic lesion experiments versus those which had not. The Shapiro-Wilk test indicated that scores did not follow a normal distribution; therefore, nonparametric methods such as the Mann-Whitney U test and the Levene test were used to compare the underlying statistics of each array's electrode population. The null hypothesis of the Mann-Whitney U test is that sample means of two sets of scores are the same. The null hypothesis of the Levene test is that the sample variance of two sets of scores are the same.

Similarly, statistical significance was assessed as described above between lesioning versus normal electrodes pooled across all four arrays used for electrolytic lesioning. Finally, this analysis was repeated between electrode scores across pairs of lesioning and non-lesioning arrays implanted in the same subject for the same length of time.

Results

All collected images, along with their associated scores, are available in interactive **Figure 1** [↗](#). Each of the twelve arrays and individual electrodes may be selected and viewed. Representative electrodes for each category and damage score are also viewable for each array when available. Electrodes used for lesioning are also viewable when available. Rough anatomical layouts of the array's implant location are also included. Electrode numbering maps are available in **Supplemental Figure 1** [↗](#).

The first set of analyses specifically considers the four arrays used in electrolytic lesioning experiments. Scores for each damage category, along with total scores, are visualized as heatmaps in **Figure 2** [↗](#). Median total scores for each radial section of the array show that the outermost electrodes tend to have the greatest total observed damage across all four arrays. Generally, electrode damage decreases when moving to the center of the array. Shank fractures tend to be spatially close on each array, suggesting that shared mechanical trauma caused these sections of fracture. As mentioned in the Methods section, these fractures may have reasonably occurred during explantation and handling, as no diminished recording performance of these fractured electrodes was observed while the array was actively implanted. Additional heatmaps are available for the four additional arrays implanted in NHP but not used for lesioning in **Supplemental Figure 2** [↗](#).

Histograms of damage scores in each category, along with average score distributions per array, are shown in **Figure 3** [↗](#). For each category, histograms of electrodes used for lesioning (black) are stacked on top of histograms of normal electrodes (gray). Additionally, the average distribution of scores is shown for each array. These plots indicate that there is no observable difference in the distribution of scores given to electrodes used for lesioning versus those not. Additional histograms are available for the four additional arrays implanted in NHP but not used for lesioning in **Supplemental Figure 3** [↗](#).

The Shapiro-Wilk test for normality returned a significant p -value for almost all sets of scores for each array and type of damage. Similarly, the Shapiro-Wilk test for normality returned a significant p -value for almost all sets of scores for each array and type of damage when split into populations used and not used for lesioning, but was not performed where electrode count was too small to carry out the test (C and F; lesioning electrodes = 2). In the majority of cases that returned an insignificant p -value, certain types of damage were not present on the array and thus scores were uniformly zero (monkey U's M1 tip breakage, parylene C delamination, and parylene C cracking scores; monkey C's PMd parylene C delamination scores and M1 parylene C cracking scores). In all other cases where the Shapiro-Wilk test returned an insignificant p -value (monkey H's total damage scores on lesioning electrodes, monkey U's coating cracks scores), low electrode counts may reduce the statistical power of the test (H = 18 lesioning electrodes, U = 8). This indicates that scores are largely not normally distributed and that nonparametric statistical tests should be used to evaluate differences between populations. All Shapiro-Wilk test p -values are available in **Supplemental Table 2** [↗](#).

When comparing lesioning and non-lesioning electrodes within the same array, each of the two nonparametric statistical tests (Mann-Whitney U-test, Levene Test) returned insignificant p -values for each category of damage as well as for total damage scores for all four arrays used in lesioning experiments. Similarly, when comparing pooled lesioning and non-lesioning electrodes across all four lesioning arrays, each of the two tests returned insignificant p -values for each category of damage and total damage scores. This indicates that the electrode populations used for lesioning and those not used for recording only do not have statistically different sample means or variances, suggesting they are samples of the same underlying population. These p -values are

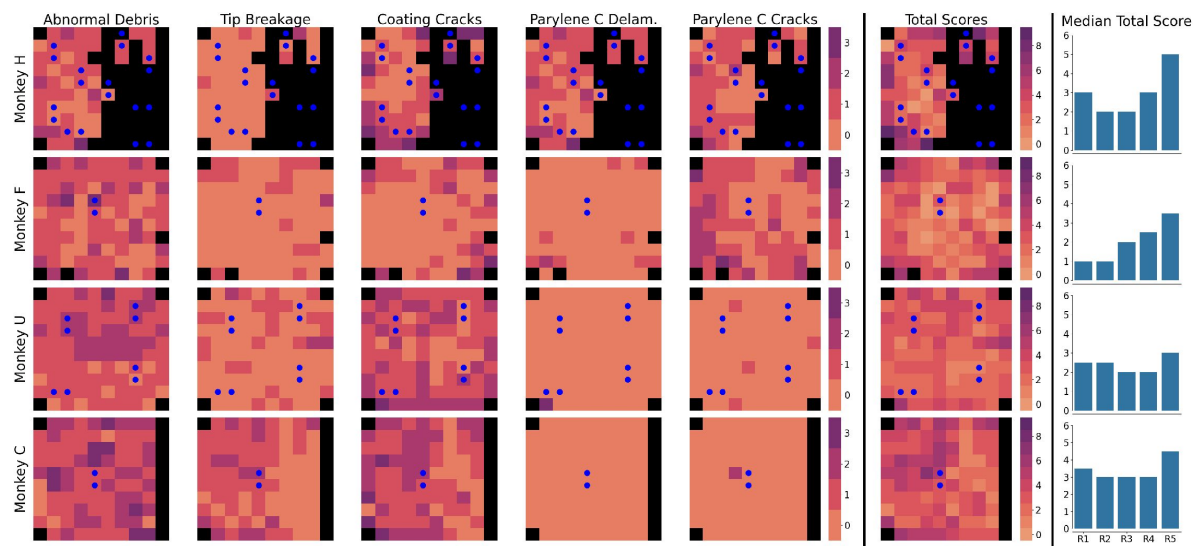


Figure 2

Heatmaps of damage scores (0-3) across the five identified types of damage and across the four imaged lesioning arrays.

Electrodes are displayed using the orientation in [Figure 1](#) (electrode tips facing viewer, wire bundle on the right). Second-to-rightmost column displays summed damage scores for each array across the five types of damage. Electrodes used for electrolytic lesioning are denoted with blue dots. Median summed scores for each radial section of the array are plotted in the bar charts to the right of the heatmaps. Ring layout and numbering information is available in [Supplementary Figure 1](#). Blank electrodes and electrodes with shank fractures are ignored and displayed in black, as they are not scored.

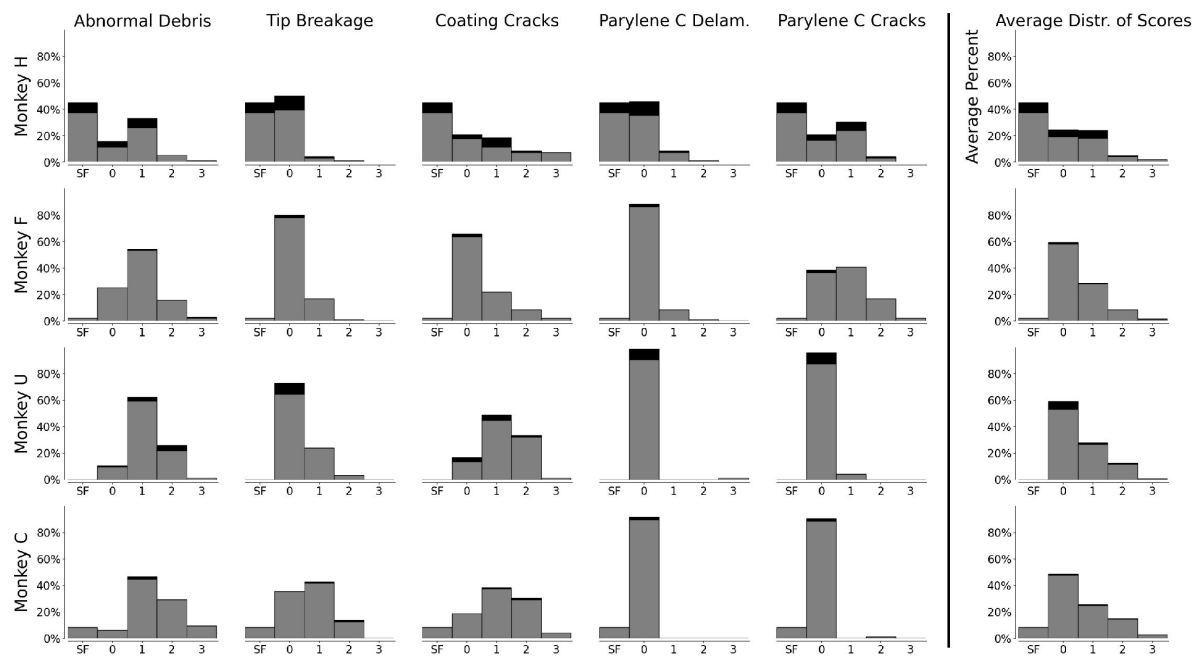


Figure 3

Stacked histograms of damage scores (0-3) across the five identified types of damage and across the four imaged lesioning arrays.

Gray indicates normal electrodes, and black indicates lesioning electrodes. Rightmost column displays the average distribution of damage scores across the five types of damage. Electrodes with shank fractures (SF) are ignored, as they are not scored.

included in **Supplemental Table 3** [\[28\]](#). However, again, it is important to note that these tests done on individual arrays have limited power due to low electrode counts ($H = 18$ lesioning electrodes, $F = 2$, $U = 8$, $C = 2$).

This next set of analyses compares entire population statistics of all eight NHP arrays. Both tests resulted in inconsistently significant/non-significant p -values when comparing lesioning arrays against non-lesioning arrays within the same implanted animal. In monkey H, the Mann-Whitney U test resulted in an insignificant p -value for coating cracks and parylene C delamination scores, while the Levene test resulted in an insignificant p -value for abnormal debris, coating cracks, and parylene C cracking scores. In monkey F, the Mann-Whitney U test resulted in an insignificant p -value for parylene C delamination scores, while the Levene test resulted in an insignificant p -value for coating cracks, parylene C delamination, and parylene C cracking scores. In monkey U, the Mann-Whitney U test resulted in significant p -values for all scores, while the Levene test resulted in an insignificant p -value for abnormal debris, tip breakage, and coating cracks scores. Finally, in monkey C, the Mann-Whitney U test resulted in an insignificant p -value for parylene C delamination and parylene C cracking scores, while the Levene test resulted in an insignificant p -value for abnormal debris, parylene C delamination, and parylene C cracking scores. This indicates that there are likely large differences between the amount and intensity of material damage dealt to implanted arrays even when implanted in the same subject. These results do not determine whether or not electrolytic lesioning experiments contribute to the magnitude of these differences, but the inconsistency in the significance of the above results may indicate that other factors, such as the brain's varied immune response, differences in mechanical forces, and disparities in external handling, may play a large role in damage to these arrays. These p -values are included in **Supplemental Table 4** [\[28\]](#).

The Pearson correlation matrix across all four arrays for the five different damage types is shown in **Figure 4** [\[28\]](#). This plot demonstrates that there is overall low pairwise correlation between each type of damage, with the exception of coating cracks and tip breakage, which display moderate positive correlation ($r = 0.47$, Bonferroni-corrected $p < 0.05$). These results align with previous comparisons on the distribution of damage scores, which showed that damage score tended to vary across the five different types. Additional correlation plots for each of the five array layout rings are available in Supplemental Materials. Raw r and p -values for each test are also available in **Supplemental Table 5** [\[28\]](#).

Discussion

Overall, these results collectively demonstrate that there is no obvious, statistically significant difference between observed damage to electrodes used versus not used for electrolytic lesioning. Because this method of lesioning involves passing limited direct current into the brain over relatively short time periods, its physical effects on the array electrodes are similar to alternating current stimulation. A recent study found that SEM-visible damage caused by stimulation on iridium oxide electrodes is highly variable between arrays, where one imaged array demonstrated noticeable stimulation-related damage and the other array had no such damage [\[28\]](#). Furthermore, the study found that array recording quality was not compromised by stimulation. Similarly, other work did not show significant differences in SEM-visible degradation between both platinum and iridium oxide coated electrodes used for stimulation [\[24\]](#), [\[25\]](#). All of these previous studies used different stimulation protocols: a pulse train delivered at 20-300 Hz at amplitudes 1-100 μA [\[28\]](#), a pulse train delivered at 300 Hz at amplitudes 1-210 μA [\[24\]](#), and an undisclosed low-current stimulation [\[25\]](#). Additionally, dissolution of electrodes due to current is most salient at aggressive levels of stimulation; one study reviewing electrode dissolution delivered variable amplitudes of current at 50 Hz for seven hours [\[40\]](#); another study utilized currents at least one order of magnitude greater than the above protocols [\[37\]](#). The electrolytic lesioning in this work primarily used direct currents delivered at around 150 μA for 45

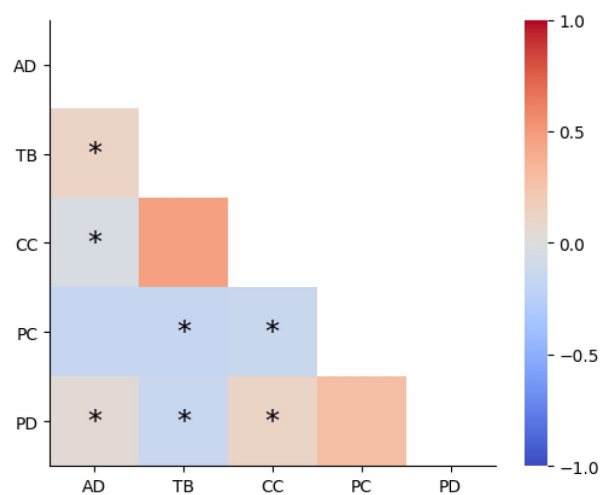


Figure 4

Correlation plot (Pearson's R) across the five different damage types.

AD = abnormal debris, TB = tip breakages, CC = metal coating cracks, PC = parylene C cracks, PD = parylene C delamination. Results demonstrate overall low correlation (magnitude < 0.25) across different damage types, with the exception of coating cracks and tip breakage, with a correlation coefficient of 0.47. Test values with Bonferroni-corrected $p < 0.05$ are displayed with asterisks. Raw p-values are separately available in Supplementary Table S1 (*corr_pvals.csv*). Electrodes with shank fractures are ignored, as they are not scored.

seconds, though parameters ranged between 50–450 μ A and 12–600 seconds. Thus, despite the differences between specific lesioning and stimulation protocols, the findings presented here are consistent with previous studies that found no unusual damage to the electrodes used for stimulation. This aligns with previous findings that electrolytic lesioning does not significantly impact the recording ability of electrodes [19].

The patterns of damage found in this work also largely reflect previous SEM analyses of explanted arrays. A prior study also found that the electrodes closest to the perimeter of the array suffered the most damage [25]. This pattern is also visually observable in other published results [26, 28]. This is likely because the edges of the arrays serve as a physical shield for the innermost electrodes. Edge electrodes are subject to greater access to brain tissue, as well as to mechanical damage incurred during surgery and handling.

The frequency of damage types identified in this work differ from previous studies, but is not unusual. In this work, the most common damage type within arrays used for lesioning is abnormal debris (n=276, 71.9%), followed by metal coating cracks (n=214, 55.7%), tip breakage (n=102, 26.6%), parylene C cracks (n=95, 24.7%), and parylene C delamination (n=48, 12.5%). On these lesioning arrays, there were n=53, or 13.8%, shank fractures. Similarly, across all eight NHP arrays imaged, the most common damage type is abnormal debris (n=518, 67.4%), followed by metal coating cracks (n=480, 62.5%), tip breakage (n=233, 30.3%), parylene C cracks (n=224, 29.2%), and parylene C delamination (n=60, 7.8%). Across all eight NHP arrays, there were n=117, or 15.2%, shank fractures. However, a prior study found that coating cracks were the most common type of observed damage, followed closely by parylene C cracks, then tip breakage, abnormal debris, and parylene C delamination [26]. While the frequency of damage types are not exactly aligned, previous work included a cleaning step during array preparation for SEM imaging; this work does not explicitly attempt to remove excess brain tissue from imaged arrays, which likely led to the relative increase we observed in abnormal debris. Additionally, variation in individual researcher's scoring standards may also contribute to differences. As mentioned above, the overall spatial pattern of damage between these two studies is consistent.

This study found a moderate positive correlation between coating cracks and tip breakage. This reflects the fact that damage to the silicon core of an electrode often occurs in tandem with cracking and flaking of the surrounding metal coating; the silicon cannot break without also breaking its coating. This correlation is visible in the collected images presented in **Figure 1**.

Conclusion

This work analyzed high-definition SEM images of previously implanted electrode arrays used for electrolytic lesioning. Across all eight arrays previously implanted in NHPs, damage disproportionately occurred to the outer edges of arrays. Additionally, no statistically significant difference was found between the damage experienced by normal and lesioning electrodes within the same array. Furthermore, statistical testing between arrays used and not used for lesioning experiments did not indicate consistent, significant differences. Finally, this work also presents the largest publicly available set of SEM images of explanted arrays, consisting of eleven different multielectrode Utah arrays (ten 96-channel, one 64-channel) and one broken 96-channel array. These results from this dataset align with previous SEM studies of chronically implanted arrays used for both recording and stimulation, while providing further evidence for electrolytic lesioning as a safe and useful technique for experimental neuroscience.

Supplemental Materials

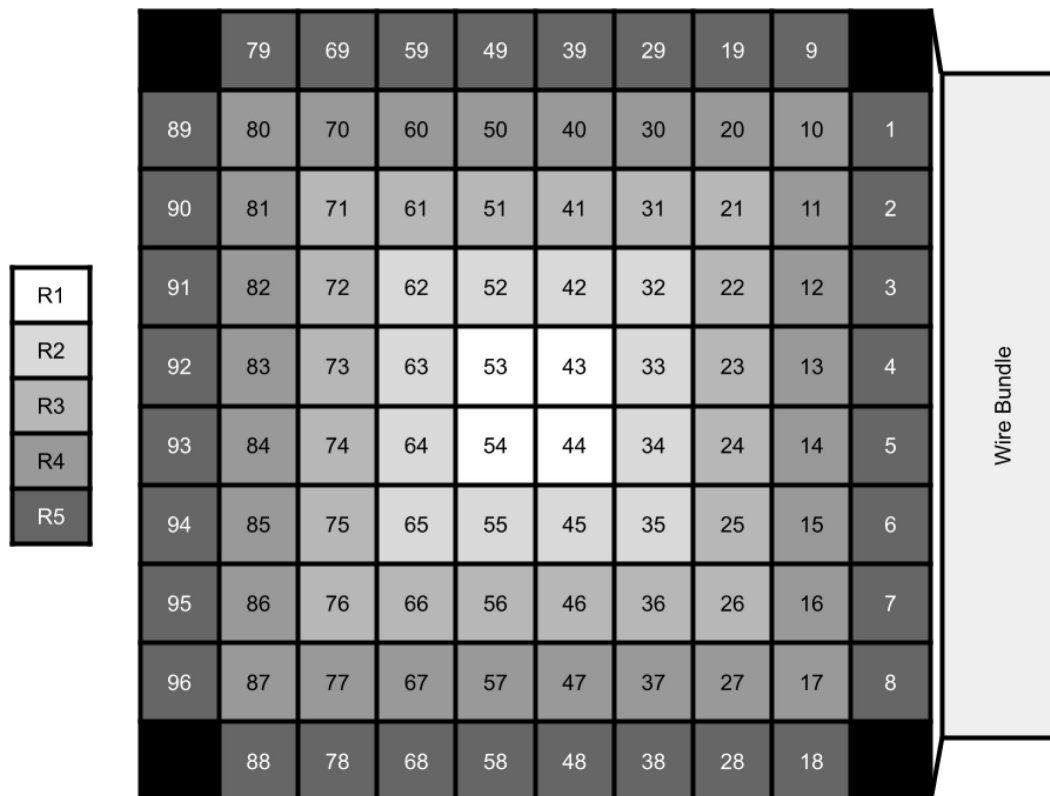


Figure 1

Numbering layout of the electrodes as imaged (pins facing outwards, towards reader).

Wire bundle is arranged to the right. Each radial section of the array is also color-coded and labeled. R1 refers to the innermost core electrodes of the array, R2 refers to the next outer ring of the array, and so on.

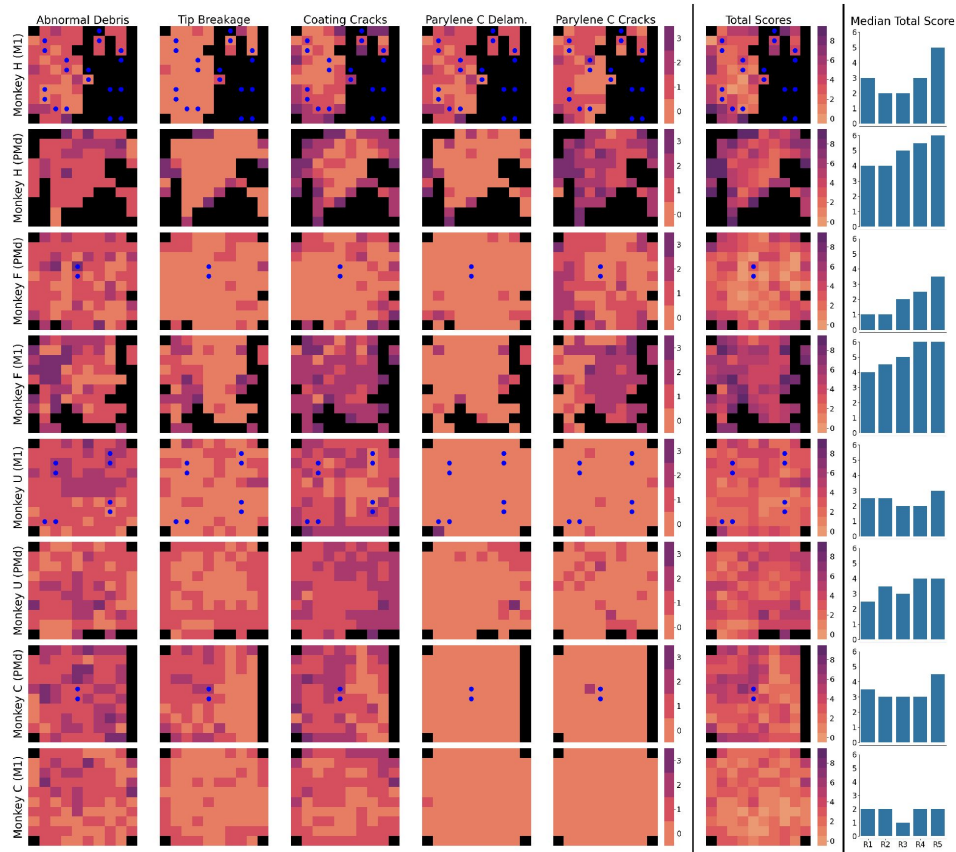


Figure 2

Heatmaps of damage scores (0-3) across the five identified types of damage and across all eight intact, imaged NHP arrays.

Electrodes are displayed using the orientation in [Figure 1](#) (electrode tips facing viewer, wire bundle on the right). Second-to-rightmost column displays summed damage scores for each array across the five types of damage. Electrodes used for electrolytic lesioning are denoted with blue dots. Median summed scores for each radial section of the array are plotted in the bar charts to the right of the heatmaps. Ring layout and numbering information is available in Supplementary Figure 1. Blank electrodes and electrodes with shank fractures are ignored and displayed in black, as they are not scored. All raw data histograms:

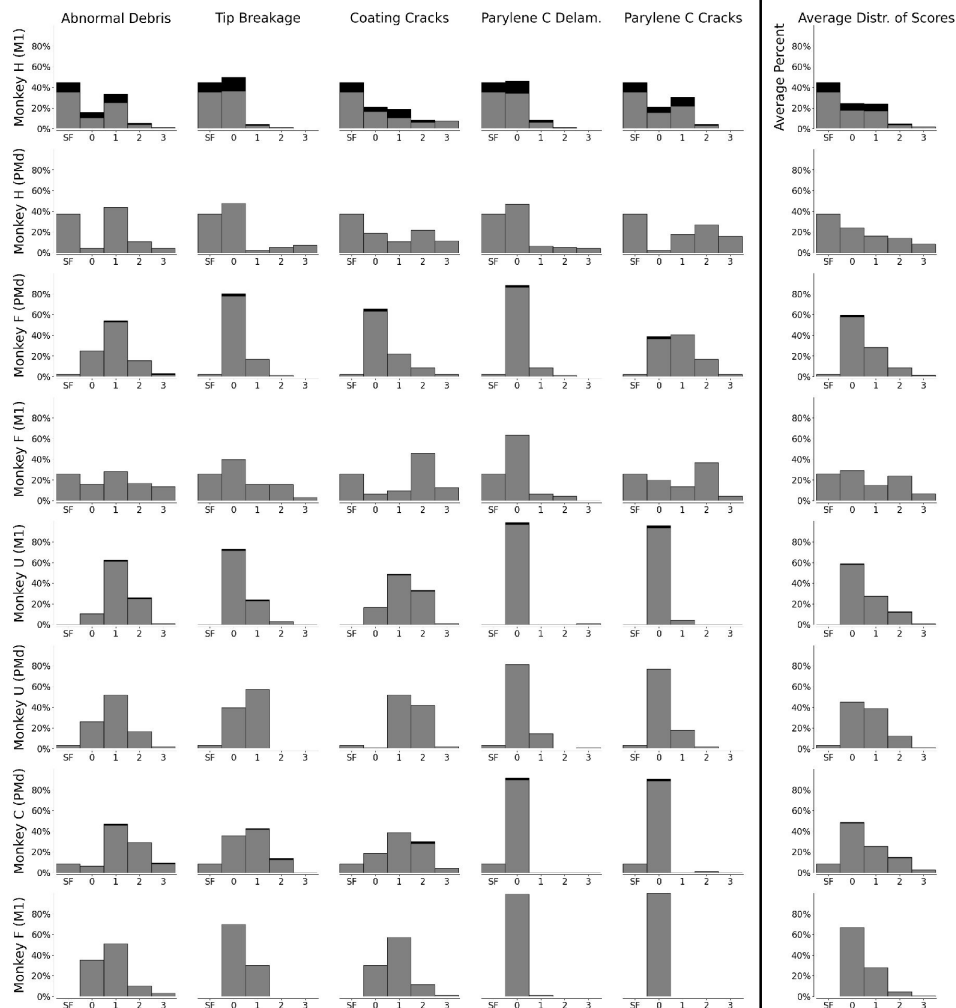


Figure 3

Stacked histograms of damage scores (0-3) across the five identified types of damage and across all eight intact, NHP imaged arrays.

Gray indicates normal electrodes, and black indicates lesioning electrodes. Rightmost column displays the average distribution of damage scores across the five types of damage. Electrodes with shank fractures (SF) are ignored, as they are not scored.

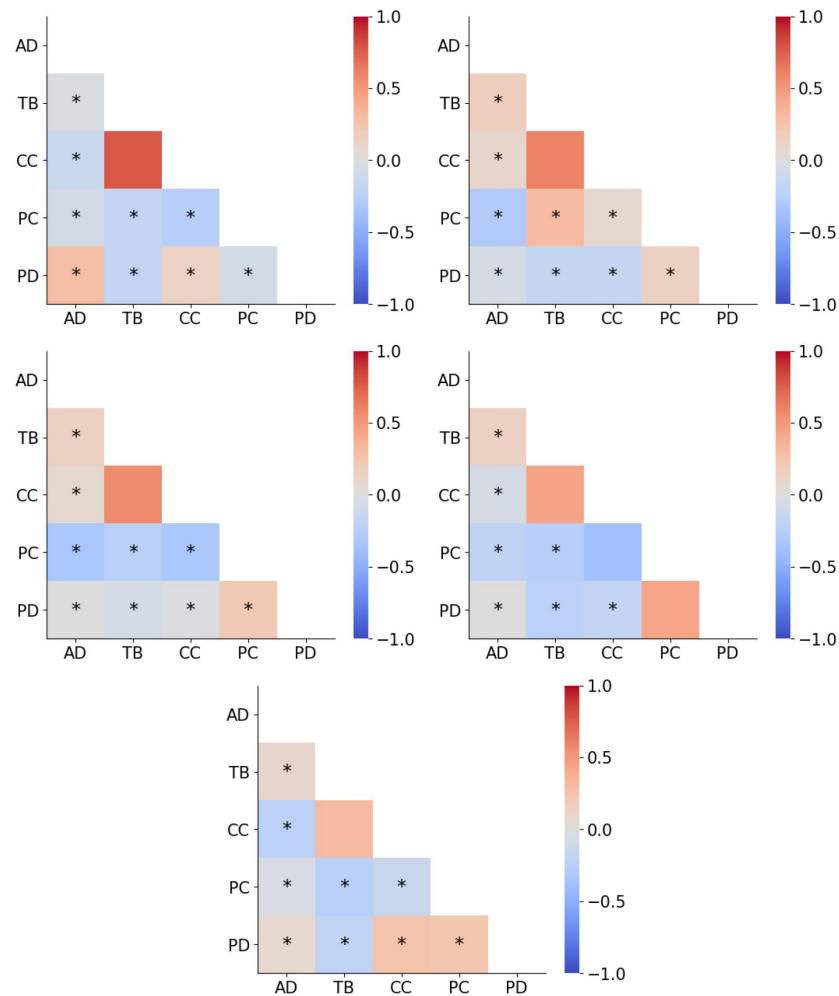


Figure 4

Correlation plots (Pearson's R) for each of the five rings across all four imaged lesioning arrays.

Test values with Bonferroni-corrected $p < 0.05$ are displayed with asterisks. Raw r and p -values are separately available in **Supplemental Table 5** [.corr_pvals.csv](#).

Subject	Region	Metal	Implant Date	Explant Date	Days	Serial Num	Size	Notes
H	PMd	Pt	Mar 17 2014	6 May 2020	2242	1024-1177	96	Missing wire bundle – layout/numbering is arbitrary
H	M1	Pt	Mar 17 2014	6 May 2020	2242	1024-1166	96	
F	PMd	Pt	Sep 8 2014	27 Oct 2019	1875	1024-1171	96	
F	M1	Pt	Sep 8 2014	27 Oct 2019	1875	1024-1175	96	Missing wire bundle; previously encapsulated in fibrin
U	PMd	IrOx	Aug 4 2017	Dec 5 2024	2680	1024-1903	96	
U	M1 medial posterior	IrOx	Aug 4 2017	Dec 5 2024	2680	1024-1902	96	Broken during extraction
U	M1 lateral anterior	IrOx	Aug 4 2017	Dec 5 2024	2680	1024-1905	96	
C	PMd	IrOx	Mar 25 2021	9 Nov 2022	594	6250-001604	96	
C	M1	IrOx	Mar 25 2021	9 Nov 2022	594	6250-001608	96	
Agar	x		25 Aug 2022	25 Aug 2022	x	1025-149	64	Implanted briefly into agar gel and used to test initial electrolytic lesioning protocols during development.
P	x	Pt	x	x	x	1024-0577	96	Used in multiple lesions associated with Bray*, Clarke*, et al., eLife 2024. Implanted and removed from brain tissue multiple times over weeks/months.
Control	x	x	x	x	x		96	Never-implanted array. Damage and debris are due to handling. One image is available per column.

Supplemental Table 1

Subject	Region	Lesioning Array	Population Type	Damage Type	Shapiro-Wilk p-value
H	M1	x	B	AD	1.42804836139459E-07
H	M1	x	L	AD	5.14581421400768E-05
H	M1	x	N	AD	3.4251327326555E-06
H	M1	x	B	TB	4.33911049381301E-14
H	M1	x	L	TB	2.24340190966374E-08
H	M1	x	N	TB	1.63199362287543E-12
H	M1	x	B	CC	1.92051001063433E-06
H	M1	x	L	CC	0.0042712561813056
H	M1	x	N	CC	1.00524346957516E-05
H	M1	x	B	PC	5.05326224327741E-08
H	M1	x	L	PC	0.00757198831234923
H	M1	x	N	PC	5.24258866624858E-07
H	M1	x	B	PD	1.57470321524184E-12
H	M1	x	L	PD	2.24340190966374E-08
H	M1	x	N	PD	9.72111013345503E-11
H	M1	x	B	TO	0.00196088898948222
H	M1	x	L	TO	0.0543916160610427
H	M1	x	N	TO	0.00575745652995584
H	PMd		N	AD	2.02488044532739E-09
H	PMd		N	TB	2.71949271992989E-12
H	PMd		N	CC	2.10503492650437E-06
H	PMd		N	PC	4.08525308564967E-06
H	PMd		N	PD	5.19181374109081E-12
H	PMd		N	TO	7.01151592562009E-05
F	PMd	x	B	AD	2.24138034381229E-09
F	PMd	x	N	AD	2.56094960787625E-09
F	PMd	x	B	TB	1.40566563727203E-16
F	PMd	x	N	TB	2.54915240329479E-16
F	PMd	x	B	CC	1.41772576549295E-13
F	PMd	x	N	CC	2.74977165926224E-13
F	PMd	x	B	PC	1.73853057453501E-09
F	PMd	x	N	PC	3.02475597652851E-09
F	PMd	x	B	PD	1.32641565577142E-18
F	PMd	x	N	PD	2.34607121360852E-18
F	PMd	x	B	TO	0.000821382536668179
F	PMd	x	N	TO	0.00100101587684811
F	M1		N	AD	2.22268865078584E-06
F	M1		N	TB	2.09458839844955E-09
F	M1		N	CC	8.38512476129703E-09
F	M1		N	PC	3.16296468295233E-08
F	M1		N	PD	2.95181625451619E-15
F	M1		N	TO	0.00712080567476207

Supplemental Table 2

U	M1	x	B	AD	1.01931015873618E-10
U	M1	x	L	AD	0.0269677691889137
U	M1	x	N	AD	1.8421430757103E-10
U	M1	x	B	TB	6.06127448212982E-15
U	M1	x	L	TB	1
U	M1	x	N	TB	7.25183149834534E-14
U	M1	x	B	CC	2.44229083679703E-09
U	M1	x	L	CC	0.055518589600575
U	M1	x	N	CC	5.93737318014387E-09
U	M1	x	B	PC	1.80366424846944E-20
U	M1	x	L	PC	1
U	M1	x	N	PC	1.57606437749686E-19
U	M1	x	B	PD	9.07914568433239E-22
U	M1	x	L	PD	1
U	M1	x	N	PD	7.16367592784744E-21
U	M1	x	B	TO	3.92990584792372E-07
U	M1	x	L	TO	0.0369705113246638
U	M1	x	N	TO	1.77768966940469E-06
U	PMd		N	AD	3.28412505296172E-09
U	PMd		N	TB	4.44829029275551E-14
U	PMd		N	CC	7.45233247435495E-12
U	PMd		N	PC	5.74342258675669E-16
U	PMd		N	PD	2.58453658531109E-17
U	PMd		N	TO	9.11695809588145E-05
C	PMd	x	B	AD	1.69628492723077E-08
C	PMd	x	N	AD	3.20127221514583E-08
C	PMd	x	B	TB	6.55085205402063E-10
C	PMd	x	N	TB	7.25214204182855E-10
C	PMd	x	B	CC	1.27161149525663E-07
C	PMd	x	N	CC	1.74411119850621E-07
C	PMd	x	B	PC	7.16367592784744E-21
C	PMd	x	N	PC	1.22364280072457E-20
C	PMd	x	B	PD	1
C	PMd	x	N	PD	1
C	PMd	x	B	TO	0.000508254345454471
C	PMd	x	N	TO	0.000609884112353611
C	M1		N	AD	3.17392329397468E-10
C	M1		N	TB	3.3334954694948E-15
C	M1		N	CC	2.05405184856033E-10
C	M1		N	PC	1
C	M1		N	PD	9.07914568433239E-22
C	M1		N	TO	2.14468981418305E-05

Supplemental Table 2 (continued)

Subject	Damage Type	Mann-Whitney p-value	Levene p-value
C	AD	0.34939796427893	0.210194589615018
C	TB	0.146299664570697	0.922337159856659
C	CC	0.601732165169982	0.755135149005505
C	PC	0.939220772891616	0.879826139676274
C	PD	1	
C	TO	0.586975166446875	0.770821921110027
H	AD	0.267269631101341	0.723668965127892
H	TB	0.965480188957675	0.827229963895785
H	CC	0.711720385395243	0.0141452099448486
H	PC	0.881728670889432	0.990000926659542
H	PD	0.438818746952947	0.414099914782603
H	TO	0.577102459345734	0.0918690459913866
F	AD	0.162311927607548	0.171541575967333
F	TB	0.517156528055703	0.519373890277442
F	CC	0.33506298012124	0.381623133289016
F	PC	0.110988060095175	0.119906163211853
F	PD	0.662292267902487	0.659852234622957
F	TO	0.631489792650266	0.649832962544392
U	AD	0.27637226224662	0.157904869032198
U	TB	0.0761724885130235	0.0895818944408695
U	CC	0.0766158007343267	0.907009685888015
U	PC	0.55276197318209	0.542838902077312
U	PD	0.791916752771162	0.764791019361425
U	TO	0.065942832319446	0.107677660373745
Aggregate	AD	0.480634974771593	0.952407623436657
Aggregate	TB	0.0682386364018035	0.108348821549793
Aggregate	CC	0.388544856985786	0.083911528663579
Aggregate	PC	0.76213264784547	0.675747175124029
Aggregate	PD	0.928399930406967	0.907614126469184
Aggregate	TO	0.10515346134016	0.0631115597608218

Supplemental Table 3

Mann-Whitney U and Levene test p-values when comparing scores between lesioning electrodes and non-lesioning electrodes on the same array.

Supplemental Table 4

Mann-Whitney U and Levene test p-values when comparing scores between all electrodes on arrays used and not used for lesioning experiments when implanted in the same subject.

Subject	Damage Type	Mann-Whitney p-value	Levene p-value
C	AD	3.9702024910792E-08	0.44237127251472
C	TB	2.34539856035073E-06	0.0012983938958146
C	CC	0.000889362010818785	0.0210633072017514
C	PC	0.301329708599682	0.297534819078251
C	PD	0.343869532236896	0.339732058028476
C	TO	8.92786689499138E-37	5.47676575956633E-24
H	AD	0.00233180554226348	0.656345273040929
H	TB	0.0290518081232991	0.00545249347108368
H	CC	0.0673025882077128	0.264196578921174
H	PC	6.00595340741551E-12	0.145802193983747
H	PD	0.191571141232335	0.0455899130122223
H	TO	0.0131545054441042	1.76091592125786E-05
F	AD	0.00988009256557466	0.00153586322205377
F	TB	1.00613698959391E-05	4.69968840817108E-07
F	CC	2.54815035508114E-18	0.947266220917349
F	PC	0.000234238887189781	0.120999207470919
F	PD	0.332612703749588	0.181411536064707
F	TO	9.00982235883871E-07	0.000304591399938728
U	AD	0.0130634950208513	0.200854879875423
U	TB	3.19600588646131E-05	0.15312649243633
U	CC	0.0101269630970059	0.634373729986051
U	PC	0.000616799344284796	0.000530598146478068
U	PD	0.000240385302394175	0.00863592585649786
U	TO	1.98232880240046E-33	4.29030343327516E-10

Supplemental Table 5

	All		R1		R2		R3		R4		R5	
Damage Types	r	p-val	r	p-val	r	p-val	r	p-val	r	p-val	r	p-val
AD/AD	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000
AD/TB	0.1226	0.0258	-0.0292	0.9178	0.1591	0.3141	0.1387	0.2521	0.1375	0.1704	0.0792	0.4268
AD/CC	-0.0443	0.4215	-0.1274	0.6509	0.0937	0.5549	0.0778	0.5221	-0.0619	0.5383	-0.2294	0.0198
AD/PC	-0.1621	0.0031	-0.0714	0.8003	-0.2846	0.0677	-0.3252	0.0060	-0.1970	0.0483	-0.0499	0.6163
AD/PD	0.0437	0.4278	0.2857	0.3019	-0.0577	0.7168	-0.0018	0.9882	-0.0064	0.9492	0.0775	0.4366
TB/TB	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000
TB/CC	0.4676	0.0000	0.7802	0.0006	0.6069	0.0000	0.5575	0.0000	0.4405	0.0000	0.3100	0.0014
TB/PC	-0.1527	0.0054	-0.1750	0.5328	0.2901	0.0624	-0.2391	0.0463	-0.2535	0.0105	-0.2411	0.0142
TB/PD	-0.1449	0.0083	-0.1750	0.5328	-0.1614	0.3071	-0.0674	0.5792	-0.2227	0.0252	-0.1925	0.0514
CC/CC	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000
CC/PC	-0.1366	0.0129	-0.2548	0.3594	0.0677	0.6701	-0.3252	0.0060	-0.3775	0.0001	-0.1396	0.1595
CC/PD	0.1203	0.0287	0.1274	0.6509	-0.1658	0.2940	-0.0188	0.8775	-0.1760	0.0783	0.2562	0.0090
PC/PC	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000
PC/PD	0.2889	0.0000	-0.0714	0.8003	0.1332	0.4003	0.1979	0.1005	0.4326	0.0000	0.2292	0.0199
PD/PD	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000	1.0000	0.0000

Acknowledgements

We thank S Baker for veterinary support, and K Chin and M Truong for administrative support. The members of the Brain Interfacing Laboratory are Michelle S Wechsler, Mackenzie Risch, Alexandra Paraskevopoulou, Stephen I Ryu, Alissa S Ling, Elizabeth Jun, Michael P Silvernagel, Yuxin Wu, Kenji Y Marshall, Muhammad Abdulla, and Sydney Hunt. MS Wechsler, A Paraskevopoulou, K Lebedev, and MJ Risch were responsible for animal care and surgical support. SI Ryu was responsible for nonhuman primate array implantation. AS Ling, E Jun, MP Silvernagel, Y Wu, K Marshall, MU Abdulla, and S Hunt assisted in animal care. Part of this work was performed at the Stanford Nano Shared Facilities (SNSF), supported by the National Science Foundation under award ECCS-2026822. A Tor was supported by the Department of Defense (DoD) through the National Defense Science & Engineering Graduate (NDSEG) Fellowship Program and by a training grant from the National Science Foundation (1828993). SE Clarke was supported by a Stanford School of Medicine's Dean's Postdoctoral Fellowship. IE Bray was supported by an American Heart Association Predoctoral Fellowship (828653) and the National Science Foundation GRFP (1656518). This work was supported by a Stanford Human-Centered AI Seed Research Grant to SE Clarke and P Nuyujukian. This work was additionally supported by the following to P Nuyujukian: the National Institutes of Health (R01NS123517, R01NS130789, U19NS118284) and the Stanford Wu Tsai Neurosciences Institute.

Additional information

Author Contributions

A Tor was responsible for data curation, formal analysis, investigation, methodology, software, validation, visualization, writing, and review/editing. SE Clarke was responsible for conceptualization, data curation, supervision, validation, writing, and review/editing. IE Bray was responsible for conceptualization and review/editing. P Nuyujukian was responsible for conceptualization, funding acquisition, methodology, project administration, resources, supervision, writing, and review/editing. The members of the Brain Interfacing Laboratory provided additional support in review/editing.

References

- [1] Cunningham J. P., Yu B. M. (2014) **Dimensionality reduction for large-scale neural recordings** *Nature Neuroscience* **17**:1500–1509 [Google Scholar](#)
- [2] Vyas S., Golub M. D., Sussillo D., Shenoy K. V. (2020) **Computation through neural population dynamics** *Annual Review of Neuroscience* **43**:249–275 [Google Scholar](#)
- [3] Ebitz R. B., Hayden B. Y. (2021) **The population doctrine in cognitive neuroscience** *Neuron* **109**:3055–3068 [Google Scholar](#)
- [4] Maynard E. M., Nordhausen C. T., Normann R. A. (1997) **The utah intracortical electrode array: A recording structure for potential brain-computer interfaces** *Electroencephalography and Clinical Neurophysiology* **102**:228–239 [Google Scholar](#)
- [5] Serruya M. D., Hatsopoulos N. G., Paninski L., Fellows M. R., Donoghue J. P. (2002) **Instant neural control of a movement signal** *Nature* **416**:141–142 [Google Scholar](#)
- [6] Gilja V., Nuyujukian P., Chestek C. A., Cunningham J. P., Yu B. M., Fan J. M., Churchland M. M., Kaufman M. T., Kao J. C., Ryu S. I., Shenoy K. V. (2012) **A high-performance neural prosthesis enabled by control algorithm design** *Nature Neuroscience* **15**:1752–1757 [Google Scholar](#)
- [7] Churchland M. M., Cunningham J. P., Kaufman M. T., Foster J. D., Nuyujukian P., Ryu S. I., Shenoy K. V. (2012) **Neural population dynamics during reaching** *Nature* **487**:51–56 [Google Scholar](#)
- [8] Gallego J. A., Perich M. G., Chowdhury R. H., Solla S. A., Miller L. E. (2020) **Long-term stability of cortical population dynamics underlying consistent behavior** *Nature Neuroscience* **23**:260–270 [Google Scholar](#)
- [9] Gilja V., Pandarinath C., Blabe C. H., Nuyujukian P., Simeral J. D., Sarma A. A., Sorice B. L., Perge J. A., Jarosiewicz B., Hochberg L. R., Shenoy K. V., Henderson J. M. (2015) **Clinical translation of a high-performance neural prosthesis** *Nature Medicine* **21**:1142–1145 [Google Scholar](#)
- [10] Willett F. R., Kunz E. M., Fan C., Avansino D. T., Wilson G. H., Choi E. Y., Kamdar F., Glasser M. F., Hochberg L. R., Druckmann S., Shenoy K. V., Henderson J. M. (2023) **A high-performance speech neuroprosthesis** *Nature* **620**:1031–1036 [Google Scholar](#)
- [11] Roelfsema P. R., Treue S. (2014) **Basic neuroscience research with nonhuman primates: A small but indispensable component of biomedical research** *Neuron* **82**:1200–1204 [Google Scholar](#)
- [12] Mitchell A. S., Thiele A., Petkov C. I., Roberts A., Robbins T. W., Schultz W., Lemon R. (2018) **Continued need for non-human primate neuroscience research** *Current Biology* **28**:R1186–R1187 [Google Scholar](#)

- [13] Tehovnik E. J., Tolias A. S., Sultan F., Slocum W. M., Logothetis N. K. (2006) **Direct and indirect activation of cortical neurons by electrical microstimulation** *Journal of Neurophysiology* **96**:512–521 [Google Scholar](#)
- [14] Kline M. T. (2007) **chapter 169 - radiofrequency techniques** In: Waldman S. D., Bloch J. I., editors. *Pain Management* Philadelphia: W.B. Saunders pp. 1411–1459 [Google Scholar](#)
- [15] Horsley V., Clarke R. H. (1908) **The structure and functions of the cerebellum examined by a new method** *Brain* **31**:45–124 [Google Scholar](#)
- [16] Sweet W. H. (1953) **Unipolar anodal electrolytic lesions in the brain of man and cat: Report of five human cases with electrically produced bulbar or mesencephalic tractotomies** *A.M.A. Archives of Neurology & Psychiatry* **70**:224 [Google Scholar](#)
- [17] Chen Y.-Y., Lai H.-Y., Lin S.-H., Cho C.-W., Chao W.-H., Liao C.-H., Tsang S., Chen Y.-F., Lin S.-Y. (2009) **Design and fabrication of a polyimide-based microelectrode array: Application in neural recording and repeatable electrolytic lesion in rat brain** *Journal of Neuroscience Methods* **182**:6–16 [Google Scholar](#)
- [18] Townsend G., Peloquin P., Kloosterman F., Hetke J. F., Leung L. (2002) **Recording and marking with silicon multichannel electrodes** *Brain Research Protocols* **9**:122–129 [Google Scholar](#)
- [19] Bray I. E., Clarke S. E., Casey K. M., Nuyujukian P. (2024) **Neuroelectrophysiology-compatible electrolytic lesioning** *eLife* **12** [Google Scholar](#)
- [20] Suner S., Fellows M., Vargas-Irwin C., Nakata G., Donoghue J. (2005) **Reliability of signals from a chronically implanted, silicon-based electrode array in non-human primate primary motor cortex** *IEEE Transactions on Neural Systems and Rehabilitation Engineering* **13**:524–541 [Google Scholar](#)
- [21] Simeral J. D., Kim S.-P., Black M. J., Donoghue J. P., Hochberg L. R. (2011) **Neural control of cursor trajectory and click by a human with tetraplegia 1000 days after implant of an intracortical microelectrode array** *Journal of Neural Engineering* **8**:025027 [Google Scholar](#)
- [22] Downey J. E., Schwed N., Chase S. M., Schwartz A. B., Collinger J. L. (2018) **Intracortical recording stability in human brain-computer interface users** *Journal of Neural Engineering* **15**:046016 [Google Scholar](#)
- [23] Chestek C. A., Gilja V., Nuyujukian P., Foster J. D., Fan J. M., Kaufman M. T., Churchland M. M., Rivera-Alvidrez Z., Cunningham J. P., Ryu S. I., Shenoy K. V. (2011) **Long-term stability of neural prosthetic control signals from silicon cortical arrays in rhesus macaque motor cortex** *Journal of Neural Engineering* **8**:045005 [Google Scholar](#)
- [24] Chen X., Wang F., Kooijmans R., Klink P. C., Boehler C., Asplund M., Roelfsema P. R. (2023) **Chronic stability of a neuroprosthesis comprising multiple adjacent Utah arrays in monkeys** *Journal of Neural Engineering* **20**:036039 [Google Scholar](#)
- [25] Bjånes D. A., Kellis S., Nickl R., Baker B., Aflalo T., Bashford L., Chivukula S., Fifer M. S., Osborn L. E., Christie B., Wester B. A., Celnik P. A., Kramer D., Pejisa K., Crone N. E., Anderson W. S., Pouratian N., Lee B., Liu C. Y., Tenore F., Rieth L., Andersen R. A. (2024) **Quantifying physical degradation alongside recording and stimulation performance of 980 intracortical**

microelectrodes chronically implanted in three humans for 956-2246 days *medRxiv*
[Google Scholar](#)

- [26] Patel P. R., Welle E. J., Letner J. G., Shen H., Bullard A. J., Caldwell C. M., Vega-Medina A., Richie J. M., Thayer H. E., Patil P. G., Cai D., Chestek C. A. (2023) **Utah array characterization and histological analysis of a multi-year implant in non-human primate motor and sensory cortices** *Journal of Neural Engineering* **20**:014001 [Google Scholar](#)
- [27] Barrese J. C., Aceros J., Donoghue J. P. (2016) **Scanning electron microscopy of chronically implanted intracortical microelectrode arrays in non-human primates** *Journal of Neural Engineering* **13**:026003 [Google Scholar](#)
- [28] Woeppel K., Hughes C., Herrera A. J., Eles J. R., Tyler-Kabara E. C., Gaunt R. A., Collinger J. L., Cui X. T. (2021) **Explant analysis of utah electrode arrays implanted in human cortex for brain-computer-interfaces** *Frontiers in Bioengineering and Biotechnology* **9** [Google Scholar](#)
- [29] Yi D., Yao Y., Wang Y., Chen L. (2022) **Manufacturing processes of implantable microelectrode array for in vivo neural electrophysiological recordings and stimulation: A state-of-the-art review** *Journal of Micro- and Nano-Manufacturing* **10** [Google Scholar](#)
- [30] Campbell P., Jones K., Huber R., Horch K., Normann R. (1991) **A silicon-based, three-dimensional neural interface: manufacturing processes for an intracortical electrode array** *IEEE Transactions on Biomedical Engineering* **38**:758–768 [Google Scholar](#)
- [31] Bhandari R., Negi S., Solzbacher F. (2010) **Wafer-scale fabrication of penetrating neural microelectrode arrays** *Biomedical Microdevices* **12**:797–807 [Google Scholar](#)
- [32] Caldwell R., Street M. G., Sharma R., Takmakov P., Baker B., Rieth L. (2020) **Characterization of parylene-c degradation mechanisms: In vitro reactive accelerated aging model compared to multiyear in vivo implantation** *Biomaterials* **232**:119731 [Google Scholar](#)
- [33] Polikov V. S., Tresco P. A., Reichert W. M. (2005) **Response of brain tissue to chronically implanted neural electrodes** *Journal of Neuroscience Methods* **148**:1–18 [Google Scholar](#)
- [34] Salatino J. W., Ludwig K. A., Kozai T. D. Y., Purcell E. K. (2017) **Glial responses to implanted electrodes in the brain** *Nature Biomedical Engineering* **1**:862–877 [Google Scholar](#)
- [35] Biran R., Martin D. C., Tresco P. A. (2007) **The brain tissue response to implanted silicon microelectrode arrays is increased when the device is tethered to the skull** *Journal of Biomedical Materials Research Part A* **82A**:169–178 [Google Scholar](#)
- [36] Potter K. A., Buck A. C., Self W. K., Capadona J. R. (2012) **Stab injury and device implantation within the brain results in inversely multiphasic neuroinflammatory and neurodegenerative responses** *Journal of Neural Engineering* **9**:046020 [Google Scholar](#)
- [37] Shepherd R. K., Carter P. M., Dalrymple A. N., Enke Y. L., Wise A. K., Nguyen T., Firth J., Thompson A., Fallon J. B. (2021) **Platinum dissolution and tissue response following long-term electrical stimulation at high charge densities** *Journal of Neural Engineering* **18**:036021 [Google Scholar](#)

- [38] Shah D. D., Carter P., Shivdasani M. N., Fong N., Duan W., Esrafilzadeh D., Poole-Warren L. A., Robles U. A. Aregueta (2024) **Deciphering platinum dissolution in neural stimulation electrodes: Electrochemistry or biology?** *Biomaterials* **309**:122575 [Google Scholar](#)
- [39] Cogan S., Plante T., Ehrlich J. (2004) **Sputtered iridium oxide films (sirofs) for low-impedance neural stimulation and recording electrodes** In: *The 26th Annual International Conference of the IEEE Engineering in Medicine and Biology Society* IEEE pp. 4153–4156 [Google Scholar](#)
- [40] Negi S., Bhandari R., Van Wagenen R., Solzbacher F. (2010) **Factors affecting degradation of sputtered iridium oxide used for neuroprosthetic applications** In: *2010 IEEE 23rd International Conference on Micro Electro Mechanical Systems (MEMS)* IEEE pp. 568–571 [Google Scholar](#)

Author information

Alice Tor

Electrical Engineering Department, Stanford University, Stanford, United States
ORCID iD: [0009-0008-7688-2018](#)

Stephen E Clarke

Bioengineering Department, Stanford University, Stanford, United States, Neurosurgery Department, Stanford University, Stanford, United States
ORCID iD: [0000-0002-3871-0185](#)

Iliana E Bray

Electrical Engineering Department, Stanford University, Stanford, United States
ORCID iD: [0000-0002-3029-8309](#)

Paul Nuyujukian

Bioengineering Department, Stanford University, Stanford, United States, Neurosurgery Department, Stanford University, Stanford, United States, Electrical Engineering Department, Stanford University, Stanford, United States, Wu Tsai Neurosciences Institute, Stanford University, Stanford, United States, Stanford Bio-X, Stanford University, Stanford, United States
ORCID iD: [0000-0001-7778-5473](#)

For correspondence: 25elife@pn.stanford.edu

the Brain Interfacing Laboratory

Editors

Reviewing Editor

Xiaomo Chen

University of California, Davis, Davis, United States of America

Senior Editor

Timothy Behrens

University of Oxford, Oxford, United Kingdom

Reviewer #1 (Public review):

Summary:

This work presents a GUI with SEM images of 8 Utah arrays (8 of which were explanted, and 4 of which were used for creating cortical lesions).

Strengths:

Visual comparison of electrode tips with SEM images, showing that electrolytic lesioning did not appear to cause extra damage to electrodes.

Weaknesses:

Given that the analysis was conducted on explanted arrays, and no functional or behavioural *in vivo* data or histological data are provided, any damage to the arrays may have occurred after explantation. This makes the results limited and inconclusive (firstly, that there was no significant relationship between degree of electrode damage and use of electrolytic lesioning, and secondly, that electrodes closer to the edge of the arrays showed more damage than those in the center).

Overall, these results do not add new insight to the field, although they do add more data and reference images.

<https://doi.org/10.7554/eLife.106452.1.sa1>

Reviewer #2 (Public review):

In this study, the authors used scanning electron microscopy (SEM) to image and analyze eleven Utah multielectrode arrays (including eight chronically implanted in four macaques). Four of the eight arrays had previously been used to deliver electrolytic lesions. Each intact electrode was scored in five damage categories. They found that damage disproportionately occurred to the outer edges of arrays. Importantly, the authors conclude that their electrolytic Lesioning protocol does not significantly increase material degradation compared to normal chronic use without lesion. Additionally, the authors have released a substantial public dataset of single-electrode SEM images of explanted Utah arrays.

The paper is well-written and addresses an important stability issue for long-term chronically implanted array recordings and electrolytic lesioning, which is relevant to both basic science and translational research. By comparing lesioning and non-lesioning electrodes on the same array and within the same animal, the study effectively controls for confounds related to the animal and surgical procedures. The shared dataset, accessible via interactive plots, enhances transparency and serves as a valuable reference for future investigations. Below, we outline some major and minor concerns that could help improve the work.

Major concerns:

(1) Electrode impedance is a critical measurement to evaluate the performance of recording electrodes. It would be helpful if the authors could provide pre-explant and post-explant impedance values for each electrode alongside the five SEM damage scores. This would allow the readers to assess how well the morphological scores align with functional degradation.

(2) The lesion parameters differ across experiments and electrodes. It would be helpful if the authors could evaluate whether damage scores (and/or impedance changes) correlate with total charge, current amplitude, duration, or frequency.

