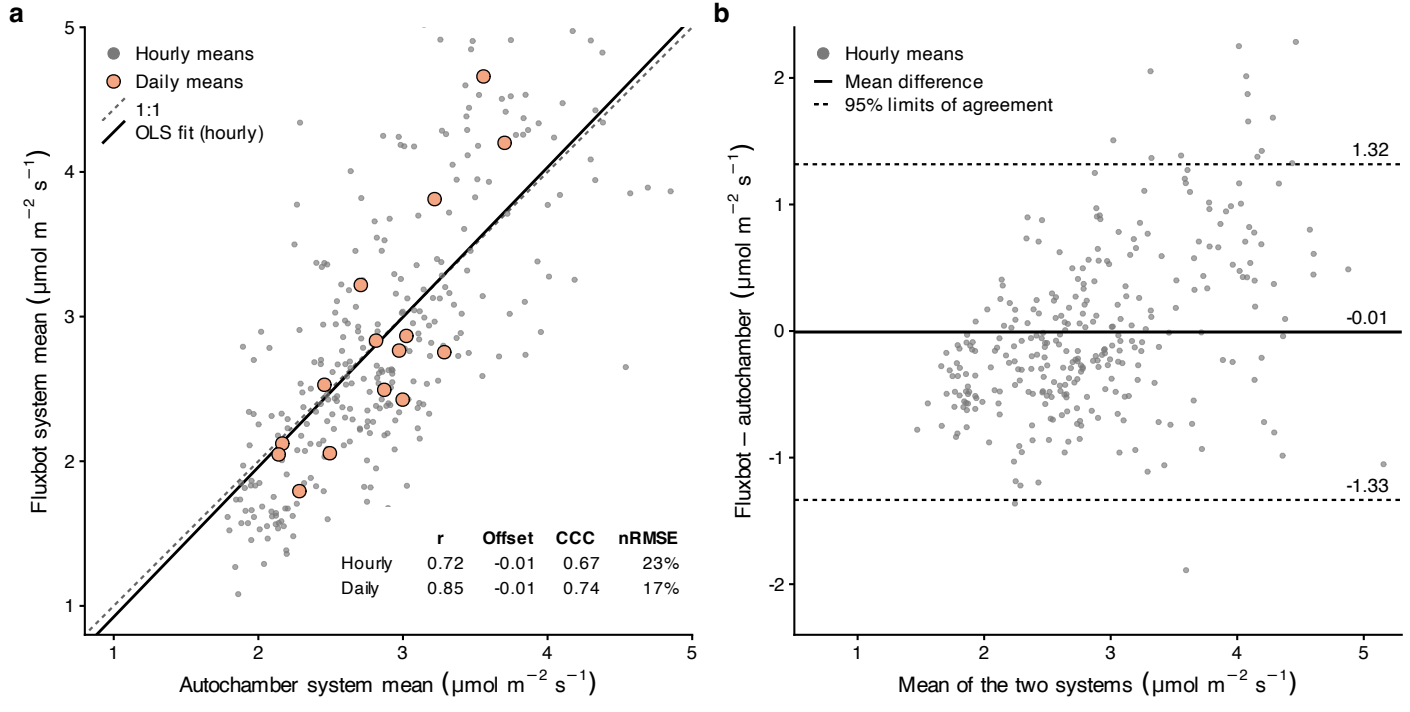

a
Hourly means
Daily means
1:1
OLS fit (hourly)
Fluxbot system mean (µmol m−2 s−1)
Autochamber system mean (µmol m−2 s−1)
r Offset CCC nRMSE
Hourly 0.72 -0.01 0.67 23%
Daily 0.85 -0.01 0.74 17%
b
Hourly means
Mean difference
95% limits of agreement
1.32
-0.01
-1.33
Fluxbot − autochamber (µmol m−2 s−1)
Mean of the two systems (µmol m−2 s−1)