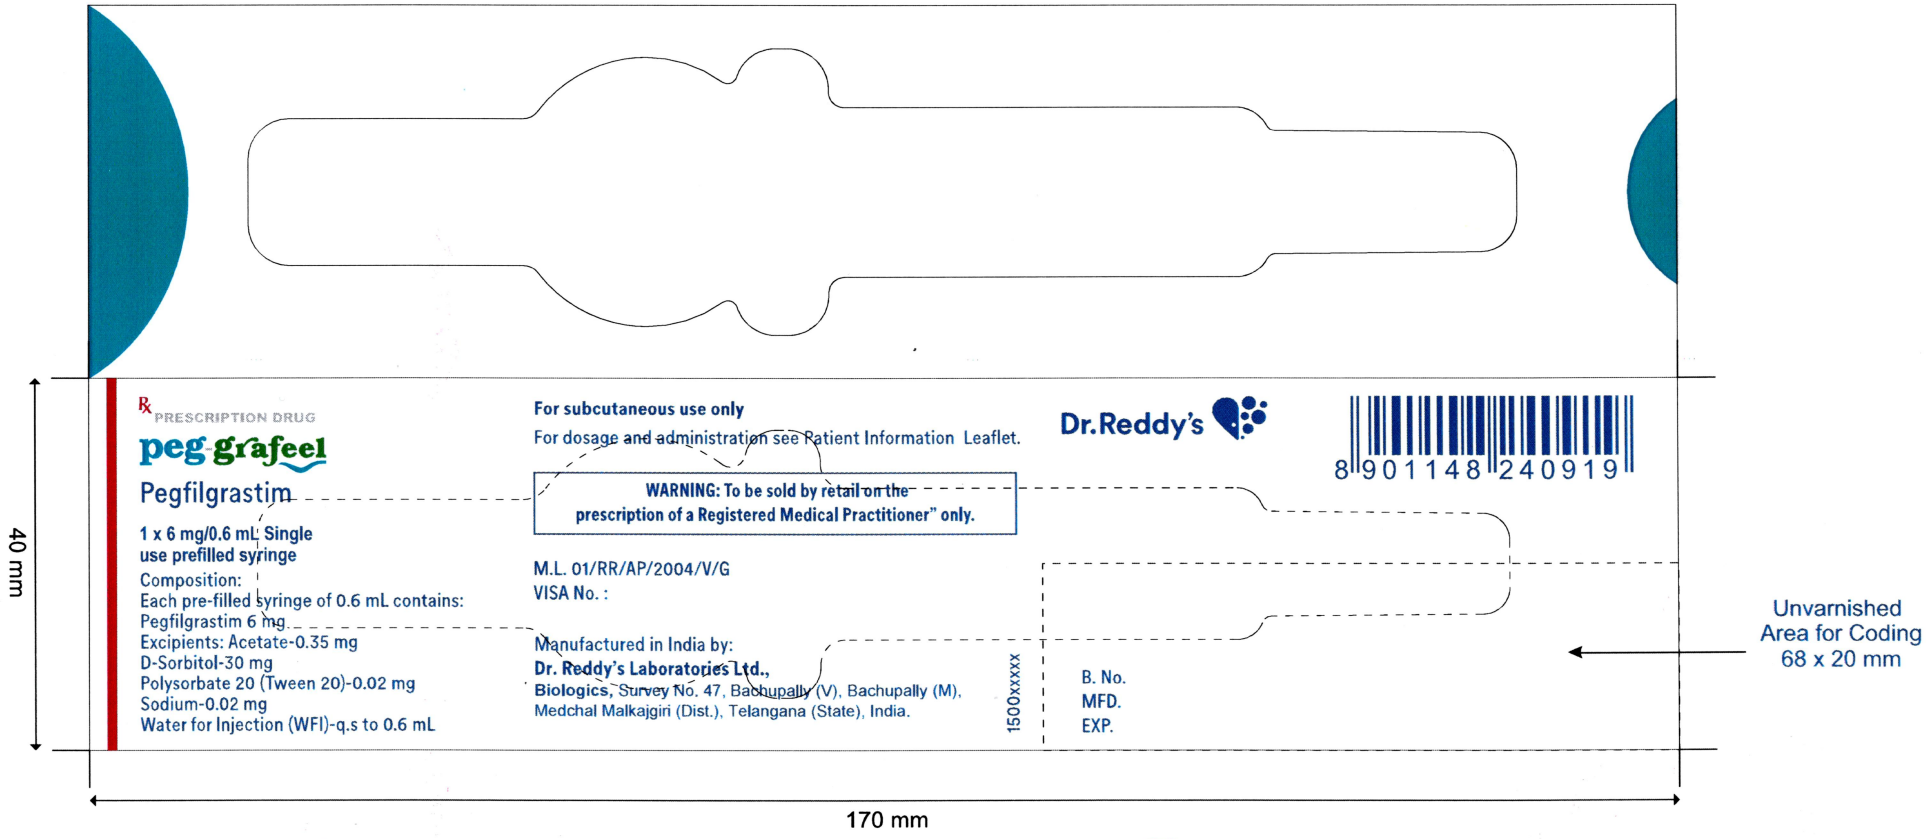


DR. REDDY'S LABORATORIES LIMITED
VĂN PHÒNG ĐẠI DIỆN TẠI THÀNH PHỐ HỒ CHÍ MINH

Dimensions: L x W (170-40 mm)

Composition:
Each pre-filled syringe of 0.6mL contains:
Pegfilgrastim 6 mg
Excipients: Acetate-0.35 mg,
D-Sorbitol-30 mg
Polysorbate 20 (Tween20)-0.02 mg
Sodium-0.02 mg,
Water for Injection(WFI)-q.s to 0.6 mL

For subcutaneous use only
Do not shake.
Keep the syringe in the carton, in order to protect from light.
For dosage and administration see Patient Information Leaflet.

Rx Thuốc kê đơn
PEG-GRAFEEL
Để xa tầm tay trẻ em
Đọc kỹ hướng dẫn sử dụng trước khi dùng
Thành phần: Mỗi bơm tiêm đóng sẵn chứa 6,0 mg pegfilgrastim trong 0,6 ml dung dịch tiêm.

Dạng bào chế: Dung dịch tiêm
Đường dùng: Tiêm dưới da
Đóng gói: Hộp x 1 bơm tiêm đóng sẵn thuốc 0,6 ml
Chỉ định, cách dùng, chống chỉ định và các thông tin khác: xem trong tờ hướng dẫn sử dụng thuốc kèm theo.
Số lô SX, NSX, Hạn dùng xem
B. No., MFD., EXP. trên vỏ hộp và bơm tiêm.

Số đăng ký:
Điều kiện bảo quản: Bảo quản 2-8°C, không đông lạnh, tránh ánh sáng.
Tiêu chuẩn chất lượng: Tiêu chuẩn cơ sở
Xuất xứ: Ấn Độ
Nhà nhập khẩu:

Dr.Reddy's

℞ PRESCRIPTION DRUG

peg grafeel

Pegfilgrastim

1 x 6 mg/0.6 mL Single use prefilled syringe

6 mg/0.6 mL

℞ PRESCRIPTION DRUG peg grafeel Pegfilgrastim

150XXXXXX

Manufactured in India by / Sản xuất tại Ấn Độ bởi:
Dr. Reddy's Laboratories Ltd.,
Biologics, Survey No. 47, Bachupally (V), Bachupally (M), Medchal Malkajgiri (Dist.), Telangana (State), India.

WARNING: To be sold by retail on the prescription of a "Registered Medical Practitioner" only.

M.L. 01/RR/AP/2004/V/G

8 901148 231740

B. No.
MFD.
EXP.
(21)

This is a variable data 2D Barcode, Which is specific to each pack and will be over coded at the time of packing operation. (This 2D barcode symbol is for reference only)

Un Varnished Area for Coding (75 x 20 mm)


Computer Generated Serial No. / Random No and will be over coded at the time of packingoperation.

Fusion Screen

peg-grafeel

GTIN (01) 18901148196442


Instructions for use:




1. Remove the needle shield by pulling it straight off the syringe.



2. Inject using the usual technique. Push the plunger to the bottom of the syringe body.




3. Remove the syringe from the injection site, keeping your Finger on the plunger rod.




4a. Then with the same hand, activate the Preventis sleeve orientating it downwards and away from yourself and others, by firmly pushing the plunger rod.




4b. The protective sleeve will automatically cover the needle. An audible "click" indicates that the system has been properly activated.




5. Immediately dispose off the syringe using a suitable container.



DR. REDDY'S LABORATORIES LIMITED
VĂN PHÒNG ĐẠI DIỆN TẠI THÀNH PHỐ HỒ CHÍ MINH

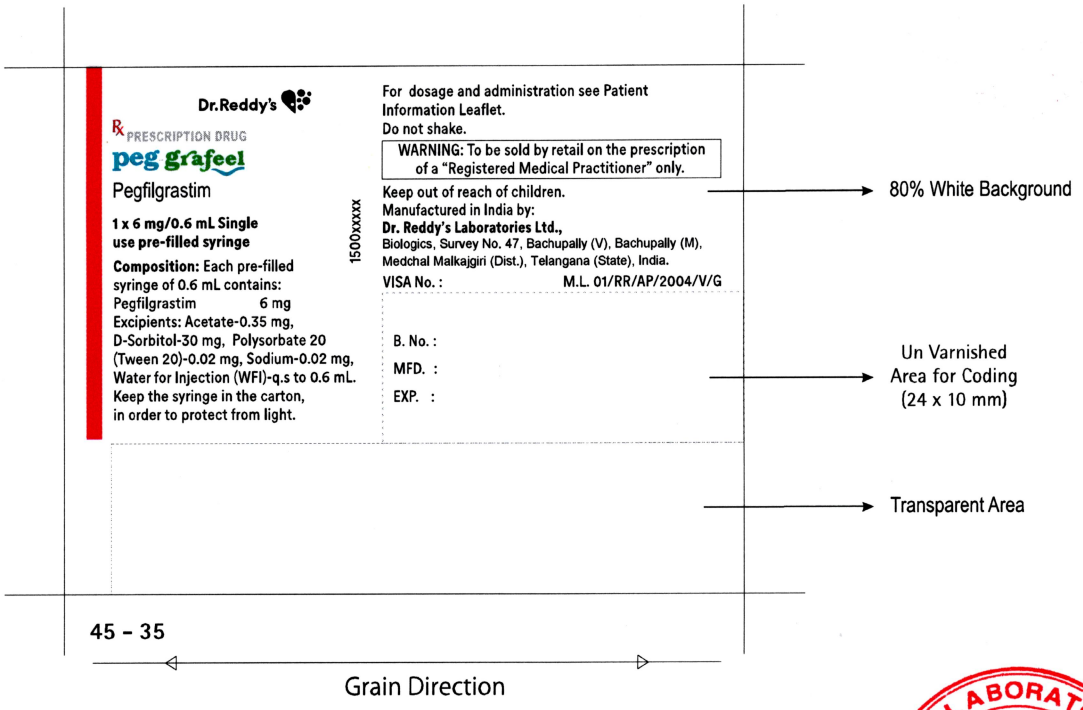

200% Actual Size

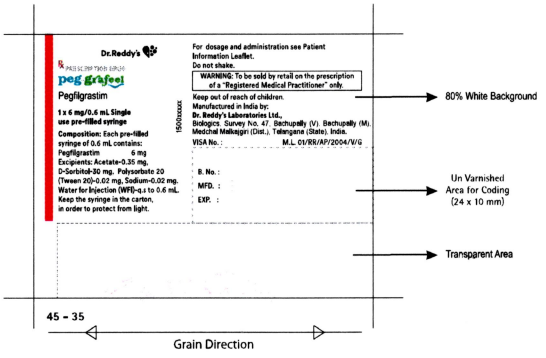

100% Actual Size

DR. REDDY'S LABORATORIES LIMITED
VĂN PHÒNG ĐẠI DIỆN TẠI THÀNH PHỐ HỒ CHÍ MINH