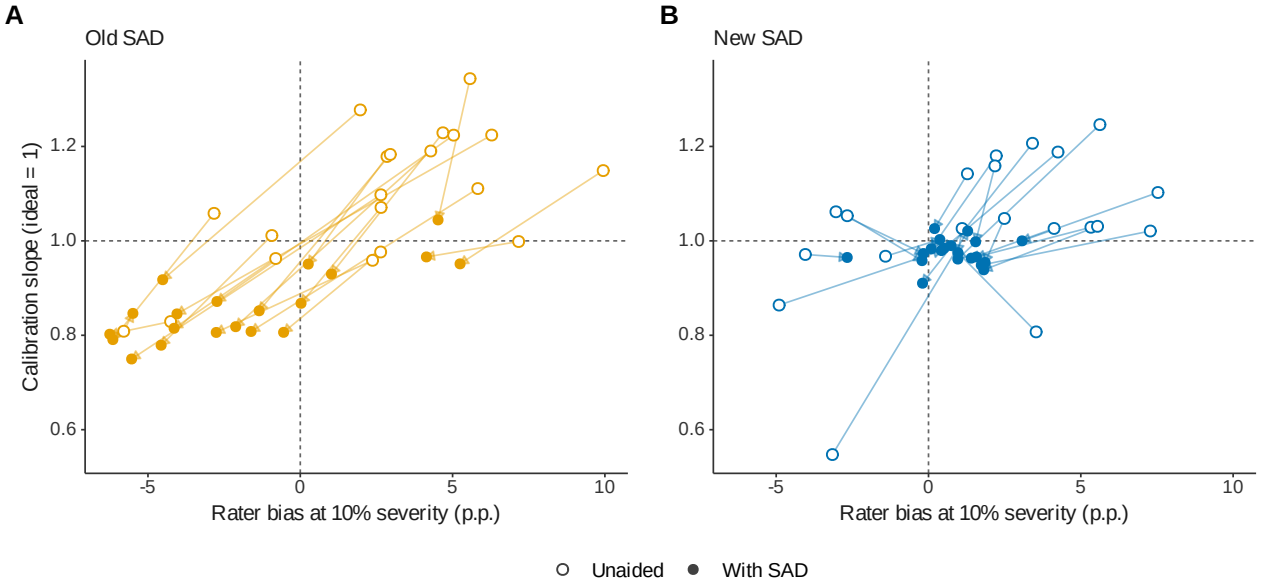
A
Old SAD
B
New SAD
Calibration slope (ideal = 1)
1.2
1.0
0.8
0.6
-5
0
5
10
Rater bias at 10% severity (p.p.)
Unaided
With SAD