


A

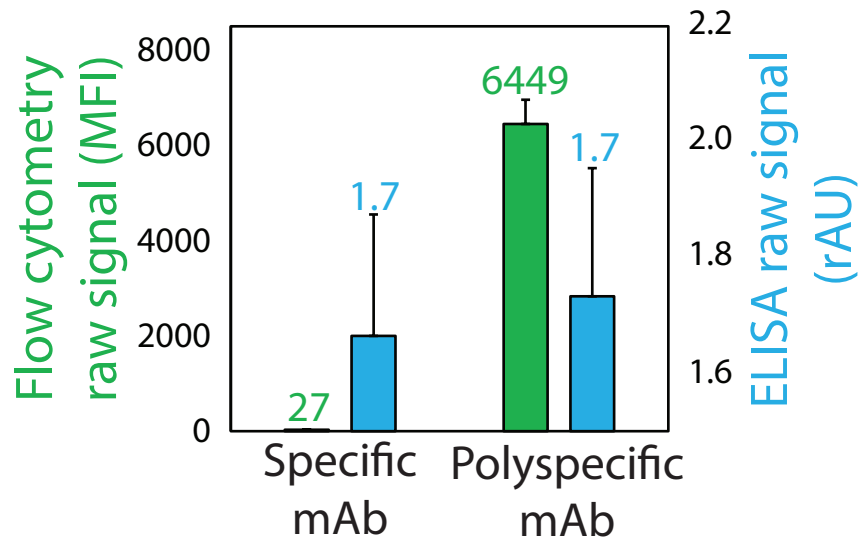

B

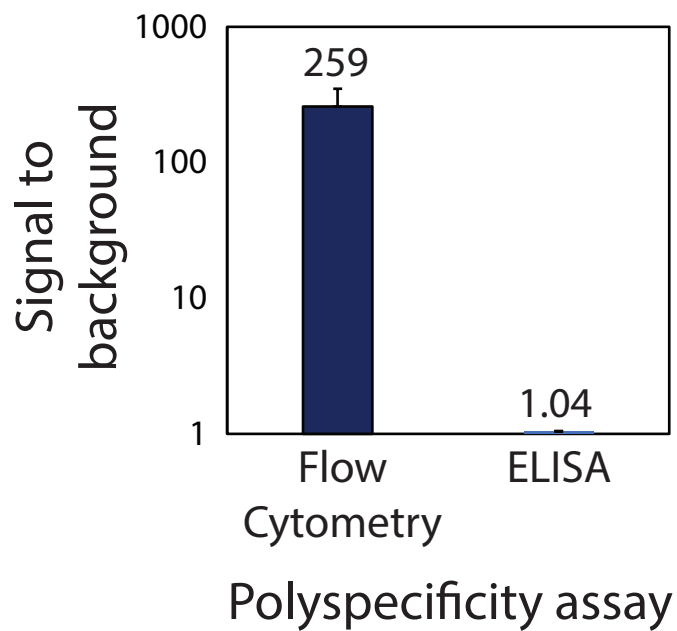


Figure 6. Validation of flow cytometry methodology. (A) Comparison of raw signals for the high and low specificity control mAbs demonstrates the sensitivity and reproducibility of flow cytometry methodology. (B) Signal to background ratios were much higher for the flow-based assay than the plate-based assay.