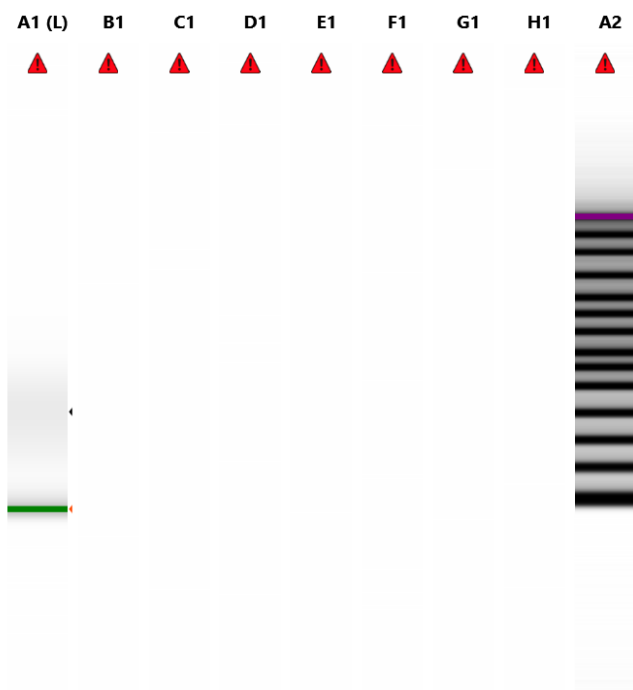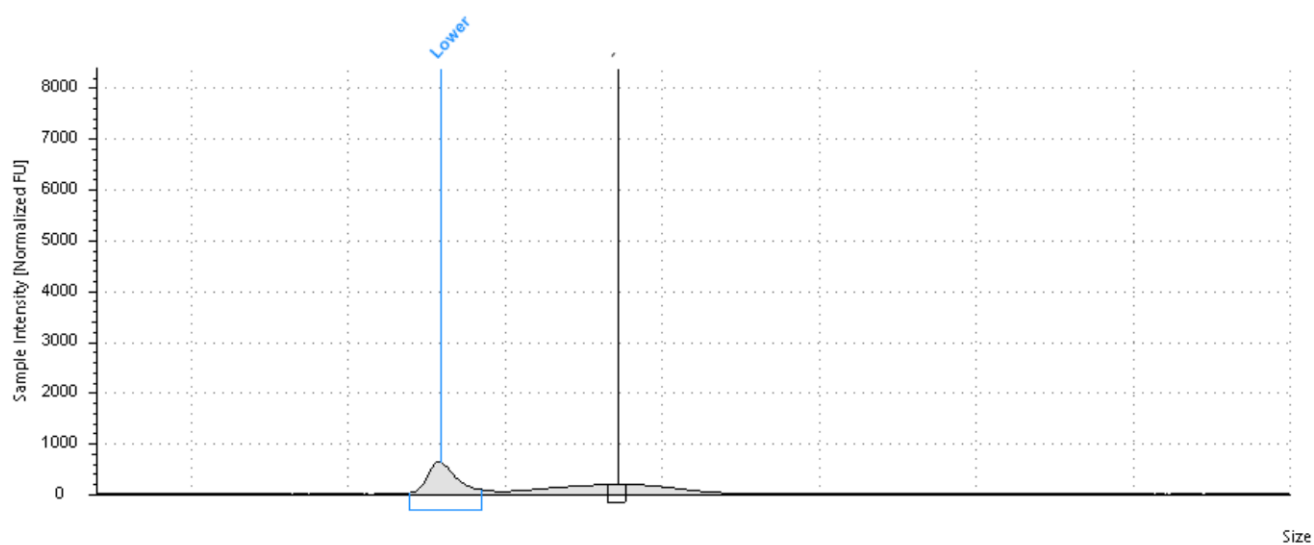## Filename: 2021-03-31 - 16.11.33.D5000

Default image (Contrast 100%)

Sample Info

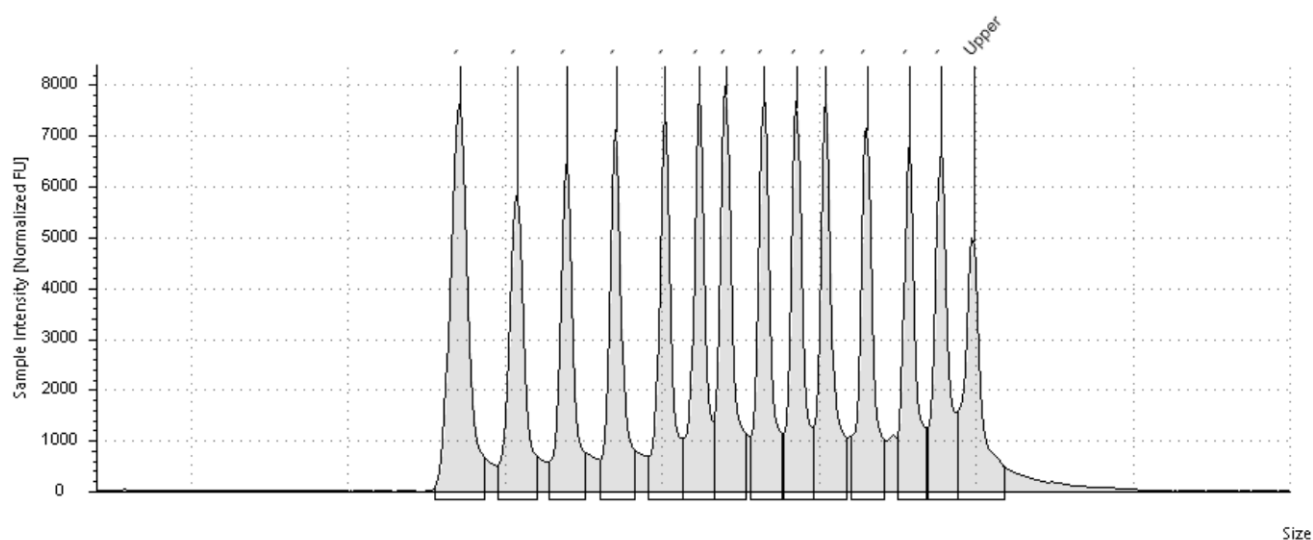| Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A1		Ladder	⚠	Issue with ladder peak detection (too few peaks detected); Marker(s) not detected; Caution! Expired ScreenTape device; Ladder
B1		1	⚠	Marker(s) not detected; Caution! Expired ScreenTape device
C1		2	⚠	Marker(s) not detected; Caution! Expired ScreenTape device
D1		3	⚠	Marker(s) not detected; Caution! Expired ScreenTape device
E1		4	⚠	Marker(s) not detected; Caution! Expired ScreenTape device
F1		5	⚠	Marker(s) not detected; Caution! Expired ScreenTape device
G1		6	⚠	Marker(s) not detected; Caution! Expired ScreenTape device
H1		7	⚠	Marker(s) not detected; Caution! Expired ScreenTape device
A2	106	8	⚠	Marker(s) not detected; Caution! Expired ScreenTape device

A1: Ladder

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A1		Ladder	⚠	Issue with ladder peak detection (too few peaks detected); Marker(s) not detected; Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
-	-	-	-	-		Lower Marker
-	-	-	-	100.00		

A2: 8

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A2	106	8	⚠	Marker(s) not detected; Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
-	12.0	-	-	11.37		
-	7.54	-	-	7.12		
-	7.59	-	-	7.17		
-	7.76	-	-	7.33		
-	7.84	-	-	7.40		
-	8.22	-	-	7.76		
-	8.52	-	-	8.04		
-	8.16	-	-	7.70		
-	7.88	-	-	7.44		
-	8.21	-	-	7.75		
-	7.62	-	-	7.19		
-	7.00	-	-	6.60		
-	7.56	-	-	7.13		
-	3.25	3.25	-	-		Upper Marker