



Filename: 2021-07-14 - 15.53.47.D5000

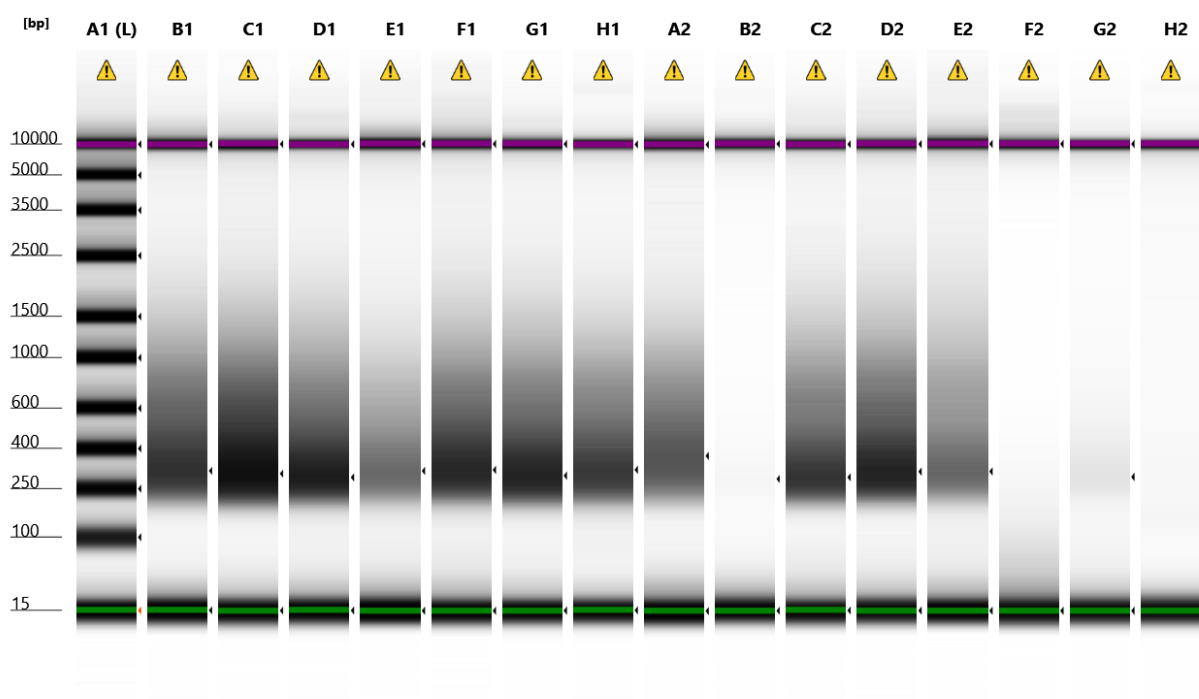

Default image (Contrast 100%)

Sample Info


Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	52.5	Ladder	⚠	Caution! Expired ScreenTape device; Ladder
B1	12.9	59	⚠	Caution! Expired ScreenTape device
C1	20.9	60	⚠	Caution! Expired ScreenTape device
D1	16.5	61	⚠	Caution! Expired ScreenTape device
E1	6.87	62	⚠	Caution! Expired ScreenTape device
F1	14.9	63	⚠	Caution! Expired ScreenTape device
G1	14.6	64	⚠	Caution! Expired ScreenTape device
H1	13.7	65	⚠	Caution! Expired ScreenTape device
A2	13.1	66	⚠	Caution! Expired ScreenTape device
B2	0.0480	67	⚠	Caution! Expired ScreenTape device
C2	12.7	68	⚠	Caution! Expired ScreenTape device
D2	15.5	69	⚠	Caution! Expired ScreenTape device
E2	7.83	70	⚠	Caution! Expired ScreenTape device
F2		71	⚠	Caution! Expired ScreenTape device
G2	0.478	72	⚠	Caution! Expired ScreenTape device
H2	0.117	73	⚠	Caution! Expired ScreenTape device; Peak out of Sizing Range

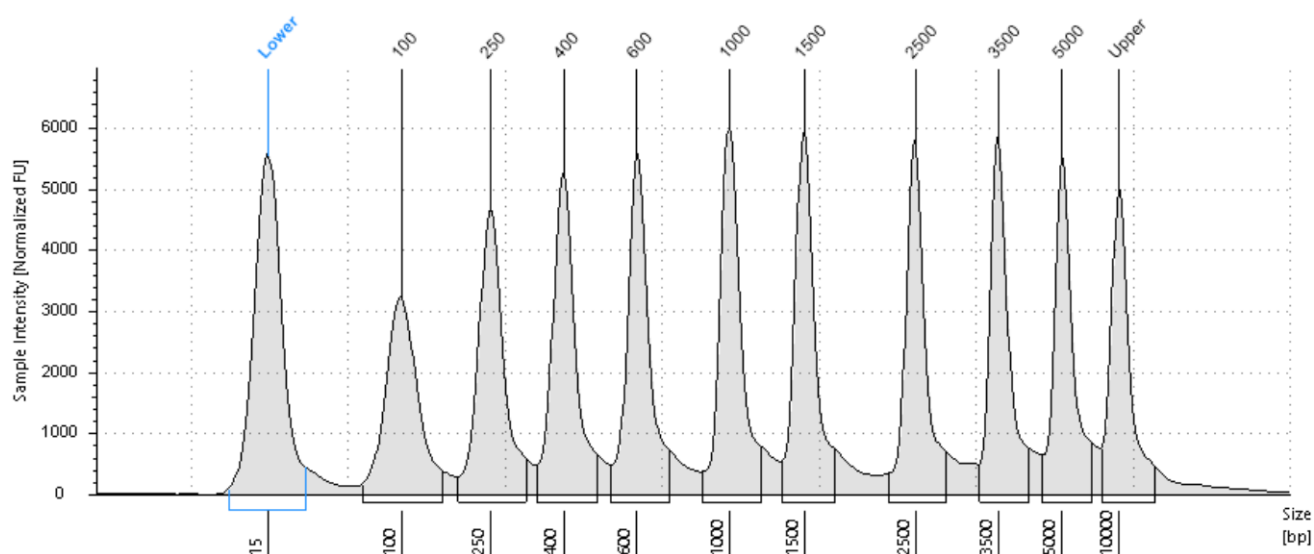A1: Ladder**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	52.5	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.96	-	713	-		Lower Marker
100	5.30	-	81.5	10.09		
250	5.96	-	36.7	11.36		
400	6.17	-	23.7	11.75		
600	6.13	-	15.7	11.68		
1000	6.30	-	9.69	12.01		
1500	6.01	-	6.16	11.45		
2500	5.71	-	3.51	10.87		
3500	5.56	-	2.44	10.59		
5000	5.35	-	1.65	10.19		
10000	3.25	3.25	0.500	-		Upper Marker

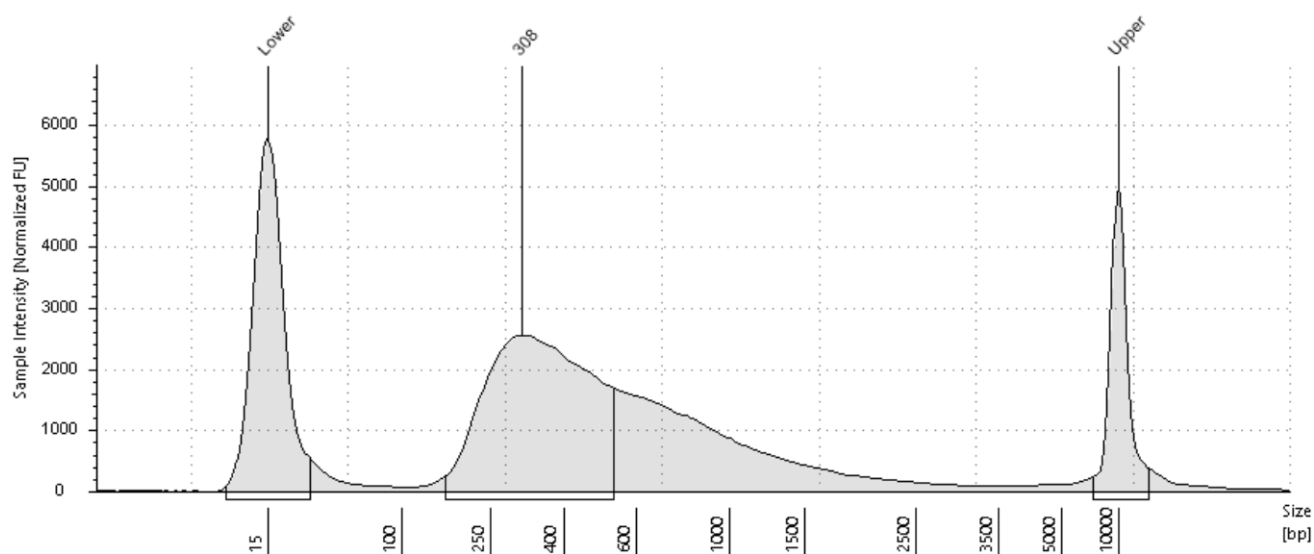
B1: 59**Sample Table**

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
B1	12.9	59	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.34	-	753	-		Lower Marker
308	12.9	-	64.2	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

C1: 60

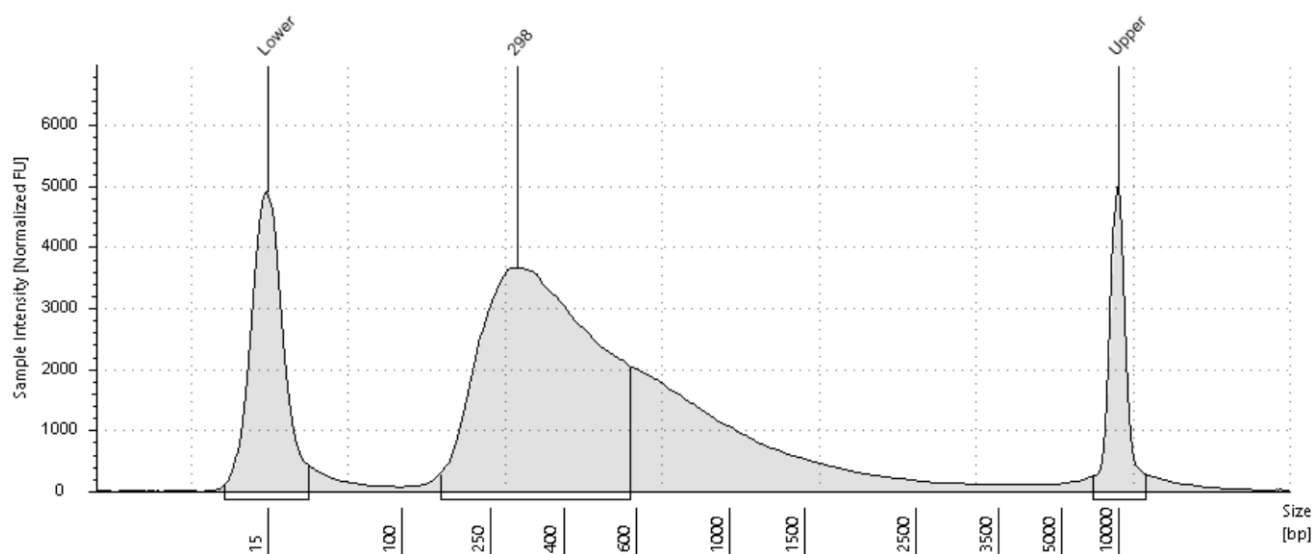


Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
C1	20.9	60		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.71	-	688	-		Lower Marker
298	20.9	-	108	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

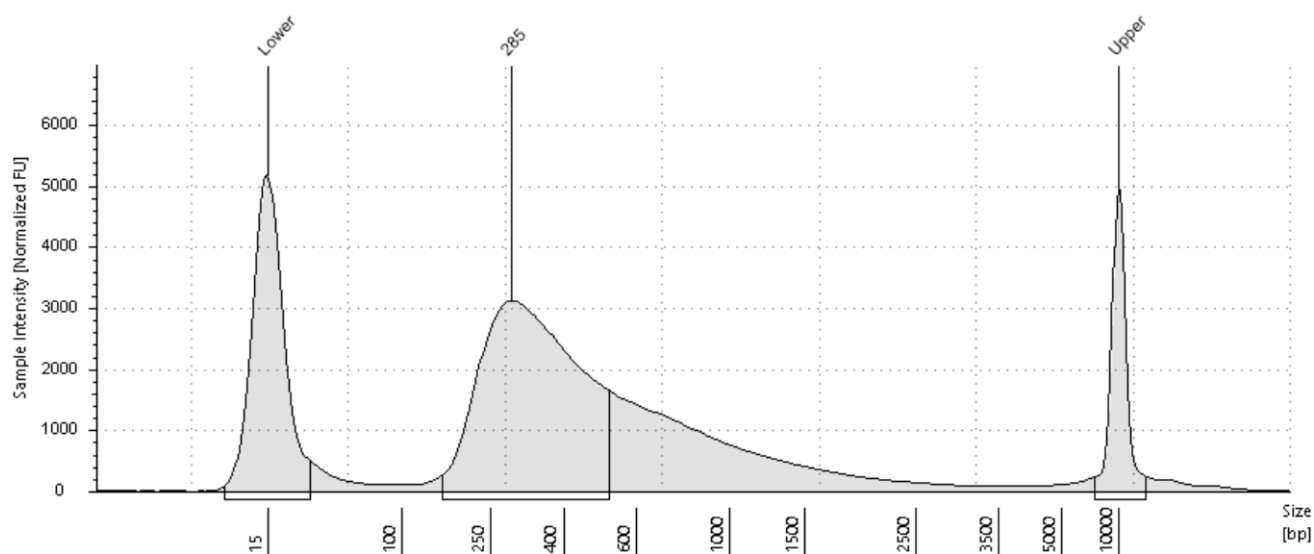
D1: 61**Sample Table**

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
D1	16.5	61		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.49	-	768	-		Lower Marker
285	16.5	-	88.7	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

E1: 62

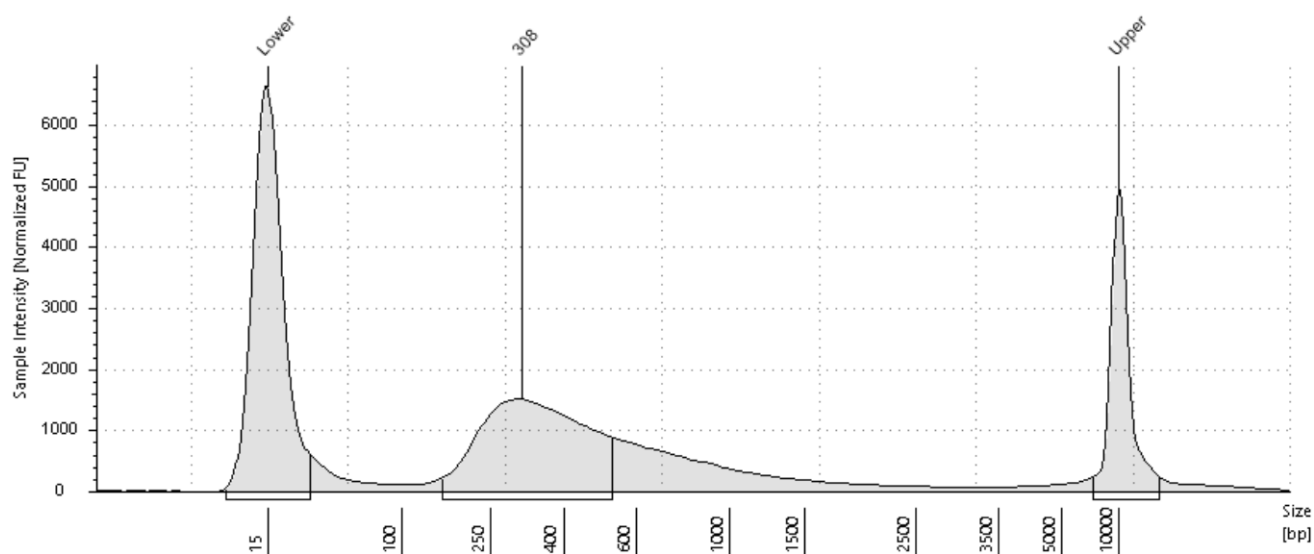


Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
E1	6.87	62	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.57	-	776	-		Lower Marker
308	6.87	-	34.3	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

F1: 63

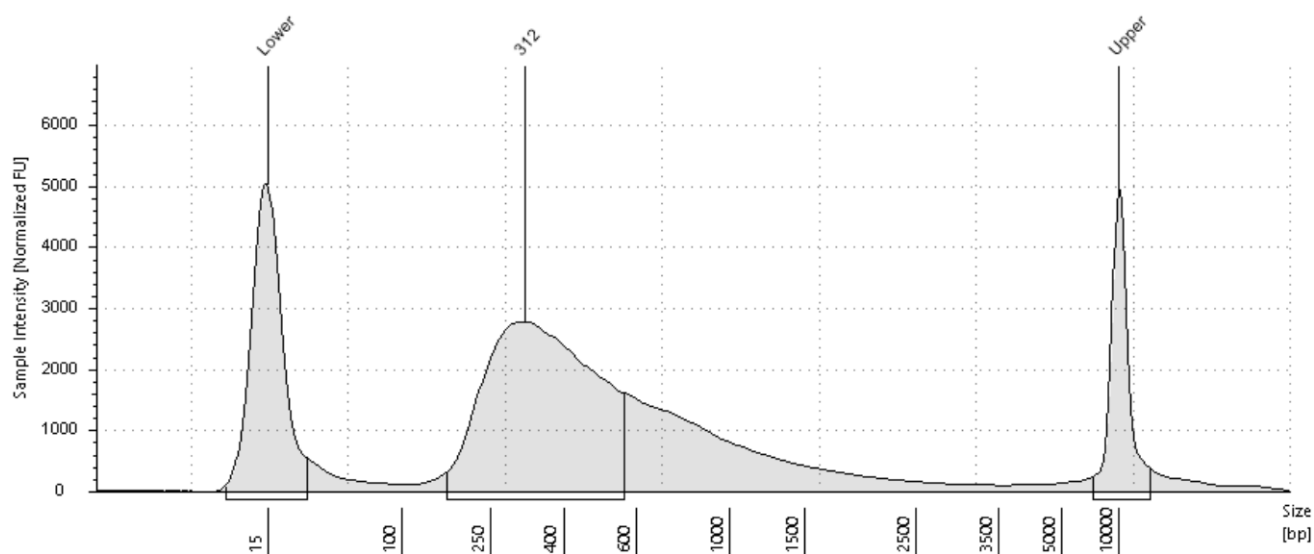


Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
F1	14.9	63		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.43	-	659	-		Lower Marker
312	14.9	-	73.5	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

G1: 64

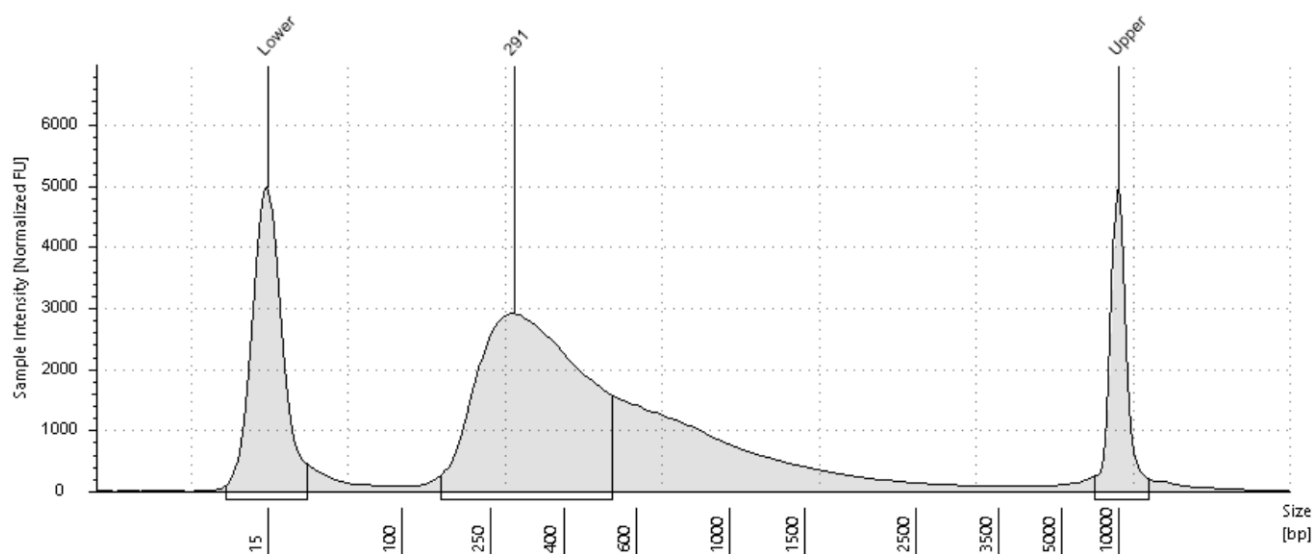


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
G1	14.6	64	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.23	-	639	-		Lower Marker
291	14.6	-	77.1	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

H1: 65

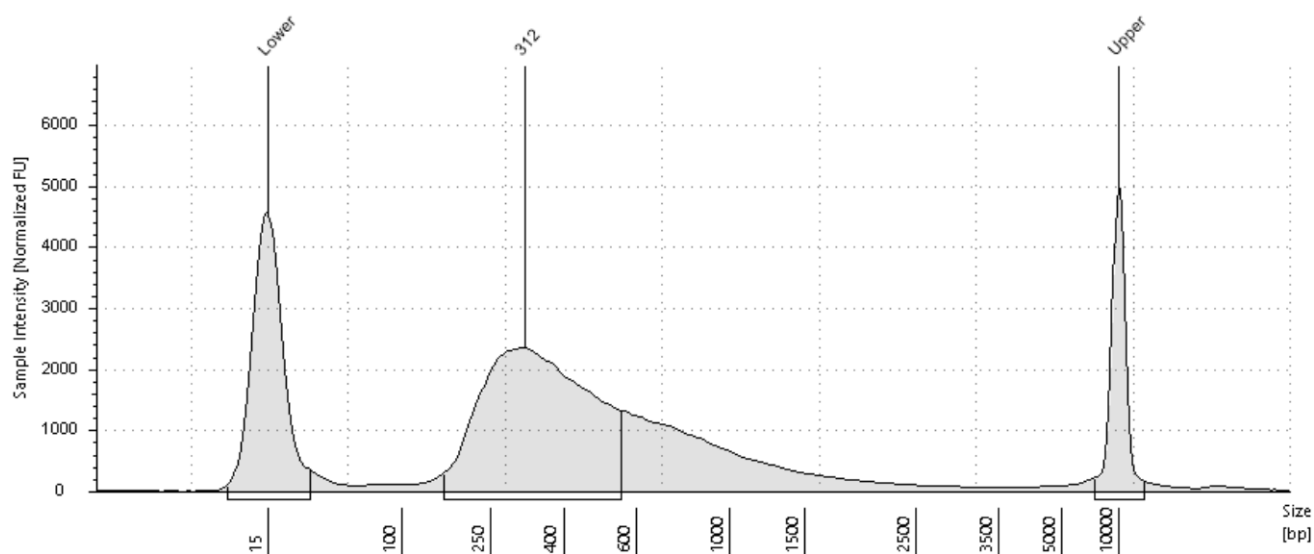


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
H1	13.7	65	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.51	-	668	-		Lower Marker
312	13.7	-	67.4	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

A2: 66

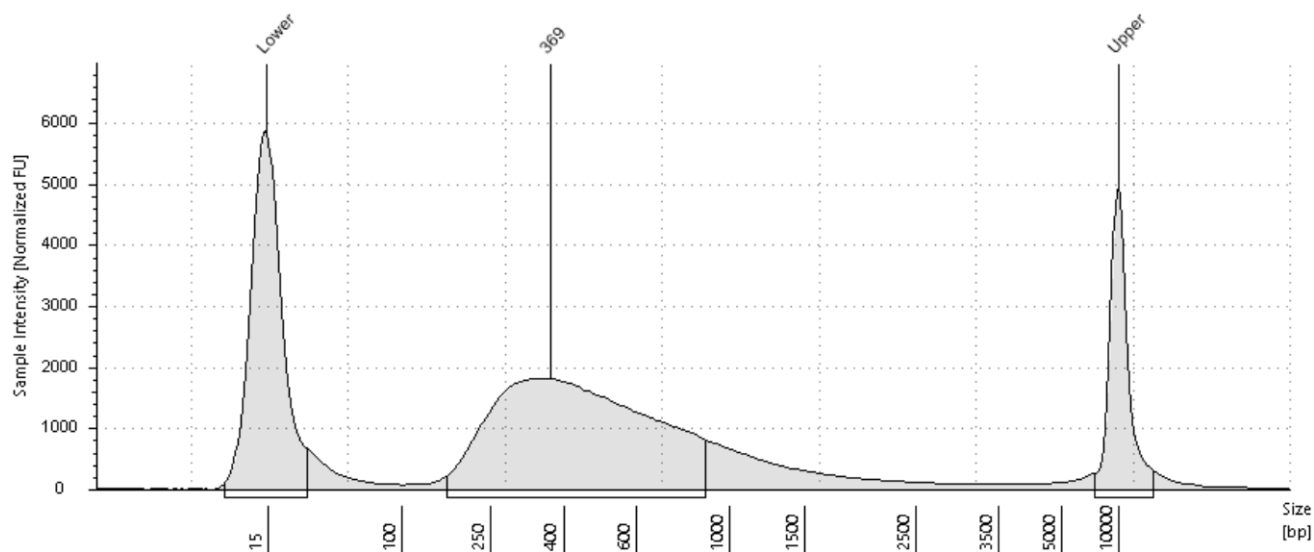


Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
A2	13.1	66	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.91	-	709	-		Lower Marker
369	13.1	-	54.5	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

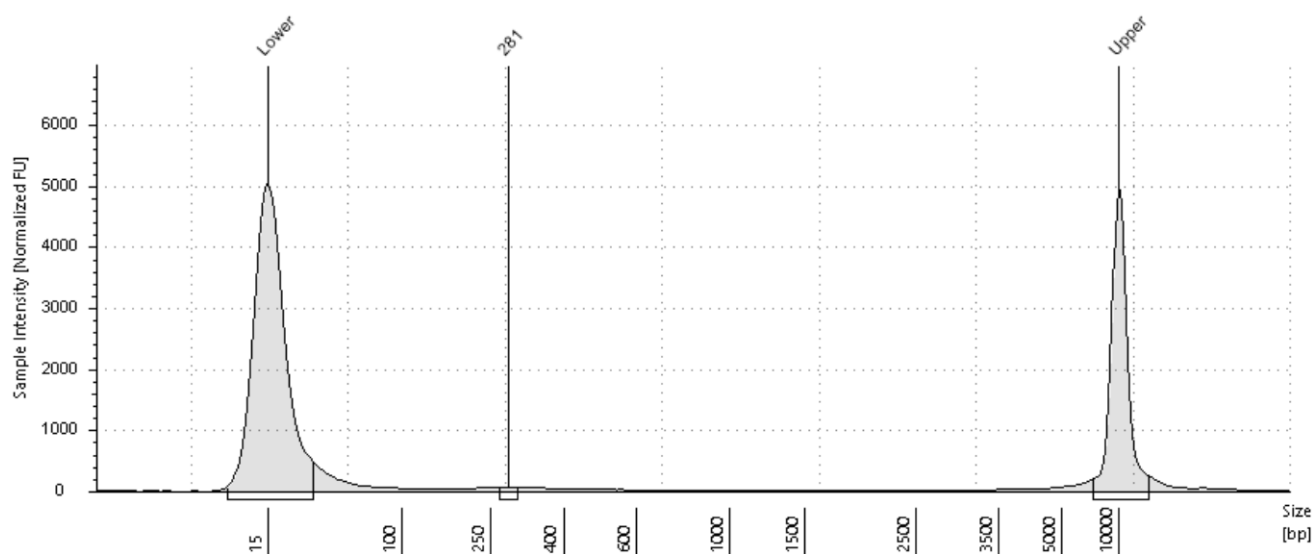
B2: 67**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B2	0.0480	67	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.59	-	676	-		Lower Marker
281	0.0480	-	0.263	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

C2: 68

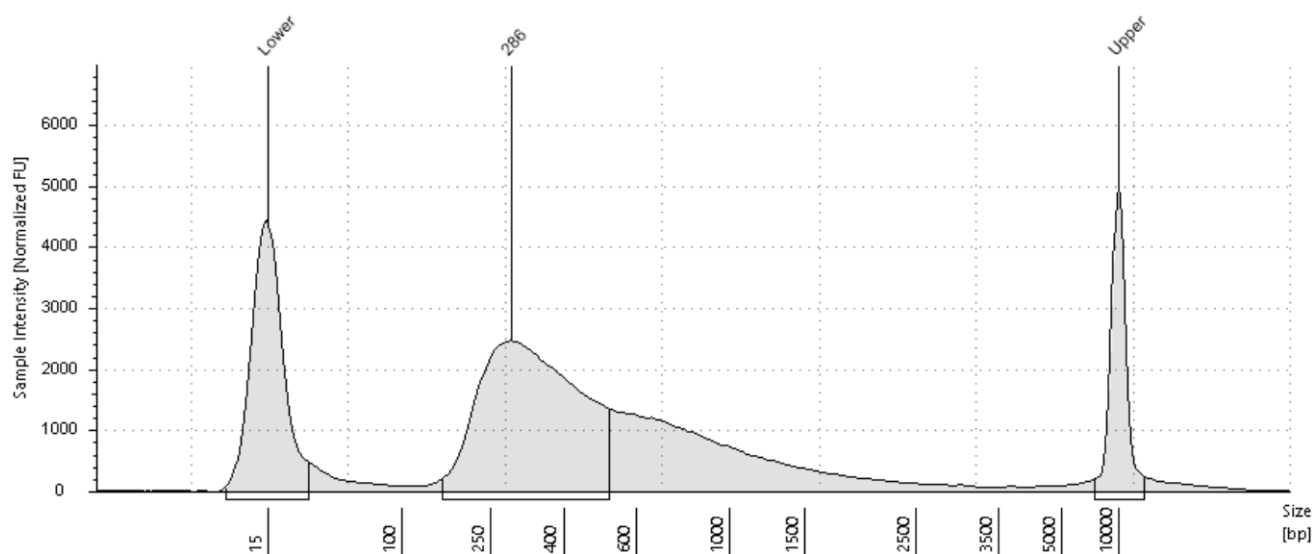


Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
C2	12.7	68		Caution! Expired ScreenTape device

Peak Table


Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.14	-	629	-		Lower Marker
286	12.7	-	68.4	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

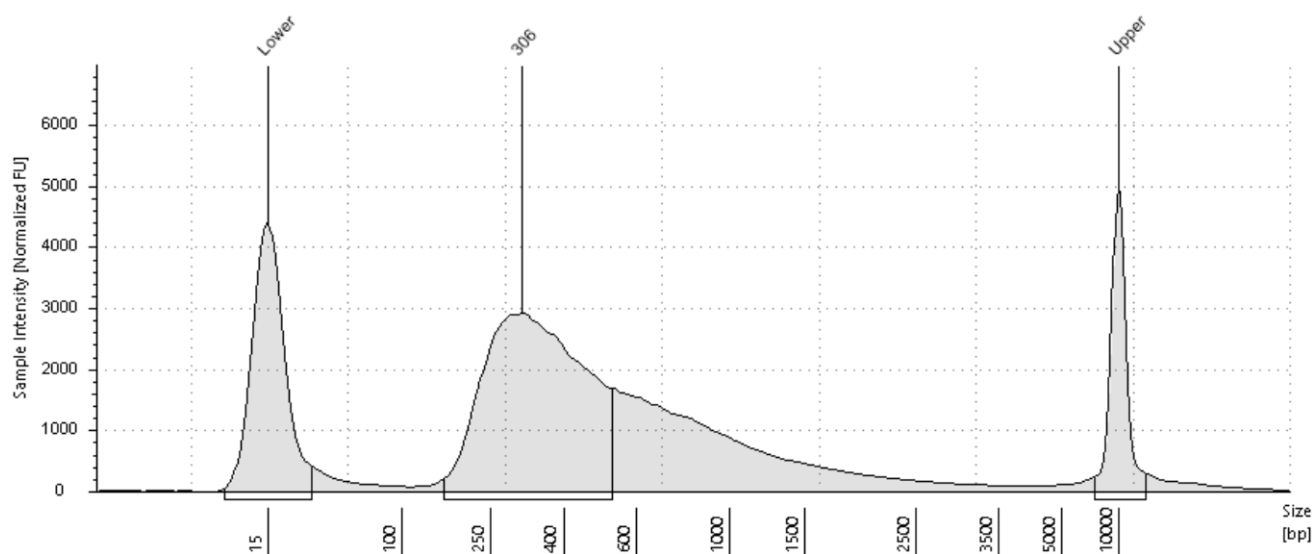D2: 69**Sample Table**

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
D2	15.5	69	⚠	Caution! Expired ScreenTape device

Peak Table


Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.47	-	663	-		Lower Marker
306	15.5	-	77.8	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

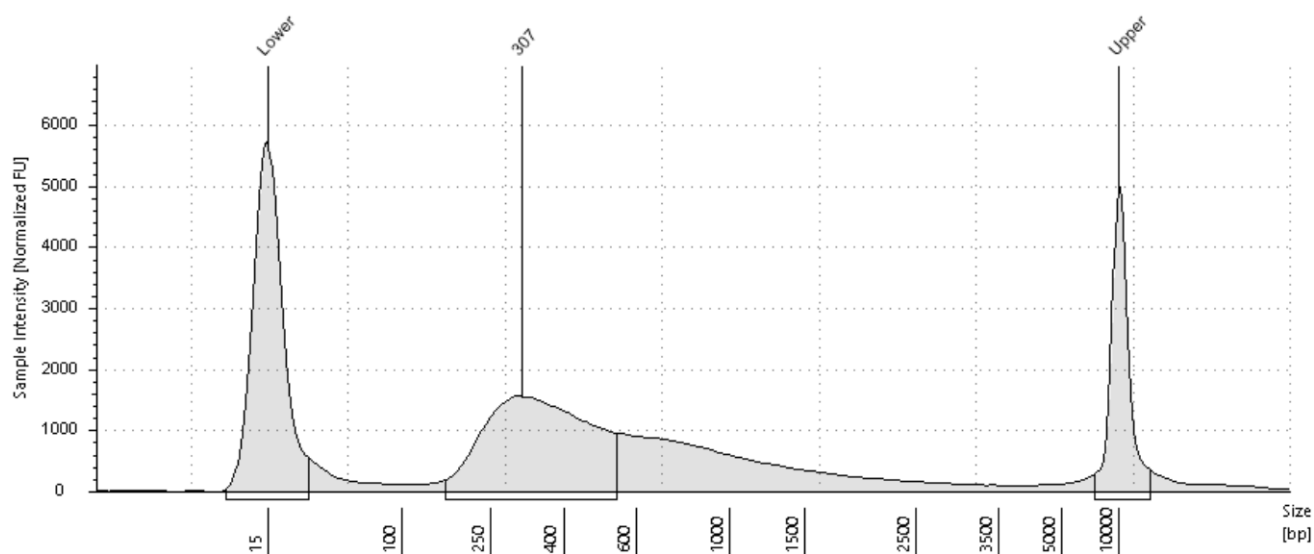E2: 70**Sample Table**

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
E2	7.83	70		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.97	-	715	-		Lower Marker
307	7.83	-	39.3	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

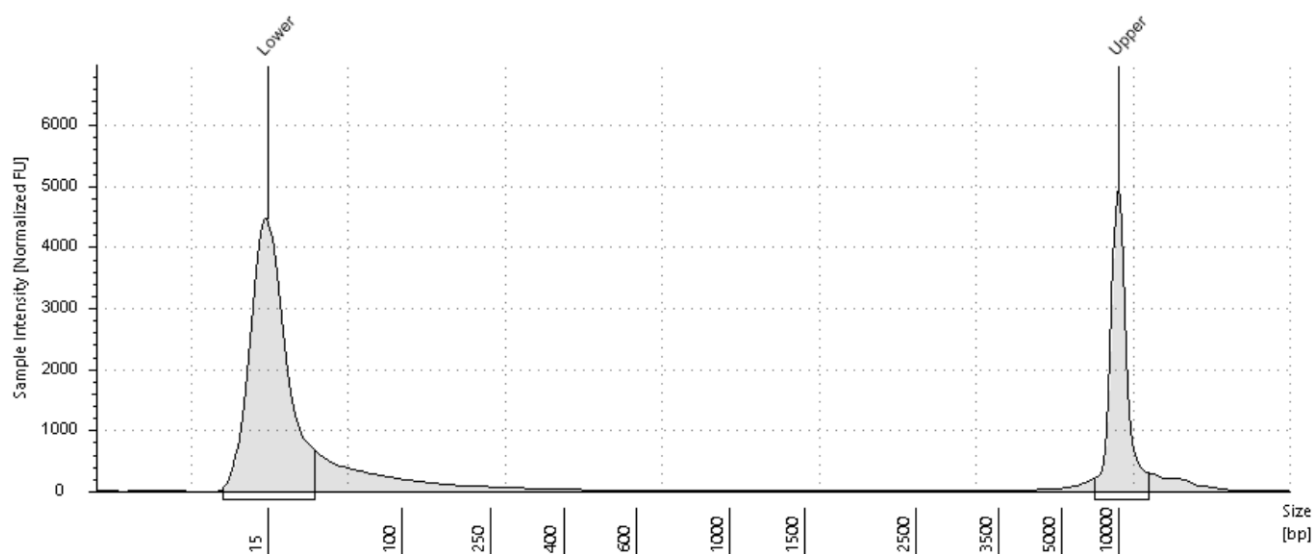
F2: 71**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
F2		71		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.71	-	688	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker

G2: 72

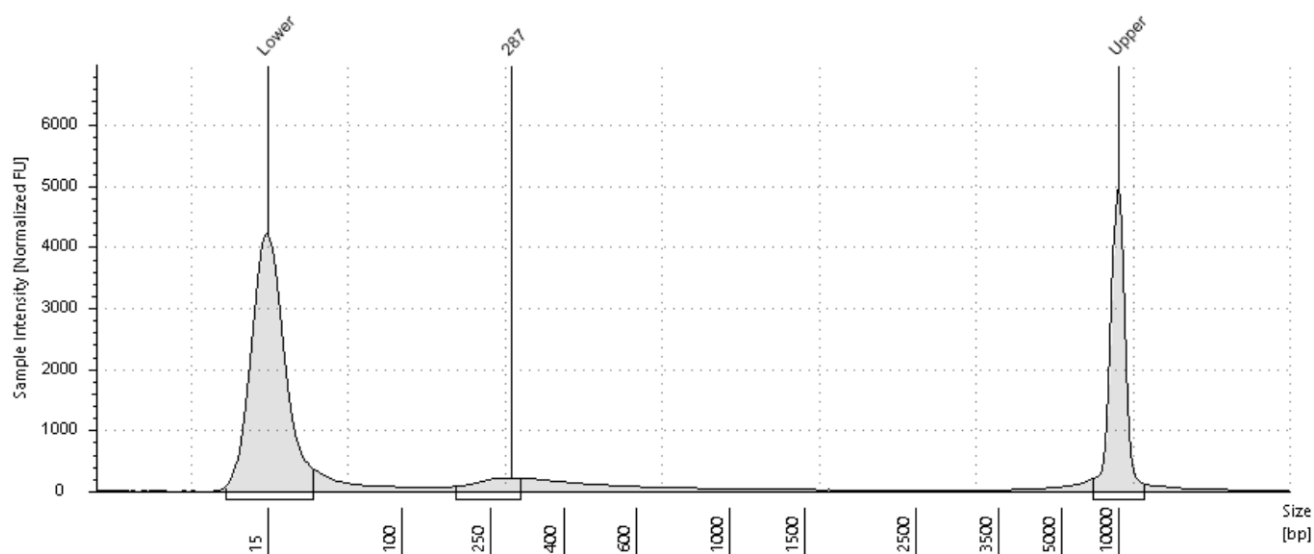


Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
G2	0.478	72		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.35	-	652	-		Lower Marker
287	0.478	-	2.56	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

H2: 73

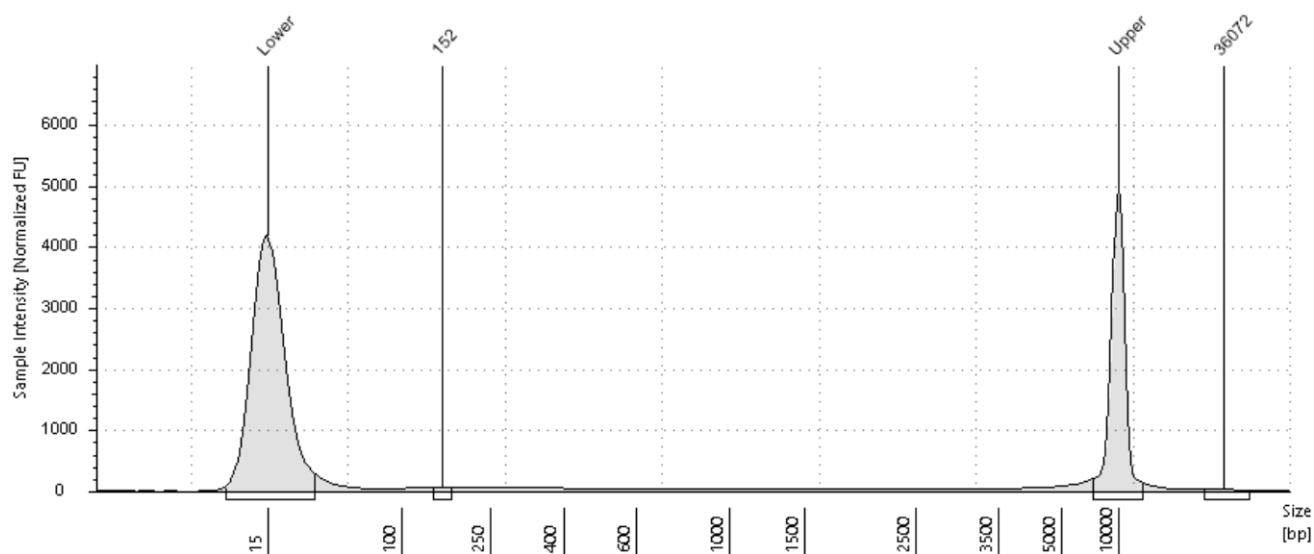

Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
H2	0.117	73		Caution! Expired ScreenTape device; Peak out of Sizing Range

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.93	-	711	-		Lower Marker
152	0.0634	-	0.641	53.99		
10000	3.25	3.25	0.500	-		Upper Marker
36072	0.0540	-	0.00230	46.01		Peak outside of Sizing Range