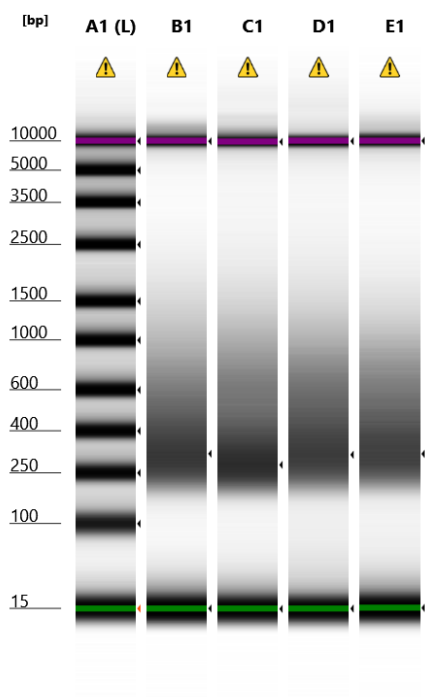


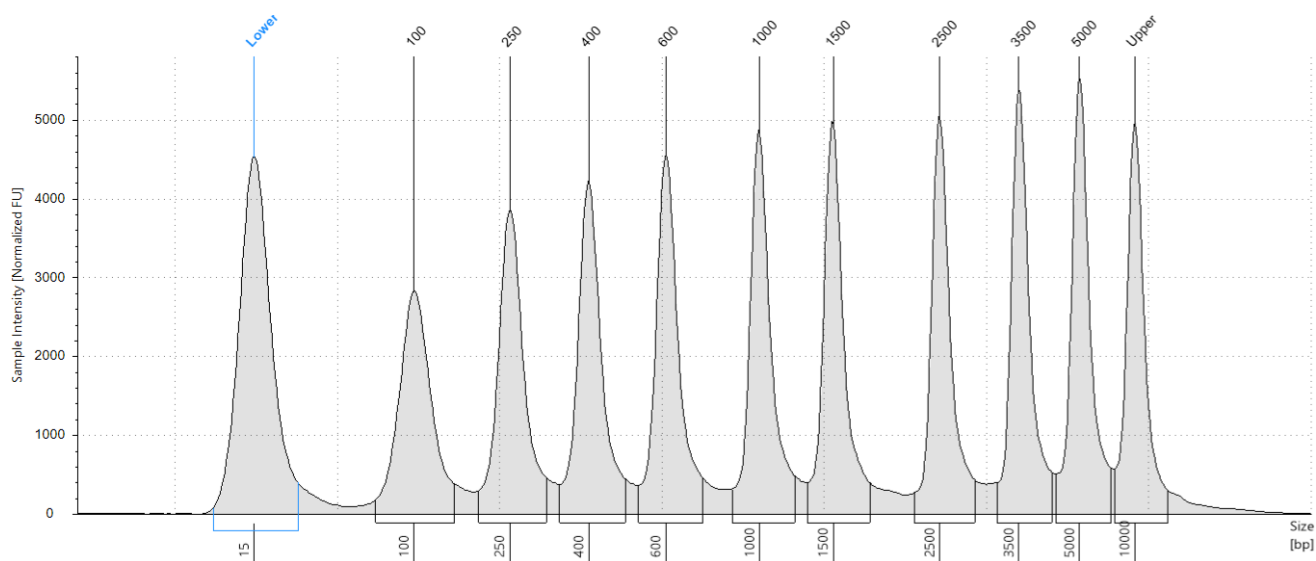
Filename: 2020-11-11 - 15.08.59.D5000



Default image (Contrast 100%)

### Sample Info

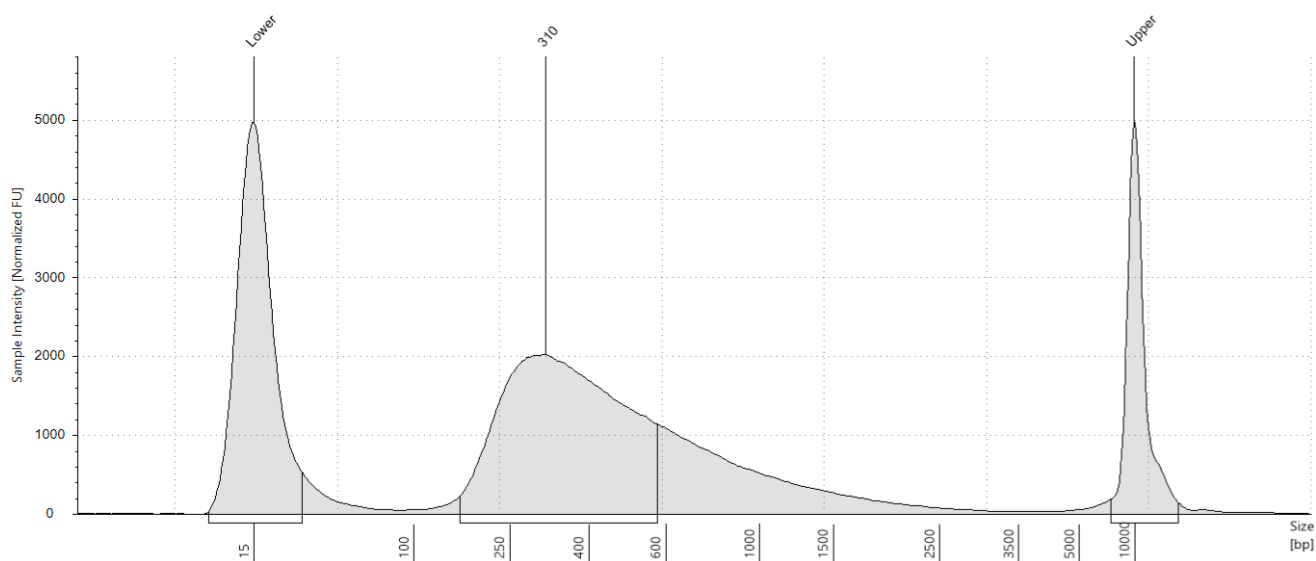
Well	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	42.8	Ladder	⚠	Caution! Expired ScreenTape device; Ladder
B1	10.8	P1	⚠	Caution! Expired ScreenTape device
C1	10.3	P3	⚠	Caution! Expired ScreenTape device
D1	14.2	2860	⚠	Caution! Expired ScreenTape device
E1	4.38	2878	⚠	Caution! Expired ScreenTape device

**A1: Ladder****Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	42.8	Ladder	⚠	Caution! Expired ScreenTape device; Ladder

**Peak Table**

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.05	-	620	-		Lower Marker
100	4.32	-	66.5	10.10		
250	4.69	-	28.8	10.96		
400	4.77	-	18.4	11.16		
600	4.94	-	12.7	11.54		
1000	4.86	-	7.48	11.36		
1500	4.84	-	4.96	11.32		
2500	4.62	-	2.84	10.81		
3500	4.81	-	2.12	11.26		
5000	4.91	-	1.51	11.49		
10000	3.25	3.25	0.500	-		Upper Marker

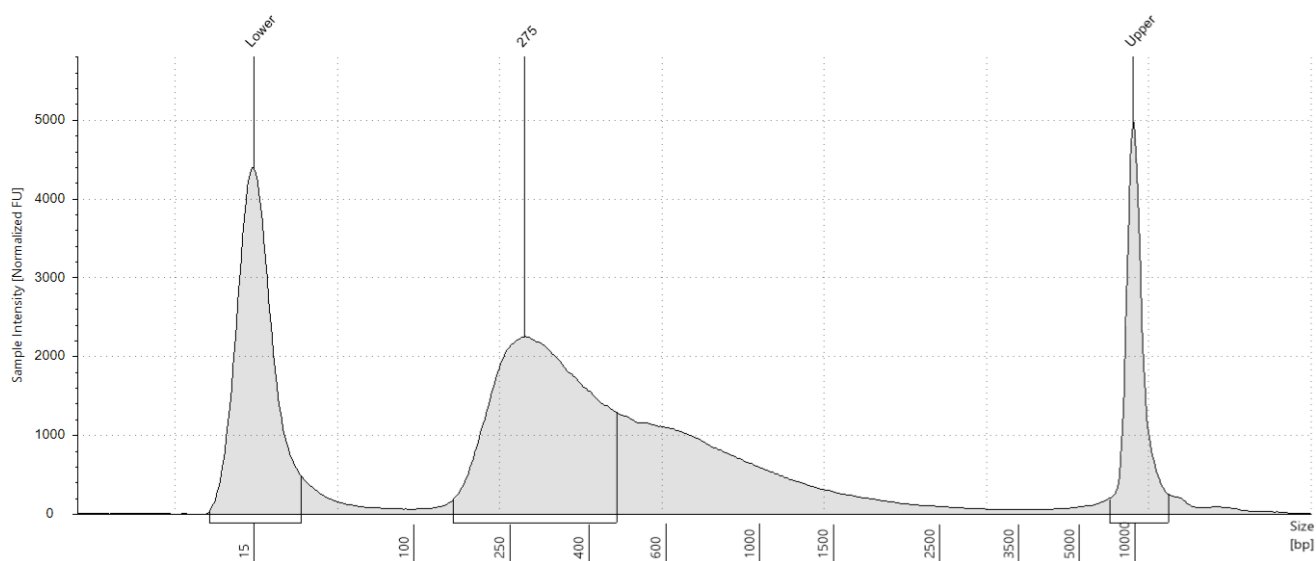
**B1: P1****Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	10.8	P1	⚠	Caution! Expired ScreenTape device

**Peak Table**

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.50	-	667	-		Lower Marker
310	10.8	-	53.4	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

## C1: P3

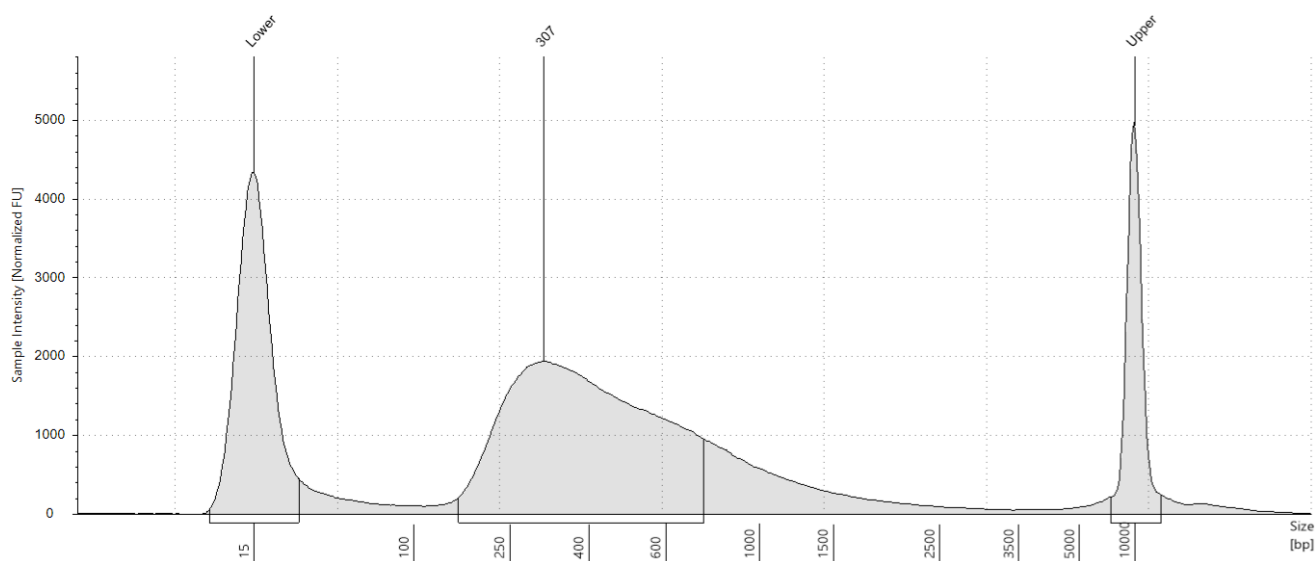


## Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
C1	10.3	P3		Caution! Expired ScreenTape device

## Peak Table

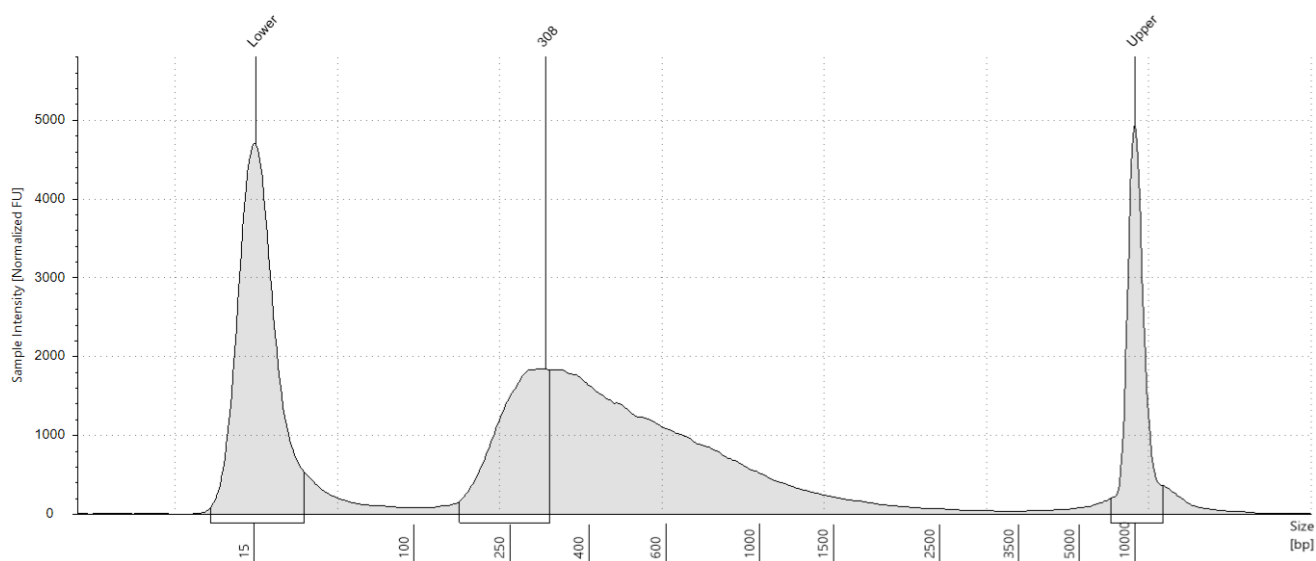
Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.20	-	636	-		Lower Marker
275	10.3	-	57.6	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

**D1: 2860****Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
D1	14.2	2860	⚠	Caution! Expired ScreenTape device

**Peak Table**

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.37	-	653	-		Lower Marker
307	14.2	-	71.3	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

**E1: 2878****Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
E1	4.38	2878	⚠	Caution! Expired ScreenTape device

**Peak Table**

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	6.93	-	711	-		Lower Marker
308	4.38	-	21.9	100.00		
10000	3.25	3.25	0.500	-		Upper Marker