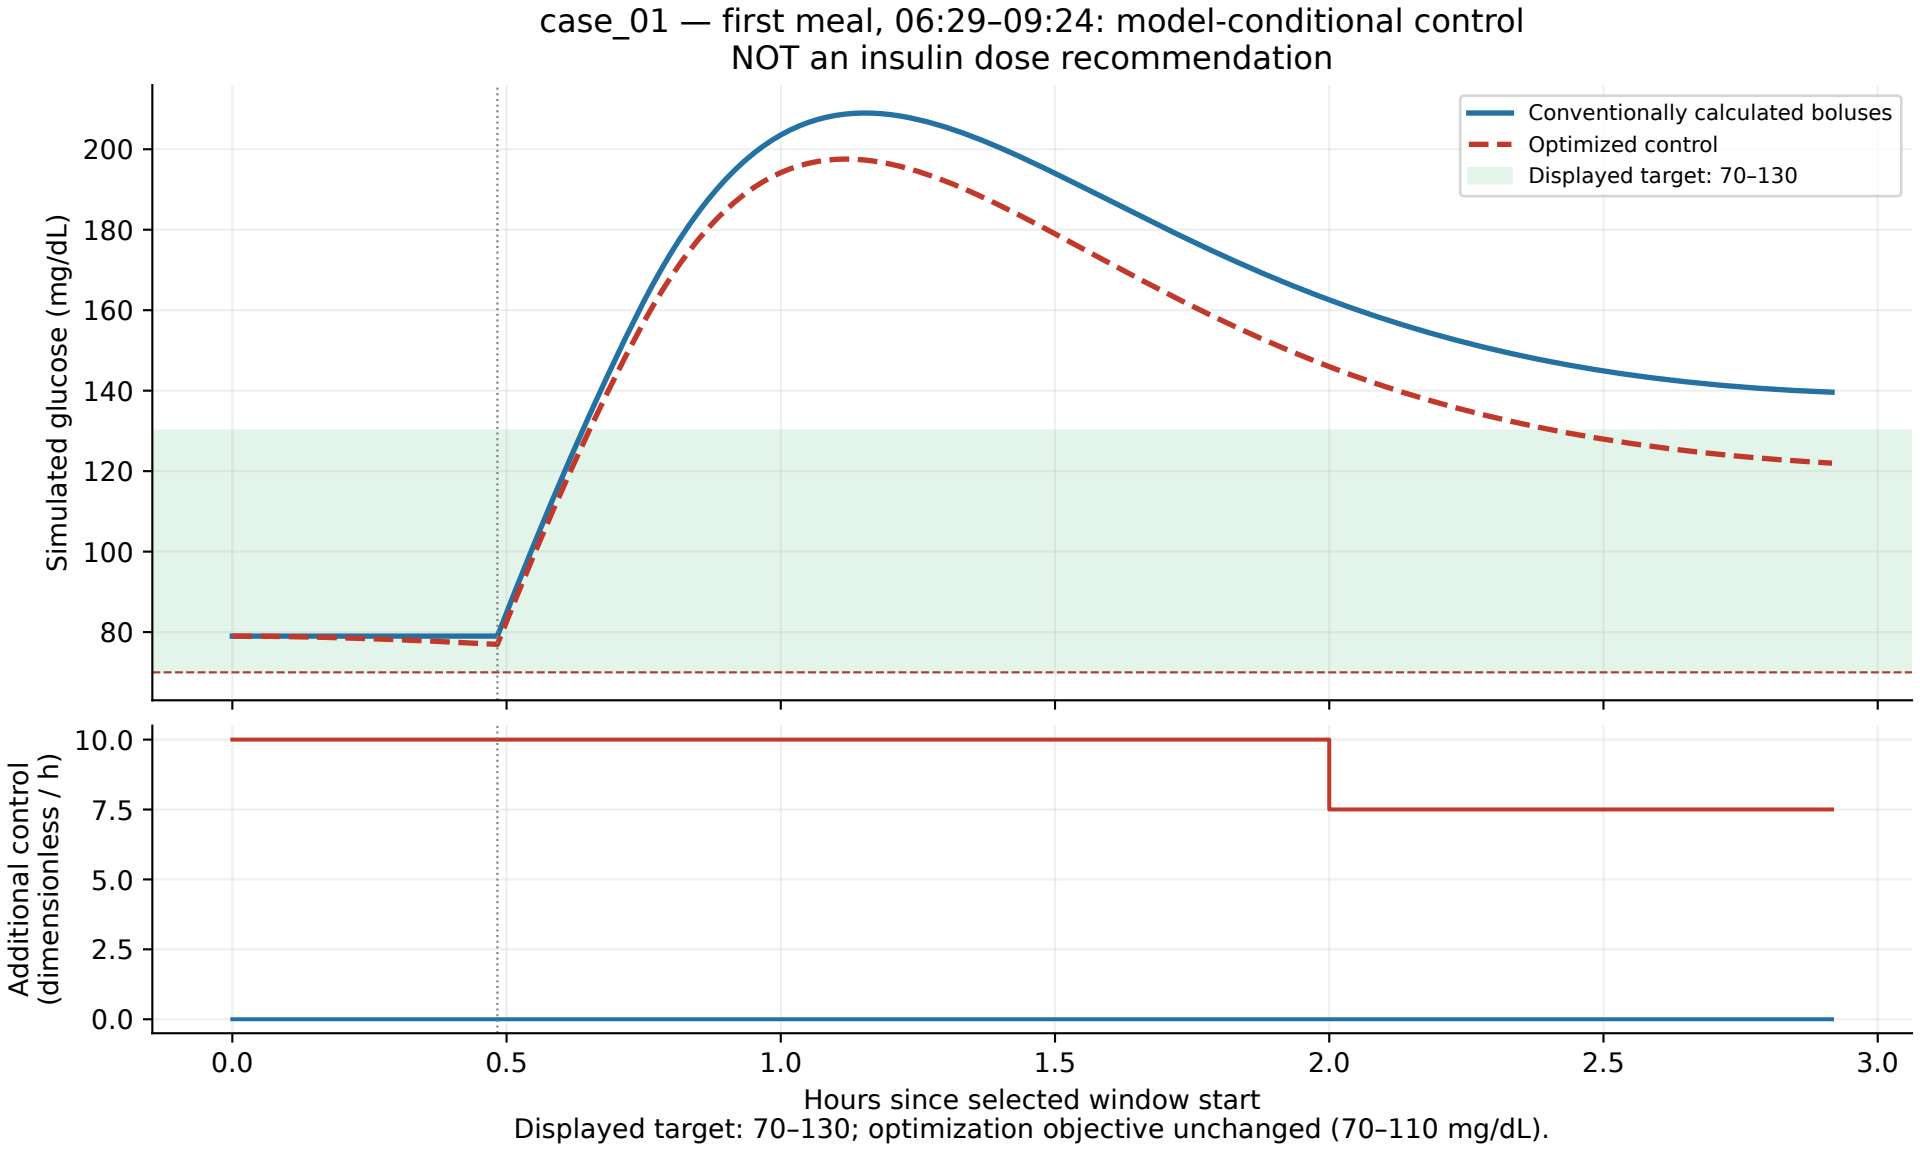
case_01 — first meal, 06:29–09:24: model-conditional control
NOT an insulin dose recommendation
Conventionally calculated boluses
Optimized control
Displayed target: 70–130
Simulated glucose (mg/dL)
200
180
160
140
120
100
80
Additional control
(dimensionless / h)
10.0
7.5
5.0
2.5
0.0
0.0
0.5
1.0
1.5
2.0
2.5
3.0
Hours since selected window start
Displayed target: 70–130; optimization objective unchanged (70–110 mg/dL).