Instrument controller software run summary:

Filename and data path: C:\Agilent Technologies\Data\2024 02 14\11-08-29\2024 02 14 11H 08M.raw
Created: 2/14/2024 11:26 AM
Number of capillaries: 6
Array serial number: 021621-09USFP
Effect length: 22 cm
Array usage count: 380
Instrument type: Femto Pulse
Instrument controller software version: 2.0.0.3
Device serial number: MY2104AD07

Method Information

Method name: FP-1002-22 - gDNA 165Kb.mthds
Gel prime: No
Full conditioning: Yes
Gel prime to buffer: No
Gel selection: Gel 1
Perform prerun: -5.0 kV, 60 sec.
Rinse: No
Marker 1: No
Rinse: Tray: 3, Row: A, Dip count: 1
Sample injection: -5.0 kV, 30 sec.
Separation: 70.0 min.
Tray name: Tray-3

Analysis mode: DNA

Notes

Time Shift: Using configured: slope=0.00025, intercept=0.0

Gel Image

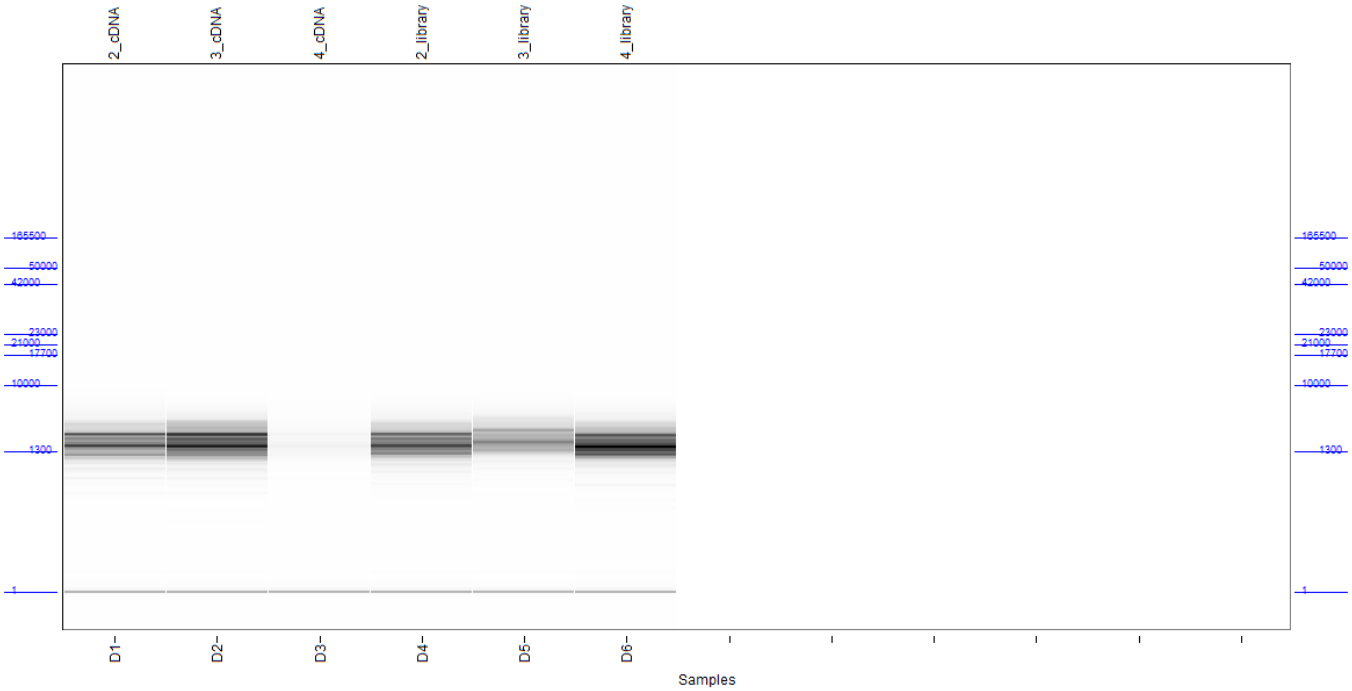
2_cDNA
3_cDNA
4_cDNA
2_library
3_library
4_library
165500
50000
42000
23000
21000
17700
10000
1300
1
D1
D2
D3
D4
D5
D6
Samples

Filename and data path: C:\Agilent Technologies\Data\2024 02 14\11-08-29\2024 02 14 11H 08M.raw

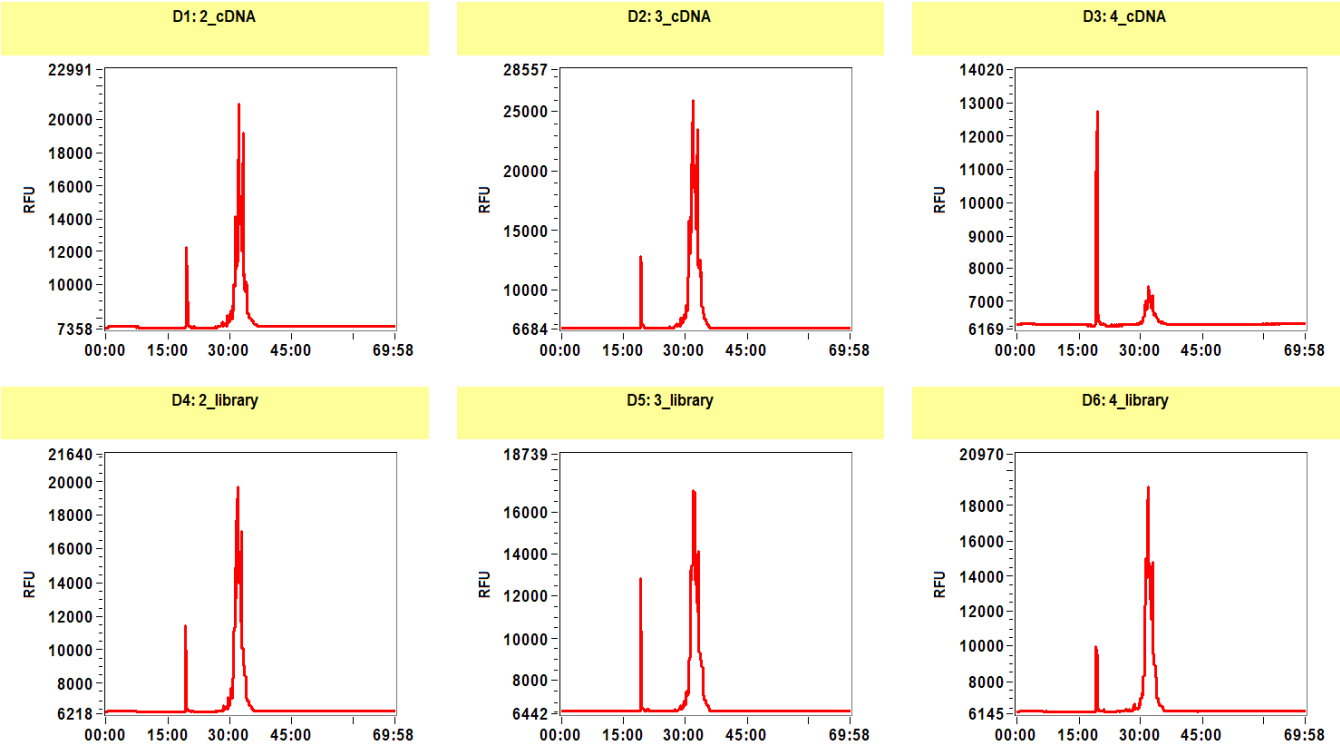

Sample: 2_cDNA
Well location: D1
Created: 2/14/2024 11:26 AM

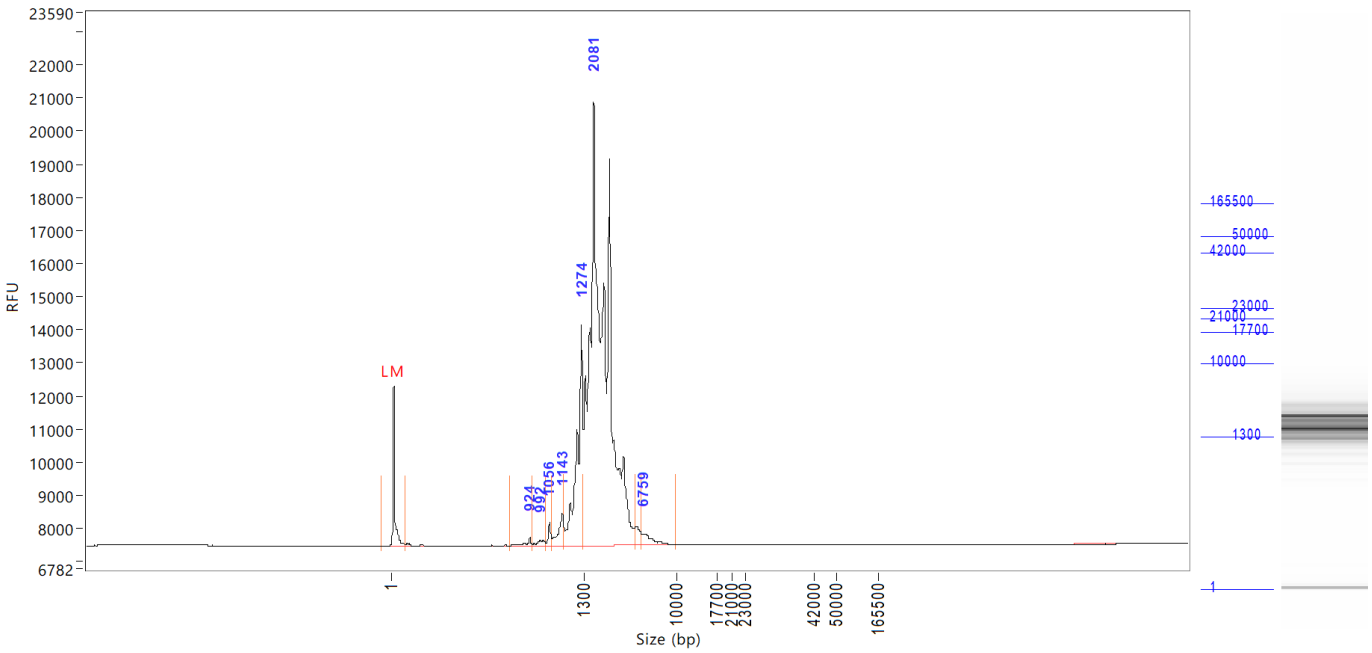

TIC:	237.6765	Pg/ul
TIM:	171.2363	Pmole/l
Total concentration:	240.4476	Pg/ul

```
Sample peak width (sec): 20   Sample min peak height: 50    Sample baseline V to V?: Y    Sample baseline V to V points: 3
Sample filter: Binomial       Number of points for filter: 3  Sample start region (min): 0  Sample end region (min): 70
Manual baseline start (min): 25     Manual baseline end (min): 70
Marker peak width (sec): 8    Marker min peak height: 500   Marker baseline V to V?: N    Marker baseline V to V points: 3
Lower marker selection: First peak > 500 RFU                Upper marker selection: Last peak > 500 RFU
Ladder size (bp)1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500
Quantification using: Ladder          Final concentration (ng/uL): 0.0200          Dilution factor: 10.0
Minimum RFU for data processing: 1
```

Sample: 3_cDNA
Well location: D2
Created: 2/14/2024 11:26 AM

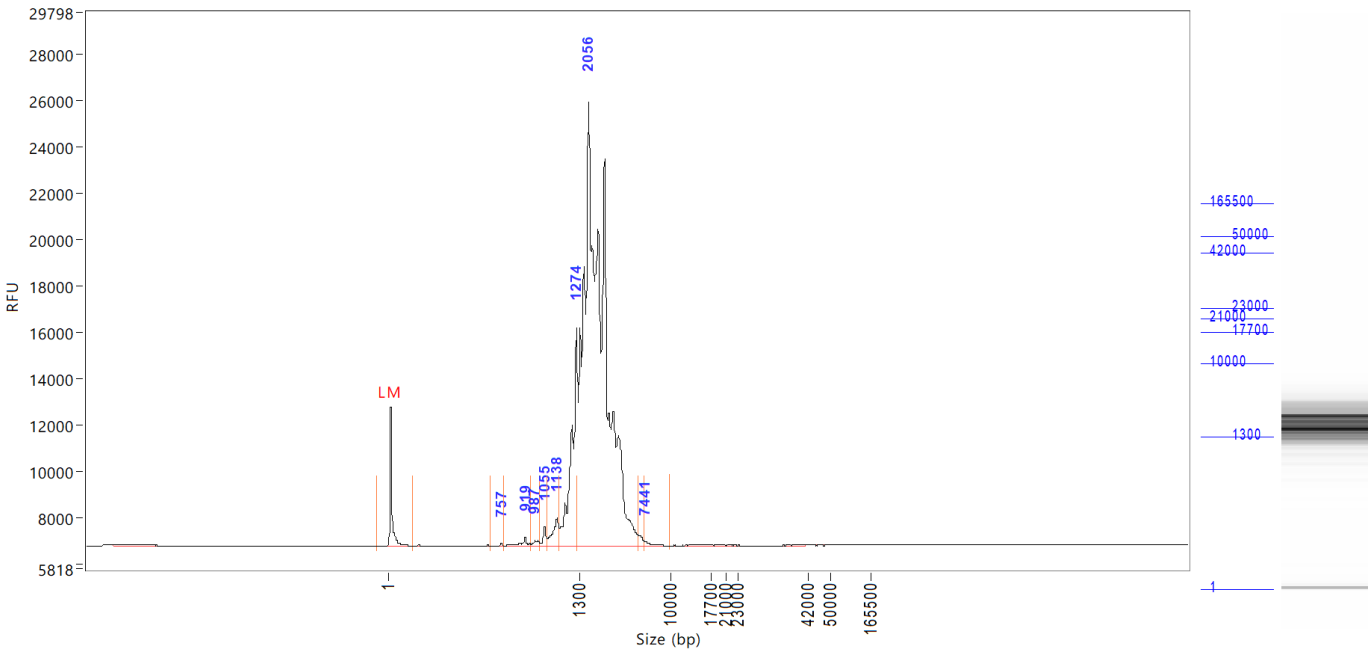

TIC:	319.9029	Pg/ul
TIM:	221.8732	Pmole/l
Total concentration:	320.3690	Pg/ul

```
Sample peak width (sec): 20   Sample min peak height: 50    Sample baseline V to V?: Y    Sample baseline V to V points: 3
Sample filter: Binomial       Number of points for filter: 3  Sample start region (min): 0  Sample end region (min): 70
Manual baseline start (min): 25     Manual baseline end (min): 70
Marker peak width (sec): 8    Marker min peak height: 500   Marker baseline V to V?: N    Marker baseline V to V points: 3
Lower marker selection: First peak > 500 RFU                Upper marker selection: Last peak > 500 RFU
Ladder size (bp)1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500
Quantification using: Ladder          Final concentration (ng/uL): 0.0200          Dilution factor: 10.0
Minimum RFU for data processing: 1
```

Sample: 4_cDNA
Well location: D3
Created: 2/14/2024 11:26 AM

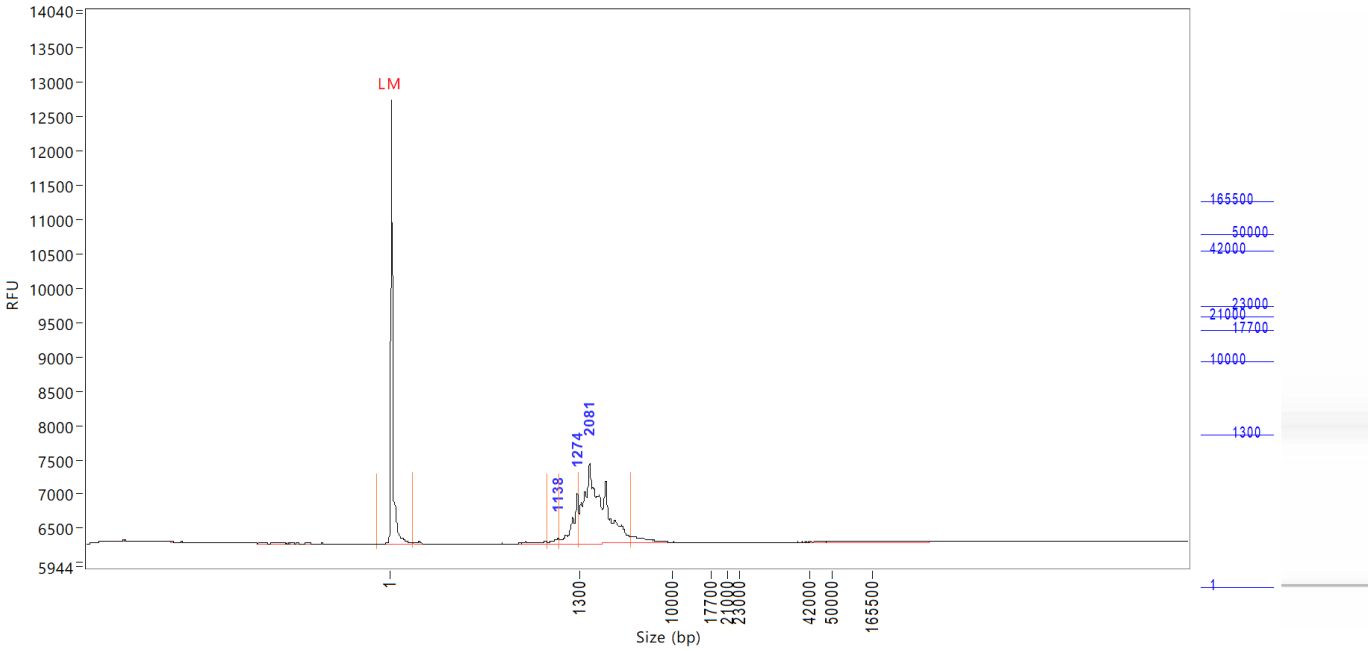

TIC:	19.1683	Pg/ul
TIM:	13.5327	Pmole/l
Total concentration:	21.6539	Pg/ul

```
Sample peak width (sec): 20   Sample min peak height: 50    Sample baseline V to V?: Y    Sample baseline V to V points: 3
Sample filter: Binomial       Number of points for filter: 3  Sample start region (min): 0  Sample end region (min): 70
Manual baseline start (min): 25     Manual baseline end (min): 70
Marker peak width (sec): 8    Marker min peak height: 500   Marker baseline V to V?: N    Marker baseline V to V points: 3
Lower marker selection: First peak > 500 RFU                Upper marker selection: Last peak > 500 RFU
Ladder size (bp)1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500
Quantification using: Ladder          Final concentration (ng/uL): 0.0200          Dilution factor: 10.0
Minimum RFU for data processing: 1
```

Sample: 2_library
Well location: D4
Created: 2/14/2024 11:26 AM

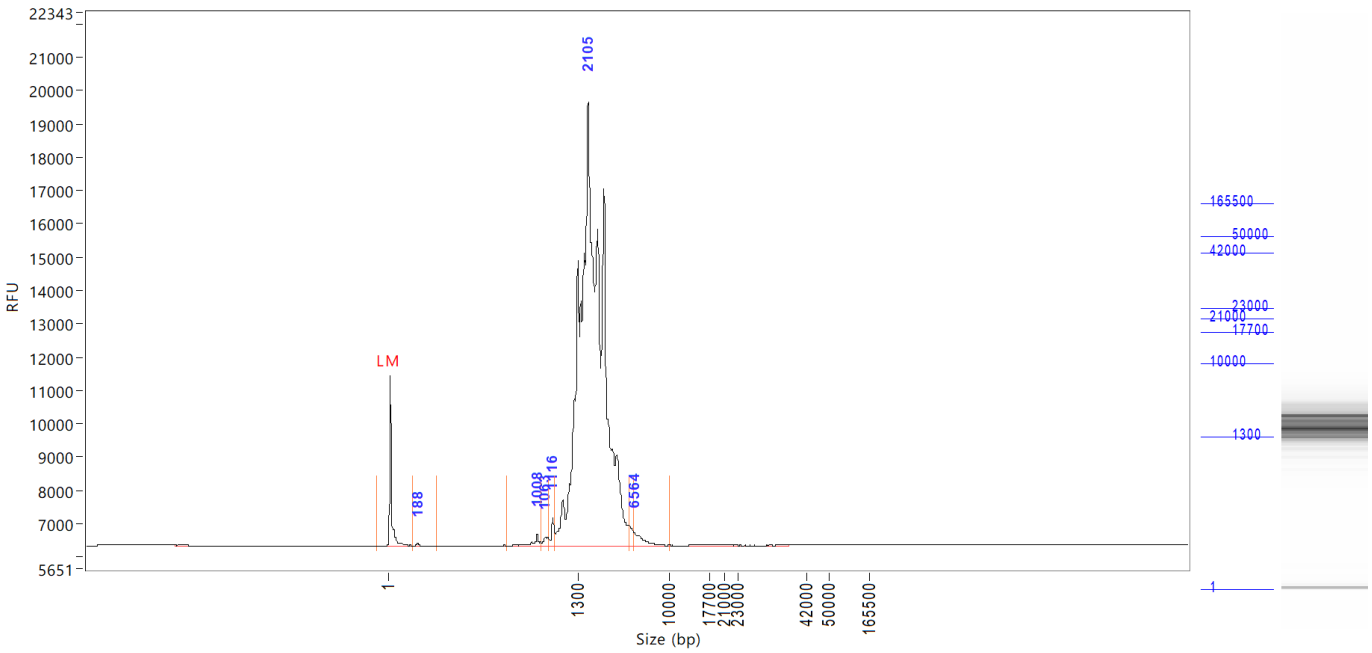

TIC:	260.9735	Pg/ul
TIM:	175.9326	Pmole/l
Total concentration:	263.6488	Pg/ul

```
Sample peak width (sec): 20   Sample min peak height: 50    Sample baseline V to V?: Y    Sample baseline V to V points: 3
Sample filter: Binomial       Number of points for filter: 3  Sample start region (min): 0  Sample end region (min): 70
Manual baseline start (min): 25     Manual baseline end (min): 70
Marker peak width (sec): 8    Marker min peak height: 500   Marker baseline V to V?: N    Marker baseline V to V points: 3
Lower marker selection: First peak > 500 RFU                Upper marker selection: Last peak > 500 RFU
Ladder size (bp)1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500
Quantification using: Ladder          Final concentration (ng/uL): 0.0200          Dilution factor: 10.0
Minimum RFU for data processing: 1
```

Sample: 3_library
Well location: D5
Created: 2/14/2024 11:26 AM

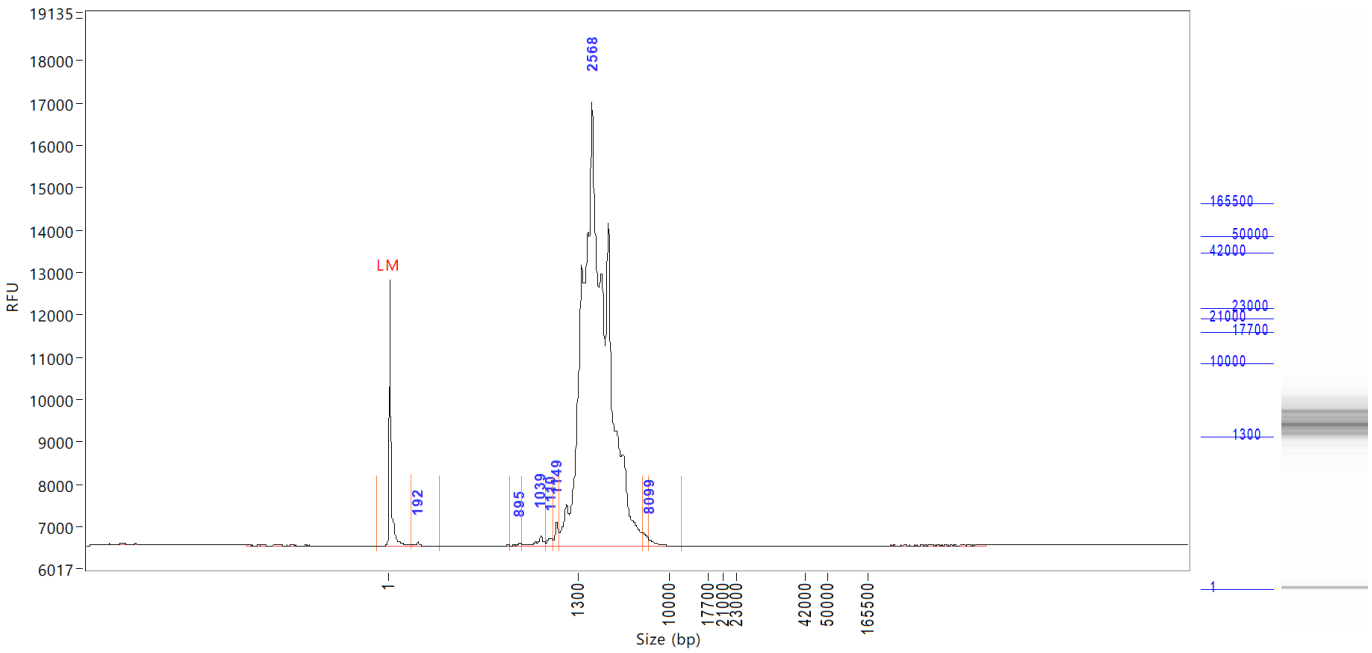

TIC:	177.0292	Pg/ul
TIM:	101.6017	Pmole/l
Total concentration:	178.2139	Pg/ul

```
Sample peak width (sec): 20   Sample min peak height: 50    Sample baseline V to V?: Y    Sample baseline V to V points: 3
Sample filter: Binomial       Number of points for filter: 3  Sample start region (min): 0  Sample end region (min): 70
Manual baseline start (min): 25     Manual baseline end (min): 70
Marker peak width (sec): 8    Marker min peak height: 500   Marker baseline V to V?: N    Marker baseline V to V points: 3
Lower marker selection: First peak > 500 RFU                Upper marker selection: Last peak > 500 RFU
Ladder size (bp)1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500
Quantification using: Ladder          Final concentration (ng/uL): 0.0200          Dilution factor: 10.0
Minimum RFU for data processing: 1
```

Sample: 4_library
Well location: D6
Created: 2/14/2024 11:26 AM

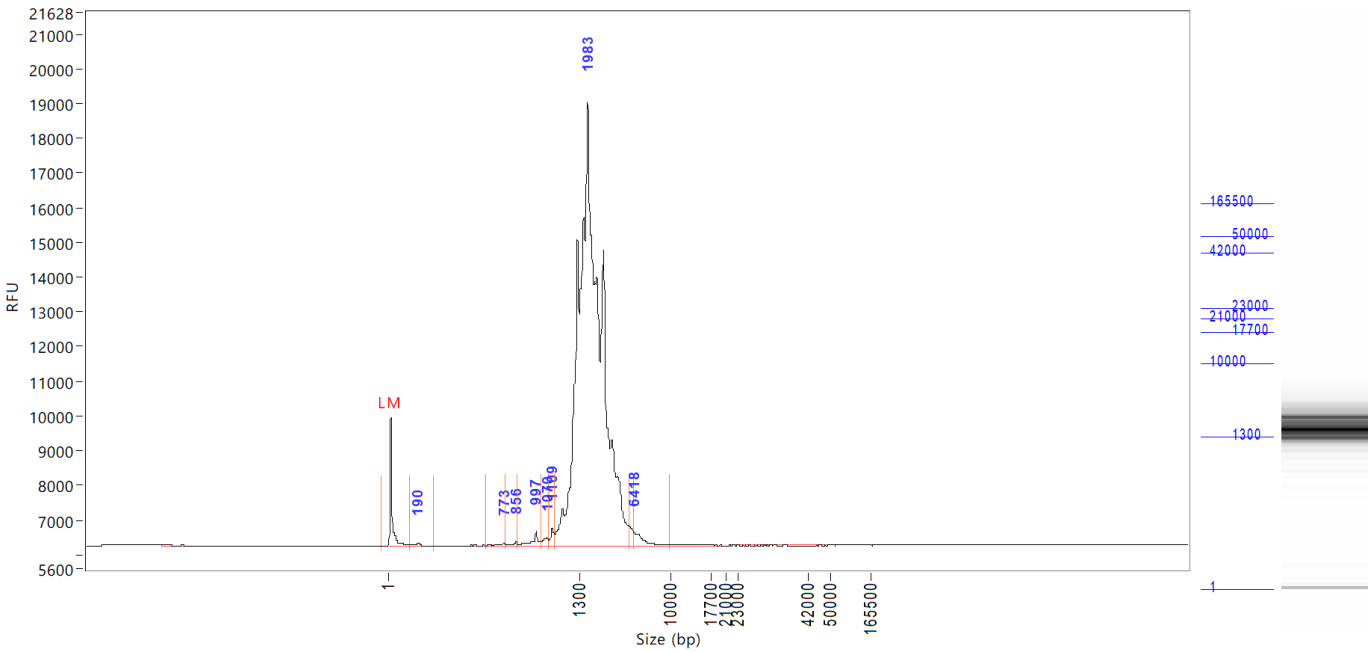

TIC:	323.1648	Pg/ul
TIM:	233.7236	Pmole/l
Total concentration:	325.4745	Pg/ul

```
Sample peak width (sec): 20   Sample min peak height: 50    Sample baseline V to V?: Y    Sample baseline V to V points: 3
Sample filter: Binomial       Number of points for filter: 3  Sample start region (min): 0  Sample end region (min): 70
Manual baseline start (min): 25     Manual baseline end (min): 70
Marker peak width (sec): 8    Marker min peak height: 500   Marker baseline V to V?: N    Marker baseline V to V points: 3
Lower marker selection: First peak > 500 RFU                Upper marker selection: Last peak > 500 RFU
Ladder size (bp)1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500
Quantification using: Ladder          Final concentration (ng/uL): 0.0200          Dilution factor: 10.0
Minimum RFU for data processing: 1
```
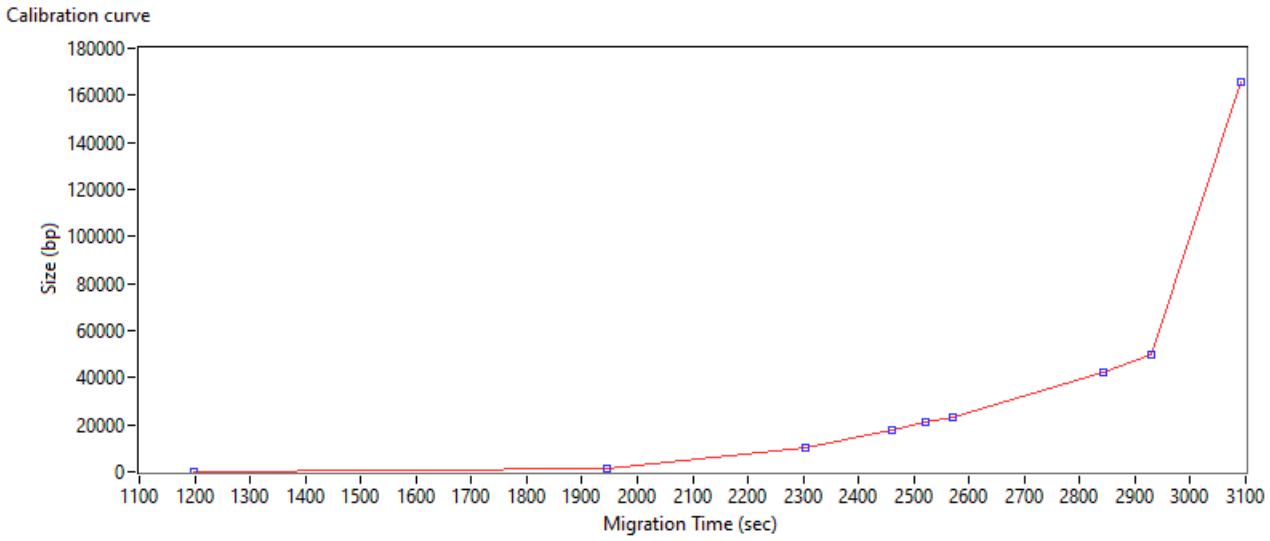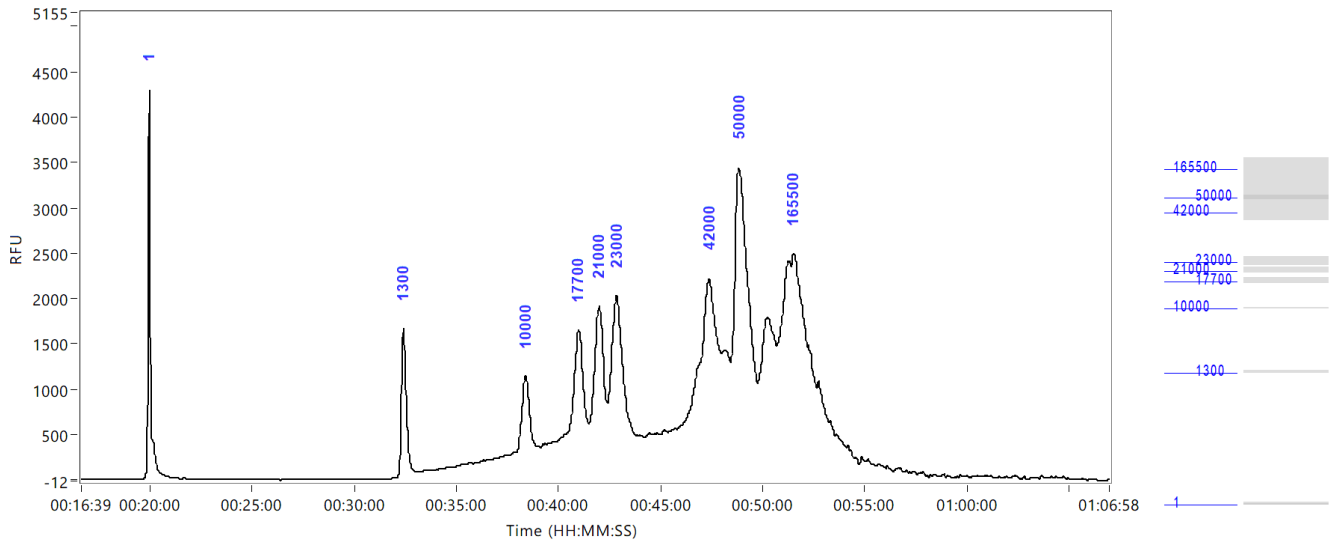
Sample: SampD12
Well location: D12
Created: 2/14/2024 11:26 AM
Fit type: Point to point