Axolabs GmbH

Document No.: MDR_2439EXNA_DOGPLASMA	Document Title: EXECUTION OF THE PNA-HPLC-ASSAY FOR DETERMINATION OF 2439-EXNA FROM DOG PLASMA (METHOD DEVELOPMENT REPORT)	
Edition: 02		Supersedes Edition: 01
Effective Date: 20.AUG.2024		Effective Date: 15.AUG.2024

SCOPE:	**Department *Bioanalytics* – nonGLP relevant activities, assays**
DISTRIBUTION:	**Network drive:** **O:\Axolabs_Kunden\AG_Vallabh_Minikel_Broad Institute** **M:\Labodogory\MDR PNA-HPLC\AG_Vallabh_Minikel_Broad Institute**

	Name; Position	Date	Signature
PREPARATION:	**Verena Schilling** **Research Associate**	16 AUG 2024	[redacted]
VERIFICATION:	**Thessa Jacob** **Scientist Bioanalytics**	16-Aug-2024	[redacted]

TABLE OF CONTENTS

1 RELATED DOCUMENTS **4**

2 DEFINITIONS AND ABBREVIATIONS **5**

3 ACTIVITIES TO BE PERFORMED **6**

3.1 Summary **7**

3.2 Limited Assay Qualification **9**

4 RESULTS FROM QUALIFICATION RUNS IN DOG PLASMA **9**

5 ASSAY PROCEDURE **16**

5.1 Preparation of Stock Solution **16**

5.1.1 Instruments and Materials 17

5.1.2 Reagents 17

5.1.3 Method 17

5.2 Preparation of the Assay Protocol **17**

5.3 Preparation of Working Solutions **17**

5.3.1 Instruments and Materials 18

5.3.2 Reagents 18

5.3.3 Method 18

5.4 Preparation of Plasma Lysate and Hybridization **18**

5.4.1 Instruments and Materials 18

5.4.2 Reagents 18

5.4.3 Method 19

5.4.3.1 Sample Dilution 20

5.5 HPLC Analysis **20**

5.5.1 Material and Reagents 20

5.5.2 Instruments 20

5.5.3 Method 21

5.6 Evaluation of HPLC Chromatograms **22**

6 RECORDS **23**

7 CHANGE HISTORY **23**

TABLE OF TABLES

Table 1 Parameters of final method 8
Table 2 Calibration Curve Accuracy in K2 EDTA dog plasma 11
Table 3 Confirmation of LLOQ in K2 EDTA dog plasma 12
Table 4 Selectivity in K2 EDTA dog plasma 13
Table 5 Carry-over in K2 EDTA dog plasma 13
Table 6 Accuracy and Precision in K2 EDTA dog plasma 14
Table 7 Freeze and thaw and short-term stability in K2 EDTA dog plasma 15
Table 8 Dilution Integrity in K2 EDTA dog plasma 16
Table 9 Gradient table 21

TABLE OF FIGURES

Figure 1 Structure and sequence of the analyte 2439exNA 6
Figure 2 HPLC Profile of 2439exNA in dog plasma. Chromatograms at the LLOQ (1 ng/mL, upper picture) and the ULOQ (1,000 ng/mL, lower picture) are shown. 7

1 RELATED DOCUMENTS

This instruction describes the execution of a PNA-HPLC-Assay based on the following documents:

- KU-RGL-SOP-002 (formerly: REG-102) – Methoden-Validierung im GLP/GCP-Bereich (*Method Validation in GLP/GCP Area*) with the following subordinate Instructions, Forms, Spreadsheet Applications:
  - KU-RGL-ESS-002 (formerly: REG-102-S02) – Method Validation Data Report
  - KU-RGL-ESS-005 (formerly: REG-102-S05) – Method Validation Protocol PNA Assay - Liquid Matrices - OnePot
- KU-RGL-SOP-009 (formerly: REG-109) – Durchführung des PNA-HPLC-Assay (*Execution of the PNA-HPLC-Assay*) with the following subordinate Instructions, Forms, Spreadsheet Applications:
  - KU-RGL-ESS-013 (formely: REG-109-S03) – PNA Assay Instruction and Protocol – Liquid Matrices - OnePot
  - KU-RGL-ESS-014 (formerly: REG-109-S04) – Preparation of HPLC Buffers & Stock Solutions
  - KU-RGL-INS-005 (formerly: REG-109-I01) – PNA-HPLC-Assay SST
- KU-RGL-SOP-010 (formerly: REG-110) – Herstellung von Standardlösungen mit einer Präzisionswaage (*Preparation of Standard Solutions Using a Precision Balance*) with the following subordinate Instructions, Forms, Spreadsheet Applications:
- Development protocol in the project folder AN400.0-24 under the following link:

  O:\Axolabs_Kunden\AG_Vallabh_Minikel_Broad Institute

The above-mentioned documents describe the assay execution under nonGLP-relevant conditions. The parameters and results described in this document are generated from a nonGLP method development, which was conducted following the above-mentioned SOPs.

2 DEFINITIONS AND ABBREVIATIONS

°C	Grad Celsius
AB0X	Analytical batch AN400.0-23_03_AB0X
ACN	Acetonitrile
AEX-HPLC	Anion-Exchange High-Performance Liquid Chromatography
CV	Coefficient of Variation
DNA	Deoxyribonucleic Acid
ed	Edition
EDTA	Ethylenediaminetetraacetic Acid
FDA	Food and Drug Administration
GLP	Good Laboratory Practice
HPLC	High Performance Liquid Chromatography
ICH	International Conference on Harmonization
IFU	Instructions For Use
K2-EDTA	Dipotassium Ethylenediaminetetraacetic Acid
LC/MS	Liquid Chromatography / Mass Spectrometry
LLOQ	Lower Limit of Quantitation
min	Minute
n.a.; N/A; N.A.	Not applicable
PBS	Phosphate Buffered Saline
PI	Principal Investigator
PNA	Peptide Nucleic Acid
QC	Quality Control
rcf	Relative centrifugal force
RNA	Ribonucleic Acid
SDS	Sodium Dodecyl Sulfate
siRNA	Small Interfering Ribonucleid Acid
SOP	Standard Operating Procedure
SD	Standard Deviation
SST	System Suitability Test(ing)
ULOQ	Upper Limit of Quantitation

3 ACTIVITIES TO BE PERFORMED

This method development report describes an anion exchange (AEX)-HPLC method with fluorescence detection that allows the specific detection of the analyte 2439-exNA from dog plasma. 2439-exNA is a dimer composed of two identical siRNAs, which are linked at their sense strands with a tetraethylene glycol linker, with the sequence depicted in Figure 1:

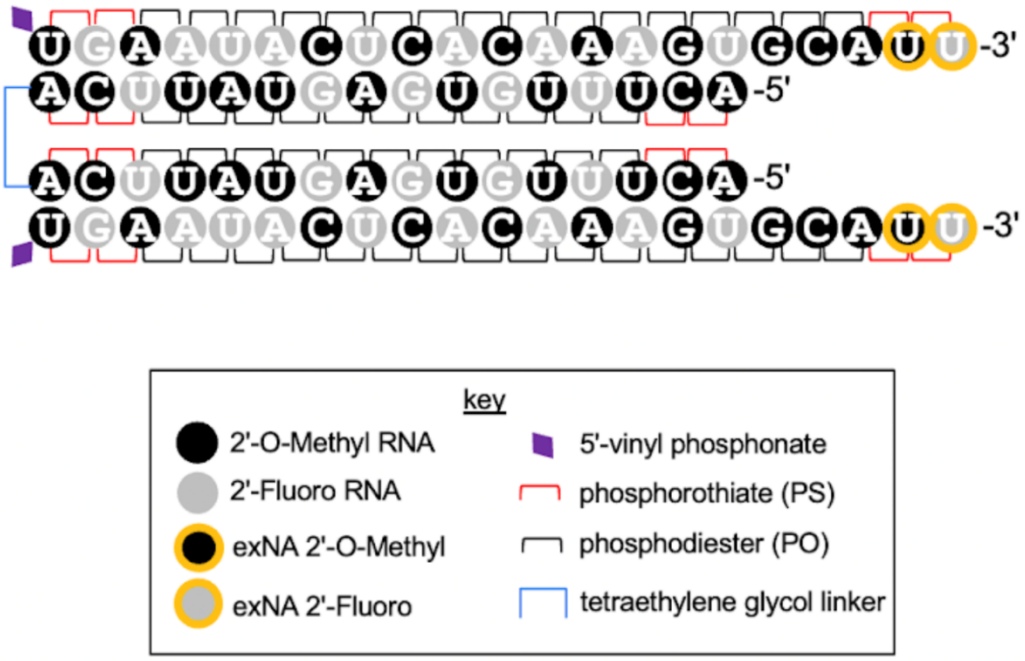

Figure 1 Structure and sequence of the analyte 2439exNA

The assay is based on the specific hybridization of the antisense strands of 2439-exNA to the complementary PNA-probe. The PNA-probe is N-terminally conjugated with an Atto425-fluorescent dye. The utilized PNA-BroadInst-01 is complementary to the antisense strand of 2439-exNA and has the following sequence:

N-term Atto425-OO-cdc ttt gtg dgt d C-term

This method was developed without having any metabolites of 2439-exNA

Figure 2 shows the HPLC-profile of 2439-exNA in dog plasma.

3.1 Summary

.

[redacted]

[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]

[redacted]

4 RESULTS FROM QUALIFICATION RUNS IN DOG PLASMA

In this section, the raw data for the determination of calibration curve accuracy (Table 2), confirmation of LLOQ (Table 3), selectivity (Table 4), carry-over (Table 5), accuracy and precision (Table 6), freeze and thaw and short term stability (Table 7) and dilution integrity (Table 8) from 2439-exNA in dog plasma are shown. The results were generated in one qualifying run. Calibration standard and QC samples were prepared by spiking 2439-exNA into dog plasma. Samples were prepared according to the assay procedure described in Section 5.

During the qualification run, the calibration range was between 1.0 ng/mL and 1,000.0 ng/mL. All calibration standards were within ±15 % (±20 % at the LLOQ) of the nominal concentration.

Selectivity and Sensitivity

The LLOQ was confirmed at 1.0 ng/mL in dog plasma. No signal was detected in corresponding blank plasma samples and the 2439-exNA peaks at the LLOQ of 1.0 ng/mL were at least 5 times the background signal in the analysis run. At the LLOQ, the mean back-calculated concentration was 105.0 % of nominal with a CV of 6.7 %.

The selectivity of the method was demonstrated by comparison of unspiked samples of dog plasma with the same plasma samples spiked with 2439-exNA at a concentration of the LLOQ. The signal for 2439-exNA in the spiked samples gave an at least 5-fold higher response (peak area) compared to the blank samples.

Carry Over

Carry over plasma samples were run after the 1,000.0 ng/mL calibration standards. There was no distinct analyte signal detectable in the carry-over samples after the 1,000.0 ng/mL standards.

Accuracy and Precision

QC samples were prepared at 4 concentration levels which are covering the calibration curve range:

- at the LLOQ (QC-LLOQ): 1.0 ng/mL
- at 3 times above the LLOQ (QC-Low): 3.0 ng/mL
- at around 50 % of the calibration curve range (QC-Mid): 450.0 ng/mL
- at least at 75 % of the upper calibration curve range (QC-High): 900.0 ng/mL

The QC samples for the determination of the accuracy and precision of the method met the acceptance criteria with following results:

- 100 % of the QC samples at all concentration levels were within ±15 % (±20 % at the LLOQ) of their nominal value.
- The mean accuracies at the 4 concentration levels were 96.7 % (QC-LLOQ), 95.3 % (QC-Low), 101.1 % (QC-Mid) and 100.4 % (QC-High).
- The mean precisions at the 4 concentration levels were 6.0 % (QC-LLOQ), 1.9 % (QC-Low), 1.0 % (QC-Mid) and 1.8 % (QC-High).

Freeze-Thaw and Short-Term-Stability

The freeze and thaw (one cycle) and short term stability of 2439-exNA in dog plasma was successfully tested. Aliquots of the 2439-exNA at the 2 QC concentration levels QC-Low and QC-High were prepared and stored at -80°C for at least 12 hours. After thawing of the samples, they were stored on wet ice for 4 hours and analyzed in triplicate.

After one freeze and thaw cycle and storage of 4 hours on wet ice the mean back-calculated concentrations were at 103.3 % (QC-Low) and 96.7 % (QC-High) of the nominal value.

Dilution Integrity

The precision and accuracy of dog plasma sample dilution was evaluated using a DI-QC standard prepared at concentration levels 500-fold (500,000.0 ng/mL) above the ULOQ of 1,000.0 ng/mL. This QC sample was analyzed and quantified after 1:1,000 dilution in 3 replicates. Samples were diluted with 4M Urea. The mean accuracy was 95.6 % and the CV was 1.5 %

Table 2 Calibration Curve Accuracy in K2 EDTA dog plasma

2439-exNA		Cal-Level-2		Cal-Level-3		Cal-Level-4		Cal-Level-5		Cal-Level-6		Cal-Level-7	
		1.0 ng/mL		5.0 ng/mL		50.0 ng/mL		100.0 ng/mL		500.0 ng/mL		1,000.0 ng/mL	
Run ID	Sample No.	Calculated 2439-exNA Conc. ng/mL	Acc. criterion +/-20 % of Nominal	Calculated 2439-exNA Conc. ng/mL	Acc. criterion +/-15 % of Nominal	Calculated 2439-exNA Conc. ng/mL	Acc. criterion +/-15 % of Nominal	Calculated 2439-exNA Conc. ng/mL	Acc. criterion +/-15 % of Nominal	Calculated 2439-exNA Conc. ng/mL	Acc. criterion +/-15 % of Nominal	Calculated 2439-exNA Conc. ng/mL	Acc. criterion +/-15 % of Nominal
AN400.0-23_01_AB02	16 - 21	1.0	100.0%	4.8	96.0%	51.1	102.2%	100.6	100.6%	501.2	100.2%	999.9	100.0%
AN400.0-23_01_AB02	56 - 61	1.1	110.0%	4.8	96.0%	50.3	100.6%	101.4	101.4%	501.6	100.3%	994.1	99.4%
Mean		1.05	105.0%	4.80	96.0%	50.70	101.4%	101.00	101.0%	501.40	100.3%	997.00	99.7%
SD (+/-)		0.07		0.00		0.57		0.57		0.28		4.10	
CV (%)		6.7%		0.0%		1.1%		0.6%		0.1%		0.4%	
N		2		2		2		2		2		2	

Table 3 Confirmation of LLOQ in K2 EDTA dog plasma

2439-exNA		Cal-Level-1			Cal-Level-2		
		0.0 ng/mL			1.0 ng/mL		
Run ID	**Sample No.**	**Peak Area [mV*min]**	**Calculated 2439-exNA Conc. ng/mL**	**Acc. Criterion ≤ 20 % of LLOQ**	**Peak Area [mV*min]**	**Calculated 2439-exNA Conc. ng/mL**	**Acc. Criterion +/-20 % of LLOQ**
AN400.0-23_01_AB02	15, 16	0.0000	BQL	0.0%	0.0368	1.0	100.0%
AN400.0-23_01_AB02	55, 56	0.0000	BQL	0.0%	0.0408	1.1	110.0%
Mean		0.00000	n.a.	0.0%	0.03880	1.05	105.0%
SD (+/-)		0.00000	n.a.		0.00283	0.07	
CV (%)		n.a.	n.a.		7.3%	6.7%	
N		2	2		2	2	

Table 4 Selectivity in K2 EDTA dog plasma

2439-exNA					Blank		QC-LLOQ	
					0.0 ng/mL		1.0 ng/mL	
Run ID	Date	Sex	Lot #	Sample No.	Peak Area [mV*min]	Acc. Criterion ≤ 20 % of LLOQ	Peak Area [mV*min]	Calculated 2439-exNA Conc. ng/mL
AN400.0-24_01_AB02	18.Jul.2024	female	BGL139136	31, 34	0.0000	0.0%	0.0368	1.0
	18.Jul.2024	male	BGL139130	32, 35	0.0000	0.0%	0.0390	1.0
	18.Jul.2024	female	BGL139137	33, 36	0.0000	0.0%	0.0341	0.9

Table 5 Carry-over in K2 EDTA dog plasma

2439-exNA		Cal-Level-2			Cal-Level-7			Carry Over		
		1.0 ng/mL			1,000.0 ng/mL			0.0 ng/mL		
Run ID	Sample No.	Peak Area [mv*min]	Calculated 2439-exNA Conc. ng/mL	Acc. Criterion +/-20 % of Nominal	Peak Area [mv*min]	Calculated 2439-exNA Conc. ng/mL	Acc. Criterion +/-15 % of Nominal	Peak Area [mv*min]	Calculated 2439-exNA Conc. ng/mL	Acc. Criterion ≤ 20 % of LLOQ
AN400.0-23_01_AB02	16, 21, 22	0.0368	1.0	100.0%	43.4117	999.9	100.0%	0.0000	BQL	0.0%
AN400.0-23_01_AB02	56, 61, 62	0.0408	1.1	110.0%	43.1616	994.1	99.4%	0.0000	BQL	0.0%

Table 6 Accuracy and Precision in K2 EDTA dog plasma

2439-exNA		QC-LLOQ		QC-Low		QC-Mid		QC-High	
		1.0 ng/mL		3.0 ng/mL		450.0 ng/mL		900.0 ng/mL	
Run ID	Sample No.	Calculated 2439-exNA Conc. ng/mL	Acc. Criterion +/-20 % of Nominal	Calculated 2439-exNA Conc. ng/mL	Acc. Criterion +/-15 % of Nominal	Calculated 2439-exNA Conc. ng/mL	Acc. Criterion +/-15 % of Nominal	Calculated 2439-exNA Conc. ng/mL	Acc. Criterion +/-15 % of Nominal
AN400.0-24_01_AB02	4, 5, 6			2.9	96.7%	460.6	102.4%	907.0	100.8%
	51, 52, 53			2.8	93.3%	457.5	101.7%	917.6	102.0%
	34, 37, 40, 43	1.0	100.0%	2.9	96.7%	449.2	99.8%	909.0	101.0%
	35, 38, 41, 44	1.0	100.0%	2.9	96.7%	453.8	100.8%	875.2	97.2%
	36, 39, 42, 45	0.9	90.0%	2.8	93.3%	453.5	100.8%	909.3	101.0%
Mean		0.97	96.7%	2.86	95.3%	454.92	101.1%	903.62	100.4%
SD (+/-)		0.06		0.05		4.33		16.40	
CV (%)		6.0%		1.9%		1.0%		1.8%	
N		3		5		5		5	

Table 7 Freeze and thaw and short-term stability in K2 EDTA dog plasma

2439-exNA				QC-Low 3.0 ng/mL		QC-High 900.0 ng/mL	
Run ID	**Date**	**Sample No.**	**Time Point**	**Calculated 2439-exNA Conc. ng/mL**	**Acc. Criterion +/-15 % of Nominal**	**Calculated 2439-exNA Conc. ng/mL**	**Acc. Criterion +/-15 % of Nominal**
AN400.0-24_01_AB02	18.Jul.2024	24, 27	FTS:C1 (-80°C)	3.0	100.0%	901.3	100.1%
	18.Jul.2024	25, 28	STS:	3.1	103.3%	883.9	98.2%
	18.Jul.2024	26, 29	4h on ice	3.2	106.7%	824.5	91.6%
Mean				3.10	103.3%	869.90	96.7%
SD (+/-)				0.10		40.27	
CV (%)				3.2%		4.6%	
N				3		3	

Table 8 **Dilution Integrity in K2 EDTA dog plasma**

2439-exNA		Dilution 1:1,000 500,000.0 ng/mL	
Run ID	**Sample No.**	**Calculated 2439-exNA Conc. ng/mL**	**Acc. Criterion +/-15 % of Nominal**
Dilution reagent: 4 M Urea			
AN400.0-24_01_AB02	47	474,472.8	94.9%
	48	485,876.8	97.2%
	49	473,032.1	94.6%
Mean		477,793.90	95.6%
SD (+/-)		7,036.96	
CV (%)		1.5%	
N		3	

[redacted]

[redacted]

[redacted]

[redacted]

[redacted]

[redacted]

[redacted]

[redacted]

[redacted]

- [redacted]
- [redacted]
- [redacted]

[redacted]

- [redacted]
- [redacted]

[redacted]

- [redacted]

[redacted]

[redacted]

- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]

[redacted]

[redacted]

- [redacted]
- [redacted]
- [redacted]

[redacted]

- [redacted]
- [redacted]

[redacted]

- [redacted]
- [redacted]

[redacted]

- [redacted]
- [redacted]

[redacted]

[redacted]

- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]

[redacted]

- [redacted]
  - [redacted]
  - [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]

[redacted]

[redacted]

[redacted]

[redacted]	[redacted]
[redacted]	[redacted]
[redacted]	[redacted]
[redacted]	[redacted]
[redacted]	[redacted]
[redacted]	[redacted]
[redacted]	[redacted]

[redacted]

[redacted]	[redacted]
[redacted]	[redacted]
[redacted]	[redacted]
[redacted]	[redacted]
[redacted]	[redacted]
[redacted]	[redacted]
[redacted]	[redacted]

[redacted]

[redacted]

[redacted]

[redacted]

[redacted]

- [redacted]
- [redacted]
- [redacted]

[redacted]

[redacted]

- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]
- [redacted]

[redacted]

[redacted]	[redacted]	[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]	[redacted]	[redacted]
[redacted]	[redacted]	[redacted]	[redacted]	[redacted]

6 RECORDS

The following records in addition to the above-mentioned Forms, Master or Spreadsheet Applications are required in this process:

- N/A

7 CHANGE HISTORY

Edition, Section(s)	Change	Rationale
Ed 01	New document	Assay description after the method development
Ed 02	Corrections in sections 2, 4, 5 and Table 1	Editorial changes, correction of dilution reagent, correction of vials (preparation of working solution for stability samples)