

HRV Report for COMGO


Filename	: 紀小姐 202404301434.pdf	Heart Rate	:	86	bpm
Test Date	: 2024/04/30 14:34	SpO2	:	97	%
Device	: CGWA0FFAB8				

【 Measured Data 】


Items	Detection Value(Units)	Results	Standard Value
SDNN	101.2611 (ms)	Lower than standard	141±39 (ms)
RMSSD	138.9801 (ms)	Higher than standard	27±12 (ms)
pNN50	16.2791 (%)	Lower than standard	>50 (%)
VLF	260.9946 (ms²)	Higher than standard	37±15 (ms²)
LF	108.2700 (ms²)	Lower than standard	1170±416 (ms²)
HF	253.7313 (ms²)	Lower than standard	975±203 (ms²)
TP	622.9959 (ms²)	Lower than standard	3466±1018 (ms²)
LF%	17.38%	Lower than standard	54±4%
HF%	40.73%	Higher than standard	29±3%
LF/HF	0.43	Lower than standard	1.5±0.5

【 Measurement Charts 】

LF/HF Index Analysis

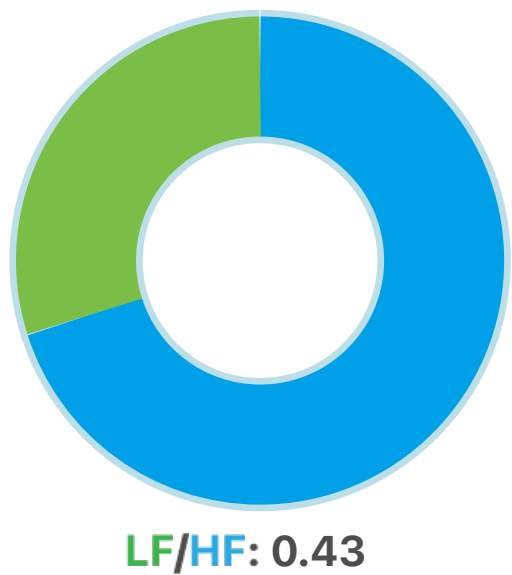

SDNN Overall Assessment

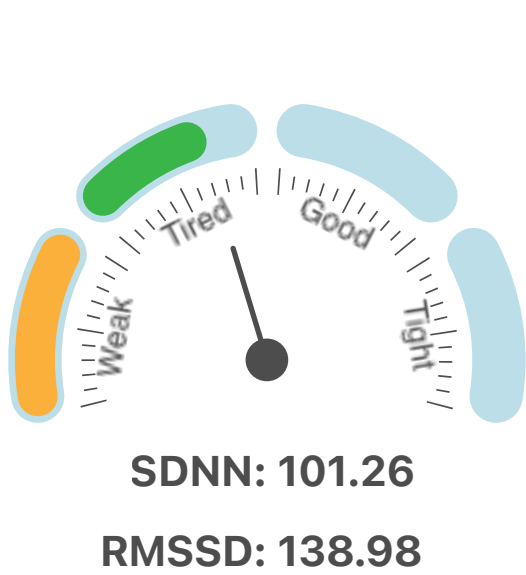

HRV Report for COMGO

Filename : 紀小姐 202404301434.pdf

Heart Rate : 86 bpm


Test Date : 2024/04/30 14:34

SpO2 : 97 %


Device : CGWA0FFAB8

【 Measurement Charts 】

Active Schematic Diagram

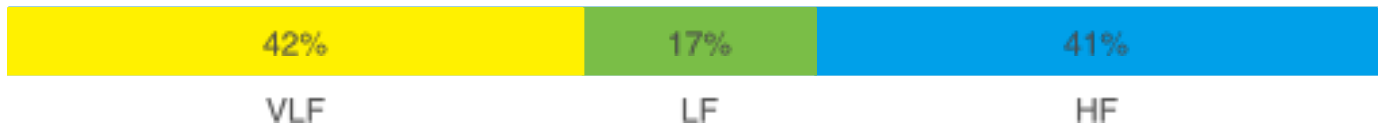


RRI Scatter Diagram

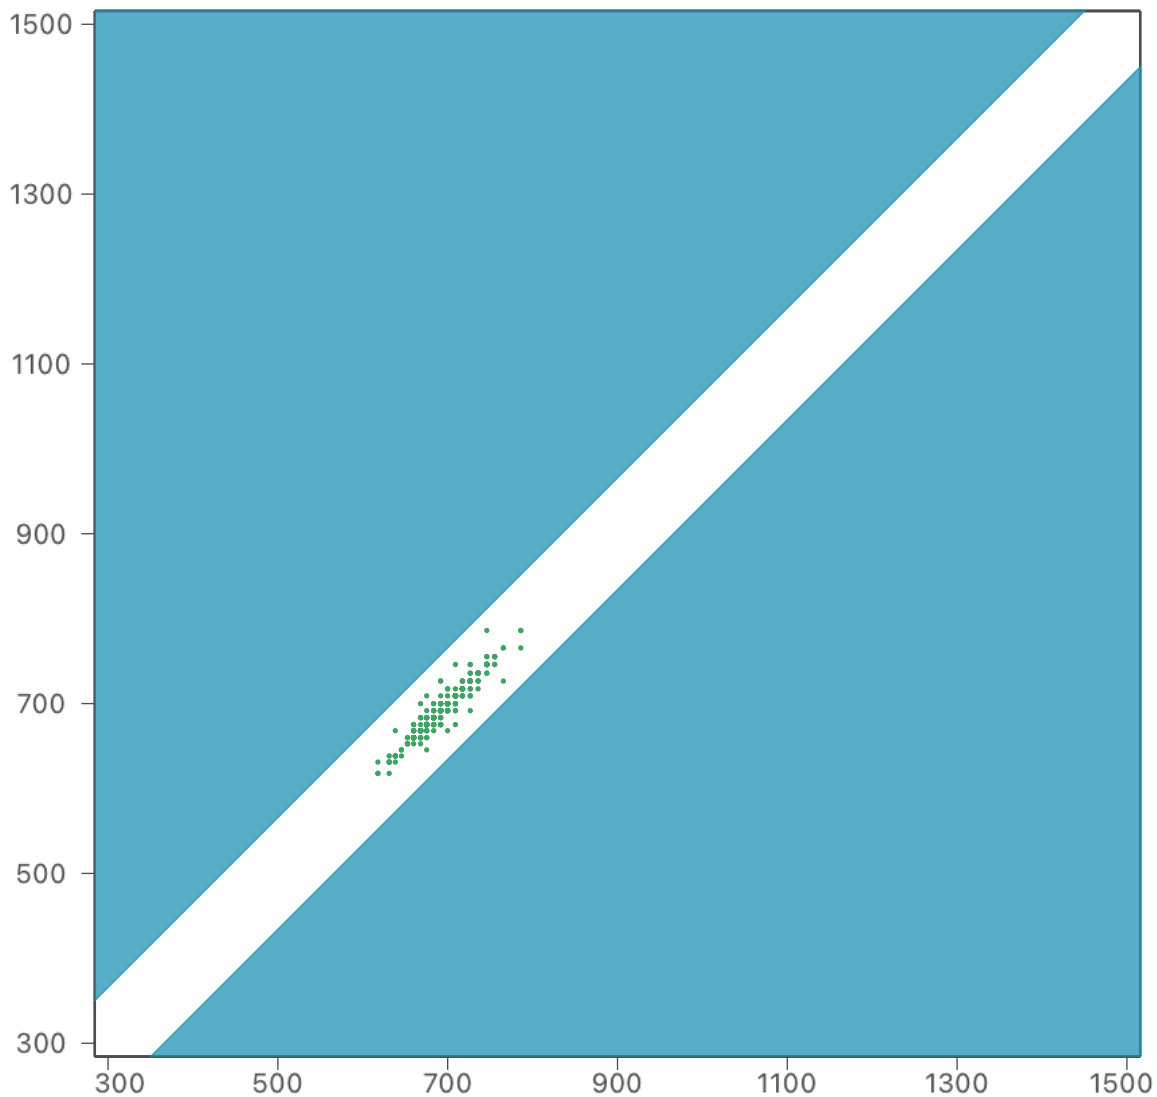

ECG Report for COMGO

Filename	: 紀小姐 202404301434.pdf	Heart Rate	:	86	bpm
Test Date	: 2024/04/30 14:34	SpO2	:	97	%
Device	: CGWA0FFAB8				

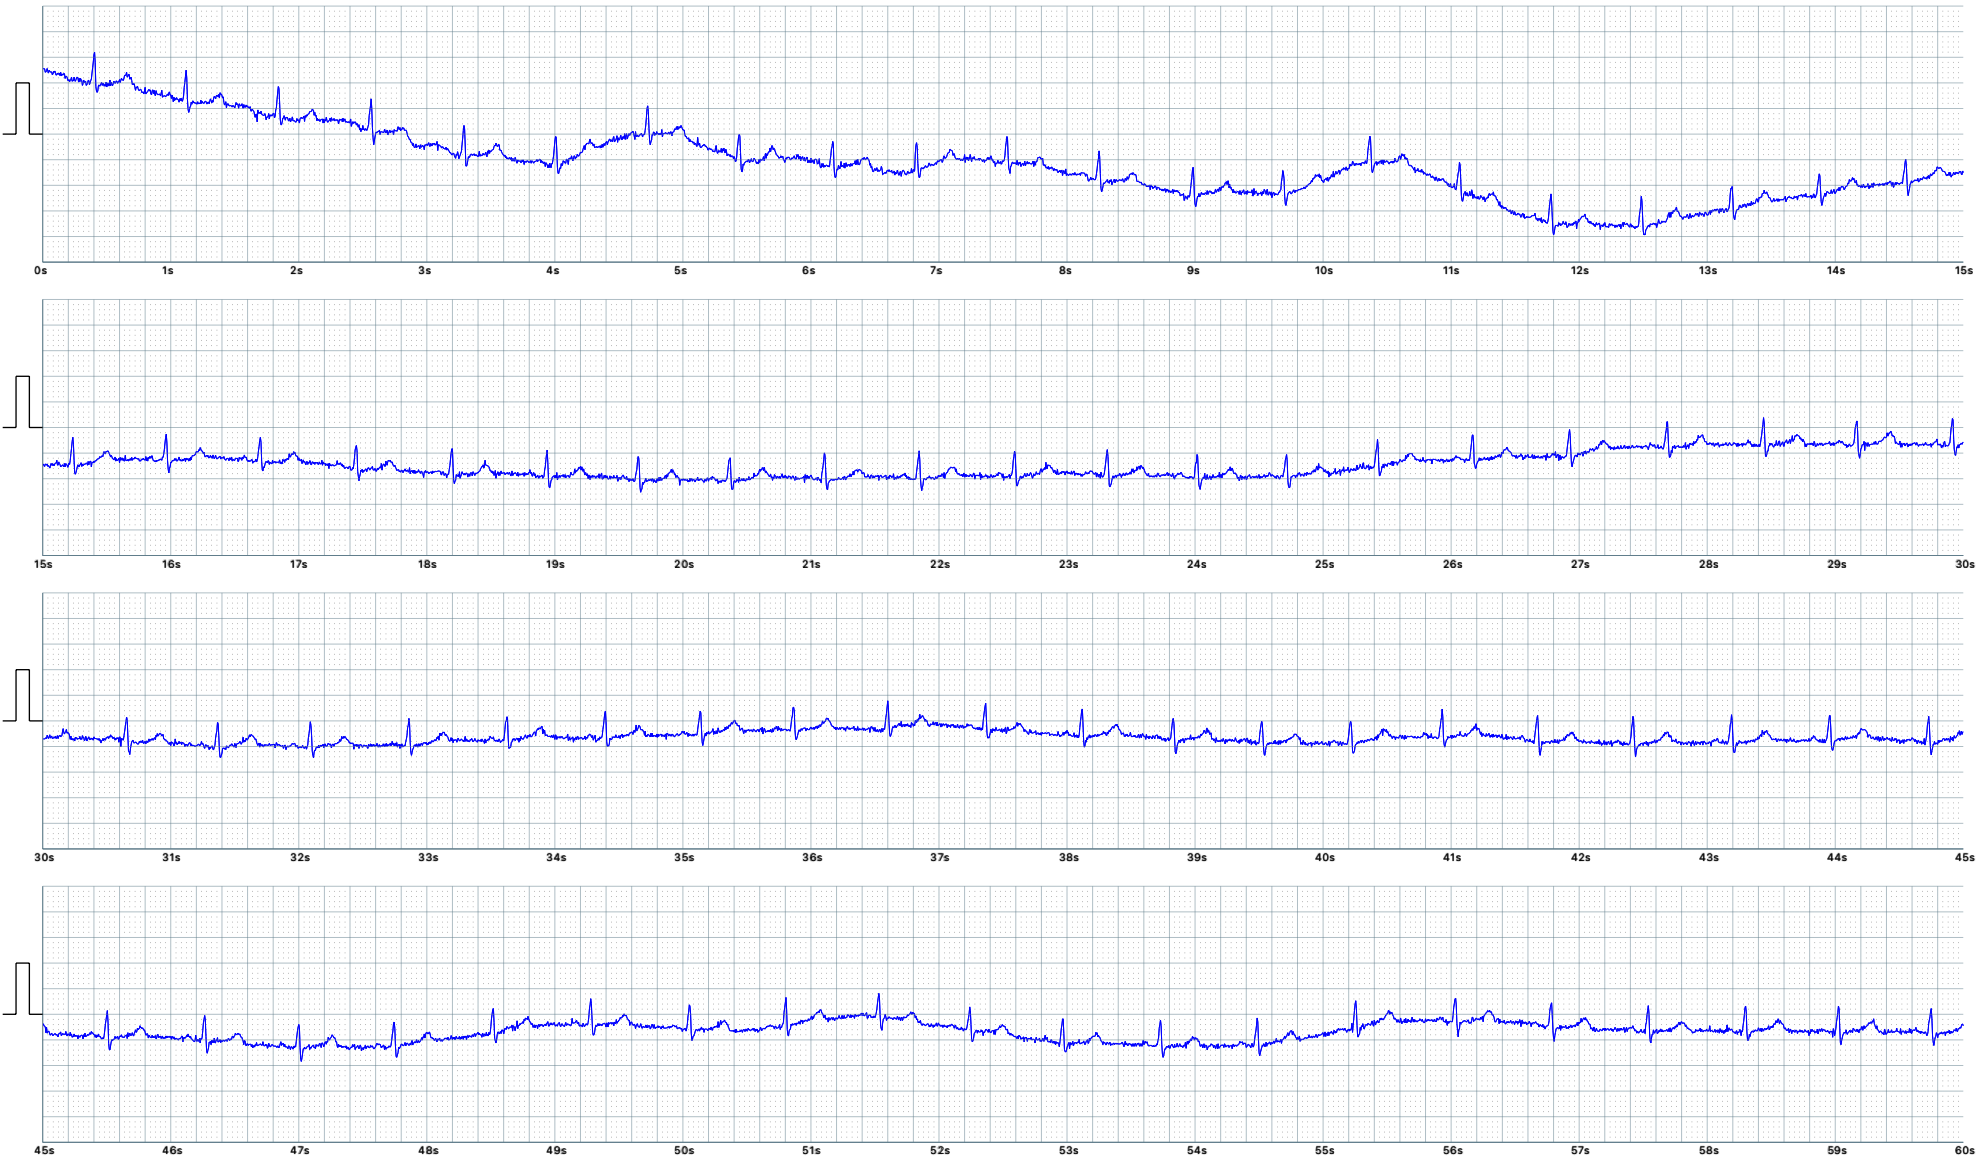


ECG Report for COMGO

Filename	: 紀小姐 202404301434.pdf	Heart Rate	:	86	bpm
Test Date	: 2024/04/30 14:34	SpO2	:	97	%
Device	: CGWA0FFAB8				




ECG Report for COMGO

Filename	: 紀小姐 202404301434.pdf	Heart Rate	:	86	bpm
Test Date	: 2024/04/30 14:34	SpO2	:	97	%
Device	: CGWA0FFAB8				

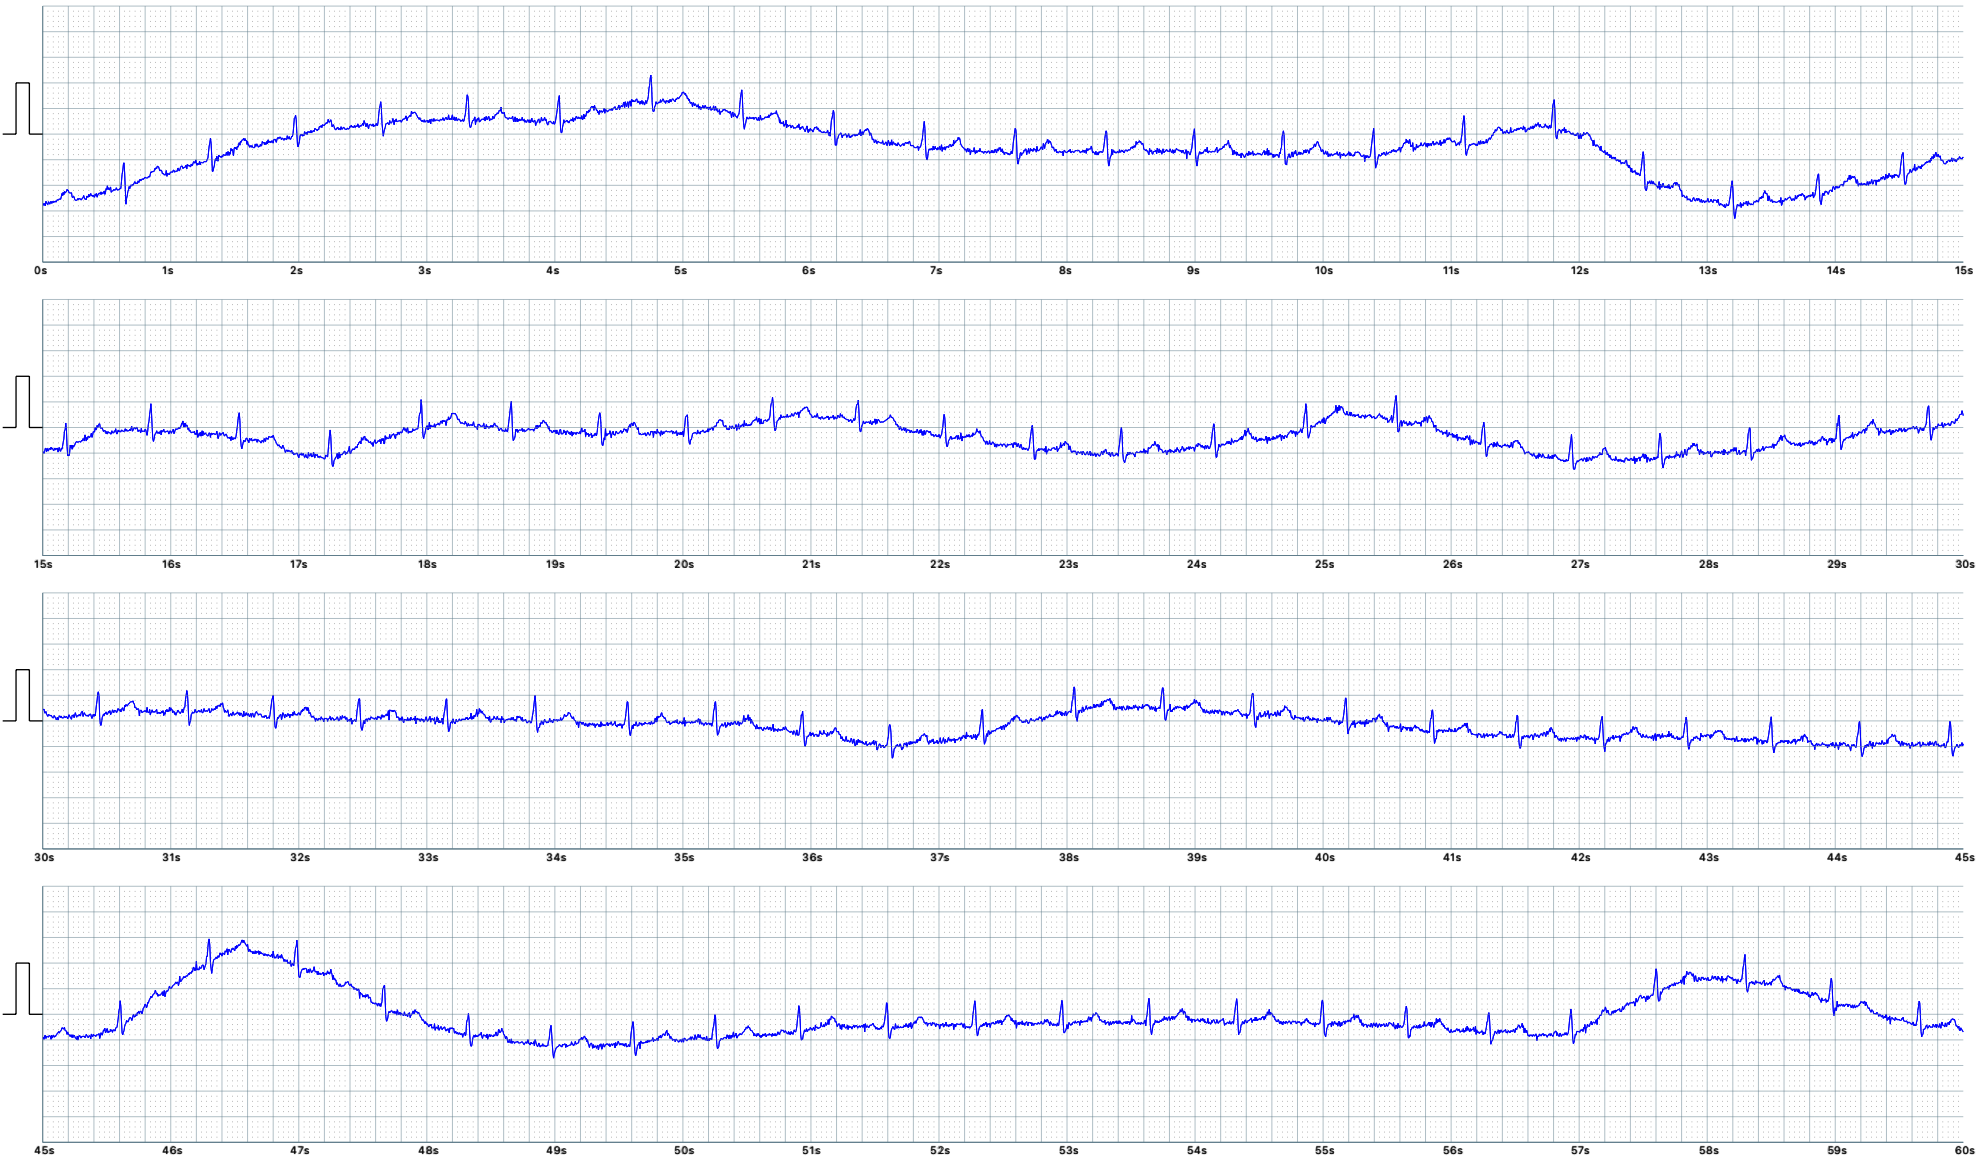

ECG Report for COMGO

Filename	: 紀小姐 202404301434.pdf	Heart Rate	:	86	bpm
Test Date	: 2024/04/30 14:34	SpO2	:	97	%
Device	: CGWA0FFAB8				

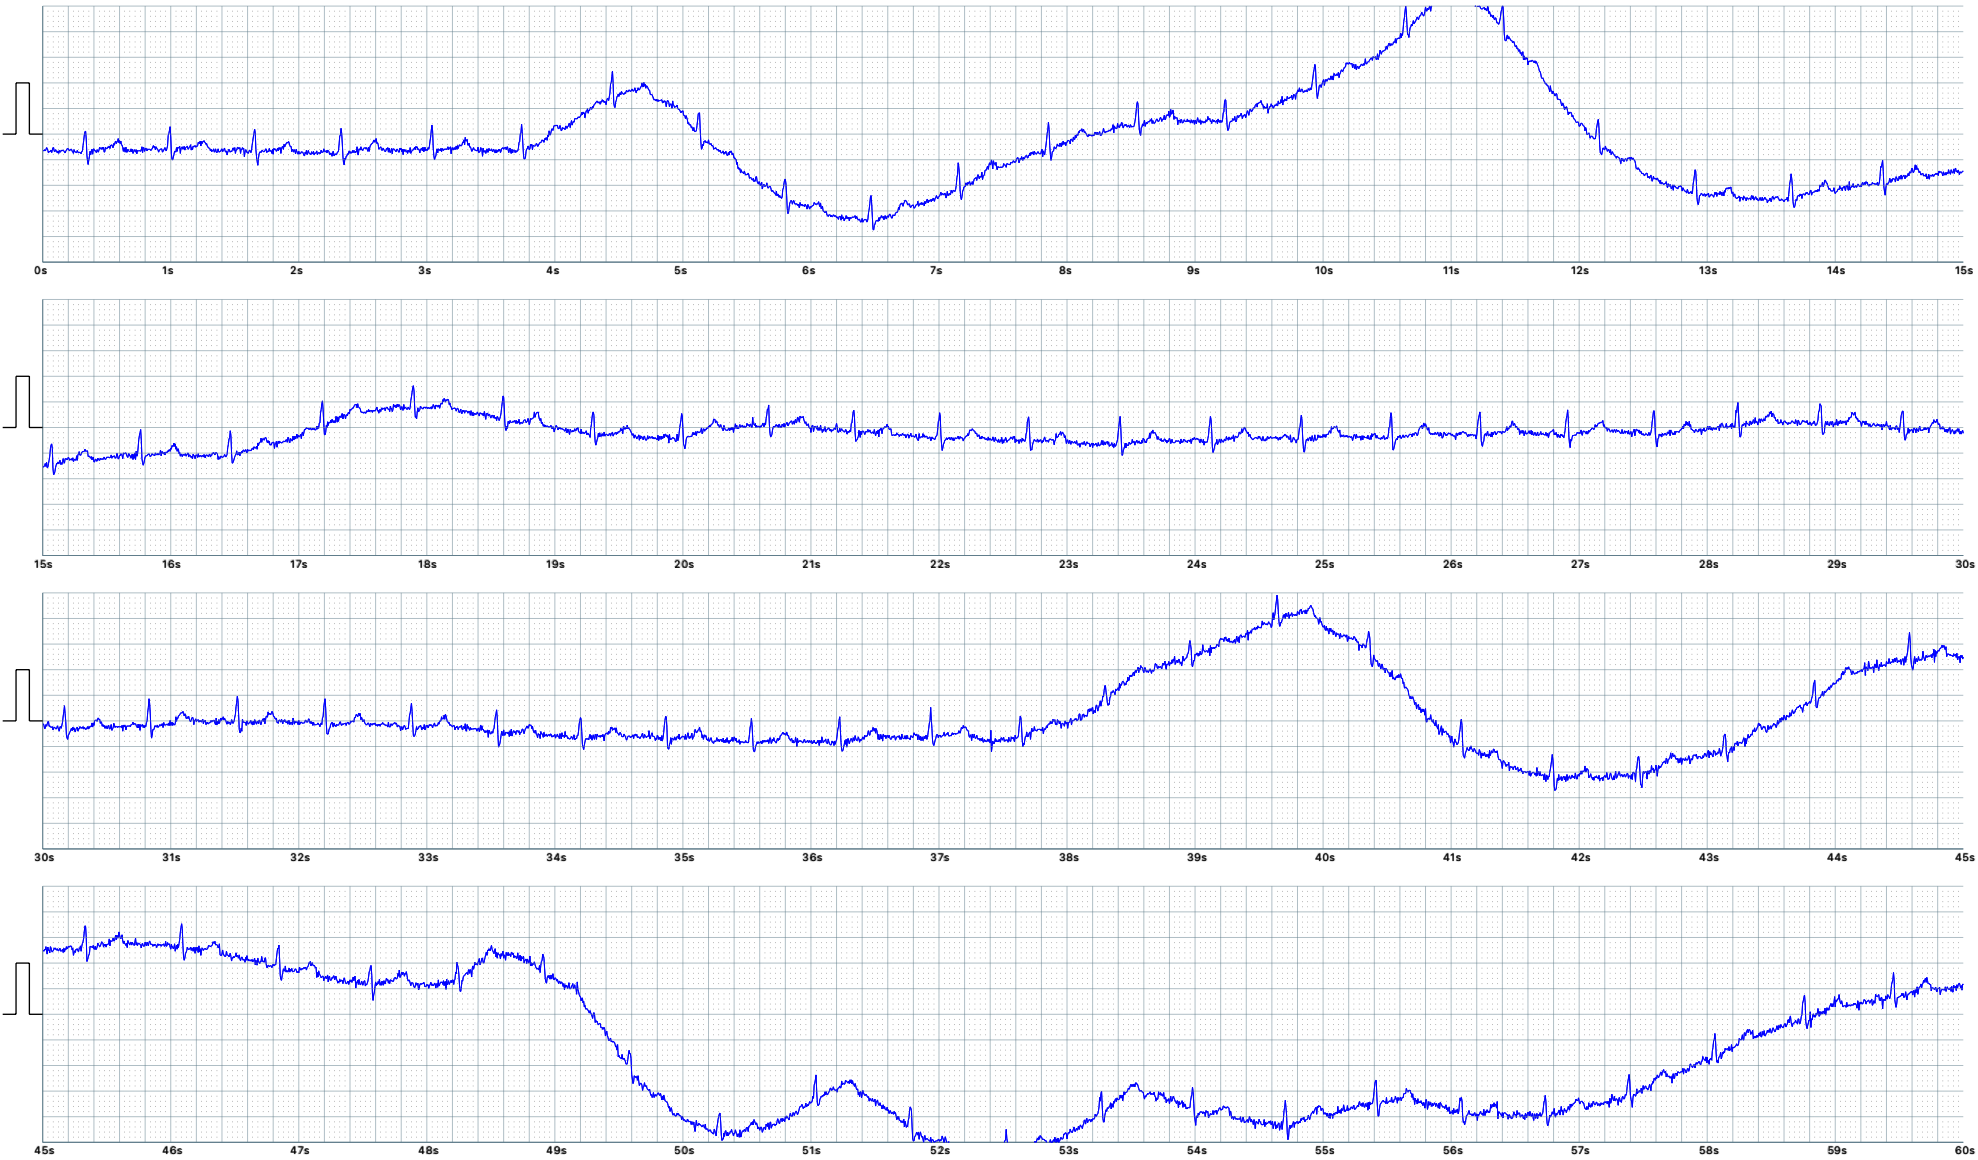

ECG Report for COMGO

Filename	: 紀小姐 202404301434.pdf	Heart Rate	:	86	bpm
Test Date	: 2024/04/30 14:34	SpO2	:	97	%
Device	: CGWA0FFAB8				

