





HP HEWLETT PACKARD SPECTRUM ANALYZER 8591E
INSTRUMENT STATE
PRESET CONFIG CAL AUX CTRL
(LOCAL)
MODE SAVE RECALL MEAS/USER
FREQUENCY

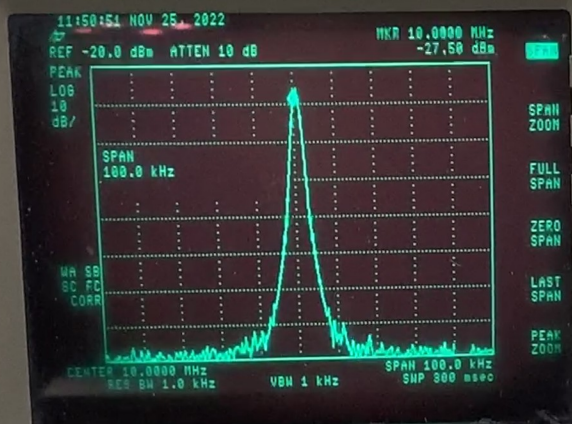

10 MHz
AM MOD 1 kHz
~~Rf~~ 10 kHz SPAN
100 kHz SPAN
AM 699.9 Hz

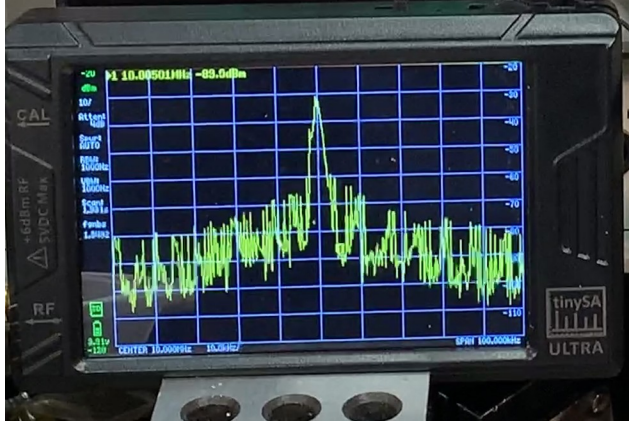

INPUT 50 Ω
kHz - 1.8 GHz
25 VDC

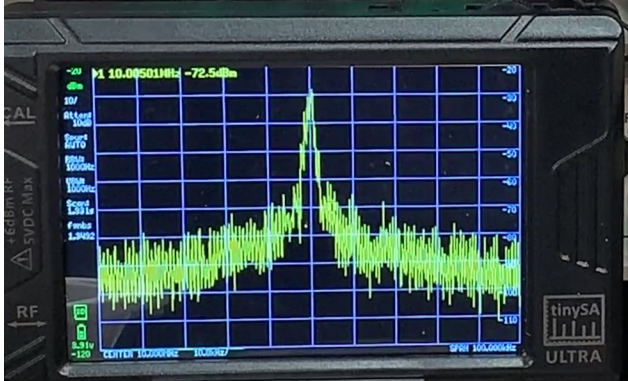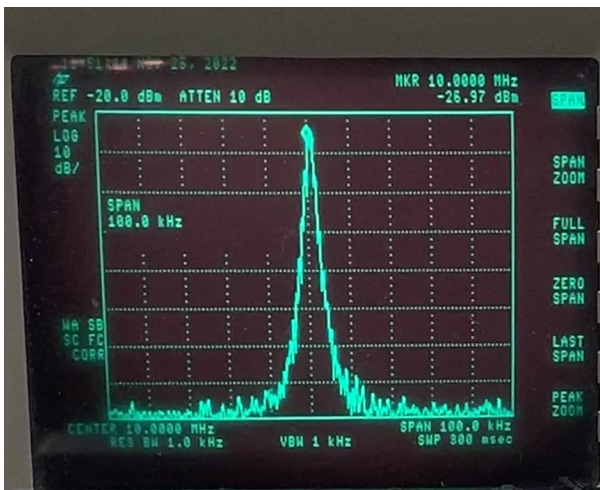

8591E
 PRESET CONFIG CAL
 (LOCAL)
 FREQUENCY MODE SAVE RECALL MEAS USE

10 MHz
 AM MOD. 1 kHz
~~RB~~ 10 kHz SPAN
 100 kHz SPAN
 AM 699.9 Hz
 399.9 Hz

