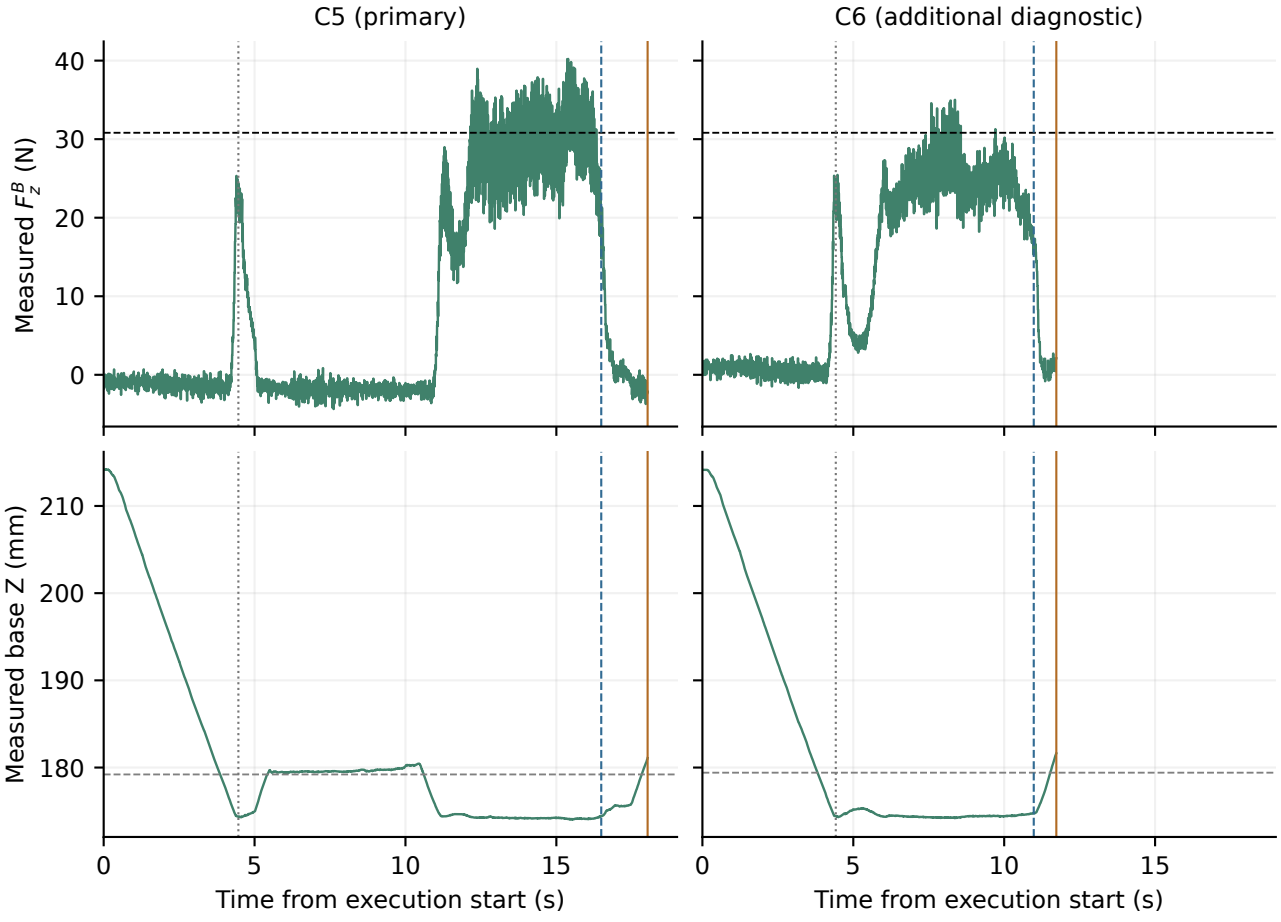

C5 (primary)
C6 (additional diagnostic)
Measured F_z^B (N)
40
30
20
10
0
Measured base Z (mm)
210
200
190
180
0
5
10
15
Time from execution start (s)
Time from execution start (s)