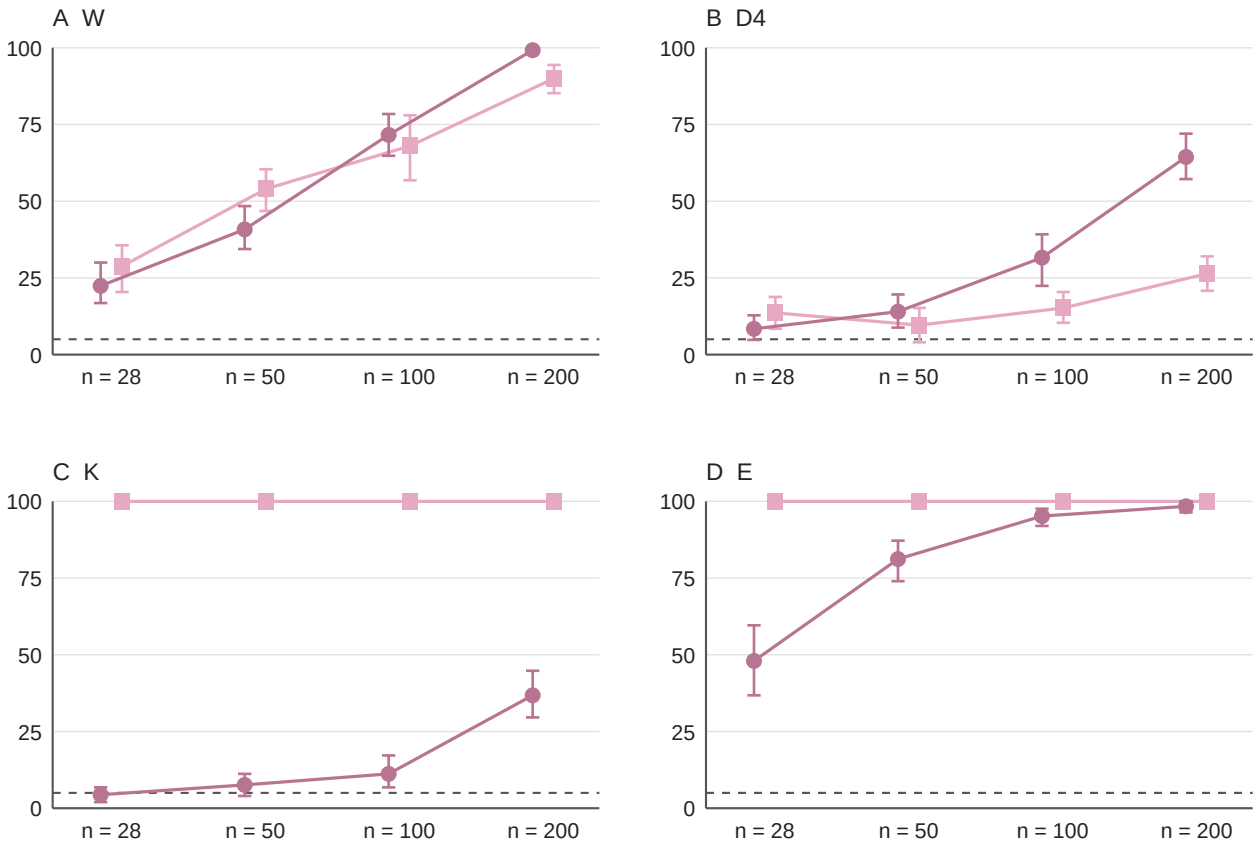

Calibrated detection (%); two-stage bootstrap 95% intervals of the cell giving the maximum; dashed line 5%.