SurgiTrack

User manual

Surgical instrument and Set traceability

Version 0.30.0 · 11/10/2026 · www.surgitrack.eu

Contents

1. Getting started
2. Setting up the hospital
3. Set / instrument card
4. Overview
5. Department Sets & Instruments
6. Sterilization
7. Issues
8. Replacements & orders
9. Sterile expiry
10. Instrument Sets
11. Instruments
12. Standalone instruments in use
13. Instrument Stock
14. Devices
15. Traceability
16. Reports
17. History
18. Users & departments
19. SurgiTrack Studio
20. Bulk import
21. Name check
22. Recycle bin

Glossary

Roles

Hospital admin	Users, departments, Studio and every screen of the hospital.
Sterilization supervisor	Everything a Sterilization user does, plus registering Sets and instruments, composition, Service.
Sterilization user	Receipt, check and composition, sterilizer, release, delivery.
Department user	Their department’s Sets and instruments: dispatch, receipt, count, problem reports.
Viewer	Sees the whole hospital without changing anything.

1

Getting started

Your first sign-in, what you see on screen and where to ask for help.

Who it is for: All users

Step by step

1. Keep the username shown after you sign up.
2. After the approval email, sign in with it and your password.
3. Open Help (the book icon, top right) on any screen you do not know.

Account

Only your hospital administrator opens accounts. If you got an invitation or a signup link, you fill in your first name, last name, department and password and see your username at once. If you signed up with the hospital’s shared link, first press "Confirm email" in the email you receive. You can sign in as soon as the administrator approves.

Several devices

You can work from several computers and tablets at once. Each screen takes what the others saved or deleted at once (live sync); when the live connection is not available it checks every 20 seconds and as soon as you come back to the window. Your own changes are saved first. If two devices change the same Set or instrument at the same time, both changes are kept when they concern different fields; when they concern the same field, the one saved first is kept and a "Changed on another device at the same time" message names the field. If the network drops, a "No network connection" notice appears at the bottom of the screen: what you record is kept on this device and saved as soon as the connection is back, even if the page closes (open it again with the same user). The device keeps a copy of the hospital’s data, so the app opens at once and fetches only what changed; the copy is wiped at sign-out and not used when older than a day. The top bar shows the state: "Live" (green) or "Sync" (grey, checking every 20 seconds), "Saving · N changes" while saving and "Not saved · retrying" if something failed; hovering over it shows the time of the last contact with the server. On a tablet the lists keep their key columns: long names take two lines, an issue’s note shows under the item and each History entry shows the action and the user on a second line; on a phone each movement is a card.

First sign-in

Once approved you get an "Your access to SurgiTrack was approved" email with your username (e.g. GN1234) and your role. Sign in with your username (or email) and the password you set when signing up: at least 8 characters, with a letter and a number. If the administrator created the account, press "Set password" in the email.

Your screen

The menu on the left shows only what your role allows, in groups: Daily work, Equipment, Insight, Administration. After signing in the Overview opens if your menu has it; otherwise the first entry of

your menu. In the scan field of the top bar, scan or type a barcode and the Set or instrument opens at once. Top right: language (EL/EN), Help, accessibility (text size, contrast) and notifications.

Unsaved changes

If you leave a page with details you have not saved (a new Set or instrument, editing a card's details, role permissions), the app first asks "Some changes are not saved". "Stay" is the default; "Leave without saving" discards them. The same goes for signing out; if you close or reload the tab, the browser asks.

Forgotten password

On the sign-in page press "Forgot password" and enter your email; you will get a link to a new password. After many wrong attempts sign-in locks for 15 minutes. The administrator can also send you a password change link.

Checks

- Do you see the right department and role? If not, tell the hospital administrator.
- Do not share your password: every movement is recorded under your name.

> **Tip.** Help always opens on the page of the screen you are on. For access, password or permissions ask the hospital administrator; for a technical problem see "Support".

2

Setting up the hospital

The administrator's guide: the steps in order, from the first sign-in to the first day of real use.

Who it is for: Hospital administrator

Step by step

1. Sign in as administrator from the Exeltos invitation.
2. Departments, libraries and sterilization flow.
3. Bulk import of instruments and Sets, then Name check.
4. Staff invitations and approvals.
5. Printer, scanners, labels.
6. Training in the Demo and a start day.

Your account

Exeltos creates your hospital and sends you an administrator invitation. From the email you set a password and sign in. If the hospital is on a trial, the app locks when it ends until activation.

Departments and libraries

In Users & departments → Departments add every department (Operating theatre, ICU, Central Sterilization...). In Hospital settings → Libraries check specialties, manufacturers, sterilizers, washers and color markers; in Sterilization Flow the stages.

Instruments and Sets

Prepare the Excel file with the "Excel template" of Bulk import (Instruments or Sets → "Bulk import"): one row per instrument, the Set name on each of its rows. Check the preview and import. Then run the "Name check" so each code has one name.

Staff

In Users & departments → Users → "Add user": "Invite a person" one by one (email or link), "Hospital signup link" for many, or "From a CSV file". First the Sterilization supervisor, then Sterilization and the departments. Approve the requests (orange) with the right role and department.

Equipment

A barcode label printer in Sterilization, a barcode scanner (USB or Bluetooth, works as a keyboard) at every handover point, a computer or tablet with Chrome or Edge. If sterilizers will be connected, see "Devices". For the IT department: the app talks only to its own site and to Supabase (https and wss on *.supabase.co), loads nothing from third parties and does not open inside other sites; the site’s security headers enforce this.

Training and go-live

Train staff in the Demo: the same screens with test data; you turn Demo access on per user in Users & departments. Label the Sets and instruments, set a start day and from that day every handover and receipt is done by scanning.

Checks

- Every department exists and is active.
- Sets have the right composition and department; the Name check shows nothing pending.
- Every user has a role and department; at least one Sterilization supervisor.
- The printer prints a label and the scanner opens the Set from the top bar.
- One test dispatch and receipt was completed by a department and Sterilization.

> **Tip.** For help with any step, write to Exeltos at info@exeltos.com (see "Support").

3


Set / instrument card

Everything about one Set or instrument: details, composition, history, photos, uses and actions.

Who it is for: All users (actions depend on the role)

Step by step

1. Check the state and remaining uses.
2. See the history for the last movement.
3. Use the action you need from the top right.

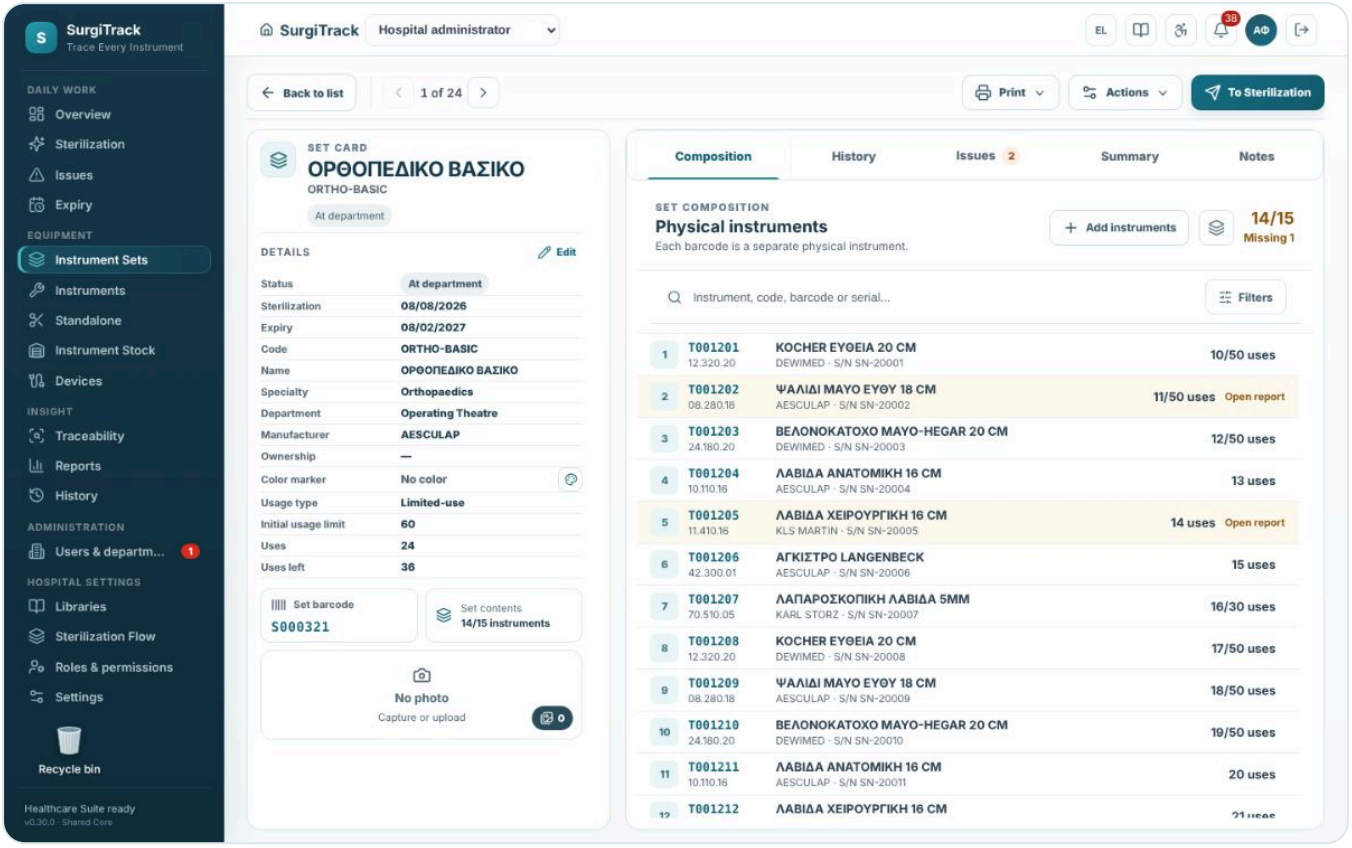

Details

On the left: barcode, code, department, specialty, manufacturer, ownership, color marker, sterilization date and expiry. Users with the right can change them with "Edit".

Uses and limits

Limited-use instruments show their remaining uses. Each dispatch after use takes one use; at zero the instrument is taken out of use automatically.

History and photos

The History, Issues, Summary and Notes tabs (and Composition on Sets) show every movement and problem report. Photos open from the details card ("Open photos").

Actions

Depending on the role: send to Sterilization, print the barcode and, under "Actions", report a problem, manage (department, Service, loss; for instruments also Set or Stock, for Sets also return) and "New barcode" when the label is lost or worn. A management action can be undone from its notice for a few seconds; the history keeps the undo too.

Previous and next card

When you open a card from a list (Sets, Instruments, Standalone, Stock), "3 of 24" with ‹ › arrows shows next to "Back to list". You move to the previous or next card in the list's order and filters, also with Alt+← / Alt+→ on the keyboard. "Back to list" always returns to the list.

4


Overview

The whole hospital at a glance: Sets, instruments, sterilization flow, issues and usage limits.

Who it is for: Hospital administrator and Sterilization supervisor

Step by step

1. Start with the orange indicators: they need attention.
2. Click an indicator to see exactly which records it counts.
3. Check the latest movements for recent activity.

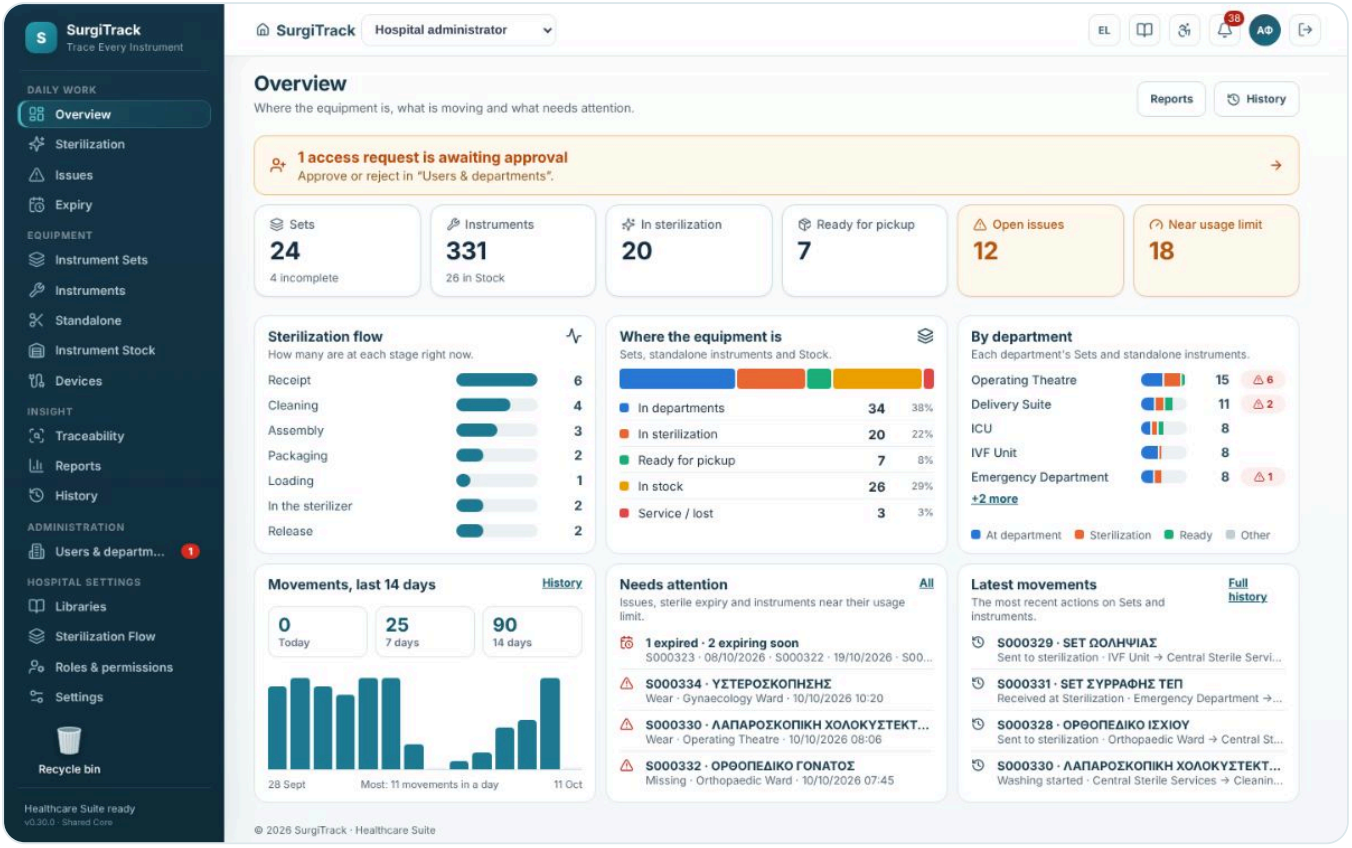

Indicators (KPIs)

Every indicator at the top is a link. It opens the matching list with its filters already applied, e.g. "Near usage limit" opens Instruments filtered to "Few uses left".

By department

One bar per department shows where its equipment is (at the department, in sterilization, ready, other) and its open issues. The five busiest departments show; "+N more" shows the rest. Clicking a department opens its page as the department itself sees it.

Sterilization flow

The bars show how many items are at each stage. Clicking a stage opens Sterilization on that tab.

The other cards

"Where the equipment is" counts Sets, standalone instruments and Stock: in departments, in sterilization, ready for pickup, in stock, service / lost. "Movements, last 14 days" shows movements per day, with totals for today, 7 and 14 days. "Needs attention" gathers issues, sterile expiry and instruments near their usage limit; each line opens the matching list.

> **Tip.** The Overview is where the day starts: anything red or orange needs action today.

5


Department Sets & Instruments

The department's Sets and standalone instruments, and sending them electronically to Central Sterilization.

Who it is for: Department users

Step by step

1. Find the Set or instrument (search or scan the barcode).
2. Press "Send to Sterilization".
3. Enter the patient code where asked and confirm.
4. When it shows "Ready for pickup", collect it from Sterilization, signing with your user code and password.

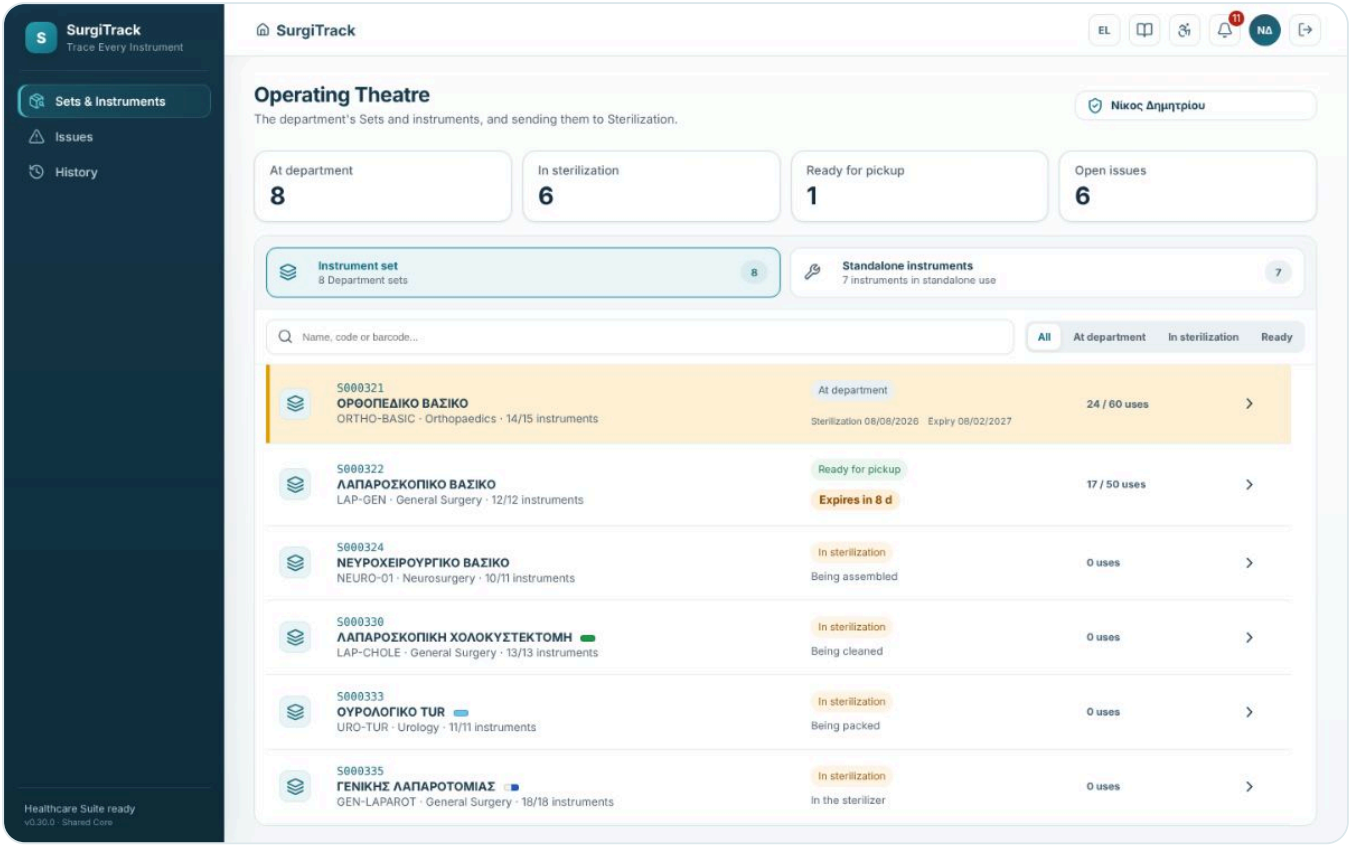

What I see

The two tabs list your Sets and standalone instruments. The indicators above filter the list: "At department", "In sterilization" (on the way to or inside Sterilization), "Ready for pickup", and "Open issues" opens the department's Issues. Whatever is in Sterilization shows "In sterilization" with the stage under it (e.g. "Composition", "Sterilizer"). Uses read "24 / 60 uses".

Surgical count

In operating theatres (Hospital settings → Libraries → Departments → "Count") "Send to Sterilization" asks for the count first. The "Count" button opens the form: Sterilization's part on top (composition,

release, sterilization and expiry, cycle), the instruments below with "Sent" and "Counted". Enter the patient code, tick or scan each instrument or press "All present", then "Sign the count" (name and time). Sending is then enabled. If instruments are missing, an issue opens and Sterilization sees it at Receipt. The form prints blank or signed, also from the Set's Print menu.

Send to Sterilization

After use, press "Send to Sterilization". The patient code is optional unless the Set or instrument has limited uses.

Instruments with a usage limit

For limited multi-use instruments (e.g. robotic), sending requires a patient code and confirming it was used: one use is recorded and the uses left are shown. When no uses are left the instrument is taken out of use automatically.

Report a problem

If an instrument is missing or damaged, open the Set, press "Actions" → "Report a problem" and describe it. Sterilization sees it under Issues.

Checks

- The patient code contains no patient name.
- The use was recorded for limited-use instruments.

> **Tip.** Scan the barcode instead of searching by name: it is faster and avoids mistakes.

6


Sterilization

The Central Sterilization flow: receipt, washing, preparation, packaging, sterilizer load, load release, storage and delivery.

Who it is for: Sterilization users and supervisor

Step by step

1. Open the tab of your stage.
2. Scan or select the item.
3. Complete the stage check and move it on to the next stage.

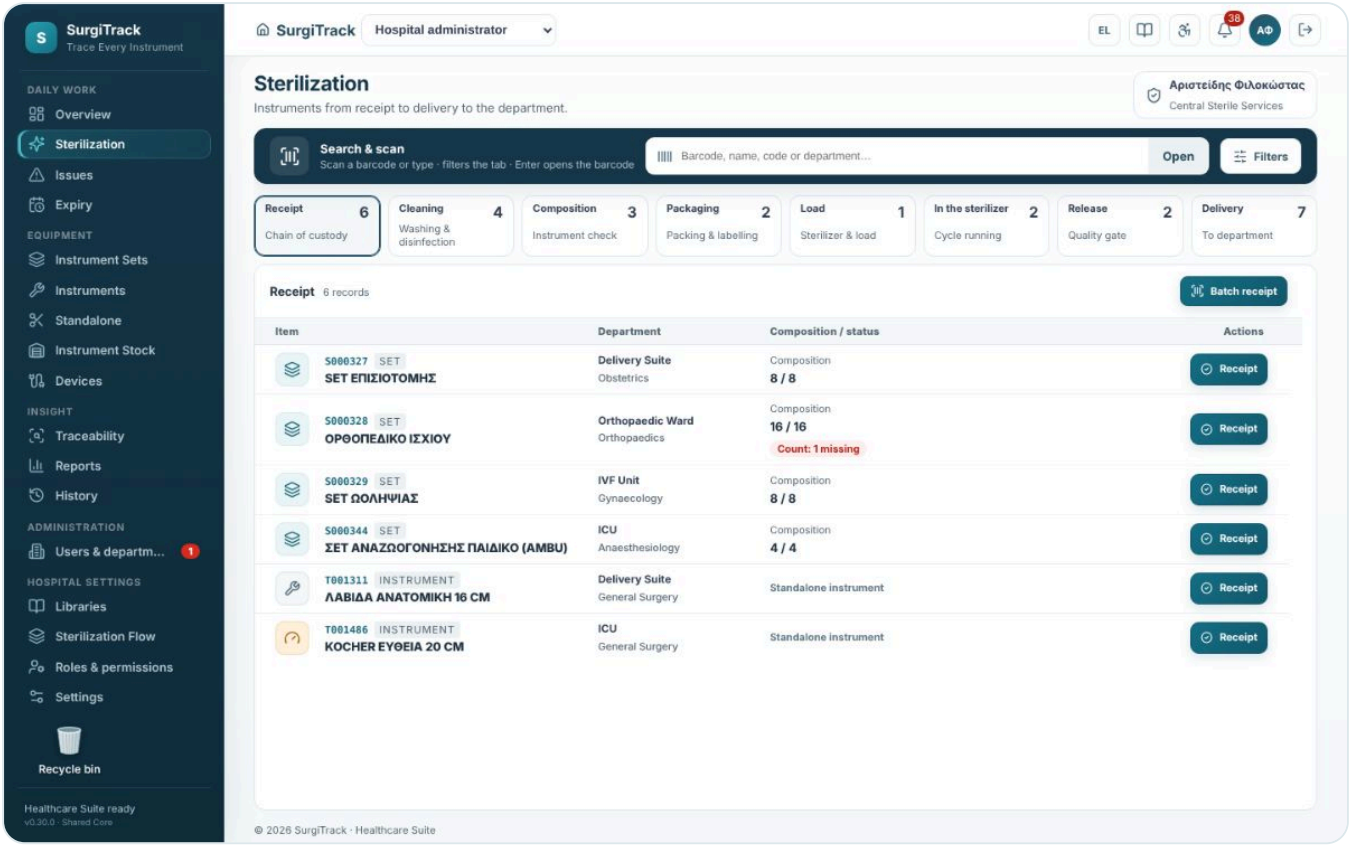

Stage tabs

Each tab is a stage, with a word under it for what happens there (e.g. Composition "Instrument check", Packaging "Labelling", Release "Quality gate"). Its number shows how many are waiting and the list has the same title as the tab (at Delivery: "Ready for delivery"). Stages disabled in Studio are not shown, unless they still hold items. The blue "Search & scan" bar filters the tab as you type; scanning a barcode and pressing Enter opens the item in its stage. The Filters (department, specialty, Sets or instruments) sit next to it.

Physical receipt

In "Receipt" scan the Set and declare any visible deviation. You are recorded automatically as the receiver; the department person handing it over signs with their user code and password. Deviations

(missing, damaged) create an issue.

Washing

In "Washing" washing is recorded with a washer load: "Washer load" above the list for several at once, or on the row for one. Pick the washer / disinfector, the cycle number and the program and press "Complete load". "Without a washer" shows only when the washing policy in Hospital settings → Sterilization Flow allows it.

Issues during Composition

Whatever needs action shows as a coloured row in the Set's instrument list, with a "Handle" button. An instrument with damage or another issue: replace it, send it to Service or Stock, or move it to another Set. A missing instrument ("Missing" row): "Cover the shortage" with an instrument from Stock, another Set or a standalone one, "Report", or "Keep as is" so the Set goes on with fewer instruments (the same as "Accept the recorded shortage" in the composition notice). An issue on the Set itself: "Fixed" with a note for the history, or "Keep as is" (the issue stays open).

Delivery to the department

In "Delivery" you are recorded automatically as the person handing over. The department person collecting signs with their user code and password on the same screen; without the signature the delivery cannot be completed.

Sterile shelf life

At "Packaging" (packaging check) you choose a shelf life of 2, 3 or 6 months for each Set or instrument; the hospital default is suggested. It counts from the release and the expiry date shows on its card. If the hospital has no packaging stage, the shelf life is chosen at preparation.

Sterilizer load

In the "Load" tab every ready Set and instrument is already ticked; untick what does not go in and press one button, "Sterilizer load". Pick the sterilizer from the hospital list, the cycle number and the program, and declare which indicators are in the load (chemical, biological). No indicator result is given here. "Start cycle" puts the load in the sterilizer. If you pick a cycle from a connected device, that cycle has already ended and the load goes straight to Release; if the device reported a failure, it goes back to reprocessing.

In the sterilizer

The "In the sterilizer" tab shows the loads being sterilized now: sterilizer, cycle, program, who loaded it and when, and the items. They are locked; nobody can change them. When the cycle ends press "End of cycle": the load moves to Release and the screen goes there (Release is always required); "Cycle failed" sends the whole load back to reprocessing.

Load release

In the "Release" tab one button, "Release load", opens the loads that are waiting; pick the load and sterilizer. Confirm the physical parameters and the packaging and record the result of the indicators placed in the load. One passed indicator is enough, unless the unit requires a specific one. A failed

indicator or "Do not release" sends the whole load back to reprocessing. Closing the release moves the items to "Delivery" to be handed to the department (or first to Storage, if the hospital uses it).

Release form

The "Form" button (in "In the sterilizer", in Release and in the recently released loads) prints the load's A4 form: load type, sterilizer, cycle, program, shelf life, the indicators with a place to stick their strip, the checks, the items with their expiry, the decision and the approval with the user's details and signature. From "In the sterilizer" it prints blank to fill in; from Release it prints filled in with what you have ticked there (indicators, checks) and the signed-in user's details; after the release it prints with the recorded decision. Items show the sterilization date (STERILE) and the expiry date (hourglass); when no shelf life is set, the hospital default is shown.

Printing

The composition sheet (A4, with a check column and signatures) and the barcode label print from the preparation step. The label comes in three sizes (50×25, 70×35, 100×50 mm) with a SurgiTrack, logo, custom text or no header; the administrator sets the hospital default.

Checks

- The Set composition was checked before packaging.
- The load was recorded with sterilizer, cycle number and indicators.
- At release at least one indicator was recorded as passed.

> **Tip.** An item under an active recall or with no uses left cannot circulate: the app stops it.

7


Issues

Missing, damaged, faulty or lost items that need handling.

Who it is for: All users

Step by step

1. Press the "Open" card (or "Over 7 days" for those waiting long).
2. Open the issue and see its note and photos.
3. Resolve and close it.

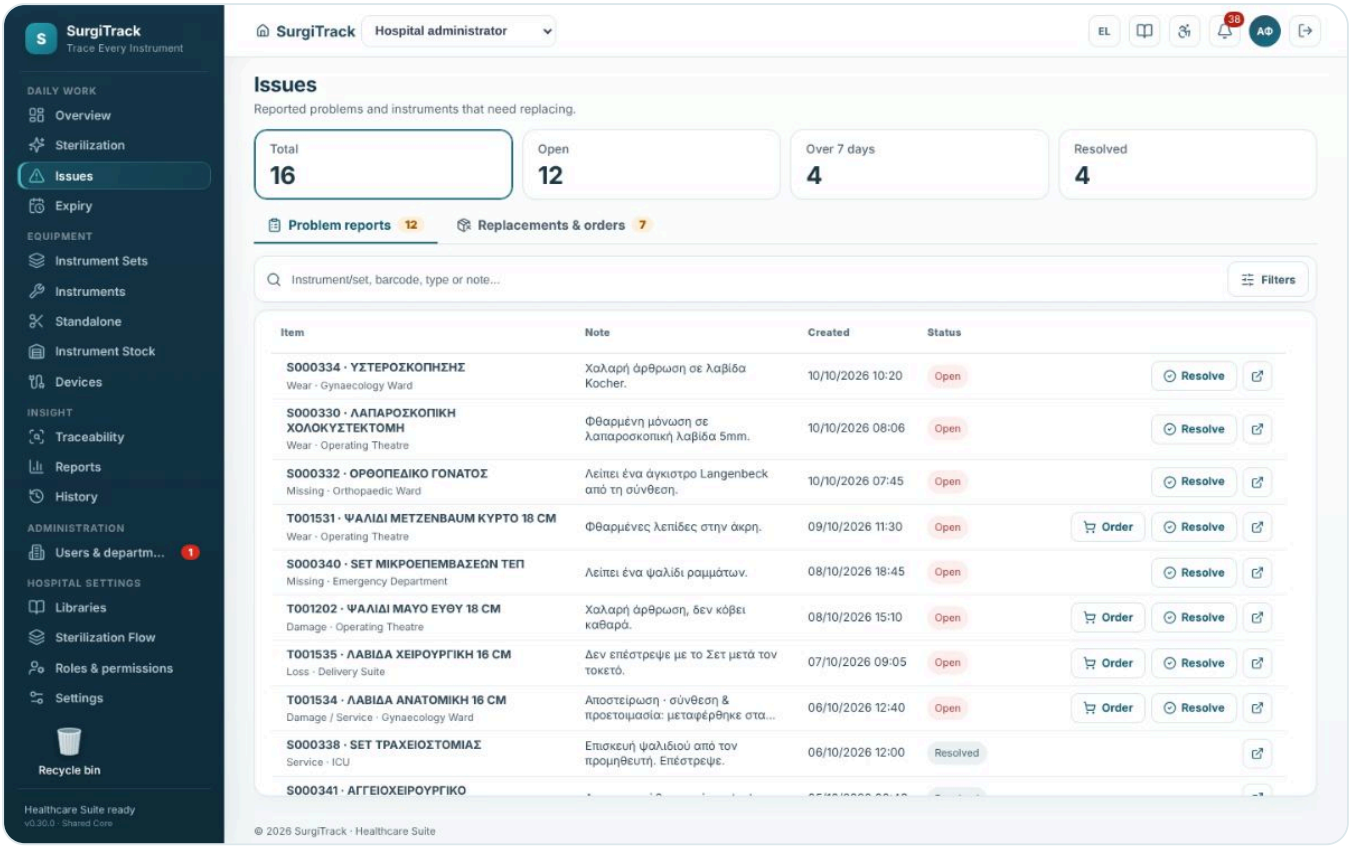

Creating

An issue is created from a Set or instrument card ("Actions" → "Report a problem") or automatically from a receipt deviation. Sterilization declares a loss or a Service send-off in "Actions" → "Manage", because they change the state; a department reports a loss and Sterilization confirms it.

Closing

Sterilization resolves the issue (replacement, service, return) and closes it. Everything is recorded in History.

Two tabs

Sterilization and the Administrator see two tabs: "Problem reports" (what was reported) and "Replacements & orders" (the instruments to replace, from Stock or with a purchase order). On a phone they read "Reports" and "Replacements".

Numbers

Above the list of reports, four cards: Total, Open, Over 7 days (open ones waiting long) and Resolved. They count within the department, type and search you chose; pressing one shows only those in the list. In "Filters" the same filter is called "Open over 7 days".

8


Replacements & orders

Instruments in Service, damaged or worn, lost or out of use: replace from Stock in one click when it holds the same instrument, otherwise record a purchase order.

Who it is for: Sterilization and Administrator

Step by step

1. Press "Need replacement", "In Stock" or "Not in Stock", or filter by reason and department.
2. Replace from Stock what it holds.
3. Record a purchase order for the rest and print it.
4. When they arrive, "Receive into Stock": the new instruments enter Stock with their own barcodes.

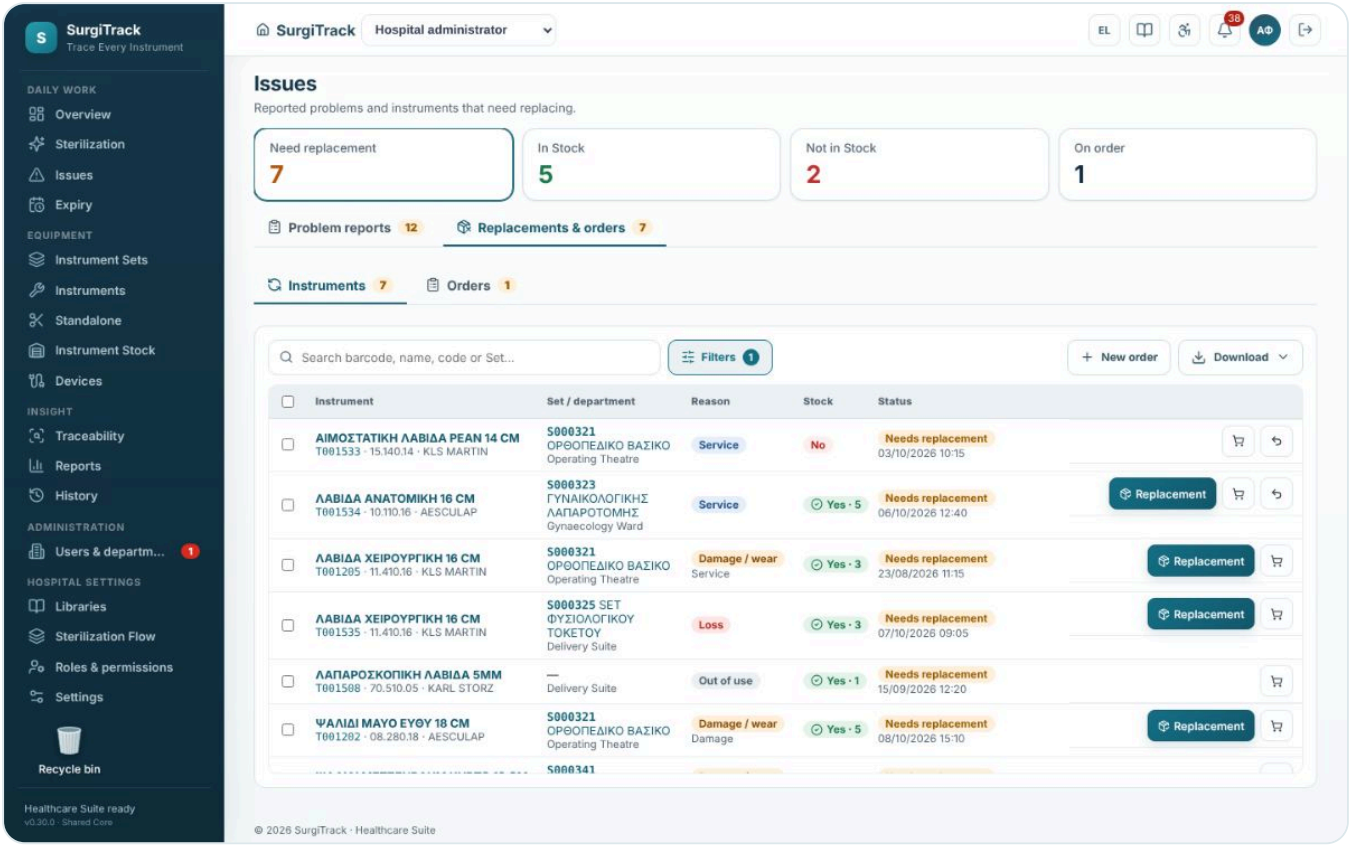

What it lists

Instruments in Service, with an open damage or wear report, lost and out of use. For each: the Set it belongs to (or left), the reason, since when, and whether Stock holds the same instrument (same code or, with no code, the same name).

Numbers

Above the list, four cards: "Need replacement", "In Stock" (Stock holds the same one), "Not in Stock" (it needs ordering) and "On order". Pressing one shows only those in the list.

Replace from Stock

"Replace" puts a matching Stock instrument into the Set. If the damaged one was still in it, it leaves for Service. Select several and press "Replace from Stock" for all at once; one Stock instrument is never used twice.

Purchase order

For what Stock lacks: select it and "Purchase order". One line per kind with its quantity; add supplier and note. In the "Orders" tab the order prints, is marked ordered or cancelled, and "Receive into Stock" registers the new instruments in Stock.

> **Tip.** "Download" (Excel, PDF / Print, CSV) takes your selection, otherwise what the filters show.

9


Sterile expiry

Sterile Sets and instruments with their expiry date: the ones expiring soon and the expired ones.

Who it is for: Sterilization and Administrator

Step by step

1. Press "Expiring soon" or "Expired" to see only those.
2. Filter by department and open the Set or instrument.
3. Ask the department to send it to Sterilization before it is used.

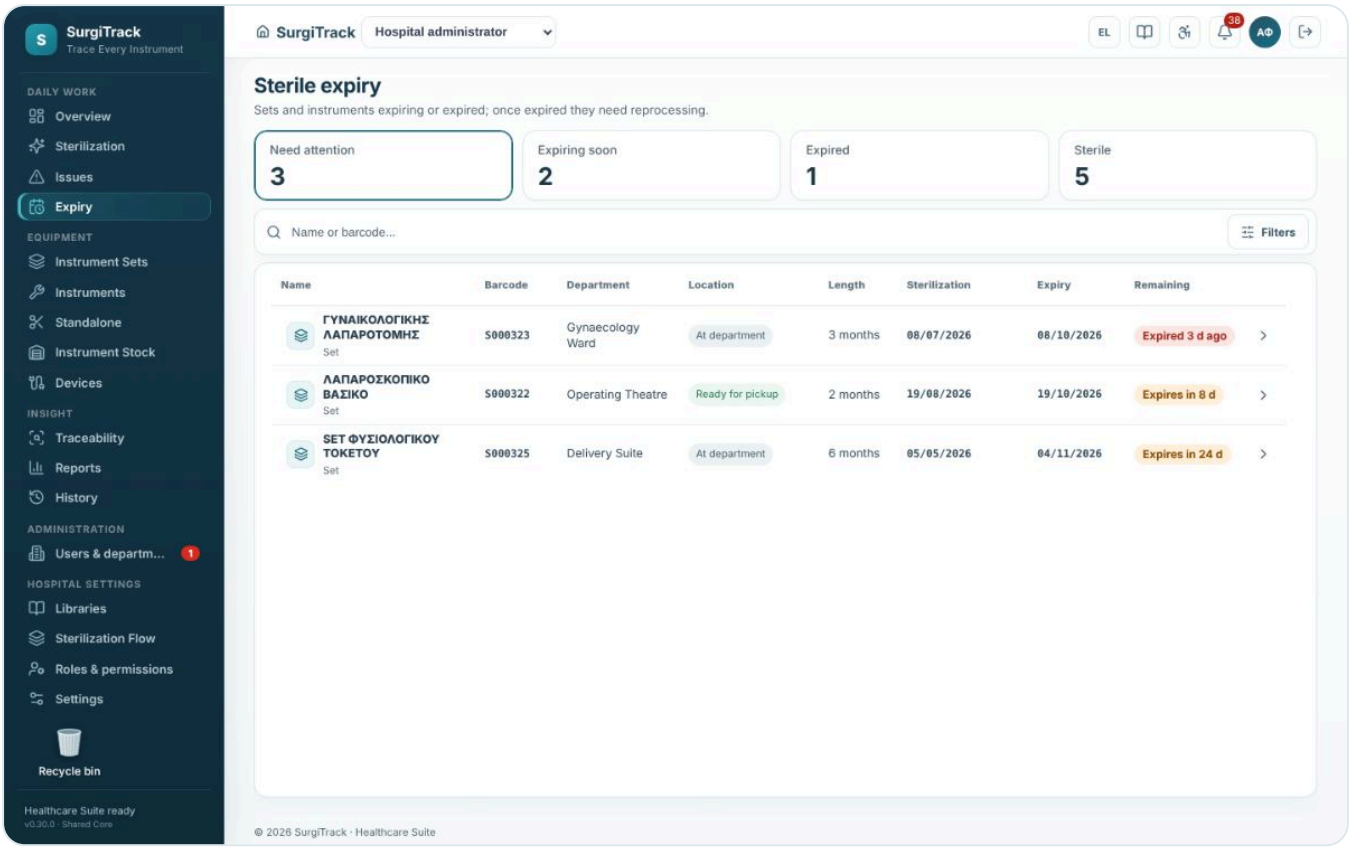

When it warns

A Set or instrument is "expiring soon" in the last month of its sterility (the last 10 days for 2 months). It then shows in the bell, in the Overview "Needs attention" and in this list; the department sees it in its own notifications.

When it expires

The app only warns and keeps it in the "Expired" list; it does not send it for reprocessing by itself. Once it is sent to Sterilization again, the expiry is cleared and a new one is set at the next release.

> **Tip.** The hospital's default shelf life is set in Hospital settings → Settings.

10


Instrument Sets

The register of Sets with composition, department, state and completeness.

Who it is for: Sterilization and Administrator

Step by step

1. Find the Set by search or filters.
2. Open it for composition, history and actions.
3. Print the composition sheet when needed.

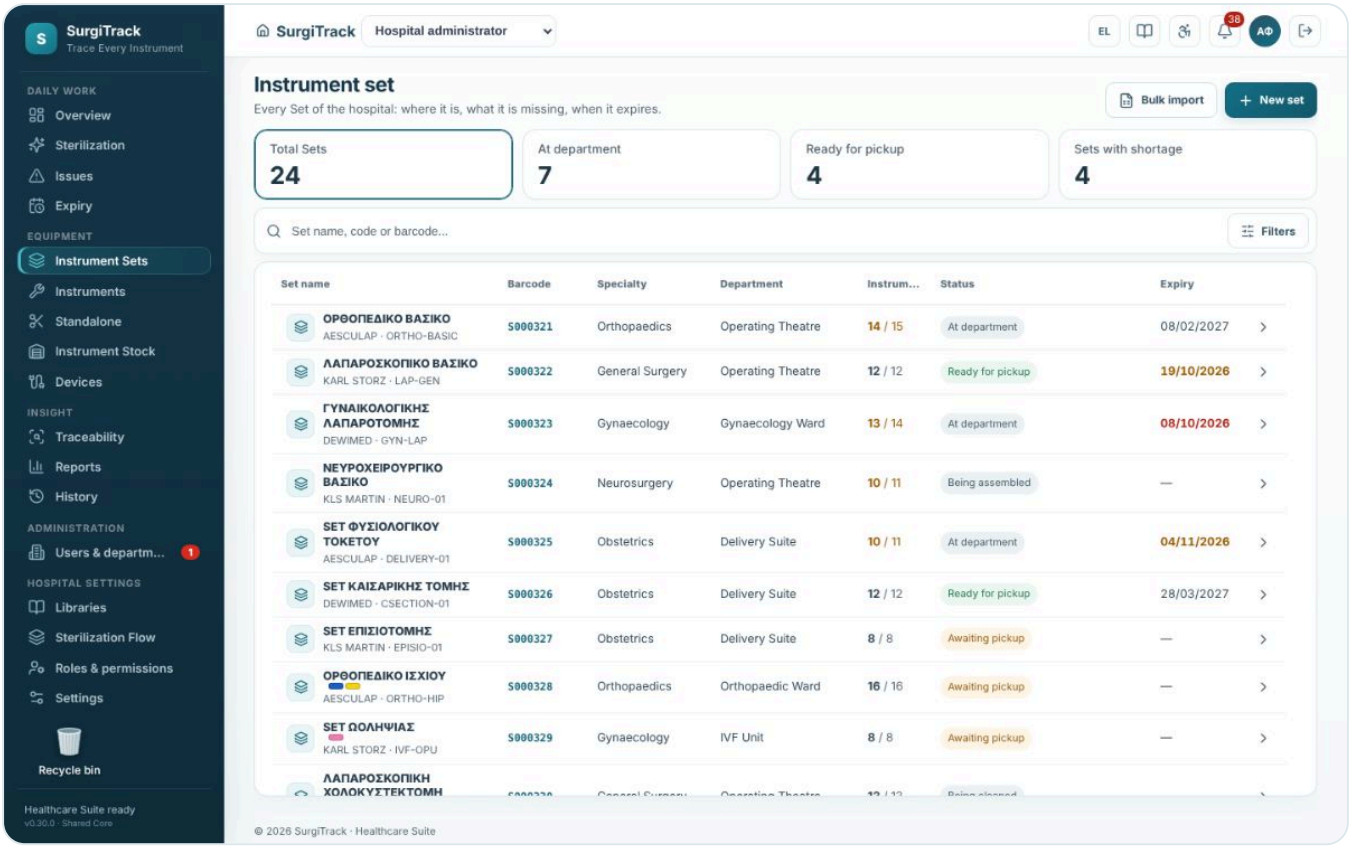

Composition

Each Set has a template composition (what it should contain) and its actual instruments. When something is missing, the Set shows as "Missing items".

Managing composition

The Sterilization supervisor adds instruments from Stock or removes them. An instrument with its own color joining a Set asks whether it keeps its color.

Ownership

A Set can belong to the hospital, a doctor or someone else. The doctor's name is searchable.

11


Instruments

The register of every physical instrument, in Sets, standalone or in Stock.

Who it is for: Sterilization and Administrator

Step by step

1. Search by name, code, barcode or serial.
2. Narrow down with the filters.
3. Open the instrument for details and actions.

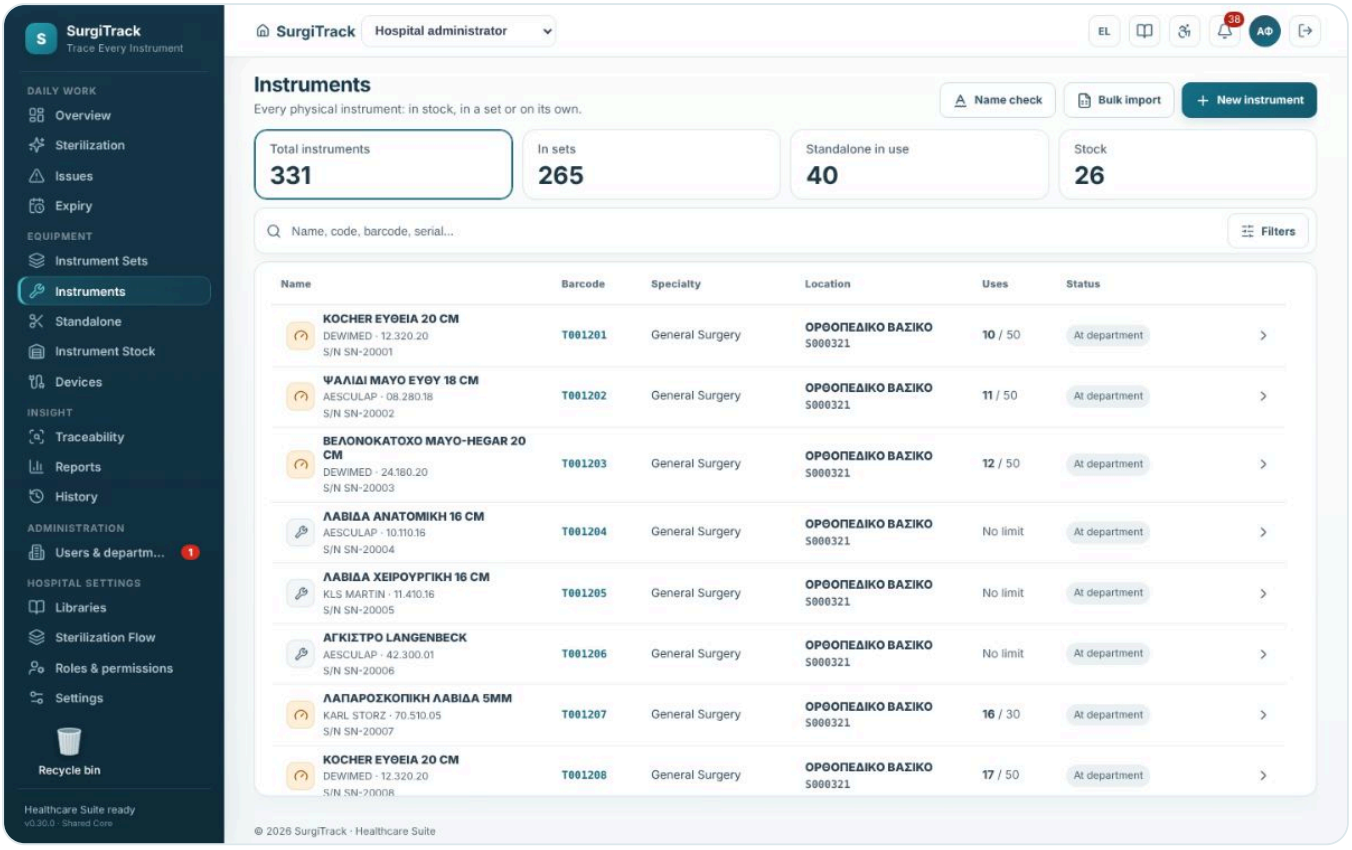

Filters

All filters are in the "Filters" button: department, specialty, manufacturer, location, state and usage type. The indicators above the list filter with one click.

Usage type

"With a usage limit" shows instruments with a usage limit, "Few uses left" those near it and "No limit" the rest.

Instrument card

Opening an instrument shows history, photos, uses, color marker and ownership. The limit and uses can be changed only by the Administrator and the Sterilization supervisor.

Import and names

"Bulk import" brings instruments and Sets from Excel. "Name check" finds names written differently and codes with many names, and unifies them.

> **Tip.** The list loads progressively as you scroll; to find something quickly, use search.

12


Standalone instruments in use

Instruments used on their own in departments, outside any Set.

Who it is for: Sterilization and Administrator

Step by step

1. Filter by department or usage type.
2. Open the instrument for details.

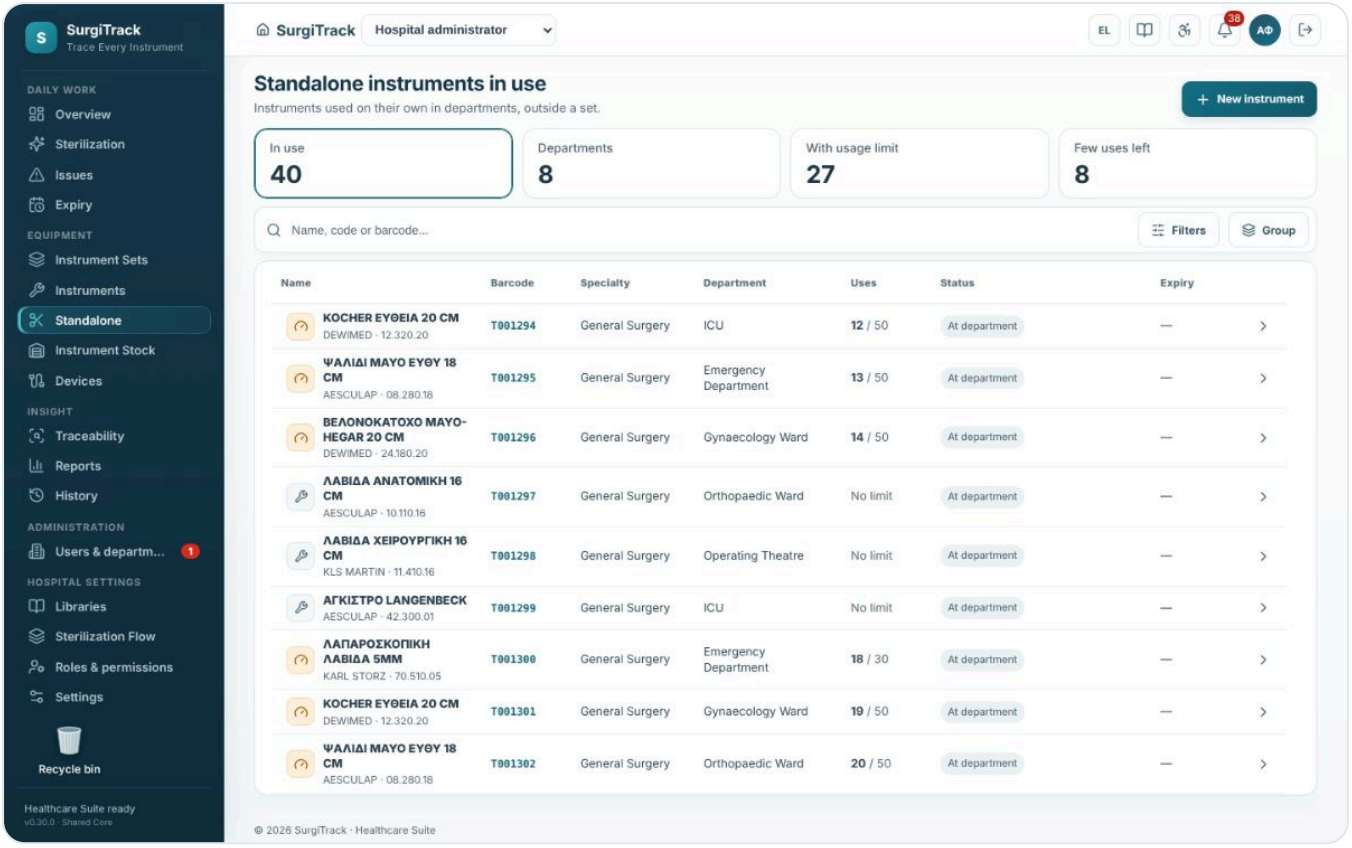

What it is

A standalone instrument belongs to a department and circulates on its own. Many robotic instruments with a usage limit are standalone.

Usage limits

The "With a usage limit" and "Few uses left" indicators filter the list. Each row shows the uses made and the limit (e.g. 11 / 50) and the sterile expiry.

Grouping

The "Group" button joins identical instruments into one row, with the number of pieces, the state, the departments and the range of uses. Clicking a group lists its pieces.

13


Instrument Stock

Available instruments outside Sets and departments, ready to complete a Set.

Who it is for: Sterilization

Step by step

1. In Instrument Sets press "Sets with shortage" to see what is missing.
2. Open the Set and press "Add instruments".
3. Pick the instrument from the Stock tab.

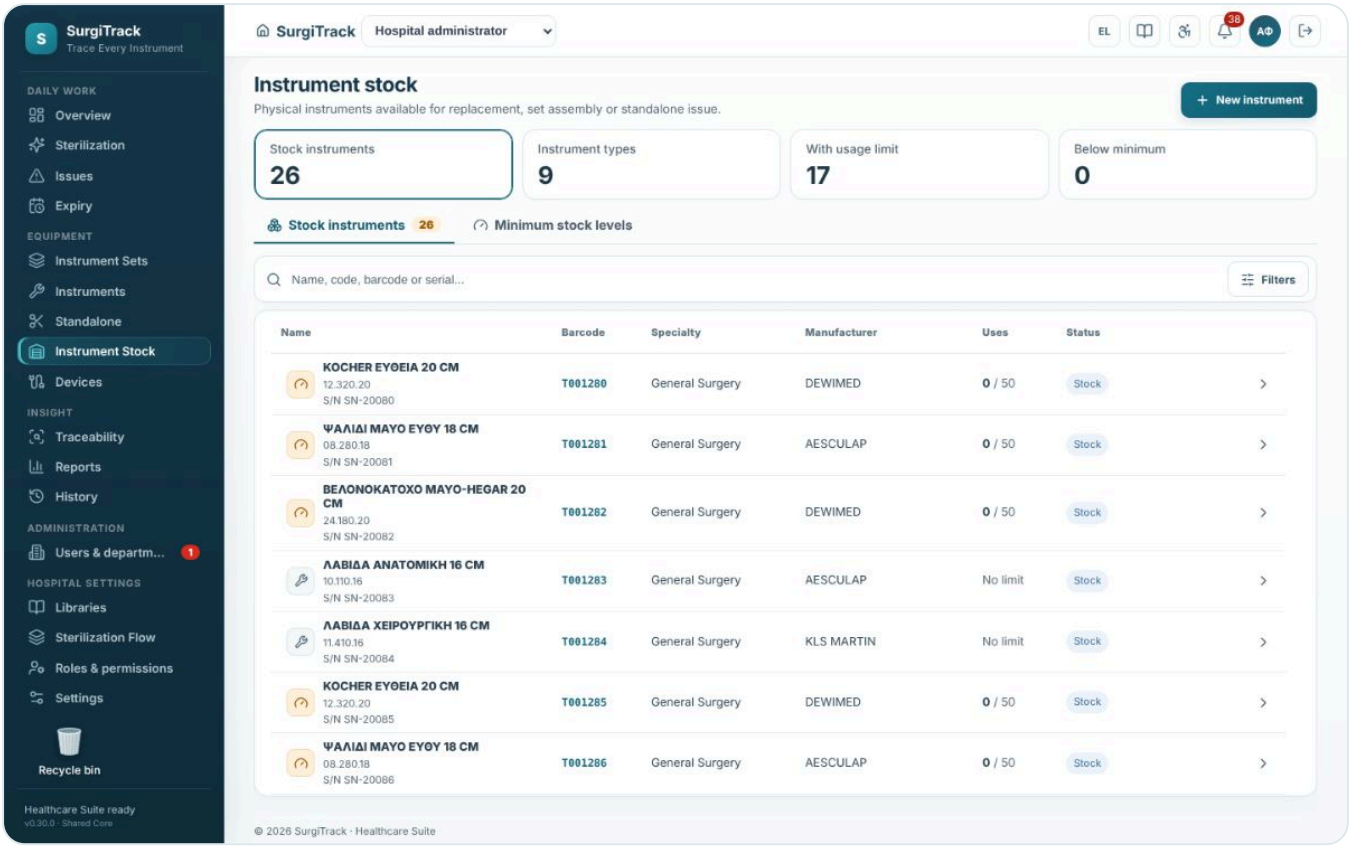

Numbers and tabs

At the top are the Stock numbers (instruments, kinds, with a usage limit, below the minimum); tapping a card filters the list, while "Instrument types" and "Below the minimum" open Minimum stock. Below them, the "Stock instruments" and "Minimum stock" tabs switch the list.

Add to a Set

Adding happens from the Set: open the Set, press "Add instruments" and pick from the Stock tab. In Instrument Sets the "Sets with shortage" indicator opens the Sets that need completing.

14


Devices

Sterilizers, washers and other devices that send their cycle data to SurgiTrack.

Who it is for: Sterilization and Administrator

Step by step

1. The admin adds the device and picks how it connects.
2. For network: “Network key”, given to the manufacturer’s technician.
3. For file or cable: “File” or “Cable” on the device card.

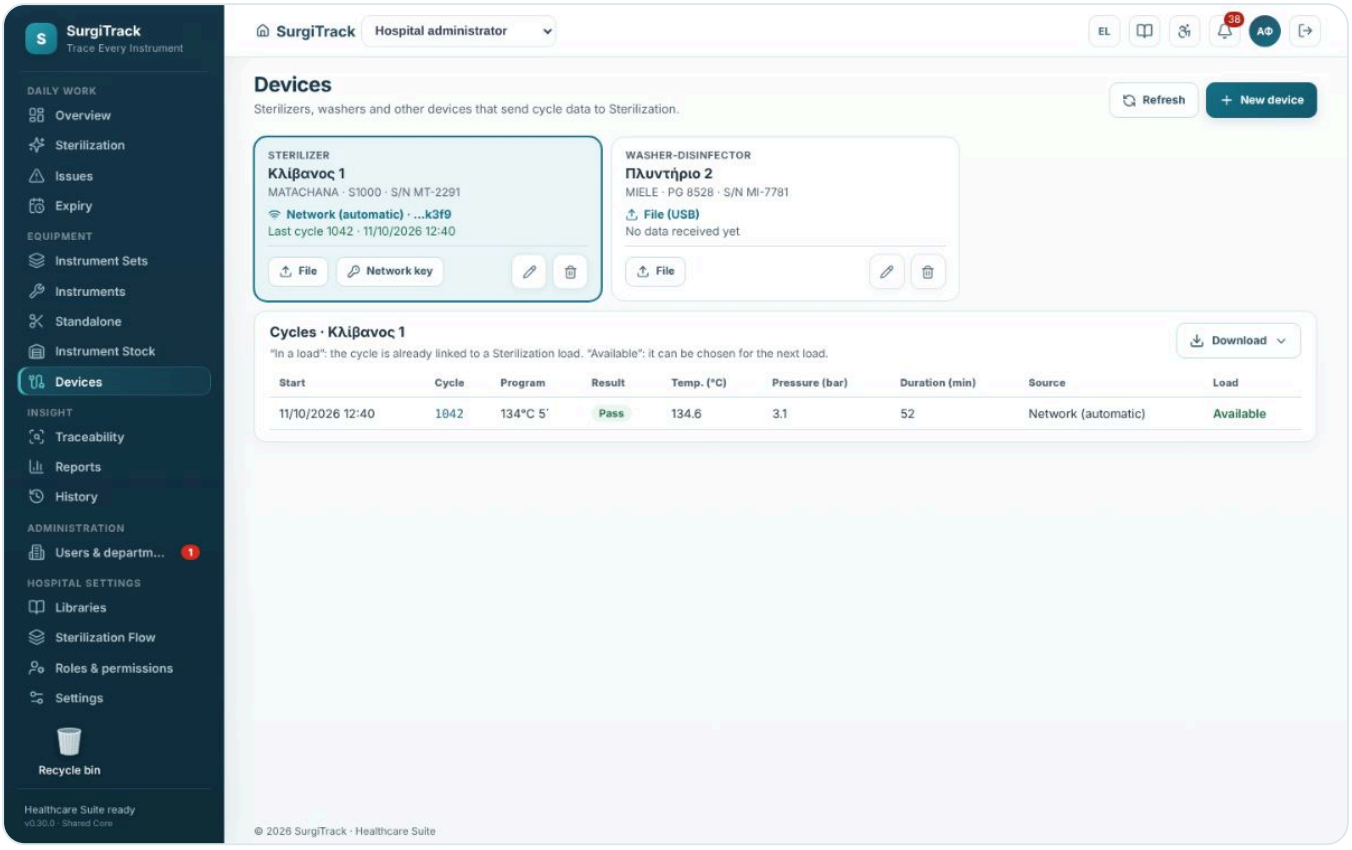

Three ways to connect

Network: the device or the manufacturer software sends every cycle automatically with a device key. File: export the cycles to USB (CSV or Excel) and upload them. Cable: the device connects to a Sterilization computer (Chrome or Edge) and what it prints is read automatically.

Cycle auto-fill

When recording a cycle or a load, the devices’ new cycles are listed. “Use” fills in sterilizer, cycle number and program; you check and confirm. A cycle the device failed is marked as failed.

Record

Each device keeps its cycles with temperature, pressure, duration and result. “Download” saves them as Excel, PDF or CSV for review or audit. The “Load” column shows whether a cycle is “In a load” or “Available” for a new load.

15


Traceability

The full path of a Set or instrument, or everything used for one patient, on a timeline.

Who it is for: Sterilization, Supervisor, Admin, Viewer

Step by step

1. Scan the barcode or type the patient code.
2. Read the timeline from the most recent movement.
3. Download or print the results if needed.

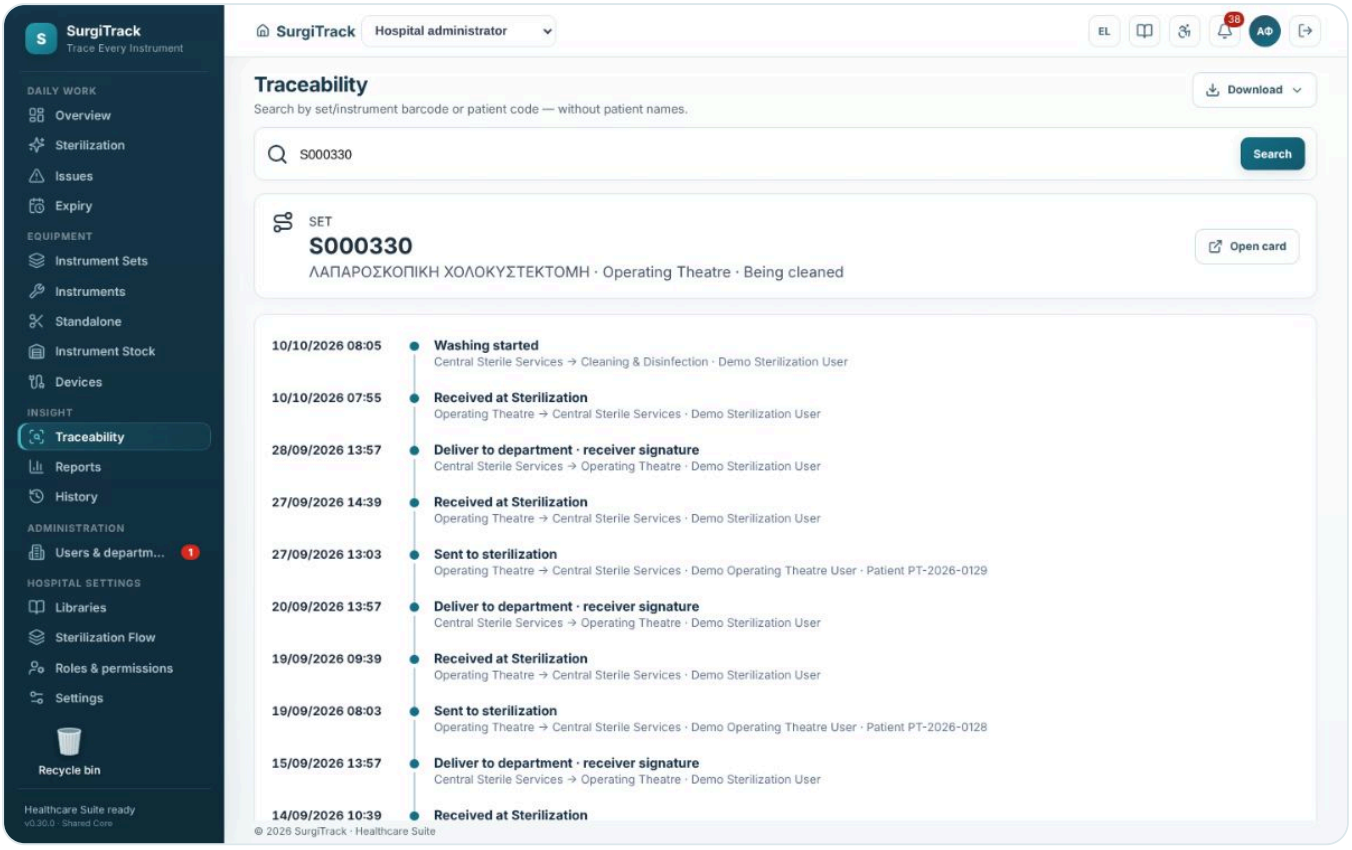

Search

Scan or type a Set (S...) or instrument (T...) barcode, or a patient code, and press "Search". Patients are searched by code only; no names are recorded.

Timeline

Each movement shows date and time, action, from where to where, user and, where there is one, the patient code. For a Set or instrument, "Open card" opens its card.

Cycles and Sets

"Sterilization cycles" lists the sterilizer loads the item went through (its own or its Set's), with sterilizer, cycle number, program and outcome. For a patient code you see what was used, each with

the last sterilization cycle before the use. An instrument in a Set also shows the "Moves of the Set". When a name matches several items, "N found — choose one" lists them.

Download and print

The "Download" button gives the results as Excel, CSV or PDF for printing, e.g. for a quality review or a recall.

16


Reports

Ready-made reports with filters and download as Excel, PDF or CSV.

Who it is for: Sterilization and Administrator

Step by step

1. Pick a report on the left.
2. Set the filters.
3. Press "Download" and choose Excel, PDF or CSV.

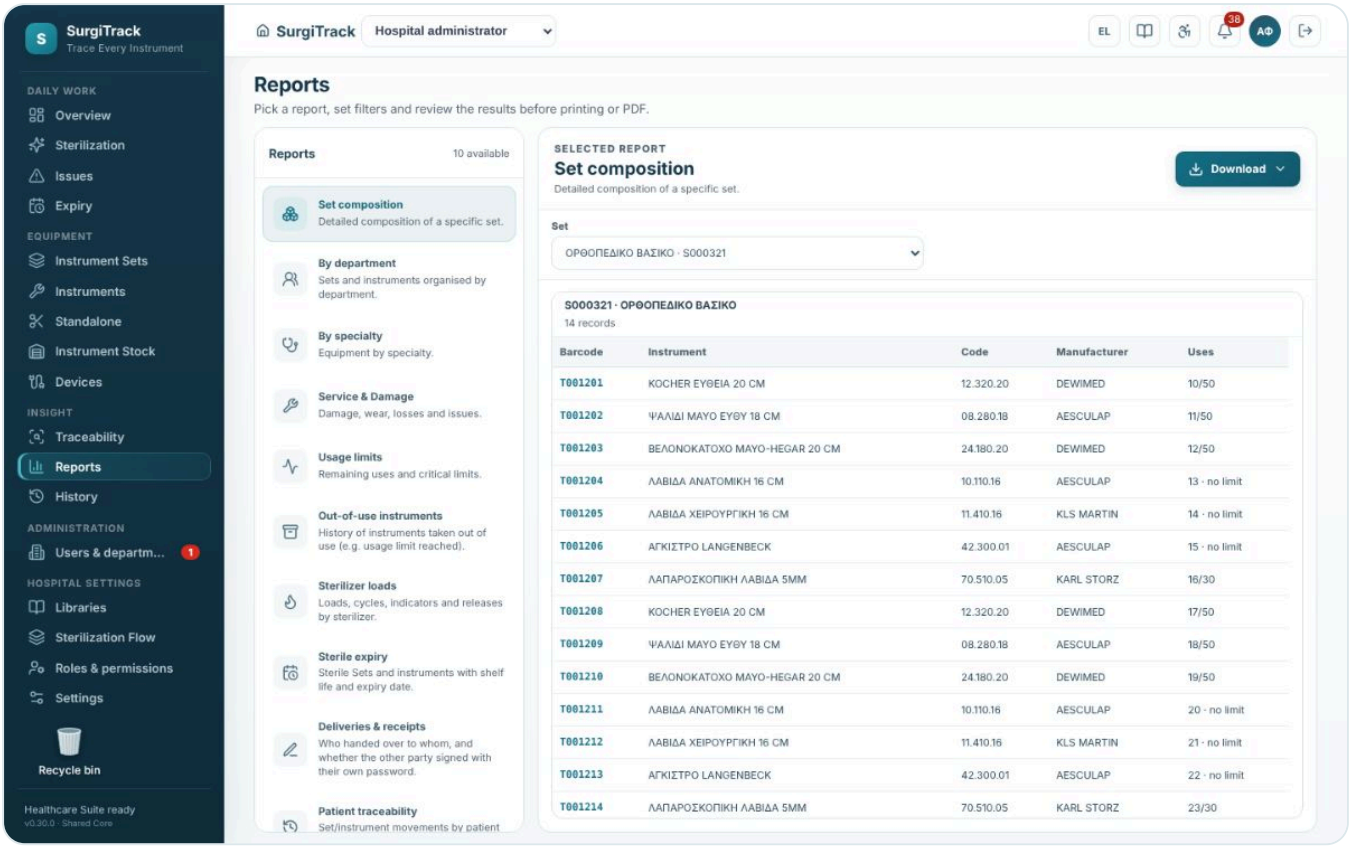

Available reports

Set composition, By department, By specialty, Service & faults, Usage limits, Out-of-use instruments, Sterilizer loads, Sterile expiry, Deliveries & receipts and Patient traceability.

Download: Excel, PDF, CSV

The "Download" button has three options: "Excel" downloads the results as a table with filters, "PDF / Print" opens an A4 preview to print or save as PDF, and "CSV" gives them as plain text for other programs. All take the results with the filters you set. Texts wrap only between words; when the table does not fit, it scrolls sideways. Columns with no value are not shown on screen; the download keeps them.

Out of use

Instruments that reached their usage limit leave the lists and stay as history in this report, with date and reason.

17


History

The chain of custody: every Set and instrument movement, who, when and from where to where.

Who it is for: All users (department users see only their department)

Step by step

1. Filter by date or barcode.
2. Click a movement for full details.

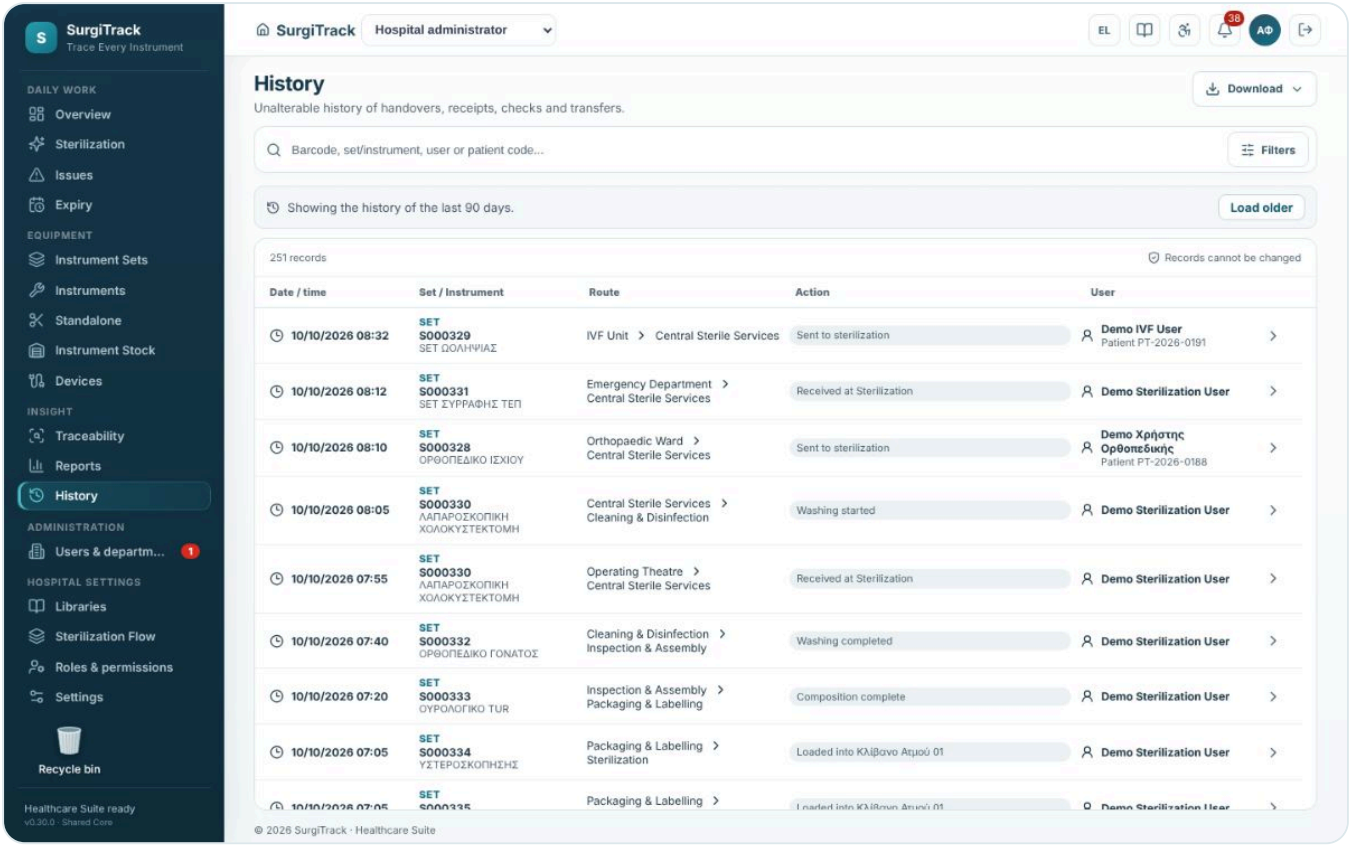

Recent and older history

To open quickly, the app loads the last 90 days of history (compositions and releases for 7 months, as long as the longest sterile shelf life). In History, "Load older" brings the rest; Traceability and Reports load it by themselves. Nothing is deleted: all history stays in the database.

Who made the movement

Every entry keeps the account it was recorded under; the database itself writes it, not the device, and it never changes. When the account differs from the name on the entry, the movement details show it as "Account that recorded it" and the list shows it in orange. From the details, "Open card" opens the Set or instrument and "Traceability" opens its traceability.

Cleaning up history (owner)

Only the platform owner, inside a hospital, sees "Clean up history". They tick the entries (or "Select all shown" after filtering) and press "Delete selected". The deletion is permanent and is recorded as a new "History clean-up · N entries" entry. For everyone else the history never changes.

Date format

All dates show the same way, day/month/year and time in 24 hours: 08/10/2026 13:05. Entries recorded earlier as "8/10/26, 1:05 μ.μ." show this way too; the entry in the database does not change.

Immutable

History records are never changed. Use the date, route and action filters to find a movement.

18


Users & departments

The hospital's users, invitations, access requests and departments.

Who it is for: Hospital administrator

Step by step

1. Departments: make sure they all exist.
2. Users → "Add user": invite a person, the hospital link or CSV.
3. Approve the requests with the right role.
4. Press "Refresh" for the latest requests.

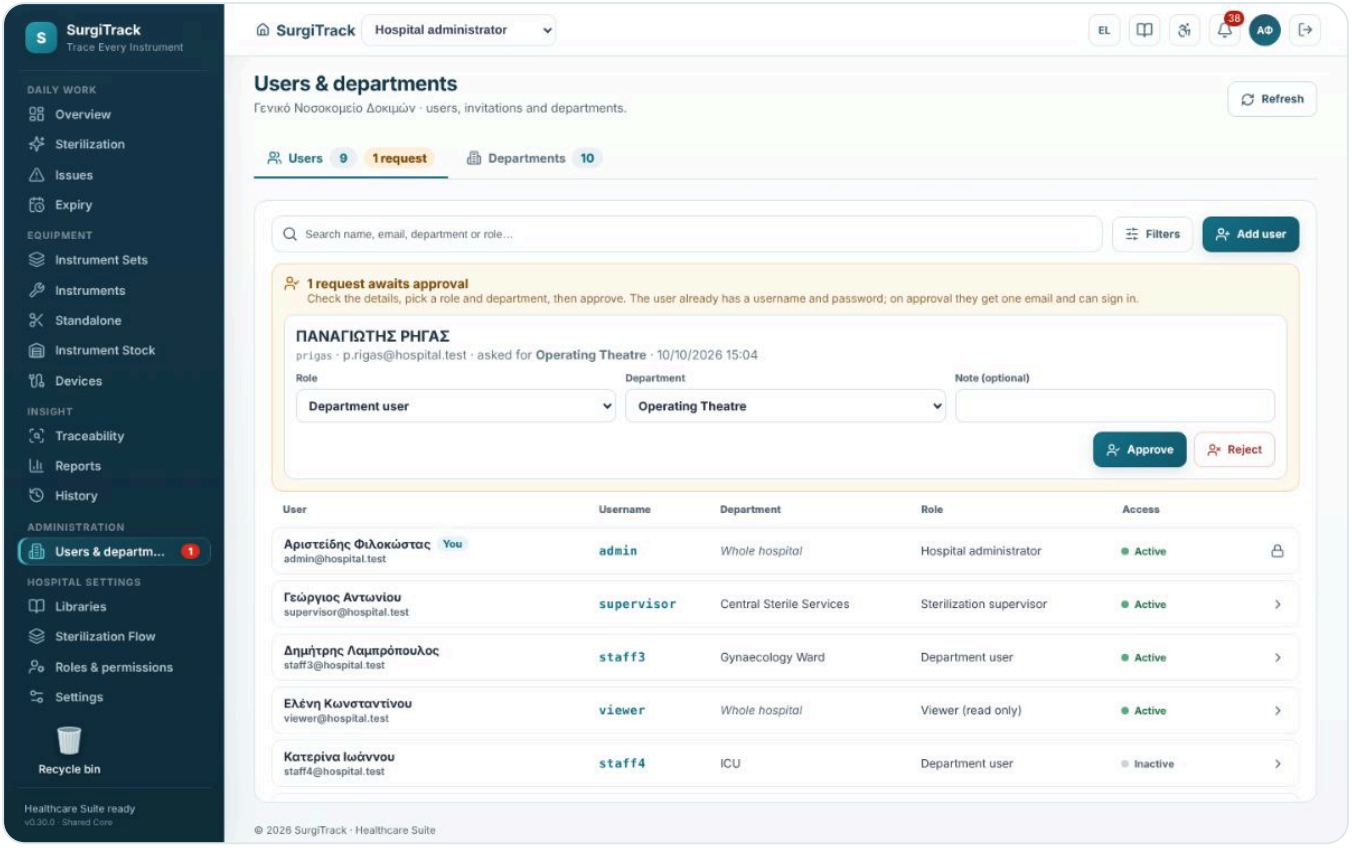

Invitation

"Add user" → "Invite a person": role, email and (if you like) department. "Send email" sends the signup link; "Copy link" copies it to send any way you like (Viber, SMS). It is valid 7 days. The user fills in their name, department and password and sees their username at once. Until they sign up the invitation shows here, where you resend it, copy the link or cancel it.

Hospital link and CSV

For many at once: share the "Hospital signup link" (10 days) with staff; they sign up the same way, confirm their email and you approve them. "From a CSV file" (Name; Email; Department; Role) creates the accounts at once, without approval, and each person gets an email with a username and a password link.

Approval

Requests show in orange, with a count on the bell (no email is sent). Check the name, email and department, set the role and press "Approve" or "Reject". On approval the user gets one email and signs in with their username and the password they set; on rejection they get one email and their account is removed.

Users

The Users tab shows "N requests" when approvals are waiting; the filters narrow the list by department, role and access (Active, Inactive, Invitation pending). Open a user to change the role, department or Demo access, or to deactivate them. "Send password change link" helps someone who forgot their password. "Delete" removes the account completely; their movement history stays.

Departments

Add, rename or deactivate departments. Each department shows what it holds, e.g. "4 users · 12 Sets". The names appear in signups, imports and every list; a deactivated department is not offered to new users.

Checks

- Every department user has the right department.
- People who left the hospital are inactive or deleted.

> **Tip.** If an invitation email does not arrive, ask them to check spam or copy the link and send it yourself.

19


SurgiTrack Studio

Hospital settings: libraries, workflow stages, role permissions, color markers and the usage warning threshold.

Who it is for: Administrator

Step by step

1. Pick a section.
2. Make your changes.
3. Save; changes apply at once.

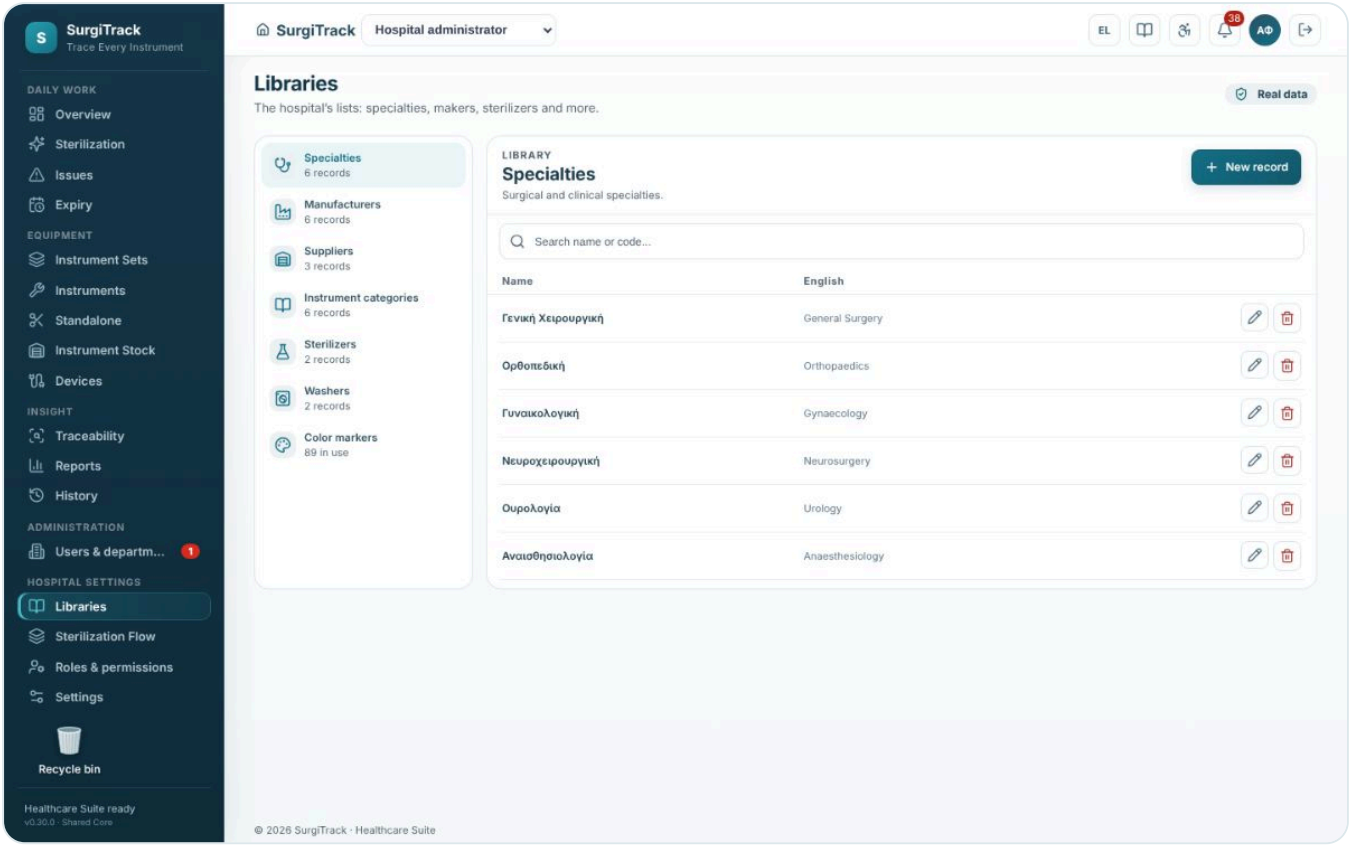

Libraries

Departments, specialties, manufacturers, suppliers, instrument categories, sterilizers, washers and color markers. Whatever you define here appears in the choices across the app. In "Sterilizers", "Add sterilizers" adds several at once in the hospital's naming (Sterilizer A, B, C... or 1, 2, 3...); the choice is kept for next time and the sterilizers appear in the Sterilizer load. "Washers" appear the same way in the Washer load.

Permissions

Set what each role can do. Some permissions (creation, composition, usage limits) belong only to the Sterilization supervisor. The database itself also limits a department user: on Sets and instruments it

changes only what its own workflow changes (dispatch to Sterilization from the department, uses, out of use at the limit, the count), and issues it can only report; anything else it sends stays as it was.

Sterilization Flow

The stages from receipt to delivery to the department. Turn on only the stages and checks your hospital’s Central Sterilization performs. In the release policy you set whether a specific indicator is required; without one, one passed indicator (chemical or biological) is enough.

Roles & permissions and Settings

In "Roles & permissions", "Who does what" explains each role, so you choose correctly when approving, and "Permissions by role" changes them. In "Settings" you set when an instrument shows as "Few uses left", the default sterile shelf life (2, 3 or 6 months), the hospital’s barcode label (size, header, logo) and "Screen lock after inactivity" (default 15 minutes, or Never): on shared tablets the screen locks when not in use and unlocks with the same user’s password, or another user signs in as themselves; syncing goes on behind it and nothing is lost. "Reminder email every morning" sends what is waiting to the administrators (and, if you like, the Sterilization supervisor) around 8, only when something is waiting. "Screen guides" sets whether users see, the first time on each screen, what it does and the first steps.

20


Bulk import

Import instruments and Sets from Excel or CSV, with a preview before anything is written.

Who it is for: Administrator and Sterilization supervisor

Step by step

1. Instruments or Sets → "Bulk import".
2. Download the template and fill it in.
3. Drag the file onto the page.
4. Check the preview, problems and names.
5. Press "Import".

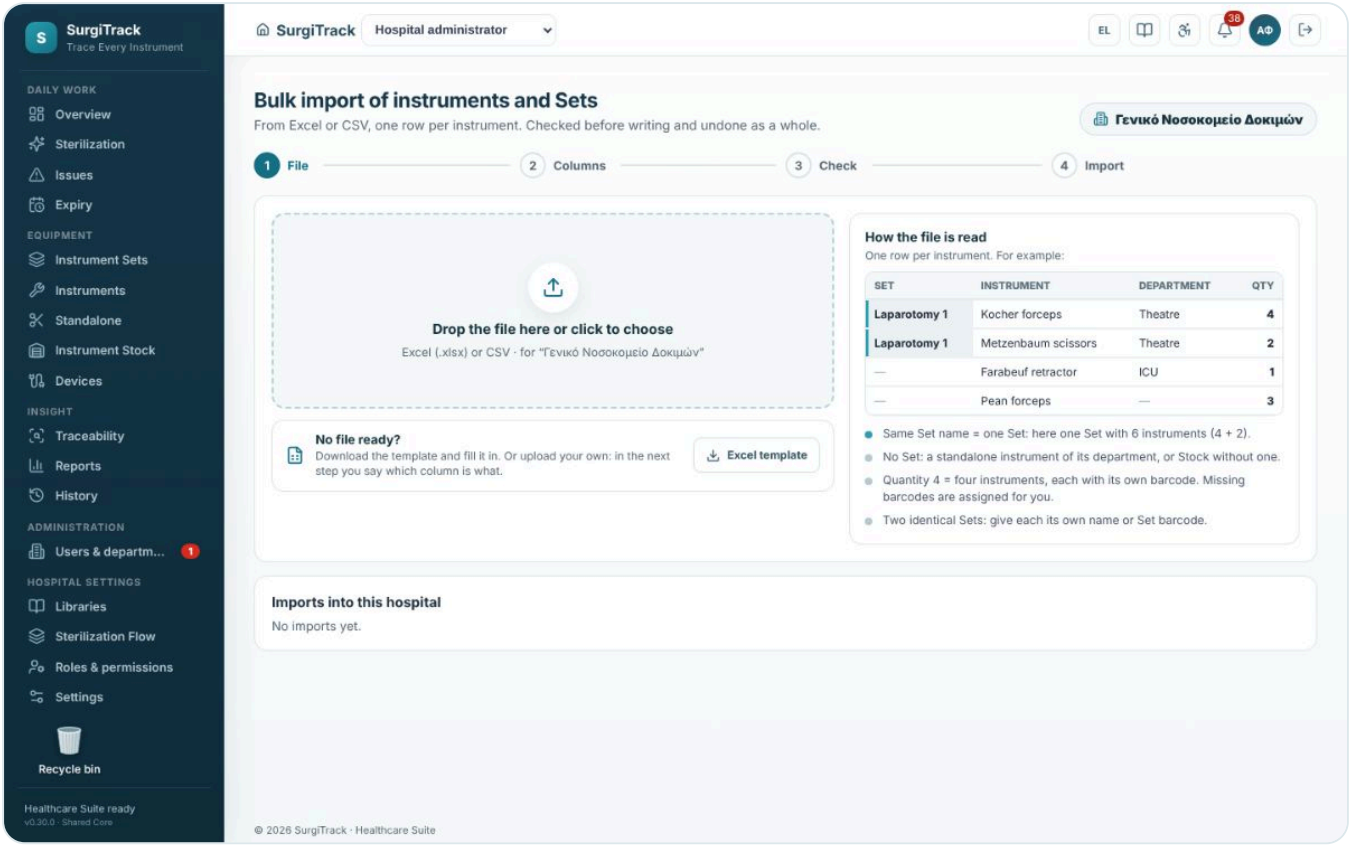

The file

Download the "Excel template". One row per instrument: Set, code, instrument name (required), quantity, department, specialty, manufacturer, max uses, serial number. Same Set name = same Set; no Set = standalone instrument; no department = Stock.

Preview

Before importing you see how many Sets, standalone and Stock instruments will be created, the instrument list with search and the rows with problems. Columns are recognized automatically; if one is not found, you map it by hand.

Names

The import can write names uniformly (capitals without accents, units written the same way) and use the name the hospital already has for the same code, so no duplicate names are created.

Undo

Every import appears under "Imports in this hospital" and can be undone in full with "Undo" (confirmed with "Undo import"), as long as none of its items has been used.

Checks

- Department names match those in Users & departments.
- Rows with problems were fixed or are not needed.
- After importing: "Name check".

21


Name check

Consistent instrument names: spelling fixes and codes that carry more than one name.

Who it is for: Administrator and Sterilization supervisor

Step by step

1. Instruments → "Name check".
2. Apply the spelling fixes.
3. Go through the codes with many names; the instrument count opens their list.
4. Update the compositions if asked.

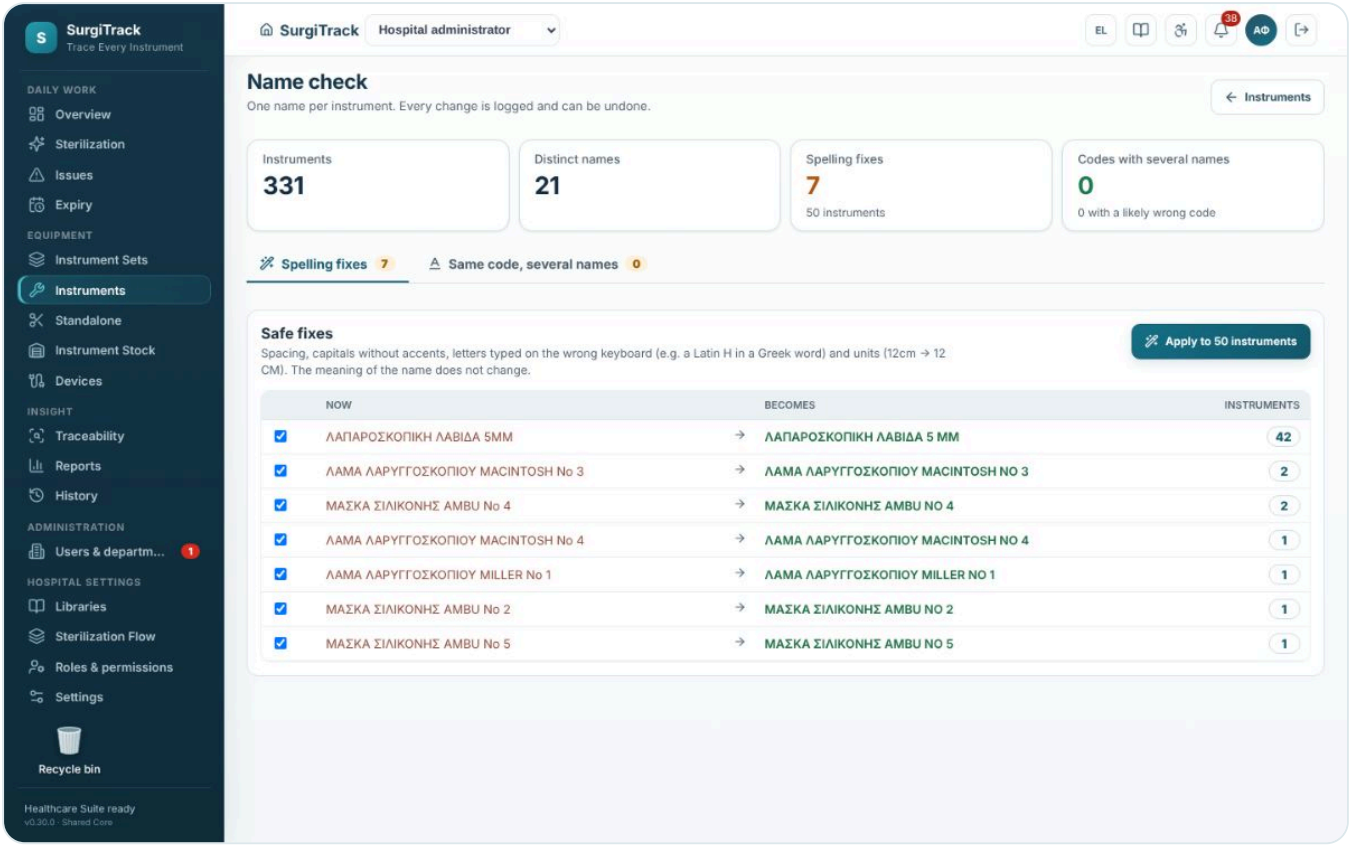

Spelling fixes

Risk-free fixes: double spaces, accents, lower case, Latin letters inside a Greek word (and the reverse), "12cm" → "12 CM". Keep the ones you want ticked and press "Apply to ... instruments".

Same code

For each code with many names the app suggests the most used one. Choose which names join, the final name (or type another) and press "Unify". "Possibly wrong code" means another instrument with the wrong code: fix it from its card.

Set compositions

A rename also reaches the Set template compositions. If "Set compositions with old names" appears, press "Update compositions".

> **Tip.** Every change can be undone from the notice that appears right after it.

22


Recycle bin

Whatever is deleted stays 30 days in the bin and can be put back as it was.

Who it is for: Sterilization and Administrator

Step by step

1. Press the bin at the bottom left.
2. Find the record and press "Restore".

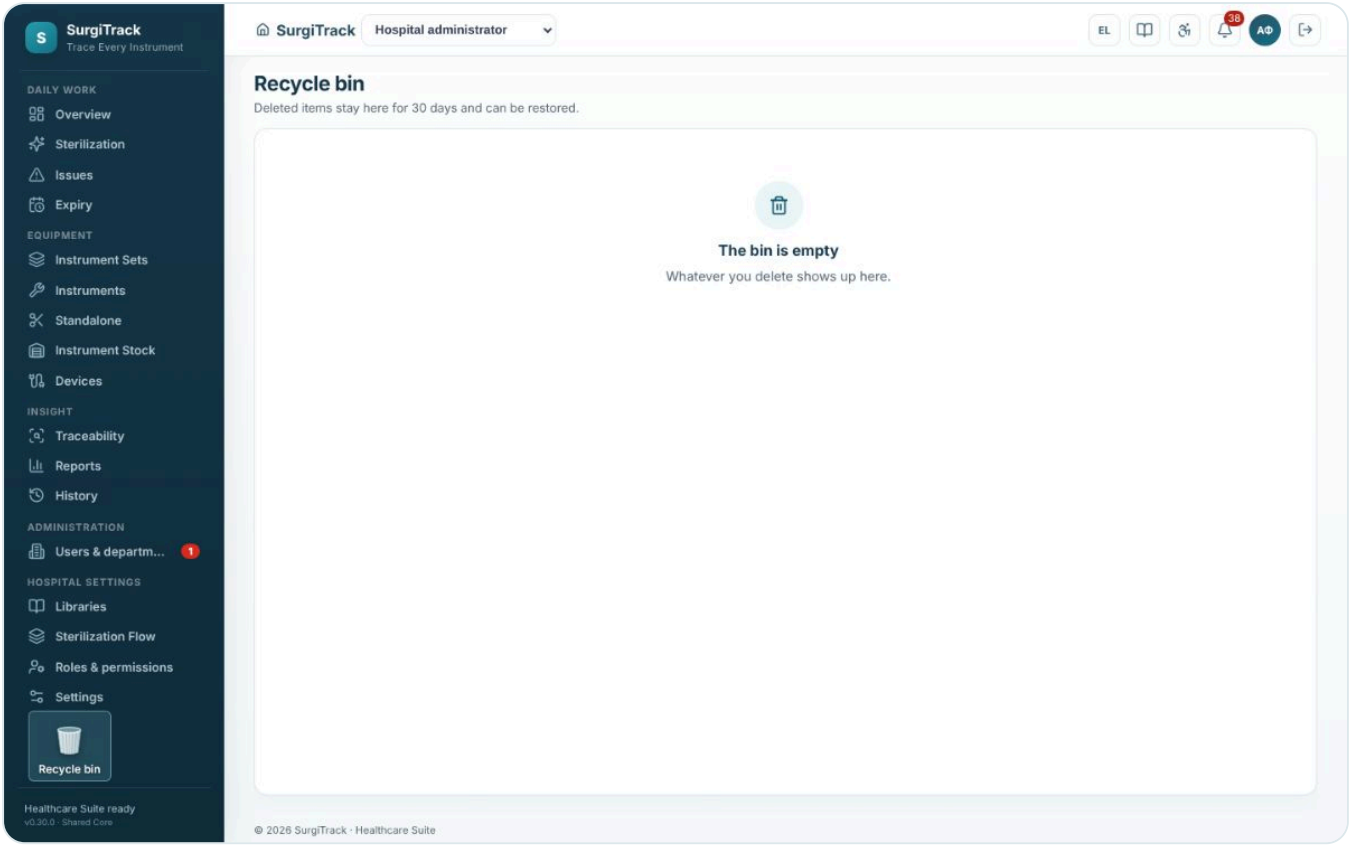

Where it is

The bin sits at the bottom left of the menu, like on a computer. When something is in it, it shows how many.

Restore

Sets, instruments, library records, color markers and devices come back as they were; after 30 days they are deleted for good. Only the Administrator restores library records.

Glossary

Όνομα χρήστη / Username
Your personal sign-in code (e.g. GN1234: your initials and four digits). It shows right after you sign up and in the approval email; you sign in with it or with your email.

Αίτηση πρόσβασης
A new user's signup (with the password they set) waiting for the hospital administrator to approve it; until then they cannot sign in.

Πρότυπη σύνθεση
What a Set should contain (code, name, quantity). It is compared with its actual instruments to show what is missing.

Έλεγχος ονομασιών
A tool that makes names consistent: the same spelling and one name per code.

Παρατηρητής / Viewer
A read-only account (e.g. Nursing Directorate): sees the overview, registries, issues, history and reports of the whole hospital and changes nothing. The hospital administrator creates it.

Σετ / Set
A group of instruments with a defined composition, sterilized and circulated together.

Μεμονωμένο / Standalone
An instrument that belongs to a department and circulates on its own.

Απόθεμα / Stock
Available instruments outside Sets and departments, used to complete Sets.

Όριο χρήσεων
How many times a limited multi-use instrument may be used. One use is counted on each dispatch after use.

Εκτός χρήσης
An instrument that reached its usage limit; it leaves the lists and stays as history in reports.

Κωδικός ασθενούς
An identifier for traceability, without the patient name.

Barcode
The unique scan code of each Set (S...) or instrument (T...).

Αποδέσμευση
The check after a sterilization cycle that allows the item to be used.

Φορτίο
The Sets and instruments that go into the same sterilizer cycle; they are released or sent back to reprocessing together.

Χημικός / βιολογικός δείκτης
Indicators placed in the load that show whether the cycle worked. They are declared at loading and their result is recorded at release; one passed indicator is enough.

Διάρκεια / λήξη αποστείρωσης
How long a Set or instrument stays sterile (2, 3 or 6 months from the release). It warns in the last month (10 days for 2 months).

Ανάκληση
A procedure that blocks items from a faulty cycle from circulating.

Χρωματικός μάρτυρας / Χρωματική σήμανση
Colored tapes that identify a Set or instrument at a glance.