


12 août 2010 14:10 CV report on CV

ROIs used for measures:

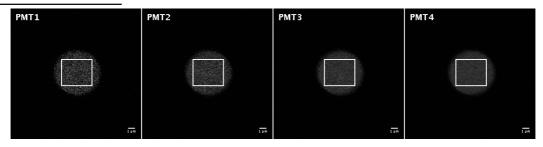

Microscope infos:


Microscope: Confocal Wavelength: 510.0 nm

NA: 1.4

Sampling rate: 0.065x0.065x0.2 μm

Pinhole: 1.0 Airy Units

Histograms:

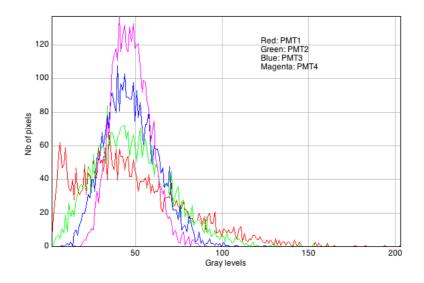

CVs table:

	Standard deviation	Average	Nb pixels	CV	CVs relative to min value
PMT1	30.401	47.784	3640	0.636	2.769
PMT2	22.194	48.653	3640	0.456	1.985
PMT3	15.538	47.88	3640	0.325	1.412
PMT4	10.941	47.617	3640	0.23	1.0