



	NON-CONFORMITY REPORT FOR ASSESSMENT VISIT	F-02/06
		Issue Date: 11/11/19
		Rev No: 06

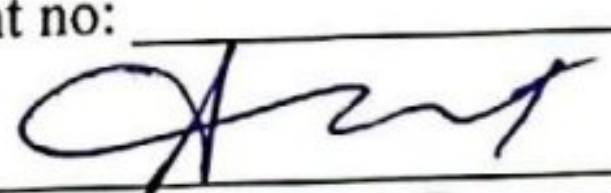
ACTIVITY:	☒ Assessment	☐ Surveillance	NCR No: 10
	☐ Re-Assessment	☐ Scope extension	Accr./Appl.No:
	☐ Other Please specify:		Non-conformity category:
			Very serious ☐ Essential ☒

ORGANIZATION:	Quality control Lab vital Agri. Nutrients (Pvt) ltd.		Time limit for correction:
Department:	Labs		6 weeks
Team Leader:	Mr. Atique Ur Rehman	Mngt. Rep.	Mr. Hammyat Hussain
Assessor	Dr. Muhammad Aftab		
Expert			

DESCRIPTION: Laboratory has not applying the decision rule and also not mentioned lab procedure of reporting of results (NC). lab has not applying the decision rule for the statement of conformity (NC). The VAN laboratory is providing interpretation like ok but the criteria regarding ok and not ok not mentioned in procedure (QCL-LSP-19) (NC). The lab has a procedure for reporting of results but not mentioned about amended/duplicate report issuance not mentioned in procedure (NC).	Requirement of: ISO/IEC 17025 ☒ ISO 15189 ☐ ISO/IEC 17021 ☐ ISO/IEC 17020 ☐ Others:
---	--

10-01-2025 Date	 Signature Assessor/Expert	 Signature (Management Representative)	Ref. Organization's doc.
--------------------	---	---	--------------------------

CORRECTIVE ACTIONS: (Note: It is mandatory to attach Root Cause Analysis) Corrective action for shortcomings on all the NCs has been taken. Lab has revised the lab procedure for reporting of results (QCL-LSP-19) and applying the decision rule for statement of conformity. Lab has revised the procedure (QCL-LSP-19) and mentioned the criteria regarding OK and Not OK. Lab has revised the procedure for reporting of results (QCL-LSP-19) and mentioned about amended/duplicate report issuance in the procedure.	☐ It is not necessary to attach documentation
--	--

Action are documented in the amendment no:	
18-02-25 Date	Signature (Management. Representative)

REASON FOR CLOSING: (To be filled in by the Team Leader.)
☐ The non-conformity is closed based on satisfactory documentation from the organization ☐ The non-conformity is closed based on recommendation from the technical assessor ☐ Implementation of the corrective actions will be followed up at the next visit

Remarks (if any)-----

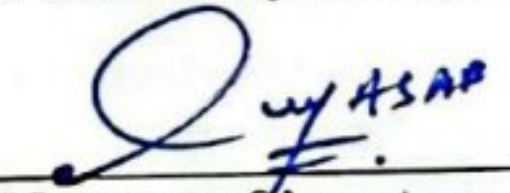

The non-conformity is closed: _____ Date _____ Signature (Team Leader.)

	CORRECTIVE ACTION REQUEST	Doc. No.	QCL-FRM-9.01
		Issue Date	01-10-2024
		Rev#	01

Initiated by: Masab Rasheed	Department: QC Lab	CAR No. CA-10-02-2025
Designation: AQCM	CAR Initiated Date: 11-02-2025	NC No. 10

CAR Initiated due to (Please tick the relevant appropriate box below)


- ☒ PNAC Assessment
 ☐ Complaint
 ☐ Accident/Incident
 ☐ Internal Audit
☐ Suggestion/Improvement
 ☐ Technical Fault
 ☐ Others

A. Description (to be filled by Initiator) Laboratory has not applying the decision rule and also not mentioned lab procedure of reporting of results (NC). Lab has not applying the decision rule for the statement of conformity (NC). The VAN laboratory is providing interpretation like ok but the criteria regarding ok and not ok not mentioned in procedure (QCL-LSP-19) (NC). The lab has a procedure for reporting of results but not mentioned about amended/duplicate report issuance not mentioned in procedure (NC).	
 Signatures	
Significance/Priority Level	☒ Urgent ☐ Normal ☐ Non-significance
☒ Accepted ☐ Rejected	Assigned to: Masab Rasheed Date: 11-02-2025
* If accepted then Manager QC to mark it to concerned person for Root Cause Analysis.	
B. Root Cause Analysis (where required) 1. The laboratory staff is not consistently applying the decision rule or mentioning lab procedures for reporting results because of insufficient training, unclear communication, or lack of a formal review process to ensure adherence to these procedures. 2. The root cause is likely insufficient training and awareness among lab staff about the importance of applying the decision rule for the statement of conformity, compounded by inadequate communication and system checks to reinforce the correct application of the procedure. 3. The root cause of this non-compliance (NC) is that the procedure QCL-LSP-19 does not clearly define the criteria for labeling results as "OK" or "Not OK." Without these clear guidelines, lab staff may interpret results in different ways, leading to inconsistency and confusion. 4. The root cause of this non-conformance (NC) is that the lab's procedure did not include instructions on how to handle amended or duplicate reports. This happened because the procedure focused mainly on the initial report creation and didn't account for situations where reports need to be changed or duplicated.	
C. Proposed Action	Target Date: 18-02-2025
Corrective action for shortcomings on all the NCs has been taken. Lab has revised the lab procedure for reporting of results (QCL-LSP-19) and applying the decision rule for statement of conformity. Lab has revised the procedure (QCL-LSP-19) and mentioned the criteria regarding OK and Not OK. Lab has revised the procedure for reporting of results (QCL-LSP-19) and mentioned about amended/duplicate report issuance in the procedure.	
 Name or Signatures (Person who carried out Root Cause Analysis and Proposed Corrective Action)	
D. Verification by Manager QC for implementation & Effectiveness	
Is Proposed Action Implemented? ☒ YES ☐ NO	Is it Effective? ☒ YES ☐ NO
Remarks (If any):	
CAR closing date: <u>18-02-25</u>	Manager QC Sign: 

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

Non-Conformance Description			
Laboratory has not applying the decision rule and also not mentioned lab procedure of reporting of results (NC).			
RCA Team Members	Himayat Hussain (QCM), Masab Rasheed (AQCM)		
RCA Team Lead / Head	Himayat Hussain (QCM)		
RCA Start Date	11-02-2025	Submission Date	18-02-2025
Methodology / Tools Used			
Cause & Effect Diagram	☐	5WHY analysis	☐
		3W2H / 5W2H	☒

Cause Effect Diagram



3W2H /5W2H	Phenomenon of Problem / Question	Explanation / Answer
WHY	Why is the decision rule not being applied?	Laboratory staff are not following the established decision rules in their analysis.
WHY	Why are laboratory staff not following the established decision rules?	Because they have not been trained or reminded on how to apply these rules correctly.
WHY	Why have the staff not been trained or reminded?	There is a lack of a formal process for reviewing and reinforcing these procedures.
WHY	Why is there a lack of a formal process for reviewing procedures?	There is no regular internal audit or review system in place to ensure staff are up to date with the laboratory procedures.
WHY	Why is there no internal audit or review system?	The management has not prioritized this area or allocated resources for ongoing procedure reinforcement.
How	How can we ensure that decision rules are applied correctly?	Implement mandatory training sessions on decision rules, along with clear documentation for reference. Regularly audit adherence to these rules during internal checks.

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

How	How can we make sure lab procedures for reporting results are mentioned clearly?	Standardize a template for all lab reports that includes a section for the applicable lab procedure, and train staff to consistently fill out this section.
Root Cause: The laboratory staff is not consistently applying the decision rule or mentioning lab procedures for reporting results because of insufficient training, unclear communication, or lack of a formal review process to ensure adherence to these procedures.		

RCA Statement: The laboratory staff is not consistently applying the decision rule or mentioning lab procedures for reporting results because of insufficient training, unclear communication, or lack of a formal review process to ensure adherence to these procedures.


Reviewed by:  ASAP

Evaluated by: 

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

Non-Conformance Description			
Lab has not applying the decision rule for the statement of conformity (NC).			
RCA Team Members	Himayat Hussain (QCM), Masab Rasheed (AQCM)		
RCA Team Lead / Head	Himayat Hussain (QCM)		
RCA Start Date	11-02-2025	Submission Date	18-02-2025
Methodology / Tools Used			
Cause & Effect Diagram	☐	5WHY analysis	☐
		3W2H / 5W2H	✓

Cause Effect Diagram



3W2H /5W2H	Phenomenon of Problem / Question	Explanation / Answer
WHY	Why is the decision rule not applied for the statement of conformity?	The lab failed to follow the established procedure for determining conformity.
WHY	Why did the lab fail to follow the established procedure?	Because the staff was unaware of the procedure, or it was not clearly defined or communicated.
WHY	Why were the staff unaware or the procedure not clearly defined?	There was a lack of proper training or regular reminders regarding the importance of the decision rule.
WHY	Why was there a lack of proper training or reminders?	Because the lab management did not prioritize regular training sessions or system updates on procedures.
WHY	Why did the lab management not prioritize regular training?	There was insufficient awareness of the potential risks and consequences of not following the decision rule.
How	How can we ensure the decision rule is applied correctly in the future?	Implement regular training sessions for lab staff on the importance of applying the decision rule for conformity statements.
How	How can we prevent this issue from happening again?	Establish a clear, accessible reference to the decision rule in standard

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

		operating procedures (SOPs) and implement a system of checks to ensure compliance.
Root Cause: The root cause is likely insufficient training and awareness among lab staff about the importance of applying the decision rule for the statement of conformity, compounded by inadequate communication and system checks to reinforce the correct application of the procedure.		

RCA Statement: The root cause is likely insufficient training and awareness among lab staff about the importance of applying the decision rule for the statement of conformity, compounded by inadequate communication and system checks to reinforce the correct application of the procedure.


Reviewed by: 

Evaluated by: 

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

Non-Conformance Description			
The VAN laboratory is providing interpretation like ok but the criteria regarding ok and not ok not mentioned in procedure (QCL-LSP-19) (NC).			
RCA Team Members	Himayat Hussain (QCM), Masab Rasheed (AQCM)		
RCA Team Lead / Head	Himayat Hussain (QCM)		
RCA Start Date	11-02-2025	Submission Date	18-02-2025
Methodology / Tools Used			
Cause & Effect Diagram	☐	5WHY analysis	☐
		3W2H / 5W2H	✓

Cause Effect Diagram

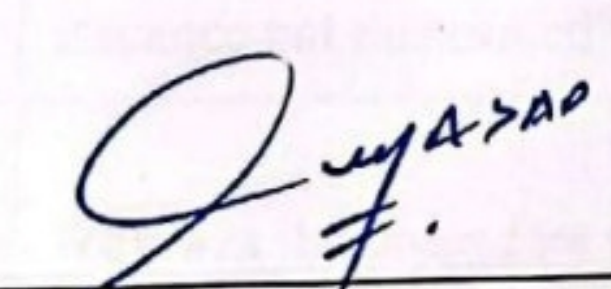


3W2H /5W2H	Phenomenon of Problem / Question	Explanation / Answer
WHY	Why is the NC occurring?	The NC occurs because the laboratory is providing interpretations (labeled as "OK" or "Not OK") without clear criteria being outlined in the procedure (QCL-LSP-19).
WHY	Why are clear criteria not included in the procedure?	The procedure (QCL-LSP-19) does not specify the exact criteria for interpretation of results (OK/Not OK).
WHY	Why was the procedure not updated to include these criteria?	The procedure was either developed without considering the need for clear criteria for interpretation, or the criteria were assumed to be understood and therefore not explicitly stated.
WHY	Why were these assumptions made?	The laboratory may have relied on historical knowledge or previous practices where such interpretations were based on tacit understanding or verbal communication.
WHY	Why was there a lack of written and documented guidelines?	There was possibly an oversight or gap in the procedure review process, or the emphasis on documentation of

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

		these specific criteria was not deemed necessary during the procedure's creation or revision.
How	How can this issue be addressed?	The procedure (QCL-LSP-19) needs to be updated to clearly define the criteria for "OK" and "Not OK" interpretations. This should include objective metrics, conditions, or thresholds to ensure consistent and transparent decision-making.
How	How will this update prevent future non-compliance?	By explicitly defining these criteria, there will be a standardized approach that all lab personnel can follow. This will ensure that all interpretations are consistent, and any variations or ambiguities are eliminated, reducing the risk of incorrect results or interpretations in the future.
Root Cause: The root cause of this non-compliance (NC) is that the procedure QCL-LSP-19 does not clearly define the criteria for labeling results as "OK" or "Not OK." Without these clear guidelines, lab staff may interpret results in different ways, leading to inconsistency and confusion.		

RCA Statement: The root cause of this non-compliance (NC) is that the procedure **QCL-LSP-19** does not clearly define the criteria for labeling results as "OK" or "Not OK." Without these clear guidelines, lab staff may interpret results in different ways, leading to inconsistency and confusion.


Reviewed by: 

Evaluated by: 

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

Non-Conformance Description			
The lab has a procedure for reporting of results but not mentioned about amended/duplicate report issuance not mentioned in procedure (NC).			
RCA Team Members	Himayat Hussain (QCM), Masab Rasheed (AQCM)		
RCA Team Lead / Head	Himayat Hussain (QCM)		
RCA Start Date	11-02-2025	Submission Date	18-02-2025
Methodology / Tools Used			
Cause & Effect Diagram	☐	5WHY analysis	☐
		3W2H / 5W2H	☒

Cause Effect Diagram



3W2H /5W2H	Phenomenon of Problem / Question	Explanation / Answer
WHY	Why was the procedure for amended/duplicate report issuance not mentioned?	The procedure was not updated to include amendments or duplicate reports.
WHY	Why was the procedure not updated?	There was no formal process for recognizing the need to update the procedure when changes or amendments to reports occur.
WHY	Why was there no formal process for recognizing the need to update?	The lab may have focused more on primary report generation and not on situations requiring amendments or duplicates.
WHY	Why was the focus only on primary report generation?	There may not have been a clear recognition of the need to account for amendments or duplicates, possibly due to the lack of comprehensive training or awareness.
WHY	Why was there a lack of training or awareness?	There might be a gap in the training materials or the procedure development process, which didn't include detailed scenarios like amendments or duplicates in reporting.

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

How	How can the issue of missing procedure for amended/duplicate reports be resolved?	The procedure can be updated to include specific guidelines on how to handle amended or duplicate reports, specifying roles, timelines, and conditions under which they should be issued.
How	How can we ensure that the new procedure is followed?	We can conduct training sessions for all involved personnel to familiarize them with the updated procedure. Regular audits can also be done to ensure compliance with the new steps for amendments and duplicates.
Root Cause: The root cause of this non-conformance (NC) is that the lab's procedure did not include instructions on how to handle amended or duplicate reports. This happened because the procedure focused mainly on the initial report creation and didn't account for situations where reports need to be changed or duplicated.		

RCA Statement: The root cause of this non-conformance (NC) is that the lab's procedure did not include instructions on how to handle amended or duplicate reports. This happened because the procedure focused mainly on the initial report creation and didn't account for situations where reports need to be changed or duplicated.

Reviewed by: 

Evaluated by: 




DECISION RULE
CONTROLLED COPY
NO. _____

Active Range (%)	Upto 2.5	2.5-10	10-25	25-50	>50
FAD Tolerances	15%	10%	6%	5%	3%


				FAD Limits (Active Ingredients)			QC Lab Acceptable Limits (Pass)	
S #	Test Parameter	Active Ingredient		Lower Limit	Upper Limit	QC Lab MU(±)	Lower Limit	Upper Limit
1	Nitrogen	8.0	% w/v	7.20	8.80	0.66	7.860	8.140
2	Phosphorus	8.0	% w/v	7.20	8.80	0.63	7.830	8.170
3	Potassium	6.0	% w/v	5.40	6.60	0.59	5.990	6.010

Prepared by (AQCМ):
 Signature:
Date: 01-02-25

Approved by (QCM):
 Signature:
Date: 01-02-25

	DOCUMENT CHANGE REQUEST	Doc.#	QCL-FRM-7.02
		Issue Date	01-02-2025
		Rev#	02

CONTROLLED COPY

NO. _____ Section A			
DCR No.	07-25	Date	15-02-25
Request Raised By	Masab Rasheed	Section	QC Lab
Document Title		Document Status	NEW EXISTING ☒
Reason(s)	☐	New Process Documentation	New Form Documentation
	☒	Addition in Document	Correction in Document
	☐	Deletion within Document	Modification in Document
Section B			
Description of Requirement	Revision of LSP required to Address the shortcomings observed in DNAC audit.		
Effected Sections (Not Applicable on New Documents)	Added division rules, criteria for amended or duplicate report issuance		
Section C			
Review by	Himayat Hussain	Review Status (Choose only one)	☒ Draft Reviewed
Designation			☐ Draft Rejected
			☐ Draft Revision Suggested
Reason for Rejection (Choose only one)	☐	Conflict with Policy	Conflict with Procedure
	☐	Conflict with Client Requirement	Conflict with Regulation
	☐	Incorrect Draft	Draft Does not reflect "Description of Requirement"
Final Remarks	Recommended for final approval.		
Submitted for Final Approval on (Date)			
Approved By		Designation	CEO



	PROCEDURE FOR REPORTING OF RESULTS	Doc. No.	QCL-LSP-19
		Issue Date	15-02-2025
		Rev#	02

MASTER

Standard Operating Procedure
For Reporting of Results

ISO/IEC 17025:2017 Clause 7.8

CONTROLLED COPY
NO. _____

Prepared By: Masab Rasheed AQCM	Reviewed By: Himayat Hussain QCM	Approved By: Ahmad Umair CEO
		
Date: 15-02-25	Date: 15-02-25	Date: 15/02/2025

Copyright

The copyright of this procedure, together with all confidential information contained herein is the sole property of **QC LAB**.

It may be copied in full or in parts only by the Management / personnel and only for the purpose of Company related activities. Disclosure and copying of any information contained within this procedure to any person (s) outside the employee of company without written permission/authorization of the Chief Executive Officer is strictly prohibited.



PROCEDURE FOR REPORTING OF RESULTS

Doc. No.	QCL-LSP-19
Issue Date	15-02-2025
Rev#	02

MASTER

CONTROLLED COPY

Amendment Sheet

Date	Revision #	Amendment Detail	Section	DCR	Amendment Approved by
01-10-24	01	Replace issue# with revision#	Header	23-24	Chief Executive Officer
01-10-24	01	Deletion of page number from header	Header	23-24	Chief Executive Officer
01-10-24	01	QC Lab reporting to CEO for Final Approval	Document Approval	23-24	Chief Executive Officer
15-02-25	02	Lab revised the LSP and Added the Decision rule, OK & Not OK Criteria and mentioned amended or Duplicated report issuance	Document	07-25	Chief Executive Officer

	PROCEDURE FOR REPORTING OF RESULTS	Doc. No.	QCL-LSP-19
		Issue Date	15-02-2025
		Rev#	02

MASTER

CONTROLLED COPY
NO. _____

1.0 PURPOSE

The purpose of this document is to define the process for reporting analytical findings and conclusions as prescribed by the organization.

2.0 SCOPE

This procedure is applicable to VAN QC Lab and the release of information.

3.0 Definitions

- **Decision Rule:** A documented rule that defines how measurement uncertainty is considered when determining conformity with specified requirements.
- **Amended Report:** A report reissued to correct errors or update information previously reported.
- **Duplicate Report:** A reissued report identical to the original report, provided upon client request, without any changes.
- **OK:** A result that meets the specified acceptance criteria or tolerance range.
- **Not OK:** A result that does not meet the specified acceptance criteria or tolerance range.

4.0 RESPONSIBILITY

4.1. Quality Control Manager

QCM is responsible to:

1. Ensure timeliness and completeness of all analytical information reported by the laboratory
2. Reviews, or designates reviews of violative worksheets prior to approval by AQCM manager.

4.2. AQCM

Assistant Quality Control Manager is responsible to:

1. Ensure timeliness, accuracy and completeness of all analytical information reported by the analyst
2. Ensure that laboratory analysts comply with the data and information recording procedures.
3. Review analytical findings and supporting records generated by analysts, enter related conclusions, and sample classification codes.
4. In the absence of QCM Ensure timeliness and completeness of all analytical information reported by the laboratory.

 PROCEDURE FOR REPORTING OF RESULTS MASTER CONTROLLED COPY NO. _____	Doc. No.	QCL-LSP-19
	Issue Date	15-02-2025
	Rev#	02

4.3. Analysts

Analyst are responsible for capturing and recording accurate and complete analytical information on Daily Lab register/worksheets, continuation sheets, electronic lab notebooks, or other records in accordance with the instructions of this procedure and are to complete worksheets and enter analytical observations and findings.

5.0 PROCEDURE

- Reports of VAN QC LAB tests are reviewed and approved by authorized personnel. All Reports of Special Test are signed by personnel explicitly authorized to do so and it will also include the phrase, "QC/M" under the signature. The list of authorized VAN QC LAB official signatories for the reports is documented in the VAN QC LAB sub-level quality documents.
- Reports of VAN QC LAB is written, issued and retained as technical records. The report includes the visible output of VAN QC LAB that is prepared to ensure that it accurately conveys all information pertaining to an Analysis so that data may be used with maximum benefit by all concerned.
- Reports of VAN QC LAB tests are composed and issued in a specific format as documented below and are not reported in a simplified way.

5.1. Common requirements for reports (test and sampling)

VAN QC LAB Reports of Test are designed by to provide accurate, clear, unambiguous and objective information necessary for the interpretation of the results and all information required by the method used. In addition to the report requirements of ISO/IEC 17025:2017, VAN QC LAB Reports of Test include the following information:

- i. the VAN QC LAB "QC No."
- ii. the sample quantity
- iii. the name of the person(s) performing the analysis
- iv. an explanation of the proper use and interpretation of the reported results, as necessary (this can be in the form of an addendum).

Reports of Test conform to ISO/IEC 17025:2017, for accredited parameters and at a minimum, contain or address the following, unless there are valid reasons for not doing so, as documented in the VAN QC LAB sub-level quality documents:

- a. a title (e.g. "Report of Test);



PROCEDURE FOR REPORTING OF RESULTS

Doc. No.	QCL-LSP-19
Issue Date	15-02-2025
Rev#	02

MASTER

CONTROLLED COPY

- b. at least the first page shall be on VAN QC LAB letterhead or be equivalently identified as originating from VAN QC LAB;
- c. the name and address of the laboratory;
- d. the VAN QC LAB "QC No.;"
- e. page numbers, with the last page designated as the end of the report;
- f. the name and address of the customer;
- g. identification of the method used;
- h. a description, unambiguous identification, and, when necessary, the condition of the item(s) or samples tested;
- i. the date of receipt of the test item(s) or samples;
- j. the conditions (e.g. environmental) under which the testing was carried out that have an influence on the measurement results;
- k. the date(s) of performance of the laboratory activity;
- l. the date of issue of the report;
- m. a statement to the effect that the results relate only to the items tested, or sampled;
- n. the results with, where appropriate, the units of measurement; an evaluation of the measurement uncertainty associated with each measured value, if requested;
- o. a description of the test method; additions to, deviations, or exclusions from the method;
- p. the name of the person(s) performing the measurements and analysis, and the name, function, and signature of the person(s) authorizing the report;
- q. an explanation of the proper use and interpretation of the reported results; as necessary (this can be in the form of an addendum).

VAN QC LAB is responsible for all information provided in the report, except when information is provided by the customer. Data provided by a customer is identified. In

Doc. No.	QCL-LSP-19
Issue Date	15-02-2025
Rev#	02

In addition, a disclaimer is put on the report when information is supplied by the customer that can affect the validity of results.

5.2. Specific requirements for test reports

Attributes and contents of test reports issued by VAN QC LAB are addressed in 4.1.

VAN QC LAB does not perform sampling as a separate or distinct. Sampling is done as part of testing in laboratory or onsite measurement.

5.3. Specific requirements for calibration certificates

VAN QC LAB does not issue calibration certificates to its clients.

5.4. Reporting sampling

VAN QC LAB does not offer sampling as a distinct service. When done as part of, it details the method of sampling in its test reports.

5.5. Reporting statements of conformity and Decision Rule Employed

- VAN QC LAB issues statements of conformity for the National or Provincial Environmental Quality Standards or other relevant international standards, as required by client.
- Appropriate reference to applied standard is provided in the reports.
- If the result of a test parameter exceeds the specified limits, the statement of conformity states "Not OK" as the case may be.
- If the result of a test parameter does not exceed specified limits, the statement of conformity states "OK".
- the decision rule employed by VAN QC LAB is based on simple acceptance or rejection.
- the decision rule is based on shared risk by both client and VAN QC LAB in equal terms within the bounds of measurement uncertainty at its specified level (most commonly 95% confidence interval).
- VAN QC LAB provides a disclaimer to this effect in measurement/test report that identifies the decision rule employed. The statement is as under

MASTER

CONTROLLED COPY

"Uncertainty of measurement (UoM) data will be provided on request, if applicable. The statement of conformity, if provided in the report, is based on the decision rule of simple acceptance or rejection with equal shared risk due to measurement uncertainty".

5.6. Defined Decision Rule:

Decision Rule					
Active Range (%)	Upto 2.5	2.5--10	10--25	25--50	>50
FAD Tolerances	15%	10%	6%	5%	3%

- Results are considered "OK" if they fall within the specified tolerance or acceptance range, accounting for measurement uncertainty.
- Results are considered "Not OK" if they fall outside the specified tolerance or acceptance range.

5.7. Reporting opinions and interpretations

Criteria for "OK" and "Not OK"

1. Criteria for "OK":

- The result meets the acceptance limits defined by the client, regulatory authority, or standard.
- Example: For a tolerance of $100 \pm 5\%$, any result between 95% and 105% is considered "OK."

2. Criteria for "Not OK":

- The result falls outside the defined acceptance limits.
- Example: Any result below 95% or above 105% is considered "Not OK."

5.8. Issuance of Amended Reports

1) When to Issue an Amended Report:

- An amended report is issued if corrections are required due to errors, omissions, or updated results.

2) Process for Issuance:

- The amended report must include:



PROCEDURE FOR REPORTING OF RESULTS

Doc. No.

QCL-LSP-19

Issue Date

15-02-2025

Rev#

02

MASTER

CONTROL NO.

Original report identifier: _____

- Clear marking as "Amended" (e.g., "Issue Status #A,B,C-Amended").
- Reason for the amendment.
- Ensure a complete record of the original report is retained.
- 3) **Authorization:**
 - Amended reports must be reviewed and approved by the Assistant Quality Control Manager or Quality Control Manager.
- 4) **Communication:**
 - Notify clients of the amendment and provide the updated report promptly.

5.9. Issuance of Duplicate Reports

1. **When to Issue a Duplicate Report:**
 - A duplicate report may be issued upon client request, provided there are no changes to the original report.
2. **Process for Issuance:**
 - The duplicate report must:
 - Be marked as "Duplicate Copy."
 - Retain the same identifier and issue date as the original report.
 - Ensure the reason for the duplicate issuance is recorded.
3. **Authorization:**
 - Duplicate reports must be reviewed and approved by the AQCM/QCM.
4. **Record Keeping:**
 - Maintain a log of all duplicate reports issued, including the reason and date of issuance.

5.10. Amendments to reports

- When VAN QC LAB issued report needs to be changed, amended or re-issued, the change of information is clearly identified and, where appropriate, the reason for the change is included in the report.



MASTER

PROCEDURE FOR REPORTING OF RESULTS

Doc. No.	QCL-LSP-19
Issue Date	15-02-2025
Rev#	02

- Amendments to VAN QC LAB issued report are made in the form of a further document, or data transfer, that meets all the requirements of the original report, and includes the statement "Amendment to Report or an equivalent form of wording, with the report number clearly showing as revised (R) as documented in the VAN QC LAB sub-level quality documents.
- When it is necessary to issue a completely new VAN QC LAB report, the new report is uniquely identified and contains a reference to the original that it replaces.

6.0 ASSOCIATED DOCUMENTS AND FORMS

1. Test Results Assignment, Summary, Review (QCL-FRM-19.01)
2. Authorization Form
3. Common Requirements for Reports
4. Requirements for Calibration Certificates
5. Requirements for Reporting Sampling
6. Conditions for Statements of Conformity
7. Conditions for Reporting Opinions and Interpretations

CONTROLLED COPY
NO. _____