

NON-CONFORMITY REPORT FOR ASSESSMENT VISIT

F-02/06

Issue Date: 11/11/19

Rev No: 06


ACTIVITY:	☒ Assessment	☐ Surveillance	NCR No: 1
	☐ Re-Assessment	☐ Scope extension	Accr./Appl.No:
	☐ Other Please specify:		Non-conformity category:
			Very serious ☐ Essential ☒
ORGANIZATION:	Quality control Lab vital Agri. Nutrients (Pvt) Ltd.		Time limit for correction:
Department:	Labs		6 weeks
Team Leader.	Mr. Atique Ur Rehman	Mngt. Rep.	Mr. Hammyat Hussain
Assessor	Dr. Muhammad Aftab		
Expert			
DESCRIPTION: The Lab Assistant has not the requisite education, training and competency to conduct the test under scope which is volition of the clause 6.2.2 of the standard ISO/IEC 17025:2017 (NC). Mr. Ahmad Umair (CEO) is supervising the analytical activities in VAN lab as a whole without authorization permit (NC). The lab has developed an annual training Program me (QCL-FRM-2.03) checked the training record of Mr. Masab Rasheed authorized for training of the staff as mentioned in the Authorization permit (QCL-FRM-2.01) but he has no training over MU but working as a trainer over MU (NC). lab has not defined the criteria of the selection of the trainer (NC). The lab has also developed a training need assessment form (QCL-FRM-2.02) but the criteria of the need assessment not mentioned in procedure as well as in training need assessment farm (QCL-FRM-2.02) (NC). The training record related to Measurement of uncertainty is not available in folder (QCL-FIL-20) (NC) however the records related to trainer evaluation is also missing (NC). 10-01-2025 Date _____ Signature Assessor/Expert _____ Signature (Management Representative) _____			Requirement of: ISO/IEC 17025 ☒ ISO 15189 ☐ ISO/IEC 17021 ☐ ISO/IEC 17020 ☐ Others: Ref. Organization's doc.
CORRECTIVE ACTIONS: (Note: It is mandatory to attach Root Cause Analysis) Corrective action for shortcomings on all the NCs has been taken by revising the Authorization permit of Lab Assistant (QCL-FRM-2.01). Revised Authorization permit of CEO (QCL-FRM-2.01). Lab has conducted internal training of Masab Rasheed on Measurement Uncertainty Certificate of training attached. Lab has revised LSP (QCL-LSP-02) and defined the criteria for the selection of trainer accordingly and revised the training need assessment Form (QCL-FRM-2.02). Lab has conducted internal training on MU and maintained record related to MU in folder (QCL-FIL-20) and record related to trainer evaluation maintained in folder (QCL-FRM-20). Action are documented in the amendment no: CA-01-02-25 13-02-25 Date _____ Signature (Management Representative) _____			☐ It is not necessary to attach documentation
REASON FOR CLOSING: (To be filled in by the Team Leader.) ☐ The non-conformity is closed based on satisfactory documentation from the organization ☐ The non-conformity is closed based on recommendation from the technical assessor ☐ Implementation of the corrective actions will be followed up at the next visit Remarks (if any) ----- ----- The non-conformity is closed: _____ Date _____ Signature (Team Leader.) _____			

	CORRECTIVE ACTION REQUEST	Doc. No.	QCL-FRM-9.01
		Issue Date	01-10-2024
		Rev#	01

Initiated by: Masab Rasheed	Department: QC Lab	CAR No. CA-01-02-2025
Designation: AQCM	CAR Initiated Date: 01-02-2025	NC No. 01

CAR Initiated due to (Please tick the relevant appropriate box below)



☒ PNAC Assessment
 ☐ Complaint
 ☐ Accident/Incident
 ☐ Internal Audit
☐ Suggestion/Improvement
 ☐ Technical Fault
 ☐ Others

A. Description (to be filled by Initiator) The Lab Assistant has not the requisite education, training and competency to conduct the test under scope which is volition of the clause 6.2.2 of the standard ISO/IEC 17025:2017 (NC). Mr. Ahmad Umair (CEO) is supervising the analytical activities in VAN lab as a whole without authorization permit (NC). The lab has developed an annual training Program me (QCL-FRM-2.03) checked the training record of Mr. Masab Rasheed authorized for training of the staff as mentioned in the Authorization permit (QCL/FRM-2.01) but he has no training over MU but working as a trainer over MU (NC). Lab has not defined the criteria of the selection of the trainer (NC). The lab has also developed a training need assessment form (QCL/FRM-2.02) but the criteria of the need assessment not mentioned in procedure as well as in training need assessment farm (QCL-FRM-2.02) (NC). The training record related to Measurement of uncertainty is not available in folder (QCL-FIL-20) (NC) however the records related to trainer evaluation is also missing (NC).	
 Signatures	
Significance/Priority Level	☒ Urgent ☐ Normal ☐ Non-significance
☒ Accepted ☐ Rejected	Assigned to: Masab Rasheed Date: 01-02-2025

* If accepted then Manager QC to mark it to concerned person for Root Cause Analysis.

B. Root Cause Analysis (where required) - Lack of a formal process to evaluate and verify the competency, education, and training of personnel before assigning them tasks related to specific tests under the scope of ISO/IEC 17025:2017. - Lack of a robust compliance framework and clearly defined procedures for supervisory roles, including a failure to prioritize and implement internal audits. - A lack of a robust verification mechanism for ensuring that training records (QCL-FRM-2.03) are checked against the authorization permit (QCL/FRM-2.01) before assigning staff as trainers. - The lab management failed to establish and prioritize a documented process for trainer selection due to a lack of focus on human resource competency frameworks within the Lab Management System (LMS). - The development process for the training need assessment procedure and form lacked a systematic approach to ensure that criteria for assessing training needs were clearly defined and documented. This resulted from inadequate consultation, review, and validation mechanisms during the document design and approval phases. - Lack of a standardized process or procedure for the proper documentation and filing of training records related to 'Measurement of Uncertainty' in the designated folder (QCL-FIL-20). - Lack of a defined process and accountability for documenting and storing trainer evaluation records, coupled with inadequate awareness of the importance of compliance and quality requirements.


	CORRECTIVE ACTION REQUEST	Doc. No.	QCL-FRM-9.01
		Issue Date	01-10-2024
		Rev#	01

C. Proposed Action	Target Date:	13-02-2025
Corrective action for shortcomings on all the NCs has been taken by revising the Authorization permit of Lab Assistant (QCL-FRM-2.01). Revised Authorization permit of CEO (QCL-FRM-2.01). Lab has conducted internal training of Masab Rasheed on Measurement Uncertainty Certificate of training attached. Lab has revised LSP (QCL-LSP-02) and defined the criteria for the selection of trainer accordingly and revised the training need assessment Form (QCL-FRM-2.02). Lab has conducted internal training on MU and maintained record related to MU in folder (QCL-FIL-20) and record related to trainer evaluation maintained in folder (QCL-FRM-20).		
		 Name or Signatures (Person who carried out Root Cause Analysis and Proposed Corrective Action)
D. Verification by Manager QC for implementation & Effectiveness		
Is Proposed Action Implemented?	☒ YES ☐ NO	Is it Effective? ☒ YES ☐ NO
Remarks (If any):		
CAR closing date: <u>13-02-25</u>		Manager QC Sign: 

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

Non-Conformance Description			
The Lab Assistant has not the requisite education, training and competency to conduct the test under scope which is volition of the clause 6.2.2 of the standard ISO/IEC 17025:2017 (NC).			
RCA Team Members	Himayat Hussain (QCM), Masab Rasheed (AQCM)		
RCA Team Lead / Head	Himayat Hussain (QCM)		
RCA Start Date	01-02-2025	Submission Date	07-02-2025
Methodology / Tools Used			
Cause & Effect Diagram	☐	5WHY analysis	☐ 3W2H / 5W2H ✓

Cause Effect Diagram



3W2H / 5W2H	Phenomenon of Problem / Question	Explanation / Answer
WHY	Why is the Lab Assistant not conducting the test correctly?	The Lab Assistant does not have the required education, training, or competency.
WHY	Why does the Lab Assistant lack the required education, training, or competency?	The organization did not properly evaluate the Lab Assistant's qualifications and skills before assigning the task.
WHY	Why was the evaluation of qualifications and skills not done properly?	The hiring or task allocation process does not include a robust check for qualifications and training relevant to the test under scope.
WHY	Why does the hiring or task allocation process not include robust checks?	There is no comprehensive procedure or system in place to ensure alignment between job roles and the required competencies.
WHY	Why is there no comprehensive procedure in place?	The management failed to prioritize or regularly review processes for competency verification as per ISO/IEC 17025:2017 Clause 6.2.2.

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

How	How can we ensure this issue does not occur again?	Develop a competency matrix: Create a detailed matrix mapping the required qualifications, training, and skills for each task/test under scope. Implement competency verification: Establish a procedure to verify education, training, and experience of staff before assigning responsibilities.
How	How can we address the current situation?	Immediate action: Reassign the test to a qualified individual until the Lab Assistant is appropriately trained. Corrective action: Enroll the Lab Assistant in necessary training programs to achieve competency for the specific test. Update their competency records.
Root Cause: Lack of a formal process to evaluate and verify the competency, education, and training of personnel before assigning them tasks related to specific tests under the scope of ISO/IEC 17025:2017.		

RCA Statement: Lack of a formal process to evaluate and verify the competency, education, and training of personnel before assigning them tasks related to specific tests under the scope of ISO/IEC 17025:2017.

Reviewed by: 




Evaluated by: 

	PERSONNEL AUTHORIZATION PERMIT	Doc. No.	QCL/FRM-2.01
		Issue Date	01-02-2025
		Rev#	02

1. General

Employee Name	Muhammad Mursaleen
Employee ID	N-069
Designation	Lab Assistant
Section	QC LAB
Laboratory	QC LAB
Academic Qualification	BA
Years of Experience	8 Years
Contact Number	03016806205
Email ID	<u>m.mursaleen15322@gmail.com</u>
Verification/Validation of Testing Methods	No
Approval & Signing of Analysis Report	No

CONTROLLED COPY
NO. _____

Prepared By: Masab Rasheed	Reviewed By: Himayat Hussain	Approved By: Ahmad Umair
AQCM	QCM	CEO
		
Date: 01-02-25	Date: 01-02-25	Date: 01/02/2025

**PERSONNEL AUTHORIZATION
PERMIT**

Doc. No.

QCL/FRM-2.01

Issue Date

01-02-2025

Rev#

02

2. Training/Technical Courses

[illegible]

	PERSONNEL AUTHORIZATION PERMIT CONTROLLED COPY	Doc. No.	QCL/FRM-2.01
		Issue Date	01-02-2025
		Rev#	02

3. Authorization: Lab Assistant **NO.** _____ Employee Name: Muhammad Mursaleen

Sr. #	Authorize to following activities	Work Type	Supervision	Relevant Data Access
1	House Keeping	LAB	AQCM/QCM	Lab Staff
2	Stock Management	All Lab Chemicals and Glassware's	AQCM/QCM	Lab Staff
3	Assist Density Test	All Liquid Products	AQCM/QCM	Lab Staff
4	Assist pH Test	For Liquids and Solids Products	AQCM/QCM	Lab Staff
5	Assist Conductivity	For Liquids and Solids Products	AQCM/QCM	Lab Staff
6	Assist to Inspects Raw Materials for Lab Use	All Materials	AQCM/QCM	Lab Staff
7	Sample Receiving	All Products	AQCM/QCM	Lab Staff
8	Identification of Non-Conformity	All Type	AQCM/QCM	Lab Staff
9	Identification of Need for improvement or Deviation	All Type	AQCM/QCM	Lab Staff
10	Assist in Operation of Analytical Balance	All ranges	AQCM/QCM	Lab Staff
11	Assist in Operation of Flame photometer	Potash	AQCM/QCM	Lab Staff
12	Assist in Operation of pH Meter	pH	AQCM/QCM	Lab Staff
13	Assist in Operation of TDS Meter	Conductivity/TDS	AQCM/QCM	Lab Staff
14	Assist in Operation of Multiparameter Photometer	All tests	AQCM/QCM	Lab Staff
15	Assist in Preparing the Analysis Reports	All Analysis Reports	AQCM/QCM	Lab Staff
16	Assist in Prepare the Control Charts	All Control Charts	AQCM/QCM	Lab Staff
17	Assist in Prepare the temperature/humidity charts	All types of Charts	AQCM/QCM	Lab Staff
18	Monitoring of Environmental conditions	Daily Environmental Check Sheet	AQCM/QCM	Lab Staff
19	Monitoring the temperature and humidity	Daily Environmental Check Sheet	AQCM/QCM	Lab Staff



**PERSONNEL AUTHORIZATION
PERMIT**

Doc. No.	QCL/FRM-2.01
Issue Date	01-02-2025
Rev#	02

19	Perform the Cleaning Inspections	House Keeping	AQCM/QCM	Lab Staff
20	Perform the Intermediates Checks	All Intermediates Checks of Instruments	AQCM/QCM	Lab Staff
21	Sample Dispose	All Fertilizer Samples	AQCM/QCM	Lab Staff
22	Sample Retain	All Fertilizer Samples	AQCM/QCM	Lab Staff
23	Housekeeping	All	AQCM/QCM	Lab Staff



CONTROLLED COPY
NO. _____

	PERSONNEL AUTHORIZATION PERMIT	Doc. No.	QCL/FRM-2.01
		Issue Date	01-02-2025
		Rev#	02

**CONTROLLED COPY
NO. _____**

1. General

Employee Name	Ahmad Umair
Employee ID	N-001
Designation	CEO
Section	NA
Laboratory	QC LAB
Academic Qualification	Chemical Engineer
Years of Experience	20 Years
Contact Number	03214019516
Email ID	<u>umair@van.com.pk</u>
Verification/Validation of Testing Methods	No
Approval & Signing of Analysis Report	No

Prepared By: Masab Rasheed AQCM	Reviewed By: Himayat Hussain QCM	Approved By: Ahmad Umair CEO
		
Date: 01-02-25	Date: 01-02-25	Date: 01/02/2025

	PERSONNEL AUTHORIZATION PERMIT	Doc. No.	QCL/FRM-2.01
		Issue Date	01-02-2025
		Rev#	02

CONTROLLED COPY
NO.

3. Authorization: CEO

Employee Name: Ahmad Umair

Sr. #	Authorize to following activities	Work Type	Supervision	Relevant Data Access
1	Management Responsibility	Responsible for the overall implementation of the quality management system and the laboratory's compliance with the standard. This includes ensuring sufficient resources, establishing policies, and maintaining the integrity of the management system.	NA	NA
2	Competency of Personnel	The laboratory must ensure that all personnel, if they are involved in laboratory activities, are competent and have the necessary qualifications for their roles.	NA	NA
3	Delegation of Authority	Responsible to delegates authority for technical operations to specific staff (such as a Quality Control Manager or Technical Manager). The CEO is ultimately responsible for ensuring that personnel have the required competencies and that the laboratory operates in compliance with ISO/IEC 17025:2017.	NA	NA
4	Documented Responsibilities	1. Approve the policies, Procedures. 2. Overseeing the implementation of the management system. 3. Ensuring impartiality and integrity of laboratory operations. 4. Promoting continual improvement.	NA	NA



PERSONNEL AUTHORIZATION PERMIT

CONTROLLED COPY

Doc. No.	QCL/FRM-2.01
Issue Date	01-02-2025
Rev#	02

NO. _____

5	Management Commitment	1. Commitment to the laboratory's quality management system by supporting its continual improvement and ensuring that the lab's goals align with the standard. 2. Resource allocation. The CEO ensures that the laboratory has adequate resources (human, financial, infrastructure) to perform testing activities competently.	NA	NA
6	Ensuring the Quality Management System (QMS)	1. Establishing policies and procedures for the laboratory's operations. 2. Reviewing and approving quality manuals and other related documents to ensure the laboratory's conformance to the standard. 3. Promoting a culture of quality, including setting expectations for quality and performance within the organization.	NA	NA
7	Impartiality and Independence	1. Ensuring that personnel within the laboratory are free from undue external influence when performing testing or issuing results. 2. Being responsible for establishing procedures that protect the objectivity of the laboratory and its staff.	NA	NA
		1. Ensuring that potential risks to testing activities (e.g., equipment failure,		


	PERSONNEL AUTHORIZATION PERMIT CONTROLLED COPY NO. _____	Doc. No.	QCL/FRM-2.01
		Issue Date	01-02-2025
		Rev#	02

8	Risk Management and Continual Improvement	data integrity issues) are identified and mitigated. 2. Promoting continual improvement: The CEO plays a vital role in fostering a culture of continuous improvement within the laboratory. This includes using data from internal audits, corrective actions, and management reviews to drive improvements in operations, equipment, and employee competencies.	NA	NA
9	Managing Nonconformities and Corrective Actions	1. Ensures that a system is in place to identify, report, and analyze nonconformities. 2. Ensures that corrective actions are taken and reviewed to prevent recurrence.	NA	NA
10	Reviewing the Effectiveness of the Management System	1. Management reviews, where the CEO evaluates the performance of the lab's processes, client feedback, audit findings, and any corrective actions taken. 2. Ensuring that decisions made during management reviews are implemented and tracked for effectiveness.	NA	NA

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

Non-Conformance Description			
Mr. Ahmad Umair (CEO) is supervising the analytical activities in VAN lab as a whole without authorization permit (NC).			
RCA Team Members	Himayat Hussain (QCM), Masab Rasheed (AQCM)		
RCA Team Lead / Head	Himayat Hussain (QCM)		
RCA Start Date	01-02-2025	Submission Date	07-02-2025
Methodology / Tools Used			
Cause & Effect Diagram	☐	5WHY analysis	☐
		3W2H / 5W2H	☒

Cause Effect Diagram

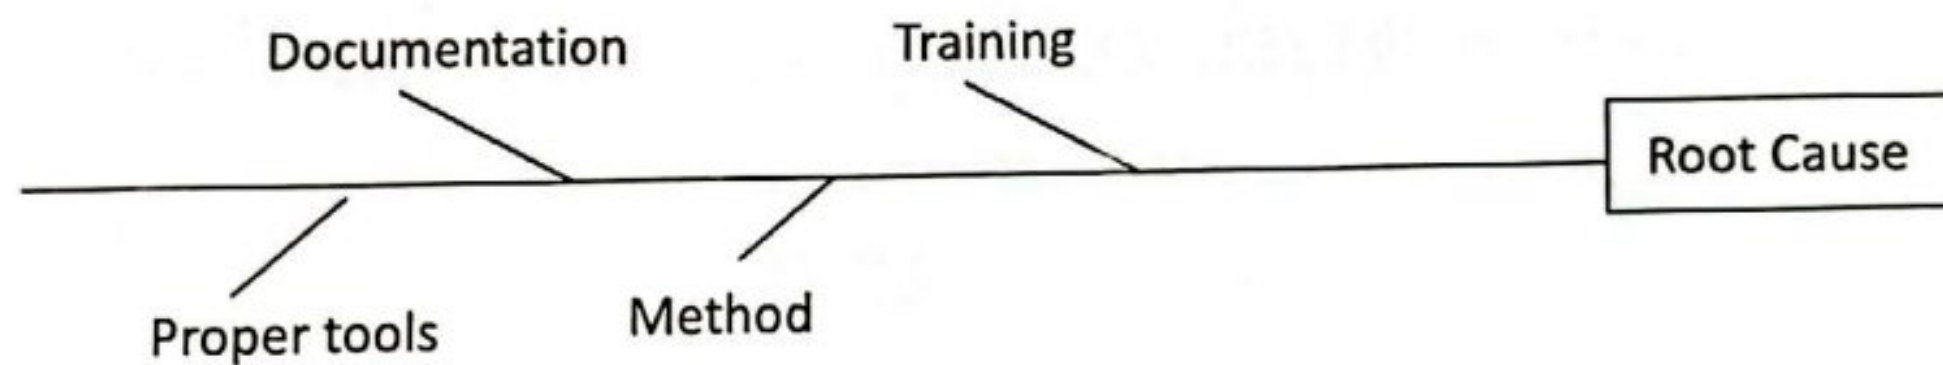


3W2H / 5W2H	Phenomenon of Problem / Question	Explanation / Answer
WHY	Why is Mr. Ahmad Umair (CEO) supervising the lab activities without an authorization permit?	The authorization process for supervision was not followed or enforced.
WHY	Why was the authorization process not followed?	The lab's operational procedures did not explicitly limit supervision responsibilities to authorized personnel.
WHY	Why do the operational procedures lack clarity on authorization requirements?	There has been no prior audit or review to identify and address gaps in procedural documentation.
WHY	Why was there no prior audit or procedural review?	Management prioritized other activities over compliance and quality assurance processes.
WHY	Why was compliance not prioritized?	There is insufficient awareness or training about the importance of compliance in maintaining operational integrity and regulatory standard (ISO/IEC 17025:2017).
How	How can we ensure unauthorized supervision does not happen again?	Implement a policy that explicitly states only authorized personnel can supervise analytical activities.

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

Non-Conformance Description			
The lab has developed an annual training Program me (QCL-FRM-2.03) checked the training record of Mr. Masab Rasheed authorized for training of the staff as mentioned in the Authorization permit (QCL/FRM-2.01) but he has no training over MU but working as a trainer over MU (NC).			
RCA Team Members	Himayat Hussain (QCM), Masab Rasheed (AQCM)		
RCA Team Lead / Head	Himayat Hussain (QCM)		
RCA Start Date	01-02-2025	Submission Date	13-02-2025
Methodology / Tools Used			
Cause & Effect Diagram	☐	5WHY analysis	☐
		3W2H / 5W2H	✓

Cause Effect Diagram



3W2H / 5W2H	Phenomenon of Problem / Question	Explanation / Answer
WHY	Why is Mr. Masab Rasheed working as a trainer on MU without proper training?	The authorization permit (QCL-FRM-2.01) lists him as a trainer without verifying his training records.
WHY	Why was his training not verified before granting authorization?	The process of verifying training records was not strictly followed during the authorization process.
WHY	Why was the process of verifying training records not strictly followed?	There is no formal procedure or checklist in place to ensure training records are cross-checked before authorization.
WHY	Why is there no formal procedure or checklist for verification?	Oversight during the development of the authorization process or lack of awareness about the need for such a step.
WHY	Why was there oversight in the process design?	Insufficient risk assessment and quality assurance reviews when designing the process for staff authorization.
How	How can we prevent this issue from recurring?	Develop and implement a formal Training Record Verification Checklist as part of the authorization

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

		process. Train supervisors and staff responsible for the authorization process on the importance of verifying training credentials.
How	How can we address the current NC?	• Immediately suspend Mr. Masab Rasheed's trainer authorization for MU until he completes the required training. • Update the authorization permit (QCL-FRM-2.01) to reflect only verified trainers. • Provide Mr. Masab Rasheed with the necessary training on MU and reassess his competency before reinstating him as a trainer.
Root Cause: A lack of a robust verification mechanism for ensuring that training records (QCL-FRM-2.03) are checked against the authorization permit (QCL-FRM-2.01) before assigning staff as trainers		

RCA Statement: A lack of a robust verification mechanism for ensuring that training records (QCL-FRM-2.03) are checked against the authorization permit (QCL-FRM-2.01) before assigning staff as trainers.

Reviewed by: 

Evaluated by: 

Certificate

This is to certify that

Mr. Masab Rasheed

has participated in one day training on

**Measurement Uncertainty Training
course based on ISO/IEC 17025:2017**

*(General requirements for measurement
uncertainties of testing)*


Conducted by

Vital Agri Nutrients (Private) Limited


on February 12, 2025

CONTROLLED COPY

NO. _____



HIMAYAT HUSSAIN
Trainer/QCM
Vital Agri Nutrients



AHMAD UMAIR
Chief Executive Officer
Vital Agri Nutrients



Certificate

This is to certify that
Mr. Masab Rasheed
has participated

CONTROLLED COPY
NO. _____

**Training Course on Laboratory Management System (LMS)
and Internal Audit based on ISO/IEC 17025:2017**


(General requirements for the competence of testing and calibration laboratories)

conducted by


Pakistan National Accreditation Council (PNAC)

22-23 October, 2024

at Faletti's Hotel, Lahore, Pakistan



Engr. M Imran

Director IB / Trainer
PNAC



Nisar Ali Khan

Director ECL /Trainer
PNAC



Ateeq ur Rehman Memon

Director General
PNAC



Certificate

This is to certify that

Himayat Hussain

has participated in

CONTROLLED COPY
NO. _____


Assessor Training Course Based on ISO/IEC 17025:2017
(General requirements for the competence of testing and calibration laboratories)


conducted by


Pakistan National Accreditation Council (PNAC)

from 27th to 31st January 2025
at Avari Hotel, Lahore, Pakistan

Note: The course has been designed in accordance with ILAC – G3 and APAC CBC-002


Muhammad Imran
Director / Trainer
PNAC



Ateeq-ur-Rehman
Director General
PNAC


Azhar Iqbal
Director / Trainer
PNAC

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

Non-Conformance Description			
Lab has not defined the criteria of the selection of the trainer (NC).			
RCA Team Members	Himayat Hussain (QCM), Masab Rasheed (AQCM)		
RCA Team Lead / Head	Himayat Hussain (QCM)		
RCA Start Date	01-02-2025	Submission Date	07-02-2025
Methodology / Tools Used			
Cause & Effect Diagram	☐	5WHY analysis	☐
		3W2H / 5W2H	✓

Cause Effect Diagram



3W2H / 5W2H	Phenomenon of Problem / Question	Explanation / Answer
WHY	Why were the trainer selection criteria not defined?	The lab management did not consider it necessary to formalize the process.
WHY	Why did the management not consider it necessary?	There was no policy or guideline in place mandating the definition of such criteria.
WHY	Why was there no policy or guideline in place?	The lab's management system (LMS) did not prioritize training-related documentation.
WHY	Why did the LMS not prioritize training documentation?	The lab's focus has been more on technical procedures rather than human resource competency frameworks.
WHY	Why has the focus been more on technical procedures?	The lab leadership has not recognized the importance of formal training processes in ensuring quality and compliance.
How	How can we prevent this issue in the future?	Develop and implement a documented procedure for trainer selection, including clear and measurable criteria (e.g.,

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

		qualifications, experience, certifications, etc.) • Integrate training-related policies into the LMS to ensure compliance and regular audits
How	How can we ensure this solution is effective?	• Conduct a review of all training-related processes during internal audits to verify the implementation and effectiveness of the trainer selection criteria. • Assign a responsible person or team to oversee training documentation and monitor the qualification of trainers regularly.
Root Cause: The lab management failed to establish and prioritize a documented process for trainer selection due to a lack of focus on human resource competency frameworks within the Lab Management System (LMS).		

RCA Statement: The lab management failed to establish and prioritize a documented process for trainer selection due to a lack of focus on human resource competency frameworks within the Lab Management System (LMS).


Reviewed by: 

Evaluated by: 

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

Non-Conformance Description			
The training record related to Measurement of uncertainty is not available in folder (QCL-FIL-20) (NC).			
RCA Team Members	Himayat Hussain (QCM), Masab Rasheed (AQCM)		
RCA Team Lead / Head	Himayat Hussain (QCM)		
RCA Start Date	01-02-2025	Submission Date	07-02-2025
Methodology / Tools Used			
Cause & Effect Diagram	☐	5WHY analysis	☐
		3W2H / 5W2H	✓

Cause Effect Diagram




3W2H /5W2H	Phenomenon of Problem / Question	Explanation / Answer
WHY	Why is the training record related to "Measurement of Uncertainty" not available in the folder (QCL-FIL-20)?	The responsible person did not file the training record in the specified folder.
WHY	Why did the responsible person not file the record in the specified folder?	They were either unaware of the requirement or overlooked the filing process.
WHY	Why were they unaware of the requirement or overlooked the process?	There was no clear procedure or checklist for managing and filing training records.
WHY	Why is there no clear procedure or checklist for managing and filing training records?	Because the documentation and record-keeping process for training sessions is not adequately defined or standardized.
WHY	Why is the process not adequately defined or standardized?	The importance of proper record management was not emphasized during process design or staff training.
How	How can the issue be corrected?	Retrieve the missing training record from alternative sources (e.g., trainer logs, emails, or other records).

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

		• Ensure the record is promptly filed in the correct folder (QCL-FIL-20). • Verify the completeness of other training records to identify any similar gaps.
How	How can recurrence of the issue be prevented?	• Develop and implement a standardized procedure for filing training records, including a checklist and timeline for documentation. • Provide training to relevant staff members on the importance of record-keeping and the new procedure. • Regularly audit training records to ensure compliance with the procedure.
Root Cause: Lack of a standardized process or procedure for the proper documentation and filing of training records related to 'Measurement of Uncertainty' in the designated folder (QCL-FIL-20).		


RCA Statement: Lack of a standardized process or procedure for the proper documentation and filing of training records related to 'Measurement of Uncertainty' in the designated folder (QCL-FIL-20).

Reviewed by: 

Evaluated by: 

	DOCUMENT CHANGE REQUEST	Doc.#	QCL-FRM-7.02
		Issue Date	01-02-2025
		Rev#	02

CONTROLLED COPY NO.

Section A			
DCR No.	03-25	Date	01-02-25
Request Raised By	Masab Rasheed	Section	QC Lab
Document Title	Personal Training Record	Document Status	NEW EXISTING ☒
Reason(s)	☐	New Process Documentation	New Form Documentation
	☒	Addition in Document	Correction in Document
	☐	Deletion within Document	Modification in Document
Section B			
Description of Requirement	Revision of document to address the shortcomings observed during PCR Audit		
Effected Sections (Not Applicable on New Documents)	Addition of competence criteria, Authorization		
	Permit revised, Revised Training need		
	Assessment form and addition of Hammer		
	evaluation		
Section C			
Review by	Himayat Hussain	Review Status (Choose only one)	☒ Draft Reviewed
Designation			☐ Draft Rejected
			☐ Draft Revision Suggested
Reason for Rejection (Choose only one)	☐	Conflict with Policy	Conflict with Procedure
	☐	Conflict with Client Requirement	Conflict with Regulation
	☐	Incorrect Draft	Draft Does not reflect "Description of Requirement"
Final Remarks	Recommend for final Approval.		
Submitted for Final Approval on (Date)			
Approved By		Designation	CEO

 PERSONNEL TRAINING RECORD MASTER	Doc. No.	QCL-LSP-02
	Issue Date	01-02-2025
	Rev#	02

CONTROLLED COPY
NO. _____

Standard Operating Procedure for PERSONNEL TRAINING RECORD

ISO/IEC 17025:2017 – Clause 6.2

Prepared By: Masab Rasheed	Reviewed By: Himayat Hussain	Approved By: Ahmad Umair
AQCM	QCM	CEO
		
Date: 01-02-25	Date: 01-02-25	Date: 01/02/2025

Copyright

The copyright of this procedure, together with all confidential information contained herein is the sole property of **VAN QC LAB**.

It may be copied in full or in parts only by the Management / personnel and only for the purpose of Company related activities. Disclosure and copying of any information contained within this procedure to any person (s) outside the employee of company without written permission/authorization of the Chief Executive Officer is strictly prohibited.

	PERSONNEL TRAINING RECORD	Doc. No.	QCL-LSP-02
		Issue Date	01-02-2025
		Rev#	02

MASTER

CONTROLLED COPY
Amendment Sheet
NO. _____

Date	Revision #	Amendment Detail	Section	DCR	Amendment Approved by
20-09-24	01	Replace issue# with revision#	Header	02-24	Chief Executive Officer
20-09-24	01	Deletion of page number from header	Header	02-24	Chief Executive Officer
20-09-24	01	QC Lab reporting to CEO for Final Approval	Document Approval	02-24	Chief Executive Officer
20-09-24	01	Selection criteria revised	Document Plaining	02-24	Chief Executive Officer
20-09-24	01	Training, supervision and Authorization revised	Document Authorization Form	02-24	Chief Executive Officer
01-02-25	02	Addition of Competence criteria, Authorization Permit revised, revised the training need assessment form and addition of trainer evaluation	Document	03-25	Chief Executive Officer

 PERSONNEL TRAINING RECORD MASTER	Doc. No.	QCL-LSP-02
	Issue Date	01-02-2025
	Rev#	02

CONTROLLED COPY
NO. _____

1.0 PURPOSE

The purpose of this procedure is to establish and define an internal / external training program for VAN QC Lab and to ensure the competency/selection of laboratory personnel. The procedure provides guidelines for;

1. Selection of personnel
2. Determining the competency requirement/training needs
3. Training of personnel
 - a) Training Planning
 - b) Training Execution
 - c) Training Evaluation
4. Authorization of personnel
5. Monitoring competency of personnel

2.0 SCOPE

The Procedure is applicable to all document related to training based on ISO/IEC 17025:2017 in VAN QC Lab.

3.0 RESPONSIBILITY

3.1 Quality Control Manager (QCM) is responsible to;

- 3.1.1 Ensure implementation of the procedure.
- 3.1.2 To ensure that record of trainings is maintained for ISO/IEC 17025:2017.
- 3.1.3 Ensures personnel receive training and demonstrate competence.
- 3.1.4 Ensure for the training and growth of the technical and quality related skills of lab staff
- 3.1.5 Review and approve the annual training plan developed in accordance with Training need assessment.
- 3.1.6 Approval of participants for External trainings.
- 3.1.7 Approval of participants for internal trainings.
- 3.1.8 Implement / arrange training and maintains employee training files.
- 3.1.9 Review training received and ensures training files are complete.
- 3.1.10 Update the training records / Lab Authorization Permit of lab staff on periodic basis.

3.2 Assistant Quality Control Manager (AQCM) is responsible to;

- 3.2.1 Assess the training needs of the laboratory staff in consultation with QCM
- 3.2.2 Identify training needs resulting from new or revised procedures and processes.
- 3.2.3 Monitor employee performance to identify the need for retraining or additional continual education.
- 3.2.4 Develop annual training plan and ensure that it has been followed.

4.0 PROCEDURE

 PERSONNEL TRAINING RECORD MASTER	Doc. No.	QCL-LSP-02
	Issue Date	01-02-2025
	Rev#	02

4.1 Selection of personnel

VAN QC LAB has documented the competence requirements based on the specific criteria defined by ISO/IEC 17025:2017, for each function influencing the results of laboratory activities, including requirements for education, qualification, training, technical knowledge, skills and experience. All such criteria are documented in Job Description (QCL-JD-NN)

VAN QC LAB personnel are selected as per following competence criteria mentioned in table A

Competence criteria (Table: A)


Sr. No	Designation	Minimum Education/Qualification	Minimum Experience	Trained on	Technical Knowledge/Skills
1	Chief Executive Officer	M. Sc (Chemical Engineer/Soil Sciences/Chemistry)	Minimum 15 Year's management experience in any reputable firm/institute	Management Techniques	Have Knowledge about fertilizer industry
2	Quality Control Manager	M. Sc/MPhil (Soil science/Analytical Chemistry)	Minimum 5 years hands on experience of working in a reputable company on fertilizer analysis and developments	ISO/IEC 17025:2017/ ISO 9001:2015, Internal System Auditing, Analytical techniques.	Spectro, pH Meter, TDS Meter, Karl Fischer and flame photometer and all technique used in fertilizer.
3	Assistant Quality Control Manager	M.Sc/BS (Hons) (Chemistry/Chemical Engineer)	Minimum 3 years' experience in any reputable firm/institute	ISO/IEC 17025:2017/ISO 9001:2015, Internal System Audit, Analytical techniques	Spectro, pH Meter, TDS Meter, Karl Fischer and flame photometer and all technique used in fertilizer. Have Skills and working experience on Lab Management System and QMS External/Internal System Audit, LMS, QMS
4	Analyst	M.Sc/B.S (Soil science /Chemistry) MA (In any subject)	Minimum 2 years' experience in the pesticide laboratory.	analytical skills, ISO/IEC 17025:2017	All technique used in fertilizer. In case of MA all the skills mentioned is mandatory and in line experience of minimum 8 years in fertilizer industry.

	PERSONNEL TRAINING RECORD CONTROLLED COPY MASTER NO.	Doc. No.	QCL-LSP-02
		Issue Date	01-02-2025
		Rev#	02

5	Assist. Analyst	M.Sc./B. S/B. Sc/F. Sc (Soil science /Chemistry/Chemical Engineer) MA (In any subject)	No experience is necessarily required for M.Sc. / BS. hons Chemistry (Analytical / Organics/Soil Science). 2 Years' experience in fertilizer laboratory is required in case of M.A. 5 Years in line experience in case of F. Sc	Familiar with ISO/IEC 17025:2017 and analytical skills.	In case of MA have skills of fertilizer testing and have experience of working in fertilizer laboratory.
6	Lab. Assistant	Bachler/Intermediate / Matric	2 years' experience in the Fertilizers analysis in case of Bachler, 3 years' experience in the Fertilizers analysis in case of intermediate 4 year's inline experience in case of Matric	trained on Physical testing, pH and EC meter and sample receiving.	Physical Testing, Sample receiving, pH and EC meter.
7	Lab. Attendant	Matric	Fresh or 1-year relevant experience	No training requirement for fresh.	Physical Testing, Sample receiving, pH and EC meter.
8	New Induction	M.Sc / B.Sc (Soil science /Chemistry)	No experience is necessarily required for M.Sc. / BS. hons Chemistry (Analytical / Organics/Soil Science).	Familiar with ISO/IEC 17025:2017 and Computer Literate	Preferred if having knowledge on analytical Skills on GC and HPLC.
9	Trainer	MPhil/M.Sc./BS. hons Chemistry (Analytical /Organics/Soil Science). /MA	3-5 years inline experience for technical training. 2 years as QCM/AQCM in any reputable firm/institute for Management Requirement training.	ISO/IEC 17025:2017, ISO 9001:2015 External/Internal System Audit. Analytical Techniques. Word, Excel & power point.	Karl Fischer, Spectro and flame photometer and all technique used in fertilizer testing. Presentation Preparation & communication skills

Competence criteria for personnel selection is communicated to the HR department for hiring of personnel. HR department give advertisement in the newspaper and arrange interview for the selection of personnel. Top management will select the personnel on the basis of defined criteria. The management of the laboratory communicates to personnel their duties, responsibilities and authorities in the job descriptions.

All personnel of the laboratory, that could influence the laboratory activities act impartially, are competent and work in accordance with the laboratory's management

 MASTER	PERSONNEL TRAINING RECORD CONTROLLED COPY NO.	Doc. No.	QCL-LSP-02
		Issue Date	01-02-2025
		Rev#	02

system. Impartiality policy (QCL-POL-03) is prepared and communicated to all employees and undertaking form (QCL-FRM-3.01) is signed by employee to legally ensure that they act impartially.

4.1 Determining the Competency Requirements / Training Needs

4.1.1 QCM and AQCM perform training need assessment of the laboratory personnel based on their skills, education and experience on Training Need Assessment form (QCL-FRM-2.02).

4.1.2 Training Need Assessment is done under following titles; but not limited to.

- 1) Equipment operation
- 2) Laboratory skills
- 3) Statistical control parameters
- 4) Quality Assurance and validity of test results
- 5) QMS awareness and auditing
- 6) Teamwork
- 7) Reporting

4.1.3 VAN QC LAB ensure that the personnel have the required competence to perform laboratory activities for which they are responsible and to evaluate the significance of deviations.

4.1.4 Nomination of participants is approved by QCM/AQCM for internal trainings. For External trainings, nomination of participants is approved by CEO/QCM.

4.2 Training Planning

4.2.1 In the beginning of a year, QCM ensures in consultation with AQCM that **Annual Training Program** is prepared and implemented for the Lab Staff.

4.2.2 AQCM define trainings related to laboratory procedures, methods and specifications, equipment manuals and other related topics in the **Annual Training Program** for a whole year.

4.2.3 The CEO/QCM approves the **Annual Training Program**.

4.3 Training Execution and Duration

4.3.1 Training is scheduled as per the **Annual Training Program**.

4.3.2 Training Title and training duration is mentioned in Annual Training Program.

4.3.3 AQCM notifies all nominated participants officially to ensure 100% attendance in the training program.

4.3.4 QCM ensures the availability of resources, including trainer, training material, venue etc.

4.3.5 Training is conducted on the scheduled date and record of the training is updated in the **Training Record Form**.

4.3.6 Attendance of participants is documented in the **Attendance Sheet**.

4.4 Training Evaluation

MASTER**CONTROLLED COPY**

4.4.1 To ensure the effectiveness of the provider training (internal or external), AQCM shall carry out evaluation of the trainees with at least one of the following methods/modes.

a. Oral test

This method is used where level of awareness needs to be assessed by taking trainee feedback on training.

b. Written exam / test

This method is used when understanding of the trainee needs to be assessed.

c. Practical demonstration

This method is used when coordination between procedure and practical application of the trainee need to be assessed.

4.4.2 Weightage of the aforesaid evaluation methods / modes is as follows:

4.4.3

Mode of Evaluation	Weightage			
	10 %	40%	–	15%
Oral Test	10 %	40%	20%	–
Written Exam / Test	15 %	60%	80%	85%
Practical Demonstration	75 %	–		
Overall Contribution	100 %			

4.4.4 Training is evaluated by AQCM and record of the evaluation of individual participant is updated in the **Training Evaluation Form**.

Note: Selected trainings are evaluated and intimation will be done in advance to participants for such trainings.

4.5 Orientation / Training plan of New Staff

4.5.1 AQCM arrange Orientation Session for newly inducted Laboratory Staff to educate the basic procedures and functions of Lab Management System.

4.5.2 Orientation session can be delivered any time of the year, and needs not be planned in the Annual Training Program.

4.5.3 Orientation/ training plan for newly inducted staff is prepared by AQCM after their joining, training title and duration are mentioned in plan as per requirement of job responsibilities.

4.5.4 QCM authorizes and approves all orientation sessions and Plan.

4.5.5 Laboratory attendant are acquired as daily wagger, works under supervision of experience staff, they appointed as attendant on contract after one-year experience if found hardworking, cooperative and having good learning attitude.

4.7 Supervision of personnel

After the training evaluation, lab staff need to work under the supervision of experienced and authorized person for the time period of six month. After the

MASTER**CONTROLLED COPY****NO.**

completion of supervision period, supervisor of the personnel comments on the personnel performance and forward to the QCM for approval for authorization of the personnel.

4.6 Authorization of Personnel

VAN QC LAB personnel are authorized for specific task on the bases of their Qualification, in line Experience, Technical skills and trainings they acquired in house or external. Once the training session is delivered and evaluation is performed, QCM approves the authorization of laboratory staff for the specific task. AQCM updates the **Lab Authorization Permit** of the Laboratory staff.

4.7 Monitoring Competence of Personnel

Competence of expert, experienced and authorized laboratory personnel are assessed once in a year by evaluating their testing performances in scope products batch analysis, replicate and retesting activities of scope products, by their performances in PT/ILC programs. These performances are supervised and evaluated by AQCM and QCM.

Acceptance criteria for monitoring competence is as below;

1. Proficiency testing /ILC $|Z| \leq 2$ Acceptable
2. Replicate, Retesting & Batch analysis

% Active	% Recovery
Product > 10%	98-102 %
Product 1 - 10%	97-103%
Product < 1%	95-105%

Reference:

- South Africa National Accreditation System ISO 17043:2010
- Guidelines on method validation to be perform in support of analytical Agrochemical Formulations (Improved version, CIPAC -3807)


8.0 Related Documents

- ✓ Lab Authorization Permit (QCL-FRM-2.01)
- ✓ Training Need Assessment (QCL-FRM-2.02)
- ✓ Annual Training Plan (QCL-FRM-2.03)
- ✓ Training Attendance Sheet (QCL-FRM-2.04)
- ✓ Training Evaluation (QCL-FRM-2.05)
- ✓ Authorized Person List (QCL-FRM-2.06)
- ✓ Training Feedback Form (QCL-FRM-2.07)
- ✓ Individual Training Record (QCL-FRM-2.08)
- ✓ Orientation Form (QCL-FRM-2.09)
- ✓ Competence Reassessment Form (QCL-FRM-2.10)
- ✓ Orientation Training Plan for Newly Inducted Staff (QCL-FRM-2.11)
- ✓ Trainer Evaluation Form (QCL-FRM-2.12)

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

Non-Conformance Description			
The records related to trainer evaluation is also missing (NC).			
RCA Team Members	Himayat Hussain (QCM), Masab Rasheed (AQCM)		
RCA Team Lead / Head	Himayat Hussain (QCM)		
RCA Start Date	01-02-2025	Submission Date	07-02-2025
Methodology / Tools Used			
Cause & Effect Diagram	☐	5WHY analysis	☐
		3W2H / 5W2H	✓

Cause Effect Diagram



3W2H /5W2H	Phenomenon of Problem / Question	Explanation / Answer
WHY	Why are the records missing?	They were not documented or properly stored.
WHY	Why were they not documented or properly stored?	There is no clear process or responsibility assigned for maintaining these records.
WHY	Why was there no clear process or responsibility?	The training evaluation process was not included in the lab system procedures (LSP).
WHY	Why was the process not included in the LSP?	The importance of trainer evaluation records was overlooked during the LSP development phase.
WHY	Why was it overlooked?	There was a lack of awareness about the compliance requirements or quality standards for trainer evaluation.
How	How can this issue be prevented in the future?	- Establish a formal process for documenting and storing trainer evaluation records. - Assign clear roles and responsibilities for record maintenance.

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

How	How can this issue be detected early if it recurs?	• Conduct periodic audits of training records. • Implement a checklist or digital tracking system to ensure all records are completed and stored after every training session.
Root Cause: Lack of a defined process and accountability for documenting and storing trainer evaluation records, coupled with inadequate awareness of the importance of compliance and quality requirements.		

RCA Statement: Lack of a defined process and accountability for documenting and storing trainer evaluation records, coupled with inadequate awareness of the importance of compliance and quality requirements.

Reviewed by: 

Evaluated by: 

	TRAINER EVALUATION FORM	Doc. No.	QCL-FRM-2.12
		Issue Date	01-02-2025
		Rev#	02

Trainer Name: _____

Training Topic: _____

Date of Training: _____

Evaluator Name: _____

Evaluation Type: Participant Evaluation

CONTROLLED COPY
NO. _____


Instructions: Please tick your level of agreement with the statements listed below

Evaluation Criteria	Strongly Agree (5)	Agree (4)	Neutral (3)	Disagree (2)	Strongly Disagree (1)
The objectives of the training were clearly defined					
Knowledge of ISO/IEC 17025:2017					
Clarity in Explanation of Concepts					
Delivery Skills (Pace, Energy)					
Ability to Address Questions					
Engagement with Participants					
Training Materials and Tools Provided					
Relevance of Content to Participants					
The topics covered were relevant to me					
The content was organized and easy to follow.					
The materials distributed were helpful.					
This training experience will be useful in my work					
The trainer was well prepared.					
The trainer was knowledgeable about the training topics.					
The training objectives were met.					
The time allotted for the training was sufficient.					
Overall Effectiveness					

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

Non-Conformance Description			
The lab has also developed a training need assessment form (QCL-FRM-2.02) but the criteria of the need assessment not mentioned in procedure as well as in training need assessment form (QCL-FRM-2.02) (NC).			
RCA Team Members	Himayat Hussain (QCM), Masab Rasheed (AQCM)		
RCA Team Lead / Head	Himayat Hussain (QCM)		
RCA Start Date	01-02-2025	Submission Date	07-02-2025
Methodology / Tools Used			
Cause & Effect Diagram	☐	5WHY analysis	☐
		3W2H / 5W2H	✓

Cause Effect Diagram



3W2H / 5W2H	Phenomenon of Problem / Question	Explanation / Answer
WHY	Why is the training need assessment form missing the criteria?	The reason is that the procedure and the form do not specify the criteria for assessing training needs.
WHY	Why do the procedure and form not specify the criteria?	Because no clear guidelines or framework were established during the development of the TNA form and procedure.
WHY	Why were no guidelines or framework established?	The team assumed that the users of the form would understand the criteria based on their knowledge or experience.
WHY	Why did the team make this assumption?	There was insufficient consultation or review during the form's design phase to identify this gap.
WHY	Why was there insufficient consultation or review?	There is no formal mechanism in place to validate and approve newly developed forms or procedures.
How	How can we ensure criteria are defined in the procedure and form?	Review the current training need assessment procedure and the form to identify gaps.

	ROOT CAUSE ANALYSIS FORM	Doc. No.	QCL-FRM-9.04
		Issue Date	01-10-2024
		Rev#	01

		- Engage relevant stakeholders (HR, training coordinators, and management) to define clear criteria for assessing training needs. - Update the procedure (e.g., include specific steps to assess training needs) and revise the form to include fields for documenting the criteria.
How	How can we prevent similar NCs in the future?	- Develop a formal review and approval process for all new or revised documents, ensuring they are aligned with requirements and best practices. - Provide training for staff involved in form and procedure development to emphasize the importance of including clear criteria and guidelines. - Implement periodic audits of forms and procedures to ensure compliance with quality standards.

Root Cause: The development process for the training need assessment procedure and form lacked a systematic approach to ensure that criteria for assessing training needs were clearly defined and documented. This resulted from inadequate consultation, review, and validation mechanisms during the document design and approval phases.

RCA Statement: The development process for the training need assessment procedure and form lacked a systematic approach to ensure that criteria for assessing training needs were clearly defined and documented. This resulted from inadequate consultation, review, and validation mechanisms during the document design and approval phases.

Reviewed by:  ASAP

Evaluated by:  _____

	TRAINING NEED ASSESSMENT	Doc.#	QCL-FRM-2.02
		Issue Date	01-02-2025
		Rev#	02

CONTROLLED COPY

Name: _____ **NO.** _____ Designation: _____

For the Year: _____ Amendment No.: _____

Sr. #	Key Points	Rating	Remarks
1	Output of Work Neatness, accuracy, on-time completion		
2	Initiative Corrective and preventive Action, practicable suggestions		
3	Validation of Analytical Methods and STM		
4	Equipment Operation Karl Fischer, pH meter, Conductivity meter, Density Meter, Analytical balance, Flame photometer, Spectrophotometer		
5	Internal Audit ISO/IEC 17025:2017 Standard / LSP		
6	Sample Handling Sample Receipt, Preparation, Extraction, Storage		
7	Reporting Opinion and Interpretation		

Total Marks (%): _____

Rating Criteria:

Outstanding	75 - 100%
Good	50 - 75 %
Average	25 - 50 %
Poor	below 25 %

Trainings Required

1

2

3

4

5

Prepared by (AQCM): _____

Approved by (QCM): _____

Approval Date: _____