

Grade 4-3-4
Sample # 230811

Analyte ReportCard
Lab Code 0584



Magruder Fertilizer Proficiency Testing Program Regular PT Scheme

Proficiency Testing For 4 Analytes

Issue Date : 09/30/2023

Analyte Group	Analyte Group (Units)	Lab 0584 Data		*Robust Analyte Values					Magruder Z Score	Your Method	Flag
		Value	range	Rob Mean	Rob SD	%RSD	Rob R-bar (n)	# Tests			
010	Total N (4%)	4.070	0.0800	4.048	0.1292	3.19%	0.0701 (58)	63	0.17	010.99	0
041	Direct Available P2O5 (3%)	3.435	0.5700	4.066	0.5415	13.32%	0.0900 (39)	42	-1.17	041.99	1
050	Soluble K2O (4%)	4.135	0.0700	4.326	0.2882	6.66%	0.0842 (65)	72	-0.66	050.99	0
148	Total S (5%)	5.070†	0.0800	6.222	0.8855	14.23%	0.1326 (36)	39	-1.30	148.01	0

Notes and Flags:

1: Interpreting Z Scores: Red indicates a normally distributed Z value >3 or <-3 (requires action), Orange = Z between 2 and 3 or -2 and -3 (warning) and a PASS at Green, where Z < 2 and Z >-2 (OK at 95%). The 9 Flag indicates a data problem - scores not calculated.

2: Flags indicate data usage: 0 = Used, 1 = rejected for duplicates too far apart, 2 = rejected as extreme outlier, 3 = removed from stats, 4 = rejected due to 0s submitted, 5 = LOD. The 9 Flag indicates a data problem - scores not calculated.

3: Analyte codes in light green indicate a guaranteed analyte. Your offset values are higher (‡) or lower (†) than the Robust Analyte value ± 1A.

4: *Robust statistics not used if < 6 labs used in calculations, in this case Values and Z Scores are grayed out and should be interpreted cautiously. R-bar is robustified to provide a fair measure of the mean range. Identical duplicates not included in calculation of Rob R-bar. The (n) in Rob R-bar (n) = number of tests used to calculate Rob R-bar.



Grade 4-3-4
 Analyte ReportCard
 Z-Score Box Plot and Guarantees
 Sample # 230811




Magruder Fertilizer Proficiency Testing Program

Regular PT Scheme

Proficiency Testing For 4 Analytes

Issue Date : 09/30/2023

Z-Score Box and Whisker Plots for Lab # 0584 <guaranteed analyte>

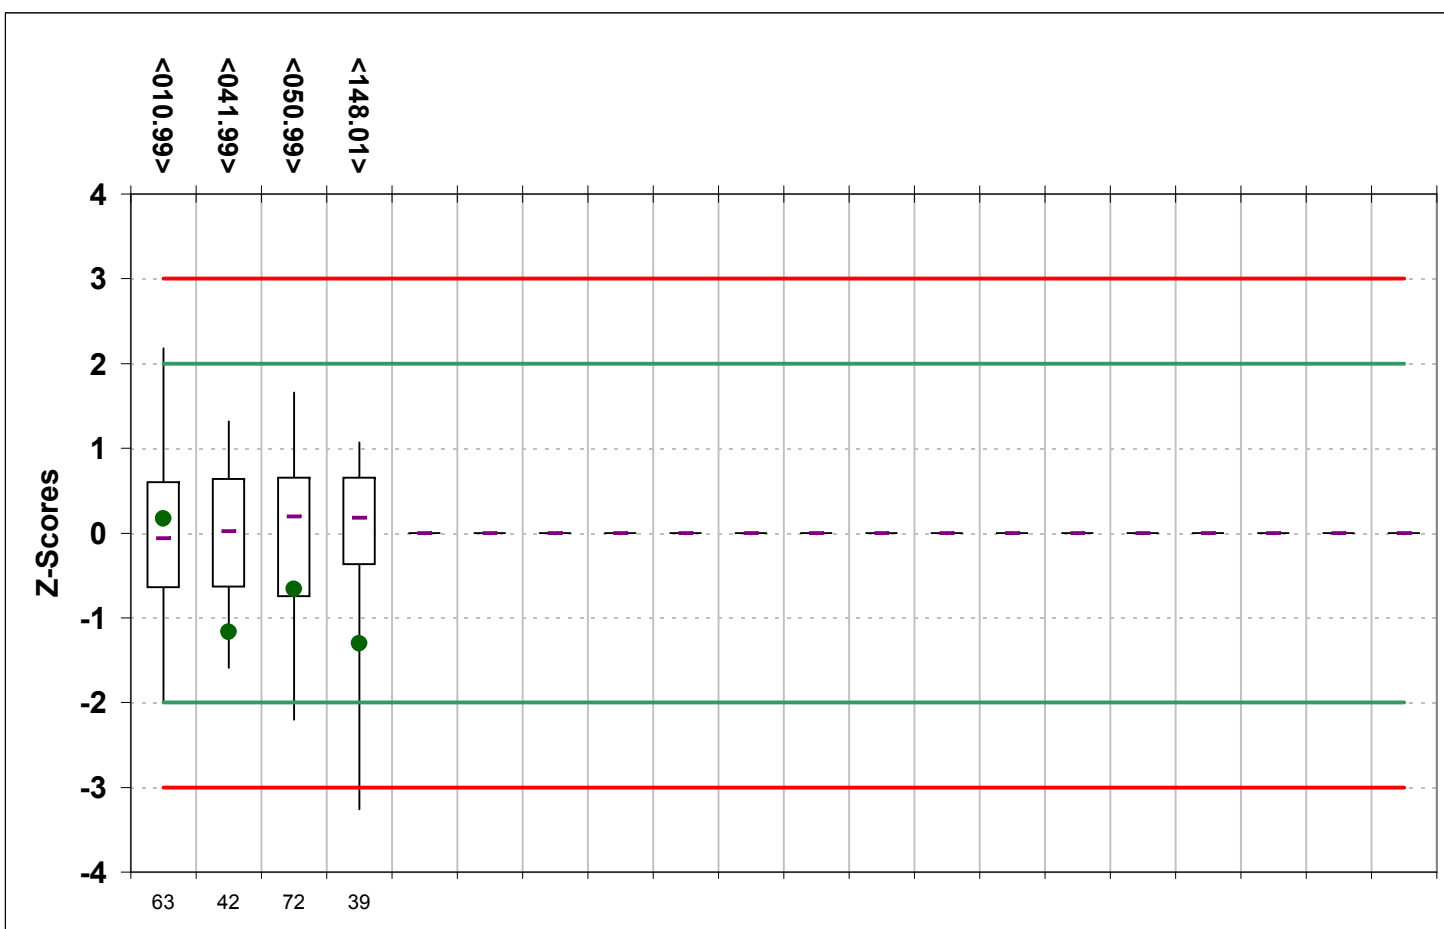

Guaranteed in This Sample			
Analyte	Code	Value*	IA
N	010	4.048	0.491
P2O5	041	4.066	0.670
K2O	050	4.326	0.417
Mg	121	1.956	0.298
S	148	6.222	0.511

* Value (if guaranteed in Sample!) is the Robust Analyte Value estimated using the primary Analyte Codes for this sample and may not reflect the Label value.

Notes: The Methods you used are indicated above and the # Labs involved are below the Box and Whisker. Your Z-Score is indicated by the Black Dot. If you do not see a Black Dot your score is off the chart. Dots between the Green lines are acceptable Z-Scores. Dots outside the Red lines are actionable. The Bar, Box and Whisker represent Median, 25% to 75% percentile and 5% to 95% percentile respectively.